

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN062719\
 Data File : VN056524.D
 Acq On : 27 Jun 2019 21:36
 Operator : JC/SP
 Sample : K3519-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SP-19-LF2-TB1

Quant Time: Jun 28 03:30:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062719SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 28 03:22:32 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	53319	5.00	ug/l	0.00
4) 1,4-Difluorobenzene	8.58	114	92482	5.00	ug/l	0.00
8) Chlorobenzene-d5	11.41	117	56144	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.34	152	8841	5.00	ug/l	0.00
System Monitoring Compounds						
3) 1,2-Dichloroethane-d4	8.02	65	32055	4.91	ug/l	0.00
Spiked Amount 5.000	Range	81 - 118	Recovery	=	98.20%	
5) Dibromofluoromethane	7.59	113	23949	4.70	ug/l	0.00
Spiked Amount 5.000	Range	80 - 119	Recovery	=	94.00%	
6) Toluene-d8	10.09	98	54099	4.69	ug/l	0.00
Spiked Amount 5.000	Range	89 - 112	Recovery	=	93.80%	
7) 4-Bromofluorobenzene	12.39	95	13928	4.72	ug/l	0.00
Spiked Amount 5.000	Range	85 - 114	Recovery	=	94.40%	
Target Compounds						
2) Vinyl Chloride	2.17	62	26	0.005	ug/l #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN062719\
Data File : VN056524.D
Acq On : 27 Jun 2019 21:36
Operator : JC/SP
Sample : K3519-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SP-19-LF2-TB1

Quant Time: Jun 28 03:30:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062719SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Fri Jun 28 03:22:32 2019
Response via : Initial Calibration

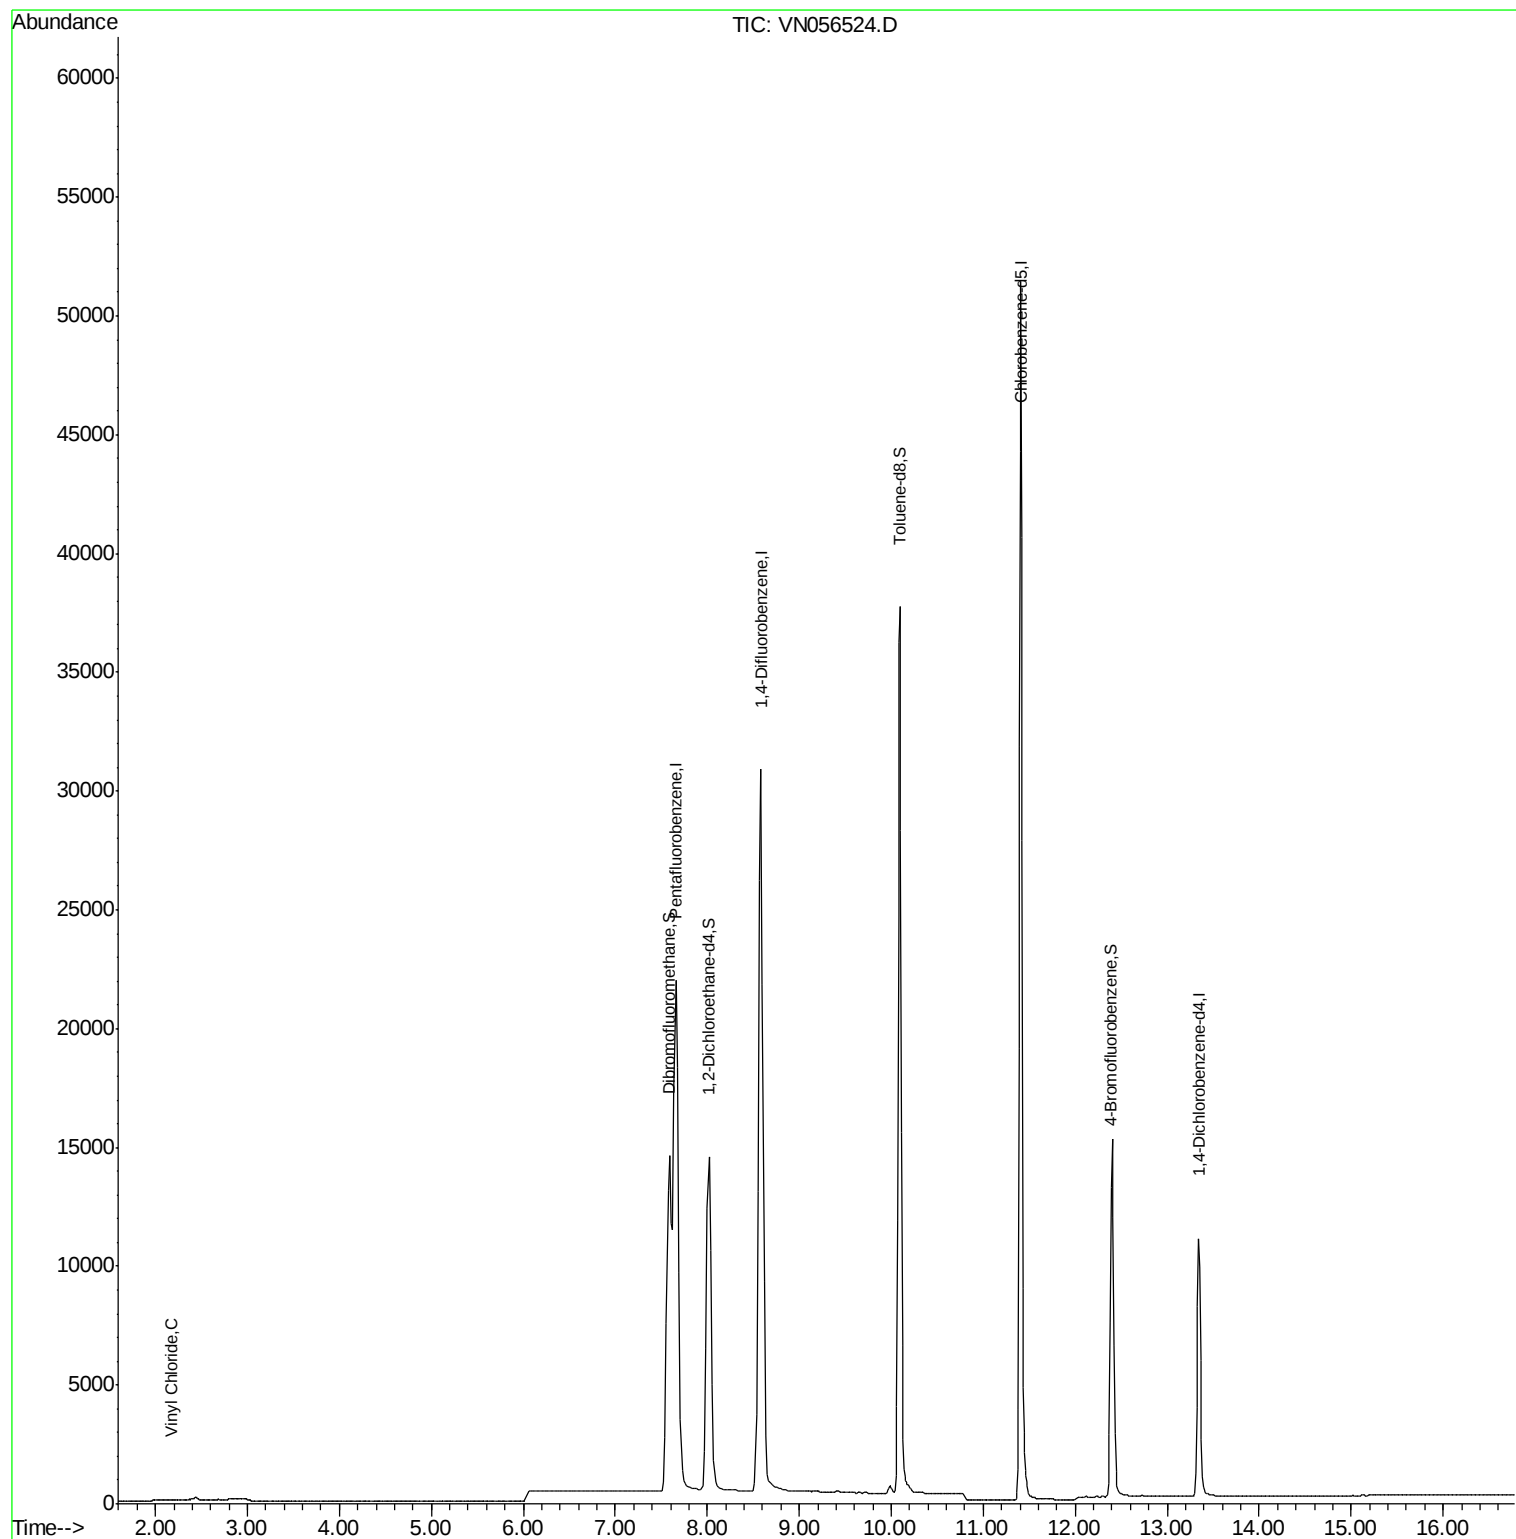



#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.66 min Scan# 1244

Delta R.T. 0.00 min

Lab File: VN056524.D

Acq: 27 Jun 2019 21:36

Instrument :

MSVOA_N

ClientSampleId :


SP-19-LF2-TB1

Tot Ion:168 Resp: 53319




Ion Ratio Lower Upper

168 100

99 49.5 41.9 62.9

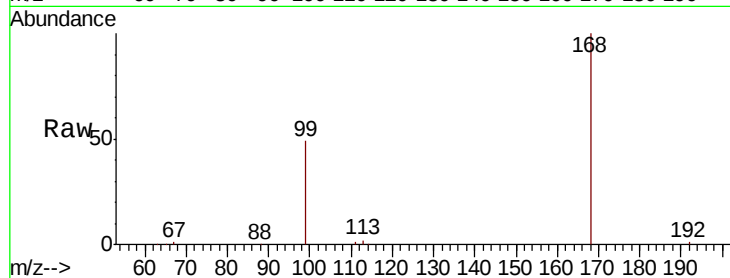

Abundance Ion 168.00 (167.70 to 168.70): VN056516.D (-1233) (-)

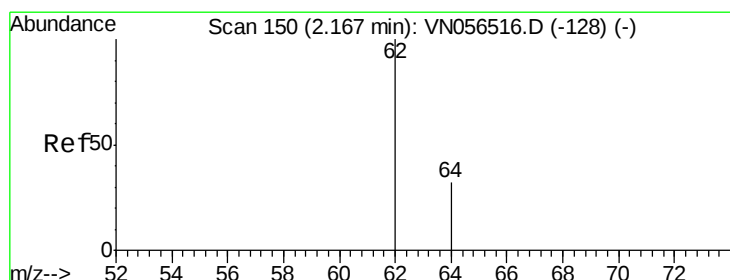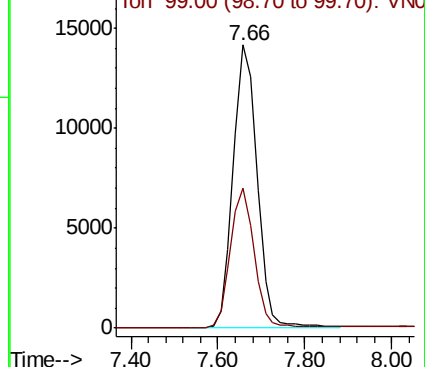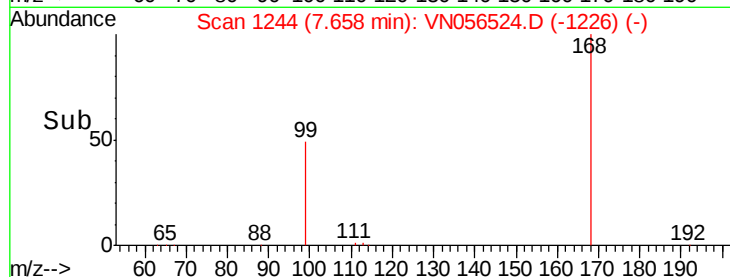

#2

Vinyl Chloride

Concen: 0.005 ug/l

RT: 2.17 min Scan# 150

Delta R.T. 0.00 min

Lab File: VN056524.D


Acq: 27 Jun 2019 21:36

Tgt Ion: 62 Resp: 26



Ion Ratio Lower Upper

62 100

64 110.1 26.1 39.1#

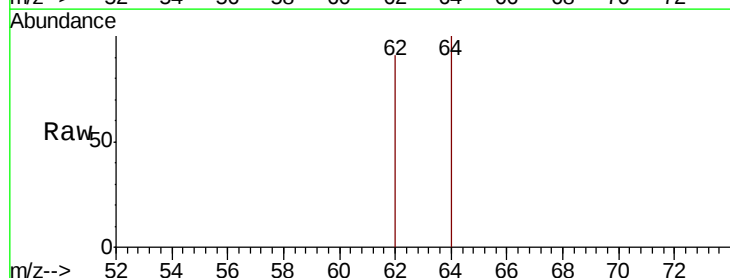

Abundance Ion 62.00 (61.70 to 62.70): VN056516.D (-128) (-)

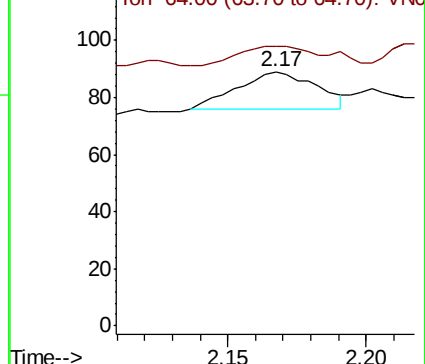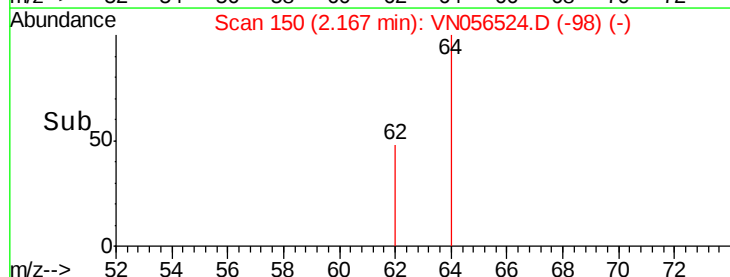



#3

1,2-Dichloroethane-d4

Concen: 4.908 ug/l

RT: 8.02 min Scan# 1265

Delta R.T. 0.00 min

Lab File: VN056524.D

Acq: 27 Jun 2019 21:36

Instrument :

MSVOA_N

ClientSampleId :





SP-19-LF2-TB1

Tot Ion: 65 Resp: 32055

Ion Ratio Lower Upper

65 100

67 54.9 0.0 108.8

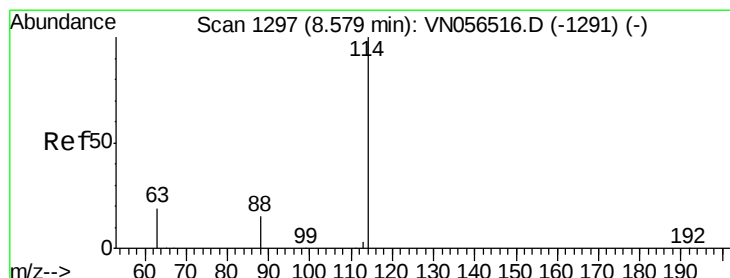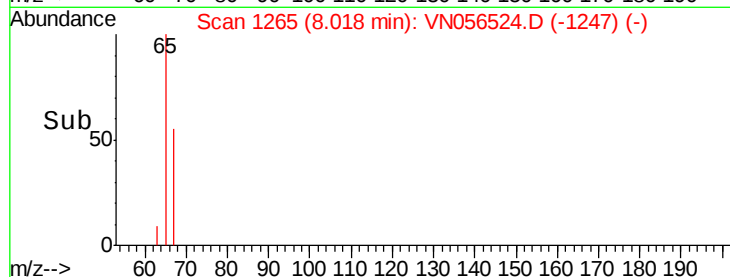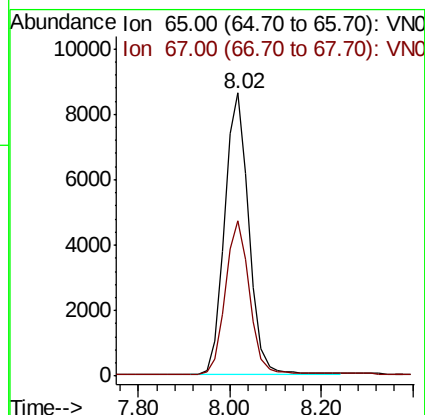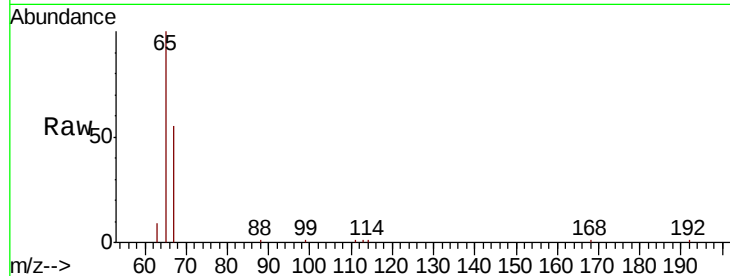

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.58 min Scan# 1298

Delta R.T. 0.00 min

Lab File: VN056524.D

Acq: 27 Jun 2019 21:36




Tgt Ion: 114 Resp: 92482

Ion Ratio Lower Upper

114 100

63 17.3 0.0 37.6

88 14.8 0.0 31.2

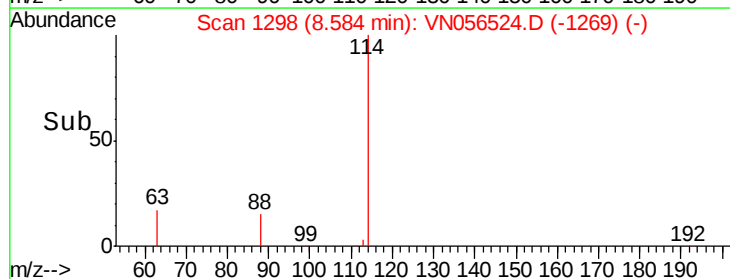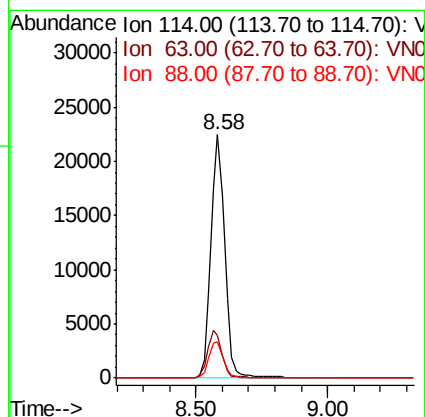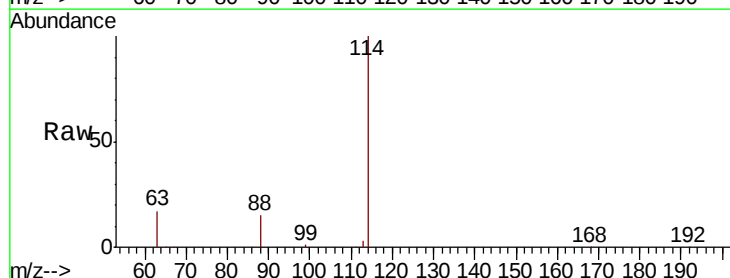



#5

Dibromofluoromethane

Concen: 4.697 ug/l

RT: 7.59 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VN056524.D

Acq: 27 Jun 2019 21:36

Instrument :

MSVOA_N

ClientSampleId :

SP-19-LF2-TB1


Tot Ion:113 Resp: 23949

Ion Ratio Lower Upper

113 100

111 101.5 81.7 122.5




192 21.7 16.9 25.3

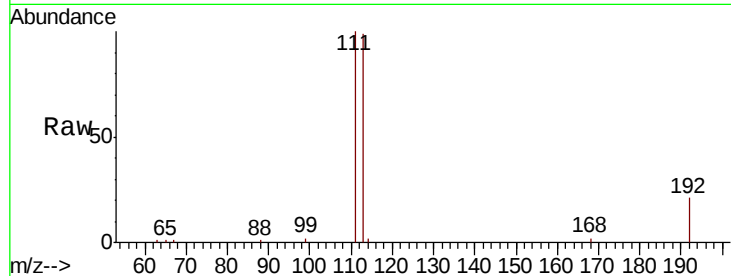

Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

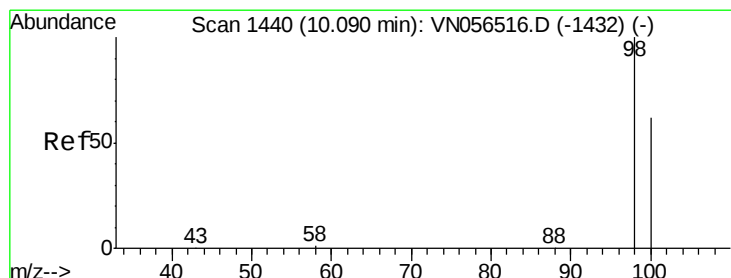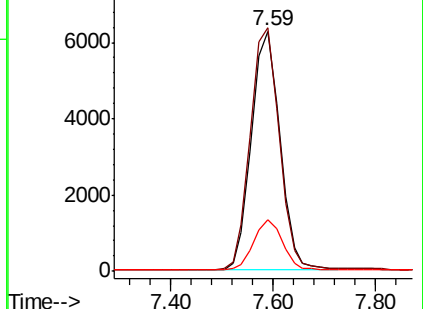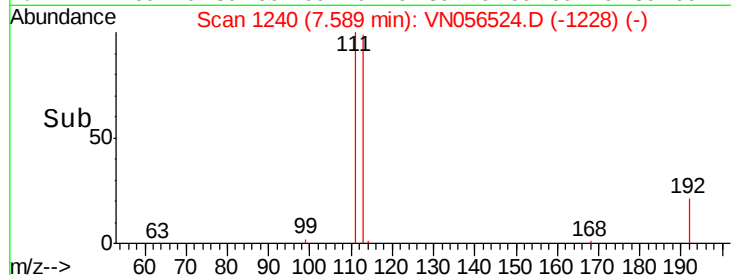

#6

Toluene-d8

Concen: 4.690 ug/l

RT: 10.09 min Scan# 1441

Delta R.T. 0.00 min

Lab File: VN056524.D


Acq: 27 Jun 2019 21:36

Tgt Ion: 98 Resp: 54099

Ion Ratio Lower Upper



98 100

100 64.6 49.7 74.5

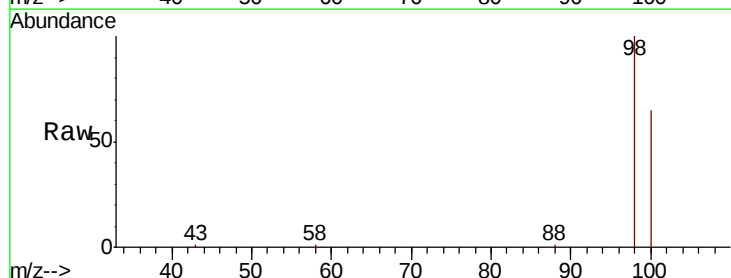

Abundance Ion 98.00 (97.70 to 98.70): VN

Ion 100.00 (99.70 to 100.70): VN

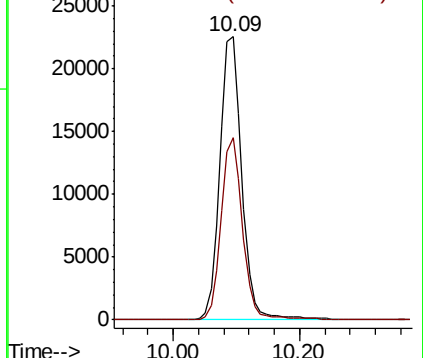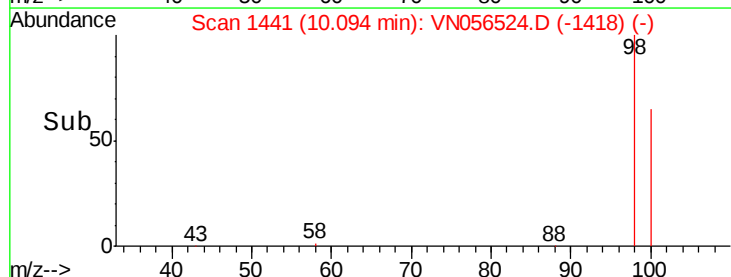



#7

4-Bromofluorobenzene

Concen: 4.720 ug/l

RT: 12.39 min Scan# 1773

Delta R.T. -0.00 min

Lab File: VN056524.D

Acq: 27 Jun 2019 21:36

Instrument :

MSVOA_N

ClientSampleId :

SP-19-LF2-TB1


Tot Ion: 95 Resp: 13928

Ion Ratio Lower Upper

95 100

174 74.8 0.0 167.8




176 67.2 0.0 158.0

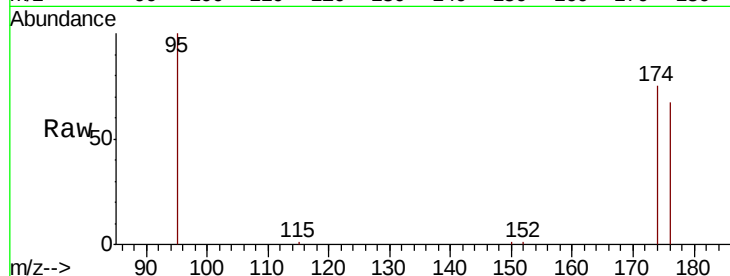

Abundance Ion 95.00 (94.70 to 95.70): VN056516.D (-1763) (-)

Ion 174.00 (173.70 to 174.70): VN056516.D (-1763) (-)

Ion 176.00 (175.70 to 176.70): VN056516.D (-1763) (-)

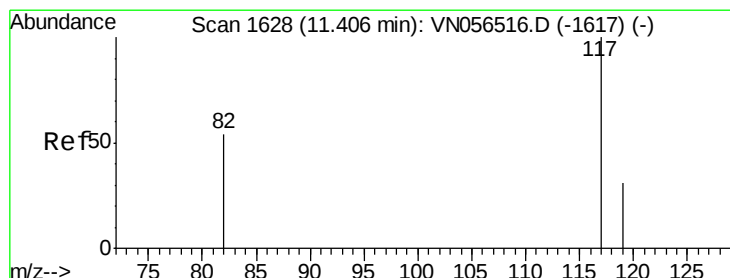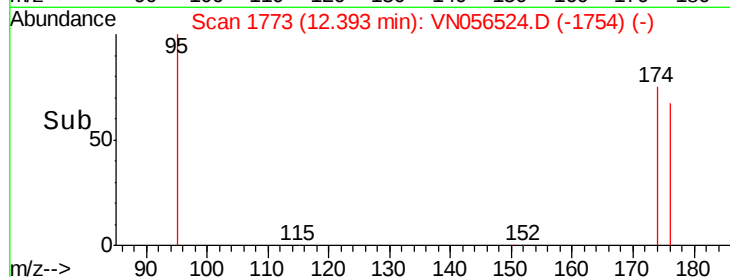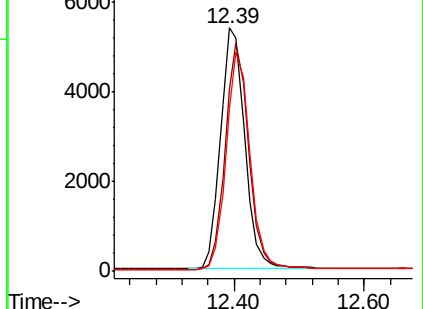

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.41 min Scan# 1629

Delta R.T. 0.00 min

Lab File: VN056524.D

Acq: 27 Jun 2019 21:36


Tgt Ion: 117 Resp: 56144

Ion Ratio Lower Upper

117 100

82 53.3 43.0 64.4



119 31.3 24.7 37.1

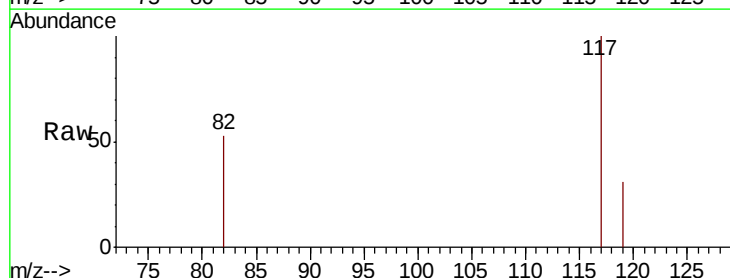

Abundance Ion 117.00 (116.70 to 117.70): VN056516.D (-1617) (-)

Ion 82.00 (81.70 to 82.70): VN056516.D (-1617) (-)

Ion 119.00 (118.70 to 119.70): VN056516.D (-1617) (-)

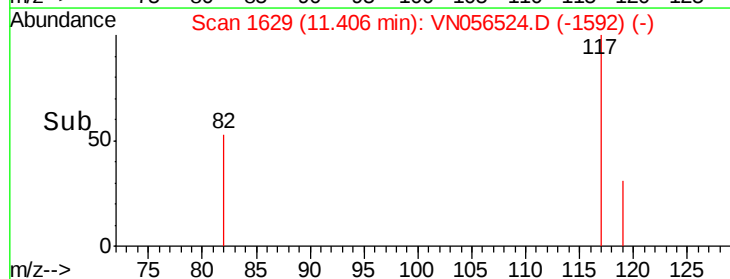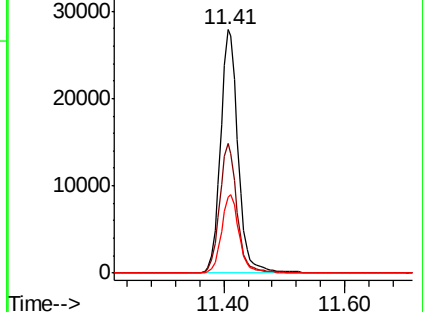



#9
 1,4-Dichlorobenzene-d4
 Concen: 5.000 ug/l
 RT: 13.34 min Scan# 1864
 Delta R.T. -0.00 min
 Lab File: VN056524.D
 Acq: 27 Jun 2019 21:36

Instrument :
 MSVOA_N
 ClientSampleId :
 SP-19-LF2-TB1

Tot Ion:152 Resp: 8841
 Ion Ratio Lower Upper
 152 100
 115 57.3 27.0 80.8
 150 158.5 0.0 306.6

