


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062719\
 Data File : VN056511.D
 Acq On : 27 Jun 2019 10:18
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062719SIM-VINYL.M
 Title : SW846 8260
 Last Update : Fri Jun 28 03:22:32 2019

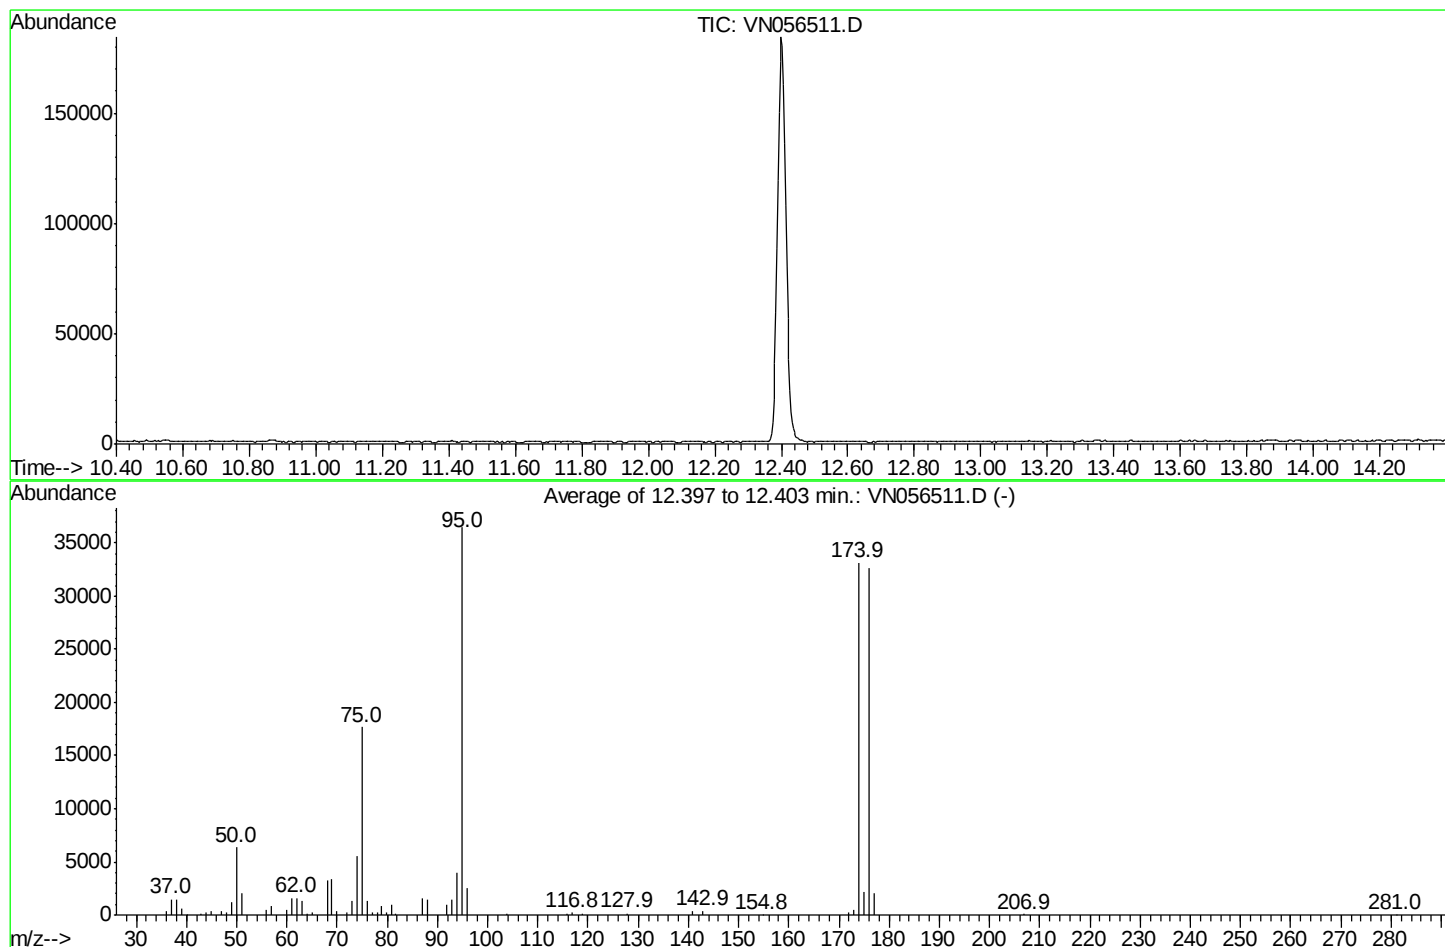

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	6345	PASS
75	95	30	60	48.5	17688	PASS
95	95	100	100	100.0	36466	PASS
96	95	5	9	7.1	2582	PASS
173	174	0.00	2	1.4	460	PASS
174	95	50	100	90.8	33114	PASS
175	174	5	9	6.6	2196	PASS
176	174	95	101	98.4	32586	PASS
177	176	5	9	6.4	2088	PASS