


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN062719\
Data File : VN056519.D
Acq On : 27 Jun 2019 18:51
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062719SIM-VINYL.M
Title : SW846 8260
Last Update : Mon Jul 01 15:45:13 2019

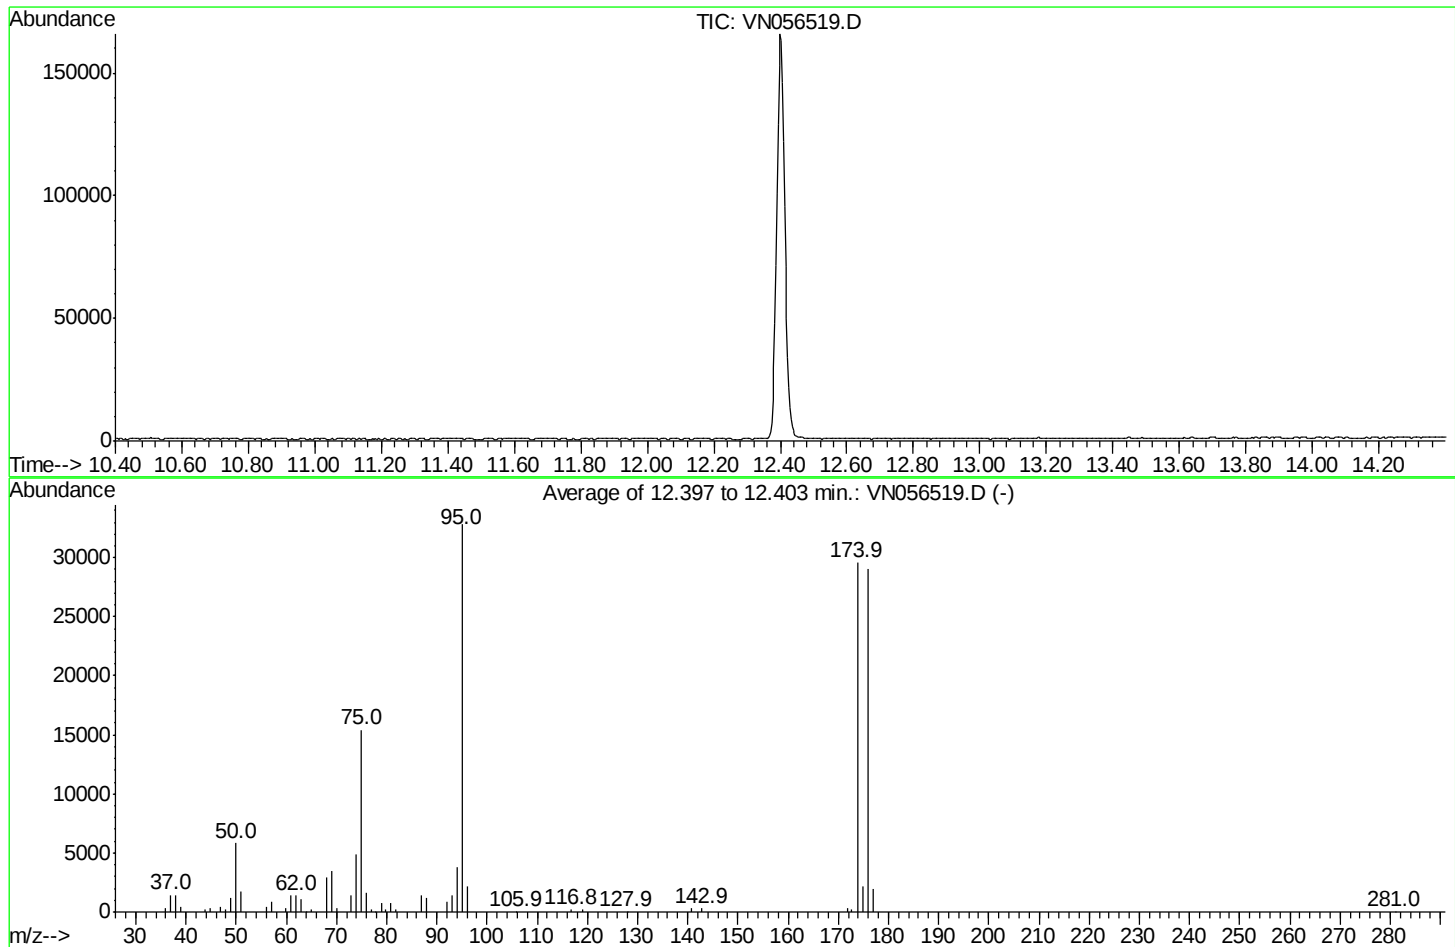

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	5807	PASS
75	95	30	60	46.9	15408	PASS
95	95	100	100	100.0	32821	PASS
96	95	5	9	6.7	2185	PASS
173	174	0.00	2	0.6	183	PASS
174	95	50	100	90.1	29578	PASS
175	174	5	9	7.5	2207	PASS
176	174	95	101	98.2	29058	PASS
177	176	5	9	6.6	1913	PASS