

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062722\
 Data File : VN073162.D
 Acq On : 27 Jun 2022 15:14
 Operator : JC\MD
 Sample : N3494-17
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SP-EXC-1-6

Quant Time: Jun 28 06:37:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.022	168	308508	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	507257	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	471196	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	242495	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	191146	45.828	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	91.660%		
35) Dibromofluoromethane	7.951	113	93427	29.798	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	59.600%#		
50) Toluene-d8	10.381	98	534498	45.815	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	91.620%		
62) 4-Bromofluorobenzene	12.669	95	242359	57.772	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	115.540%		
Target Compounds						Qvalue
3) Chloromethane	2.263	50	569	0.747	ug/l	93
11) Tert butyl alcohol	5.298	59	284	0.264	ug/l #	72
16) Acetone	4.228	43	77354	33.739	ug/l	93
18) Methyl Acetate	4.787	43	2671	0.437	ug/l #	58
20) Methylene Chloride	5.010	84	113937	31.951	ug/l	95
23) Vinyl Acetate	6.493	43	2680	0.247	ug/l #	68
25) 2-Butanone	7.269	43	16779	4.612	ug/l	92
26) 2,2-Dichloropropane	7.263	77	63	Below Cal	#	53
29) Tetrahydrofuran	7.628	42	1276	0.531	ug/l #	61
31) Cyclohexane	8.016	56	7989	1.416	ug/l #	30
36) 1,1-Dichloropropene	8.016	75	25254	5.953	ug/l #	49
37) Ethyl Acetate	7.269	43	16779	2.473	ug/l #	67
38) Carbon Tetrachloride	8.016	117	31452	7.048	ug/l #	17
39) Methylcyclohexane	9.398	83	2198	0.430	ug/l	94
40) Benzene	8.392	78	314830	23.613	ug/l	100
42) 1,2-Dichloroethane	8.392	62	3123	0.659	ug/l	79
48) Methyl methacrylate	9.492	41	7184	1.622	ug/l #	40
51) 4-Methyl-2-Pentanone	10.269	43	9866	1.560	ug/l	88
52) Toluene	10.439	92	3849	0.470	ug/l	84
59) 2-Hexanone	10.992	43	146191	29.881	ug/l #	21
65) Chlorobenzene	11.710	112	1192444	129.582	ug/l	100
67) Ethyl Benzene	11.780	91	6177	0.381	ug/l	95
68) m/p-Xylenes	11.892	106	1823	0.287	ug/l	87
74) N-amyl acetate	12.286	43	3061	0.314	ug/l #	48
76) 1,2,3-Trichloropropane	12.669	75	124959	21.254	ug/l #	1
78) n-propylbenzene	12.857	91	4726	0.229	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.669	75	124959	57.400	ug/l #	10
85) sec-Butylbenzene	13.433	105	4025	0.214	ug/l	89
87) 1,3-Dichlorobenzene	13.545	146	2586	0.322	ug/l	91
88) 1,4-Dichlorobenzene	13.545	146	2586	0.318	ug/l	89
90) Hexachloroethane	14.157	117	3357	1.168	ug/l #	9
91) 1,2-Dichlorobenzene	13.921	146	23749	2.838	ug/l	99
95) Naphthalene	15.433	128	5793370	309.256	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062722\
Data File : VN073162.D
Acq On : 27 Jun 2022 15:14
Operator : JC\MD
Sample : N3494-17
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6

Quant Time: Jun 28 06:37:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




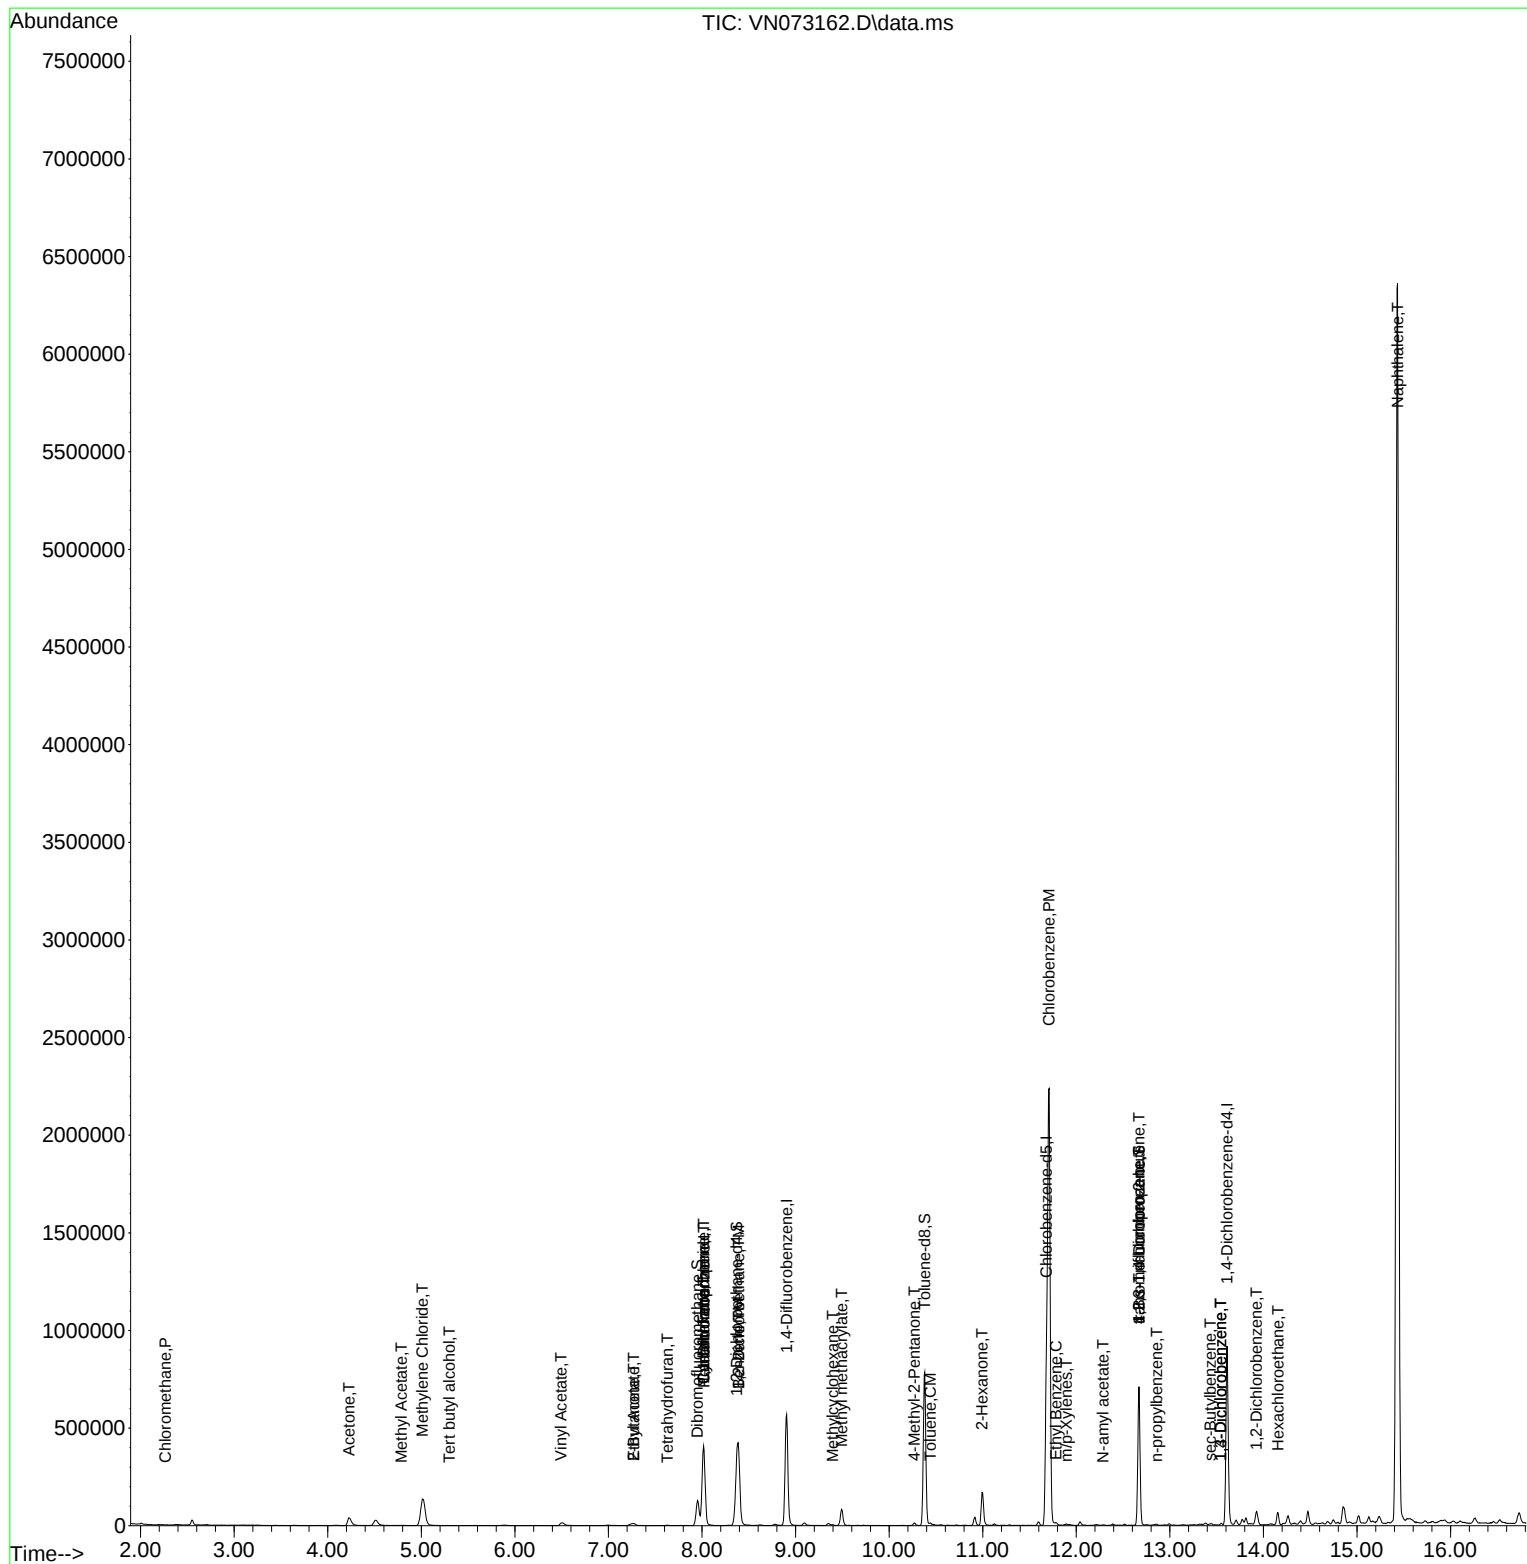




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.022 min Scan# 1
Delta R.T. 0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion:168 Resp: 308508
Ion Ratio Lower Upper
168 100
99 57.8 42.3 63.5

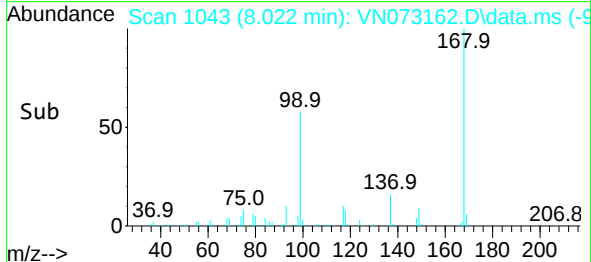

#3
Chloromethane
Concen: 0.747 ug/l
RT: 2.263 min Scan# 64
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 50 Resp: 569
Ion Ratio Lower Upper
50 100
52 35.9 25.7 38.5


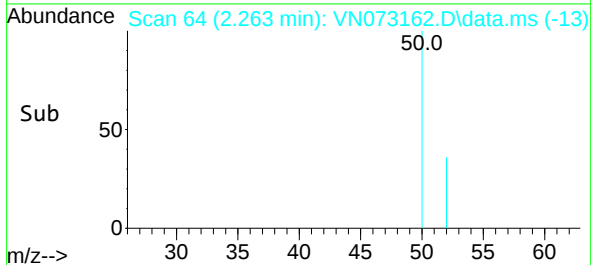

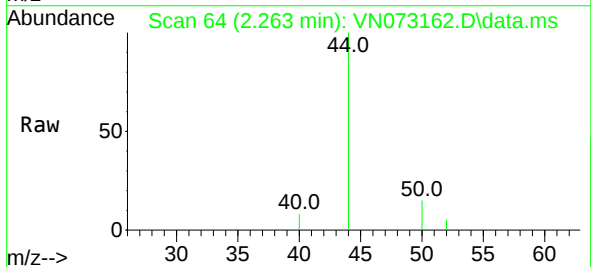




#11
Tert butyl alcohol
Concen: 0.264 ug/l
RT: 5.298 min Scan# 581
Delta R.T. -0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion: 59 Resp: 284
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

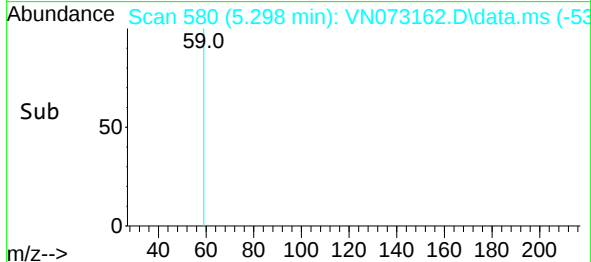

#16
Acetone
Concen: 33.739 ug/l
RT: 4.228 min Scan# 398
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 43 Resp: 77354
Ion Ratio Lower Upper
43 100
58 28.6 26.0 39.0


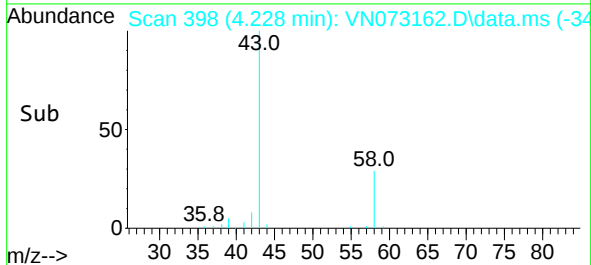

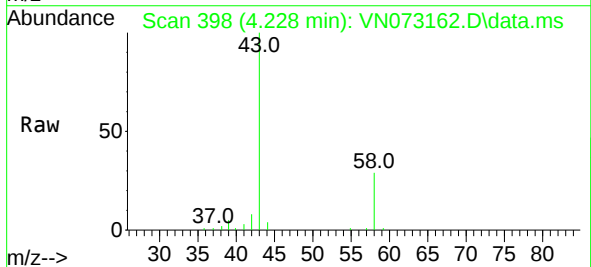




#18
Methyl Acetate
Concen: 0.437 ug/l
RT: 4.787 min Scan# 492
Delta R.T. 0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion: 43 Resp: 2671
Ion Ratio Lower Upper
43 100
74 5.1 21.6 32.4#

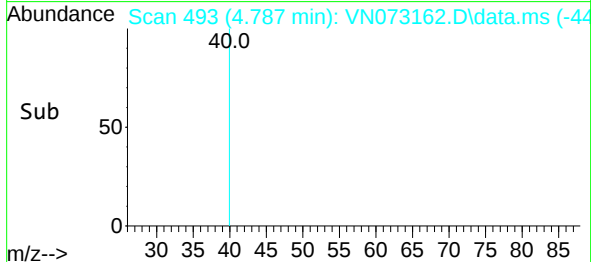

#20
Methylene Chloride
Concen: 31.951 ug/l
RT: 5.010 min Scan# 531
Delta R.T. -0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 84 Resp: 113937
Ion Ratio Lower Upper
84 100
49 119.3 88.3 132.5
51 37.1 28.2 42.2
86 62.2 50.6 76.0


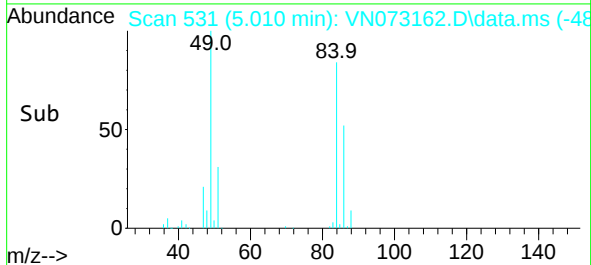

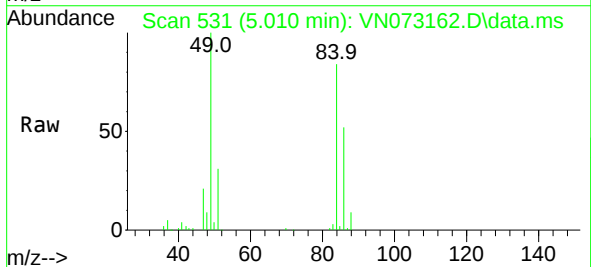




#23
 Vinyl Acetate
 Concen: 0.247 ug/l
 RT: 6.493 min Scan# 71
 Delta R.T. 0.141 min
 Lab File: VN073162.D
 Acq: 27 Jun 2022 15:14




Instrument :
 MSVOA_N
 ClientSampleId :
 SP-EXC-1-6


Tgt Ion: 43 Resp: 2680
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.0 15.0#

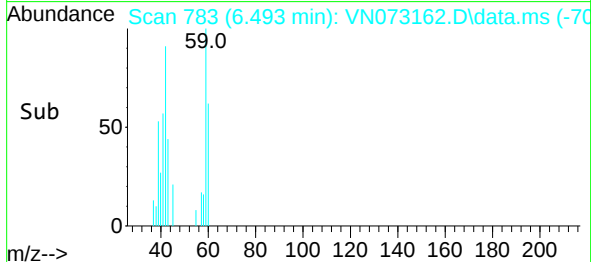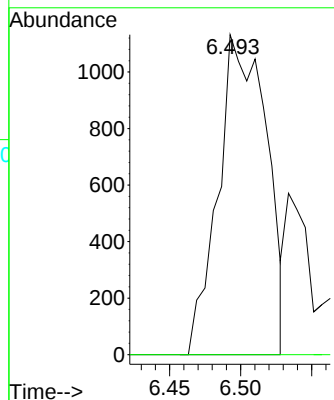

#25
 2-Butanone
 Concen: 4.612 ug/l
 RT: 7.269 min Scan# 915
 Delta R.T. 0.006 min
 Lab File: VN073162.D
 Acq: 27 Jun 2022 15:14

Tgt Ion: 43 Resp: 16779
 Ion Ratio Lower Upper
 43 100
 72 25.0 23.7 35.5


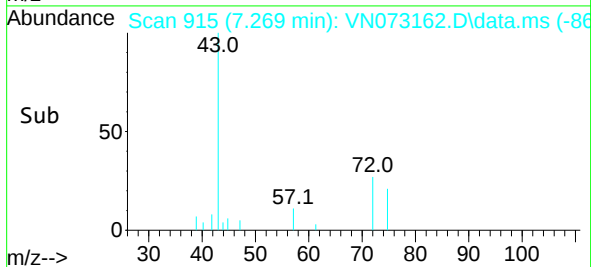
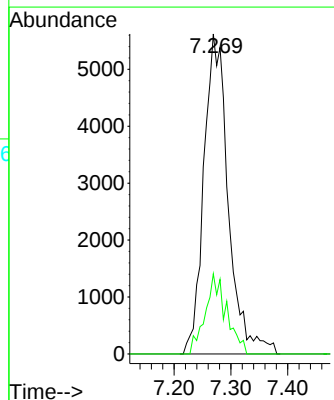
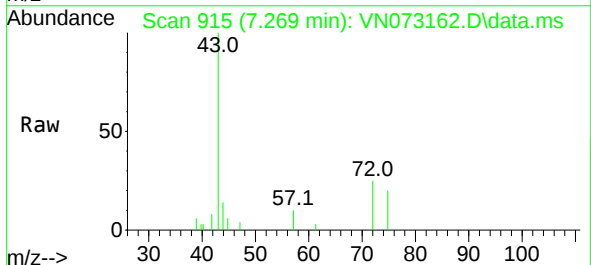




#26
2,2-Dichloropropane
Concen: Below Cal
RT: 7.263 min Scan# 912
Delta R.T. 0.012 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion: 77 Resp: 63
Ion Ratio Lower Upper
77 100
97 0.0 11.4 34.2#

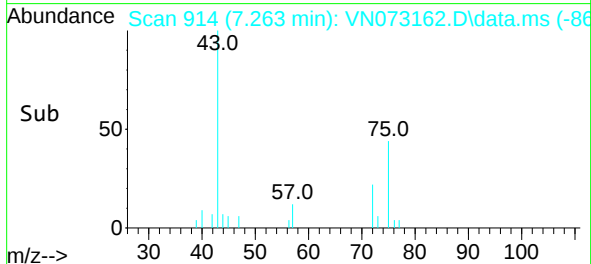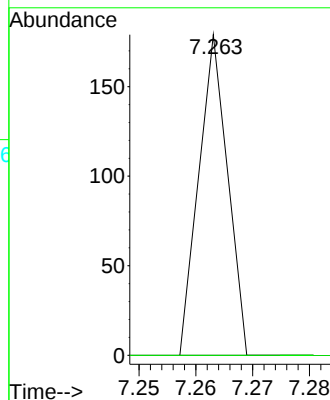

#29
Tetrahydrofuran
Concen: 0.531 ug/l
RT: 7.628 min Scan# 976
Delta R.T. 0.018 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14


Tgt Ion: 42 Resp: 1276
Ion Ratio Lower Upper
42 100
72 15.0 39.7 59.5#
71 27.7 36.6 55.0#

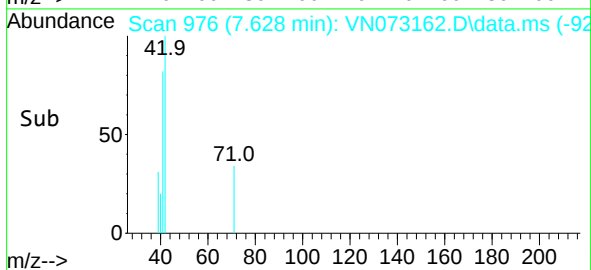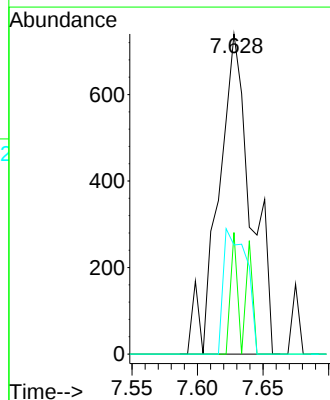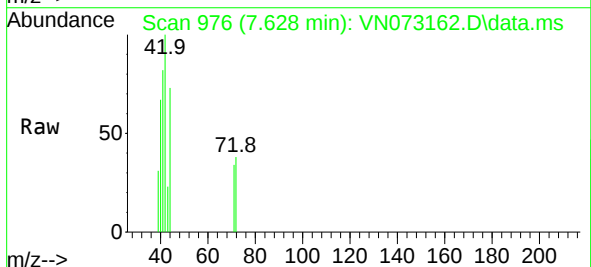






#31
Cyclohexane
Concen: 1.416 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6



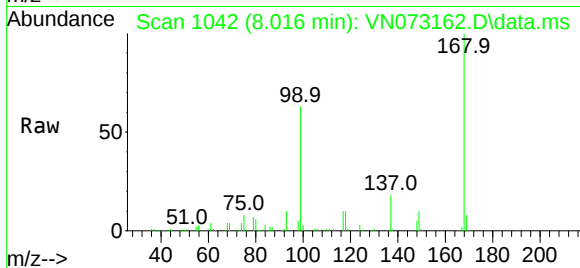



Tgt Ion: 56 Resp: 7989
Ion Ratio Lower Upper
56 100
69 151.9 27.8 41.8#
84 117.4 76.9 115.3#

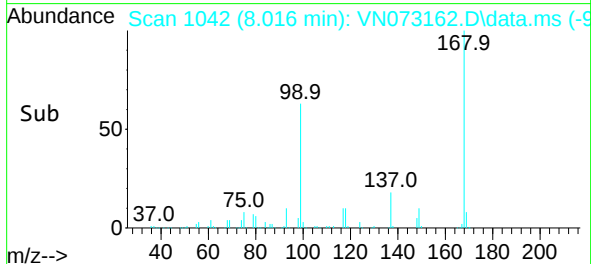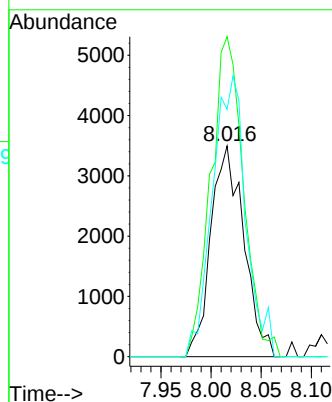

#33
1,2-Dichloroethane-d4
Concen: 45.828 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 65 Resp: 191146
Ion Ratio Lower Upper
65 100
67 51.0 0.0 104.8

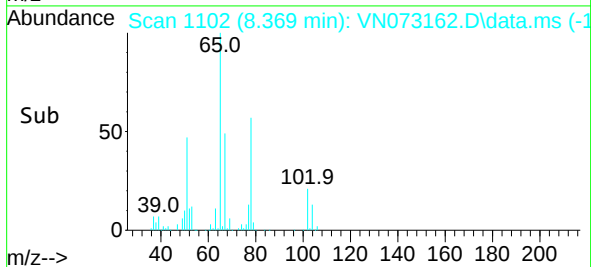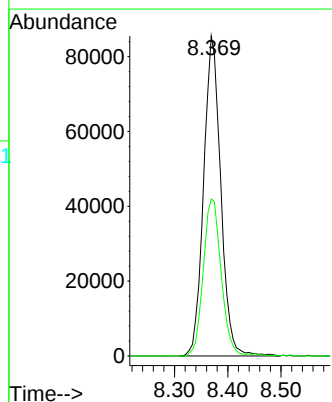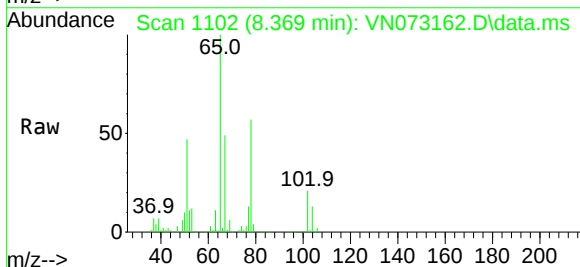

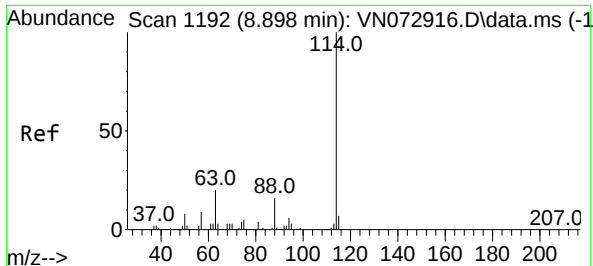

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1192

Delta R.T. 0.006 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14

Instrument :

MSVOA_N

ClientSampleId :

SP-EXC-1-6





Tgt Ion:114 Resp: 507257

Ion Ratio Lower Upper

114 100

63 21.2 0.0 40.0

88 15.1 0.0 32.6

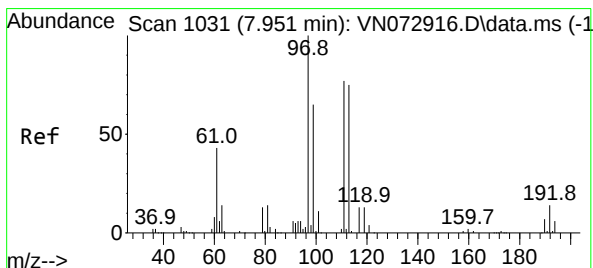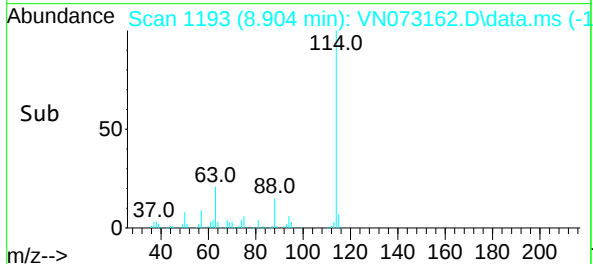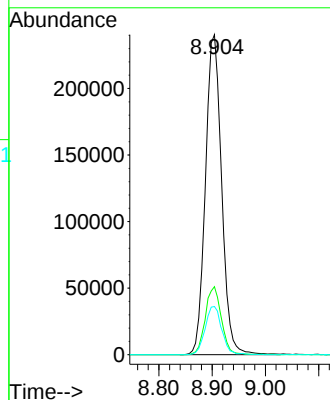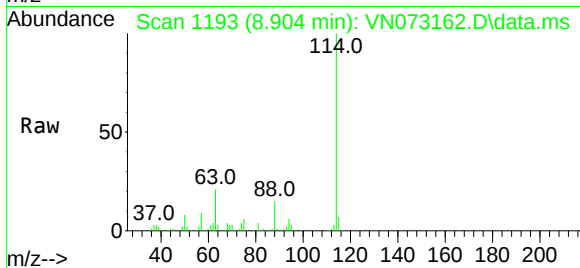

#35

Dibromofluoromethane

Concen: 29.798 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14




Tgt Ion:113 Resp: 93427


Ion Ratio Lower Upper

113 100

111 103.8 81.4 122.0

192 18.5 17.0 25.6

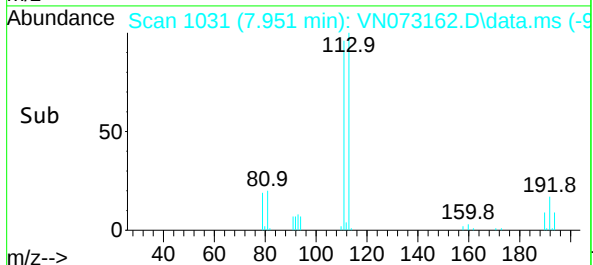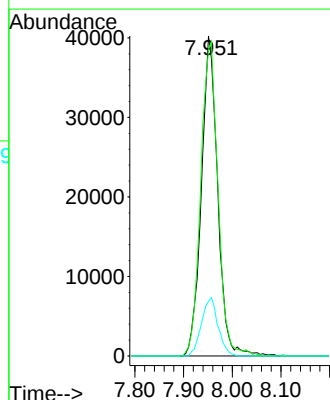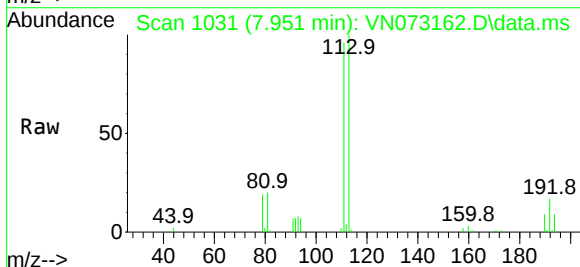



#36

1,1-Dichloropropene

Concen: 5.953 ug/l

RT: 8.016 min Scan# 1

Delta R.T. -0.135 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14

Instrument :

MSVOA_N

ClientSampleId :

SP-EXC-1-6





Tgt Ion: 75 Resp: 25254

Ion Ratio Lower Upper

75 100

110 8.7 18.3 54.8#

77 0.0 25.1 37.7#

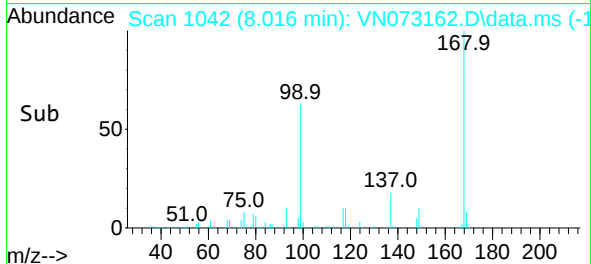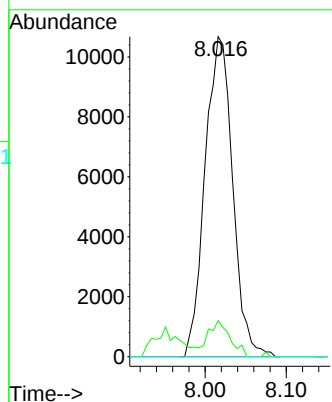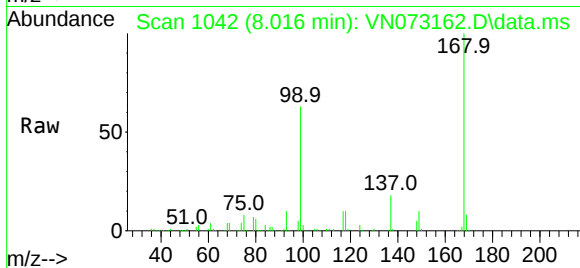

#37

Ethyl Acetate

Concen: 2.473 ug/l

RT: 7.269 min Scan# 915

Delta R.T. -0.076 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14




Tgt Ion: 43 Resp: 16779


Ion Ratio Lower Upper

43 100

61 0.3 11.8 17.6#

70 0.0 9.3 13.9#


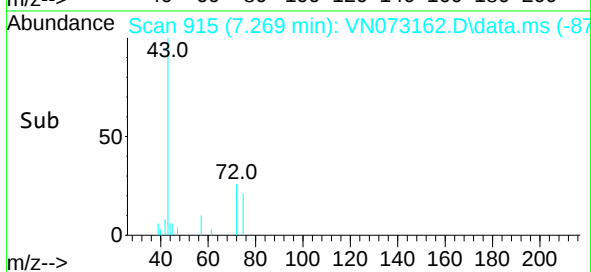
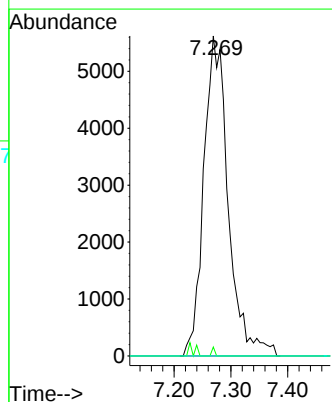
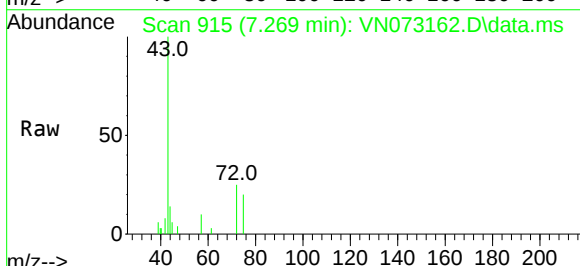


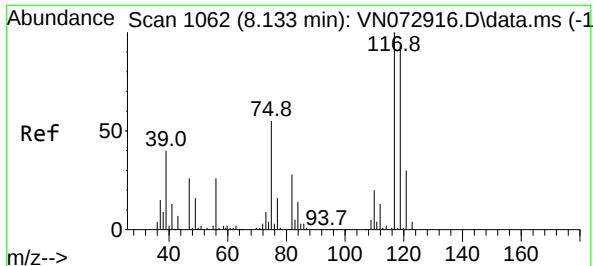

#38
Carbon Tetrachloride
Concen: 7.048 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.117 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion:117 Resp: 31452
Ion Ratio Lower Upper
117 100
119 6.3 75.8 113.8#
121 0.0 24.6 37.0#

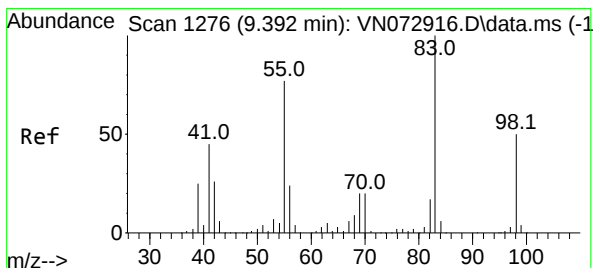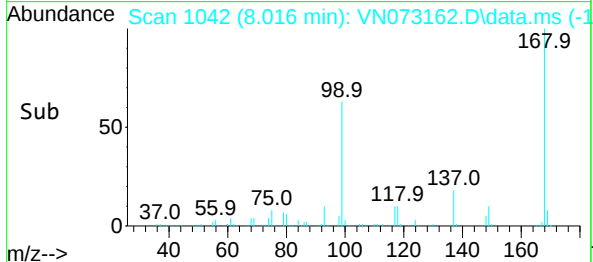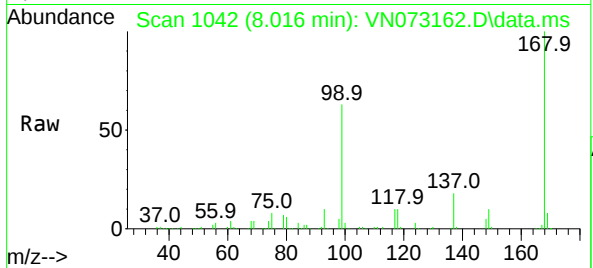

#39
Methylcyclohexane
Concen: 0.430 ug/l
RT: 9.398 min Scan# 1277
Delta R.T. 0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 83 Resp: 2198
Ion Ratio Lower Upper
83 100
55 64.5 57.8 86.8
98 49.4 39.4 59.2


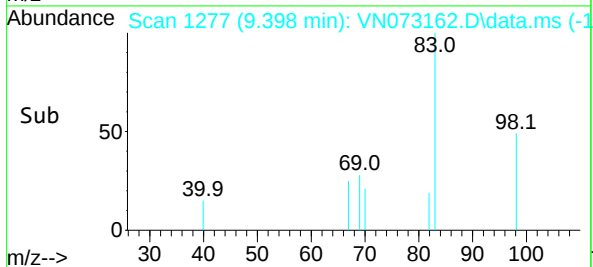

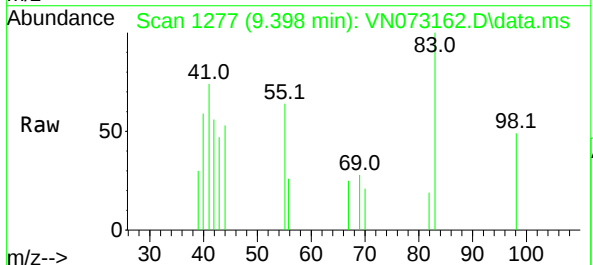


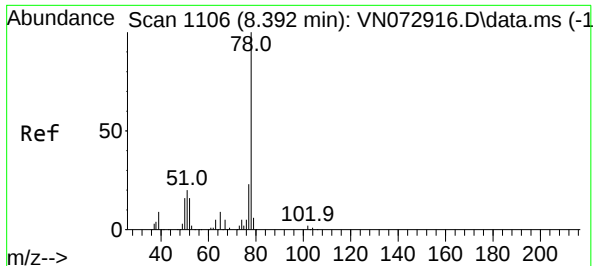

#40
Benzene
Concen: 23.613 ug/l
RT: 8.392 min Scan# 1106
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion: 78 Resp: 314830
Ion Ratio Lower Upper
78 100
77 24.1 19.4 29.0

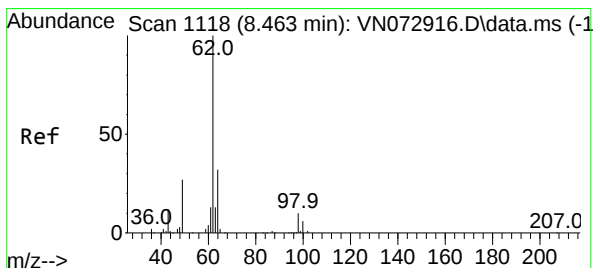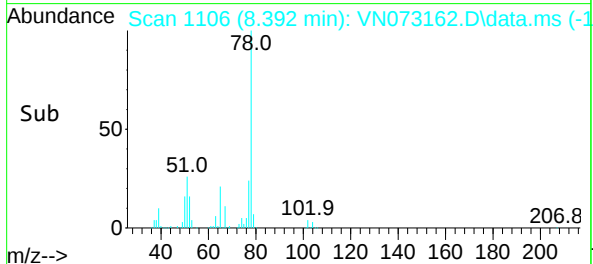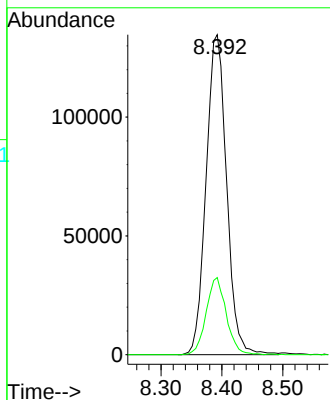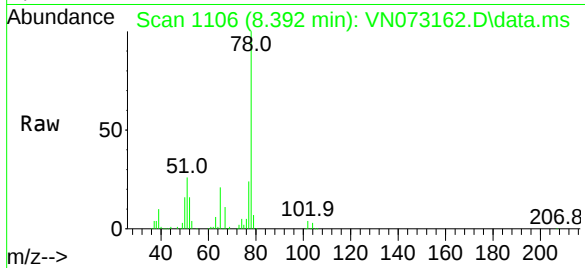

#42
1,2-Dichloroethane
Concen: 0.659 ug/l
RT: 8.392 min Scan# 1106
Delta R.T. -0.070 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 62 Resp: 3123
Ion Ratio Lower Upper
62 100
98 1.8 0.0 19.4

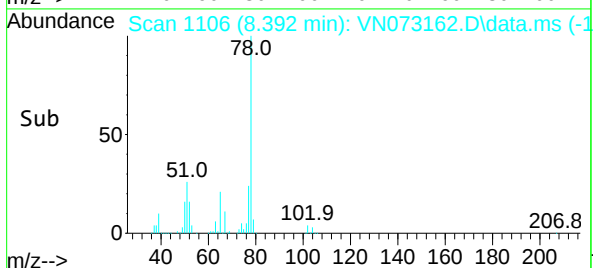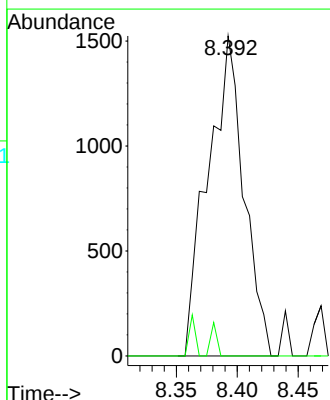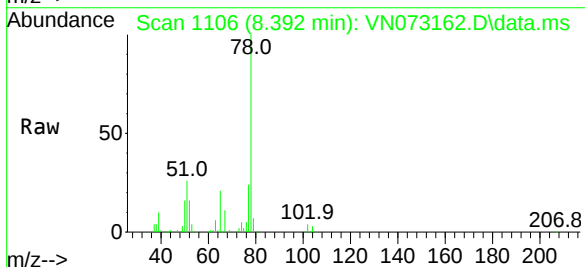

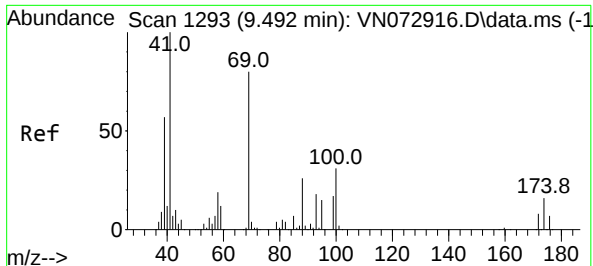

#48

Methyl methacrylate

Concen: 1.622 ug/l

RT: 9.492 min Scan# 1293

Delta R.T. 0.000 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14

Instrument :

MSVOA_N

ClientSampleId :

SP-EXC-1-6





Tgt Ion: 41 Resp: 7184

Ion Ratio Lower Upper

41 100

69 0.9 74.7 112.1#

39 58.3 45.6 68.4

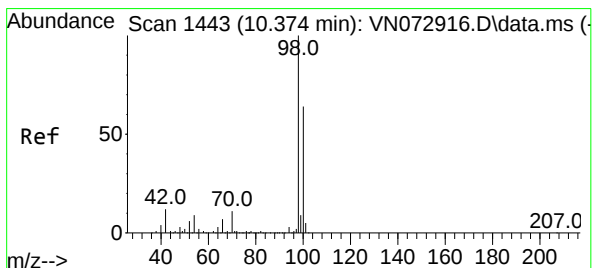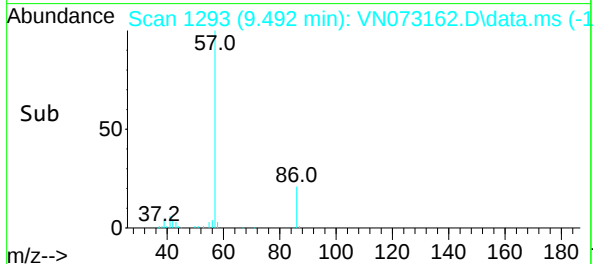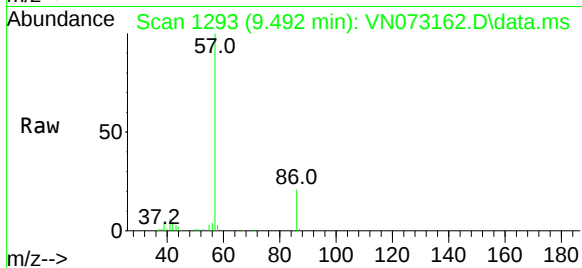

#50

Toluene-d8

Concen: 45.815 ug/l

RT: 10.381 min Scan# 1444

Delta R.T. 0.006 min

Lab File: VN073162.D




Acq: 27 Jun 2022 15:14


Tgt Ion: 98 Resp: 534498

Ion Ratio Lower Upper

98 100

100 66.4 52.6 78.8


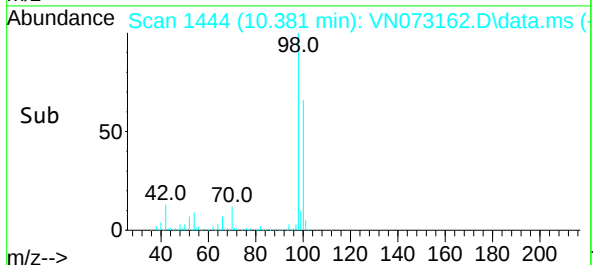
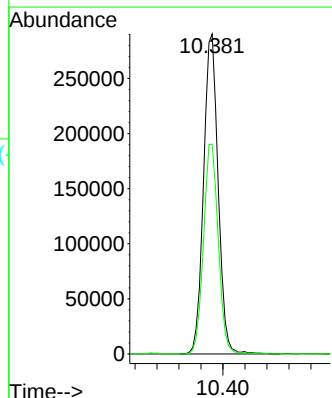
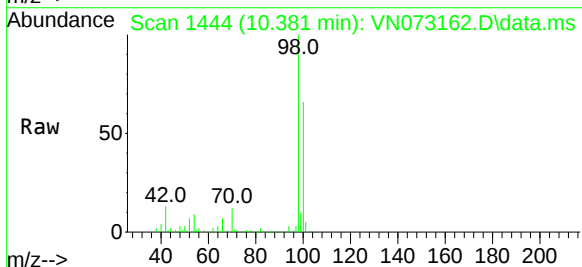


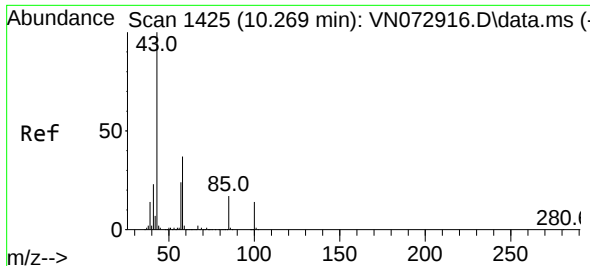

#51
4-Methyl-2-Pentanone
Concen: 1.560 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion: 43 Resp: 9866
Ion Ratio Lower Upper
43 100
58 34.8 34.1 51.1

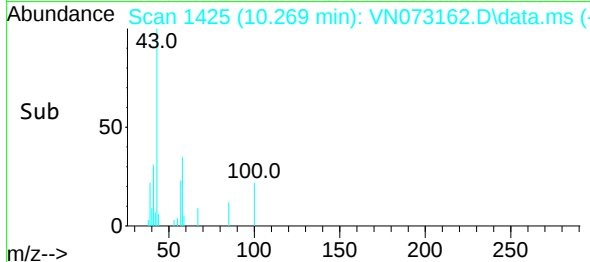

#52
Toluene
Concen: 0.470 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 92 Resp: 3849
Ion Ratio Lower Upper
92 100
91 196.0 138.6 207.8


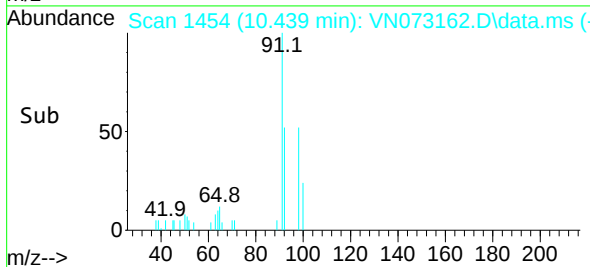

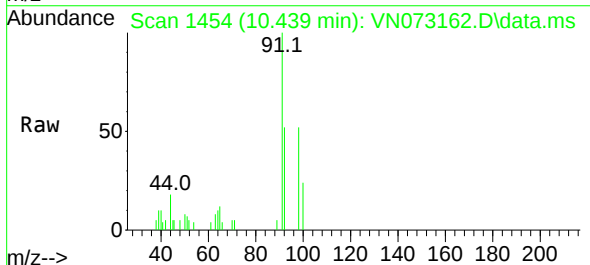




#59
2-Hexanone
Concen: 29.881 ug/l
RT: 10.992 min Scan# 1548
Delta R.T. -0.029 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion: 43 Resp: 146191
Ion Ratio Lower Upper
43 100
58 0.0 29.7 89.1#

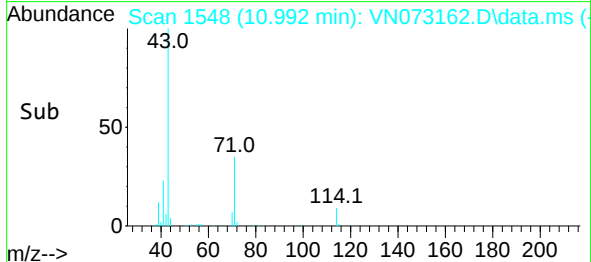

#62
4-Bromofluorobenzene
Concen: 57.772 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 95 Resp: 242359
Ion Ratio Lower Upper
95 100
174 74.6 0.0 167.6
176 72.3 0.0 163.4

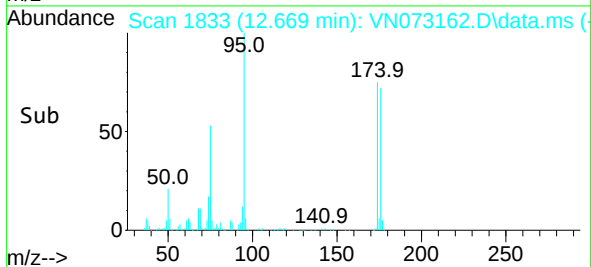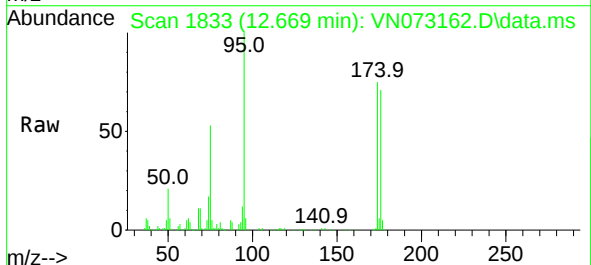



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.680 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14

Instrument :

MSVOA_N

ClientSampleId :

SP-EXC-1-6





Tgt Ion:117 Resp: 471196

Ion Ratio Lower Upper

117 100

82 56.4 44.2 66.2

119 32.5 25.4 38.0

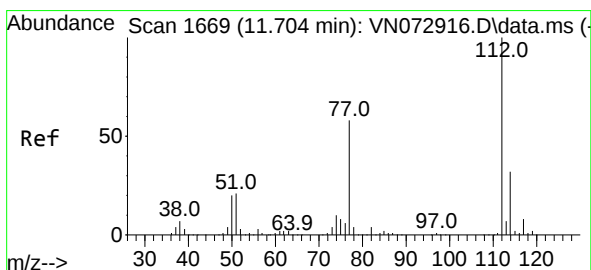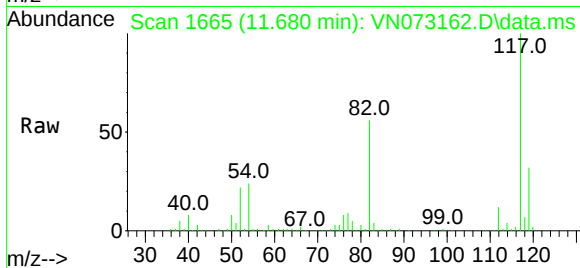

#65

Chlorobenzene

Concen: 129.582 ug/l

RT: 11.710 min Scan# 1670

Delta R.T. 0.006 min

Lab File: VN073162.D




Acq: 27 Jun 2022 15:14


Tgt Ion:112 Resp: 1192444

Ion Ratio Lower Upper

112 100

114 31.6 25.4 38.2


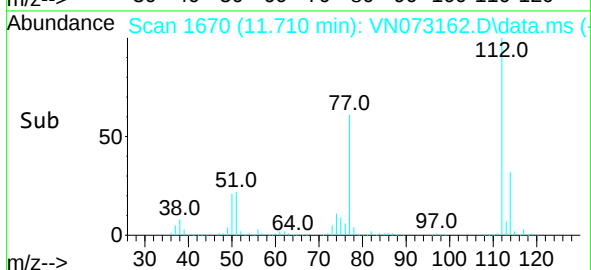

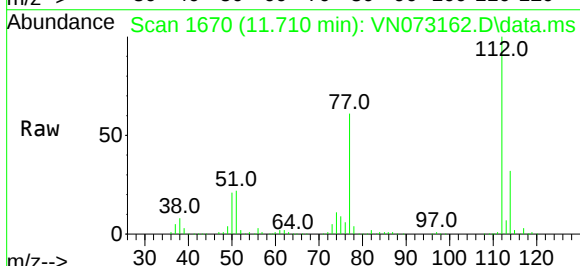




#67
Ethyl Benzene
Concen: 0.381 ug/l
RT: 11.780 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion: 91 Resp: 6177
Ion Ratio Lower Upper
91 100
106 28.3 24.9 37.3

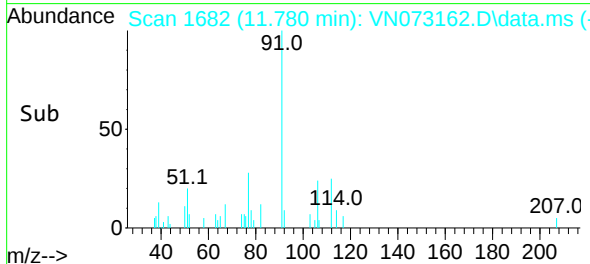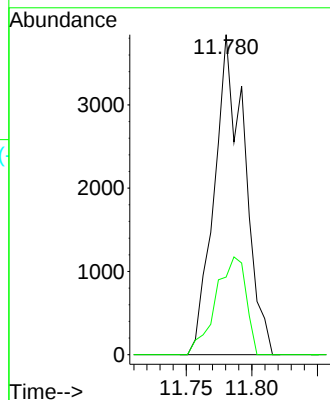

#68
m/p-Xylenes
Concen: 0.287 ug/l
RT: 11.892 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 106 Resp: 1823
Ion Ratio Lower Upper
106 100
91 218.8 158.9 238.3

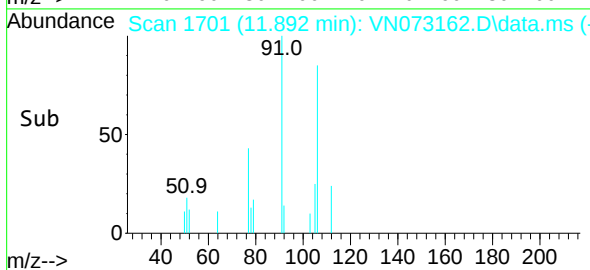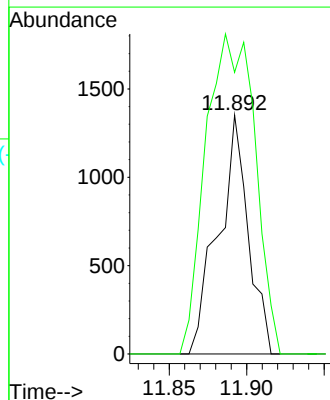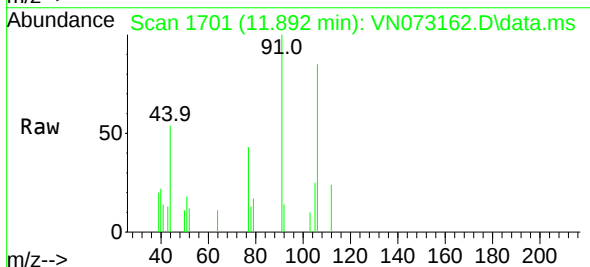



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.610 min Scan# 1993

Delta R.T. 0.000 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14

Instrument :

MSVOA_N

ClientSampleId :

SP-EXC-1-6





Tgt Ion:152 Resp: 242495

Ion Ratio Lower Upper

152 100

115 60.2 28.9 86.7

150 157.5 0.0 356.2

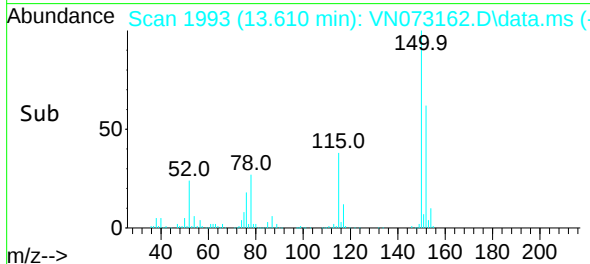

#74

N-ethyl acetate

Concen: 0.314 ug/l

RT: 12.286 min Scan# 1768

Delta R.T. -0.041 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14

Tgt Ion: 43 Resp: 3061




Ion Ratio Lower Upper


43 100

70 0.0 39.0 58.4#

55 18.9 21.1 31.7#

61 0.0 21.1 31.7#

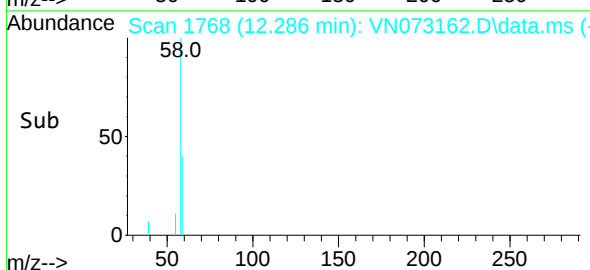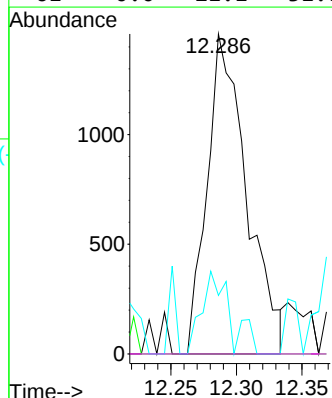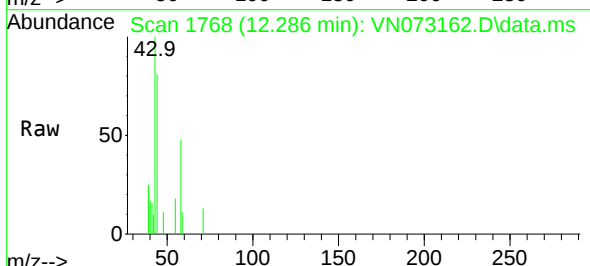



#76

1,2,3-Trichloropropane

Concen: 21.254 ug/l

RT: 12.669 min Scan# 1833

Delta R.T. -0.147 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14

Instrument :

MSVOA_N

ClientSampleId :





SP-EXC-1-6

Tgt Ion: 75 Resp: 124959

Ion Ratio Lower Upper

75 100

77 1.3 98.5 295.5#

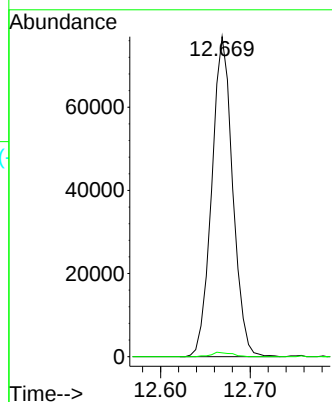

#78

n-propylbenzene

Concen: 0.229 ug/l

RT: 12.857 min Scan# 1865

Delta R.T. 0.000 min

Lab File: VN073162.D




Acq: 27 Jun 2022 15:14


Tgt Ion: 91 Resp: 4726

Ion Ratio Lower Upper

91 100

120 25.1 11.9 35.5


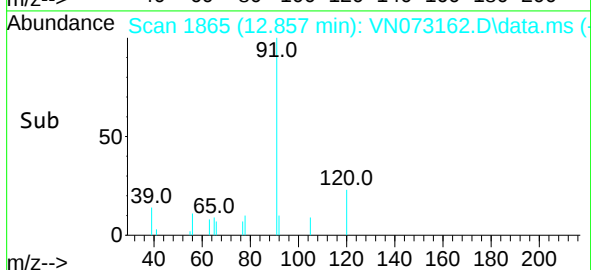






#81
trans-1,4-Dichloro-2-butene
Concen: 57.400 ug/l
RT: 12.669 min Scan# 1815
Delta R.T. 0.106 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion: 75 Resp: 124959
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

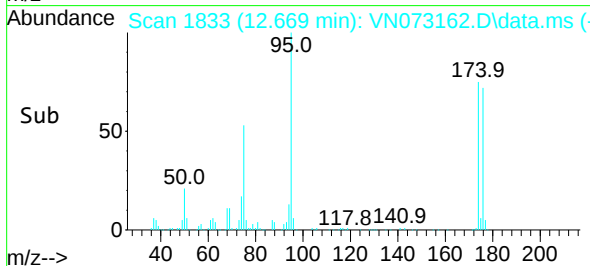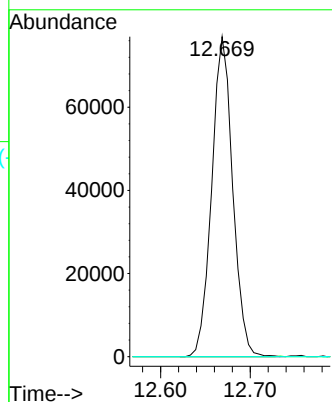

#85
sec-Butylbenzene
Concen: 0.214 ug/l
RT: 13.433 min Scan# 1963
Delta R.T. -0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Tgt Ion: 105 Resp: 4025
Ion Ratio Lower Upper
105 100
134 15.8 10.4 31.1

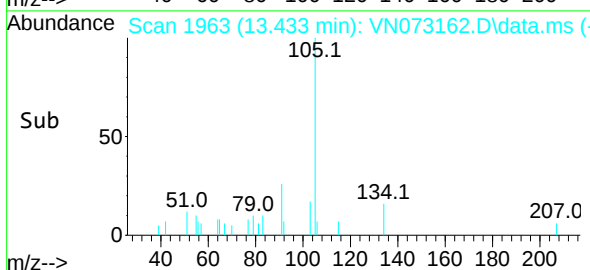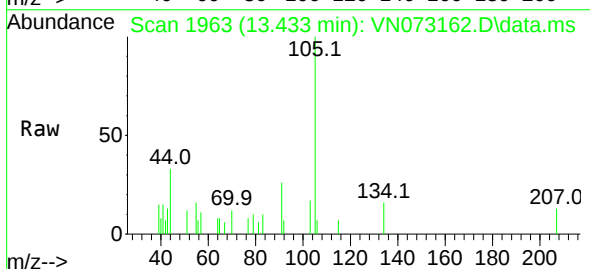

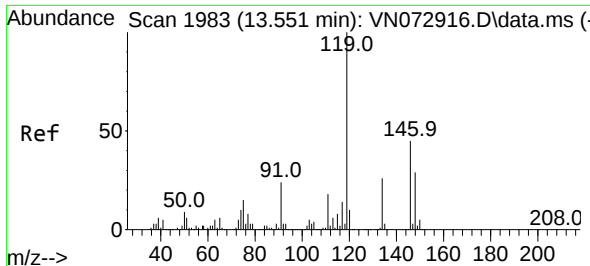

#87

1,3-Dichlorobenzene

Concen: 0.322 ug/l

RT: 13.545 min Scan# 1982

Delta R.T. -0.006 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14

Instrument :

MSVOA_N

ClientSampleId :

SP-EXC-1-6





Tgt Ion:146 Resp: 2586

Ion Ratio Lower Upper

146 100

111 44.4 20.0 60.0

148 71.7 32.0 96.0

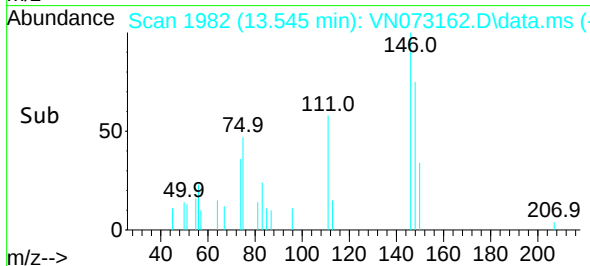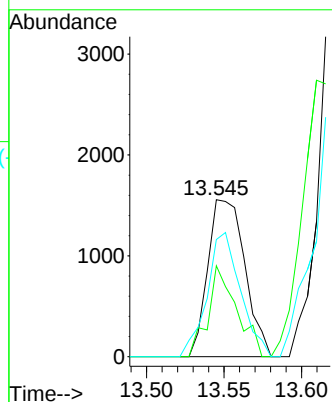

#88

1,4-Dichlorobenzene

Concen: 0.318 ug/l

RT: 13.545 min Scan# 1982

Delta R.T. -0.082 min

Lab File: VN073162.D

Acq: 27 Jun 2022 15:14




Tgt Ion:146 Resp: 2586


Ion Ratio Lower Upper

146 100

111 44.4 19.1 57.1

148 71.7 31.4 94.3


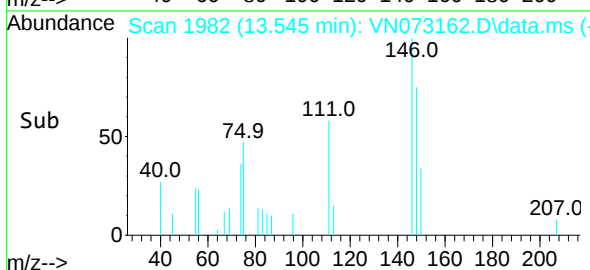

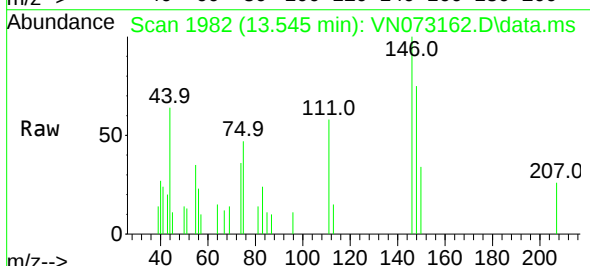




#90
Hexachloroethane
Concen: 1.168 ug/l
RT: 14.157 min Scan# 2086
Delta R.T. 0.012 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6


Tgt Ion:117 Resp: 3357
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

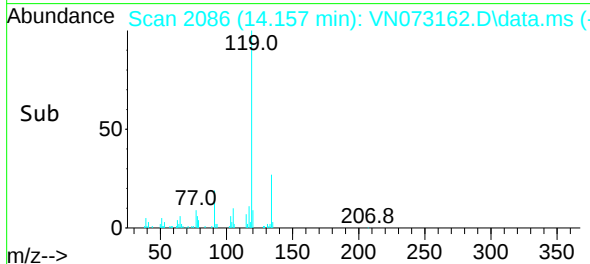

#91
1,2-Dichlorobenzene
Concen: 2.838 ug/l
RT: 13.921 min Scan# 2046
Delta R.T. 0.000 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14


Tgt Ion:146 Resp: 23749
Ion Ratio Lower Upper
146 100
111 41.1 20.9 62.8
148 64.7 32.1 96.3

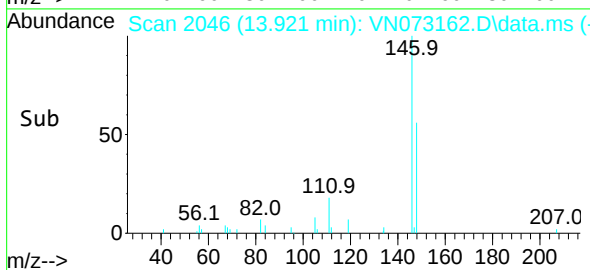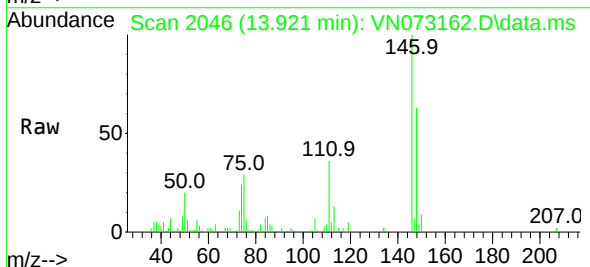

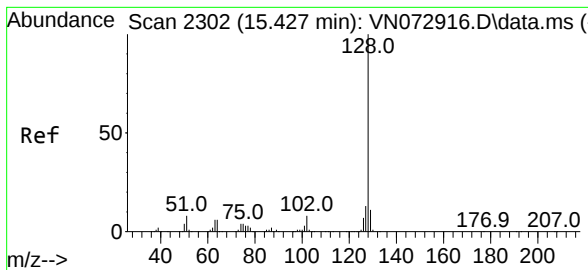

#95
Naphthalene
Concen: 309.256 ug/l
RT: 15.433 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN073162.D
Acq: 27 Jun 2022 15:14

Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-1-6

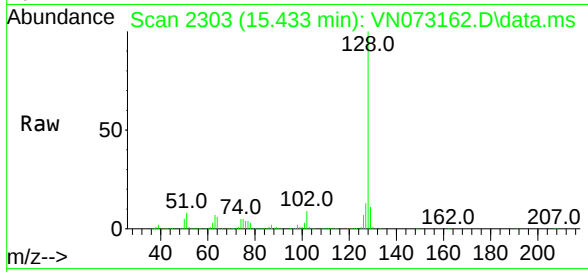

Tgt Ion:128 Resp: 5793370
Ion Ratio Lower Upper
128 100
127 13.2 10.3 15.5
129 11.0 8.6 13.0

