

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062722\
 Data File : VN073170.D
 Acq On : 27 Jun 2022 18:29
 Operator : JC\MD
 Sample : N3436-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 31677

Quant Time: Jun 28 06:39:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	334712	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	530212	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	485535	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	247404	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.375	65	198545	43.875	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	87.760%
35) Dibromofluoromethane	7.951	113	170374	51.988	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.980%
50) Toluene-d8	10.380	98	564504	46.292	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	92.580%
62) 4-Bromofluorobenzene	12.668	95	249043	56.795	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	113.580%


Target Compounds						Qvalue
3) Chloromethane	2.269	50	456	0.701	ug/l #	43
5) Bromomethane	2.828	94	263	0.234	ug/l #	2
11) Tert butyl alcohol	5.287	59	5934	5.076	ug/l #	72
15) Acrylonitrile	5.475	53	5152	1.912	ug/l #	93
16) Acetone	4.222	43	108748	43.718	ug/l	93
17) Carbon Disulfide	4.457	76	150059	18.276	ug/l	99
20) Methylene Chloride	5.022	84	709	Below Cal	#	53
22) Diisopropyl ether	6.498	45	5042	0.395	ug/l #	1
23) Vinyl Acetate	6.498	43	11277	0.957	ug/l #	68
25) 2-Butanone	7.269	43	32178	8.152	ug/l #	89
29) Tetrahydrofuran	7.622	42	8273	3.174	ug/l	95
31) Cyclohexane	8.022	56	8166	1.334	ug/l #	17
36) 1,1-Dichloropropene	8.016	75	27191	6.132	ug/l #	48
37) Ethyl Acetate	7.269	43	32178	4.537	ug/l #	67
38) Carbon Tetrachloride	8.016	117	34001	7.290	ug/l #	15
39) Methylcyclohexane	9.404	83	1447	0.271	ug/l #	71
40) Benzene	8.392	78	57460	4.123	ug/l	96
41) Methacrylonitrile	7.622	41	5483	1.630	ug/l #	24
48) Methyl methacrylate	9.474	41	1345	0.291	ug/l #	35
49) 1,4-Dioxane	9.504	88	60	0.576	ug/l #	1
51) 4-Methyl-2-Pentanone	10.269	43	6297	0.952	ug/l #	69
52) Toluene	10.439	92	37151	4.342	ug/l	99
59) 2-Hexanone	11.027	43	6524	1.276	ug/l	85
67) Ethyl Benzene	11.786	91	7894	0.473	ug/l	98
68) m/p-Xylenes	11.892	106	14360	2.193	ug/l	92
69) o-Xylene	12.215	106	5450	0.833	ug/l	84
70) Styrene	12.227	104	2593	0.247	ug/l #	59
74) N-amyl acetate	12.292	43	15683	1.579	ug/l #	39
76) 1,2,3-Trichloropropane	12.668	75	130984	21.837	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.498	75	198473	89.359	ug/l #	21
84) 1,2,4-Trimethylbenzene	13.304	105	9852	0.629	ug/l	90
95) Naphthalene	15.427	128	25095	1.313	ug/l #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062722\
Data File : VN073170.D
Acq On : 27 Jun 2022 18:29
Operator : JC\MD
Sample : N3436-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
31677

Quant Time: Jun 28 06:39:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




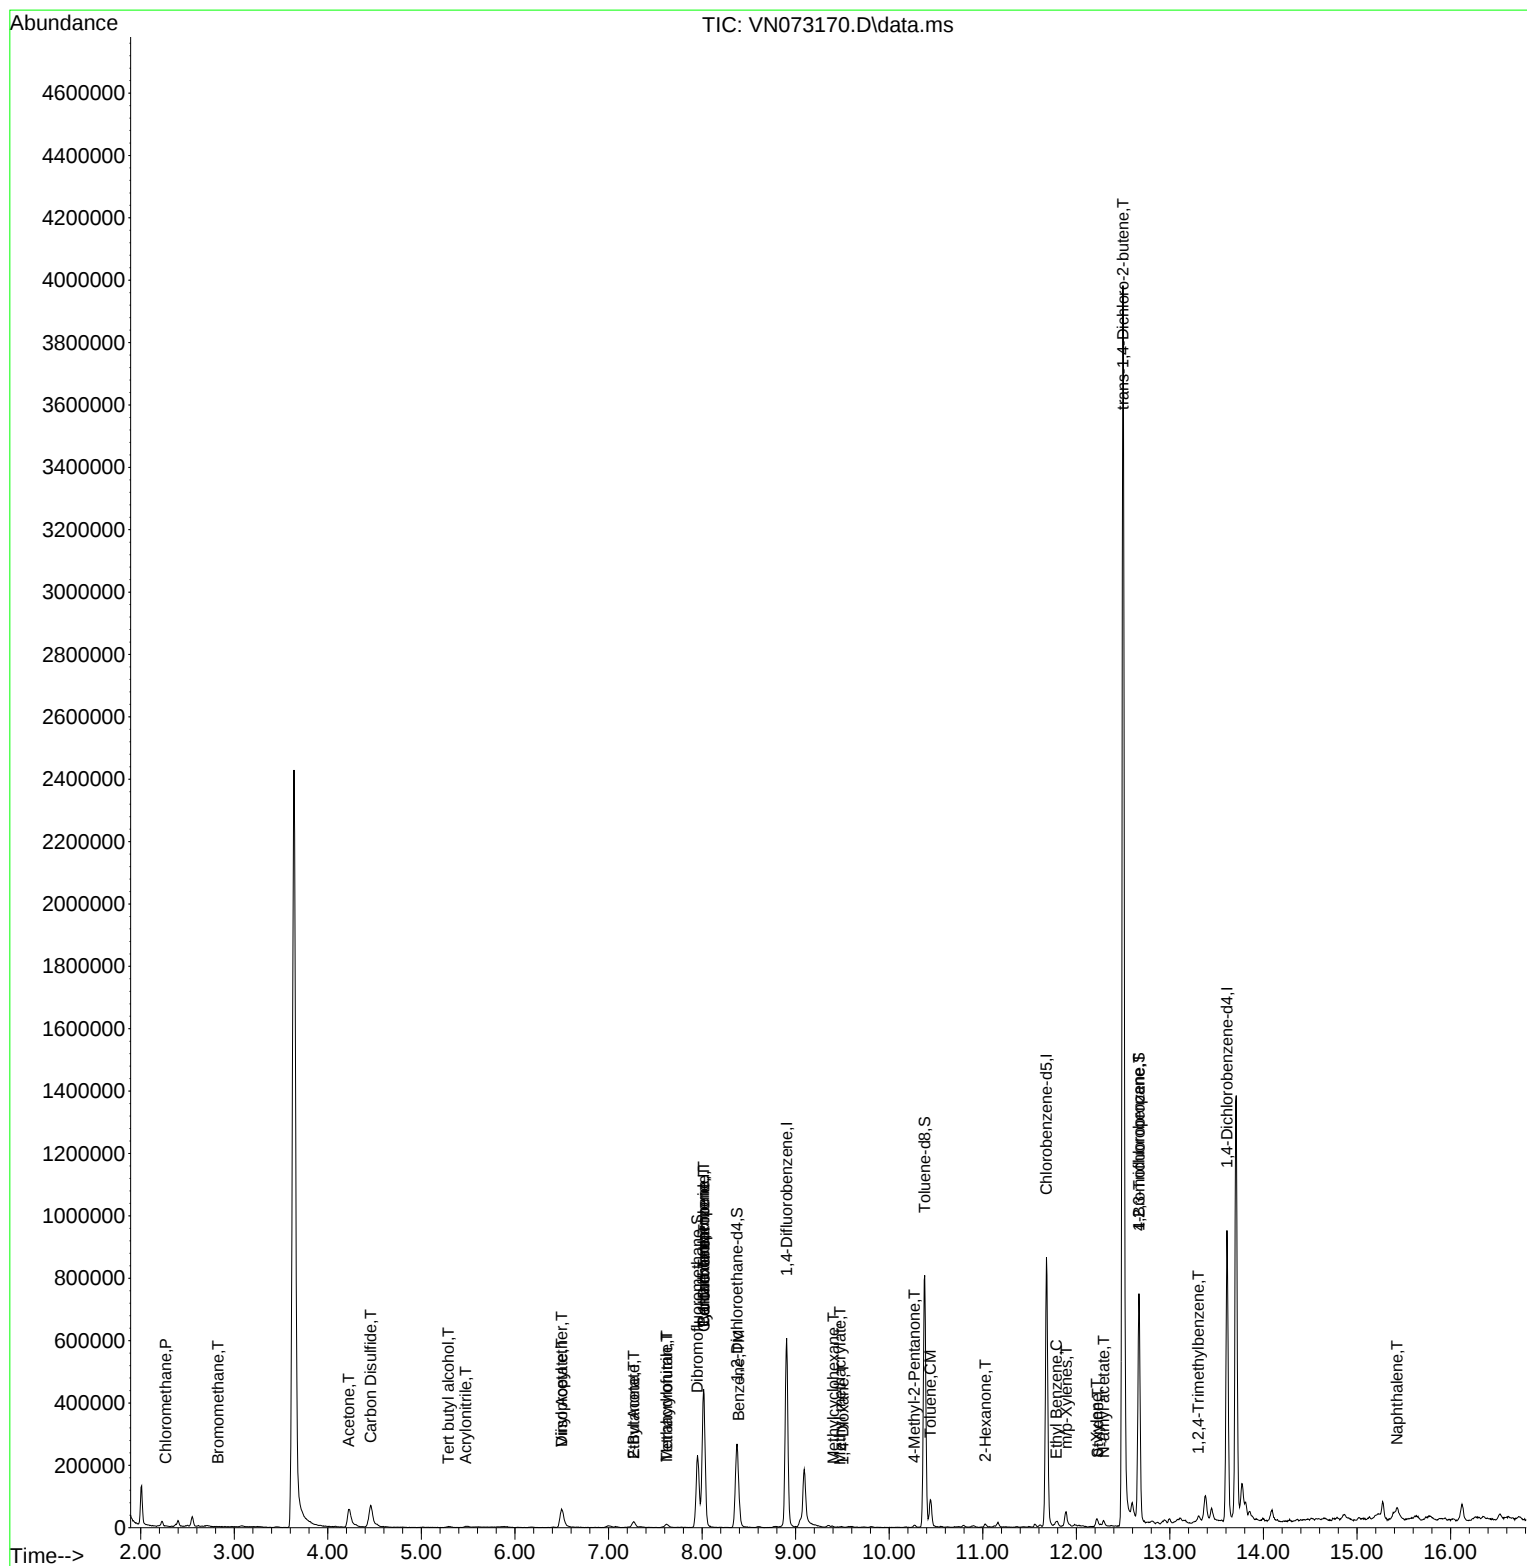




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion:168 Resp: 334712
Ion Ratio Lower Upper
168 100
99 61.3 42.3 63.5

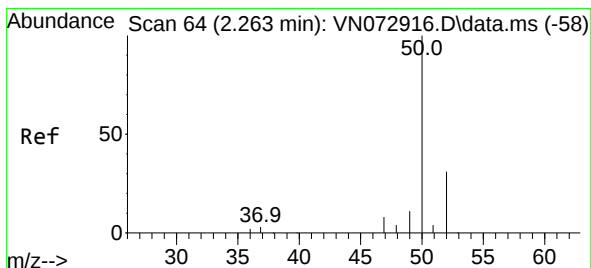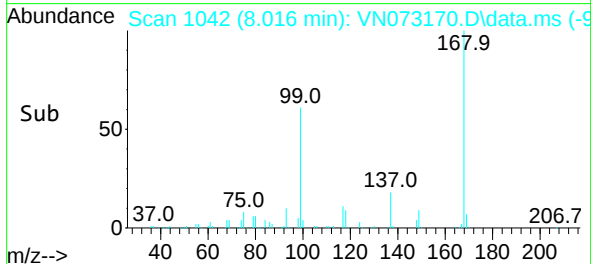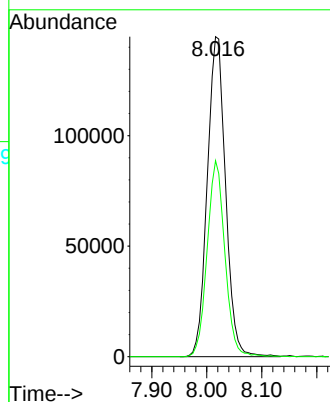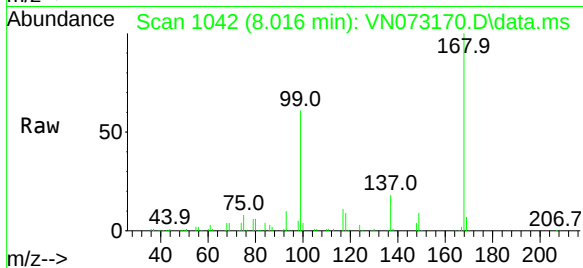

#3
Chloromethane
Concen: 0.701 ug/l
RT: 2.269 min Scan# 65
Delta R.T. 0.006 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 50 Resp: 456
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#


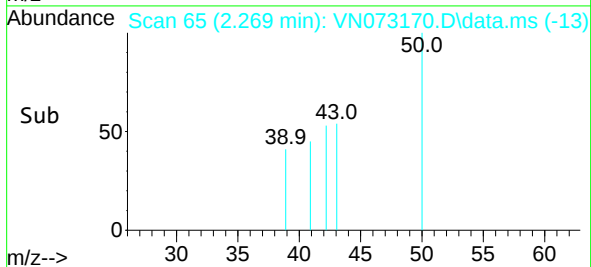
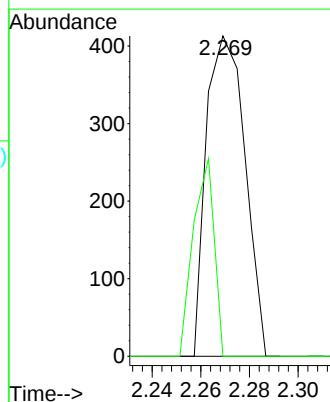
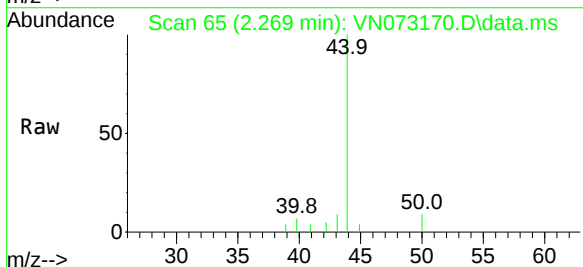


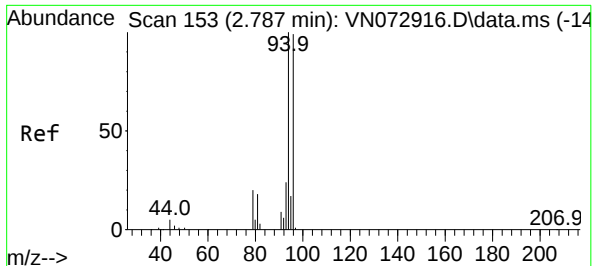

#5
Bromomethane
Concen: 0.234 ug/l
RT: 2.828 min Scan# 11
Delta R.T. 0.041 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion: 94 Resp: 263
Ion Ratio Lower Upper
94 100
96 0.0 76.0 114.0#

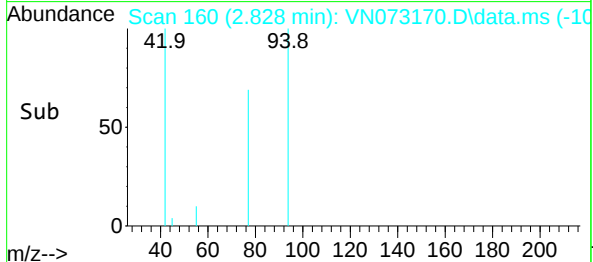

#11
Tert butyl alcohol
Concen: 5.076 ug/l
RT: 5.287 min Scan# 578
Delta R.T. -0.018 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29


Tgt Ion: 59 Resp: 5934
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

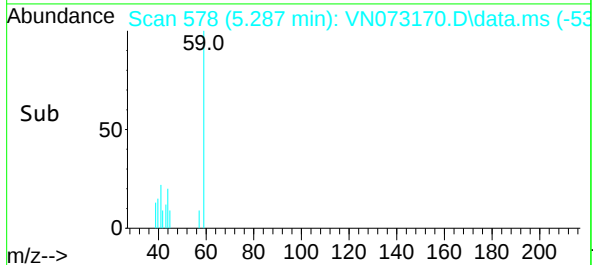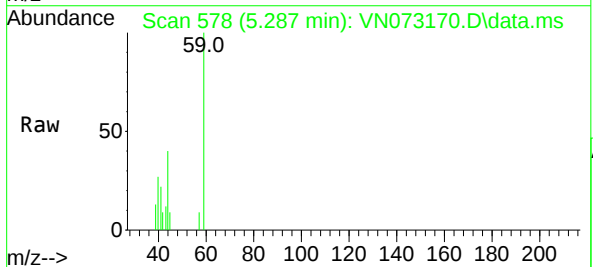






#15
Acrylonitrile
Concen: 1.912 ug/l
RT: 5.475 min Scan# 610
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Instrument :
MSVOA_N
ClientSampleId :
31677



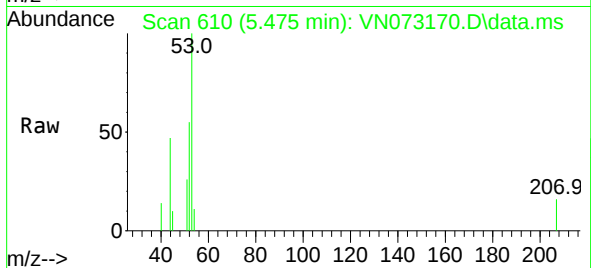



Tgt Ion: 53 Resp: 5152
Ion Ratio Lower Upper
53 100
52 83.9 66.4 99.6
51 23.7 28.5 42.7#

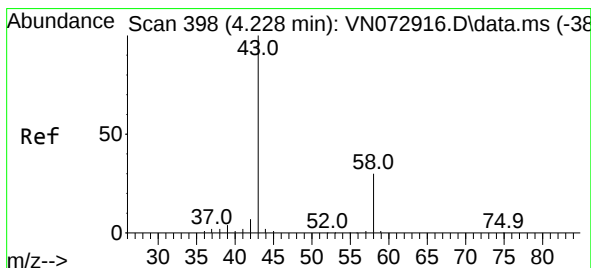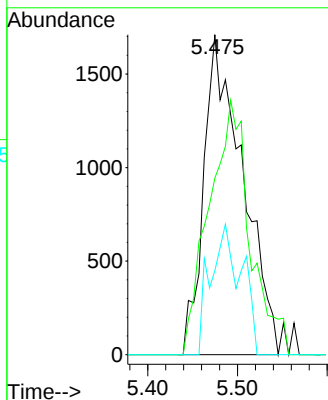

#16
Acetone
Concen: 43.718 ug/l
RT: 4.222 min Scan# 397
Delta R.T. -0.006 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29


Tgt Ion: 43 Resp: 108748
Ion Ratio Lower Upper
43 100
58 28.6 26.0 39.0

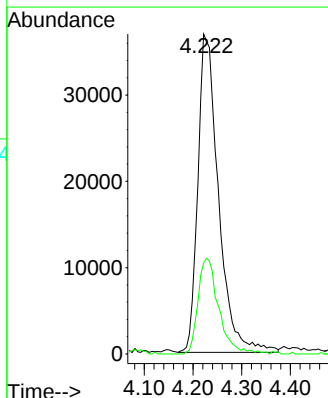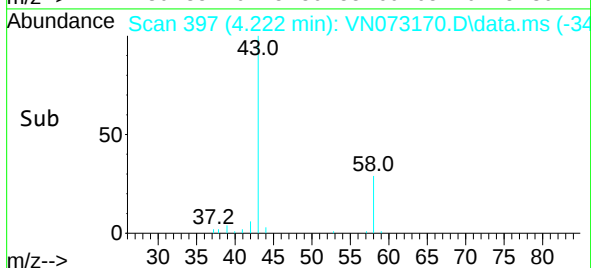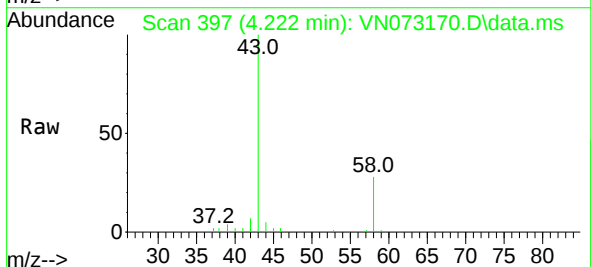



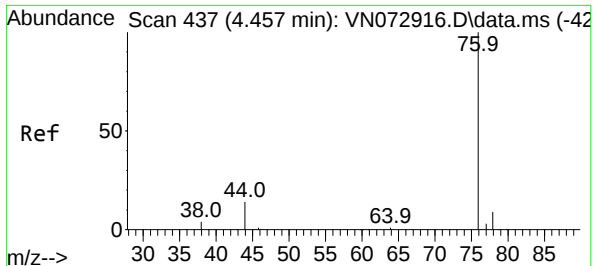


#17
Carbon Disulfide
Concen: 18.276 ug/l
RT: 4.457 min Scan# 41
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Instrument :
MSVOA_N
ClientSampleId :
31677







Tgt Ion: 76 Resp: 150059
Ion Ratio Lower Upper
76 100
78 8.6 7.2 10.8

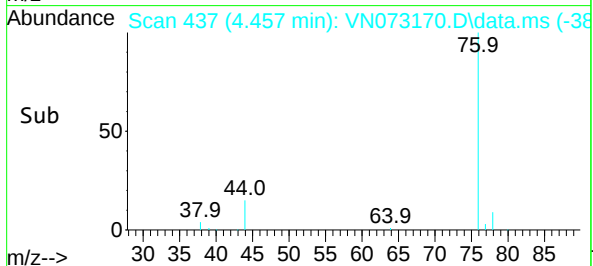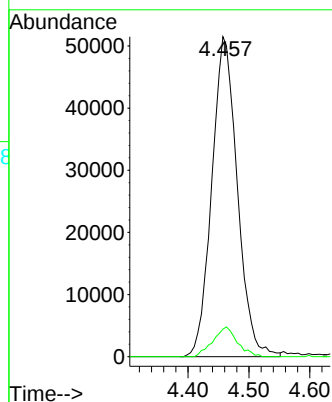

#22
Diisopropyl ether
Concen: 0.395 ug/l
RT: 6.498 min Scan# 784
Delta R.T. 0.082 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 45 Resp: 5042
Ion Ratio Lower Upper
45 100
43 175.2 46.6 70.0#
87 0.0 24.3 36.5#
59 646.1 9.6 14.4#


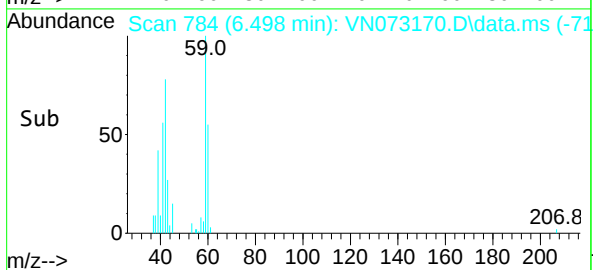

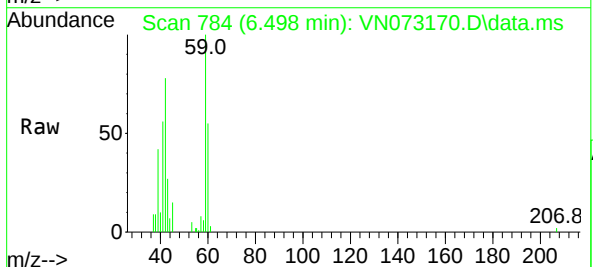




#23
 Vinyl Acetate
 Concen: 0.957 ug/l
 RT: 6.498 min Scan# 71
 Delta R.T. 0.147 min
 Lab File: VN073170.D
 Acq: 27 Jun 2022 18:29




Instrument :
 MSVOA_N
 ClientSampleId :
 31677


Tgt Ion: 43 Resp: 11277
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.0 15.0#

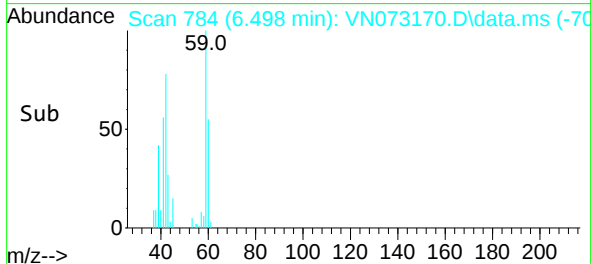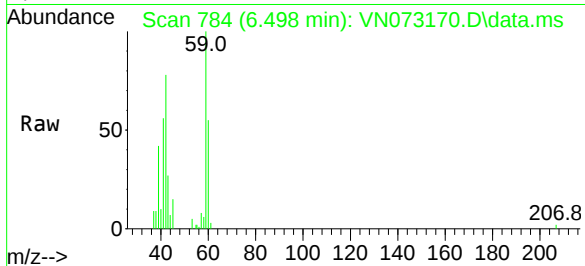

#25
 2-Butanone
 Concen: 8.152 ug/l
 RT: 7.269 min Scan# 915
 Delta R.T. 0.006 min
 Lab File: VN073170.D
 Acq: 27 Jun 2022 18:29

Tgt Ion: 43 Resp: 32178
 Ion Ratio Lower Upper
 43 100
 72 23.5 23.7 35.5#

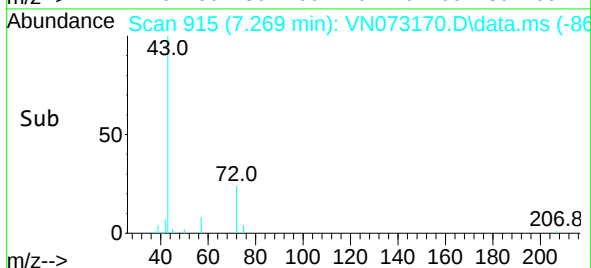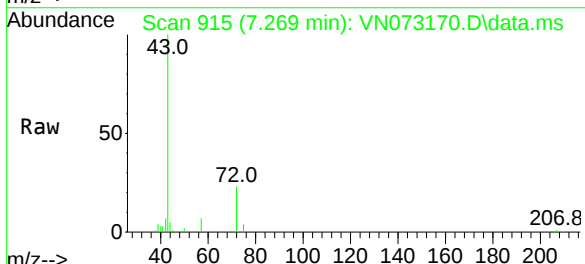



#29

Tetrahydrofuran

Concen: 3.174 ug/l

RT: 7.622 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN073170.D

Acq: 27 Jun 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :

31677





Tgt Ion: 42 Resp: 8273

Ion Ratio Lower Upper

42 100

72 46.8 39.7 59.5

71 41.8 36.6 55.0

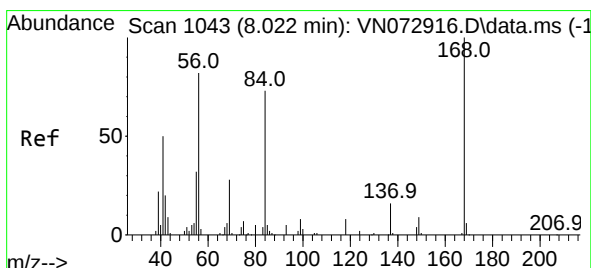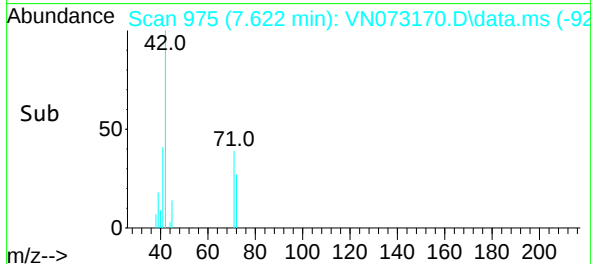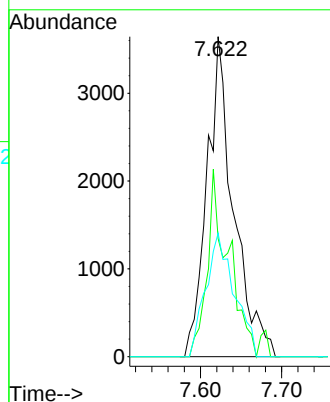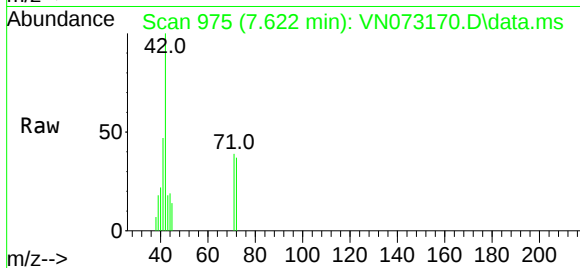

#31

Cyclohexane

Concen: 1.334 ug/l

RT: 8.022 min Scan# 1043

Delta R.T. -0.000 min

Lab File: VN073170.D

Acq: 27 Jun 2022 18:29




Tgt Ion: 56 Resp: 8166


Ion Ratio Lower Upper

56 100

69 151.7 27.8 41.8#

84 135.0 76.9 115.3#

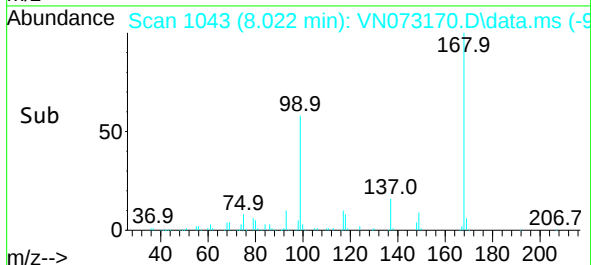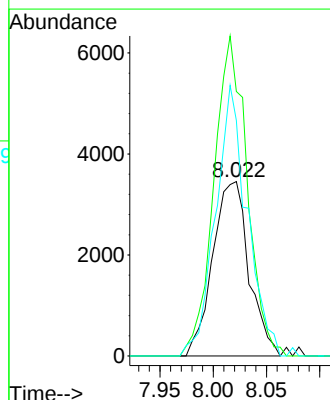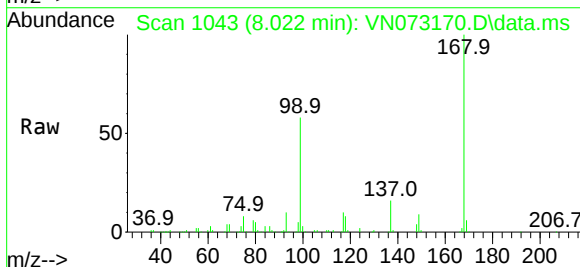

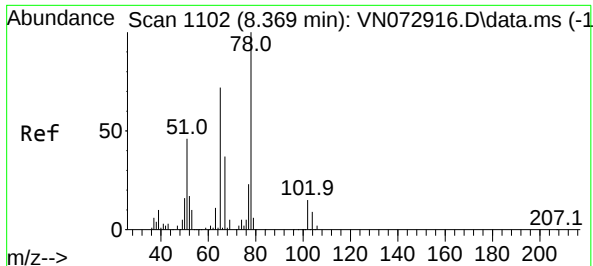

#33

1,2-Dichloroethane-d4

Concen: 43.875 ug/l

RT: 8.375 min Scan# 1103

Delta R.T. 0.006 min

Lab File: VN073170.D

Acq: 27 Jun 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :





31677

Tgt Ion: 65 Resp: 198545

Ion Ratio Lower Upper

65 100

67 52.6 0.0 104.8

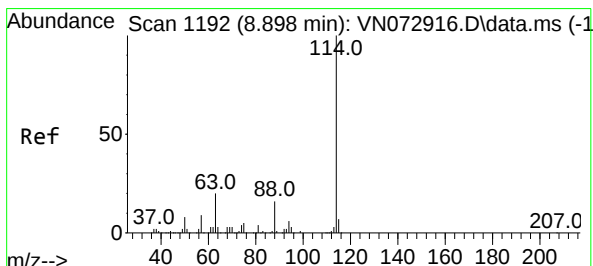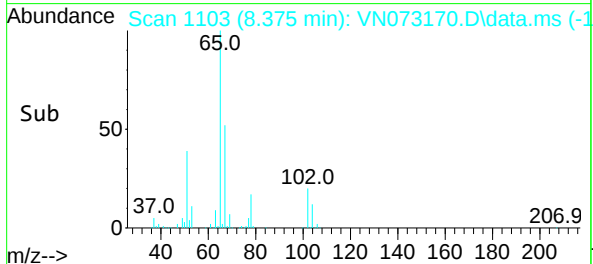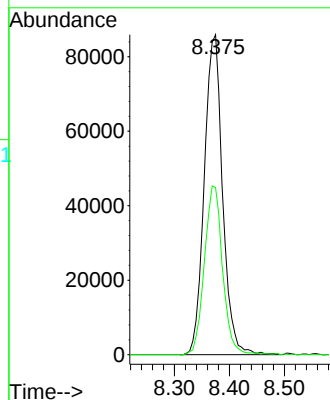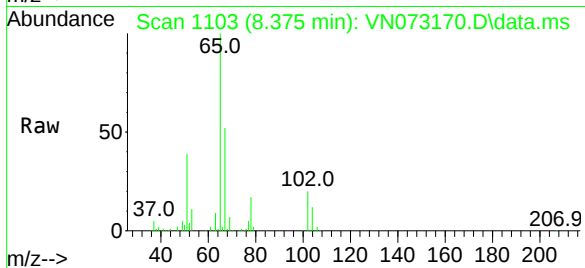

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN073170.D

Acq: 27 Jun 2022 18:29




Tgt Ion: 114 Resp: 530212


Ion Ratio Lower Upper

114 100

63 21.7 0.0 40.0

88 15.5 0.0 32.6


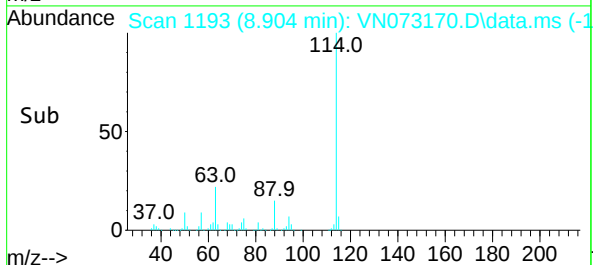
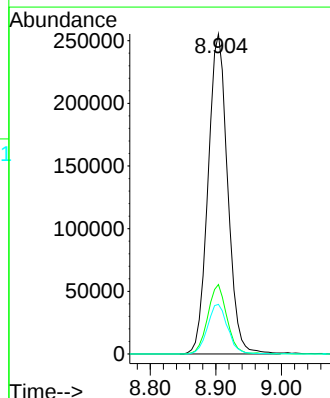
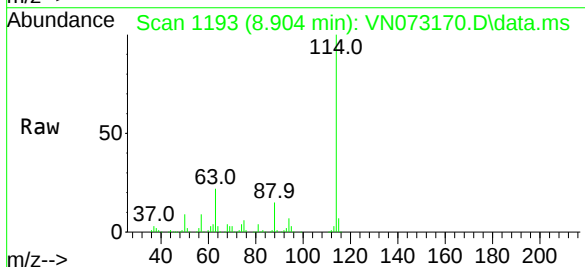


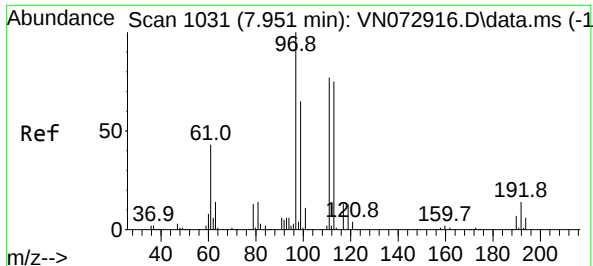

#35
Dibromofluoromethane
Concen: 51.988 ug/l
RT: 7.951 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion:113 Resp: 170374
Ion Ratio Lower Upper
113 100
111 101.3 81.4 122.0
192 18.8 17.0 25.6

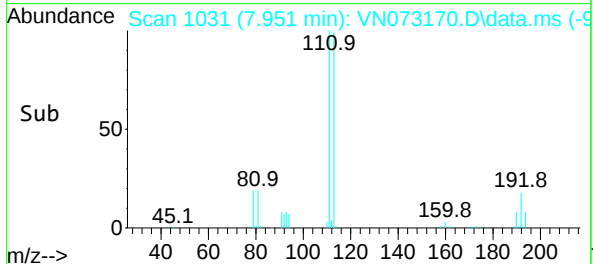

#36
1,1-Dichloropropene
Concen: 6.132 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.135 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 75 Resp: 27191
Ion Ratio Lower Upper
75 100
110 8.6 18.3 54.8#
77 0.0 25.1 37.7#

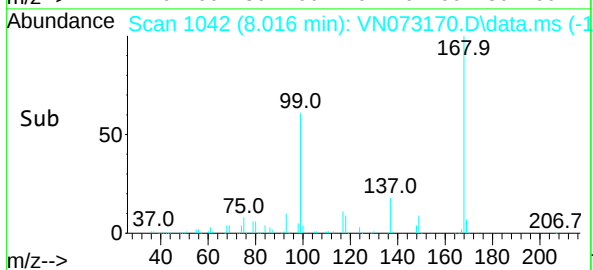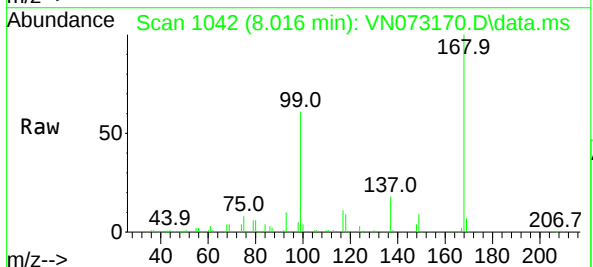



#37

Ethyl Acetate

Concen: 4.537 ug/l

RT: 7.269 min Scan# 91

Delta R.T. -0.077 min

Lab File: VN073170.D


Acq: 27 Jun 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :

31677

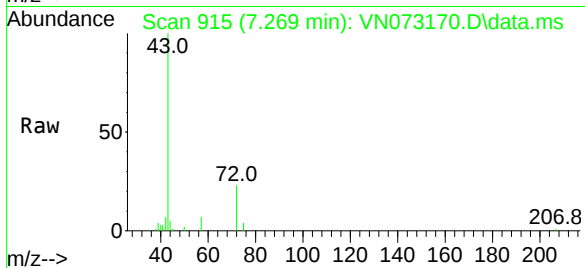




Tgt Ion: 43 Resp: 32178

Ion Ratio Lower Upper

43 100

61 0.0 11.8 17.6#

70 0.0 9.3 13.9#

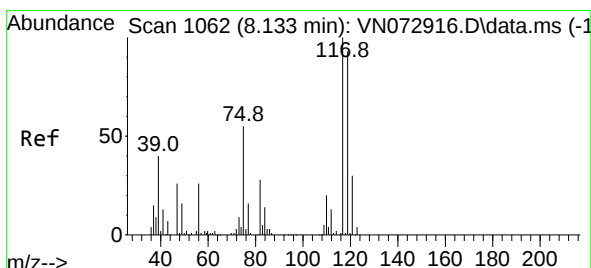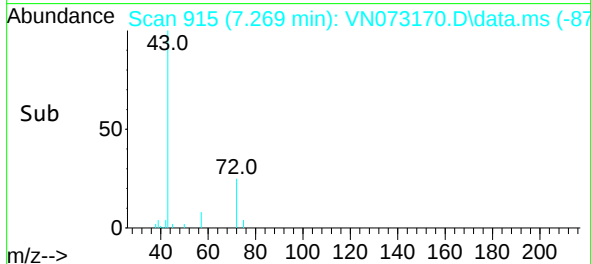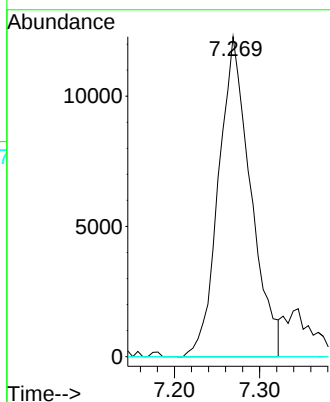

#38

Carbon Tetrachloride

Concen: 7.290 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.118 min

Lab File: VN073170.D

Acq: 27 Jun 2022 18:29




Tgt Ion: 117 Resp: 34001


Ion Ratio Lower Upper

117 100

119 3.7 75.8 113.8#

121 0.0 24.6 37.0#

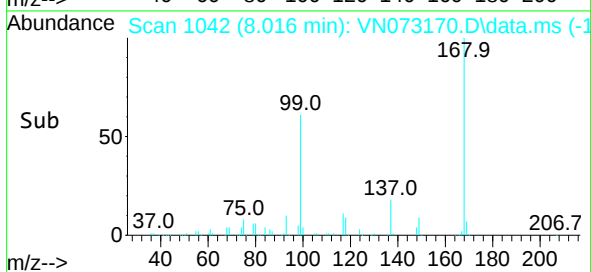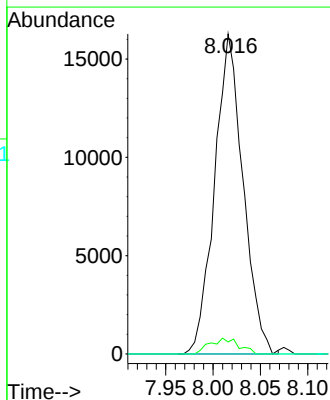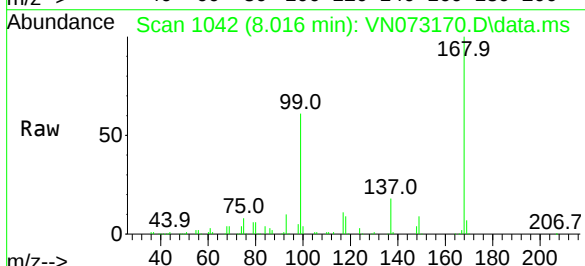



#39

Methylcyclohexane

Concen: 0.271 ug/l

RT: 9.404 min Scan# 1127

Delta R.T. 0.012 min

Lab File: VN073170.D

Acq: 27 Jun 2022 18:29

Instrument :

MSVOA_N

ClientSampleId :

31677





Tgt Ion: 83 Resp: 1447

Ion Ratio Lower Upper

83 100

55 52.2 57.8 86.8#

98 24.7 39.4 59.2#

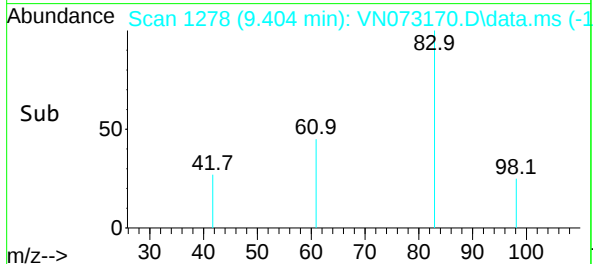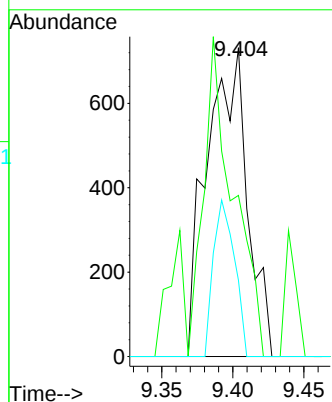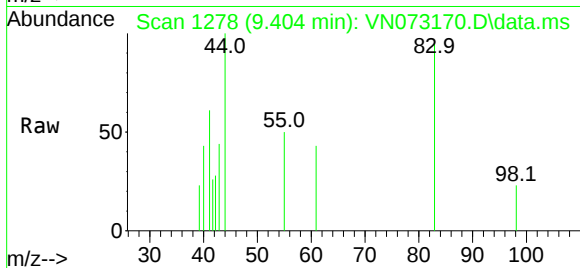

#40

Benzene

Concen: 4.123 ug/l

RT: 8.392 min Scan# 1106

Delta R.T. -0.000 min

Lab File: VN073170.D




Acq: 27 Jun 2022 18:29


Tgt Ion: 78 Resp: 57460

Ion Ratio Lower Upper

78 100

77 22.3 19.4 29.0




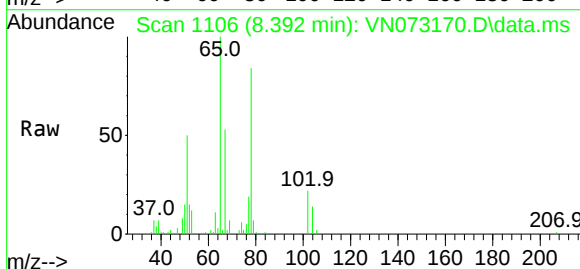




#41
Methacrylonitrile
Concen: 1.630 ug/l
RT: 7.622 min Scan# 91
Delta R.T. 0.059 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion: 41 Resp: 5483
Ion Ratio Lower Upper
41 100
39 20.4 48.6 73.0#
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

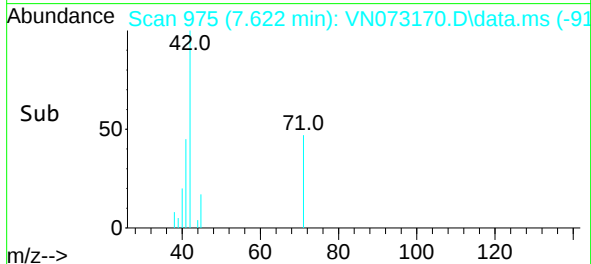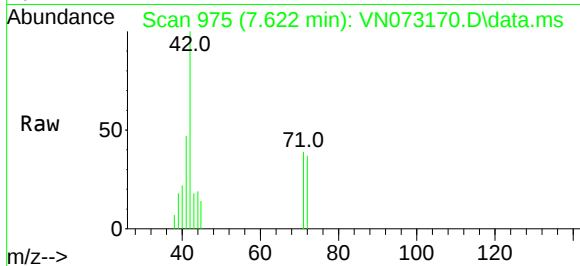

#48
Methyl methacrylate
Concen: 0.291 ug/l
RT: 9.474 min Scan# 1290
Delta R.T. -0.018 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 41 Resp: 1345
Ion Ratio Lower Upper
41 100
69 0.0 74.7 112.1#
39 47.9 45.6 68.4


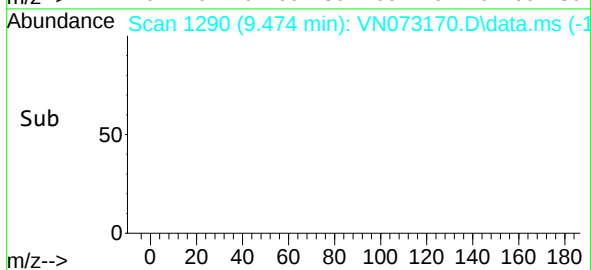

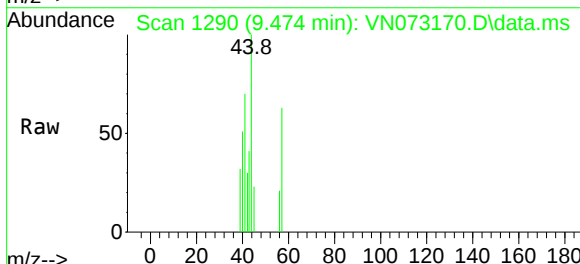


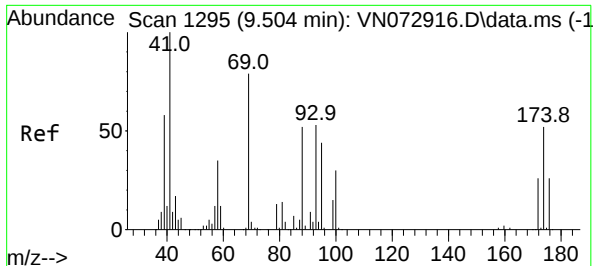

#49
1,4-Dioxane
Concen: 0.576 ug/l
RT: 9.504 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion: 88 Resp: 60
Ion Ratio Lower Upper
88 100
43 615.0 20.2 30.4#
58 103.3 54.2 81.4#

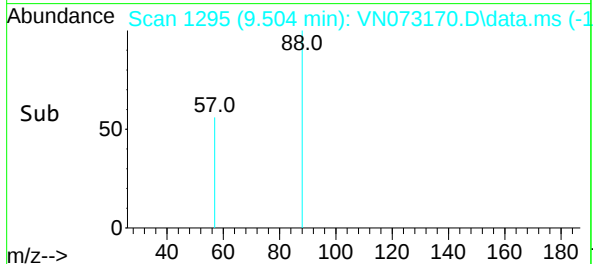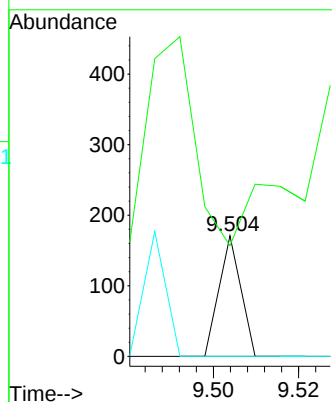

#50
Toluene-d8
Concen: 46.292 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.006 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 98 Resp: 564504
Ion Ratio Lower Upper
98 100
100 65.4 52.6 78.8


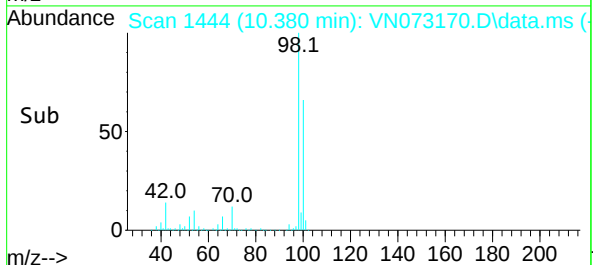

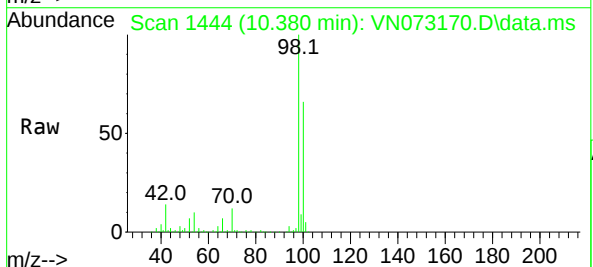


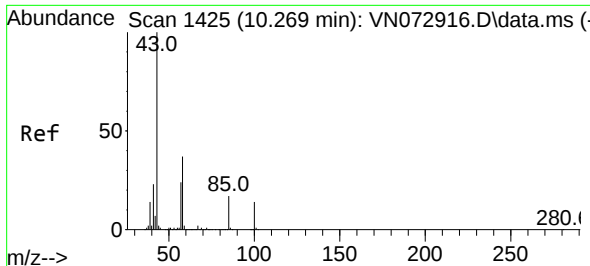

#51
4-Methyl-2-Pentanone
Concen: 0.952 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion: 43 Resp: 6297
Ion Ratio Lower Upper
43 100
58 23.0 34.1 51.1#

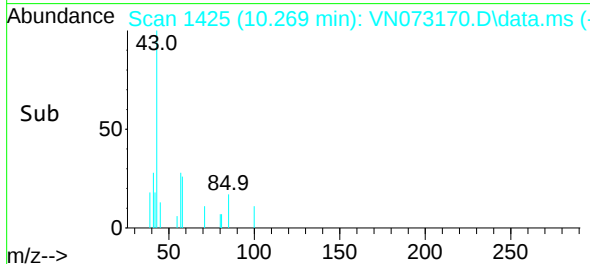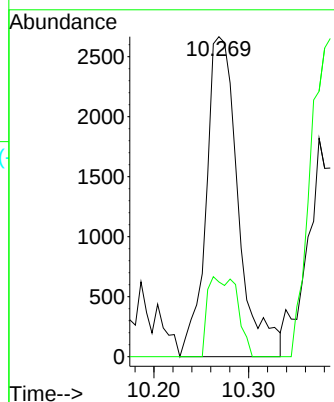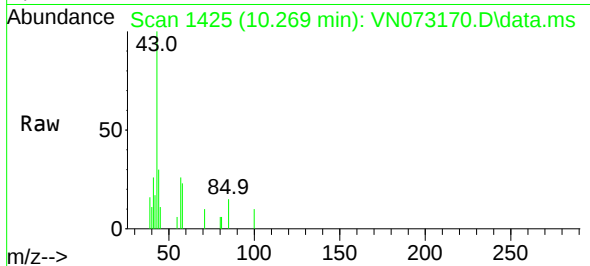

#52
Toluene
Concen: 4.342 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 92 Resp: 37151
Ion Ratio Lower Upper
92 100
91 172.3 138.6 207.8


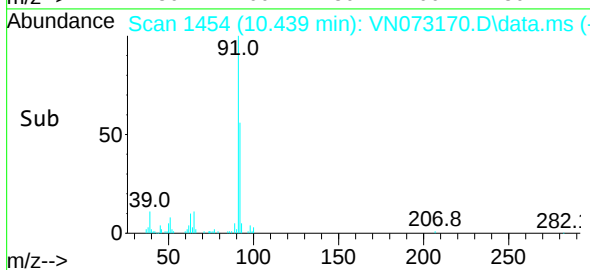
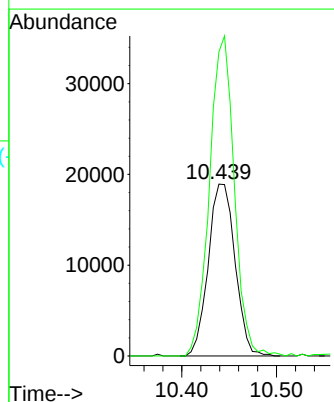
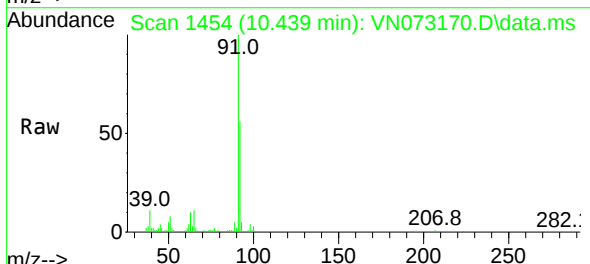




#59
2-Hexanone
Concen: 1.276 ug/l
RT: 11.027 min Scan# 1554
Delta R.T. 0.006 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion: 43 Resp: 6524
Ion Ratio Lower Upper
43 100
58 48.0 29.7 89.1

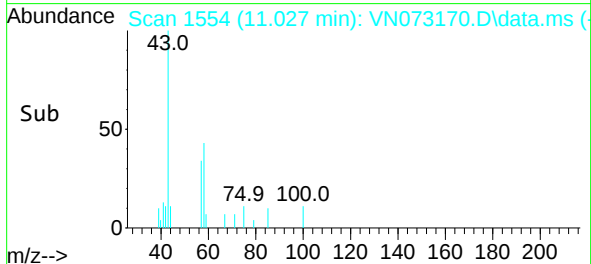

#62
4-Bromofluorobenzene
Concen: 56.795 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 95 Resp: 249043
Ion Ratio Lower Upper
95 100
174 77.0 0.0 167.6
176 73.8 0.0 163.4


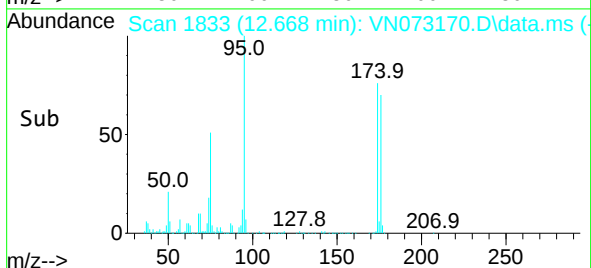

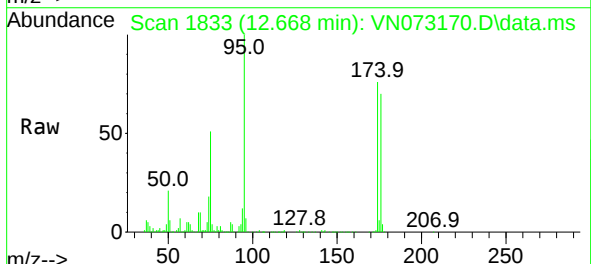




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion:117 Resp: 485535
Ion Ratio Lower Upper
117 100
82 57.6 44.2 66.2
119 32.6 25.4 38.0

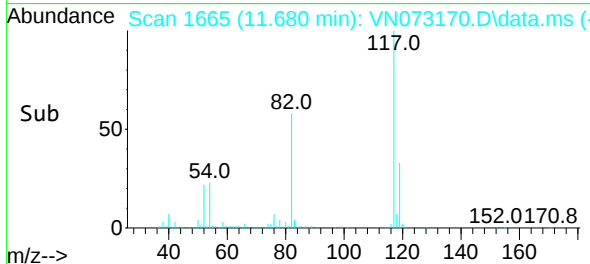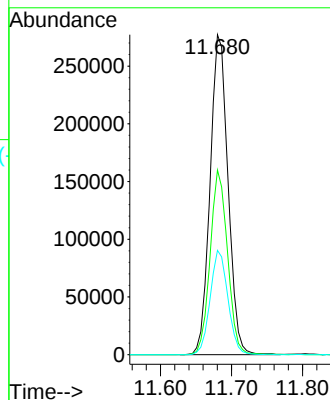

#67
Ethyl Benzene
Concen: 0.473 ug/l
RT: 11.786 min Scan# 1683
Delta R.T. 0.006 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 91 Resp: 7894
Ion Ratio Lower Upper
91 100
106 30.2 24.9 37.3



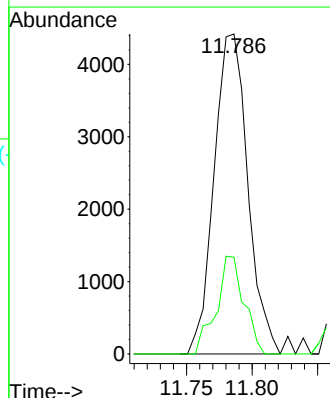
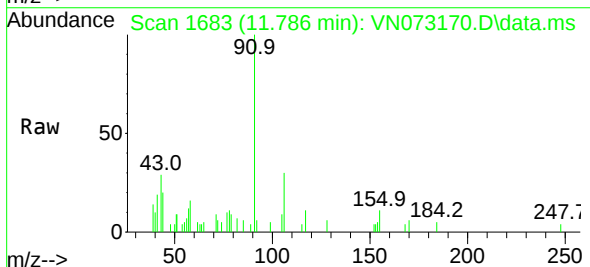


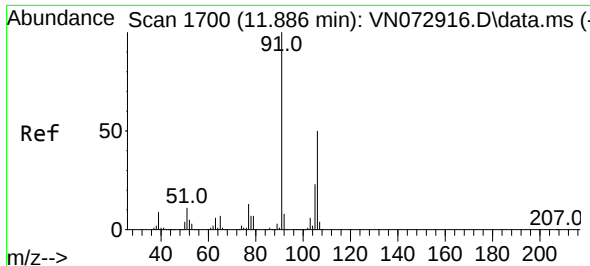

#68
m/p-Xylenes
Concen: 2.193 ug/l
RT: 11.892 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion:106 Resp: 14360
Ion Ratio Lower Upper
106 100
91 210.3 158.9 238.3

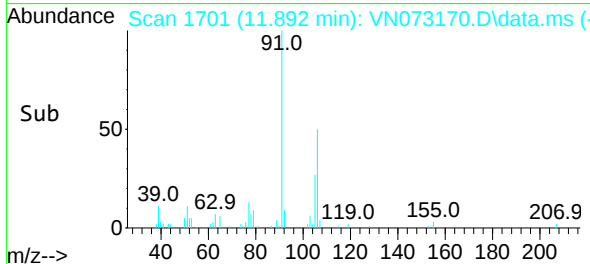

#69
o-Xylene
Concen: 0.833 ug/l
RT: 12.215 min Scan# 1756
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion:106 Resp: 5450
Ion Ratio Lower Upper
106 100
91 237.4 106.0 318.0


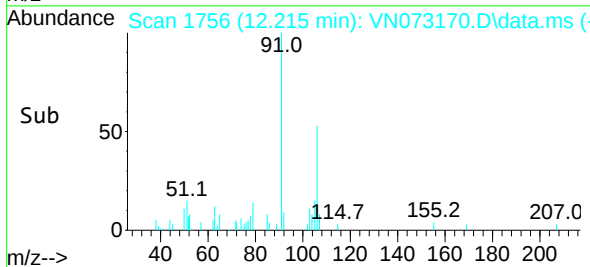

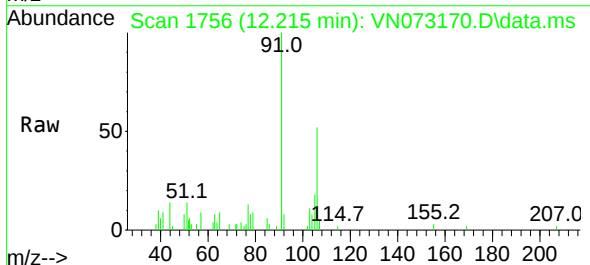




#70
Styrene
Concen: 0.247 ug/l
RT: 12.227 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion:104 Resp: 2593
Ion Ratio Lower Upper
104 100
78 78.8 39.5 59.3#
103 83.1 44.0 66.0#

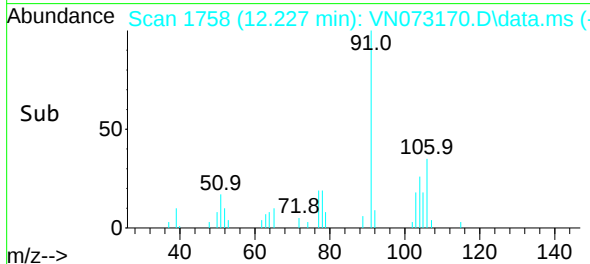

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion:152 Resp: 247404
Ion Ratio Lower Upper
152 100
115 60.4 28.9 86.7
150 155.3 0.0 356.2


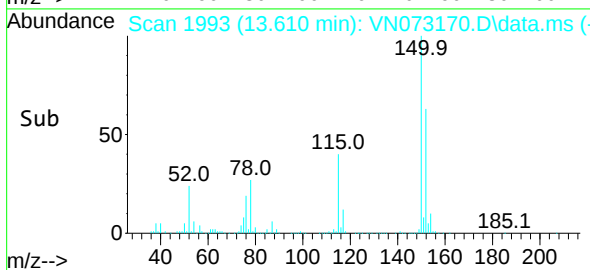

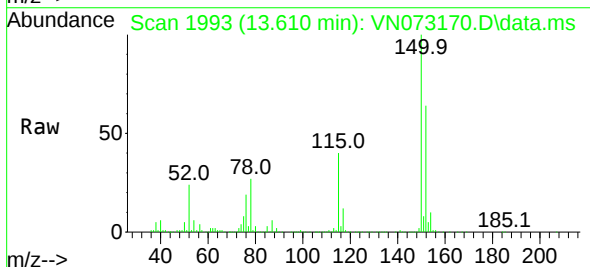


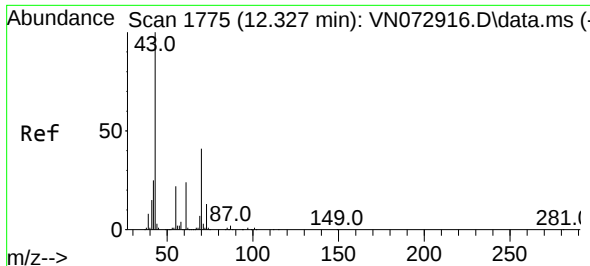

#74
N-amy1 acetate
Concen: 1.579 ug/l
RT: 12.292 min Scan# 11
Delta R.T. -0.035 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion: 43 Resp: 15683
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 0.0 21.1 31.7#
61 0.0 21.1 31.7#

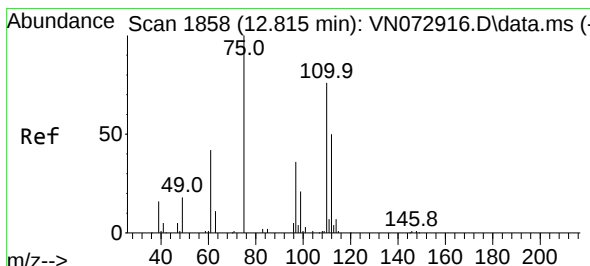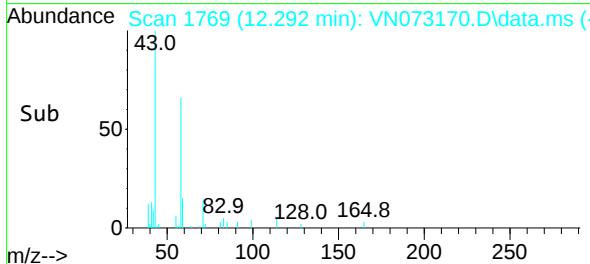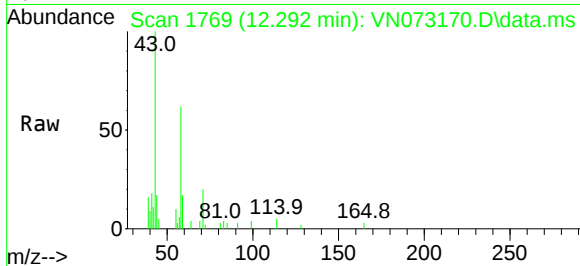

#76
1,2,3-Trichloropropane
Concen: 21.837 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.147 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Tgt Ion: 75 Resp: 130984
Ion Ratio Lower Upper
75 100
77 1.7 98.5 295.5#


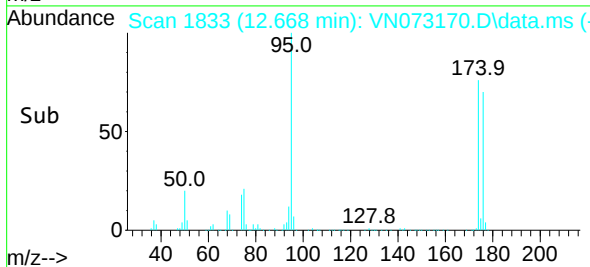

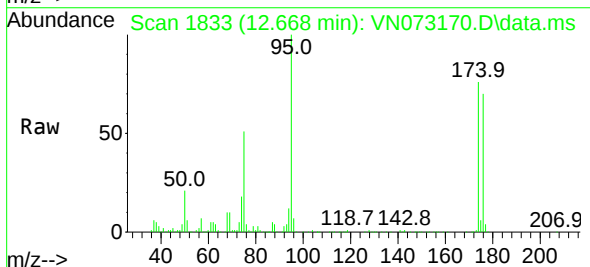


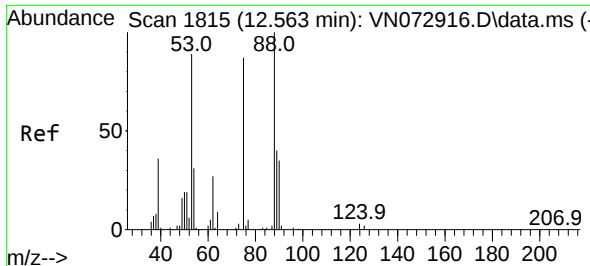

#81
trans-1,4-Dichloro-2-butene
Concen: 89.359 ug/l
RT: 12.498 min Scan# 1804
Delta R.T. -0.065 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29




Instrument :
MSVOA_N
ClientSampleId :
31677


Tgt Ion: 75 Resp: 198473
Ion Ratio Lower Upper
75 100
53 12.2 78.0 117.0#
89 5.0 37.2 55.8#

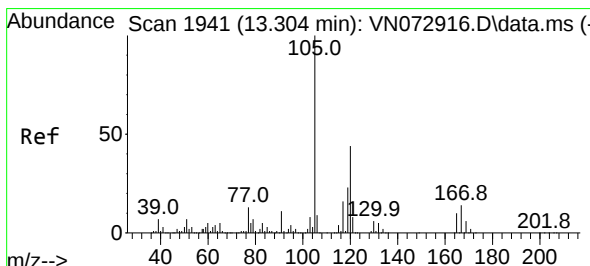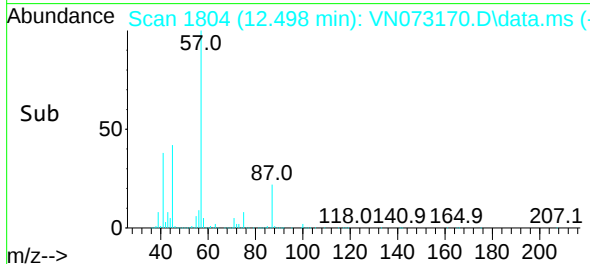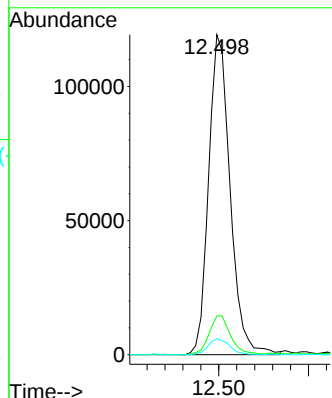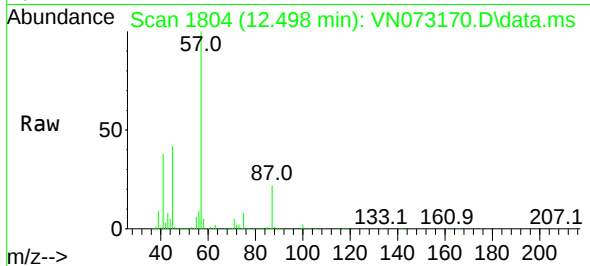

#84
1,2,4-Trimethylbenzene
Concen: 0.629 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29


Tgt Ion: 105 Resp: 9852
Ion Ratio Lower Upper
105 100
120 39.6 23.3 69.8

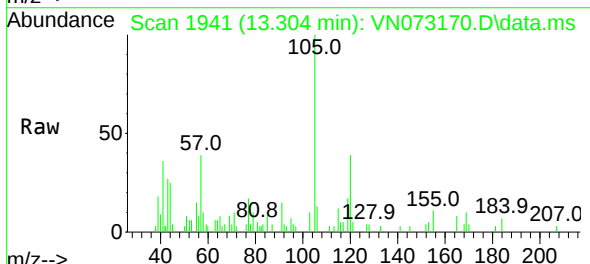

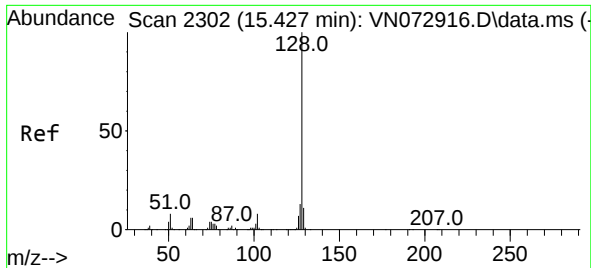

#95
Naphthalene
Concen: 1.313 ug/l
RT: 15.427 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN073170.D
Acq: 27 Jun 2022 18:29

Instrument :
MSVOA_N
ClientSampleId :
31677

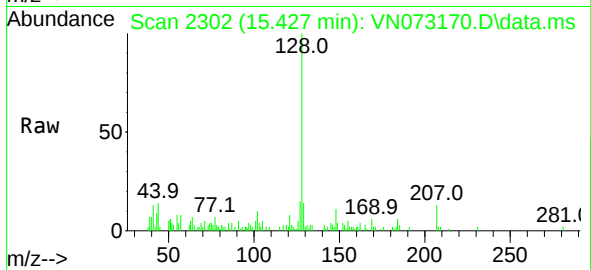

Tgt Ion:128 Resp: 25095
Ion Ratio Lower Upper
128 100
127 16.8 10.3 15.5#
129 14.8 8.6 13.0#

