

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062722\
 Data File : VN073182.D
 Acq On : 28 Jun 2022 00:35
 Operator : JC\MD
 Sample : N3455-07
 Misc : 5.14g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SP-EXC-2-2-GR

Quant Time: Jun 28 06:41:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.004	168	320164	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	8.898	114	512635	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	494713	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	254294	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.363	65	188293	43.500	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	87.000%		
35) Dibromofluoromethane	7.945	113	155932	49.212	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.420%		
50) Toluene-d8	10.375	98	546161	46.323	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	92.640%		
62) 4-Bromofluorobenzene	12.668	95	261323	61.639	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	123.280%#		
Target Compounds						Qvalue
3) Chloromethane	2.257	50	694	0.779	ug/l	95
11) Tert butyl alcohol	5.210	59	16814	15.038	ug/l #	72
16) Acetone	4.257	43	2570	1.080	ug/l #	42
18) Methyl Acetate	4.775	43	10067	1.589	ug/l	91
20) Methylene Chloride	4.981	84	7609	1.829	ug/l #	89
25) 2-Butanone	7.281	43	4754	1.259	ug/l	97
26) 2,2-Dichloropropane	7.275	77	1176	Below Cal	#	53
29) Tetrahydrofuran	7.628	42	719	0.288	ug/l #	41
31) Cyclohexane	8.010	56	7960	1.359	ug/l #	44
36) 1,1-Dichloropropene	8.004	75	24062	5.612	ug/l #	50
38) Carbon Tetrachloride	8.004	117	31024	6.879	ug/l #	17
39) Methylcyclohexane	9.386	83	1905	0.369	ug/l #	80
40) Benzene	8.375	78	10758	0.798	ug/l	100
52) Toluene	10.439	92	4204	0.508	ug/l	94
53) t-1,3-Dichloropropene	10.522	75	2811	0.565	ug/l #	81
54) cis-1,3-Dichloropropene	9.892	75	1820	0.335	ug/l #	36
59) 2-Hexanone	10.986	43	1603	0.324	ug/l #	21
65) Chlorobenzene	11.704	112	2055	0.213	ug/l	96
67) Ethyl Benzene	11.780	91	13256	0.779	ug/l	95
68) m/p-Xylenes	11.886	106	10407	1.560	ug/l	94
74) N-amyl acetate	12.304	43	3896	0.382	ug/l #	49
76) 1,2,3-Trichloropropane	12.668	75	134338	21.789	ug/l #	1
78) n-propylbenzene	12.863	91	15303	0.707	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.668	75	134338	58.845	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.304	105	9584	0.595	ug/l	96
89) n-Butylbenzene	13.880	91	3410	0.261	ug/l #	77
90) Hexachloroethane	14.157	117	691	0.229	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	14.551	75	55	Below Cal	#	49
93) 1,2,4-Trichlorobenzene	15.186	180	1017	0.209	ug/l #	3
95) Naphthalene	15.433	128	14970	0.762	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062722\
Data File : VN073182.D
Acq On : 28 Jun 2022 00:35
Operator : JC\MD
Sample : N3455-07
Misc : 5.14g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR

Quant Time: Jun 28 06:41:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




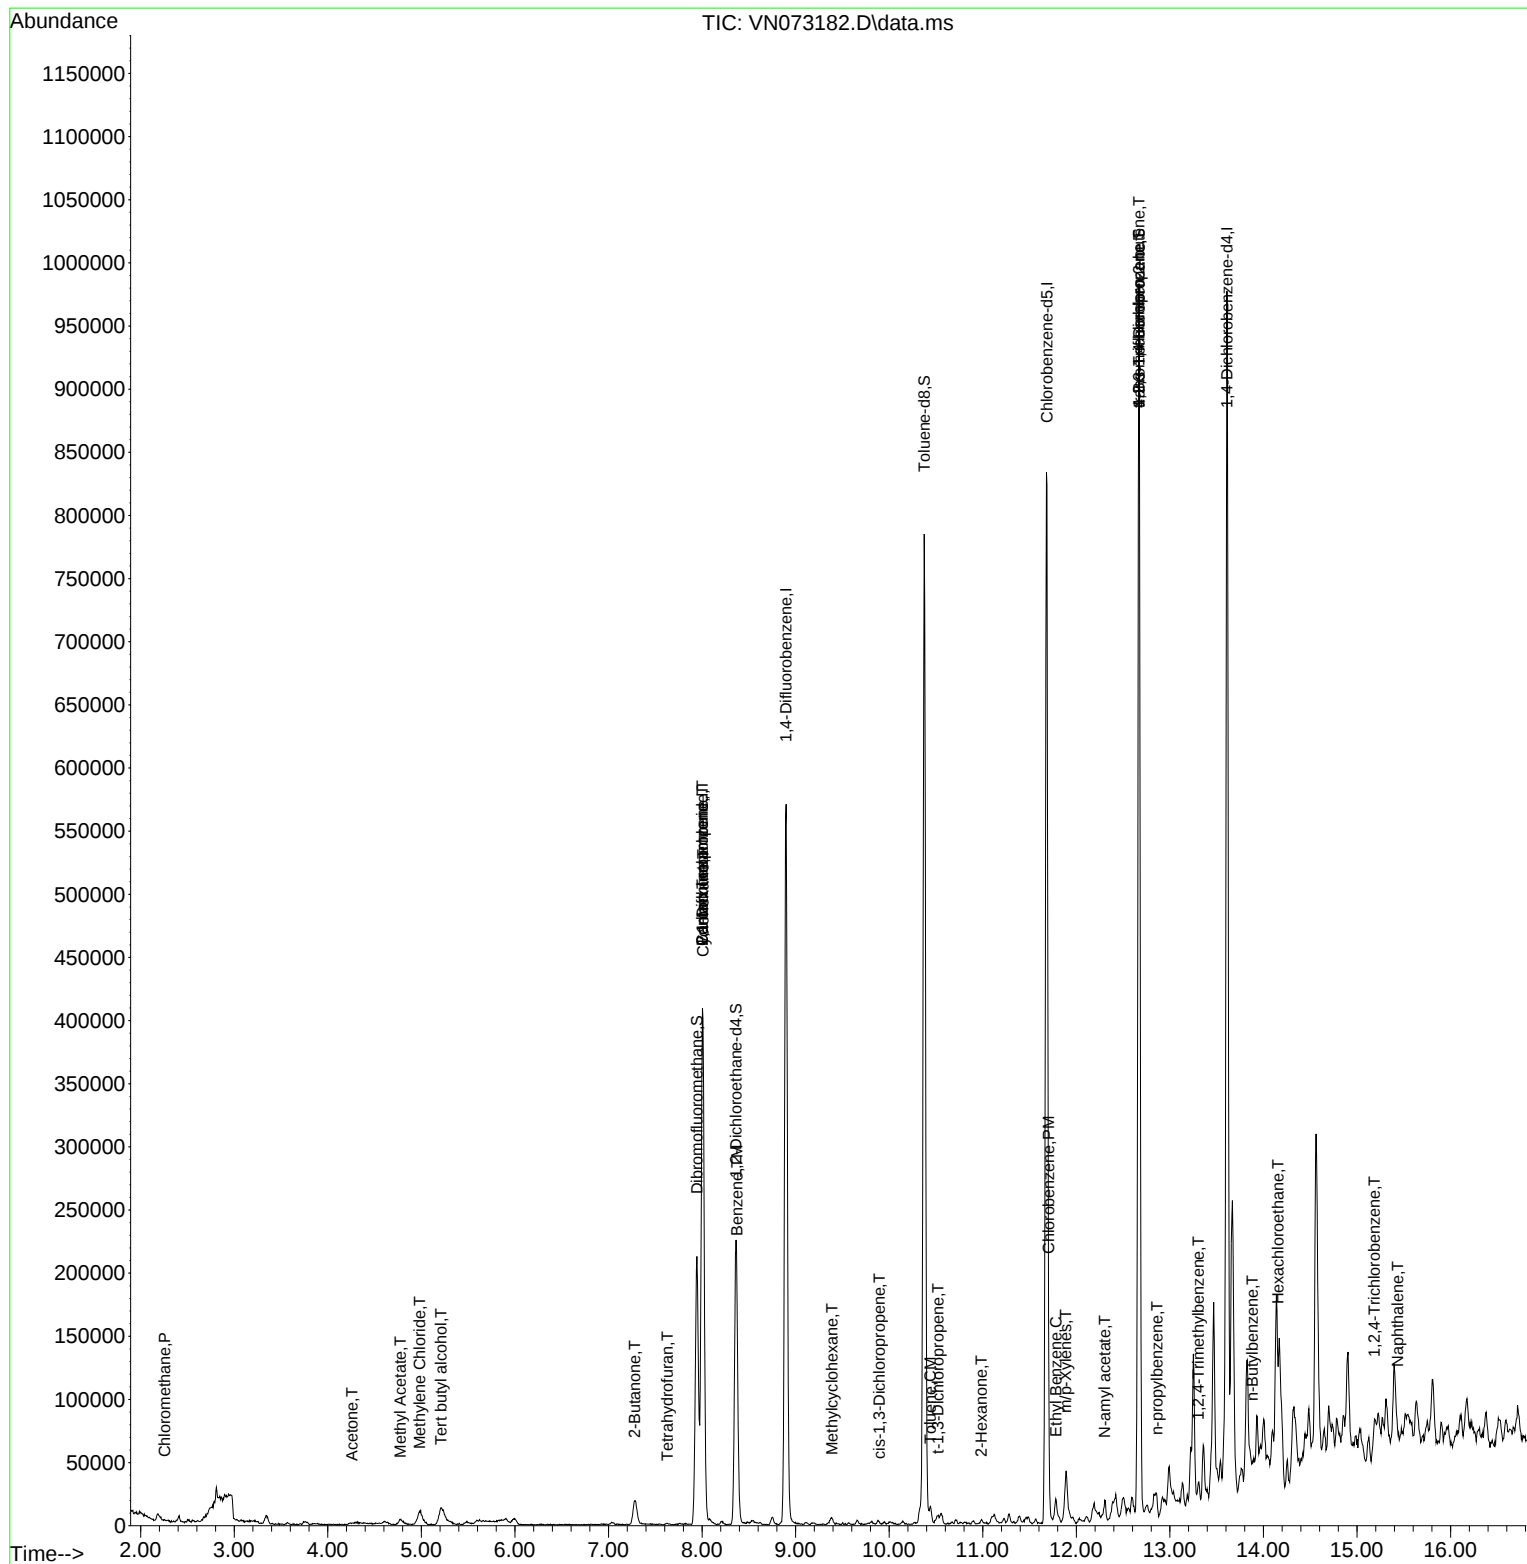




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.004 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion:168 Resp: 320164
Ion Ratio Lower Upper
168 100
99 57.2 42.3 63.5

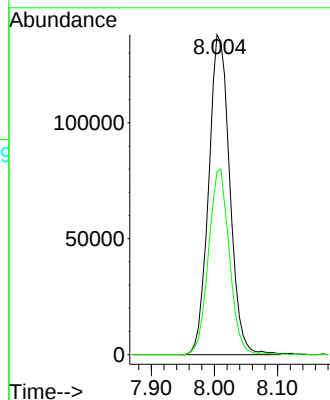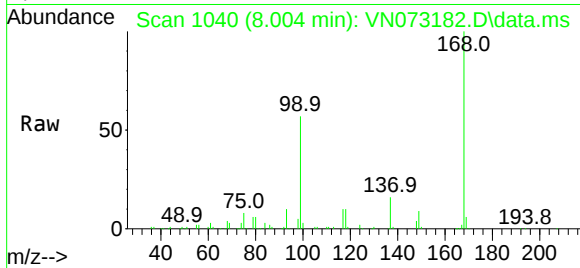

#3
Chloromethane
Concen: 0.779 ug/l
RT: 2.257 min Scan# 63
Delta R.T. -0.006 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 50 Resp: 694
Ion Ratio Lower Upper
50 100
52 34.7 25.7 38.5


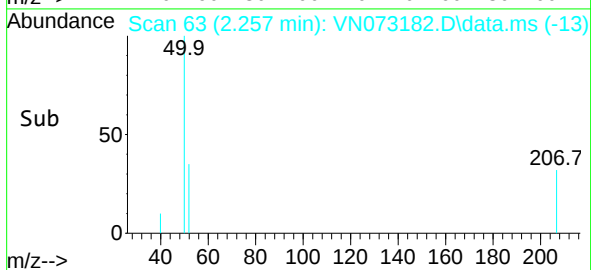
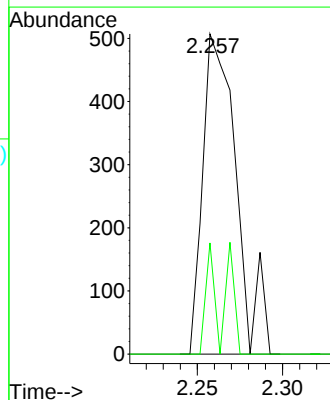
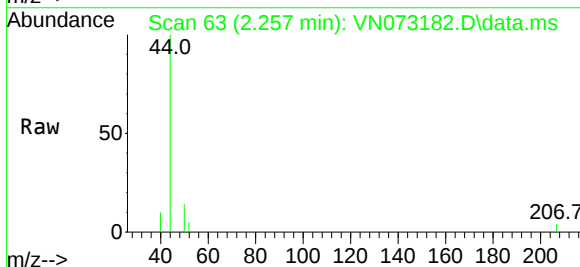




#11
Tert butyl alcohol
Concen: 15.038 ug/l
RT: 5.210 min Scan# 51
Delta R.T. -0.094 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion: 59 Resp: 16814
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

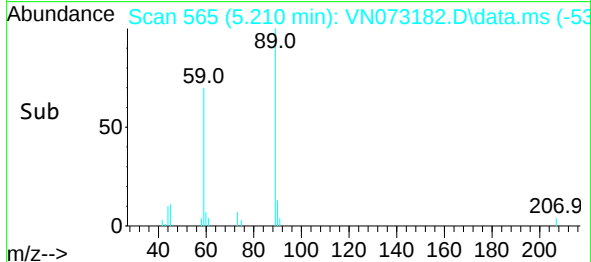

#16
Acetone
Concen: 1.080 ug/l
RT: 4.257 min Scan# 403
Delta R.T. 0.029 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 43 Resp: 2570
Ion Ratio Lower Upper
43 100
58 0.0 26.0 39.0#


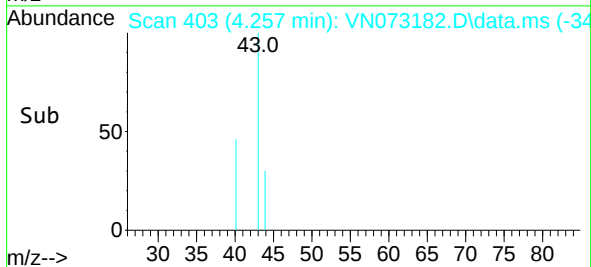

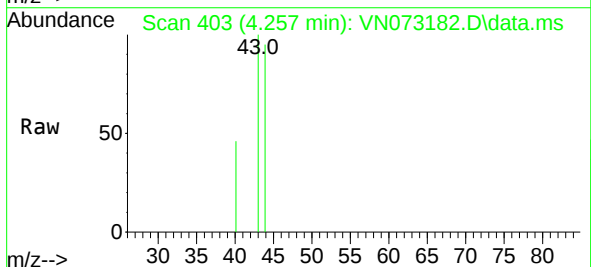




#18
Methyl Acetate
Concen: 1.589 ug/l
RT: 4.775 min Scan# 491
Delta R.T. -0.006 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion: 43 Resp: 10067
Ion Ratio Lower Upper
43 100
74 22.1 21.6 32.4

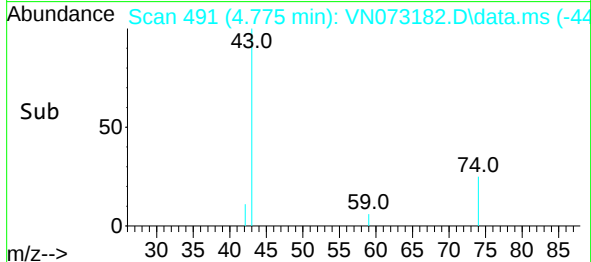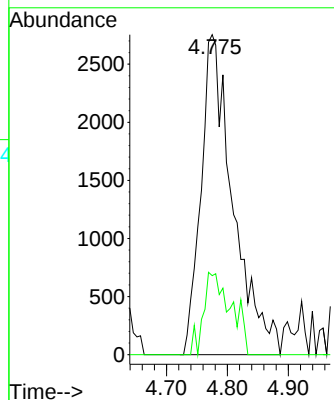

#20
Methylene Chloride
Concen: 1.829 ug/l
RT: 4.981 min Scan# 526
Delta R.T. -0.035 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 84 Resp: 7609
Ion Ratio Lower Upper
84 100
49 118.4 88.3 132.5
51 33.7 28.2 42.2
86 46.8 50.6 76.0#

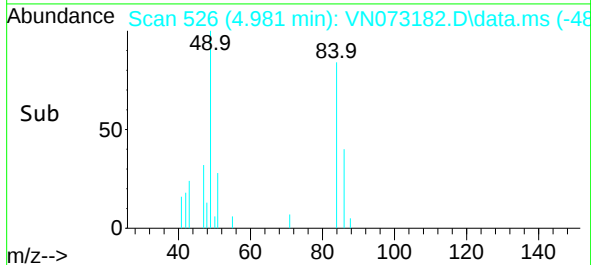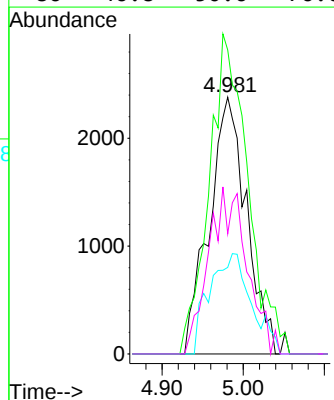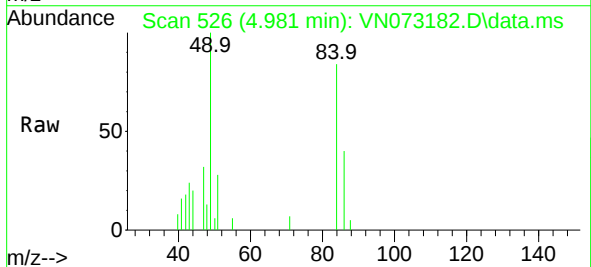

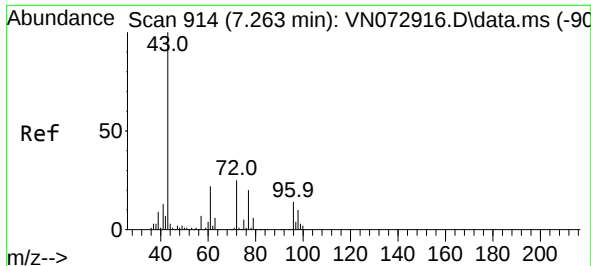

#25

2-Butanone

Concen: 1.259 ug/l

RT: 7.281 min Scan# 917

Delta R.T. 0.018 min

Lab File: VN073182.D

Acq: 28 Jun 2022 00:35

Instrument :

MSVOA_N

ClientSampleId :





SP-EXC-2-2-GR

Tgt Ion: 43 Resp: 4754

Ion Ratio Lower Upper

43 100

72 28.1 23.7 35.5

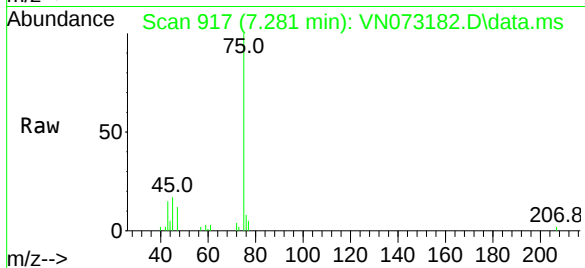

#26

2,2-Dichloropropane

Concen: Below Cal

RT: 7.275 min Scan# 916

Delta R.T. 0.024 min

Lab File: VN073182.D




Acq: 28 Jun 2022 00:35


Tgt Ion: 77 Resp: 1176

Ion Ratio Lower Upper

77 100

97 0.0 11.4 34.2#

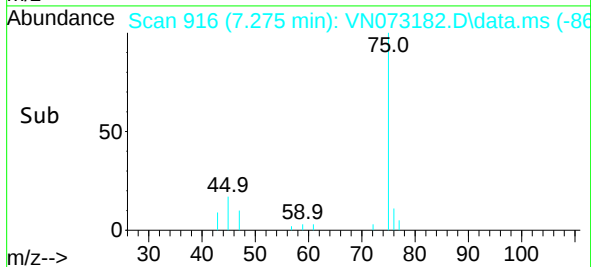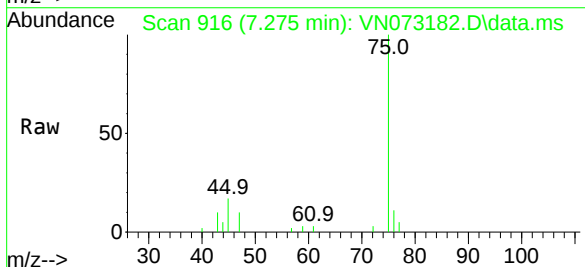



#29

Tetrahydrofuran

Concen: 0.288 ug/l

RT: 7.628 min Scan# 91

Delta R.T. 0.018 min

Lab File: VN073182.D


Acq: 28 Jun 2022 00:35

Instrument :




MSVOA_N

ClientSampleId :

SP-EXC-2-2-GR



Tgt Ion:	42	Resp:	719
Ion Ratio	Lower	Upper	
42	100		
72	15.6	39.7	59.5#
71	0.0	36.6	55.0#

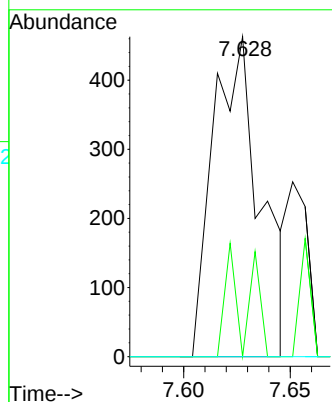

#31

Cyclohexane

Concen: 1.359 ug/l




RT: 8.010 min Scan# 1041


Delta R.T. -0.012 min

Lab File: VN073182.D

Acq: 28 Jun 2022 00:35

Tgt Ion:	56	Resp:	7960
Ion Ratio	Lower	Upper	
56	100		
69	140.0	27.8	41.8#
84	106.8	76.9	115.3


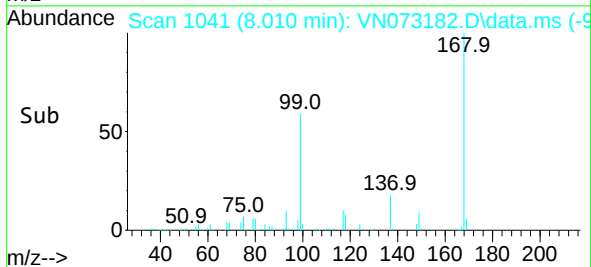

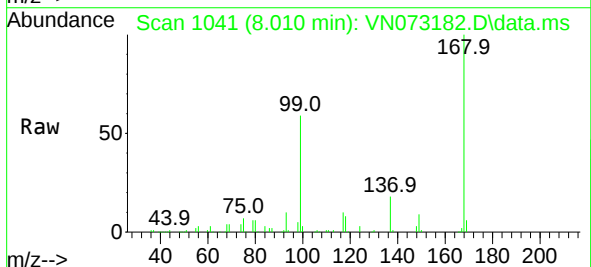


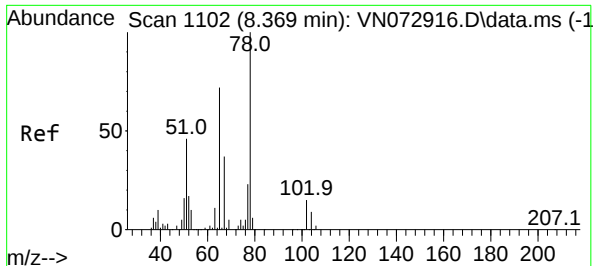

#33
1,2-Dichloroethane-d4
Concen: 43.500 ug/l
RT: 8.363 min Scan# 1102
Delta R.T. -0.006 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion: 65 Resp: 188293
Ion Ratio Lower Upper
65 100
67 51.1 0.0 104.8

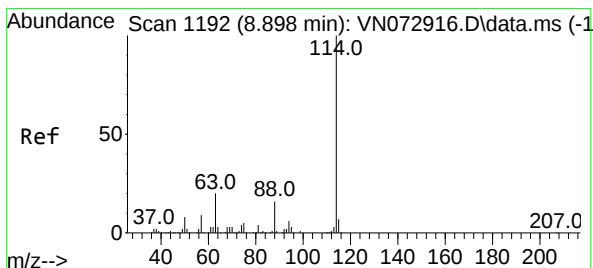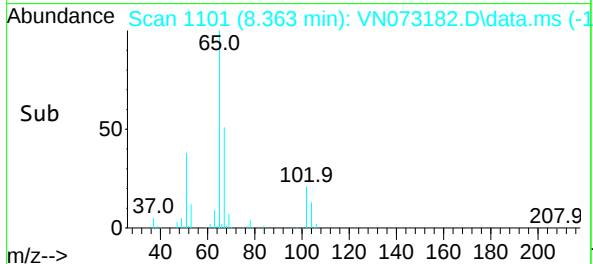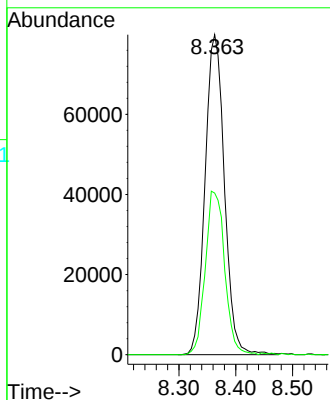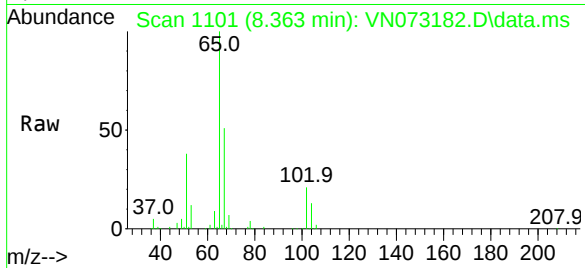

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.898 min Scan# 1192
Delta R.T. 0.000 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 114 Resp: 512635
Ion Ratio Lower Upper
114 100
63 20.7 0.0 40.0
88 15.1 0.0 32.6


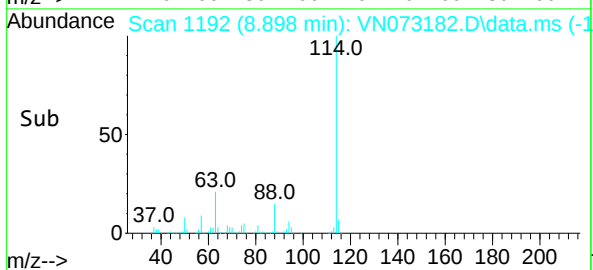
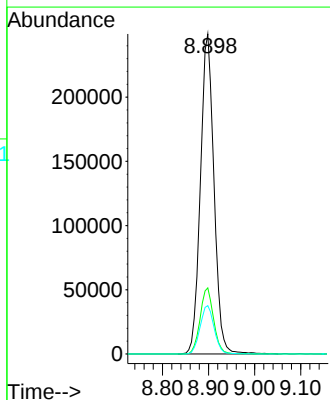
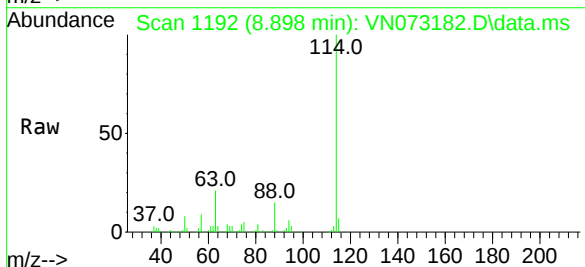


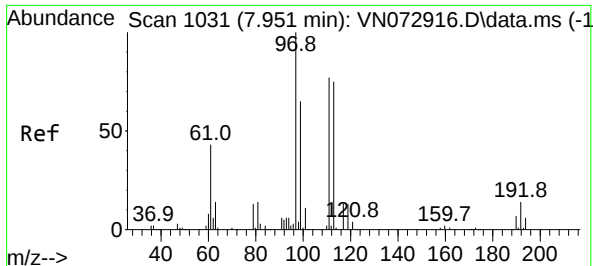

#35
Dibromofluoromethane
Concen: 49.212 ug/l
RT: 7.945 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion:113 Resp: 155932
Ion Ratio Lower Upper
113 100
111 104.1 81.4 122.0
192 19.4 17.0 25.6

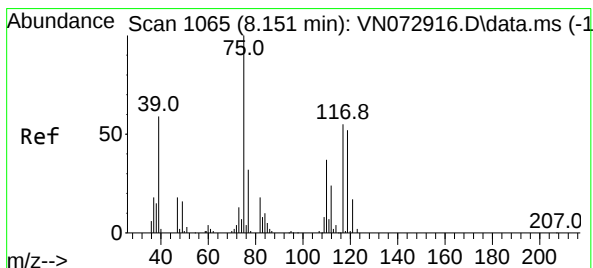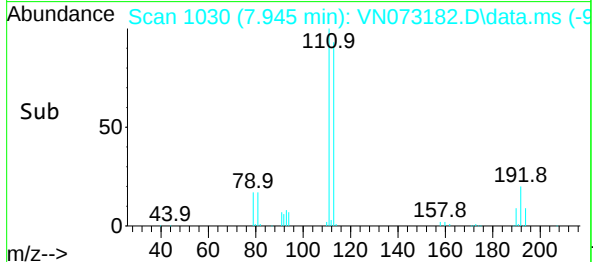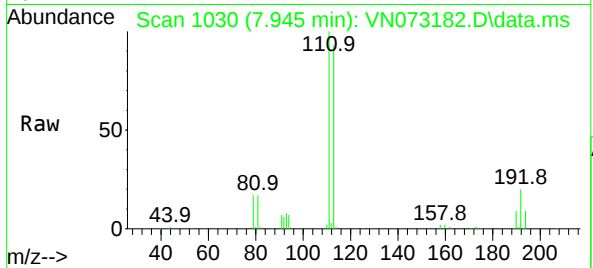

#36
1,1-Dichloropropene
Concen: 5.612 ug/l
RT: 8.004 min Scan# 1040
Delta R.T. -0.147 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 75 Resp: 24062
Ion Ratio Lower Upper
75 100
110 10.5 18.3 54.8#
77 0.0 25.1 37.7#


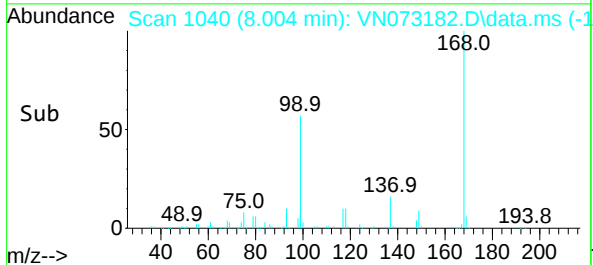

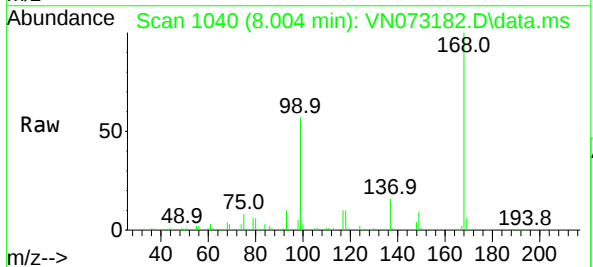


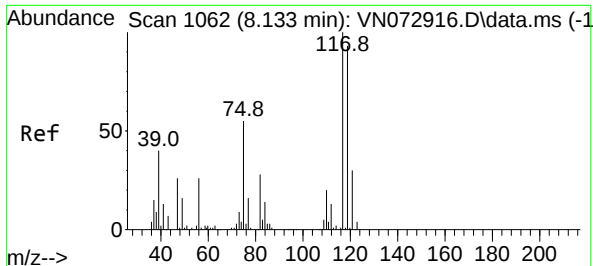

#38
Carbon Tetrachloride
Concen: 6.879 ug/l
RT: 8.004 min Scan# 117
Delta R.T. -0.129 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion:117 Resp: 31024
Ion Ratio Lower Upper
117 100
119 6.2 75.8 113.8#
121 0.0 24.6 37.0#

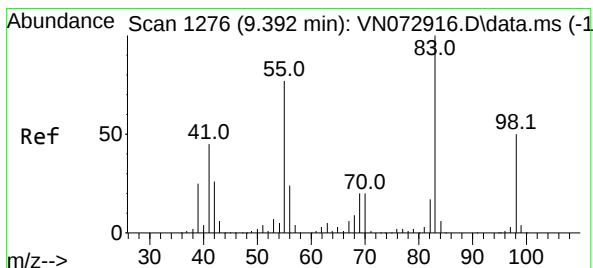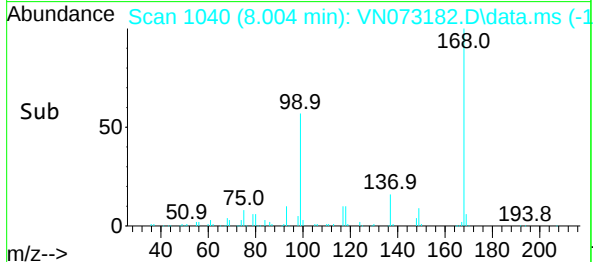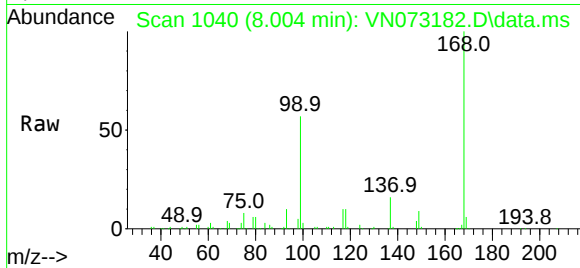

#39
Methylcyclohexane
Concen: 0.369 ug/l
RT: 9.386 min Scan# 1275
Delta R.T. -0.006 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 83 Resp: 1905
Ion Ratio Lower Upper
83 100
55 88.3 57.8 86.8#
98 35.4 39.4 59.2#

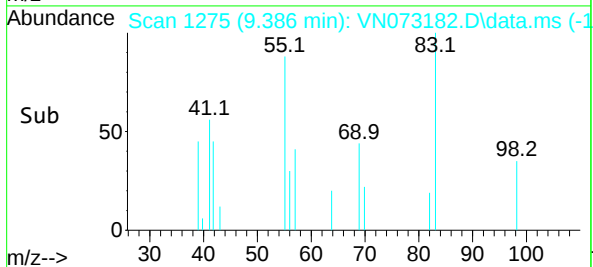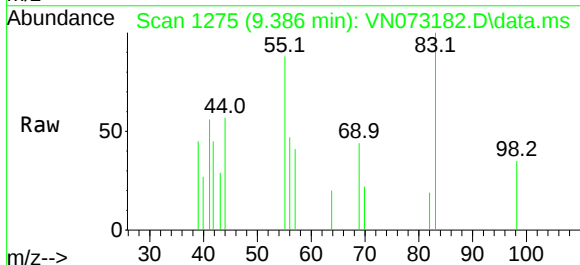

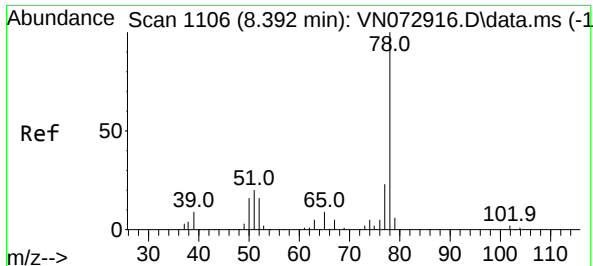

#40

Benzene

Concen: 0.798 ug/l

RT: 8.375 min Scan# 1106

Delta R.T. -0.018 min

Lab File: VN073182.D

Acq: 28 Jun 2022 00:35

Instrument :

MSVOA_N

ClientSampleId :





SP-EXC-2-2-GR

Tgt Ion: 78 Resp: 10758

Ion Ratio Lower Upper

78 100

77 24.4 19.4 29.0

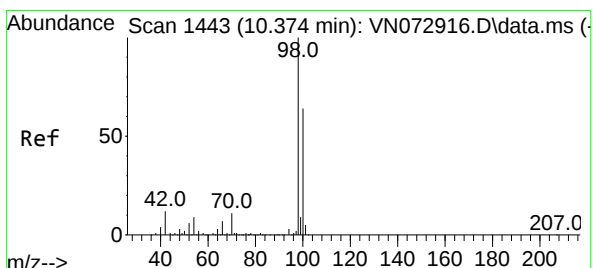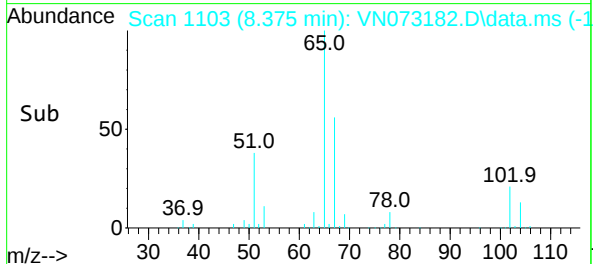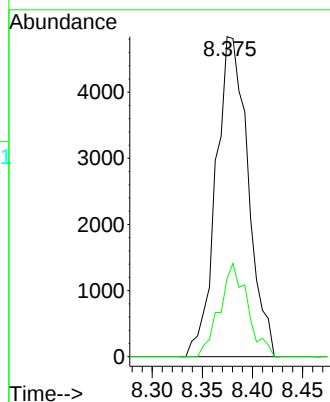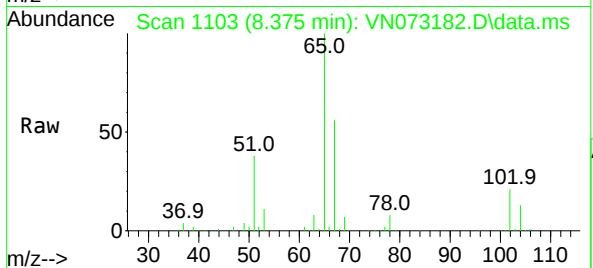

#50

Toluene-d8

Concen: 46.323 ug/l

RT: 10.375 min Scan# 1443

Delta R.T. 0.000 min

Lab File: VN073182.D




Acq: 28 Jun 2022 00:35


Tgt Ion: 98 Resp: 546161

Ion Ratio Lower Upper

98 100

100 66.2 52.6 78.8


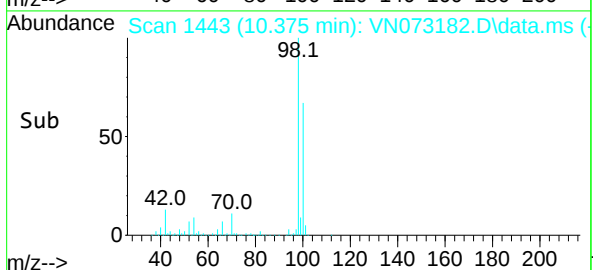
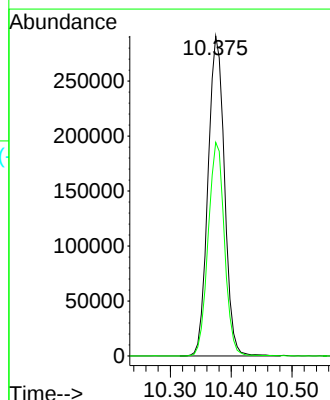
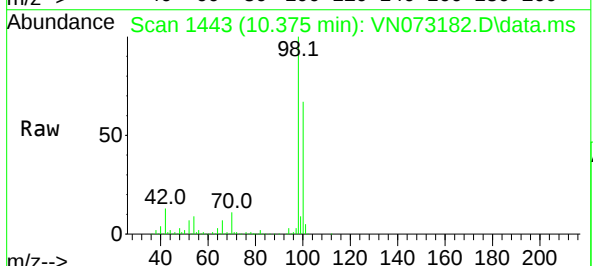




#52
Toluene
Concen: 0.508 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. 0.000 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion: 92 Resp: 4204
Ion Ratio Lower Upper
92 100
91 181.3 138.6 207.8

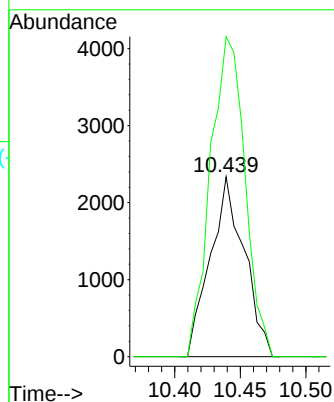

#53
t-1,3-Dichloropropene
Concen: 0.565 ug/l
RT: 10.522 min Scan# 1468
Delta R.T. -0.135 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 75 Resp: 2811
Ion Ratio Lower Upper
75 100
77 42.9 25.6 38.4#


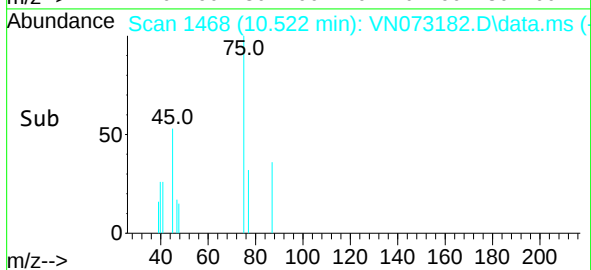
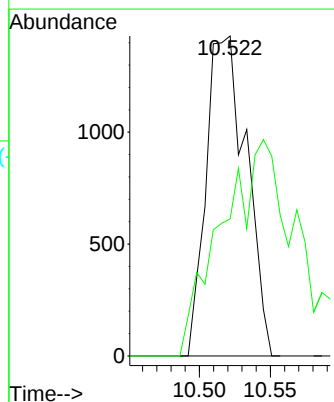
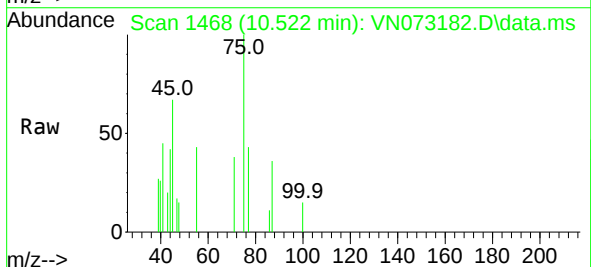




#54
 cis-1,3-Dichloropropene
 Concen: 0.335 ug/l
 RT: 9.892 min Scan# 1547
 Delta R.T. -0.229 min
 Lab File: VN073182.D
 Acq: 28 Jun 2022 00:35




Instrument :
 MSVOA_N
 ClientSampleId :
 SP-EXC-2-2-GR


Tgt Ion: 75 Resp: 1820
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.2 37.8#
 39 0.0 35.7 53.5#

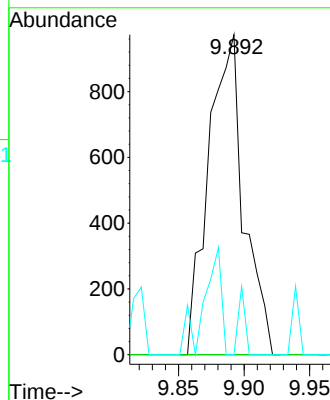

#59
 2-Hexanone
 Concen: 0.324 ug/l
 RT: 10.986 min Scan# 1547
 Delta R.T. -0.035 min
 Lab File: VN073182.D
 Acq: 28 Jun 2022 00:35

Tgt Ion: 43 Resp: 1603
 Ion Ratio Lower Upper
 43 100
 58 0.0 29.7 89.1#



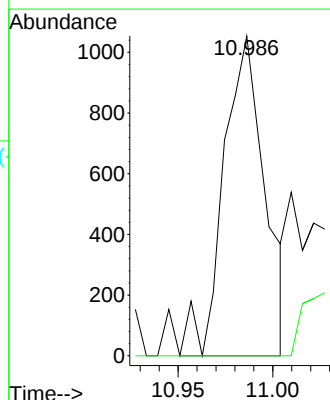





#62
4-Bromofluorobenzene
Concen: 61.639 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion: 95 Resp: 261323
Ion Ratio Lower Upper
95 100
174 74.1 0.0 167.6
176 72.5 0.0 163.4

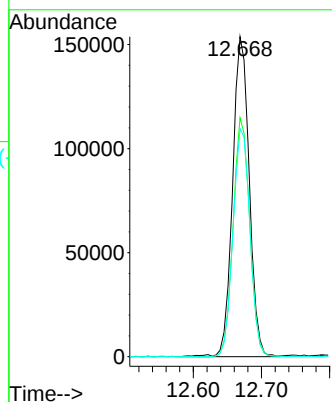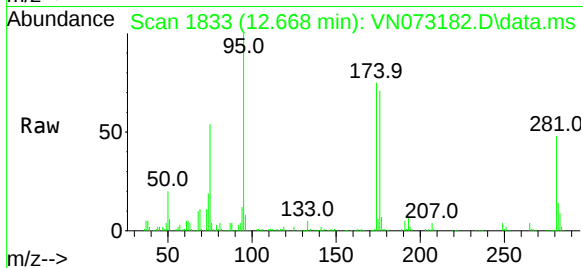

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.006 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 117 Resp: 494713
Ion Ratio Lower Upper
117 100
82 54.8 44.2 66.2
119 31.5 25.4 38.0


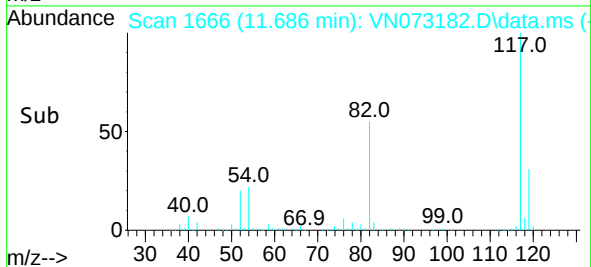
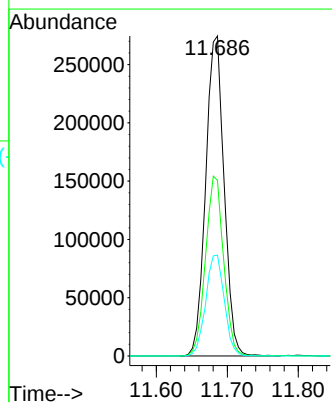
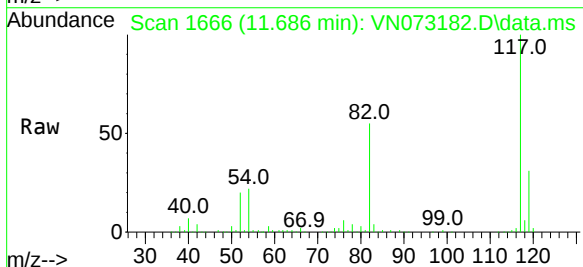




#65
Chlorobenzene
Concen: 0.213 ug/l
RT: 11.704 min Scan# 1669
Delta R.T. 0.000 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion:112 Resp: 2055
Ion Ratio Lower Upper
112 100
114 29.4 25.4 38.2

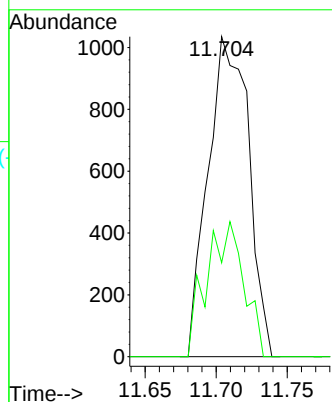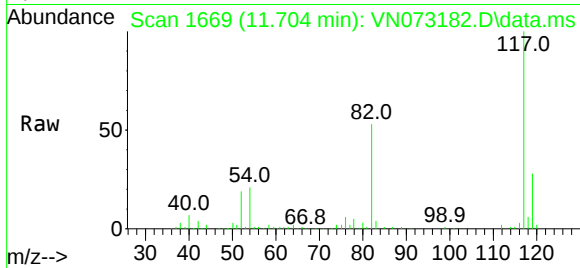

#67
Ethyl Benzene
Concen: 0.779 ug/l
RT: 11.780 min Scan# 1682
Delta R.T. 0.000 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 91 Resp: 13256
Ion Ratio Lower Upper
91 100
106 33.7 24.9 37.3


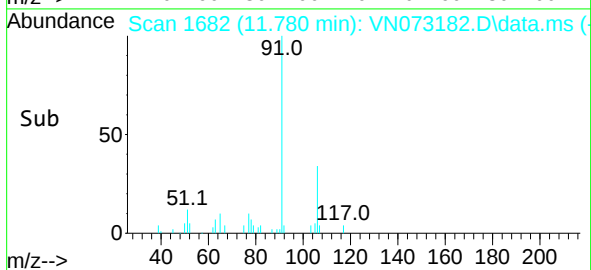
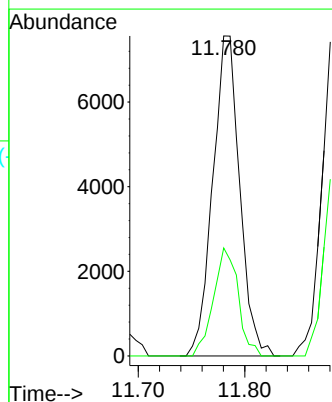
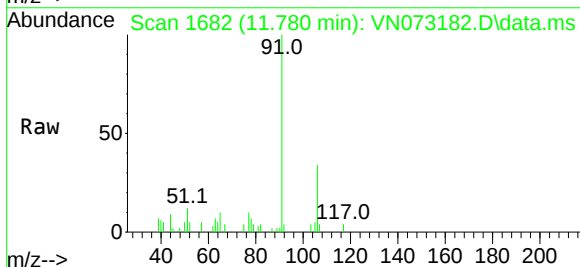


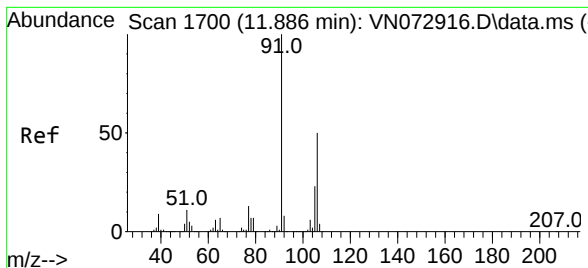

#68
m/p-Xylenes
Concen: 1.560 ug/l
RT: 11.886 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion:106 Resp: 10407
Ion Ratio Lower Upper
106 100
91 189.0 158.9 238.3

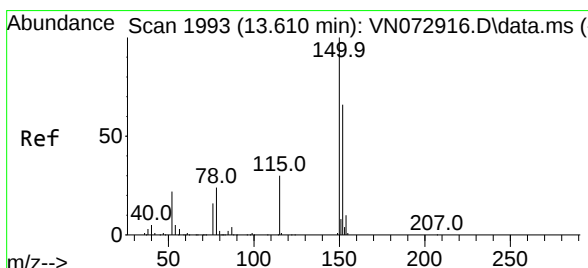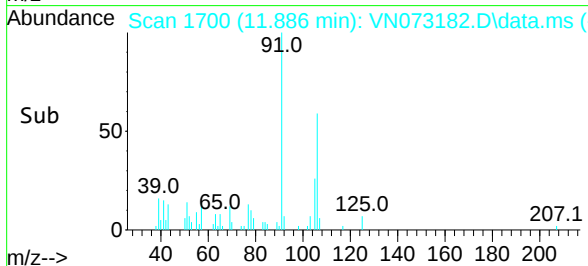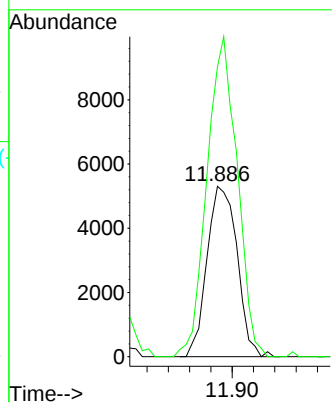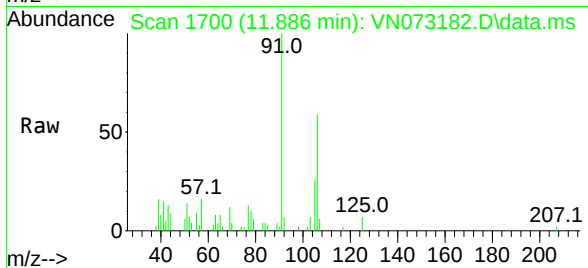

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. 0.000 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion:152 Resp: 254294
Ion Ratio Lower Upper
152 100
115 59.8 28.9 86.7
150 157.5 0.0 356.2


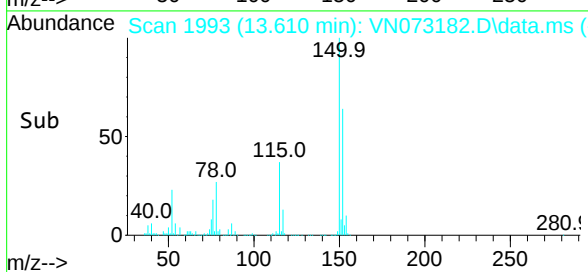
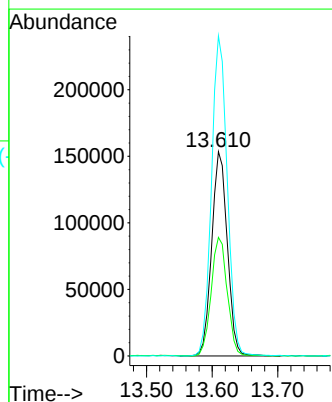
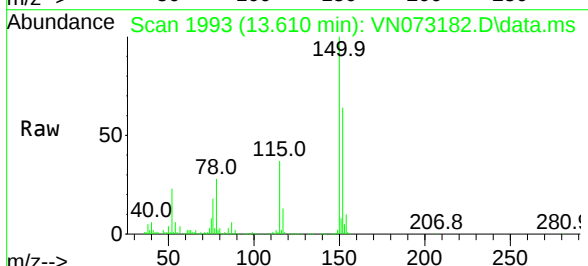




#74
N-amy1 acetate
Concen: 0.382 ug/l
RT: 12.304 min Scan# 11
Delta R.T. -0.023 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion: 43	Resp: 3896
Ion Ratio	Lower Upper
43 100	
70 14.8	39.0 58.4#
55 0.0	21.1 31.7#
61 0.0	21.1 31.7#

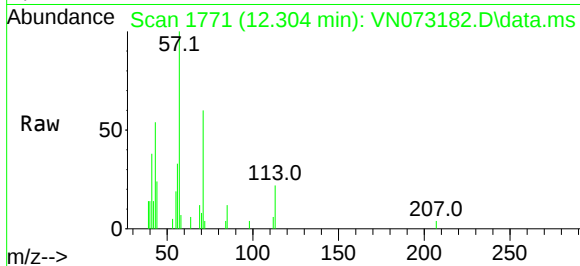

#76
1,2,3-Trichloropropane
Concen: 21.789 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.147 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Tgt Ion: 75	Resp: 134338
Ion Ratio	Lower Upper
75 100	
77 1.4	98.5 295.5#

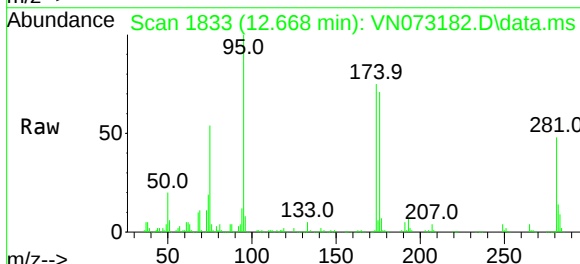

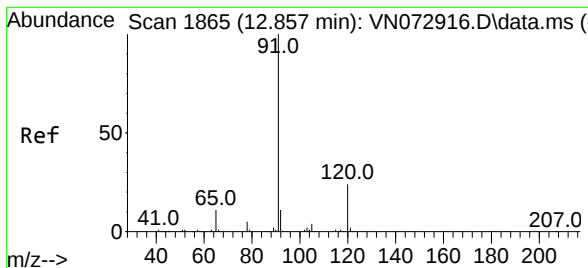

#78

n-propylbenzene

Concen: 0.707 ug/l

RT: 12.863 min Scan# 1866

Delta R.T. 0.006 min

Lab File: VN073182.D

Acq: 28 Jun 2022 00:35

Instrument :

MSVOA_N

ClientSampleId :





SP-EXC-2-2-GR

Tgt Ion: 91 Resp: 15303

Ion Ratio Lower Upper

91 100

120 22.1 11.9 35.5

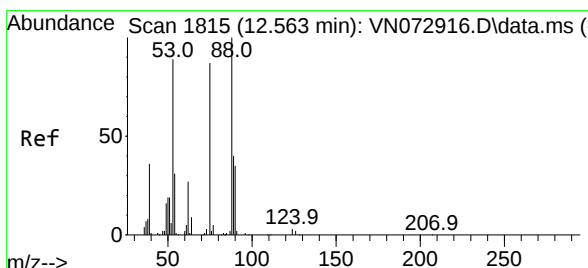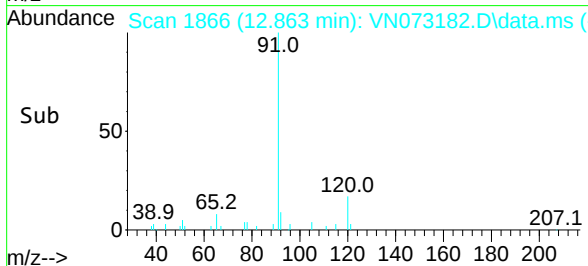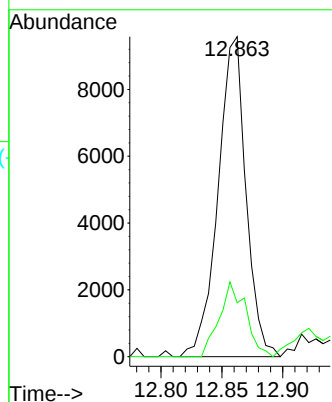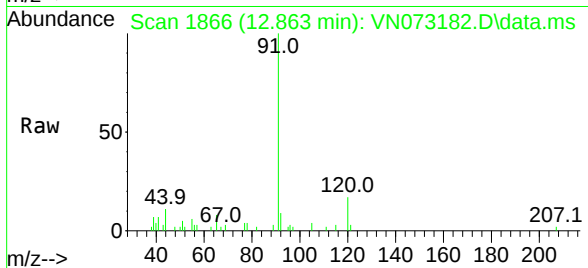

#81

trans-1,4-Dichloro-2-butene

Concen: 58.845 ug/l

RT: 12.668 min Scan# 1833

Delta R.T. 0.106 min

Lab File: VN073182.D

Acq: 28 Jun 2022 00:35




Tgt Ion: 75 Resp: 134338


Ion Ratio Lower Upper

75 100

53 0.1 78.0 117.0#

89 0.6 37.2 55.8#

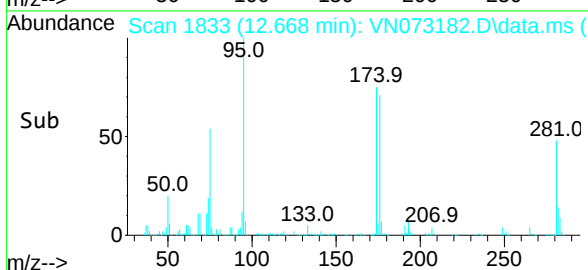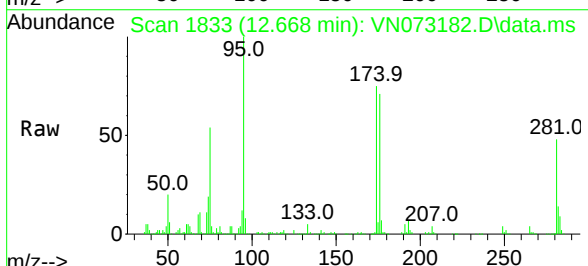



#84

1,2,4-Trimethylbenzene

Concen: 0.595 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. 0.000 min

Lab File: VN073182.D

Acq: 28 Jun 2022 00:35

Instrument :

MSVOA_N

ClientSampleId :





SP-EXC-2-2-GR

Tgt Ion:105 Resp: 9584

Ion Ratio Lower Upper

105 100

120 48.9 23.3 69.8



#89

n-Butylbenzene

Concen: 0.261 ug/l

RT: 13.880 min Scan# 2039

Delta R.T. 0.006 min

Lab File: VN073182.D

Acq: 28 Jun 2022 00:35




Tgt Ion: 91 Resp: 3410


Ion Ratio Lower Upper

91 100

92 48.4 26.9 80.7

134 0.0 13.6 40.8#


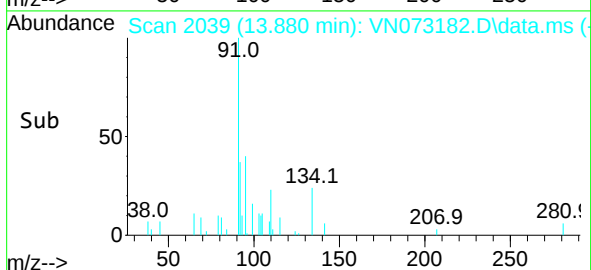




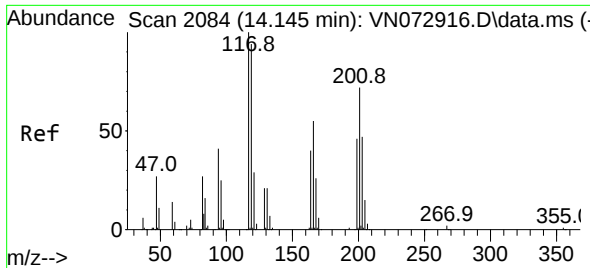

#90
Hexachloroethane
Concen: 0.229 ug/l
RT: 14.157 min Scan# 2086
Delta R.T. 0.012 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35




Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR


Tgt Ion:117 Resp: 691
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

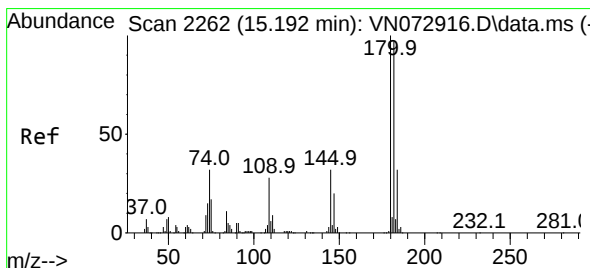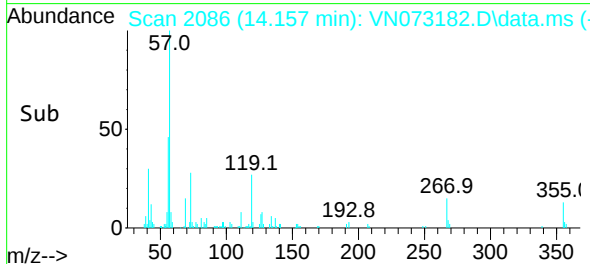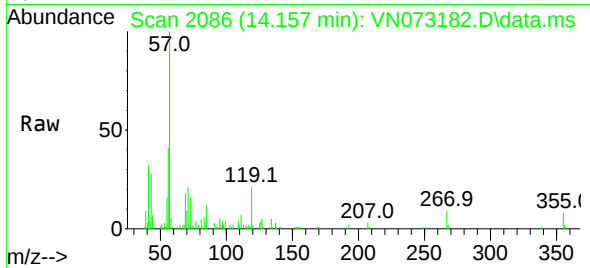

#93
1,2,4-Trichlorobenzene
Concen: 0.209 ug/l
RT: 15.186 min Scan# 2261
Delta R.T. -0.006 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35


Tgt Ion:180 Resp: 1017
Ion Ratio Lower Upper
180 100
182 181.8 47.5 142.5#
145 93.1 14.5 43.5#

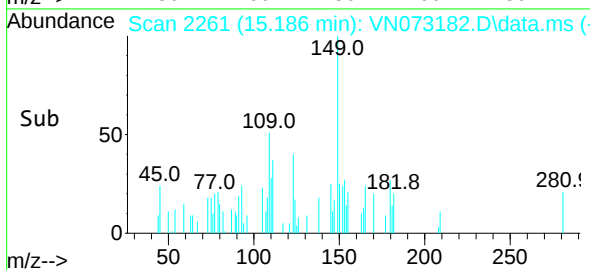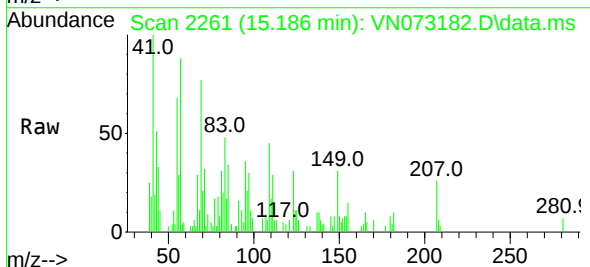

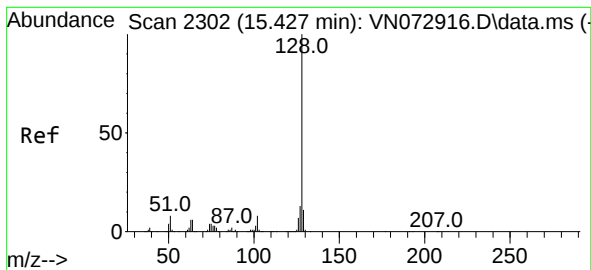

#95
Naphthalene
Concen: 0.762 ug/l
RT: 15.433 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN073182.D
Acq: 28 Jun 2022 00:35

Instrument :
MSVOA_N
ClientSampleId :
SP-EXC-2-2-GR

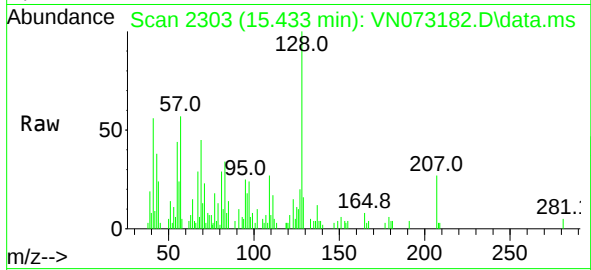

Tgt Ion:128 Resp: 14970
Ion Ratio Lower Upper
128 100
127 13.8 10.3 15.5
129 11.3 8.6 13.0

