

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN062723\  
Data File : VN078421.D  
Acq On : 27 Jun 2023 17:05  
Operator : JC\MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060623W.M

Title : SW846 8260

Signal : TIC: VN078421.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 8.177       | 1047          | 1058        | 1062         | rBV      | 301540         | 720447        | 34.86%          | 7.224%        |
| 2         | 8.236       | 1062          | 1068        | 1080         | rVB      | 487105         | 1120135       | 54.20%          | 11.231%       |
| 3         | 8.588       | 1119          | 1128        | 1144         | rBV      | 304204         | 686461        | 33.21%          | 6.883%        |
| 4         | 9.106       | 1206          | 1216        | 1230         | rBV      | 733510         | 1512749       | 73.19%          | 15.168%       |
| 5         | 10.571      | 1457          | 1465        | 1478         | rBV      | 1081666        | 2066813       | 100.00%         | 20.723%       |
| 6         | 11.112      | 1550          | 1557        | 1564         | rBV5     | 17327          | 32058         | 1.55%           | 0.321%        |
| 7         | 11.871      | 1678          | 1686        | 1700         | rBV      | 937245         | 1738996       | 84.14%          | 17.436%       |
| 8         | 12.853      | 1845          | 1853        | 1865         | rBV      | 602418         | 1098024       | 53.13%          | 11.009%       |
| 9         | 13.800      | 2006          | 2014        | 2023         | rBV      | 572846         | 997858        | 48.28%          | 10.005%       |




Sum of corrected areas: 9973541

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN062723\  
Data File : VN078421.D  
Acq On : 27 Jun 2023 17:05  
Operator : JC\MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060623W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

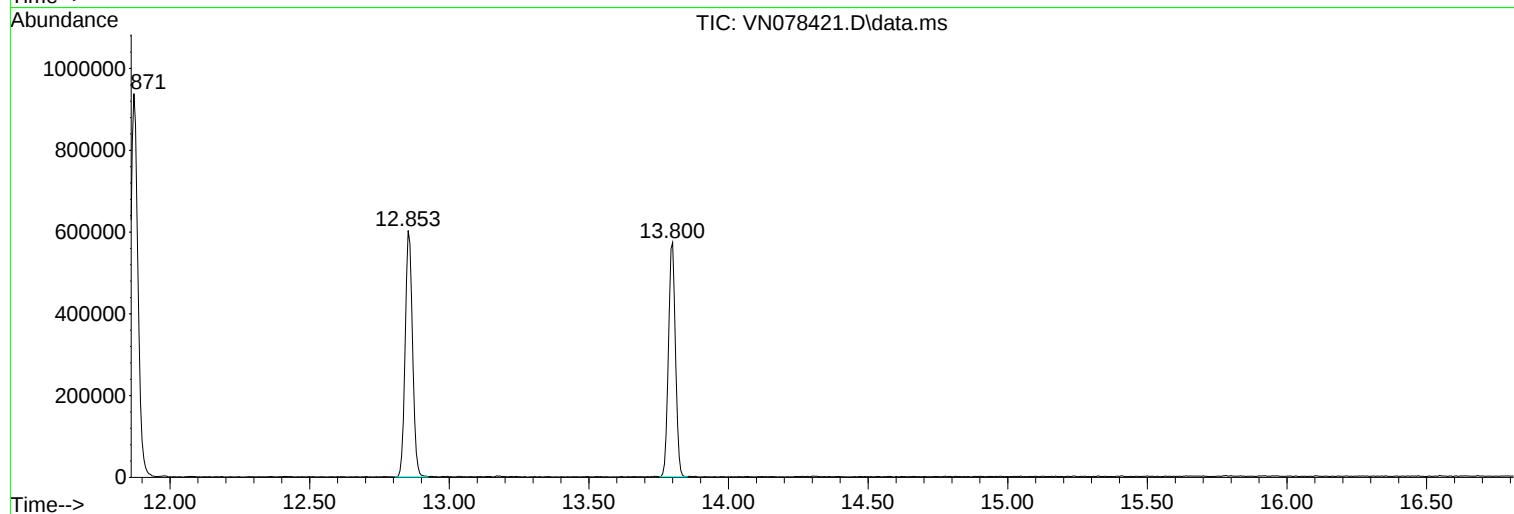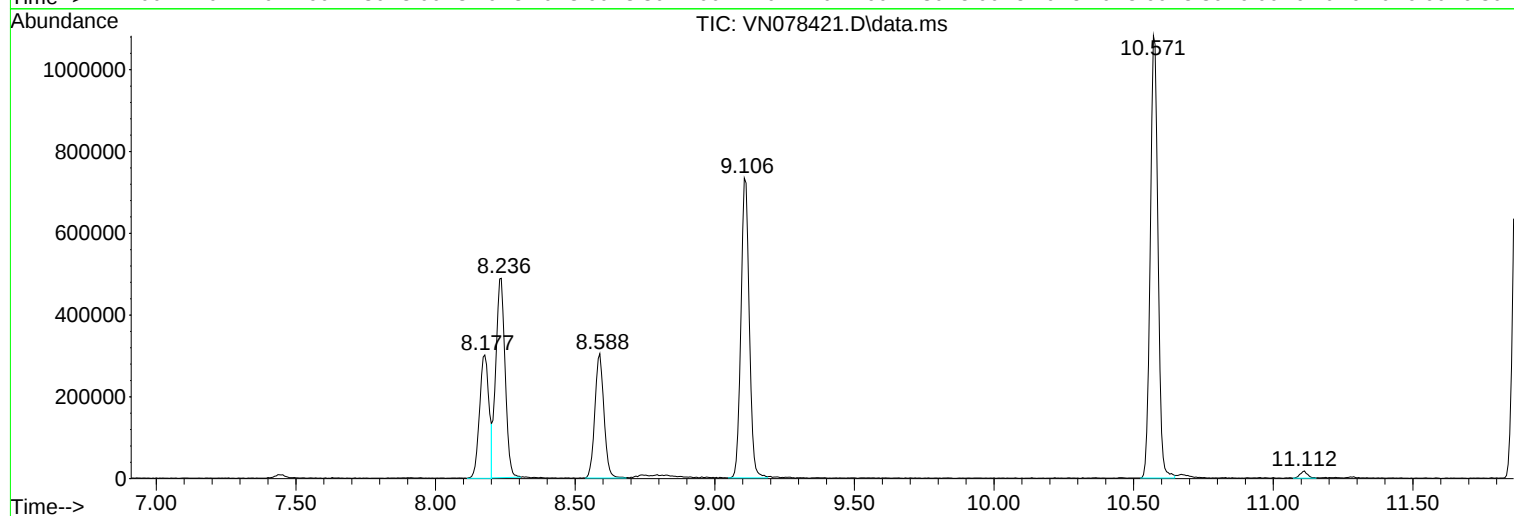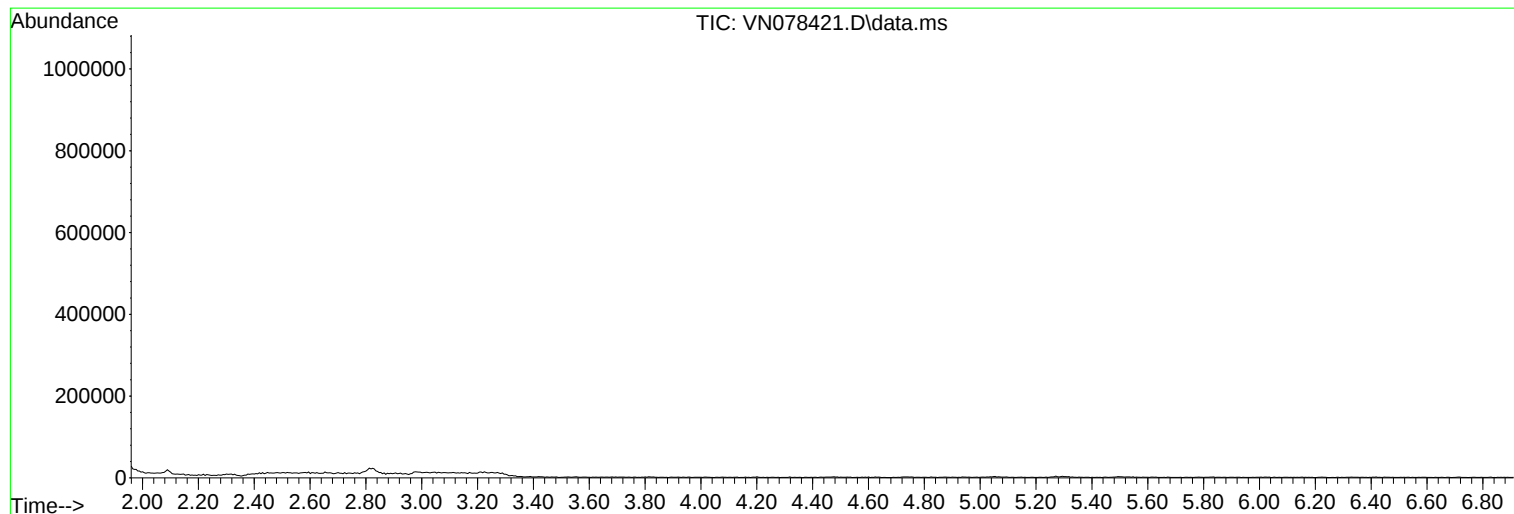

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN062723\  
Data File : VN078421.D  
Acq On : 27 Jun 2023 17:05  
Operator : JC\MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060623W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN062723\  
Data File : VN078421.D  
Acq On : 27 Jun 2023 17:05  
Operator : JC\MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060623W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|