
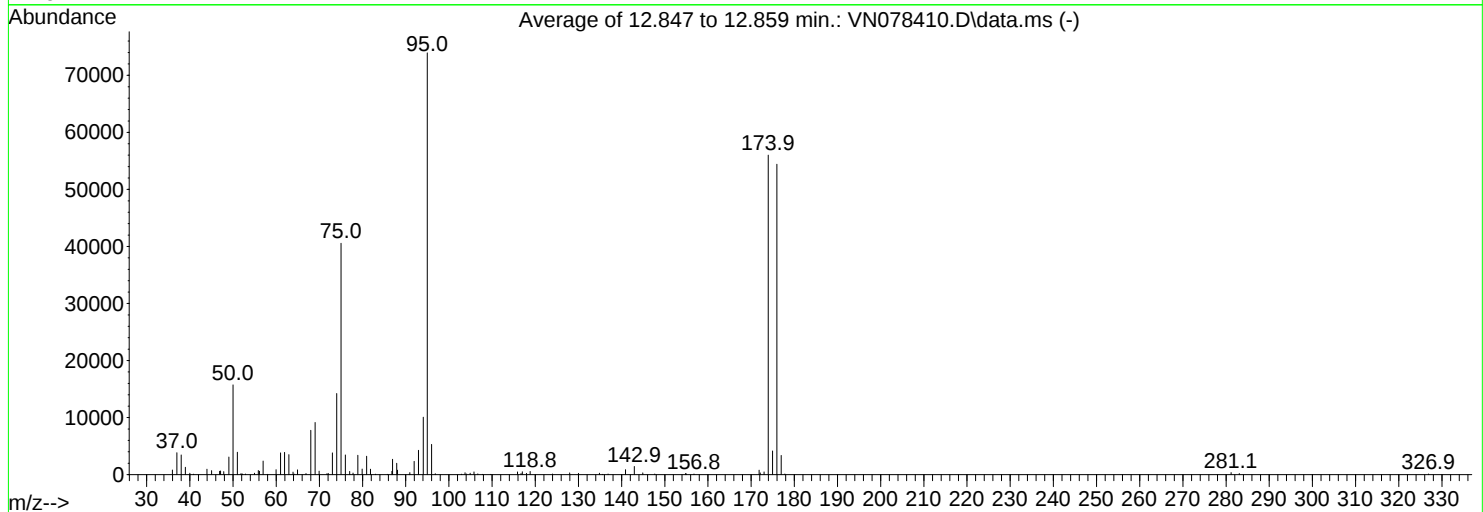


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062723\
Data File : VN078410.D
Acq On : 27 Jun 2023 09:02
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Title : SW846 8260
Last Update : Wed Jun 07 05:05:00 2023

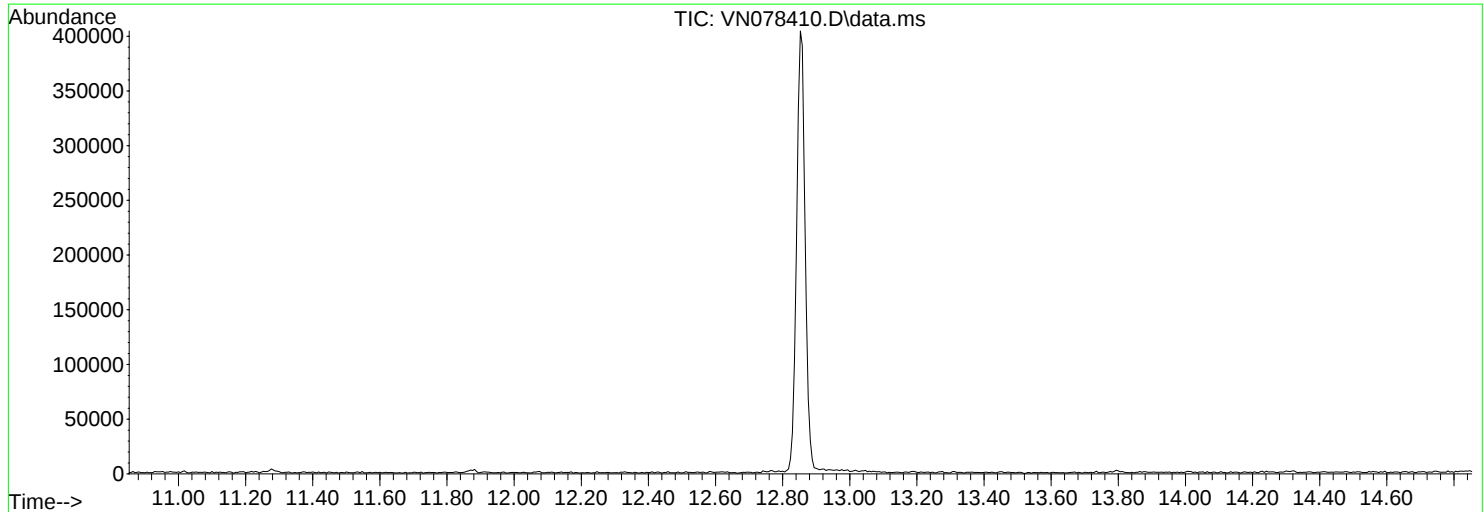

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	15751	PASS
75	95	30	60	54.9	40563	PASS
95	95	100	100	100.0	73939	PASS
96	95	5	9	7.2	5304	PASS
173	174	0.00	2	0.8	468	PASS
174	95	50	100	75.7	56000	PASS
175	174	5	9	7.4	4159	PASS
176	174	95	101	97.2	54427	PASS
177	176	5	9	6.2	3371	PASS

Average of 12.847 to 12.859 min.: VN078410.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	825	49.05	3099	59.95	877	71.75	16
37.00	3832	50.00	15751	61.00	3804	72.05	22
38.00	3464	51.00	3916	61.95	3894	73.00	382
38.95	1295	51.85	199	62.95	3501	74.00	1422
40.00	243	52.20	102	63.90	439	75.00	40563
40.90	87	52.90	106	64.10	124	76.00	3462
43.95	963	54.95	266	64.95	855	77.00	557
45.05	710	55.85	739	66.90	204	77.80	275
46.90	594	56.10	579	68.00	7783	78.90	3393
47.10	642	56.95	2387	69.00	9148	79.90	994
47.85	540	58.00	55	69.95	609	80.95	3232

Average of 12.847 to 12.859 min.: VN078410.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	966	94.05	10083	109.70	57	136.85	124
83.00	78	95.00	73939	115.90	476	140.90	887
85.80	55	96.00	5304	116.70	202	142.95	1433
86.80	595	96.85	165	117.00	493	144.90	315
86.95	2688	102.90	75	117.95	226	147.70	118
87.90	1994	103.75	332	118.80	549	154.80	192
88.10	784	104.10	105	124.00	126	155.00	133
90.80	75	104.90	246	127.95	308	156.75	116
90.95	375	105.80	468	130.00	215	171.85	803
91.95	2324	106.70	138	134.85	243	172.10	316
92.95	4277	107.80	53	135.60	65	173.00	468

Average of 12.847 to 12.859 min.: VN078410.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.95	56000						
174.95	4159						
175.95	54427						
176.95	3371						
177.80	107						
281.15	368						
283.05	200						
326.90	111						