
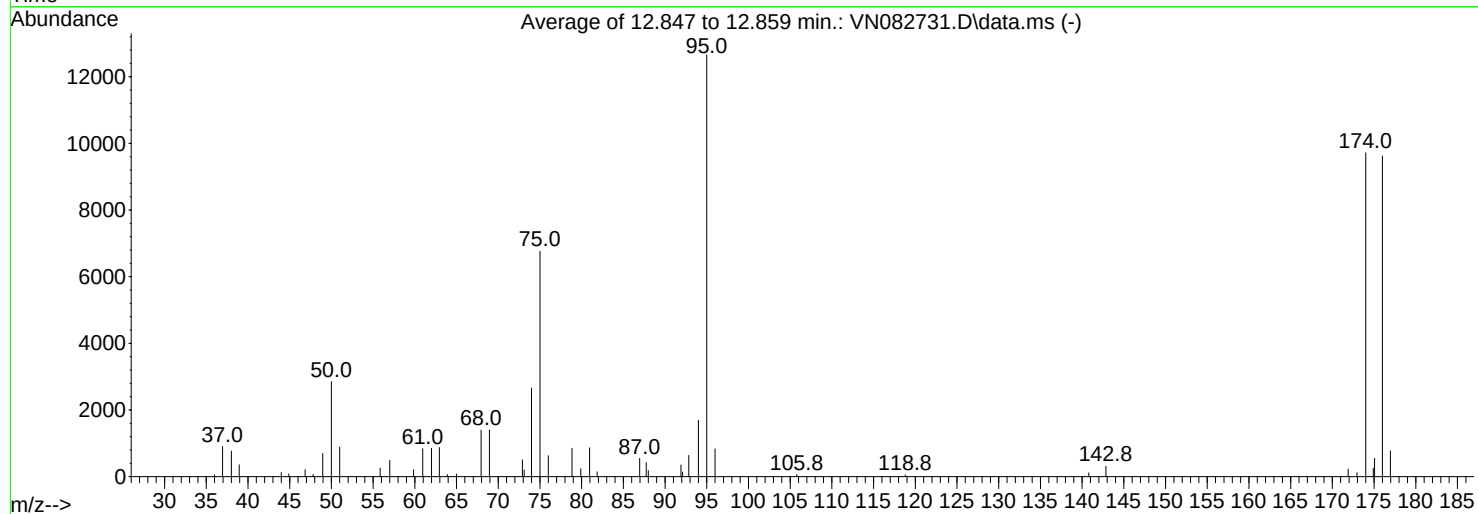


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062724\
Data File : VN082731.D
Acq On : 27 Jun 2024 20:48
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062724W.M
Title : SW846 8260
Last Update : Fri Jun 28 06:02:21 2024

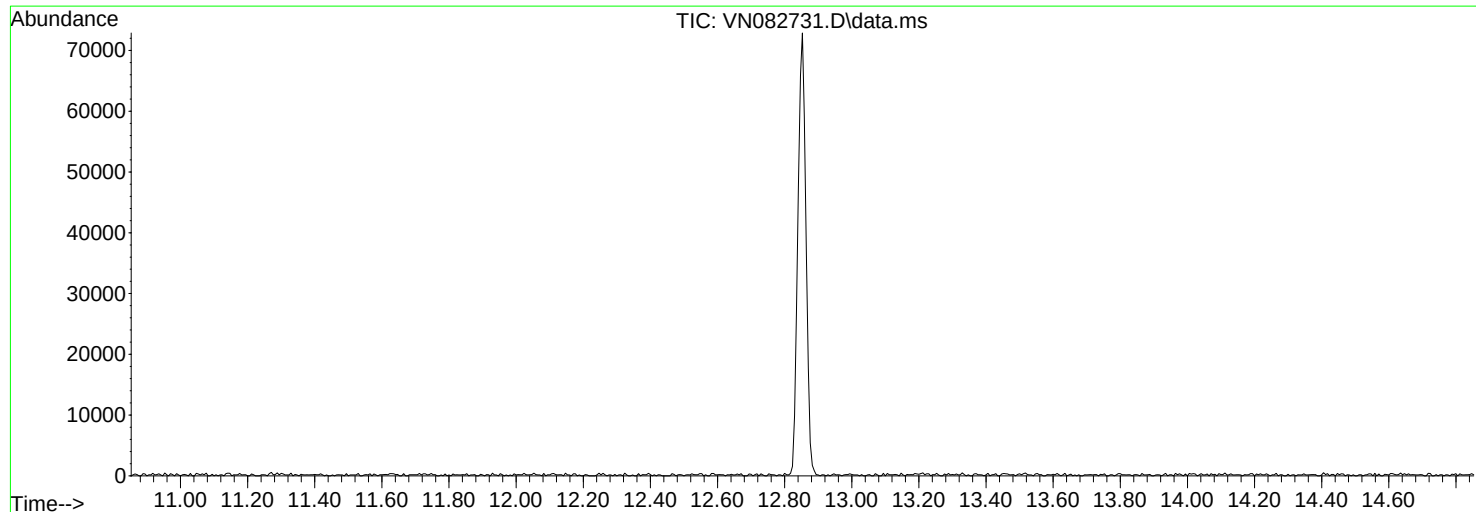

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	2853	PASS
75	95	30	60	53.5	6767	PASS
95	95	100	100	100.0	12657	PASS
96	95	5	9	6.6	831	PASS
173	174	0.00	2	1.2	115	PASS
174	95	50	100	76.8	9718	PASS
175	174	5	9	5.6	546	PASS
176	174	95	101	99.0	9621	PASS
177	176	5	9	8.0	773	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	59	55.85	260	73.10	201	91.90	351
36.95	902	57.00	491	74.00	2662	92.10	131
38.00	766	59.85	207	75.00	6767	92.85	63
38.95	355	60.95	840	76.00	631	94.00	169
44.00	123	62.00	851	78.85	848	95.00	12657
44.90	80	62.95	874	79.90	242	96.00	831
46.85	213	63.90	63	80.95	866	105.80	61
47.80	66	65.00	76	81.85	143	118.80	55
48.95	696	67.95	1396	86.95	546	140.80	115
50.00	2853	68.95	1398	87.75	423	142.85	314
51.00	887	72.90	504	88.00	182	171.90	226

Average of 12.847 to 12.859 min.: VN082731.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.95	115						
174.00	9718						
174.90	248						
175.05	546						
176.00	9621						
176.95	773						

Instrument :

MSVOA_N

ClientSampleId :

BFB