


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062818\  
 Data File : VN049607.D  
 Acq On : 28 Jun 2018 23:09  
 Operator : MD\SY  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N061618W.M  
 Title : SW846 8260  
 Last Update : Sat Jun 16 01:02:01 2018

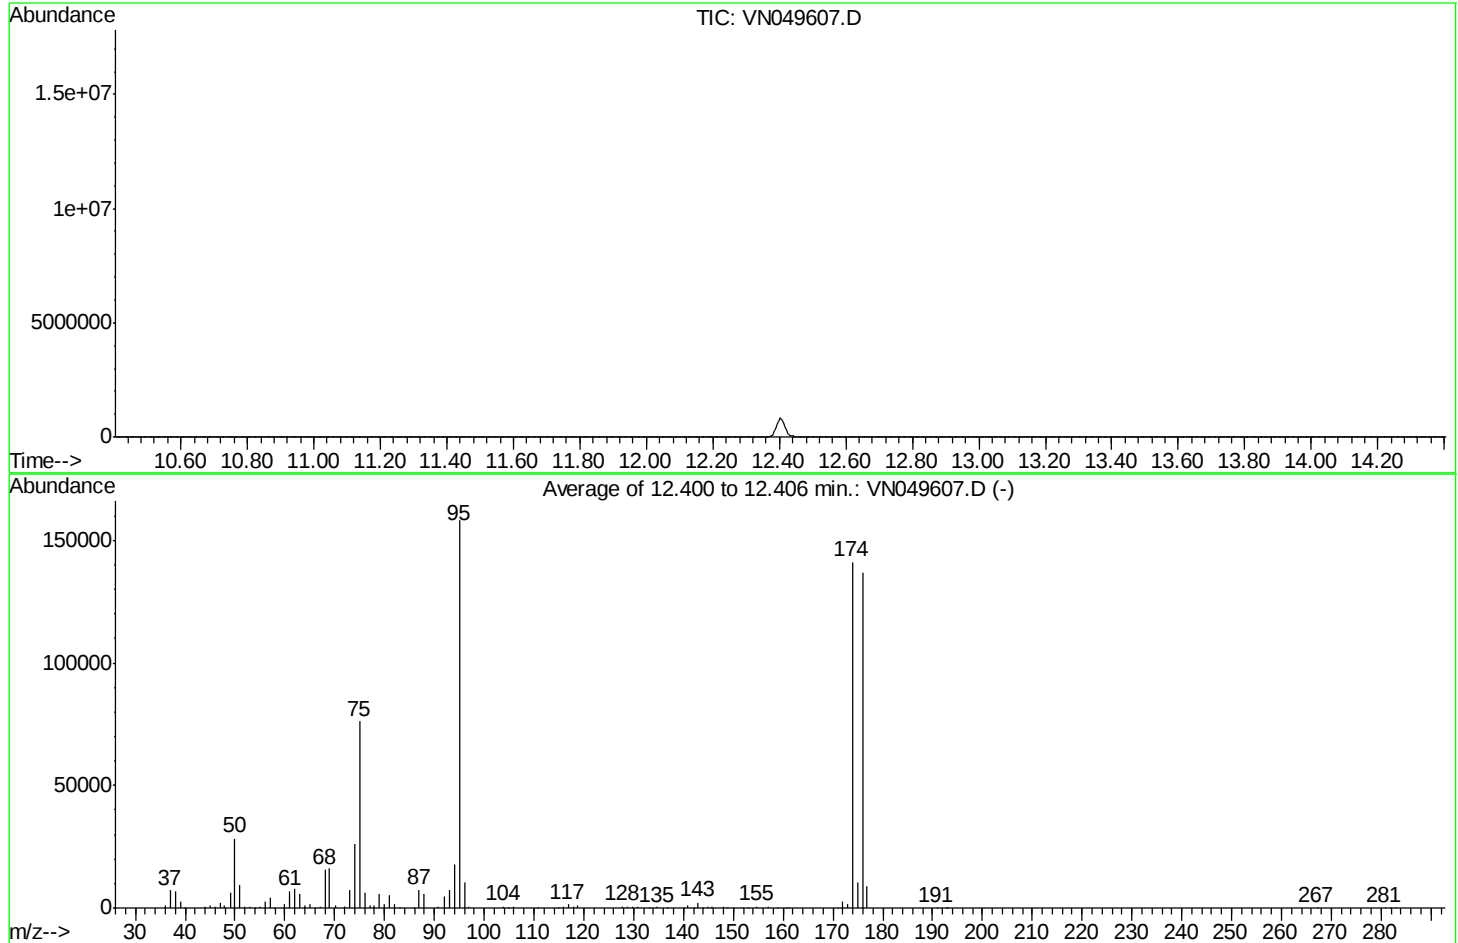

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3347

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.9      | 28285   | PASS             |
| 75          | 95           | 30           | 60           | 48.2      | 76213   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 158208  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 10639   | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 1539    | PASS             |
| 174         | 95           | 50           | 100          | 89.3      | 141290  | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 10575   | PASS             |
| 176         | 174          | 95           | 101          | 96.7      | 136664  | PASS             |
| 177         | 176          | 5            | 9            | 6.4       | 8729    | PASS             |