

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN062819\
 Data File : VN056540.D
 Acq On : 28 Jun 2019 8:51
 Operator : JC/SP
 Sample : VSSTDCCC005
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VSSTDCCC005

Quant Time: Jun 28 23:35:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062719SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 28 03:22:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	52503	5.00	ug/l	0.00
4) 1,4-Difluorobenzene	8.58	114	84460	5.00	ug/l	0.00
8) Chlorobenzene-d5	11.41	117	48663	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.35	152	6284	5.00	ug/l	0.00

System Monitoring Compounds

3) 1,2-Dichloroethane-d4	8.01	65	32402	5.04	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	100.80%
5) Dibromofluoromethane	7.59	113	25046	5.38	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	107.60%
6) Toluene-d8	10.09	98	54736	5.20	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	104.00%
7) 4-Bromofluorobenzene	12.40	95	12930	4.80	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	96.00%

Target Compounds


	R.T.	QIon	Response	Conc	Units	Qvalue
2) Vinyl Chloride	2.17	62	26897	5.124	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN062819\
Data File : VN056540.D
Acq On : 28 Jun 2019 8:51
Operator : JC/SP
Sample : VSSTDCCC005
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VSSTDCCC005

Quant Time: Jun 28 23:35:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062719SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Fri Jun 28 03:22:32 2019
Response via : Initial Calibration

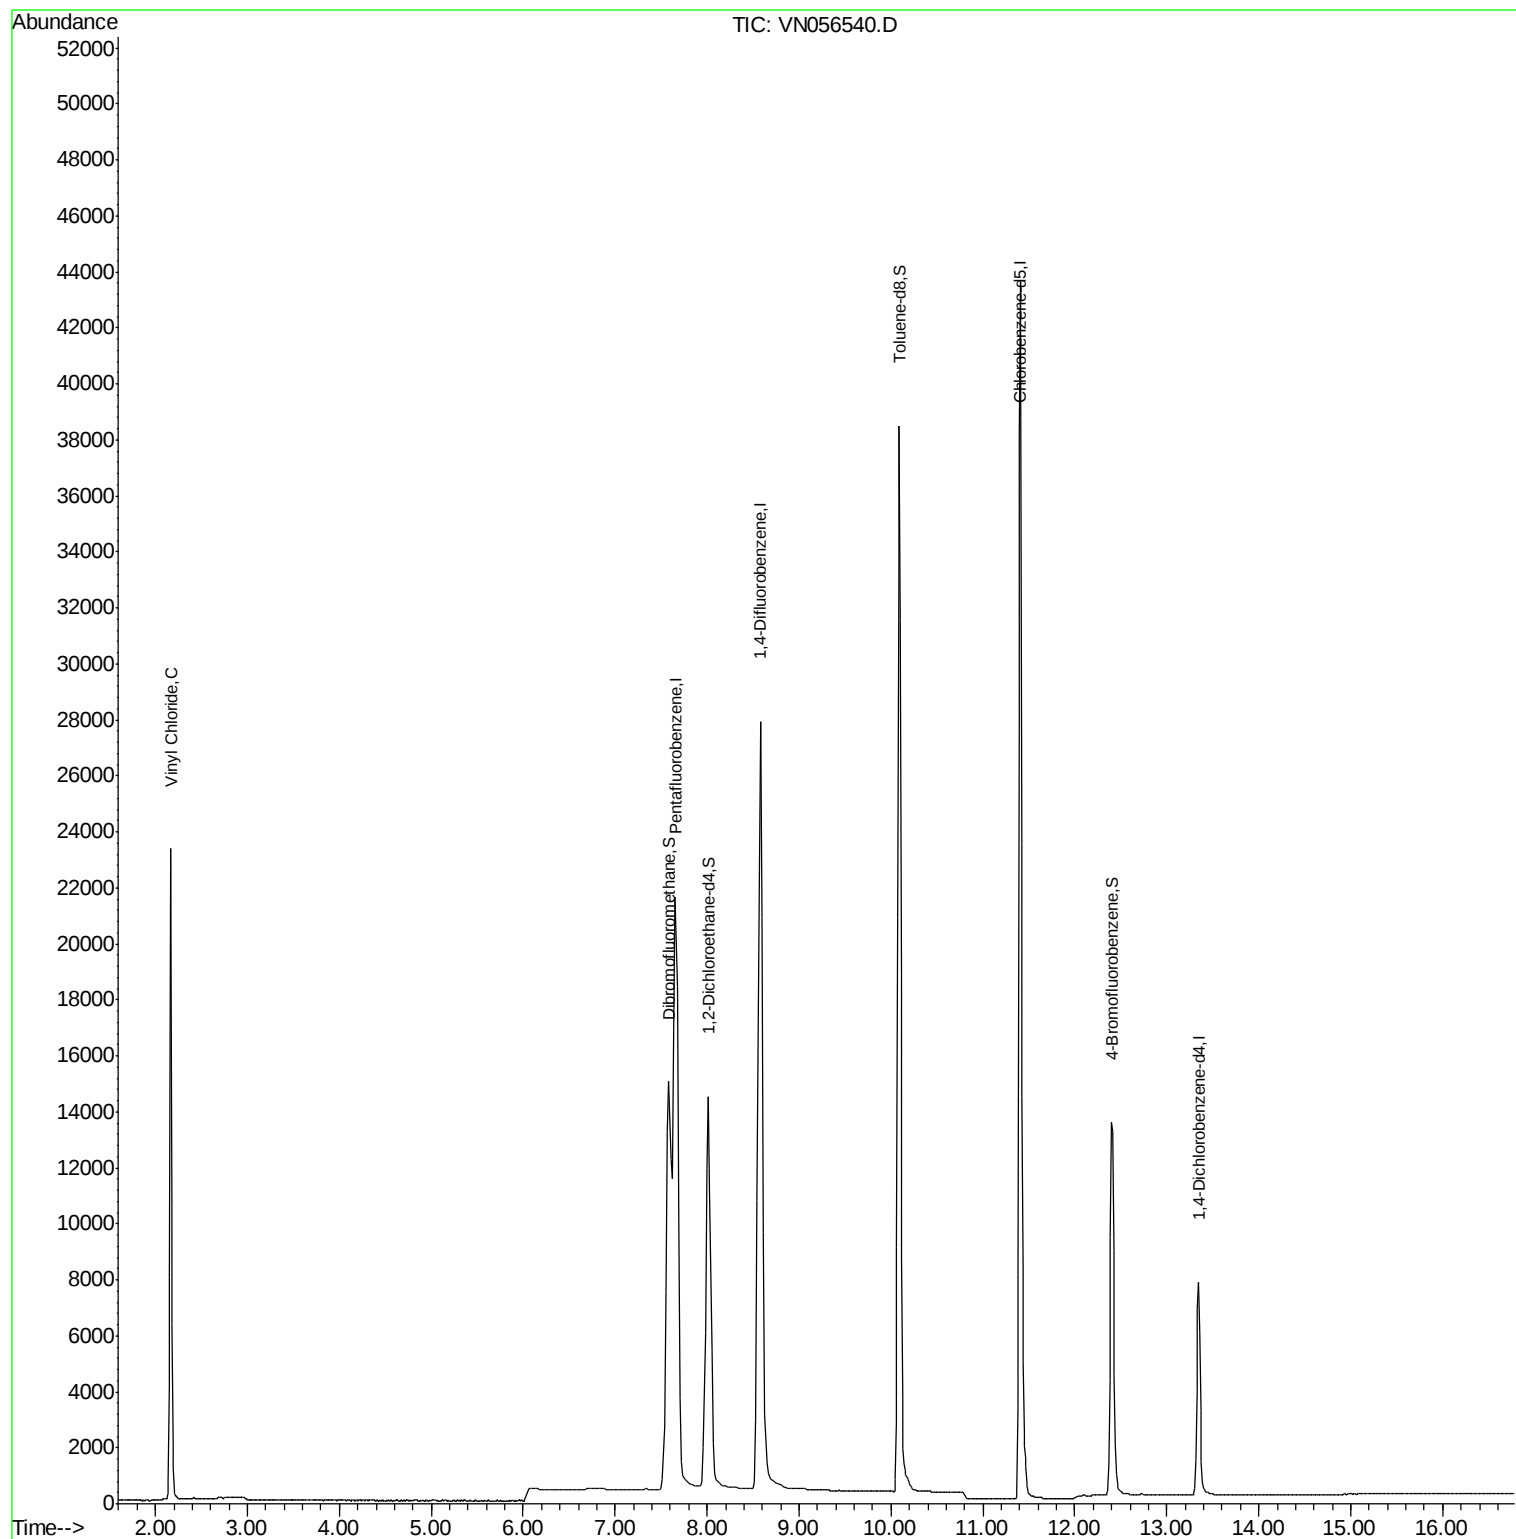

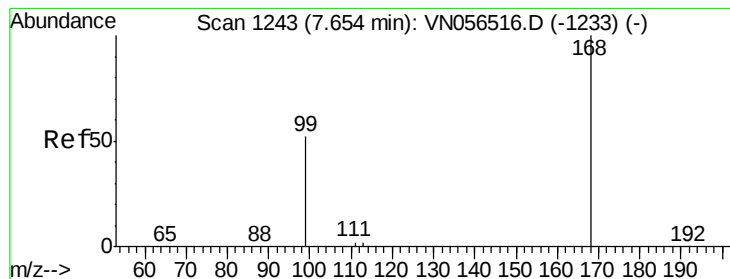

#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.65 min Scan# 1243

Delta R.T. 0.00 min

Lab File: VN056540.D

Acq: 28 Jun 2019 8:51

Instrument :

MSVOA_N

ClientSampleId :


VSTDCCC005

Tot Ion:168 Resp: 52503




Ion Ratio Lower Upper

168 100

99 49.8 41.9 62.9

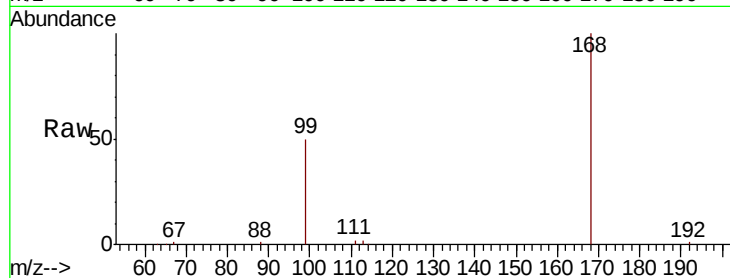

Abundance Ion 168.00 (167.70 to 168.70): VN056540.D (-1226) (-)

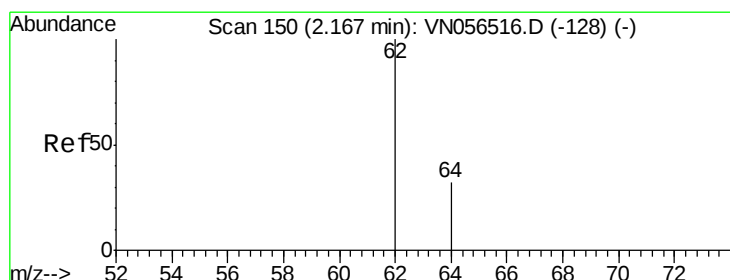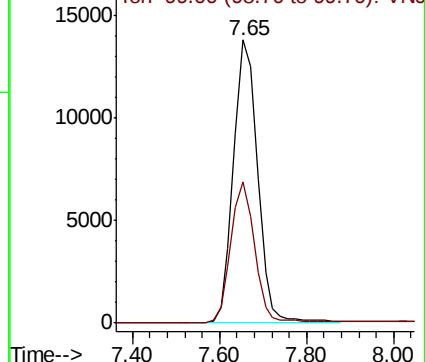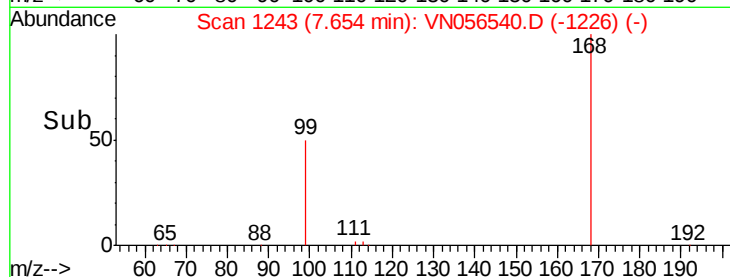

#2

Vinyl Chloride

Concen: 5.124 ug/l

RT: 2.17 min Scan# 150

Delta R.T. 0.00 min

Lab File: VN056540.D


Acq: 28 Jun 2019 8:51

Tgt Ion: 62 Resp: 26897



Ion Ratio Lower Upper


62 100

64 32.8 26.1 39.1

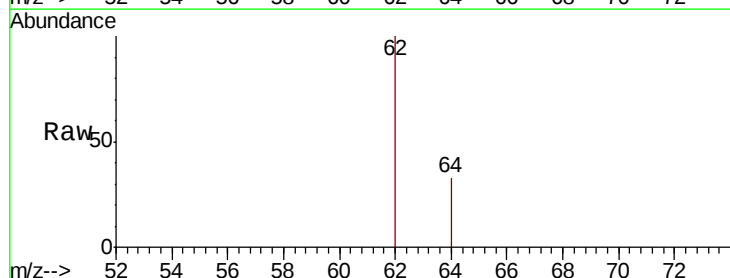

Abundance Ion 62.00 (61.70 to 62.70): VN056540.D (-98) (-)

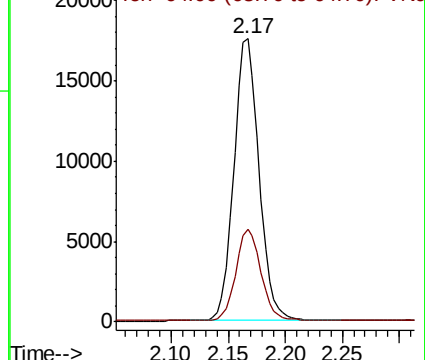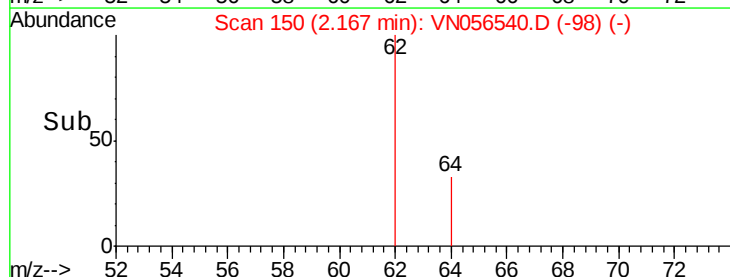

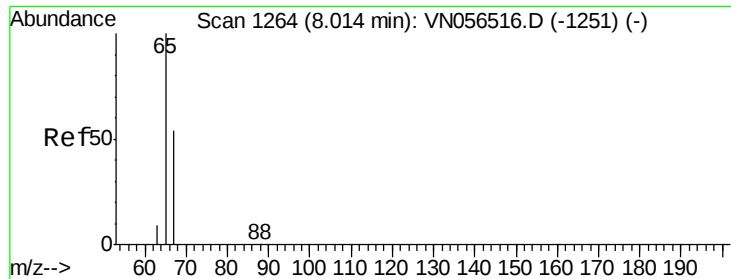

#3

1,2-Dichloroethane-d4

Concen: 5.038 ug/l

RT: 8.01 min Scan# 1264

Delta R.T. -0.00 min

Lab File: VN056540.D

Acq: 28 Jun 2019 8:51

Instrument :

MSVOA_N

ClientSampleId :





VSTDCCC005

Tot Ion: 65 Resp: 32402

Ion Ratio Lower Upper

65 100

67 54.7 0.0 108.8

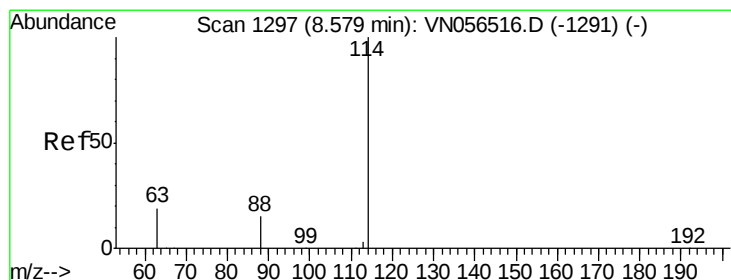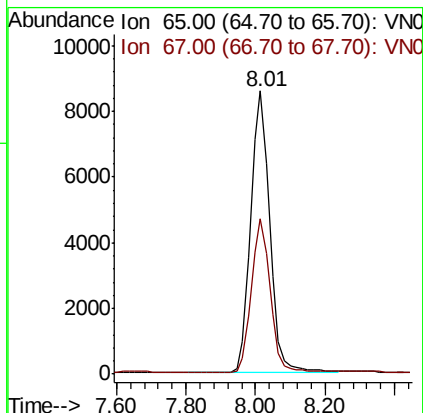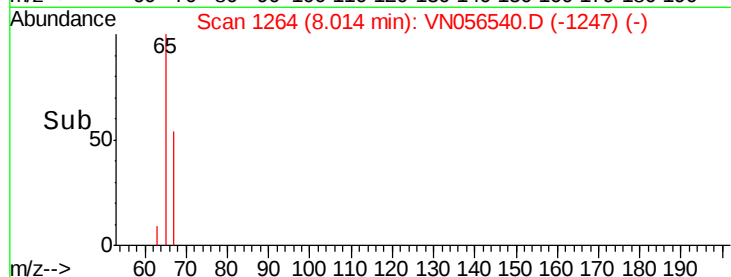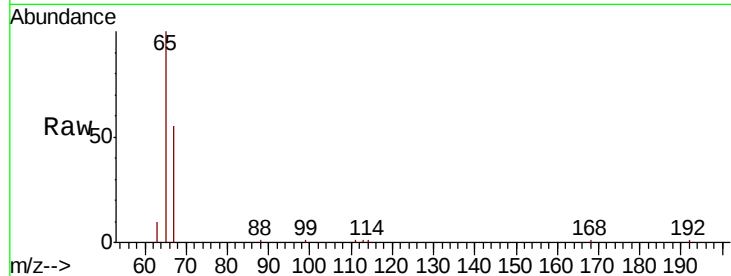

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.58 min Scan# 1297

Delta R.T. 0.00 min

Lab File: VN056540.D

Acq: 28 Jun 2019 8:51




Tgt Ion: 114 Resp: 84460


Ion Ratio Lower Upper

114 100

63 18.2 0.0 37.6

88 15.0 0.0 31.2

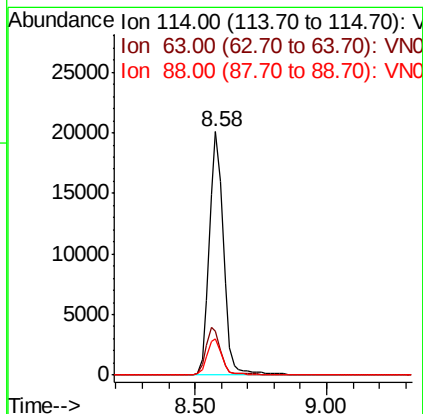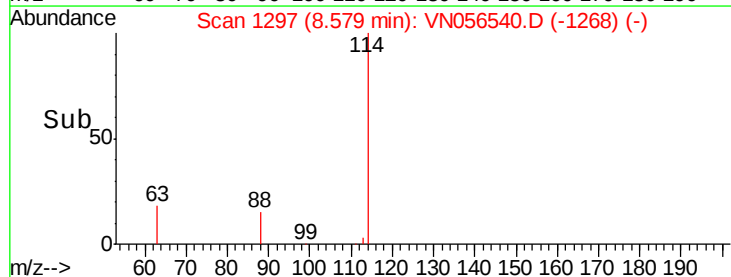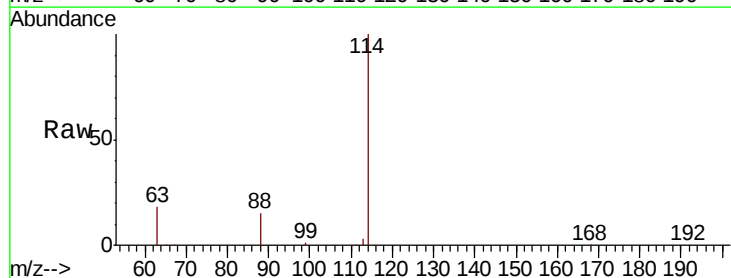

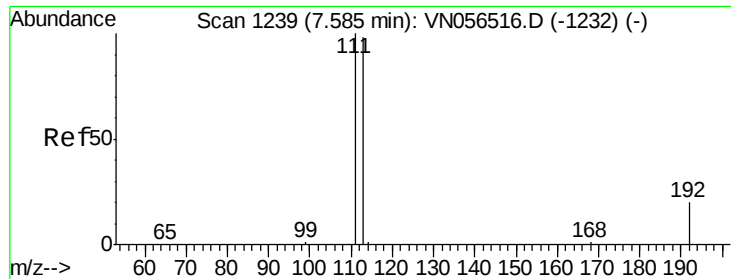

#5

Dibromofluoromethane

Concen: 5.379 ug/l

RT: 7.59 min Scan# 1239

Delta R.T. -0.00 min

Lab File: VN056540.D

Acq: 28 Jun 2019 8:51

Instrument :

MSVOA_N

ClientSampleId :

VSSTDCCC005


Tot Ion:113 Resp: 25046

Ion Ratio Lower Upper

113 100

111 100.7 81.7 122.5




192 21.2 16.9 25.3

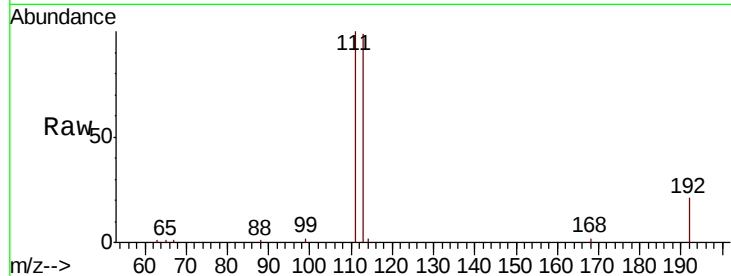

Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

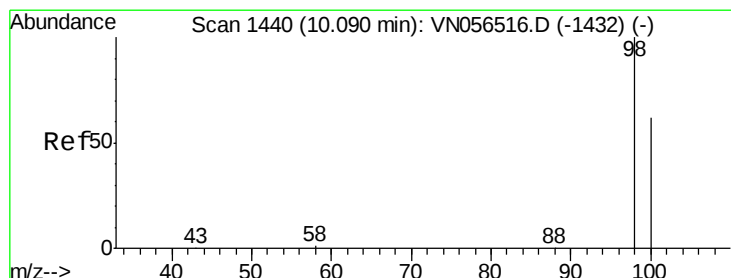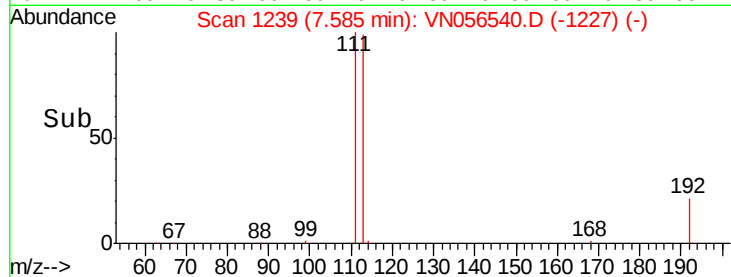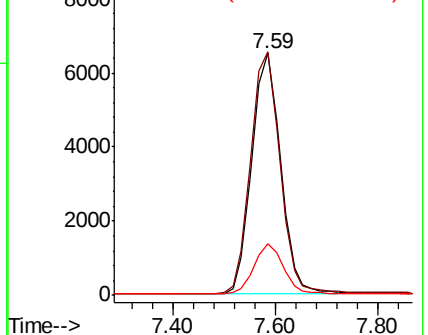

#6

Toluene-d8

Concen: 5.195 ug/l

RT: 10.09 min Scan# 1440

Delta R.T. 0.00 min

Lab File: VN056540.D


Acq: 28 Jun 2019 8:51

Tgt Ion: 98 Resp: 54736

Ion Ratio Lower Upper



98 100


100 63.1 49.7 74.5

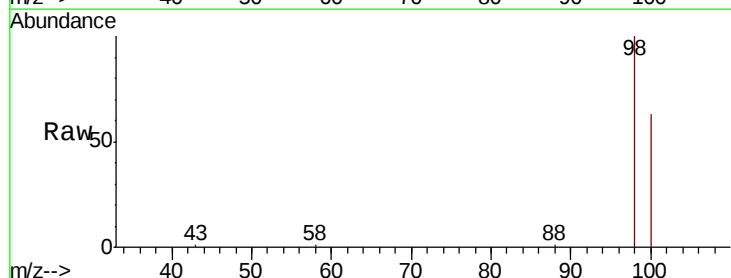

Abundance Ion 98.00 (97.70 to 98.70): VN

Ion 100.00 (99.70 to 100.70): VN

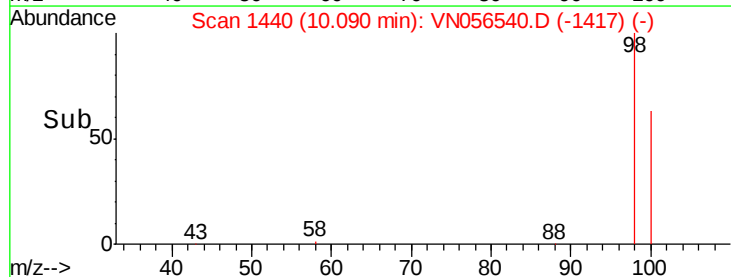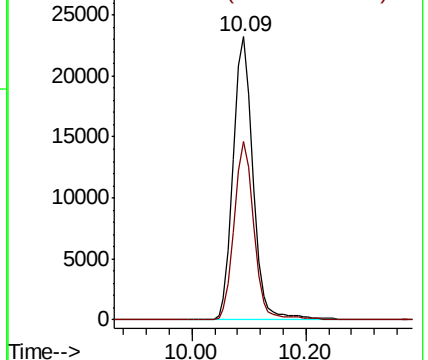

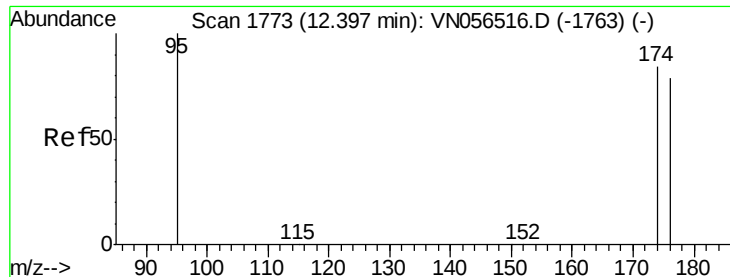

#7

4-Bromofluorobenzene

Concen: 4.798 ug/l

RT: 12.40 min Scan# 1773

Delta R.T. 0.00 min

Lab File: VN056540.D

Acq: 28 Jun 2019 8:51

Instrument :

MSVOA_N

ClientSampleId :

VSSTDCCC005


Tot Ion: 95 Resp: 12930

Ion Ratio Lower Upper

95 100

174 85.1 0.0 167.8




176 78.0 0.0 158.0

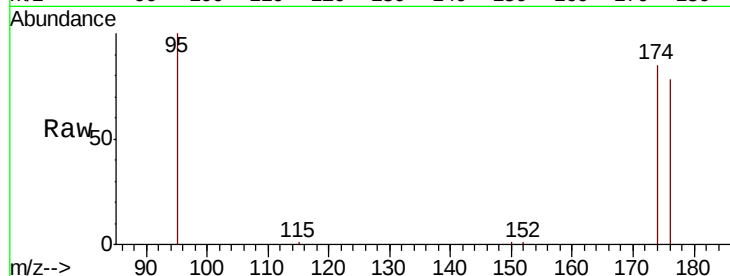

Abundance Ion 95.00 (94.70 to 95.70): VN0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

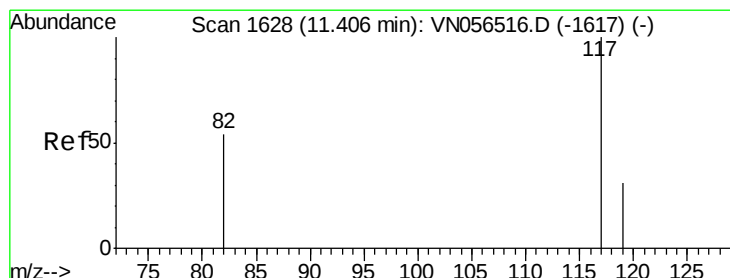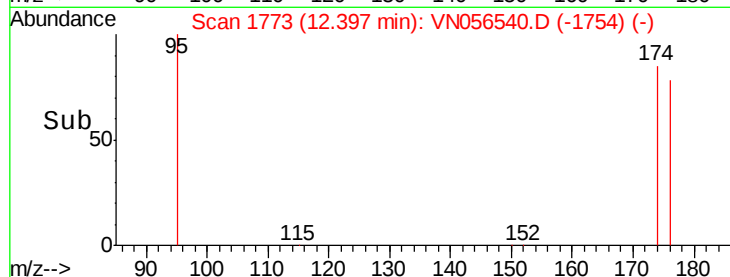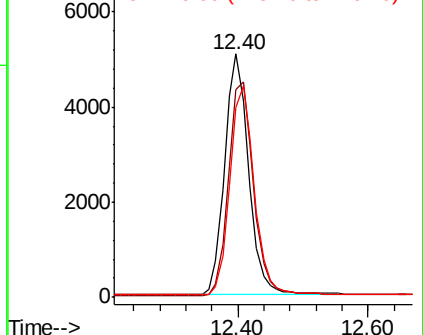

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.41 min Scan# 1628

Delta R.T. -0.00 min

Lab File: VN056540.D

Acq: 28 Jun 2019 8:51


Tgt Ion: 117 Resp: 48663

Ion Ratio Lower Upper

117 100

82 53.4 43.0 64.4



119 31.4 24.7 37.1



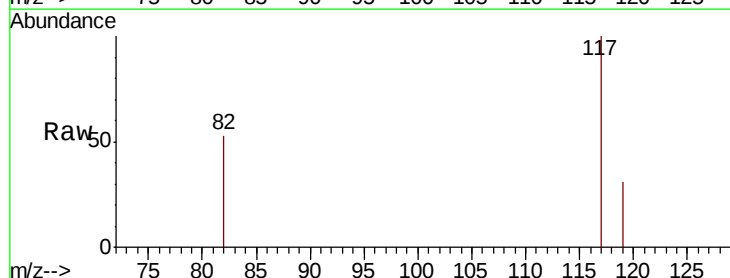


Abundance Ion 117.00 (116.70 to 117.70): V

Ion 82.00 (81.70 to 82.70): VN0

Ion 119.00 (118.70 to 119.70): V

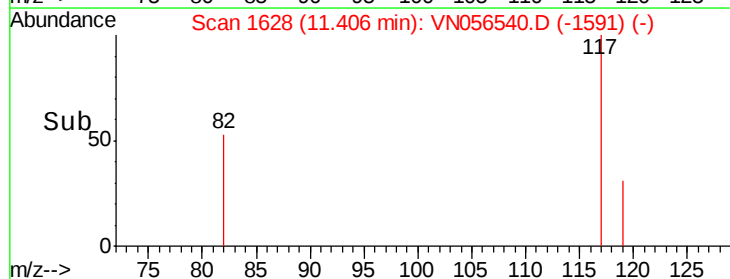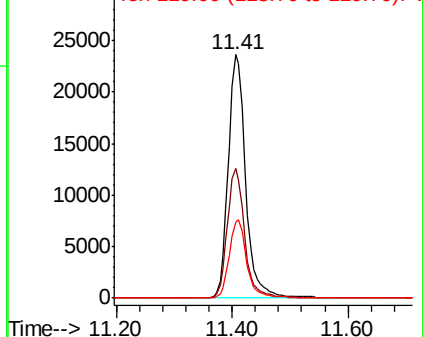

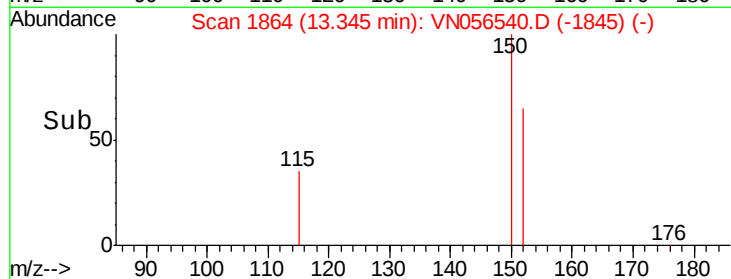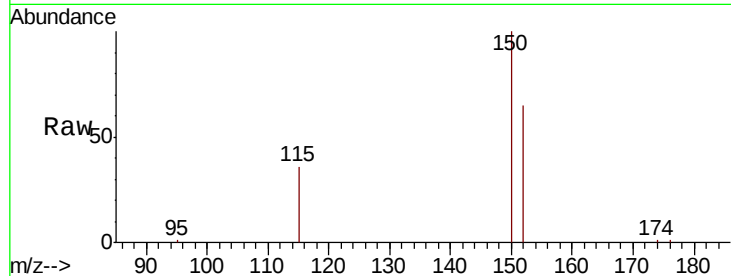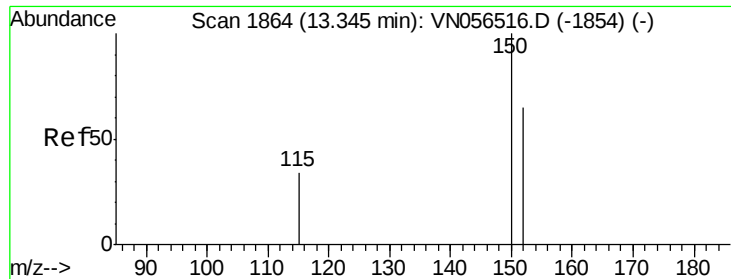

#9

1,4-Dichlorobenzene-d4

Concen: 5.000 ug/l

RT: 13.35 min Scan# 1864

Delta R.T. -0.00 min

Lab File: VN056540.D

Acq: 28 Jun 2019 8:51

Instrument :

MSVOA_N

ClientSampleId :

VSSTDCCC005

Tot Ion:152 Resp: 6284

Ion Ratio Lower Upper

152 100

115 55.1 27.0 80.8

150 153.5 0.0 306.6

Abundance

Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

