

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN062819\
 Data File : VN056544.D
 Acq On : 28 Jun 2019 10:34
 Operator : JC/SP
 Sample : 0.05ppb LOD
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 0.05ppb LOD

Quant Time: Jun 28 23:30:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062719SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 28 03:22:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	52455	5.00	ug/l	0.00
4) 1,4-Difluorobenzene	8.59	114	89261	5.00	ug/l	0.00
8) Chlorobenzene-d5	11.41	117	54068	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.34	152	8327	5.00	ug/l	0.00

System Monitoring Compounds						
3) 1,2-Dichloroethane-d4	8.01	65	25912	4.03	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	80.60%#
5) Dibromofluoromethane	7.58	113	19345	3.93	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	78.60%#
6) Toluene-d8	10.09	98	42667	3.83	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	76.60%#
7) 4-Bromofluorobenzene	12.39	95	10973	3.85	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	77.00%#


Target Compounds					Qvalue
2) Vinyl Chloride	2.16	62	397	0.076 ug/l #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN062819\
Data File : VN056544.D
Acq On : 28 Jun 2019 10:34
Operator : JC/SP
Sample : 0.05ppb LOD
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
0.05ppb LOD

Quant Time: Jun 28 23:30:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062719SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Fri Jun 28 03:22:32 2019
Response via : Initial Calibration

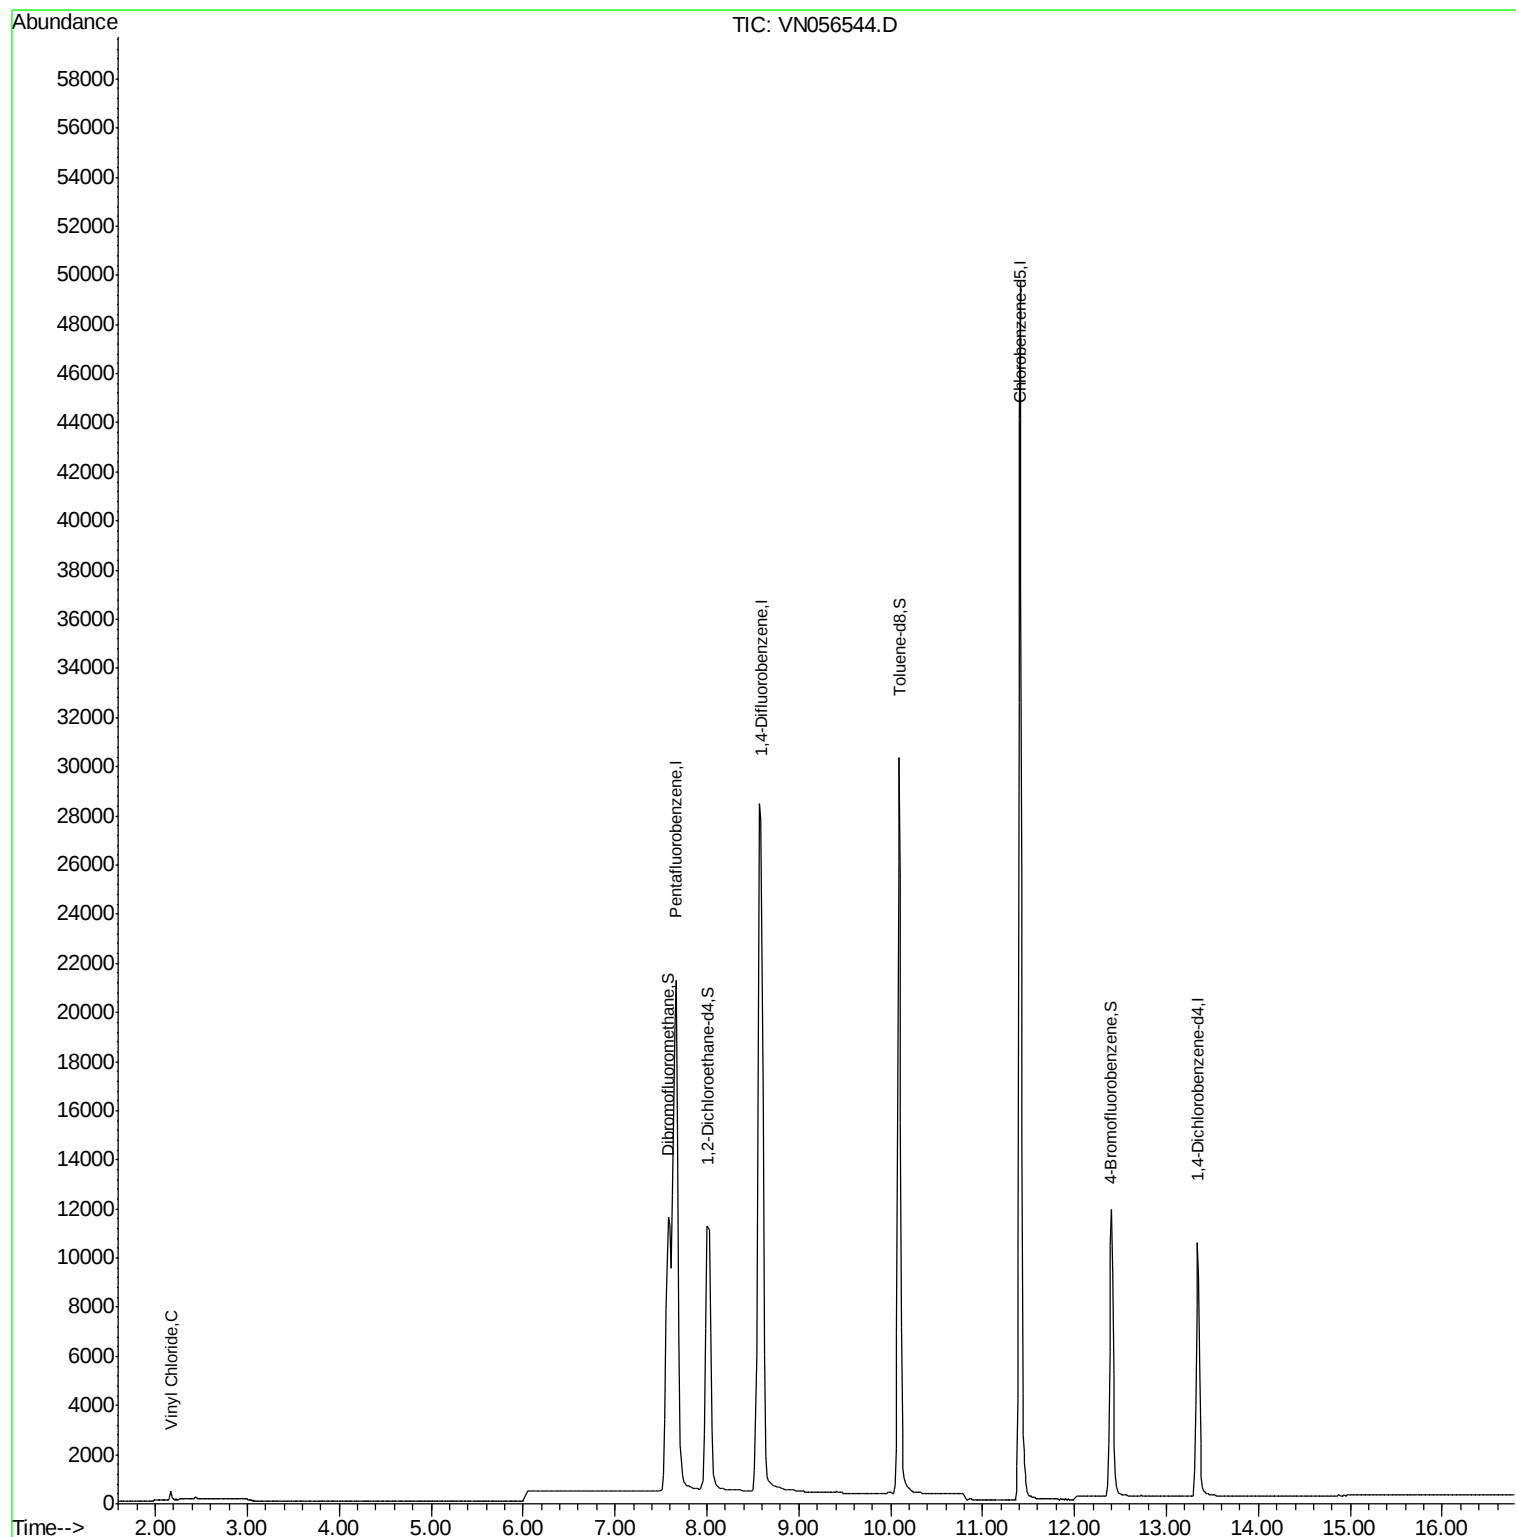

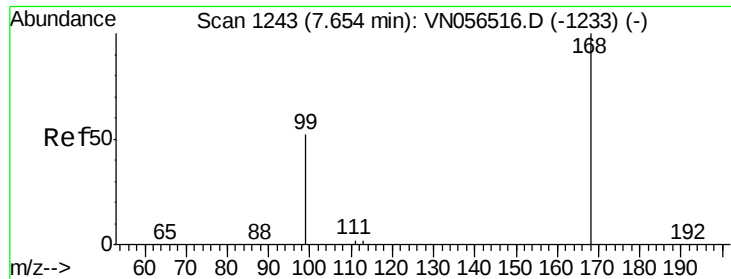

#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.66 min Scan# 1242

Delta R.T. 0.01 min

Lab File: VN056544.D

Acq: 28 Jun 2019 10:34

Instrument :

MSVOA_N

ClientSampleId :


0.05ppb LOD

Tot Ion:168 Resp: 52455

Ion Ratio Lower Upper

168 100

99 46.8 41.9 62.9

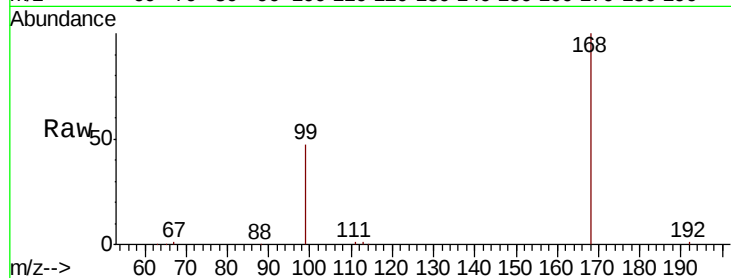

Abundance Ion 168.00 (167.70 to 168.70): VN056516.D (-1233) (-)

Ion 99.00 (98.70 to 99.70): VN056516.D (-1233) (-)

7.66

15000



10000

5000

0

7.40 7.60 7.80 8.00

Time-->

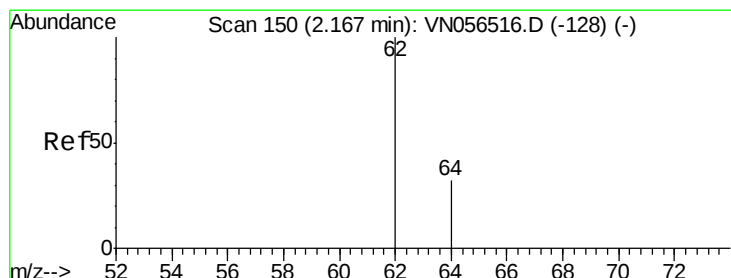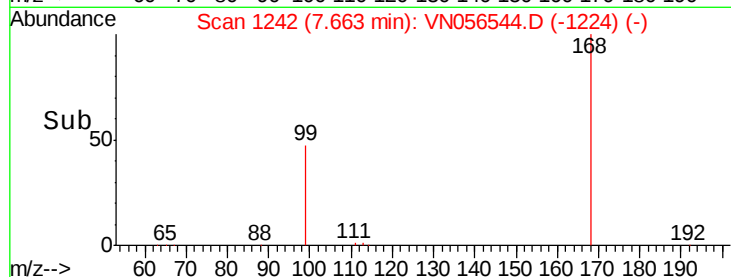

#2

Vinyl Chloride

Concen: 0.076 ug/l

RT: 2.16 min Scan# 149

Delta R.T. -0.00 min

Lab File: VN056544.D


Acq: 28 Jun 2019 10:34

Tgt Ion: 62 Resp: 397

Ion Ratio Lower Upper

62 100

64 51.4 26.1 39.1#

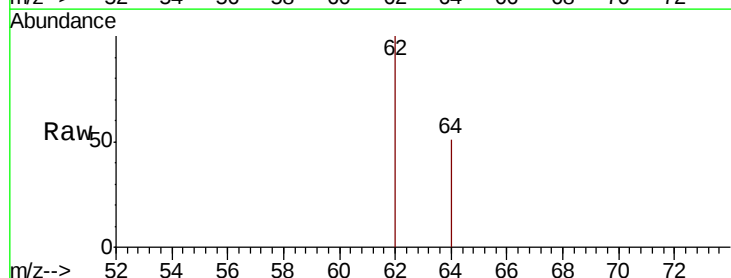

Abundance Ion 62.00 (61.70 to 62.70): VN056516.D (-128) (-)

Ion 64.00 (63.70 to 64.70): VN056516.D (-128) (-)

2.16

300


200


100

0

2.10 2.15 2.20

Time-->

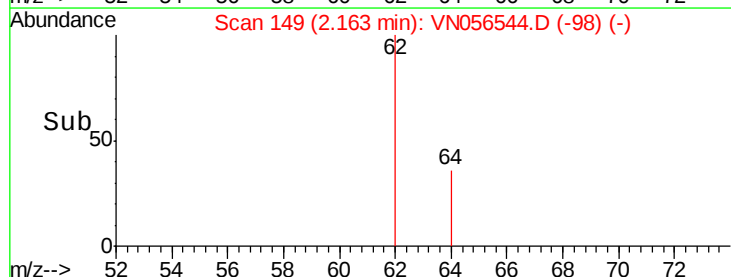

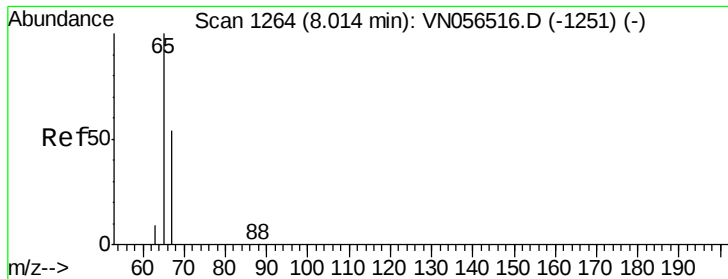

#3

1,2-Dichloroethane-d4

Concen: 4.033 ug/l

RT: 8.01 min Scan# 1262

Delta R.T. -0.01 min

Lab File: VN056544.D

Acq: 28 Jun 2019 10:34

Instrument :

MSVOA_N

ClientSampleId :


0.05ppb LOD

Tot Ion: 65 Resp: 25912

Ion Ratio Lower Upper




65 100

67 52.9 0.0 108.8

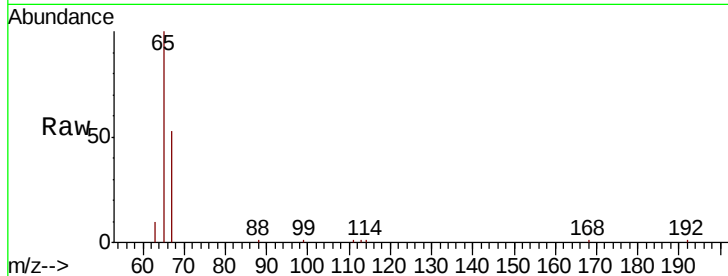

Abundance Ion 65.00 (64.70 to 65.70): VN056516.D (-1251) (-)

Ion 67.00 (66.70 to 67.70): VN056516.D (-1251) (-)

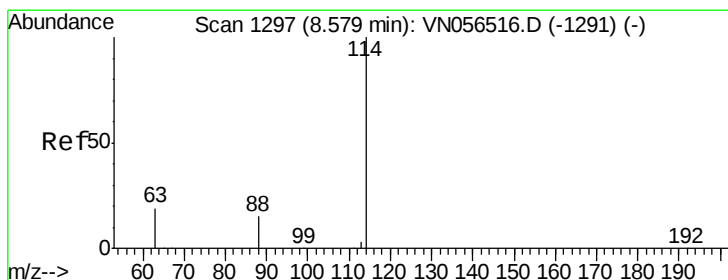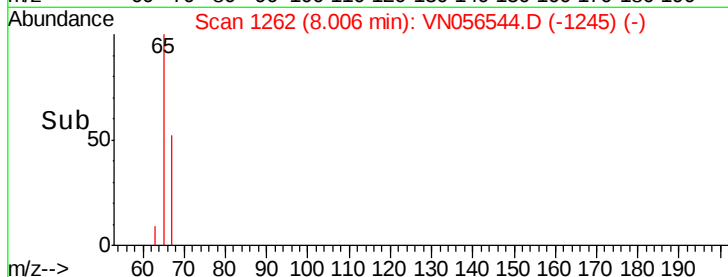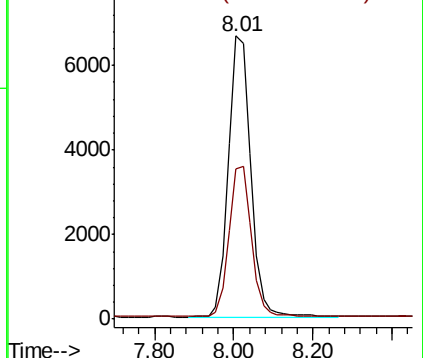

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.59 min Scan# 1296

Delta R.T. 0.01 min

Lab File: VN056544.D

Acq: 28 Jun 2019 10:34


Tgt Ion: 114 Resp: 89261

Ion Ratio Lower Upper

114 100

63 15.3 0.0 37.6



88 13.8 0.0 31.2

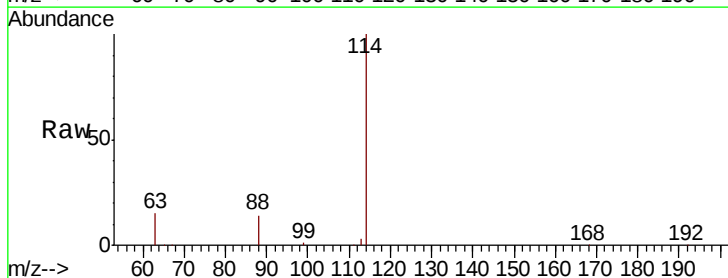

Abundance Ion 114.00 (113.70 to 114.70): VN056516.D (-1291) (-)

Ion 63.00 (62.70 to 63.70): VN056516.D (-1291) (-)

Ion 88.00 (87.70 to 88.70): VN056516.D (-1291) (-)

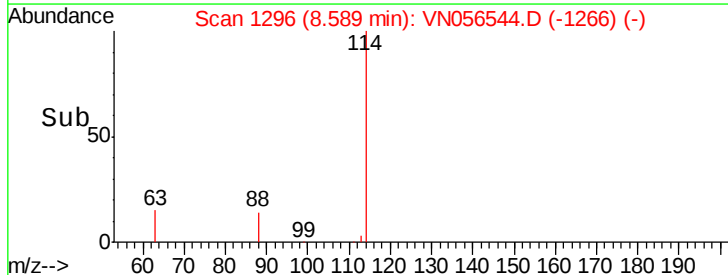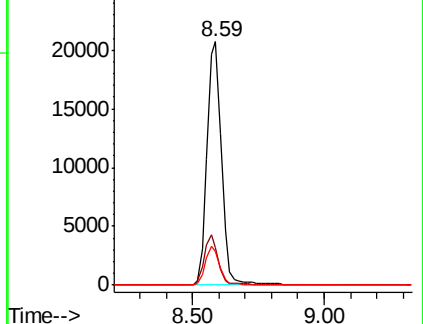



#5

Dibromofluoromethane

Concen: 3.931 ug/l

RT: 7.58 min Scan# 1237

Delta R.T. -0.01 min

Lab File: VN056544.D

Acq: 28 Jun 2019 10:34

Instrument :

MSVOA_N

ClientSampleId :

0.05ppb LOD


Tot Ion:113 Resp: 19345

Ion Ratio Lower Upper

113 100

111 104.2 81.7 122.5




192 20.0 16.9 25.3

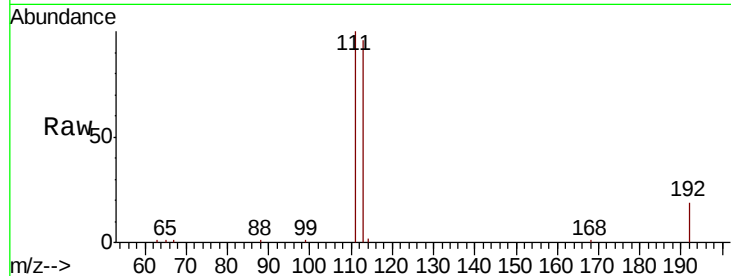

Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

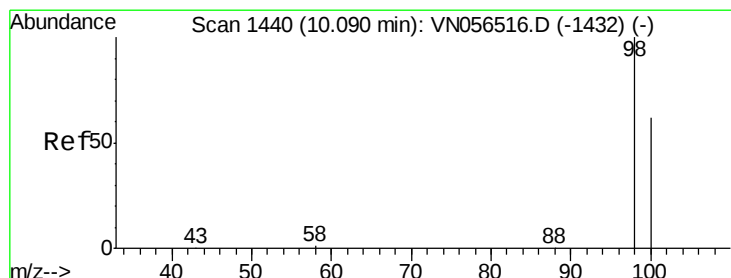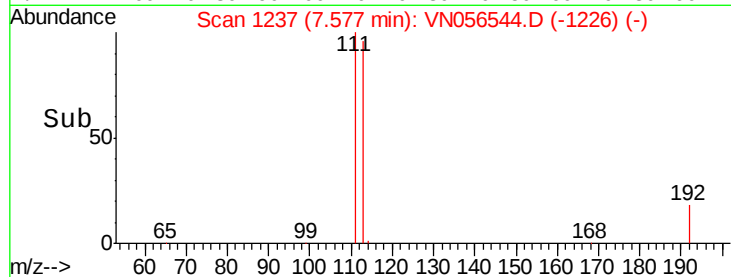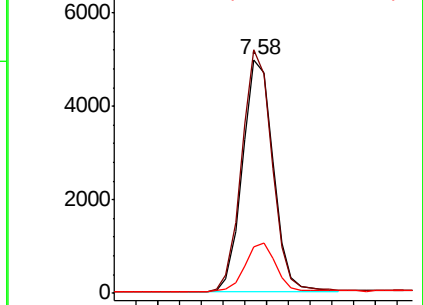

#6

Toluene-d8

Concen: 3.832 ug/l

RT: 10.09 min Scan# 1438

Delta R.T. 0.00 min

Lab File: VN056544.D


Acq: 28 Jun 2019 10:34

Tgt Ion: 98 Resp: 42667

Ion Ratio Lower Upper



98 100

100 63.1 49.7 74.5

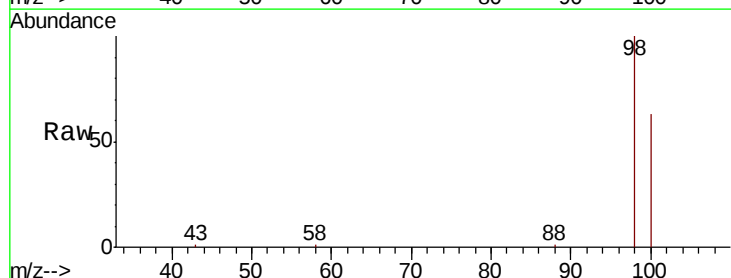

Abundance Ion 98.00 (97.70 to 98.70): V

Ion 100.00 (99.70 to 100.70): V

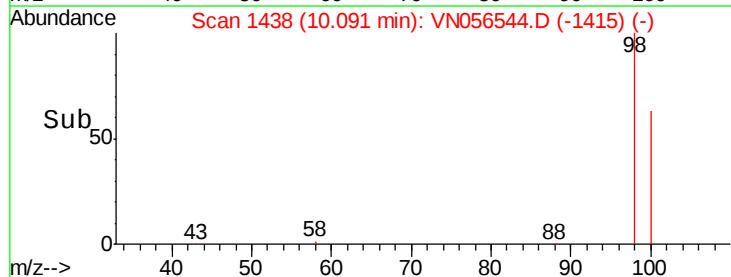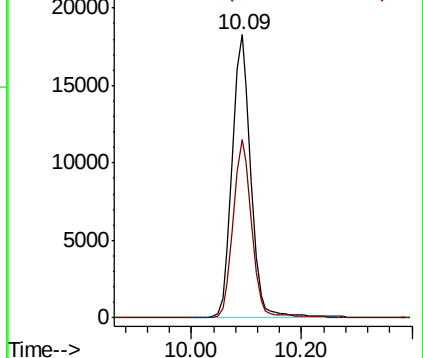



#7

4-Bromofluorobenzene

Concen: 3.853 ug/l

RT: 12.39 min Scan# 1770

Delta R.T. -0.00 min

Lab File: VN056544.D

Acq: 28 Jun 2019 10:34

Instrument :

MSVOA_N

ClientSampled :

0.05ppb LOD


Tot Ion: 95 Resp: 10973

Ion Ratio Lower Upper

95 100

174 75.2 0.0 167.8




176 67.1 0.0 158.0

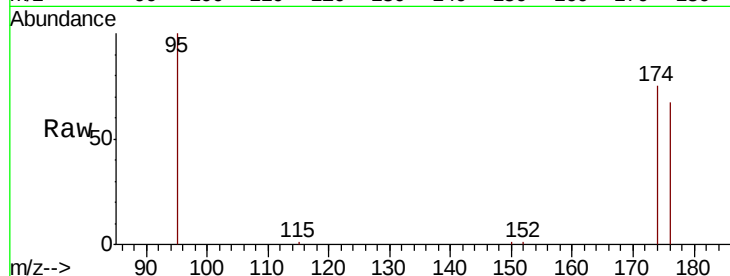

Abundance Ion 95.00 (94.70 to 95.70): VN056516.D (-1763) (-)

Ion 174.00 (173.70 to 174.70): VN056516.D (-1763) (-)

Ion 176.00 (175.70 to 176.70): VN056516.D (-1763) (-)

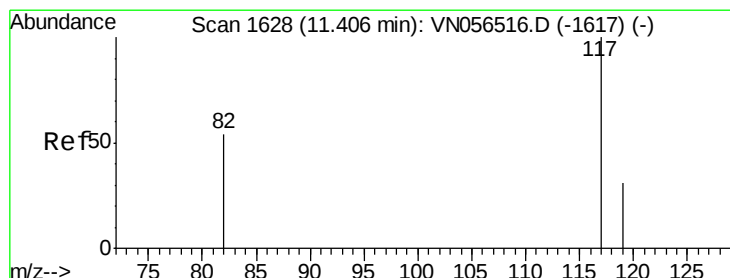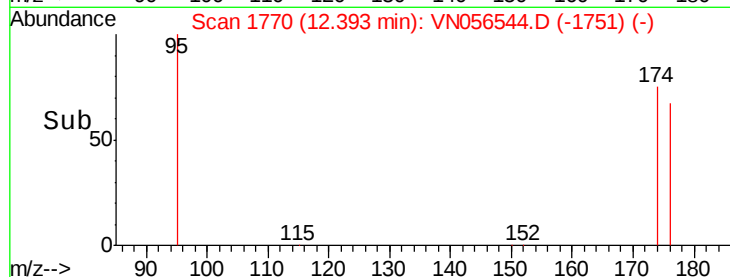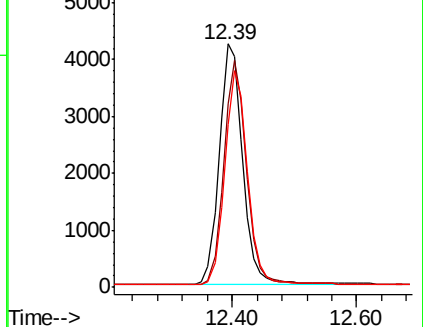

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.41 min Scan# 1626

Delta R.T. 0.00 min

Lab File: VN056544.D

Acq: 28 Jun 2019 10:34


Tgt Ion: 117 Resp: 54068

Ion Ratio Lower Upper

117 100

82 53.0 43.0 64.4



119 31.7 24.7 37.1



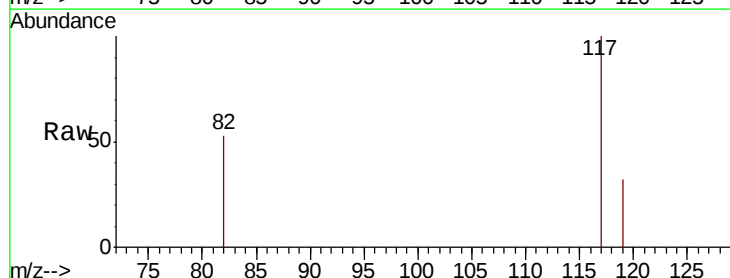


Abundance Ion 117.00 (116.70 to 117.70): VN056516.D (-1617) (-)

Ion 82.00 (81.70 to 82.70): VN056516.D (-1617) (-)

Ion 119.00 (118.70 to 119.70): VN056516.D (-1617) (-)

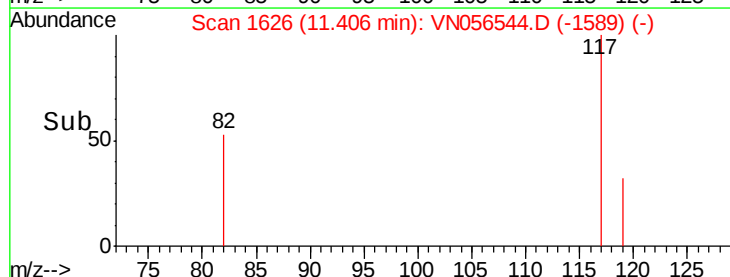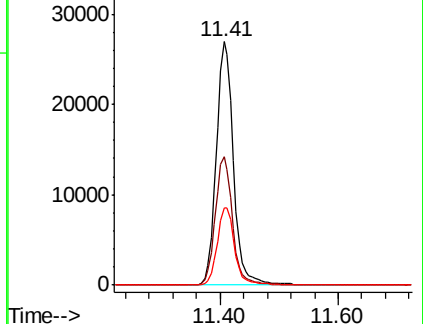

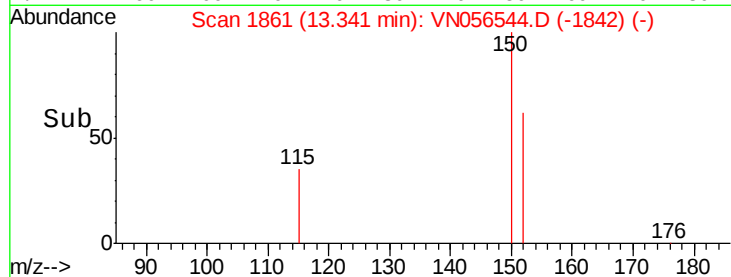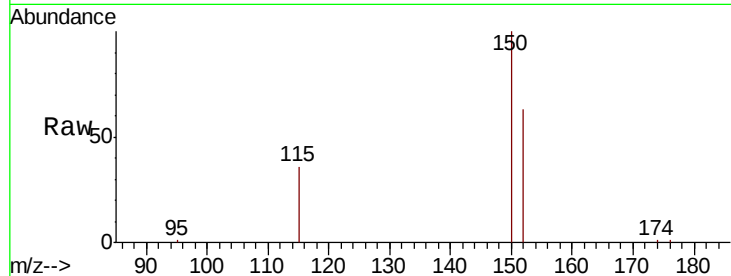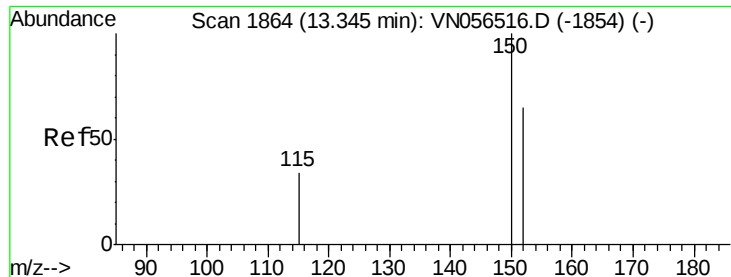

#9

1,4-Dichlorobenzene-d4

Concen: 5.000 ug/l

RT: 13.34 min Scan# 1861

Delta R.T. -0.00 min

Lab File: VN056544.D

Acq: 28 Jun 2019 10:34

Instrument :

MSVOA_N

ClientSampleId :

0.05ppb LOD

Tot Ion:152 Resp: 8327

Ion Ratio Lower Upper

152 100

115 56.9 27.0 80.8

150 159.7 0.0 306.6

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

