

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062821\
 Data File : VN067535.D
 Acq On : 28 Jun 2021 17:02
 Operator : JC/MD
 Sample : VN0628MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0628MBL01

Quant Time: Jun 29 05:24:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062821W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 28 14:31:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	243735	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	454066	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	415656	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	141438	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	172730	51.782	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 103.560%			
35) Dibromofluoromethane	8.024	113	136629	48.533	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 97.060%			
50) Toluene-d8	10.443	98	580667	50.775	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 101.560%			
62) 4-Bromofluorobenzene	12.734	95	186214	46.616	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 93.240%			
Target Compounds						Qvalue
3) Chloromethane	2.303	50	631	0.208	ug/l #	43
5) Bromomethane	2.880	94	1223	0.407	ug/l	91
13) Acrolein	4.052	56	302	3.139	ug/l #	14
16) Acetone	4.299	43	873	0.793	ug/l #	87
17) Carbon Disulfide	4.527	76	1572	0.236	ug/l #	74
20) Methylene Chloride	5.109	84	2094	0.522	ug/l #	65
29) Tetrahydrofuran	7.713	42	347	0.307	ug/l #	54
31) Cyclohexane	8.088	56	5929	Below Cal	#	4
36) 1,1-Dichloropropene	8.086	75	21525	5.251	ug/l #	53
38) Carbon Tetrachloride	8.088	117	27744	6.318	ug/l #	17
51) 4-Methyl-2-Pentanone	10.339	43	2059	0.531	ug/l #	82
53) t-1,3-Dichloropropene	10.719	75	226	2.297	ug/l #	43
59) 2-Hexanone	11.095	43	3584	1.309	ug/l	97
70) Styrene	12.294	104	721	1.949	ug/l	90
71) Bromoform	12.726	173	123	3.503	ug/l #	1
74) N-amyl acetate	12.390	43	1106	0.284	ug/l #	70
76) 1,2,3-Trichloropropane	12.734	75	97205	34.288	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.734	75	97205	98.579	ug/l #	6
82) 4-Chlorotoluene	13.109	91	2150	0.272	ug/l	83
86) p-Isopropyltoluene	13.619	119	2047	0.219	ug/l	86
87) 1,3-Dichlorobenzene	13.621	146	1568	0.321	ug/l	86
88) 1,4-Dichlorobenzene	13.621	146	1568	0.325	ug/l	87
89) n-Butylbenzene	13.946	91	3724	0.483	ug/l	99
91) 1,2-Dichlorobenzene	13.994	146	1506	0.324	ug/l	92
92) 1,2-Dibromo-3-Chloropr...	14.598	75	207	0.351	ug/l #	16
93) 1,2,4-Trichlorobenzene	15.268	180	2699	1.317	ug/l	97
94) Hexachlorobutadiene	15.370	225	254	0.281	ug/l #	68
95) Naphthalene	15.509	128	14511	5.131	ug/l	99
96) 1,2,3-Trichlorobenzene	15.700	180	2998	1.495	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062821\
Data File : VN067535.D
Acq On : 28 Jun 2021 17:02
Operator : JC/MD
Sample : VN0628MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01

Quant Time: Jun 29 05:24:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062821W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 28 14:31:03 2021
Response via : Initial Calibration




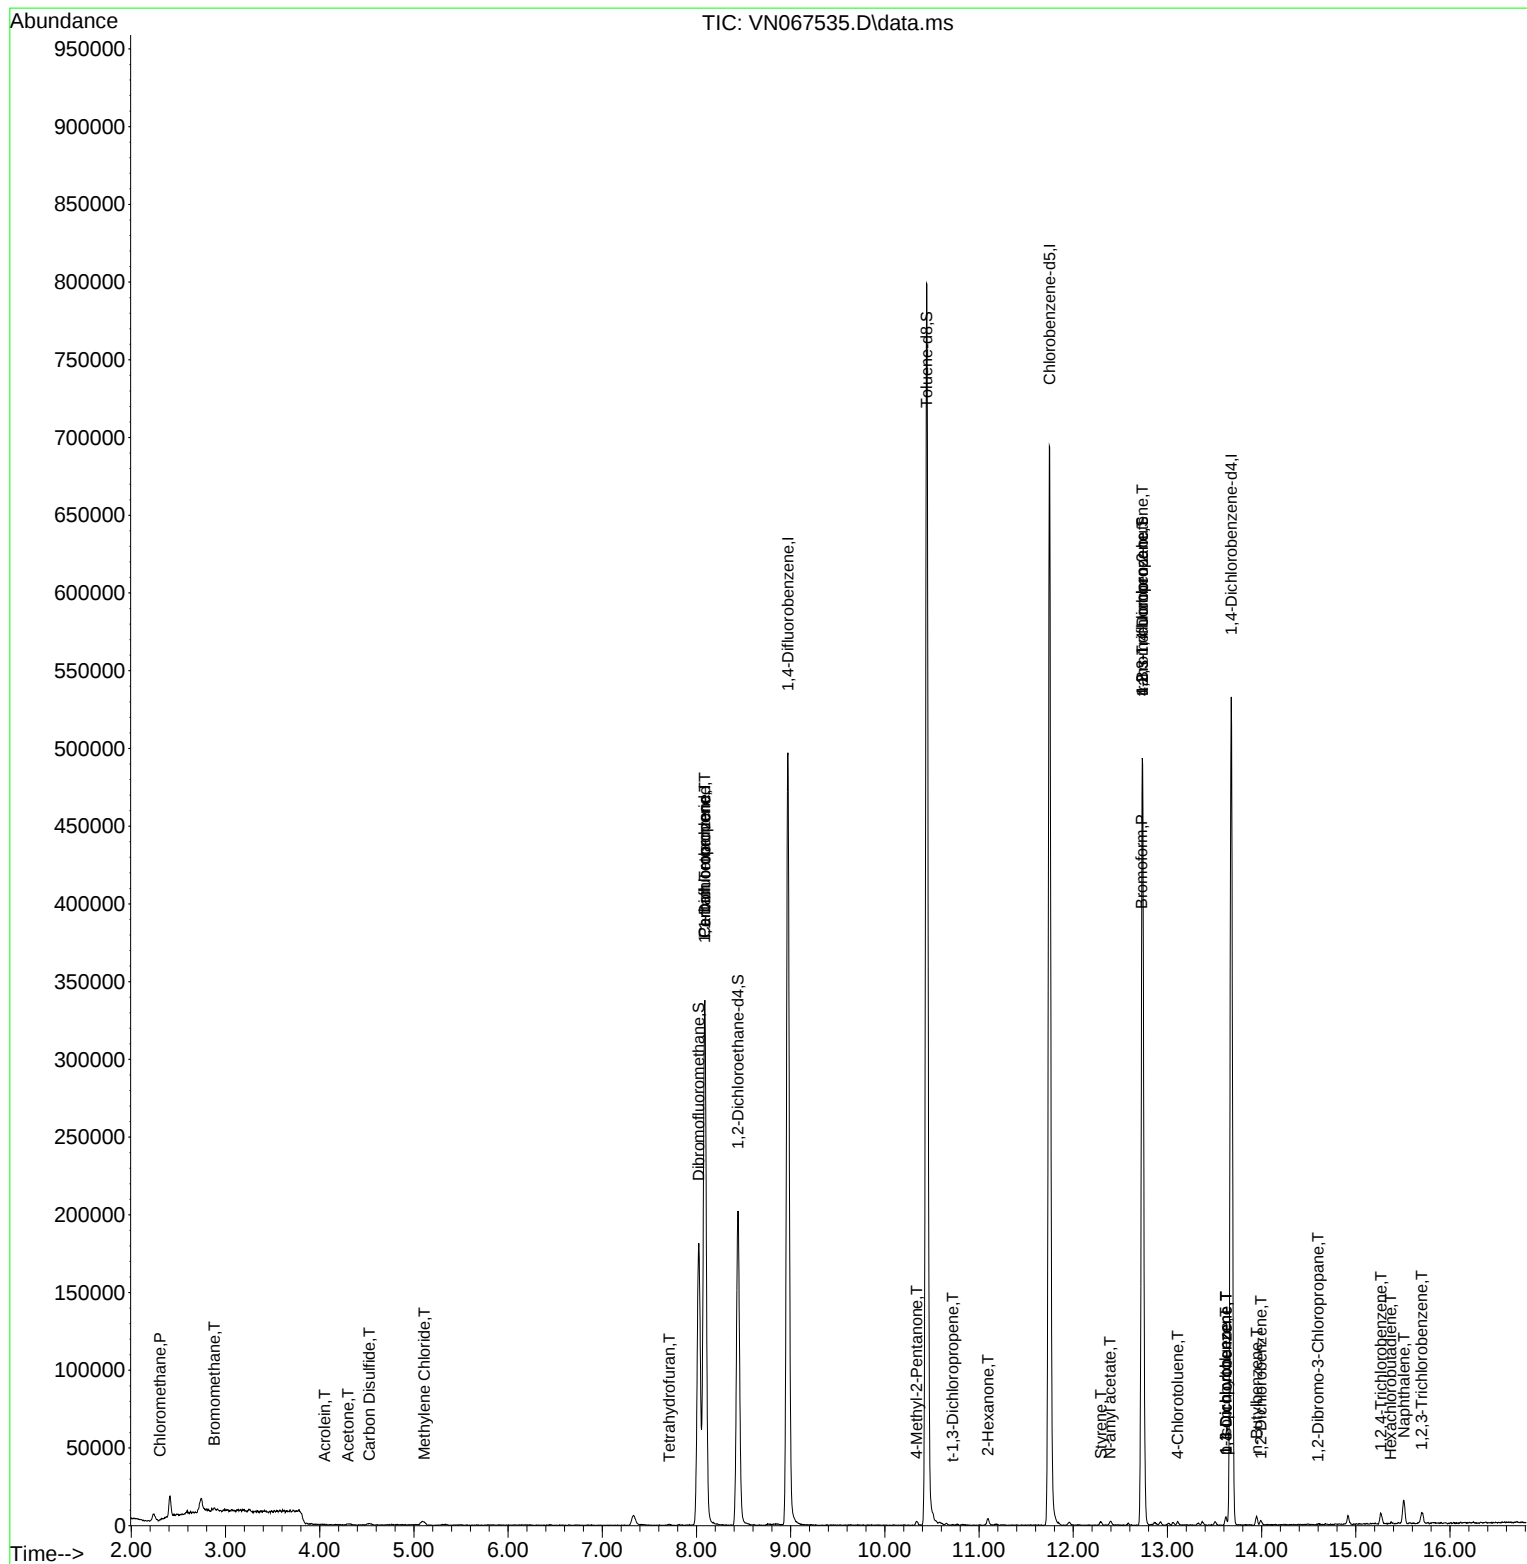




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion:168 Resp: 243735
Ion Ratio Lower Upper
168 100
99 67.5 62.9 94.3

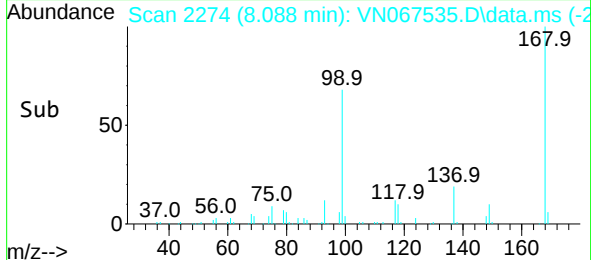

#3
Chloromethane
Concen: 0.208 ug/l
RT: 2.303 min Scan# 117
Delta R.T. 0.002 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 50 Resp: 631
Ion Ratio Lower Upper
50 100
52 0.0 25.6 38.4#


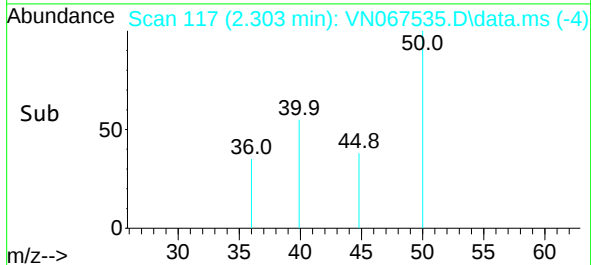

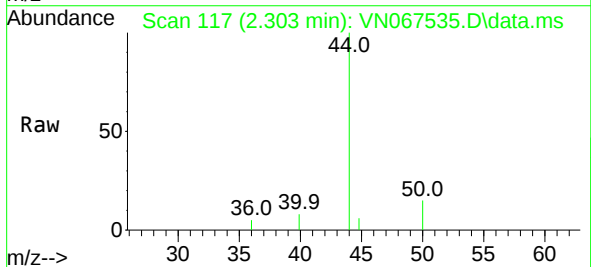


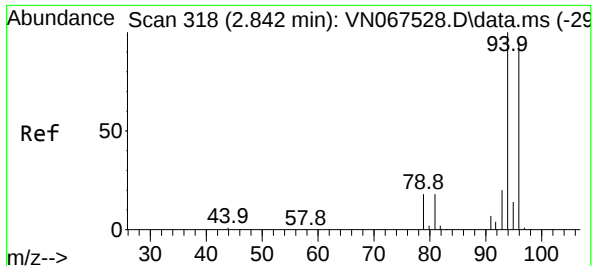

#5
Bromomethane
Concen: 0.407 ug/l
RT: 2.880 min Scan# 332
Delta R.T. 0.038 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 94 Resp: 1223
Ion Ratio Lower Upper
94 100
96 100.8 73.7 110.5

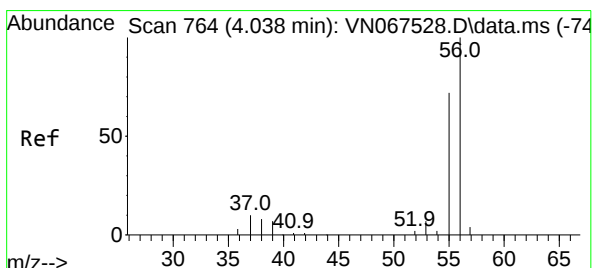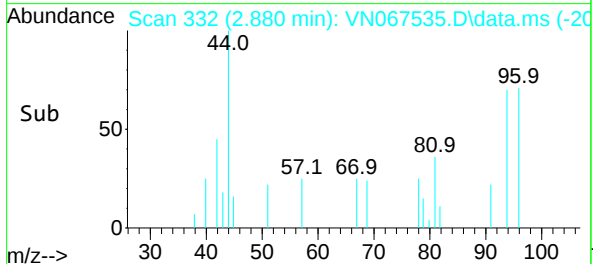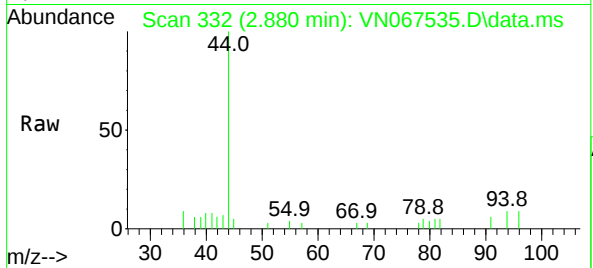

#13
Acrolein
Concen: 3.139 ug/l
RT: 4.052 min Scan# 769
Delta R.T. 0.014 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 56 Resp: 302
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.0#


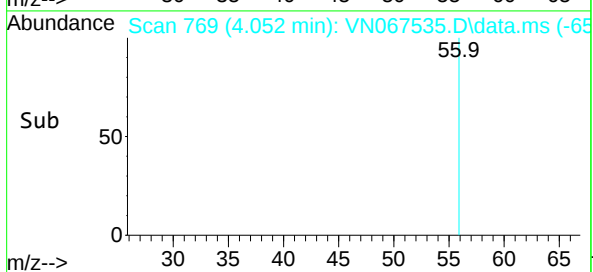

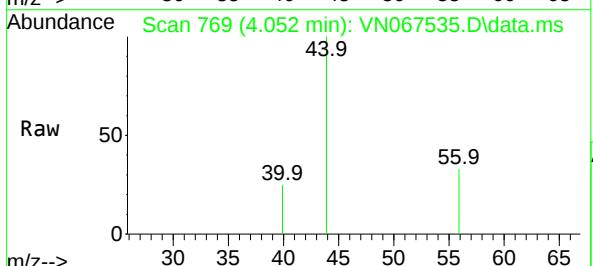


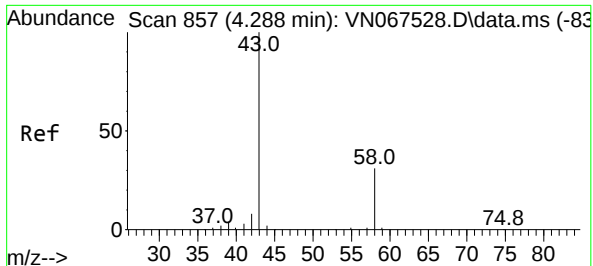

#16
Acetone
Concen: 0.793 ug/l
RT: 4.299 min Scan# 861
Delta R.T. 0.011 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 43 Resp: 873
Ion Ratio Lower Upper
43 100
58 33.3 21.2 31.8#

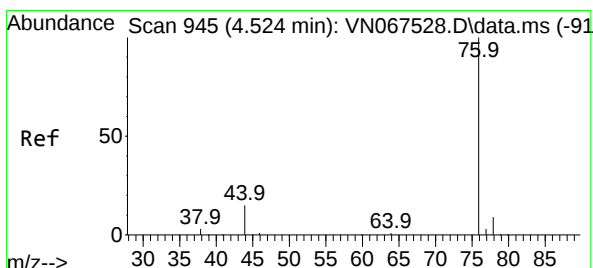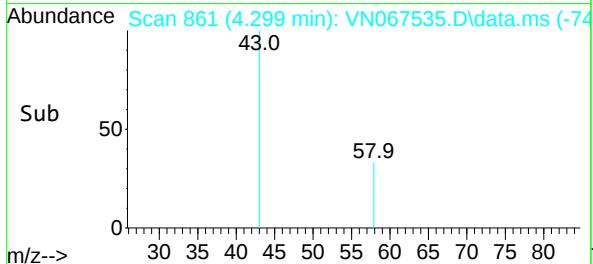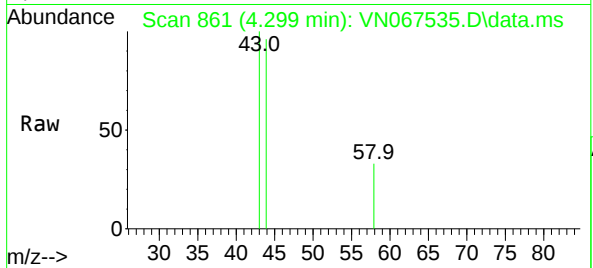

#17
Carbon Disulfide
Concen: 0.236 ug/l
RT: 4.527 min Scan# 946
Delta R.T. 0.003 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02


Tgt Ion: 76 Resp: 1572
Ion Ratio Lower Upper
76 100
78 0.0 7.7 11.5#

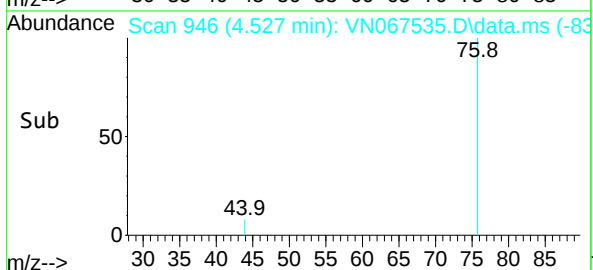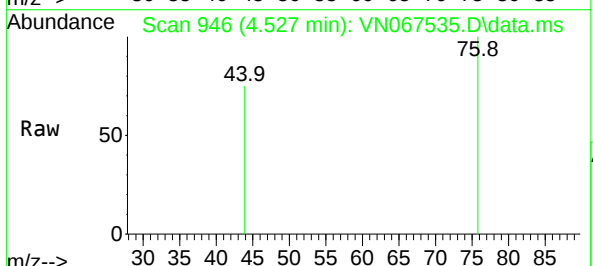

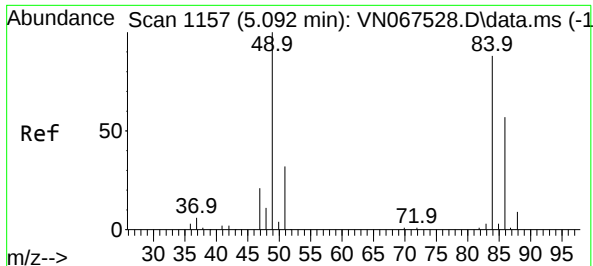




#20
Methylene Chloride
Concen: 0.522 ug/l
RT: 5.109 min Scan# 1163
Delta R.T. 0.017 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01

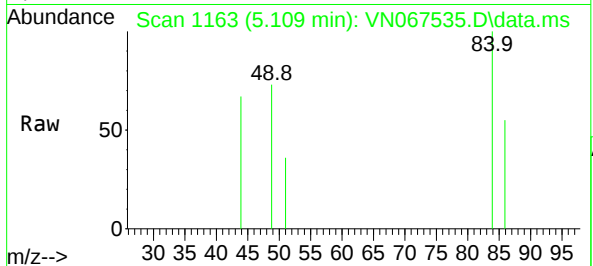


Tgt Ion: 84 Resp: 2094

Ion	Ratio	Lower	Upper
84	100		
49	73.4	110.9	166.3#
51	35.9	32.6	49.0
86	55.3	51.6	77.4

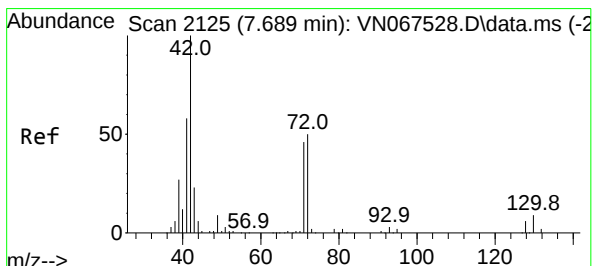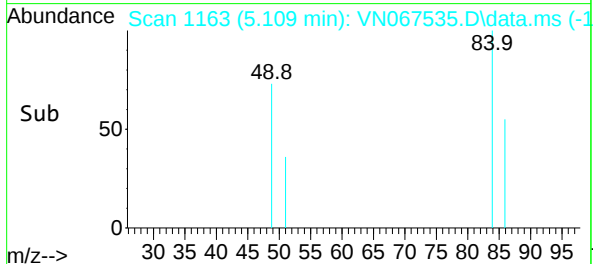




#29
Tetrahydrofuran
Concen: 0.307 ug/l
RT: 7.713 min Scan# 2134
Delta R.T. 0.024 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

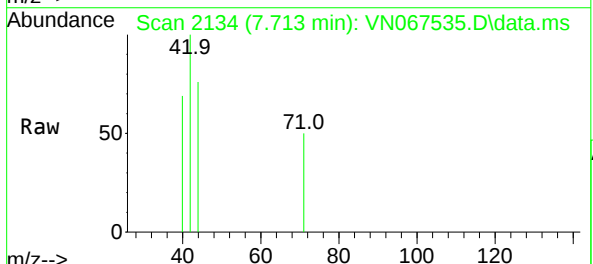

Tgt Ion: 42 Resp: 347

Ion	Ratio	Lower	Upper
42	100		
72	0.0	32.8	49.2#
71	23.3	31.2	46.8#



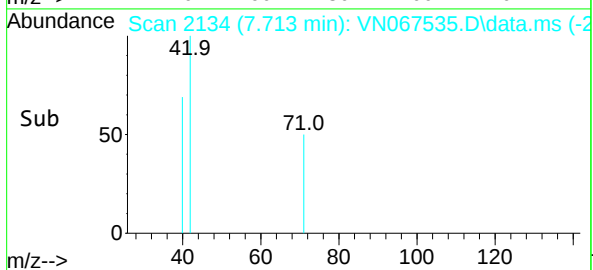





#31
Cyclohexane
Concen: Below Cal
RT: 8.088 min Scan# 2274
Delta R.T. -0.008 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 56 Resp: 5929
Ion Ratio Lower Upper
56 100
69 153.9 27.3 40.9#
84 124.9 64.9 97.3#

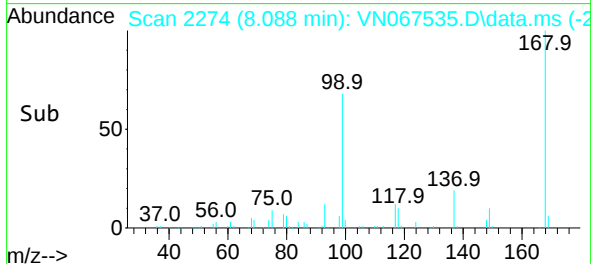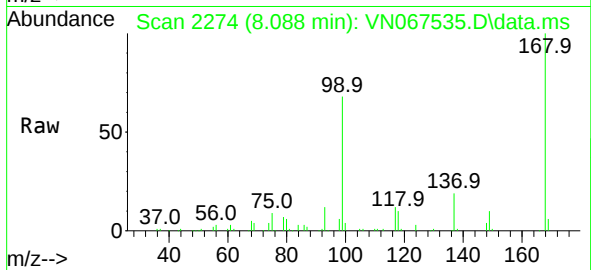

#33
1,2-Dichloroethane-d4
Concen: 51.782 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 65 Resp: 172730
Ion Ratio Lower Upper
65 100
67 51.6 0.0 98.6


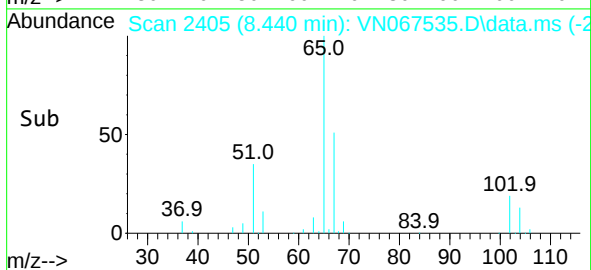

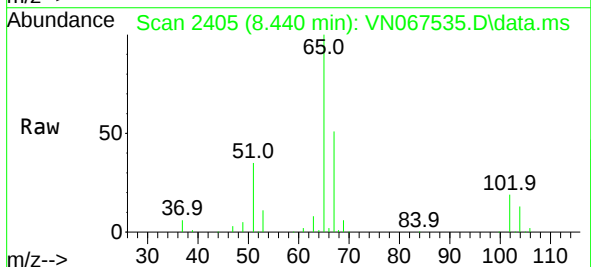




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion:114 Resp: 454066
Ion Ratio Lower Upper
114 100
63 20.3 0.0 49.0
88 15.6 0.0 36.6

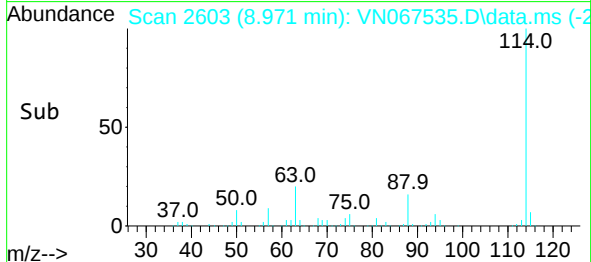

#35
Dibromofluoromethane
Concen: 48.533 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion:113 Resp: 136629
Ion Ratio Lower Upper
113 100
111 102.9 83.8 125.8
192 15.7 13.4 20.0


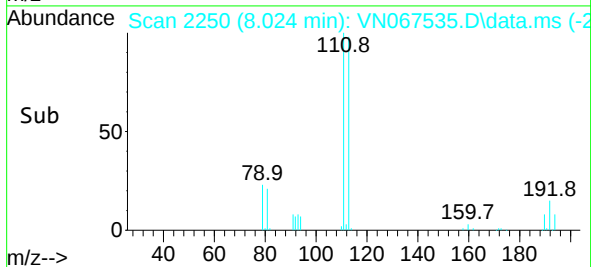

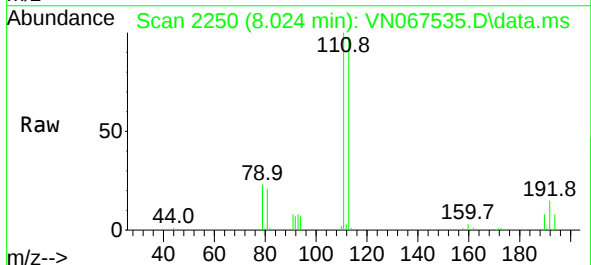




#36
1,1-Dichloropropene
Concen: 5.251 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 75 Resp: 21525
Ion Ratio Lower Upper
75 100
110 10.0 15.7 47.0#
77 0.0 24.6 37.0#

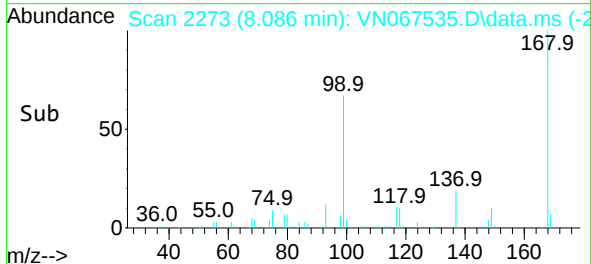

#38
Carbon Tetrachloride
Concen: 6.318 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 117 Resp: 27744
Ion Ratio Lower Upper
117 100
119 5.2 75.4 113.2#
121 0.0 23.5 35.3#


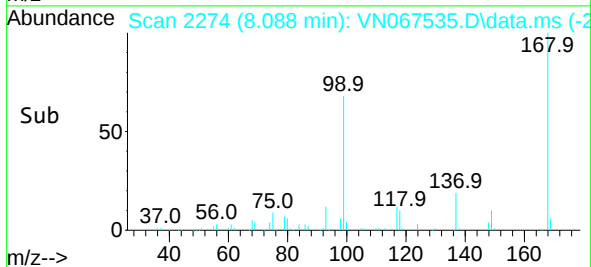

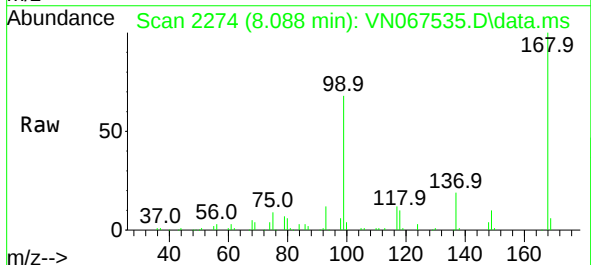




#50
Toluene-d8
Concen: 50.775 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 98 Resp: 580667
Ion Ratio Lower Upper
98 100
100 63.4 51.7 77.5

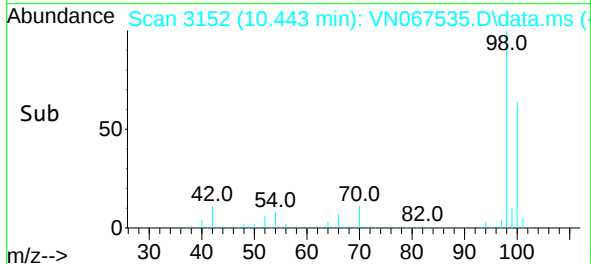

#51
4-Methyl-2-Pentanone
Concen: 0.531 ug/l
RT: 10.339 min Scan# 3113
Delta R.T. 0.006 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 43 Resp: 2059
Ion Ratio Lower Upper
43 100
58 25.0 28.6 43.0#


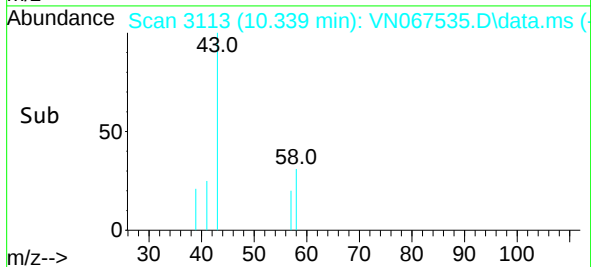

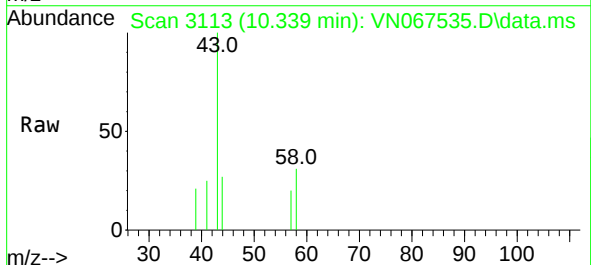




#53
t-1,3-Dichloropropene
Concen: 2.297 ug/l
RT: 10.719 min Scan# 3255
Delta R.T. -0.003 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 75 Resp: 226
Ion Ratio Lower Upper
75 100
77 0.0 25.1 37.7#

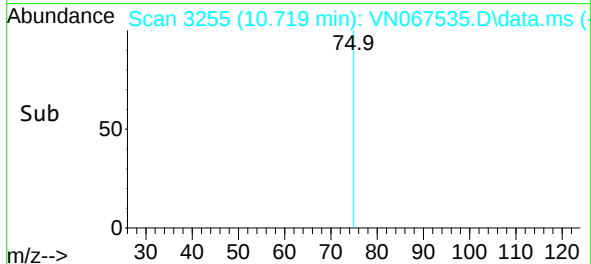

#59
2-Hexanone
Concen: 1.309 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.006 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 43 Resp: 3584
Ion Ratio Lower Upper
43 100
58 51.3 24.7 74.1




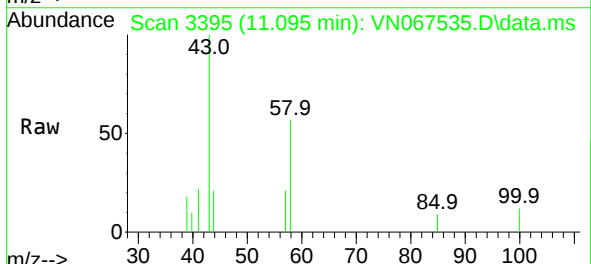




#62
4-Bromofluorobenzene
Concen: 46.616 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 95 Resp: 186214
Ion Ratio Lower Upper
95 100
174 69.8 0.0 122.0
176 65.9 0.0 117.6

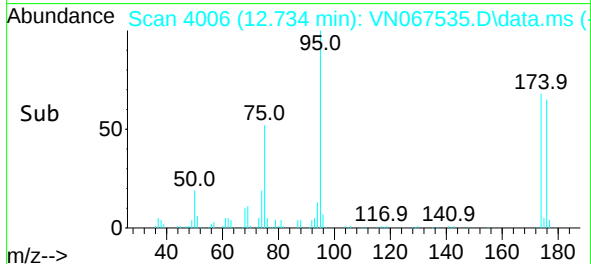

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 117 Resp: 415656
Ion Ratio Lower Upper
117 100
82 57.2 53.1 79.7
119 31.9 25.5 38.3

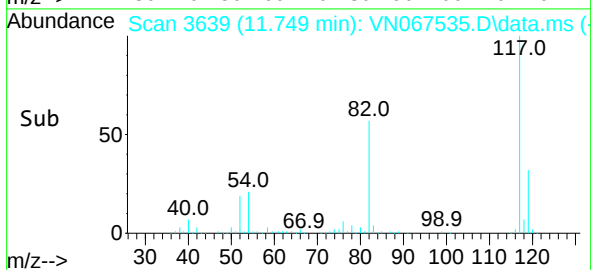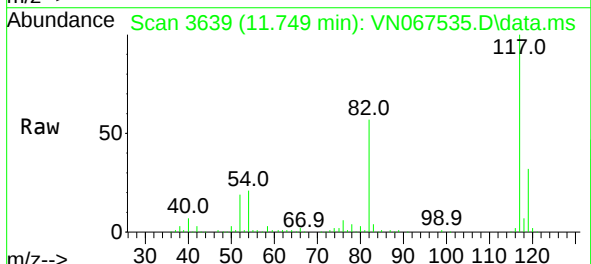



#70

Styrene

Concen: 1.949 ug/l

RT: 12.294 min Scan# 3842





Delta R.T. -0.002 min

Lab File: VN067535.D

Acq: 28 Jun 2021 17:02

Tgt Ion:	104	Resp:	721
Ion	Ratio	Lower	Upper
104	100		
78	52.4	48.2	72.2
103	62.7	44.5	66.7

Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01



#71

Bromoform

Concen: 3.503 ug/l




RT: 12.726 min Scan# 4003


Delta R.T. 0.266 min

Lab File: VN067535.D

Acq: 28 Jun 2021 17:02

Tgt Ion:	173	Resp:	123
Ion	Ratio	Lower	Upper
173	100		
175	7398.4	23.9	71.8#
254	0.0	0.0	0.0


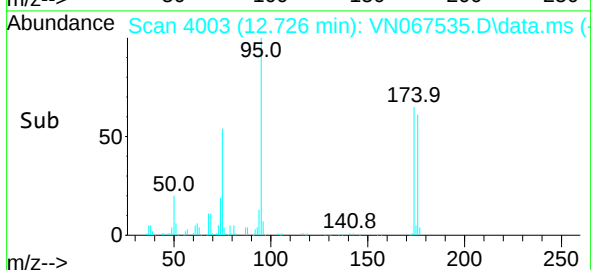

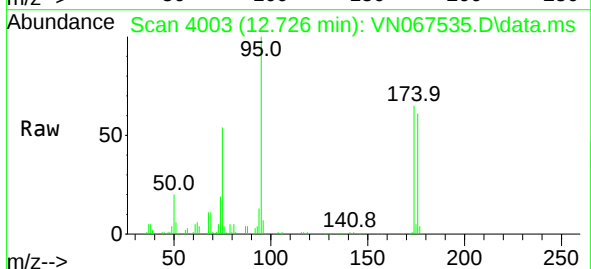


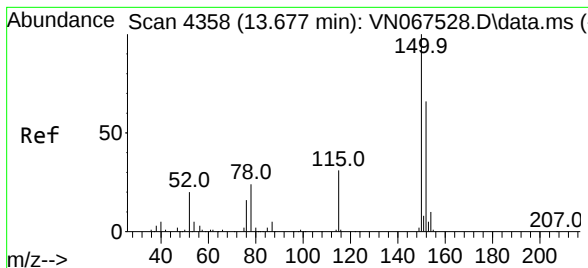

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.001 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion:152 Resp: 141438
Ion Ratio Lower Upper
152 100
115 65.0 36.1 108.5
150 160.3 0.0 351.8

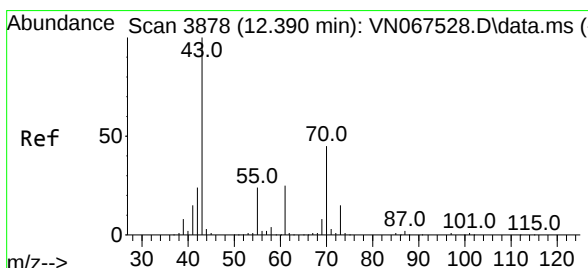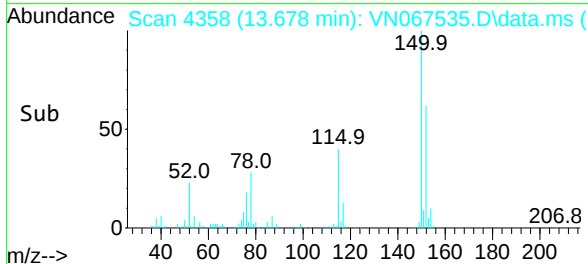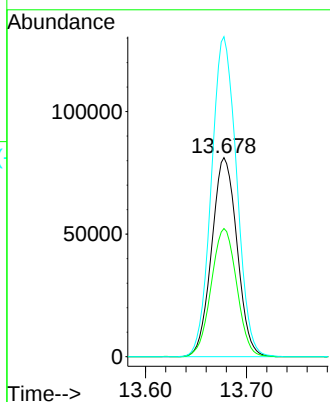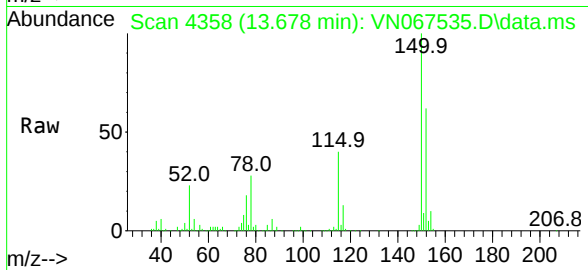

#74
N-ethyl acetate
Concen: 0.284 ug/l
RT: 12.390 min Scan# 3878
Delta R.T. 0.000 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 43 Resp: 1106
Ion Ratio Lower Upper
43 100
70 54.8 29.4 44.2#
55 34.2 17.0 25.4#
61 36.8 17.6 26.4#


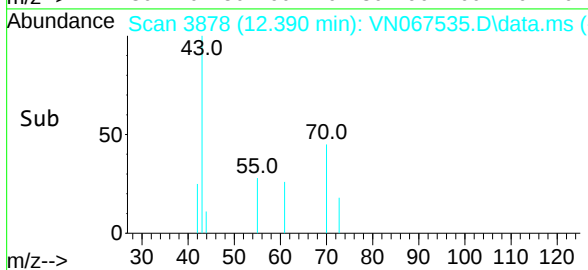
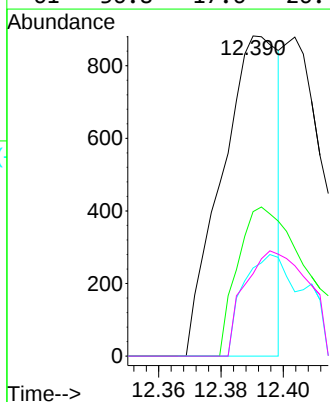
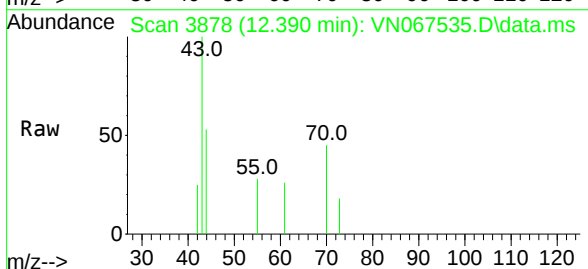




#76
1,2,3-Trichloropropane
Concen: 34.288 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 75 Resp: 97205
Ion Ratio Lower Upper
75 100
77 0.9 0.0 0.0#

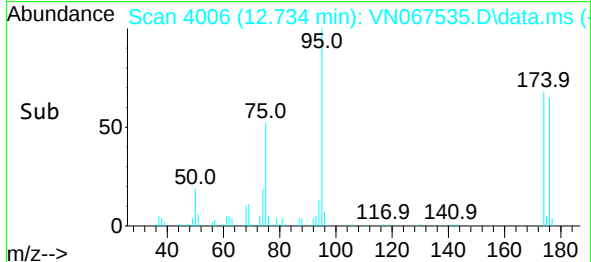

#81
trans-1,4-Dichloro-2-butene
Concen: 98.579 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.108 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 75 Resp: 97205
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#


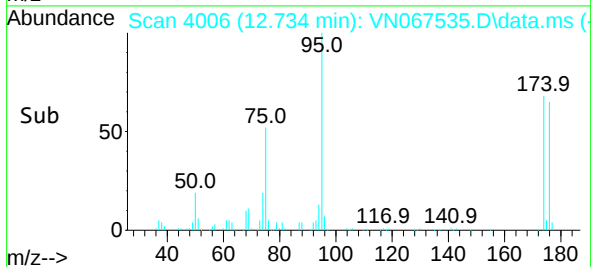

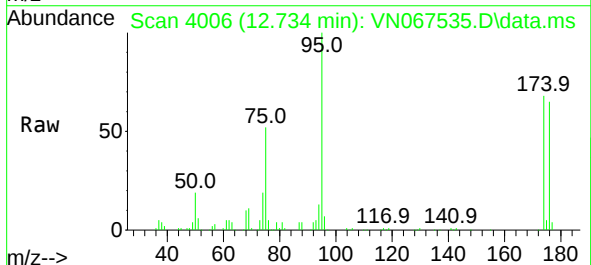


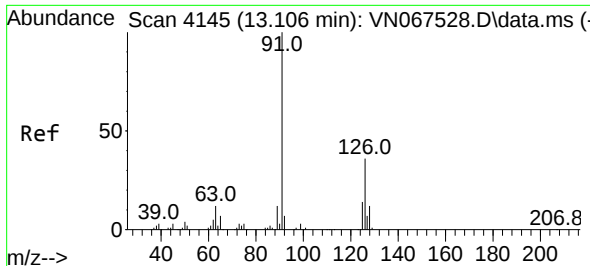

#82
4-Chlorotoluene
Concen: 0.272 ug/l
RT: 13.109 min Scan# 4146
Delta R.T. 0.003 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 91 Resp: 2150
Ion Ratio Lower Upper
91 100
126 20.6 14.8 44.4

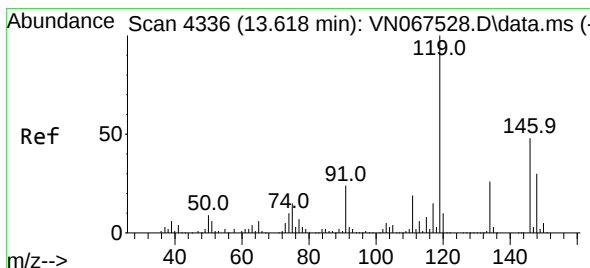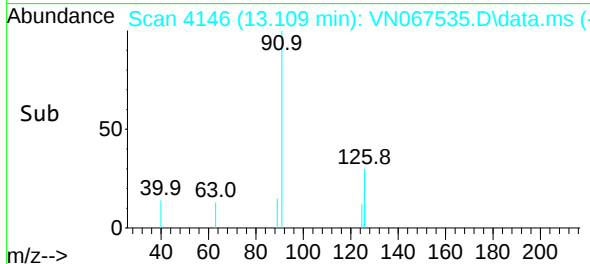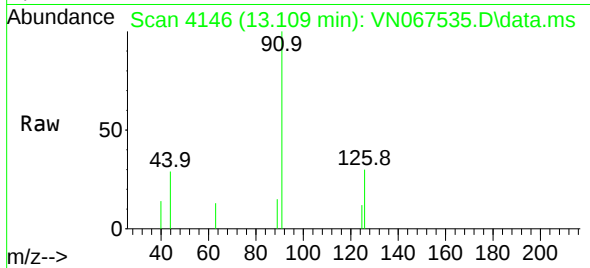

#86
p-Isopropyltoluene
Concen: 0.219 ug/l
RT: 13.619 min Scan# 4336
Delta R.T. 0.001 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 119 Resp: 2047
Ion Ratio Lower Upper
119 100
134 24.2 12.4 37.4
91 15.9 14.8 44.3

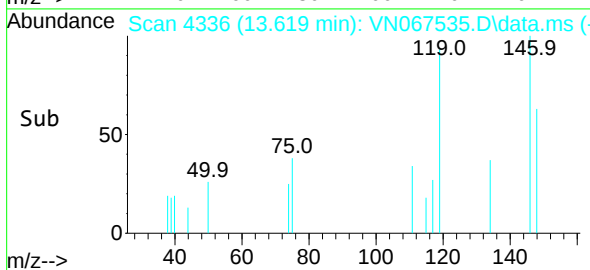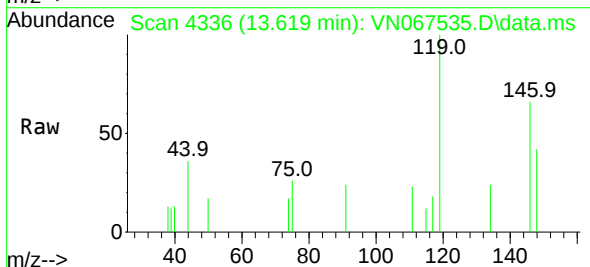







#87

1,3-Dichlorobenzene
Concen: 0.321 ug/l
RT: 13.621 min Scan# 4337
Delta R.T. 0.003 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01




Tgt Ion:146 Resp: 1568
Ion Ratio Lower Upper
146 100
111 32.7 24.3 72.8
148 58.7 32.0 96.0

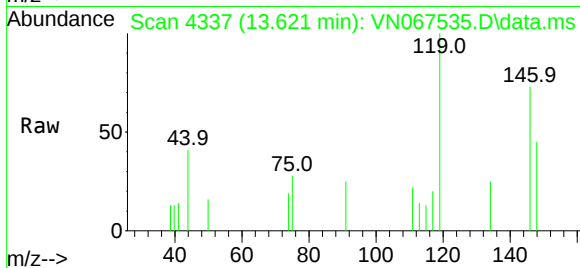


#88

1,4-Dichlorobenzene
Concen: 0.325 ug/l
RT: 13.621 min Scan# 4337
Delta R.T. -0.075 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion:146 Resp: 1568
Ion Ratio Lower Upper
146 100
111 32.7 23.4 70.2
148 58.7 31.8 95.3


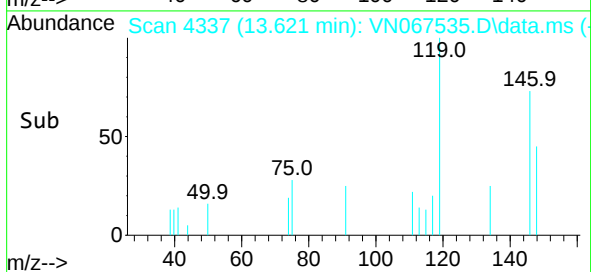

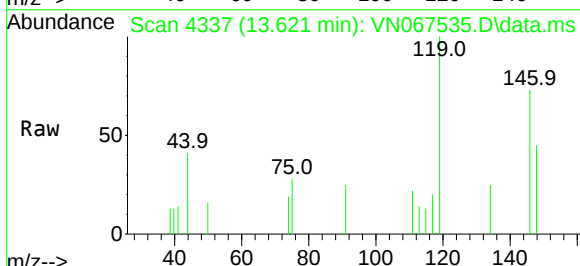


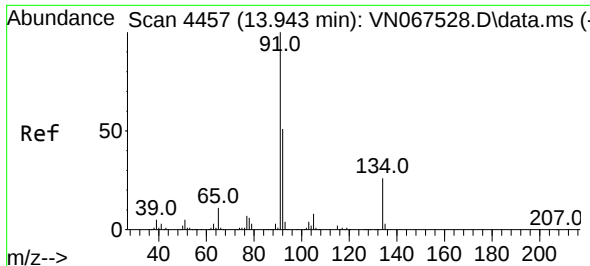

#89
n-Butylbenzene
Concen: 0.483 ug/l
RT: 13.946 min Scan# 4458
Delta R.T. 0.003 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion: 91 Resp: 3724
Ion Ratio Lower Upper
91 100
92 51.6 25.7 77.1
134 23.3 11.2 33.6

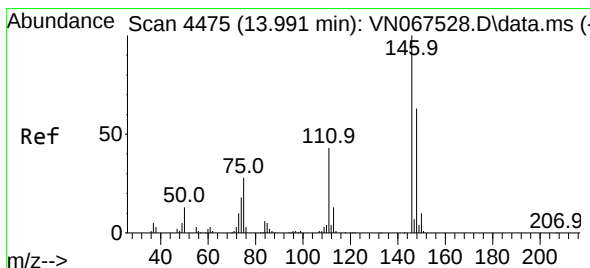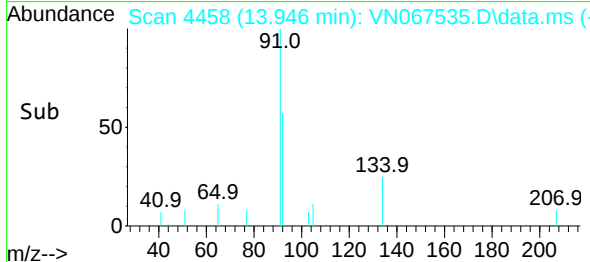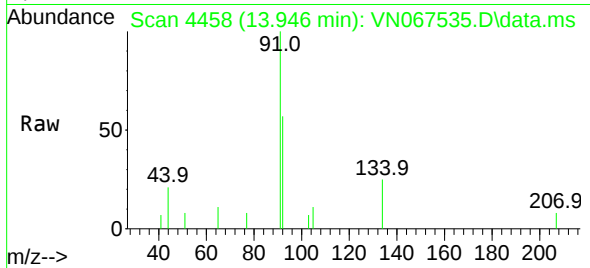

#91
1,2-Dichlorobenzene
Concen: 0.324 ug/l
RT: 13.994 min Scan# 4476
Delta R.T. 0.003 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion: 146 Resp: 1506
Ion Ratio Lower Upper
146 100
111 43.2 24.9 74.6
148 58.4 31.6 95.0

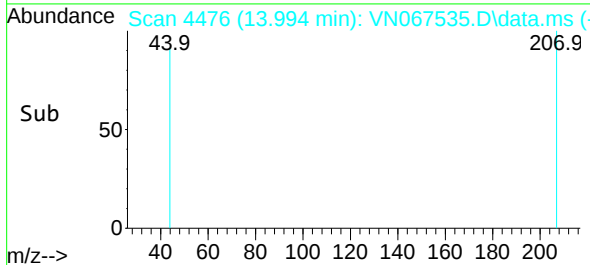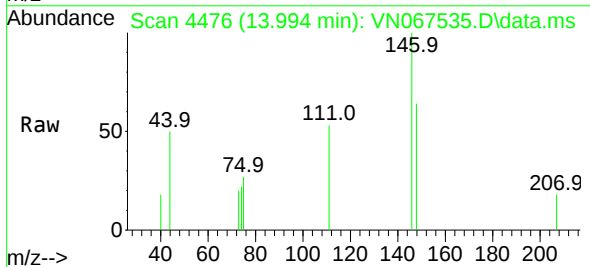



#92

1,2-Dibromo-3-Chloropropane

Concen: 0.351 ug/l

RT: 14.598 min Scan# 4701

Delta R.T. -0.007 min

Lab File: VN067535.D

Acq: 28 Jun 2021 17:02





Instrument :

MSVOA_N

ClientSampleId :

VN0628MBL01

Tgt Ion:	75	Resp:	207
Ion	Ratio	Lower	Upper
75	100		
155	0.0	29.8	89.5#
157	0.0	37.6	112.8#

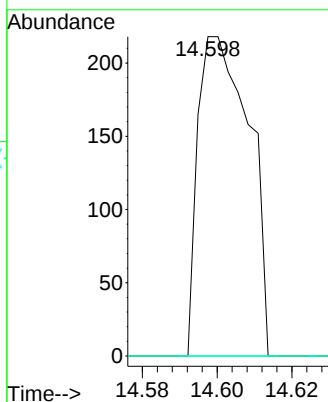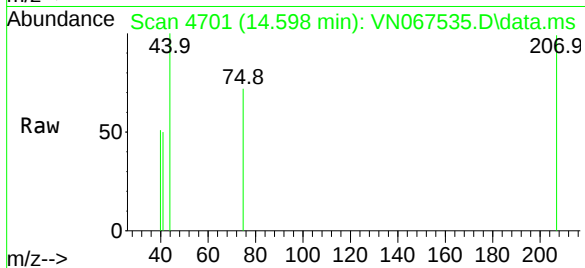

#93

1,2,4-Trichlorobenzene

Concen: 1.317 ug/l




RT: 15.268 min Scan# 4951


Delta R.T. 0.003 min

Lab File: VN067535.D

Acq: 28 Jun 2021 17:02

Tgt Ion:	180	Resp:	2699
Ion	Ratio	Lower	Upper
180	100		
182	95.0	47.5	142.5
145	28.0	17.2	51.6


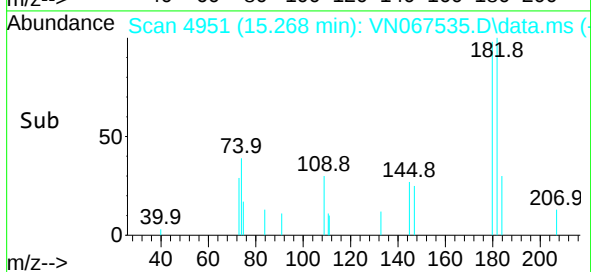
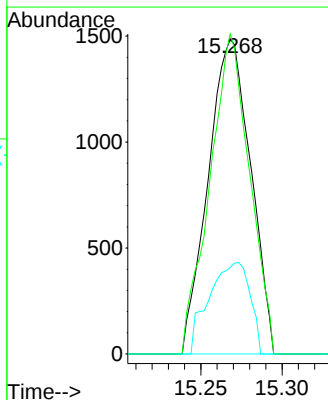
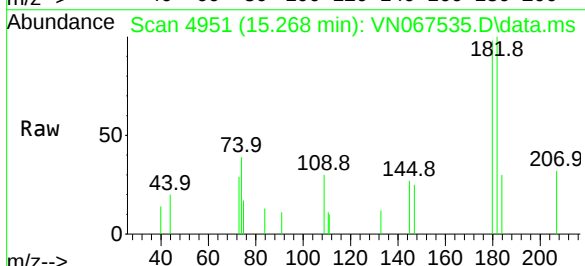


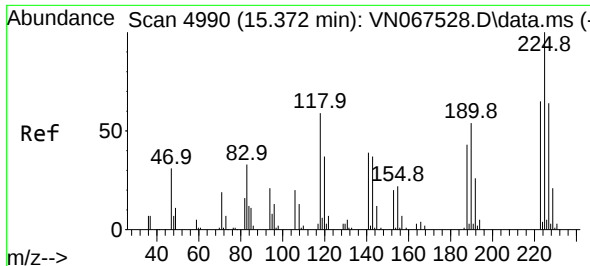

#94
Hexachlorobutadiene
Concen: 0.281 ug/l
RT: 15.370 min Scan# 4989
Delta R.T. -0.002 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02




Instrument :
MSVOA_N
ClientSampleId :
VN0628MBL01


Tgt Ion:225 Resp: 254
Ion Ratio Lower Upper
225 100
223 45.3 31.4 94.0
227 29.9 31.2 93.6#

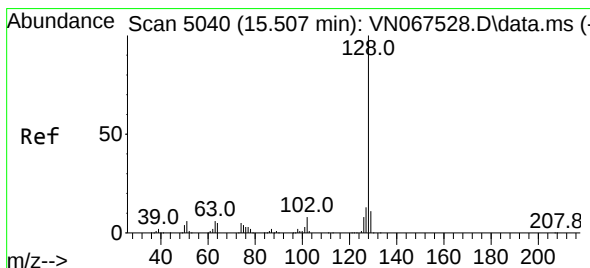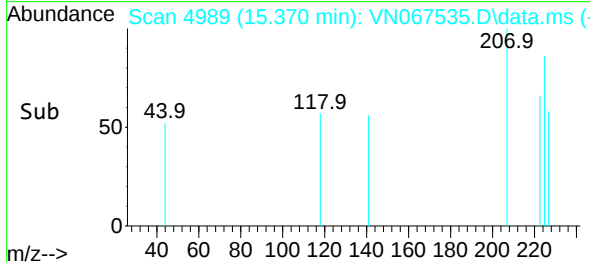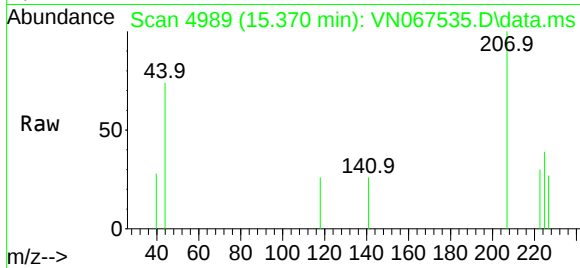

#95
Naphthalene
Concen: 5.131 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN067535.D
Acq: 28 Jun 2021 17:02

Tgt Ion:128 Resp: 14511
Ion Ratio Lower Upper
128 100
127 13.4 10.6 15.8
129 9.9 8.6 12.8

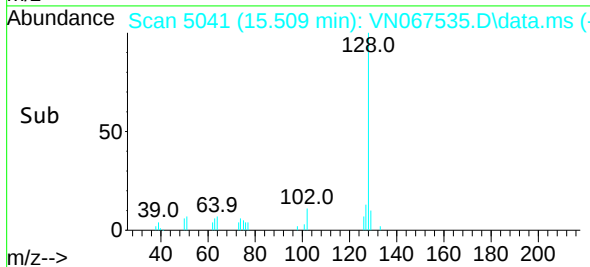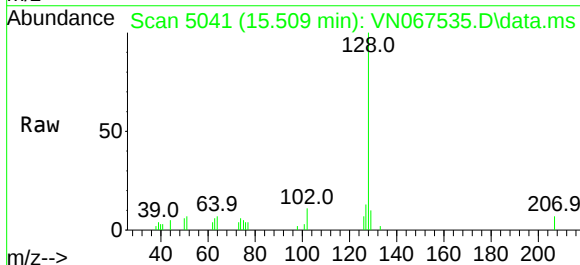

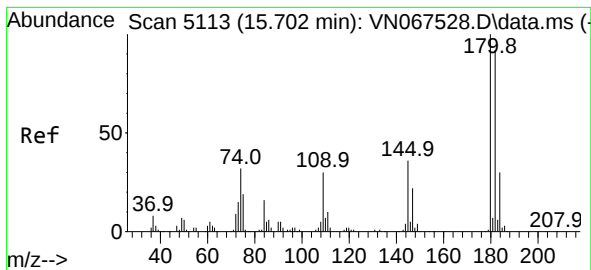

#96
 1,2,3-Trichlorobenzene
 Concen: 1.495 ug/l
 RT: 15.700 min Scan# 5112
 Delta R.T. -0.002 min
 Lab File: VN067535.D
 Acq: 28 Jun 2021 17:02

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0628MBL01

Tgt Ion:180 Resp: 2998

Ion	Ratio	Lower	Upper
180	100		
182	100.5	47.8	143.3
145	37.7	18.2	54.6

