
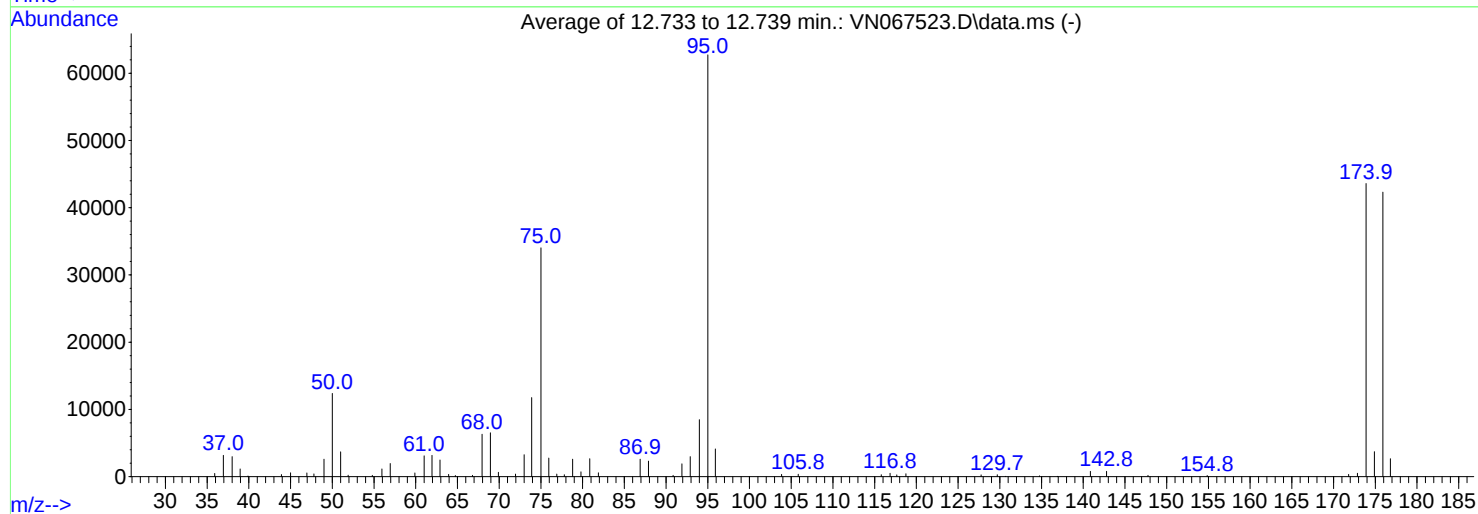


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062821\
Data File : VN067523.D
Acq On : 28 Jun 2021 9:39
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062821W.M
Title : SW846 8260
Last Update : Mon Jun 28 14:31:03 2021

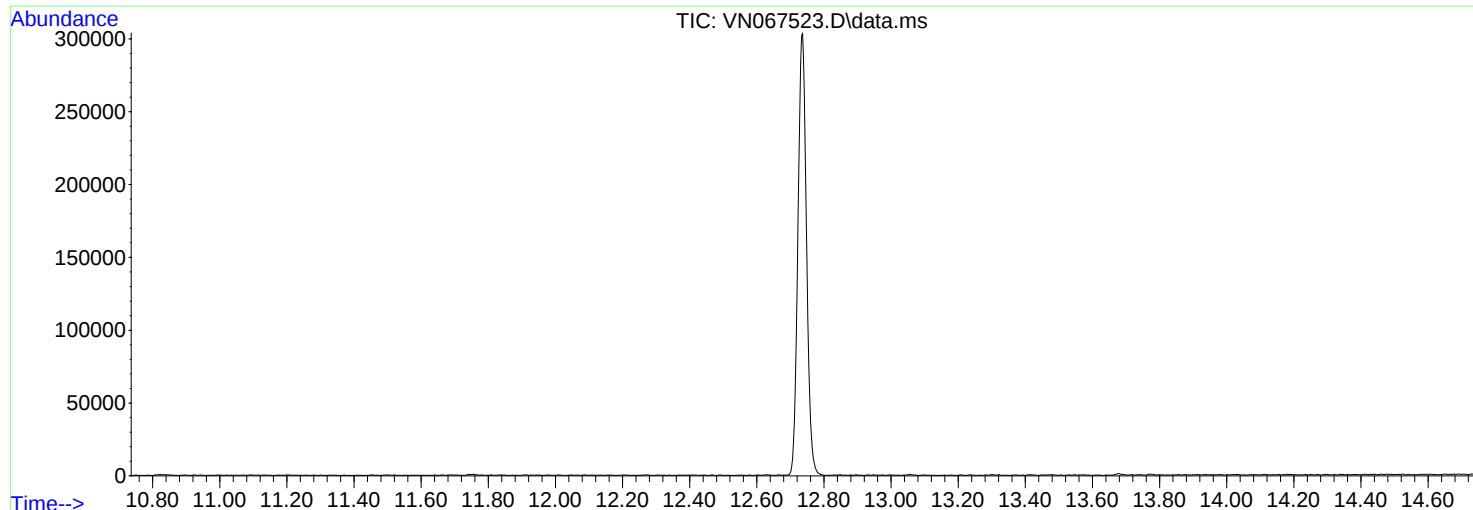

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3989

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	12373	PASS
75	95	30	60	54.3	34035	PASS
95	95	100	100	100.0	62736	PASS
96	95	5	9	6.6	4127	PASS
173	174	0.00	2	1.2	505	PASS
174	95	50	100	69.5	43592	PASS
175	174	5	9	8.5	3711	PASS
176	174	95	101	97.1	42315	PASS
177	176	5	9	6.3	2659	PASS