

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062822\
 Data File : VN073225.D
 Acq On : 29 Jun 2022 02:42
 Operator : JC\MD
 Sample : N3376-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-3

Quant Time: Jun 29 04:28:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	312763	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	520554	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	489044	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	251021	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	195785	43.362	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	86.720%		
35) Dibromofluoromethane	7.951	113	167386	48.331	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.660%		
50) Toluene-d8	10.374	98	548180	44.566	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	89.140%		
62) 4-Bromofluorobenzene	12.668	95	251308	53.164	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	106.320%		
Target Compounds						
					Qvalue	
6) Chloroethane	2.946	64	560	0.252	ug/l #	42
11) Tert butyl alcohol	5.228	59	473	0.432	ug/l #	72
16) Acetone	4.245	43	2155	0.850	ug/l #	76
25) 2-Butanone	7.245	43	1608	0.399	ug/l #	45
31) Cyclohexane	8.016	56	10576	1.430	ug/l #	49
36) 1,1-Dichloropropene	8.010	75	25999	4.879	ug/l #	48
38) Carbon Tetrachloride	8.016	117	31385	5.695	ug/l #	15
39) Methylcyclohexane	9.386	83	3106	0.468	ug/l	89
52) Toluene	10.439	92	101534	9.990	ug/l	97
67) Ethyl Benzene	11.780	91	1080592	53.815	ug/l	100
68) m/p-Xylenes	11.886	106	1861452	245.636	ug/l	95
69) o-Xylene	12.216	106	917022	118.537	ug/l	96
70) Styrene	12.216	104	47062	3.940	ug/l #	1
71) Bromoform	12.668	173	2202	0.740	ug/l #	1
73) Isopropylbenzene	12.515	105	72994	3.367	ug/l	98
74) N-amyl acetate	12.221	43	2409	0.222	ug/l #	1
76) 1,2,3-Trichloropropane	12.915	75	5753	0.876	ug/l #	1
78) n-propylbenzene	12.857	91	115063	4.778	ug/l	96
79) 2-Chlorotoluene	12.921	91	59143	3.881	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.998	105	184157	10.423	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.668	75	134822	56.332	ug/l #	10
82) 4-Chlorotoluene	12.992	91	20849	1.413	ug/l #	40
83) tert-Butylbenzene	13.304	119	81241	5.129	ug/l #	54
84) 1,2,4-Trimethylbenzene	13.304	105	724224	41.056	ug/l	97
85) sec-Butylbenzene	13.304	105	724224	34.050	ug/l #	56
86) p-Isopropyltoluene	13.498	119	8306	0.483	ug/l	90
89) n-Butylbenzene	13.880	91	4752	0.332	ug/l #	61
90) Hexachloroethane	14.151	117	3957	1.236	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	14.521	75	435	0.249	ug/l #	1
95) Naphthalene	15.433	128	172466	8.915	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062822\
Data File : VN073225.D
Acq On : 29 Jun 2022 02:42
Operator : JC\MD
Sample : N3376-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-3

Quant Time: Jun 29 04:28:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




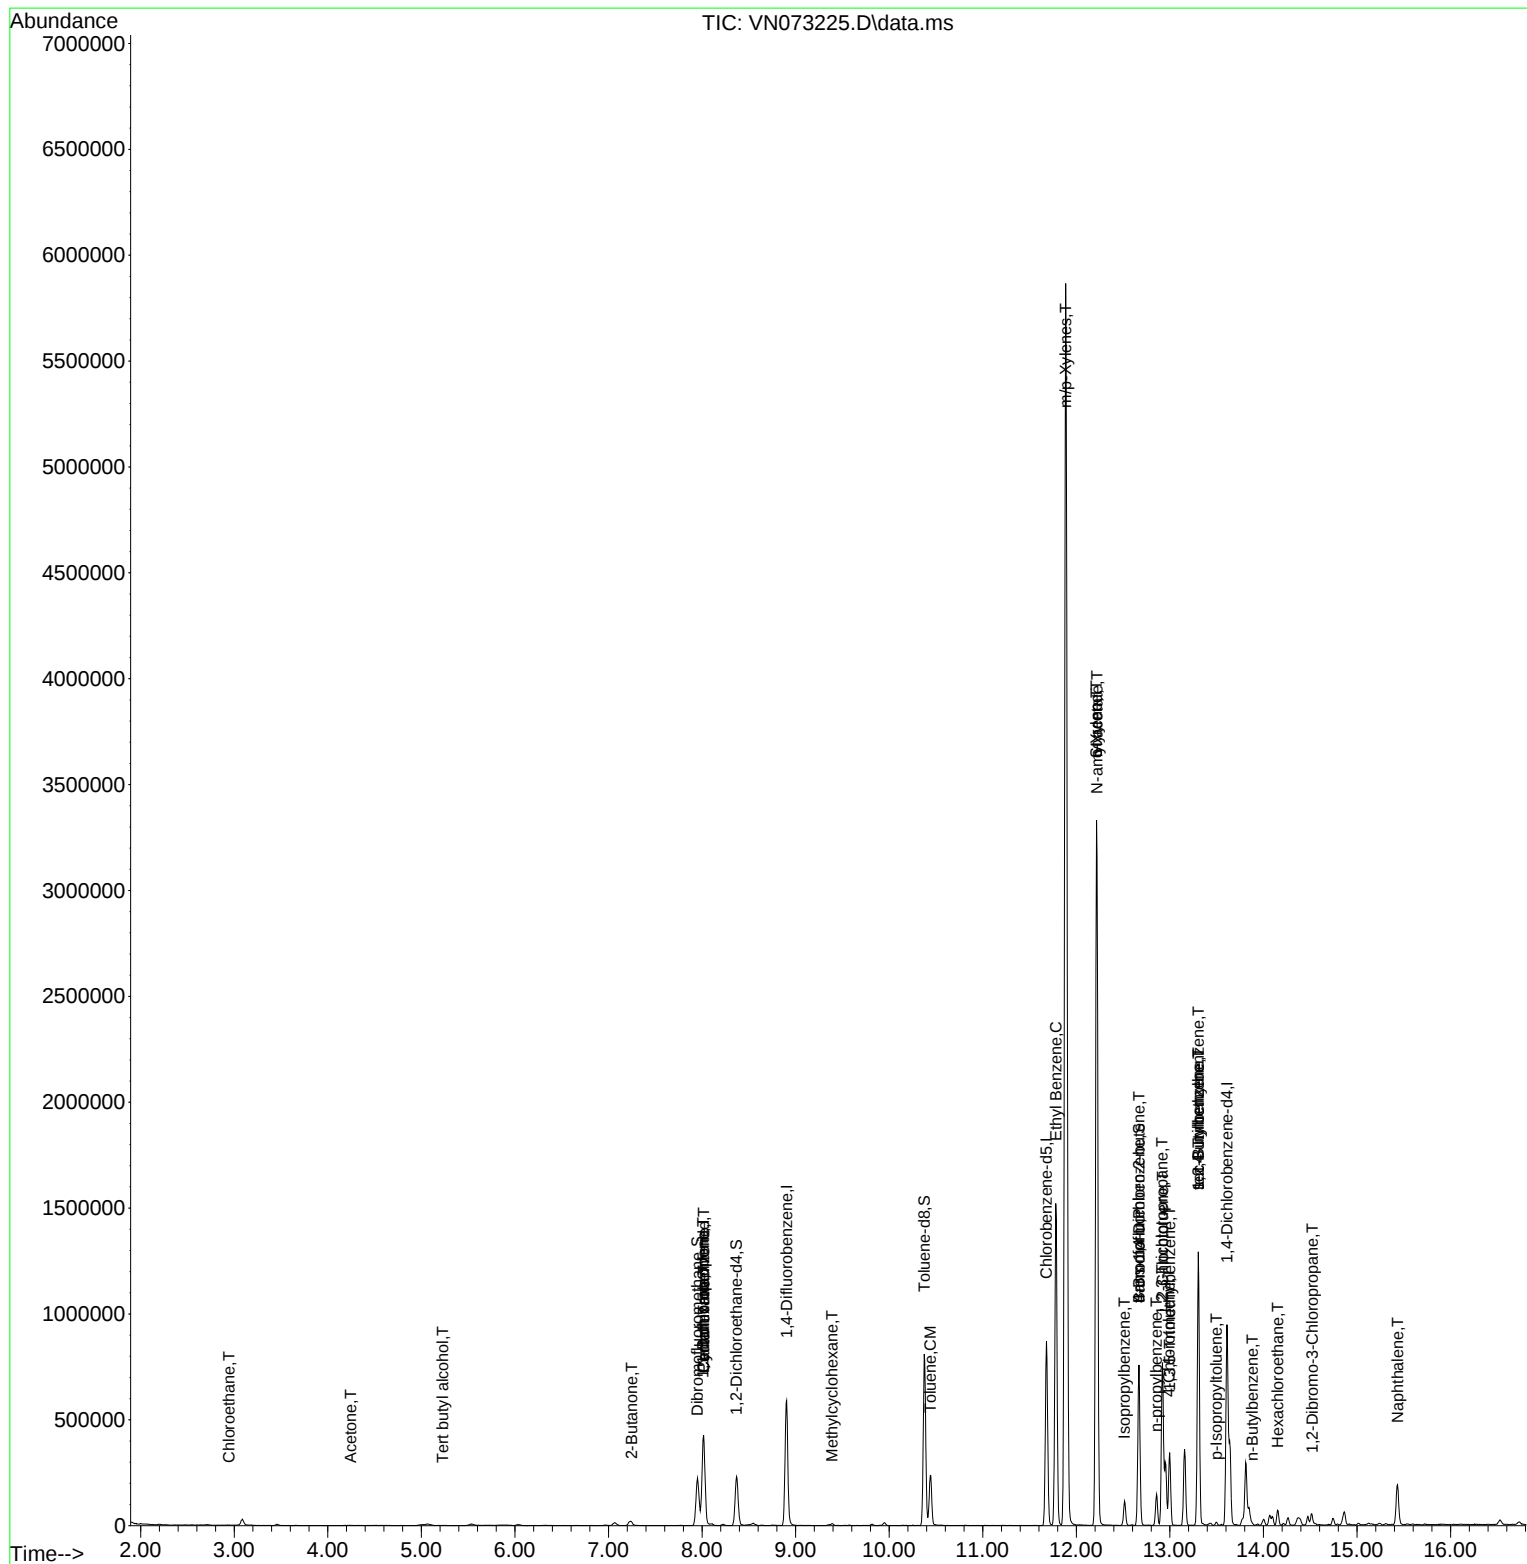


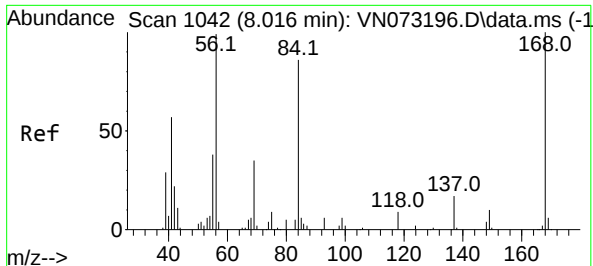

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion:168 Resp: 312763
Ion Ratio Lower Upper
168 100
99 59.2 42.3 63.5

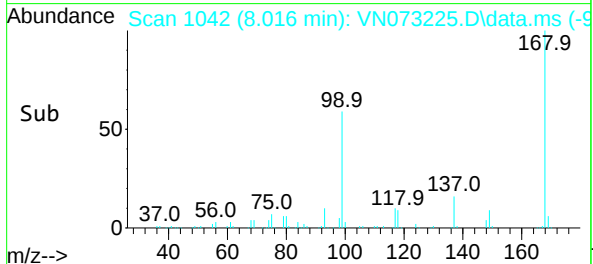

#6
Chloroethane
Concen: 0.252 ug/l
RT: 2.946 min Scan# 180
Delta R.T. -0.017 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 64 Resp: 560
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#




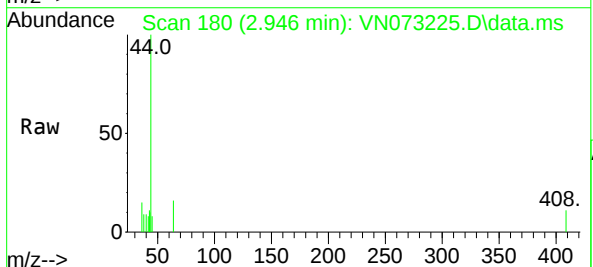


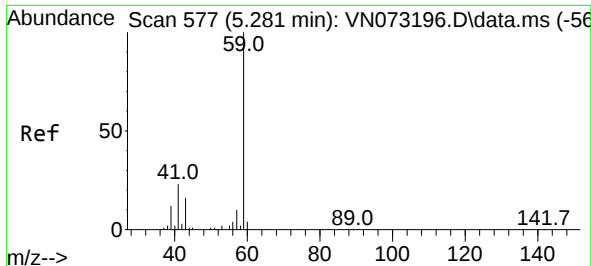

#11
Tert butyl alcohol
Concen: 0.432 ug/l
RT: 5.228 min Scan# 50
Delta R.T. -0.053 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion: 59 Resp: 473
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

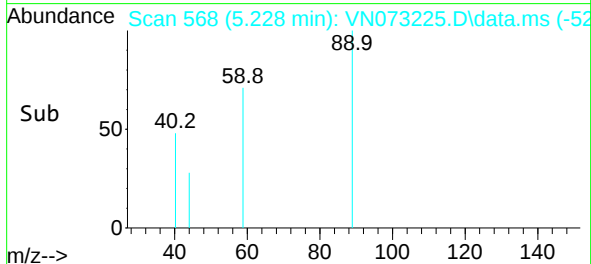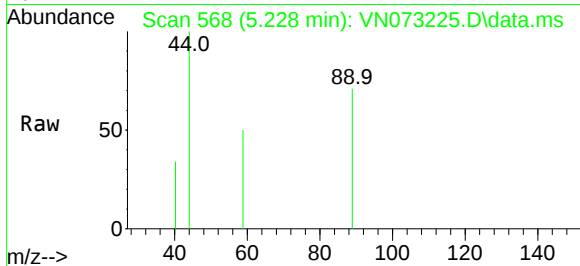

#16
Acetone
Concen: 0.850 ug/l
RT: 4.245 min Scan# 401
Delta R.T. 0.023 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 43 Resp: 2155
Ion Ratio Lower Upper
43 100
58 45.9 26.0 39.0#

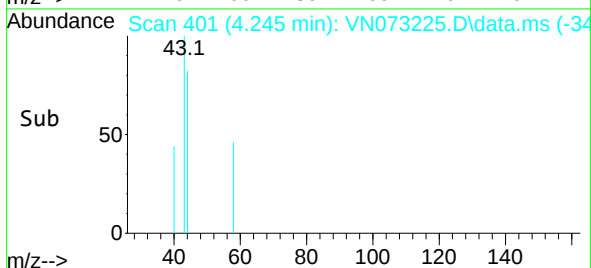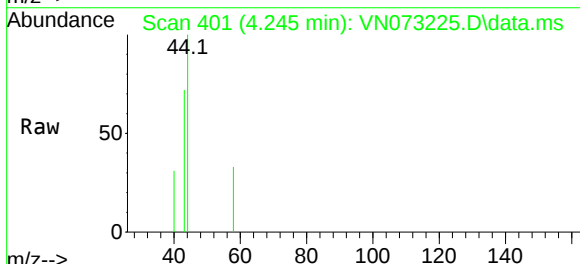

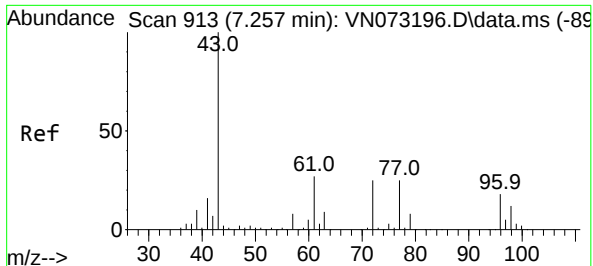

#25

2-Butanone

Concen: 0.399 ug/l

RT: 7.245 min Scan# 91

Delta R.T. -0.012 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42

Instrument :

MSVOA_N

ClientSampleId :





MW-3

Tgt Ion: 43 Resp: 1608

Ion Ratio Lower Upper

43 100

72 0.0 23.7 35.5#

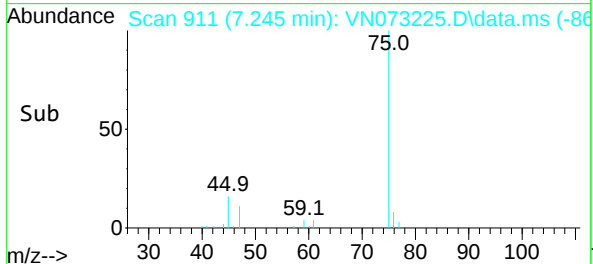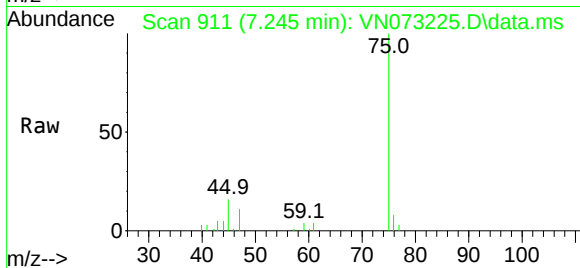

#31

Cyclohexane

Concen: 1.430 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.006 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42




Tgt Ion: 56 Resp: 10576


Ion Ratio Lower Upper

56 100

69 134.3 27.8 41.8#

84 103.8 76.9 115.3

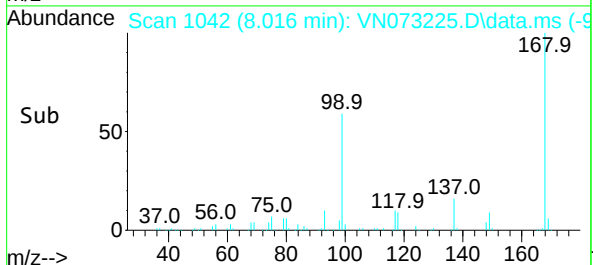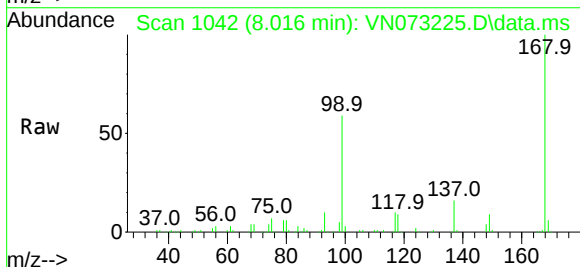

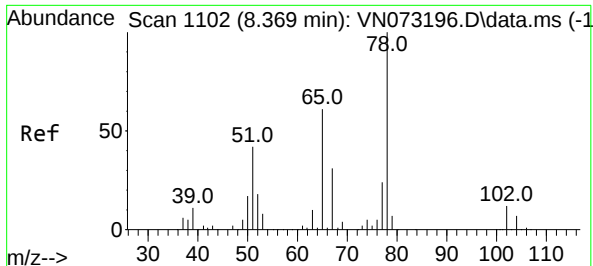

#33

1,2-Dichloroethane-d4

Concen: 43.362 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42

Instrument :

MSVOA_N

ClientSampleId :





MW-3

Tgt Ion: 65 Resp: 195785

Ion Ratio Lower Upper

65 100

67 51.8 0.0 104.8

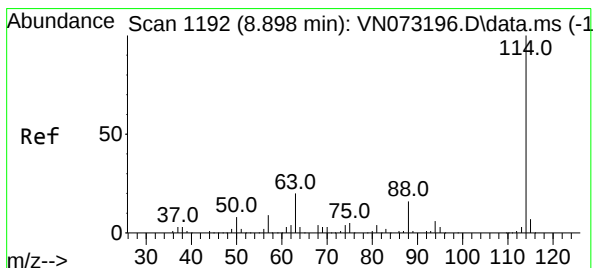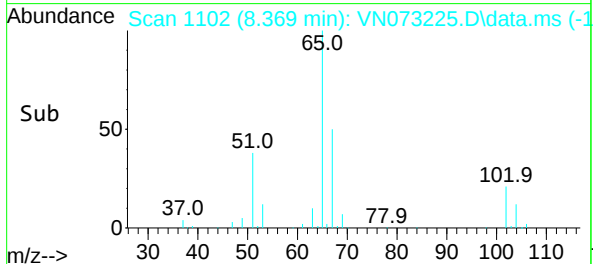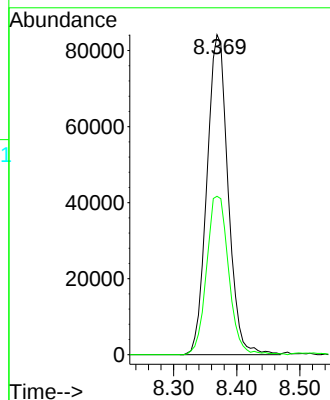

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42




Tgt Ion: 114 Resp: 520554


Ion Ratio Lower Upper

114 100

63 21.1 0.0 40.0

88 16.2 0.0 32.6

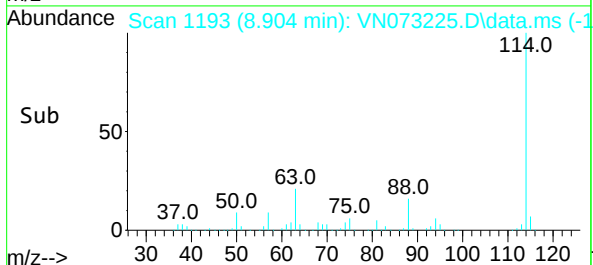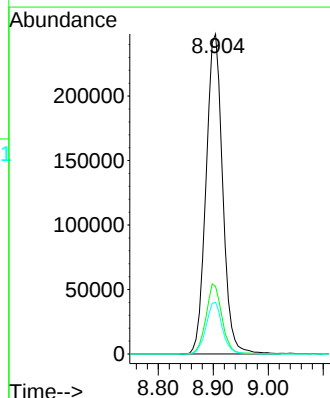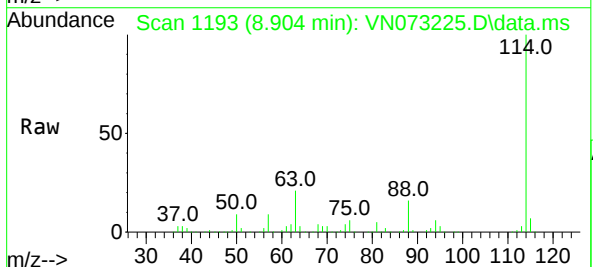

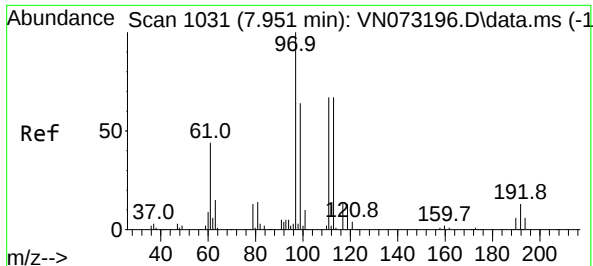

#35

Dibromofluoromethane

Concen: 48.331 ug/l

RT: 7.951 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42

Instrument :

MSVOA_N

ClientSampleId :

MW-3





Tgt Ion:113 Resp: 167386

Ion Ratio Lower Upper

113 100

111 101.1 81.4 122.0

192 17.5 17.0 25.6

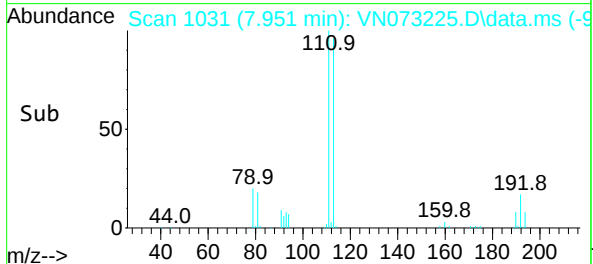

#36

1,1-Dichloropropene

Concen: 4.879 ug/l

RT: 8.010 min Scan# 1041

Delta R.T. -0.135 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42




Tgt Ion: 75 Resp: 25999


Ion Ratio Lower Upper

75 100

110 8.4 18.3 54.8#

77 0.0 25.1 37.7#


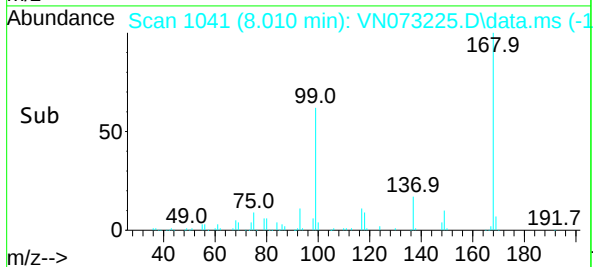

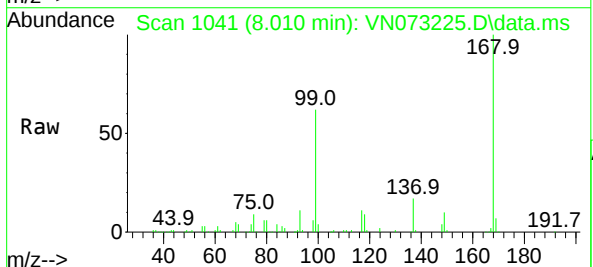


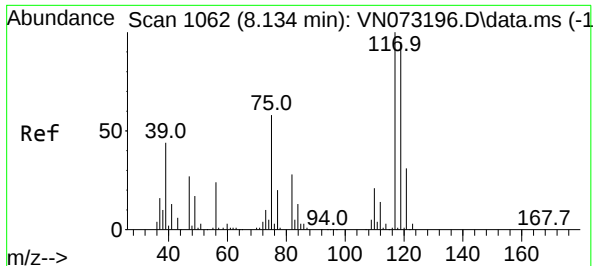

#38
Carbon Tetrachloride
Concen: 5.695 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.118 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion:117 Resp: 31385
Ion Ratio Lower Upper
117 100
119 3.9 75.8 113.8#
121 0.0 24.6 37.0#

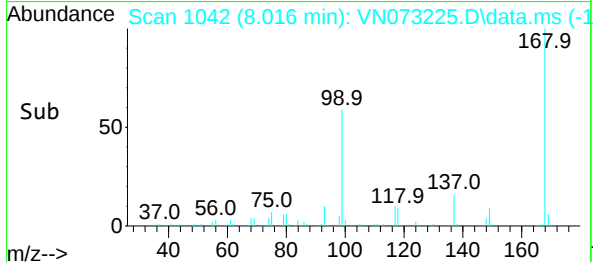

#39
Methylcyclohexane
Concen: 0.468 ug/l
RT: 9.386 min Scan# 1275
Delta R.T. -0.006 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 83 Resp: 3106
Ion Ratio Lower Upper
83 100
55 82.7 57.8 86.8
98 55.2 39.4 59.2


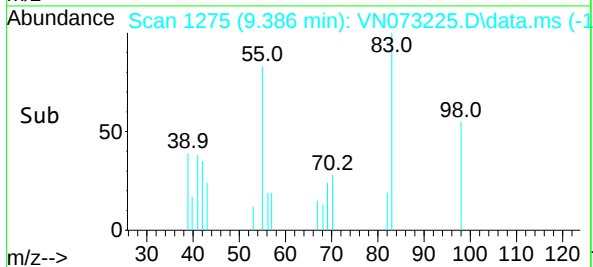

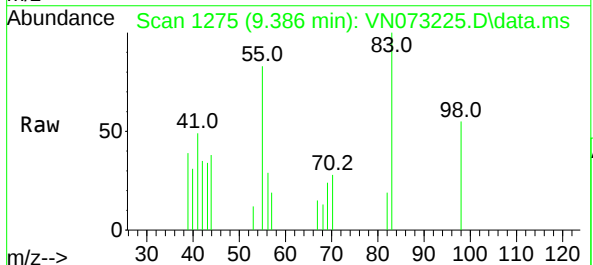


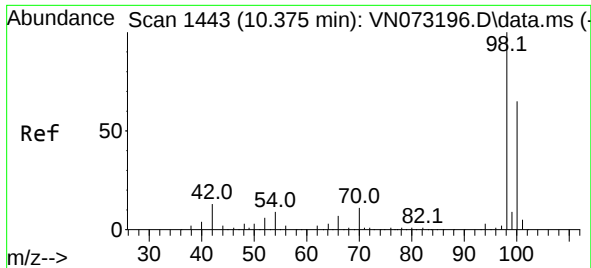

#50
Toluene-d8
Concen: 44.566 ug/l
RT: 10.374 min Scan# 1443
Delta R.T. -0.001 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion: 98 Resp: 548180
Ion Ratio Lower Upper
98 100
100 66.0 52.6 78.8

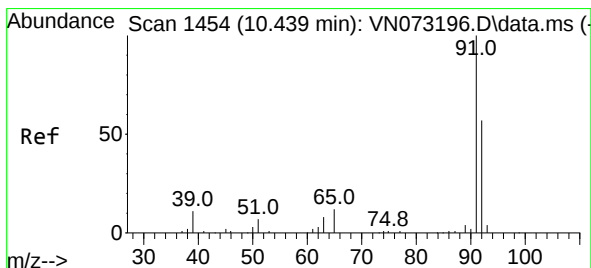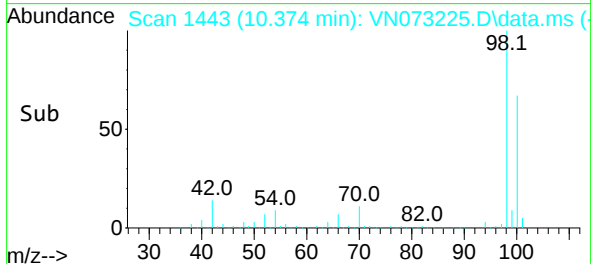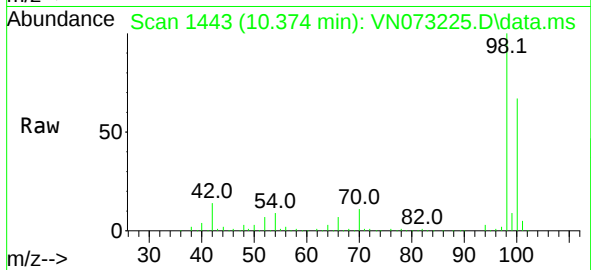

#52
Toluene
Concen: 9.990 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. 0.000 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 92 Resp: 101534
Ion Ratio Lower Upper
92 100
91 176.7 138.6 207.8


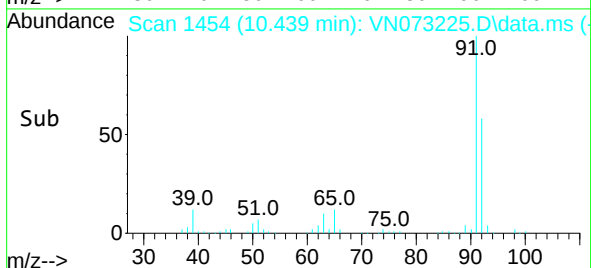

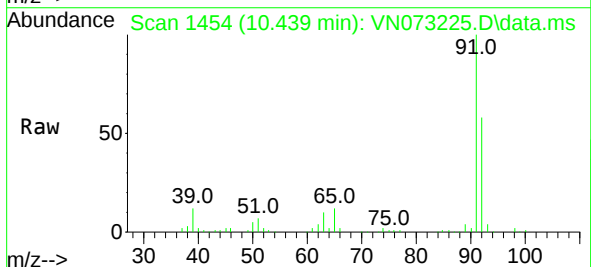




#62
4-Bromofluorobenzene
Concen: 53.164 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.001 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion: 95 Resp: 251308
Ion Ratio Lower Upper
95 100
174 75.6 0.0 167.6
176 72.2 0.0 163.4

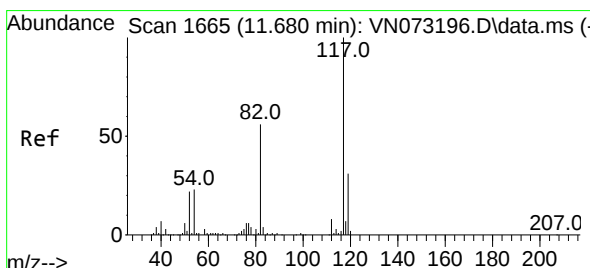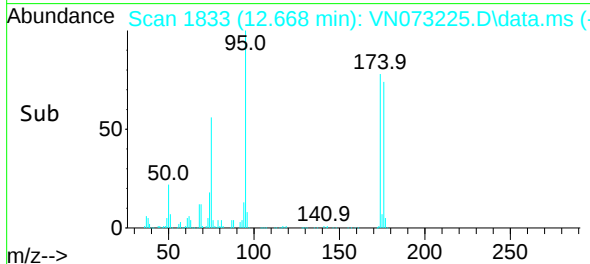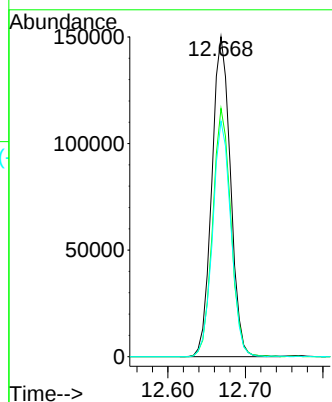

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1665
Delta R.T. 0.000 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 117 Resp: 489044
Ion Ratio Lower Upper
117 100
82 58.1 44.2 66.2
119 31.8 25.4 38.0

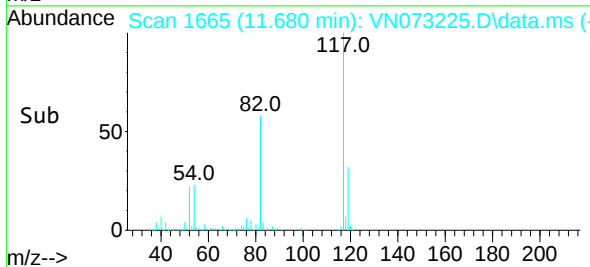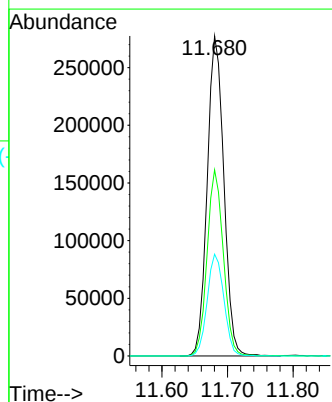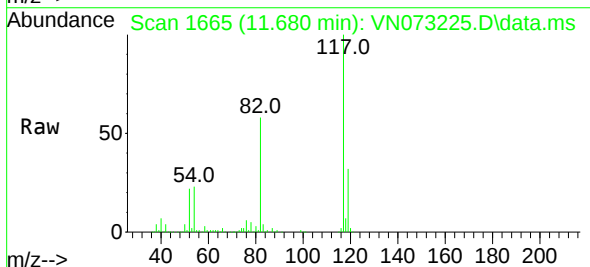



#67

Ethyl Benzene

Concen: 53.815 ug/l

RT: 11.780 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42

Instrument :

MSVOA_N

ClientSampleId :





MW-3

Tgt Ion: 91 Resp: 1080592

Ion Ratio Lower Upper

91 100

106 31.1 24.9 37.3

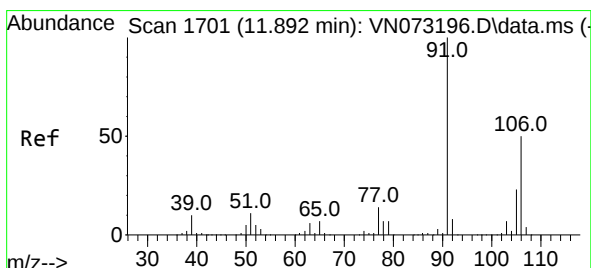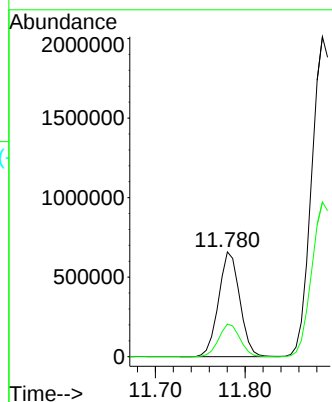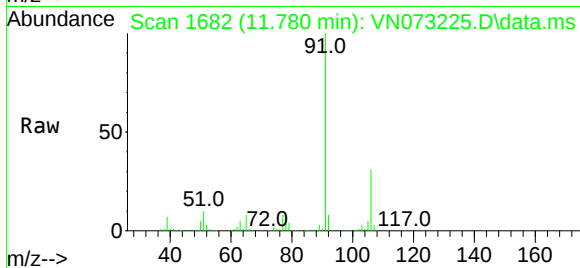

#68

m/p-Xylenes

Concen: 245.636 ug/l

RT: 11.886 min Scan# 1700

Delta R.T. -0.006 min

Lab File: VN073225.D




Acq: 29 Jun 2022 02:42


Tgt Ion:106 Resp: 1861452

Ion Ratio Lower Upper

106 100

91 206.5 158.9 238.3


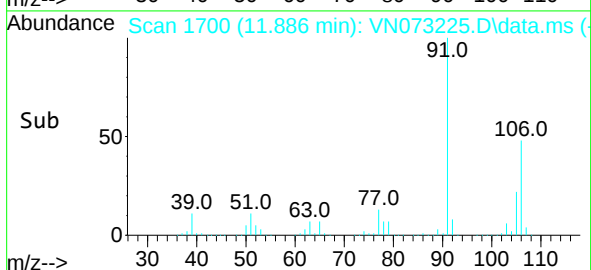

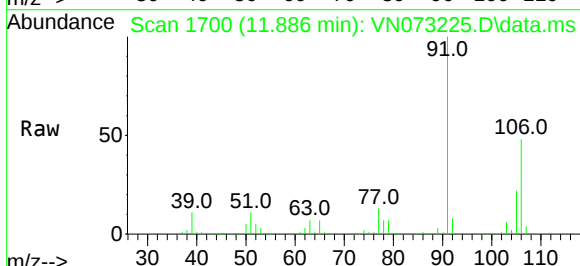




#69
o-Xylene
Concen: 118.537 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. -0.000 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion:106 Resp: 917022
Ion Ratio Lower Upper
106 100
91 218.1 106.0 318.0

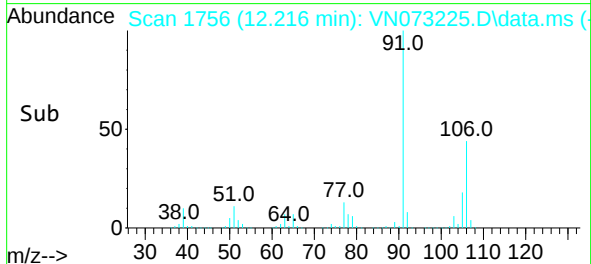

#70
Styrene
Concen: 3.940 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. -0.018 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion:104 Resp: 47062
Ion Ratio Lower Upper
104 100
78 301.0 39.5 59.3#
103 266.3 44.0 66.0#


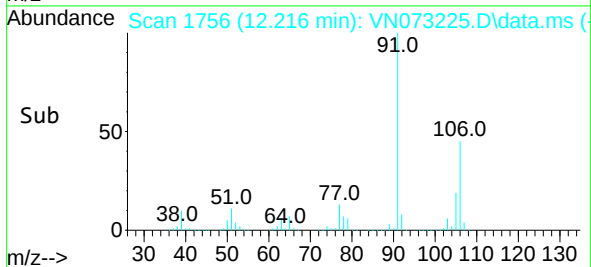

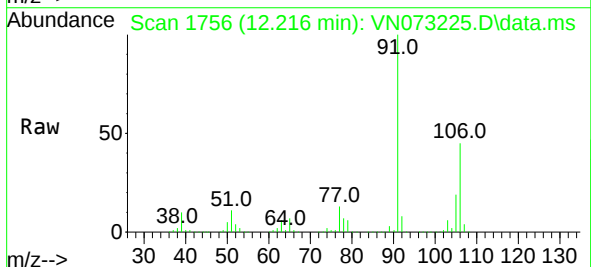




#71
Bromoform
Concen: 0.740 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.270 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion:173 Resp: 2202
Ion Ratio Lower Upper
173 100
175 514.6 24.6 73.6#
254 0.0 0.1 0.1#

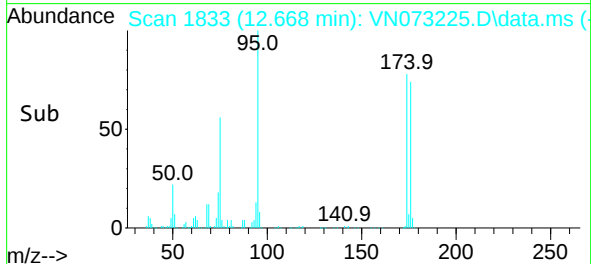

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion:152 Resp: 251021
Ion Ratio Lower Upper
152 100
115 63.7 28.9 86.7
150 155.6 0.0 356.2


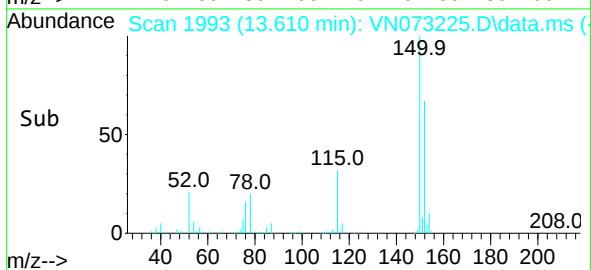

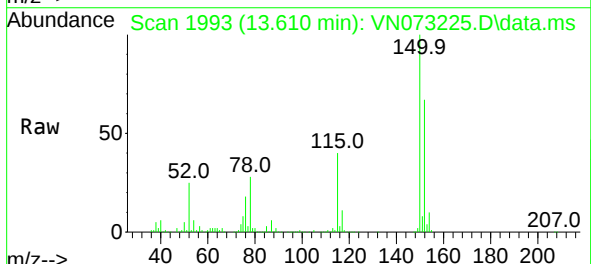


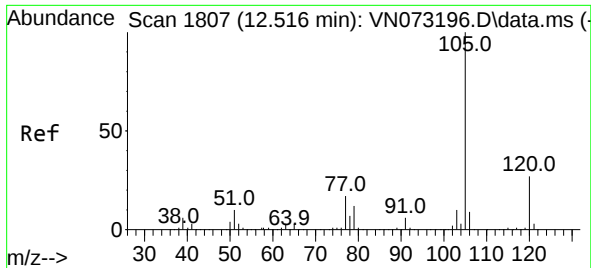

#73
Isopropylbenzene
Concen: 3.367 ug/l
RT: 12.515 min Scan# 11
Delta R.T. -0.001 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion:105 Resp: 72994
Ion Ratio Lower Upper
105 100
120 25.8 13.5 40.4

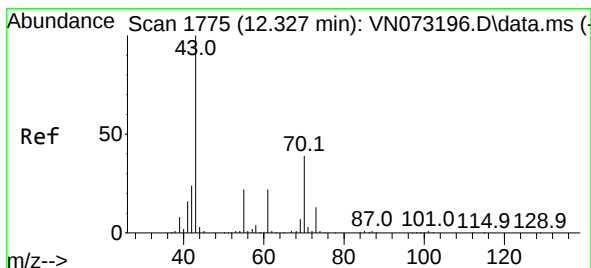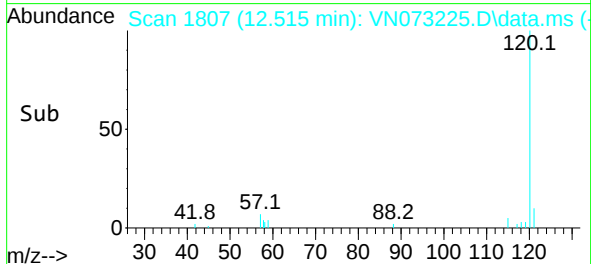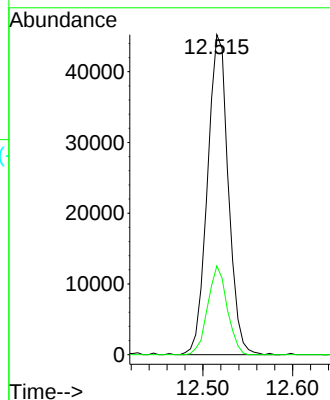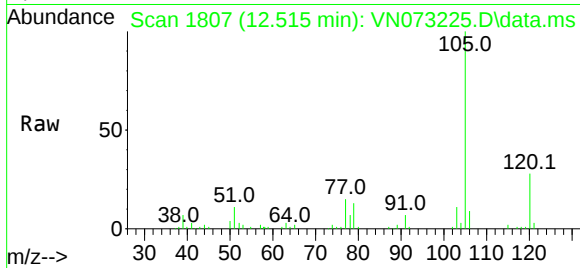

#74
N-ethyl acetate
Concen: 0.222 ug/l
RT: 12.221 min Scan# 1757
Delta R.T. -0.106 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 43 Resp: 2409
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 58.7 21.1 31.7#
61 707.0 21.1 31.7#


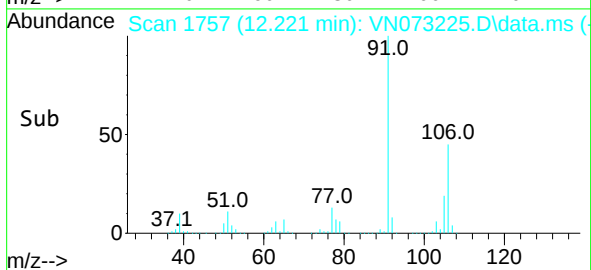
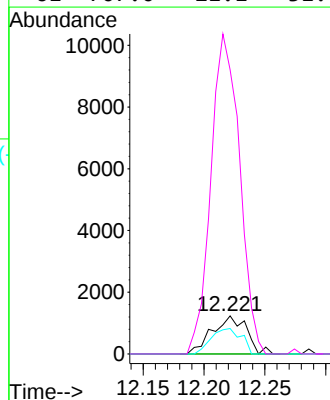
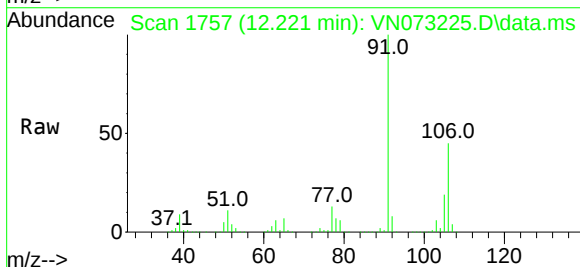




#76
1,2,3-Trichloropropane
Concen: 0.876 ug/l
RT: 12.915 min Scan# 1875
Delta R.T. 0.099 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion: 75 Resp: 5753
Ion Ratio Lower Upper
75 100
77 1066.1 98.5 295.5#

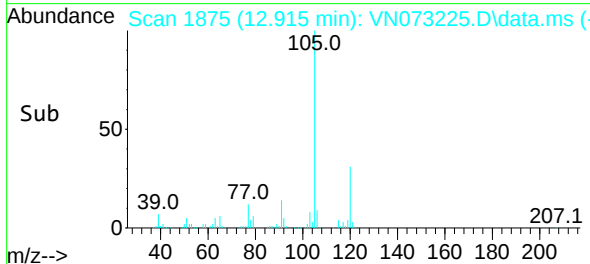

#78
n-propylbenzene
Concen: 4.778 ug/l
RT: 12.857 min Scan# 1865
Delta R.T. -0.000 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 91 Resp: 115063
Ion Ratio Lower Upper
91 100
120 21.9 11.9 35.5


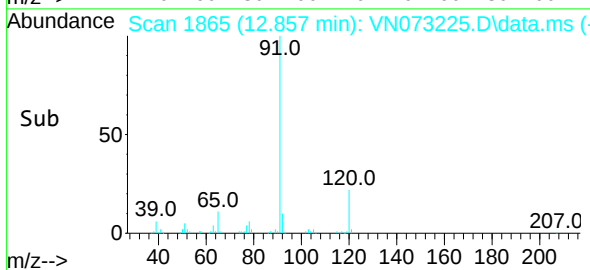

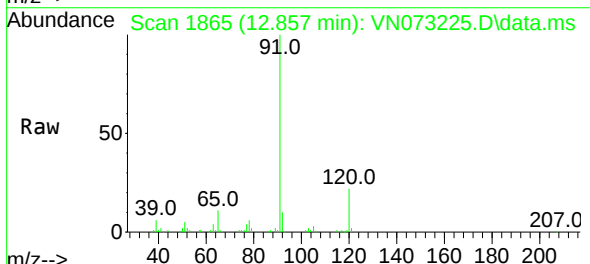


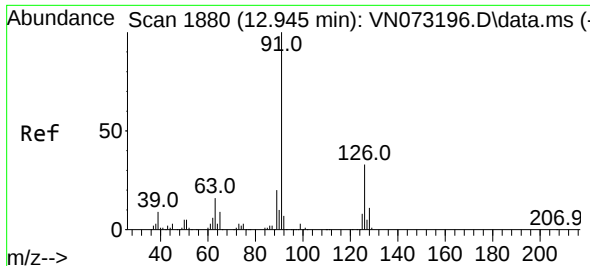

#79
2-Chlorotoluene
Concen: 3.881 ug/l
RT: 12.921 min Scan# 1876
Delta R.T. -0.024 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion: 91 Resp: 59143
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

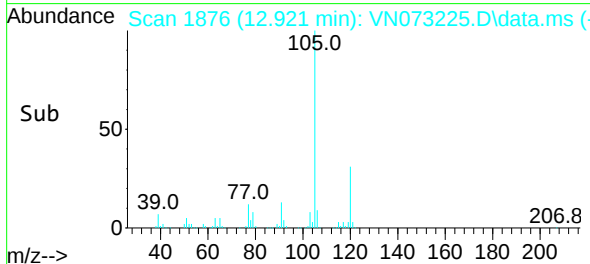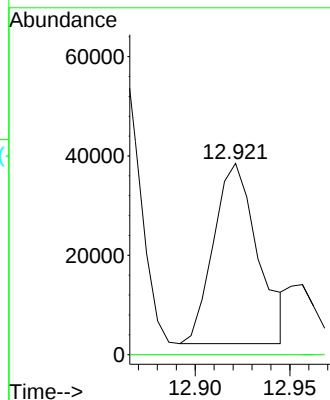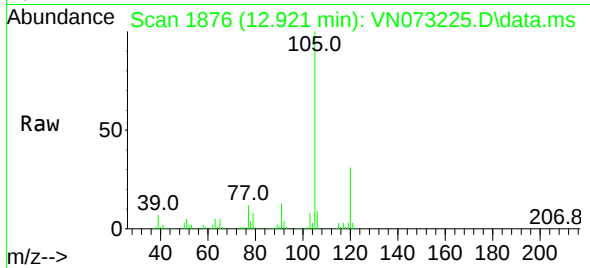

#80
1,3,5-Trimethylbenzene
Concen: 10.423 ug/l
RT: 12.998 min Scan# 1889
Delta R.T. -0.000 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 105 Resp: 184157
Ion Ratio Lower Upper
105 100
120 47.2 24.9 74.7


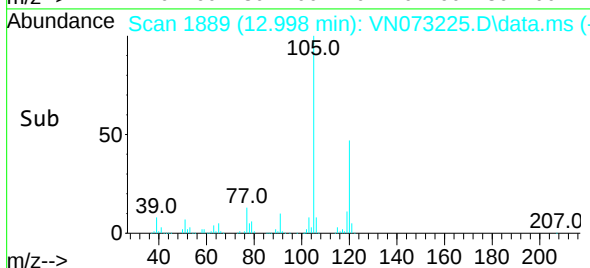
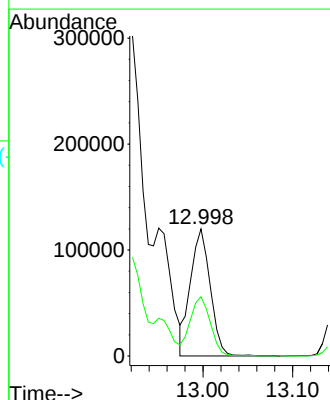
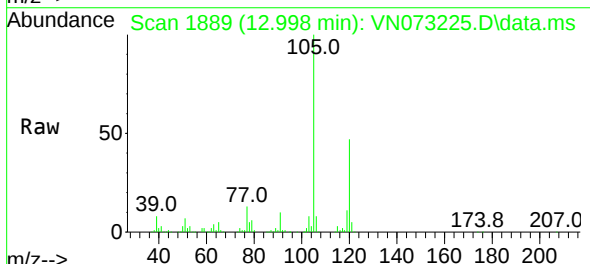




#81
trans-1,4-Dichloro-2-butene
Concen: 56.332 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.105 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion: 75 Resp: 134822
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

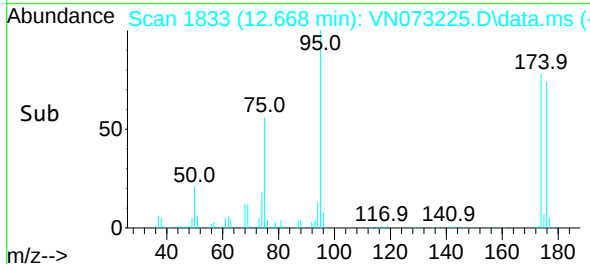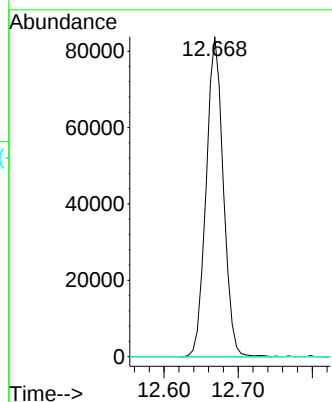

#82
4-Chlorotoluene
Concen: 1.413 ug/l
RT: 12.992 min Scan# 1888
Delta R.T. -0.047 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 91 Resp: 20849
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

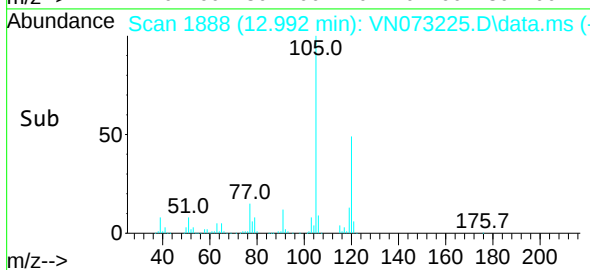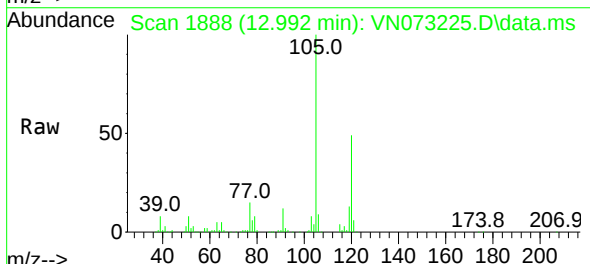

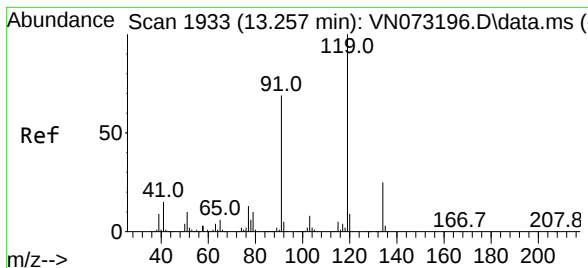

#83

tert-Butylbenzene

Concen: 5.129 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. 0.047 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42

Instrument :

MSVOA_N

ClientSampleId :

MW-3





Tgt Ion:119 Resp: 81241

Ion Ratio Lower Upper

119 100

91 96.8 31.6 94.8#

134 0.0 13.7 41.1#

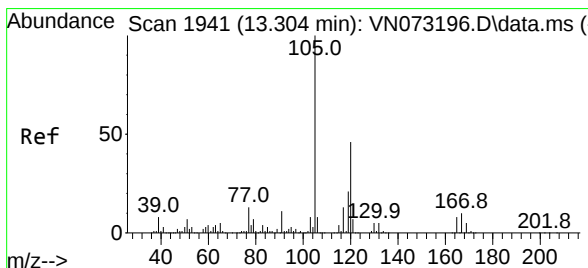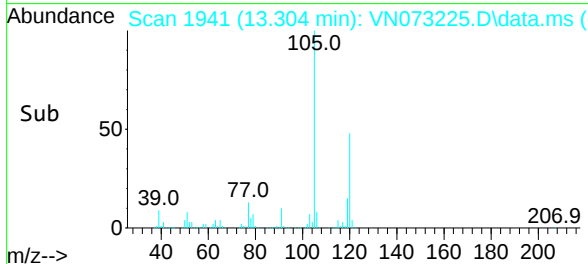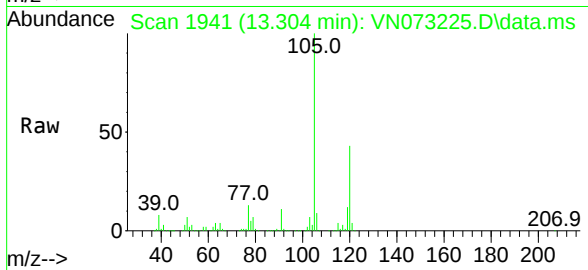

#84

1,2,4-Trimethylbenzene

Concen: 41.056 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. -0.000 min

Lab File: VN073225.D




Acq: 29 Jun 2022 02:42


Tgt Ion:105 Resp: 724224

Ion Ratio Lower Upper

105 100

120 44.4 23.3 69.8

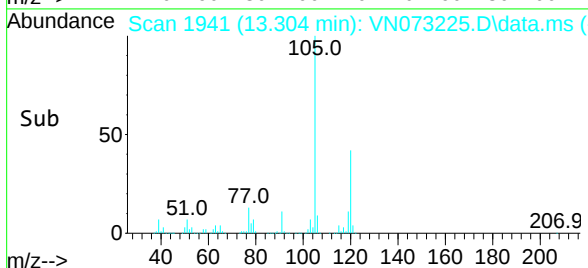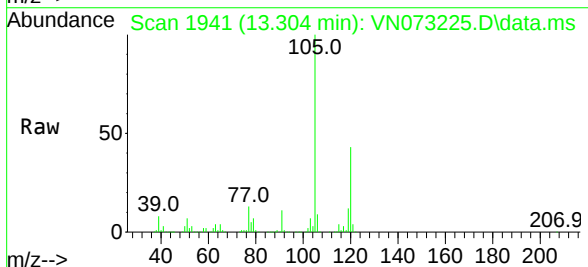

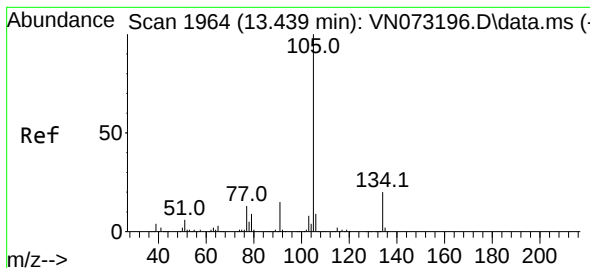

#85

sec-Butylbenzene

Concen: 34.050 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. -0.135 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42

Instrument :

MSVOA_N

ClientSampleId :





MW-3

Tgt Ion:105 Resp: 724224

Ion Ratio Lower Upper

105 100

134 0.0 10.4 31.1#

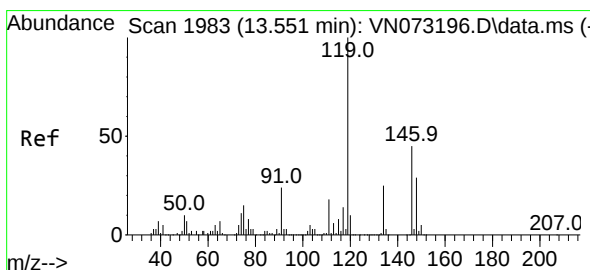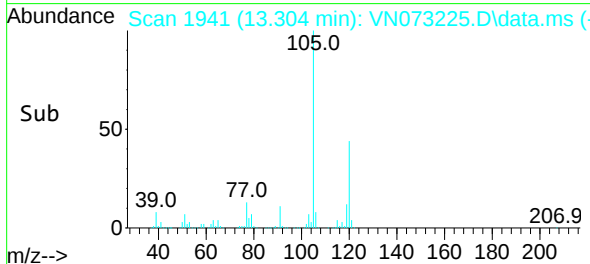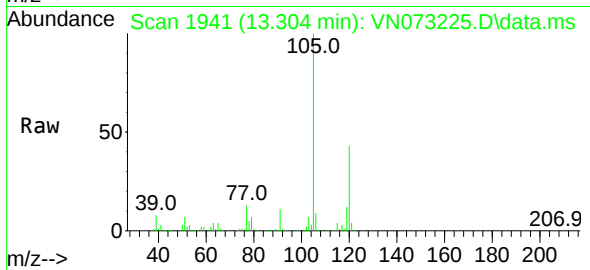

#86

p-Isopropyltoluene

Concen: 0.483 ug/l

RT: 13.498 min Scan# 1974

Delta R.T. -0.053 min

Lab File: VN073225.D

Acq: 29 Jun 2022 02:42




Tgt Ion:119 Resp: 8306


Ion Ratio Lower Upper

119 100

134 30.1 13.3 39.8

91 29.3 11.3 33.9


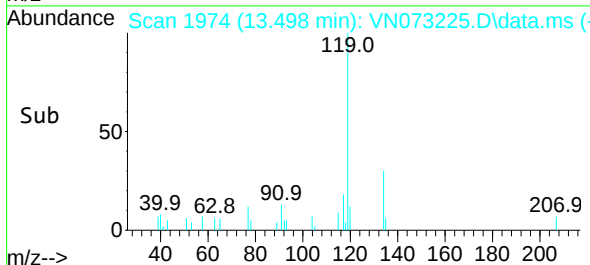
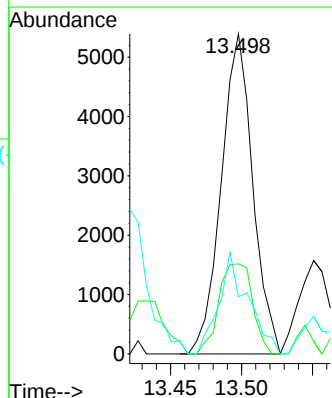
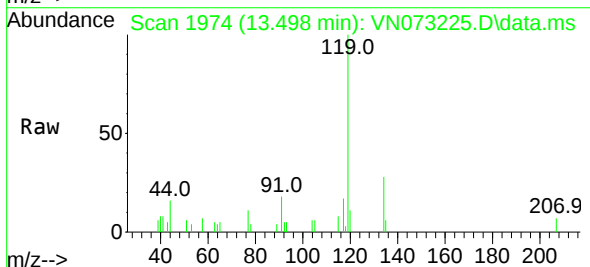




#89
n-Butylbenzene
Concen: 0.332 ug/l
RT: 13.880 min Scan# 2039
Delta R.T. 0.000 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion: 91 Resp: 4752
Ion Ratio Lower Upper
91 100
92 77.0 26.9 80.7
134 0.0 13.6 40.8#

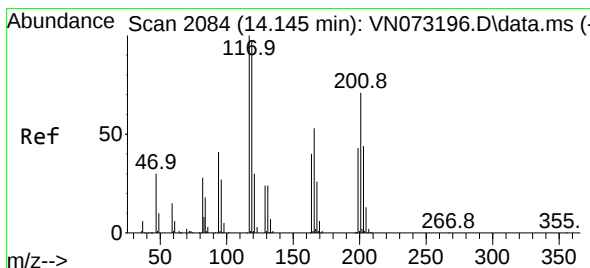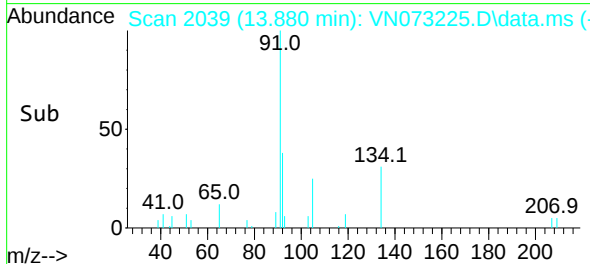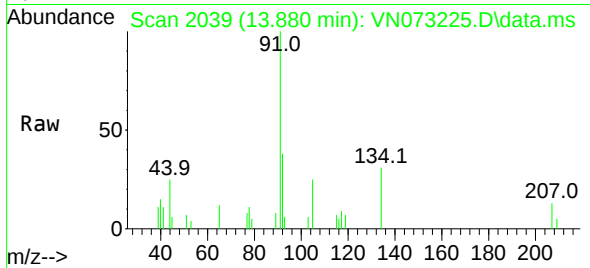

#90
Hexachloroethane
Concen: 1.236 ug/l
RT: 14.151 min Scan# 2085
Delta R.T. 0.006 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 117 Resp: 3957
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#


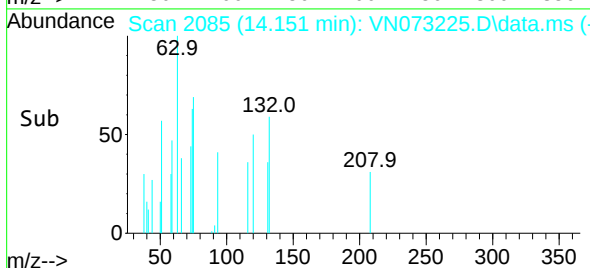

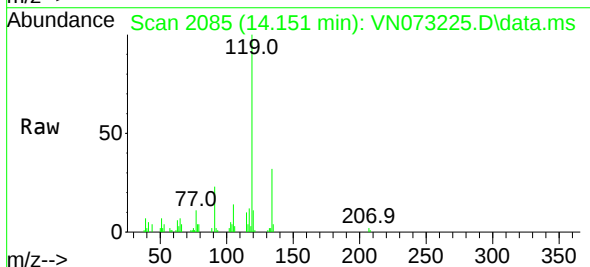


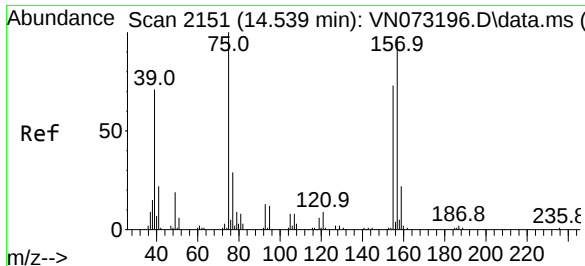

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.249 ug/l
RT: 14.521 min Scan# 2151
Delta R.T. -0.018 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Instrument :
MSVOA_N
ClientSampleId :
MW-3

Tgt Ion: 75 Resp: 435
Ion Ratio Lower Upper
75 100
155 0.0 44.9 134.5#
157 0.0 59.0 176.8#

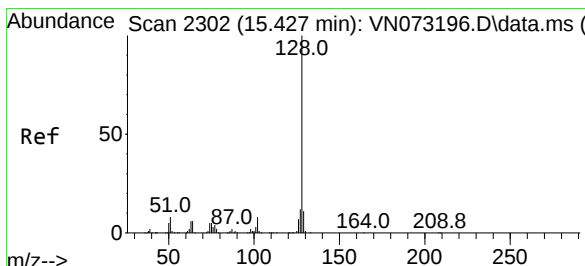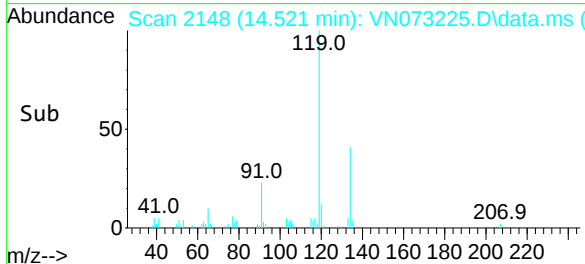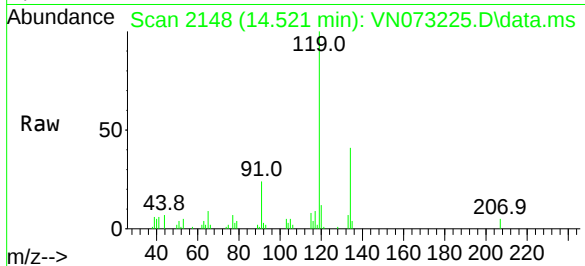

#95
Naphthalene
Concen: 8.915 ug/l
RT: 15.433 min Scan# 2303
Delta R.T. 0.006 min
Lab File: VN073225.D
Acq: 29 Jun 2022 02:42

Tgt Ion: 128 Resp: 172466
Ion Ratio Lower Upper
128 100
127 12.7 10.3 15.5
129 10.6 8.6 13.0

