

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062822\
 Data File : VN073226.D
 Acq On : 29 Jun 2022 03:06
 Operator : JC\MD
 Sample : N3409-07 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-4

Quant Time: Jun 29 04:28:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	324512	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.898	114	536546	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	510852	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	256882	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	201606	43.035	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.080%
35) Dibromofluoromethane	7.945	113	169776	47.560	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.120%
50) Toluene-d8	10.374	98	571285	45.060	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	90.120%
62) 4-Bromofluorobenzene	12.668	95	267966	54.998	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	110.000%


Target Compounds				Qvalue		
6) Chloroethane	2.957	64	1160	0.504	ug/l #	42
11) Tert butyl alcohol	5.228	59	9040	7.966	ug/l #	74
16) Acetone	4.234	43	1568	0.596	ug/l #	42
18) Methyl Acetate	4.781	43	2976	0.404	ug/l #	70
20) Methylene Chloride	4.998	84	1076	0.233	ug/l #	73
25) 2-Butanone	7.228	43	952	0.227	ug/l #	45
26) 2,2-Dichloropropane	7.233	77	1487	0.207	ug/l #	53
29) Tetrahydrofuran	7.622	42	745	0.260	ug/l #	44
31) Cyclohexane	8.010	56	10180	1.327	ug/l #	53
36) 1,1-Dichloropropene	8.016	75	27682	5.040	ug/l #	48
38) Carbon Tetrachloride	8.016	117	34484	6.071	ug/l #	17
39) Methylcyclohexane	9.392	83	4125	0.603	ug/l #	76
52) Toluene	10.445	92	21105	2.015	ug/l	98
67) Ethyl Benzene	11.780	91	393664	18.768	ug/l	98
68) m/p-Xylenes	11.892	106	331072	41.823	ug/l	96
69) o-Xylene	12.216	106	78761	9.746	ug/l	97
70) Styrene	12.216	104	4164	0.334	ug/l #	1
71) Bromoform	12.668	173	1005	0.323	ug/l #	1
73) Isopropylbenzene	12.515	105	41771	1.883	ug/l	99
76) 1,2,3-Trichloropropane	12.668	75	140661	20.941	ug/l #	1
78) n-propylbenzene	12.857	91	91904	3.729	ug/l	96
79) 2-Chlorotoluene	12.921	91	26675	1.710	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.998	105	131003	7.245	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.668	75	140661	57.430	ug/l #	10
82) 4-Chlorotoluene	12.998	91	14920	0.988	ug/l #	40
83) tert-Butylbenzene	13.304	119	62919	3.882	ug/l #	62
84) 1,2,4-Trimethylbenzene	13.304	105	525581	29.115	ug/l	98
85) sec-Butylbenzene	13.304	105	525581	24.147	ug/l #	56
86) p-Isopropyltoluene	13.498	119	5143	0.292	ug/l #	78
89) n-Butylbenzene	13.810	91	25064	1.711	ug/l #	55
90) Hexachloroethane	14.151	117	3946	1.204	ug/l #	9
95) Naphthalene	15.433	128	128553	6.493	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062822\
Data File : VN073226.D
Acq On : 29 Jun 2022 03:06
Operator : JC\MD
Sample : N3409-07 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-4

Quant Time: Jun 29 04:28:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




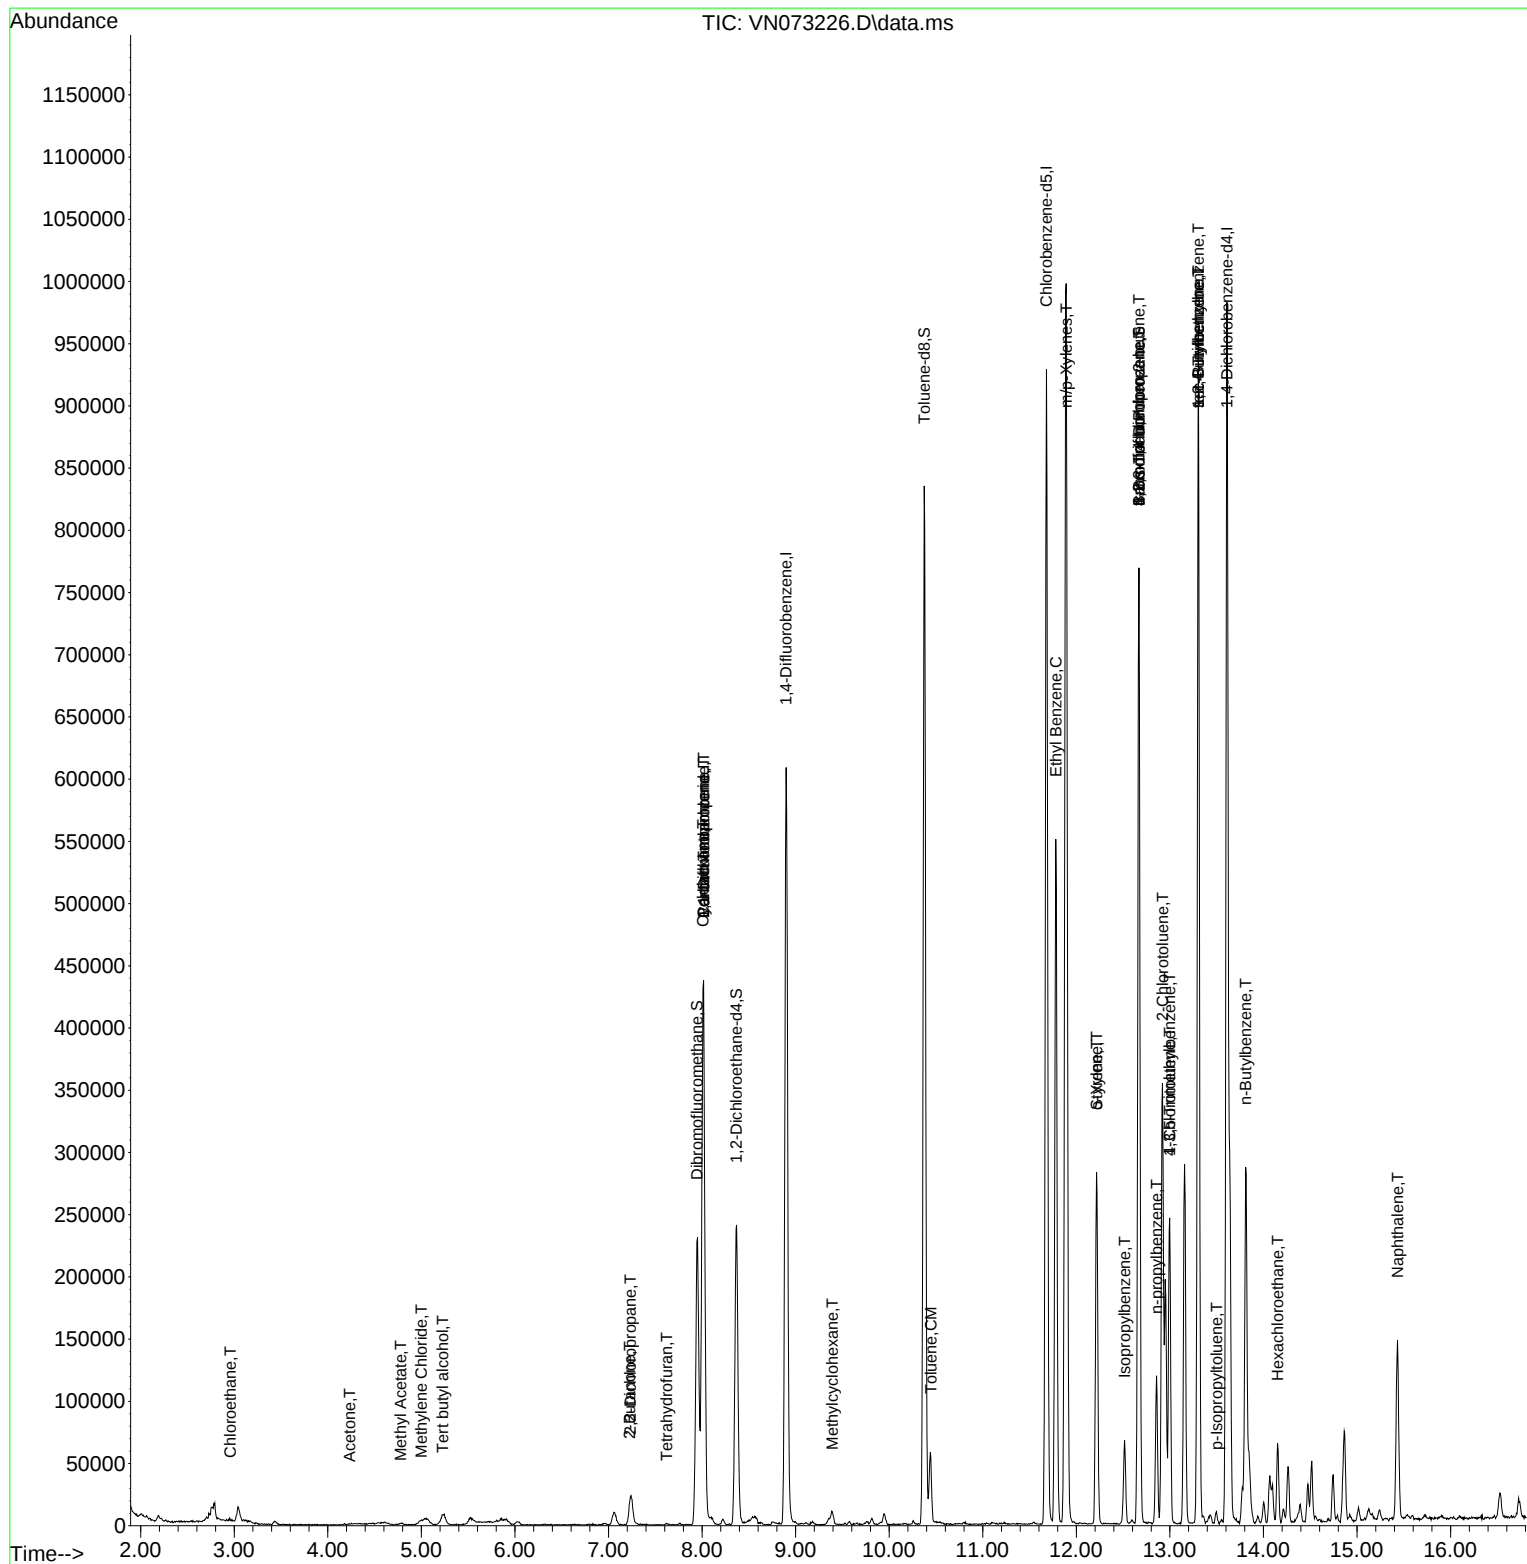


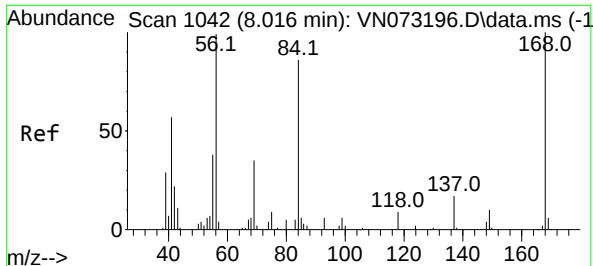

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:168 Resp: 324512
Ion Ratio Lower Upper
168 100
99 60.3 42.3 63.5

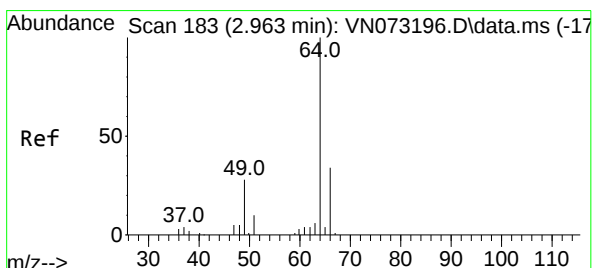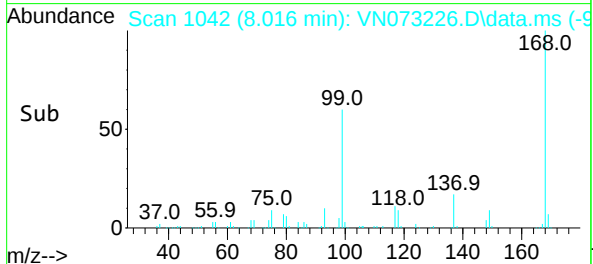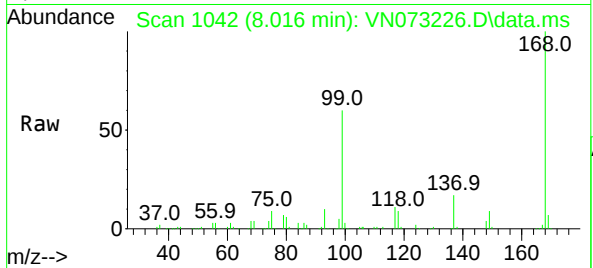

#6
Chloroethane
Concen: 0.504 ug/l
RT: 2.957 min Scan# 182
Delta R.T. -0.006 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 64 Resp: 1160
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

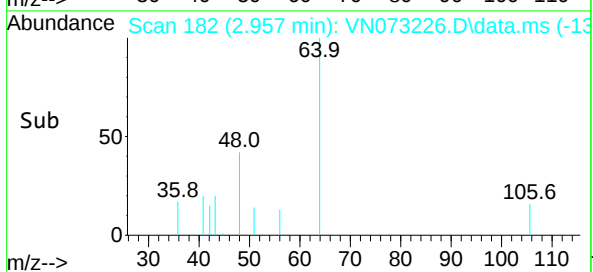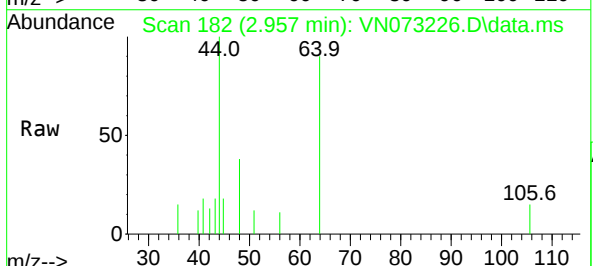

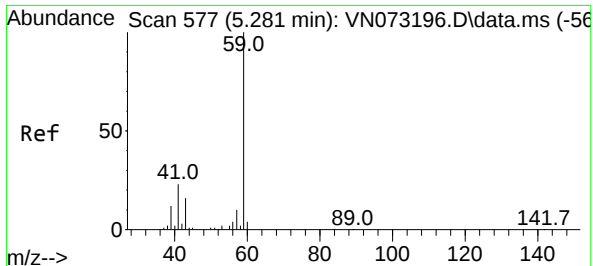

#11

Tert butyl alcohol

Concen: 7.966 ug/l

RT: 5.228 min Scan# 50

Delta R.T. -0.053 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Instrument :

MSVOA_N

ClientSampleId :





MW-4

Tgt Ion: 59 Resp: 9040

Ion Ratio Lower Upper

59 100

57 0.6 8.3 12.5#

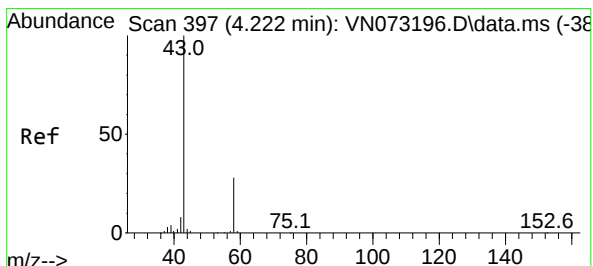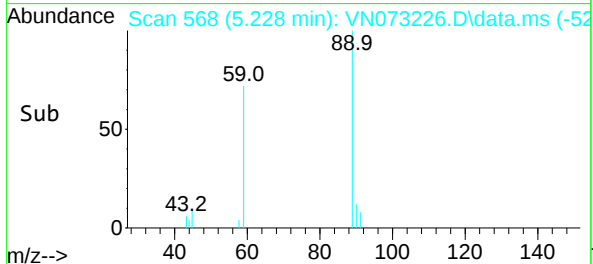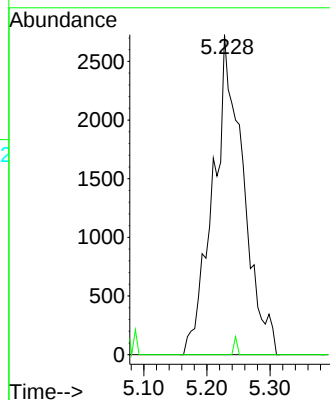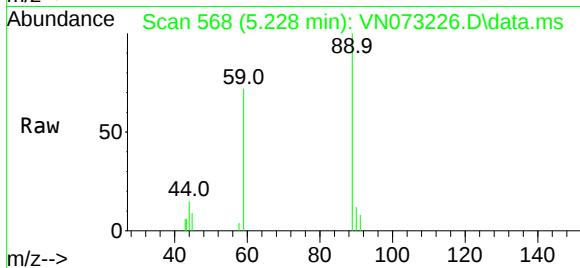

#16

Acetone

Concen: 0.596 ug/l

RT: 4.234 min Scan# 399

Delta R.T. 0.012 min

Lab File: VN073226.D




Acq: 29 Jun 2022 03:06


Tgt Ion: 43 Resp: 1568

Ion Ratio Lower Upper

43 100

58 0.0 26.0 39.0#


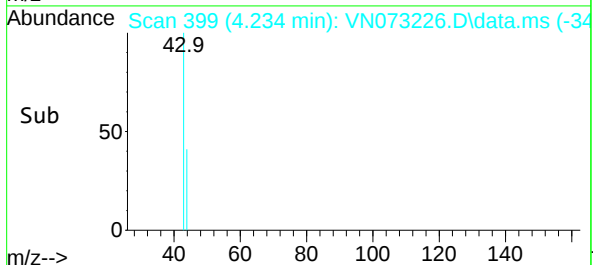
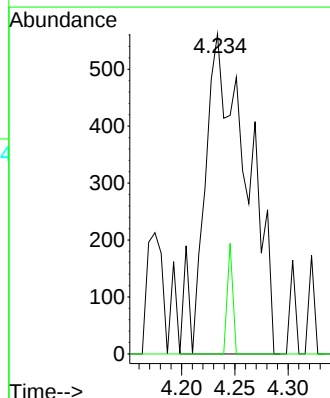
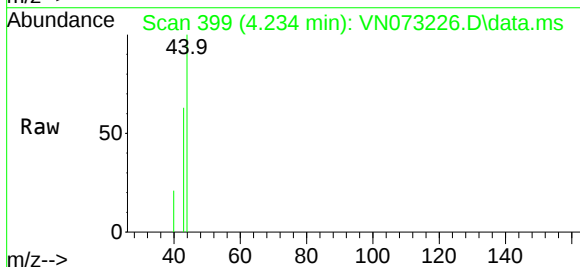




#18
Methyl Acetate
Concen: 0.404 ug/l
RT: 4.781 min Scan# 491
Delta R.T. 0.006 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 43 Resp: 2976
Ion Ratio Lower Upper
43 100
74 11.5 21.6 32.4#

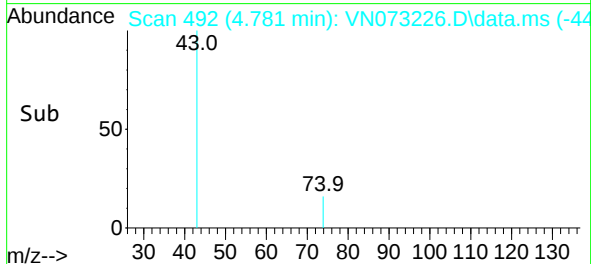

#20
Methylene Chloride
Concen: 0.233 ug/l
RT: 4.998 min Scan# 529
Delta R.T. -0.018 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 84 Resp: 1076
Ion Ratio Lower Upper
84 100
49 76.9 88.3 132.5#
51 41.0 28.2 42.2
86 41.0 50.6 76.0#

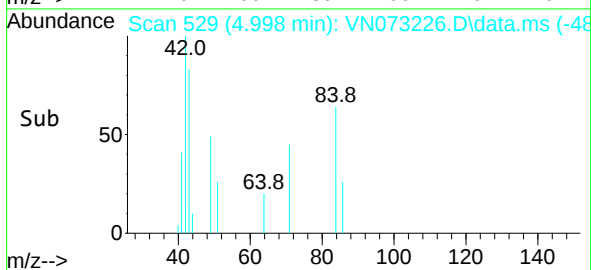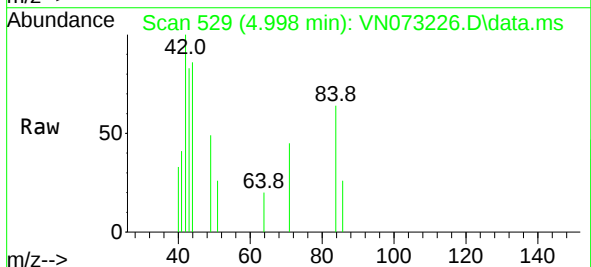

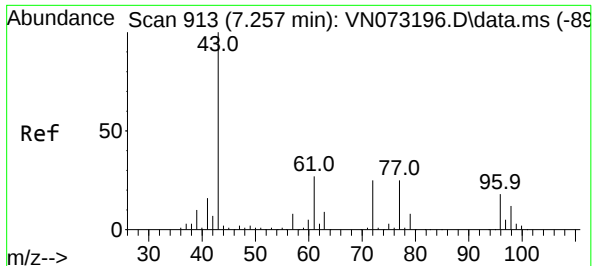

#25

2-Butanone

Concen: 0.227 ug/l

RT: 7.228 min Scan# 908

Delta R.T. -0.029 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Instrument :

MSVOA_N

ClientSampleId :





MW-4

Tgt Ion: 43 Resp: 952

Ion Ratio Lower Upper

43 100

72 0.0 23.7 35.5#

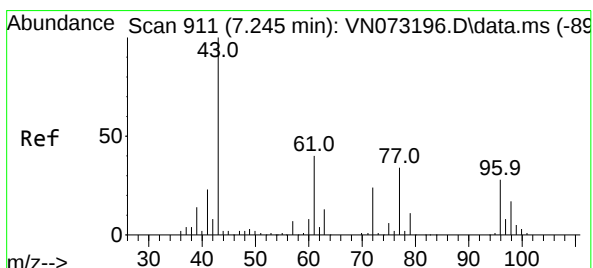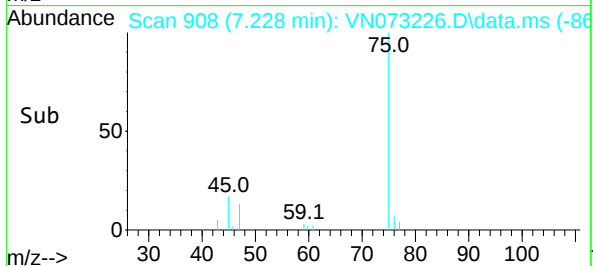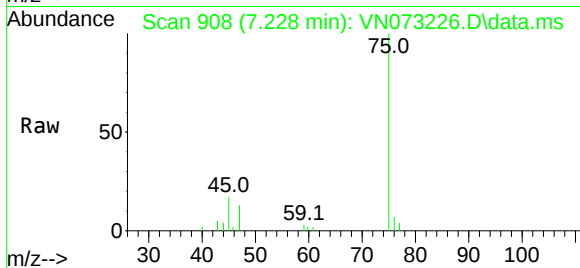

#26

2,2-Dichloropropane

Concen: 0.207 ug/l

RT: 7.233 min Scan# 909

Delta R.T. -0.012 min

Lab File: VN073226.D




Acq: 29 Jun 2022 03:06


Tgt Ion: 77 Resp: 1487

Ion Ratio Lower Upper

77 100

97 0.0 11.4 34.2#

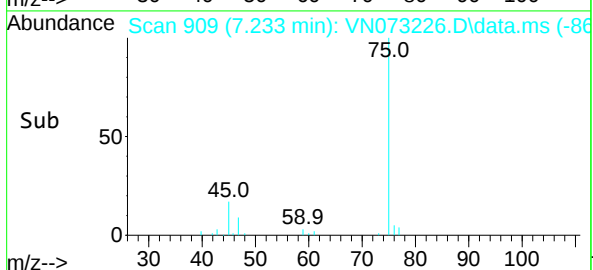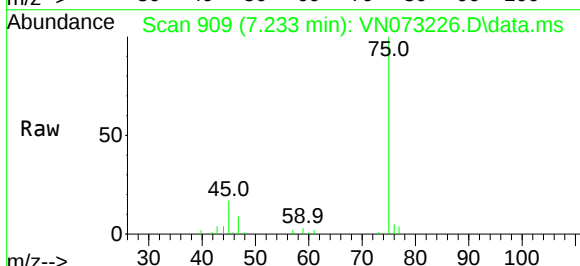

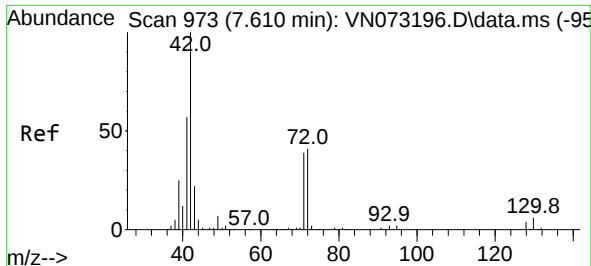

#29

Tetrahydrofuran

Concen: 0.260 ug/l

RT: 7.622 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Instrument :

MSVOA_N

ClientSampleId :

MW-4





Tgt Ion: 42 Resp: 745

Ion Ratio Lower Upper

42 100

72 20.3 39.7 59.5#

71 0.0 36.6 55.0#

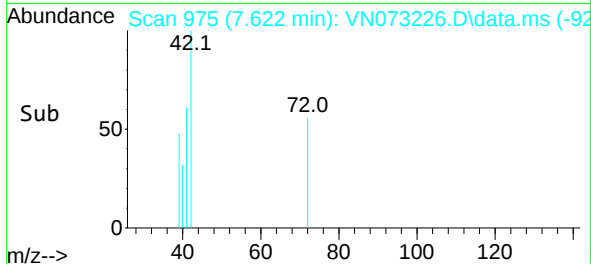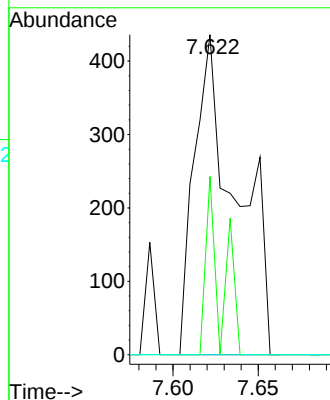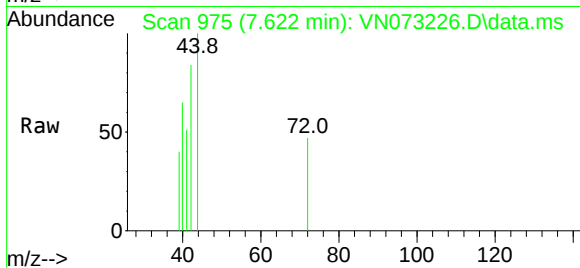

#31

Cyclohexane

Concen: 1.327 ug/l

RT: 8.010 min Scan# 1041

Delta R.T. -0.012 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06




Tgt Ion: 56 Resp: 10180


Ion Ratio Lower Upper

56 100

69 113.6 27.8 41.8#

84 110.4 76.9 115.3


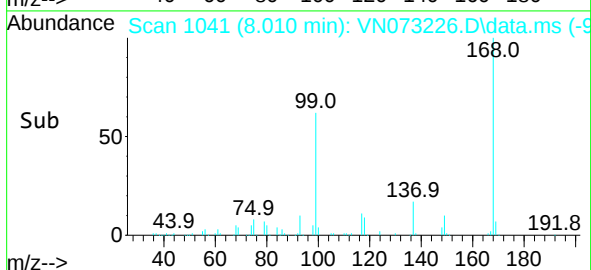
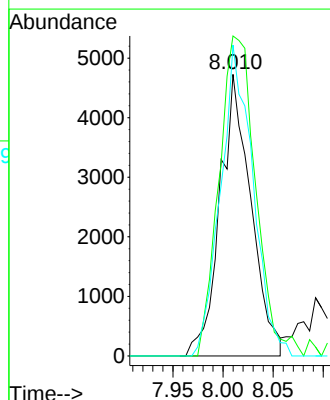
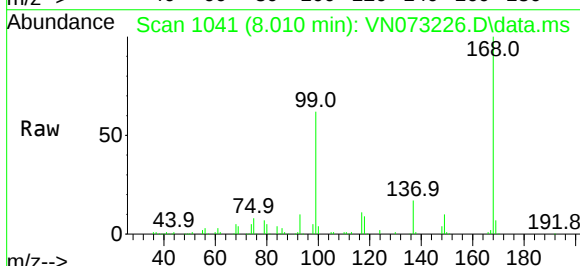


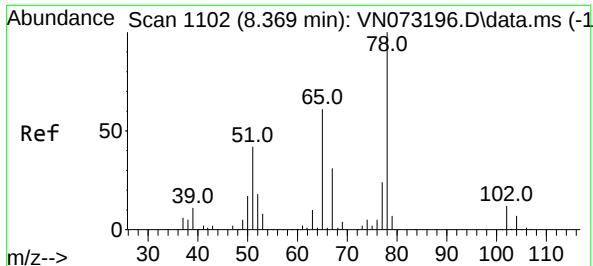

#33
1,2-Dichloroethane-d4
Concen: 43.035 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 65 Resp: 201606
Ion Ratio Lower Upper
65 100
67 52.4 0.0 104.8

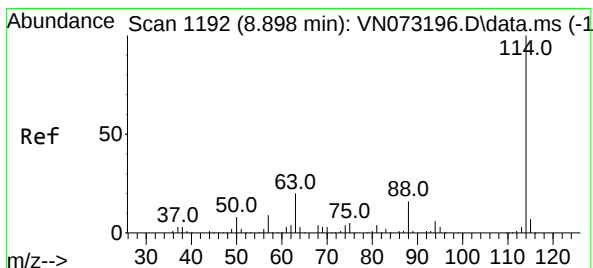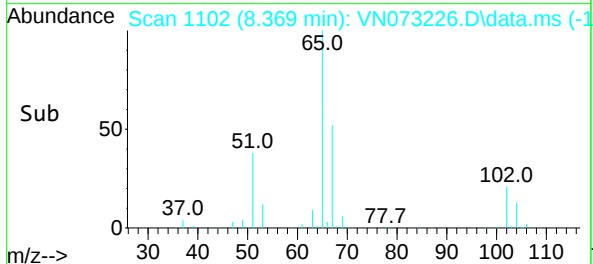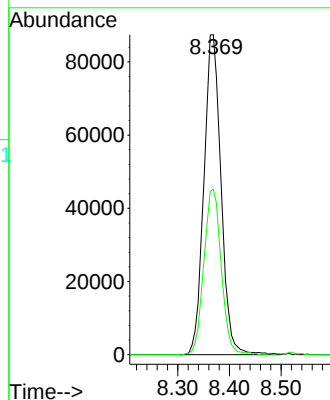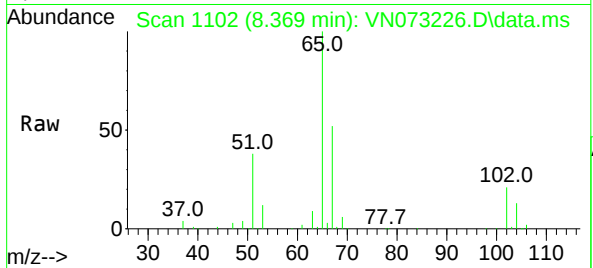

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.898 min Scan# 1192
Delta R.T. 0.000 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 114 Resp: 536546
Ion Ratio Lower Upper
114 100
63 21.0 0.0 40.0
88 15.5 0.0 32.6

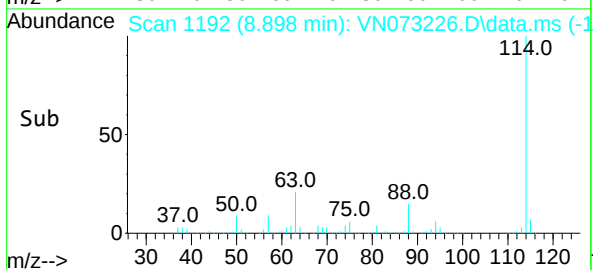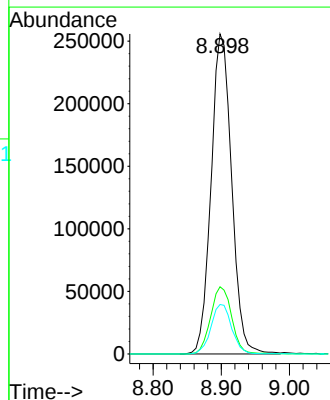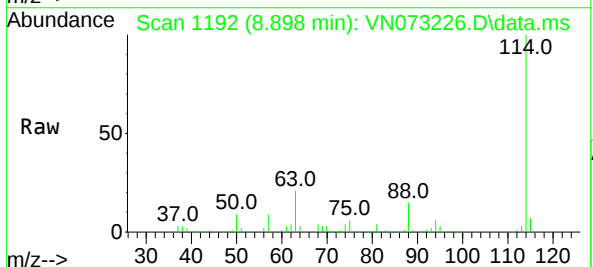

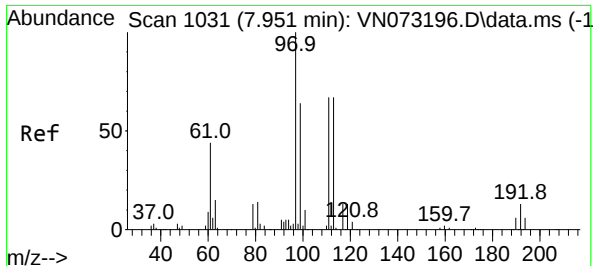

#35

Dibromofluoromethane

Concen: 47.560 ug/l

RT: 7.945 min Scan# 1030

Delta R.T. -0.006 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Instrument :

MSVOA_N

ClientSampleId :

MW-4





Tgt Ion:113 Resp: 169776

Ion Ratio Lower Upper

113 100

111 101.6 81.4 122.0

192 17.7 17.0 25.6

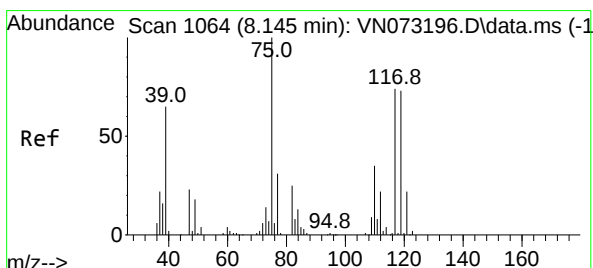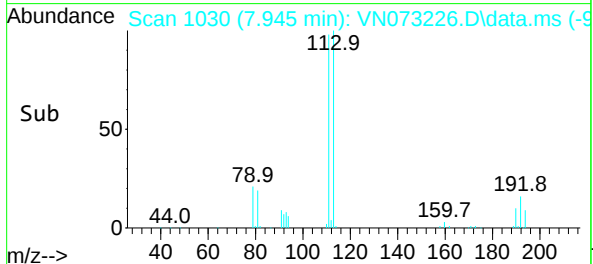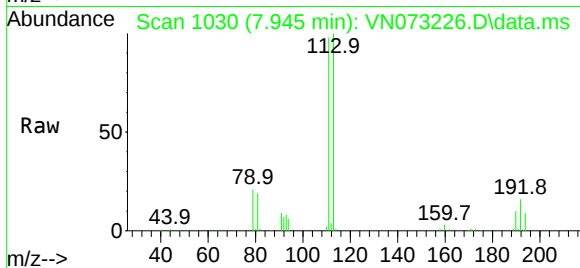

#36

1,1-Dichloropropene

Concen: 5.040 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.129 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06




Tgt Ion: 75 Resp: 27682


Ion Ratio Lower Upper

75 100

110 7.9 18.3 54.8#


77 0.0 25.1 37.7#

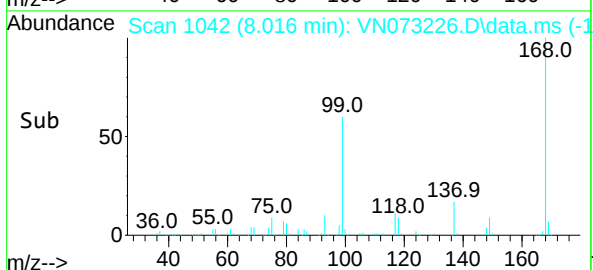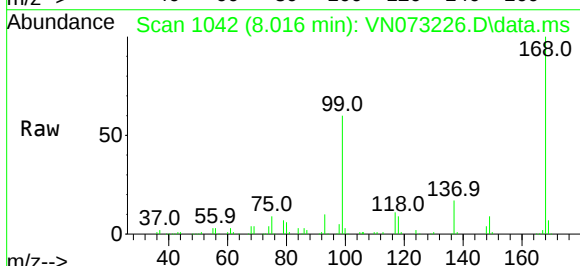



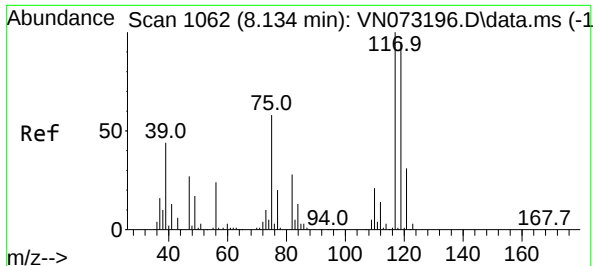


#38
Carbon Tetrachloride
Concen: 6.071 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.118 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Instrument :
MSVOA_N
ClientSampleId :
MW-4



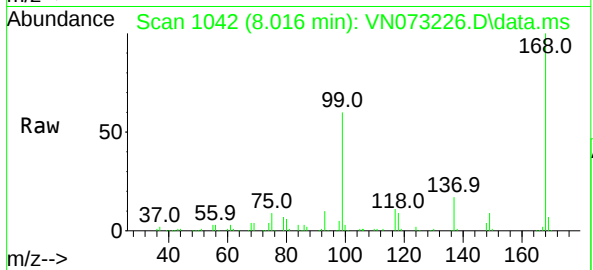



Tgt Ion:117 Resp: 34484
Ion Ratio Lower Upper
117 100
119 5.4 75.8 113.8#
121 0.0 24.6 37.0#

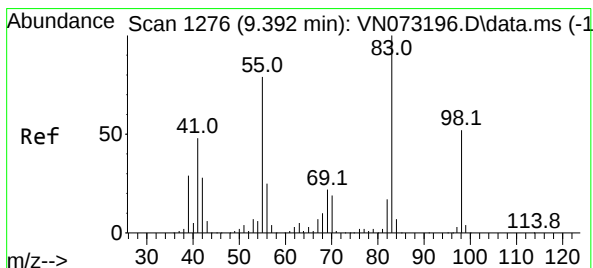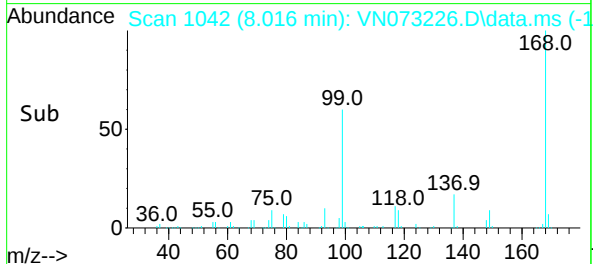

#39
Methylcyclohexane
Concen: 0.603 ug/l
RT: 9.392 min Scan# 1276
Delta R.T. 0.000 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 83 Resp: 4125
Ion Ratio Lower Upper
83 100
55 86.4 57.8 86.8
98 73.6 39.4 59.2#


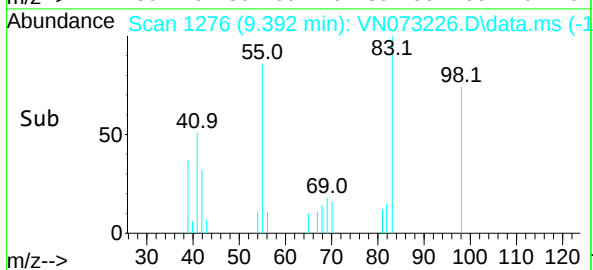

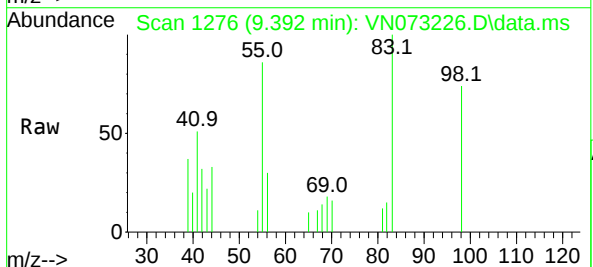




#50
Toluene-d8
Concen: 45.060 ug/l
RT: 10.374 min Scan# 1443
Delta R.T. -0.001 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 98 Resp: 571285
Ion Ratio Lower Upper
98 100
100 65.7 52.6 78.8

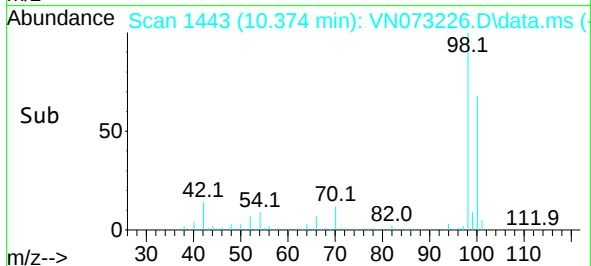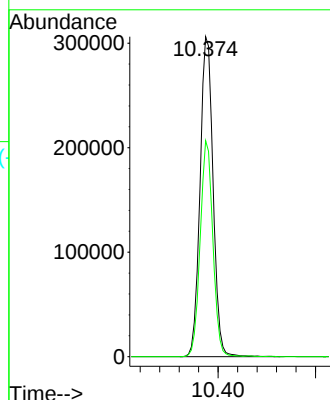

#52
Toluene
Concen: 2.015 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.006 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 92 Resp: 21105
Ion Ratio Lower Upper
92 100
91 176.5 138.6 207.8


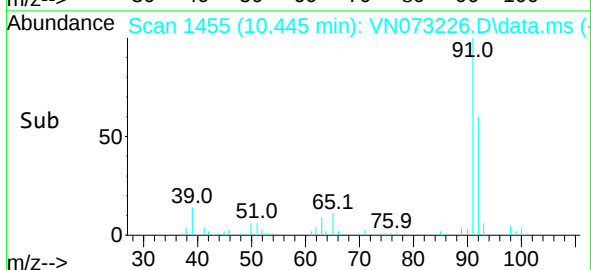
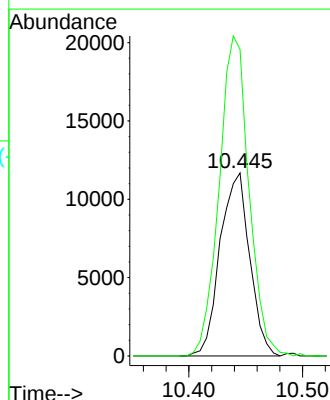
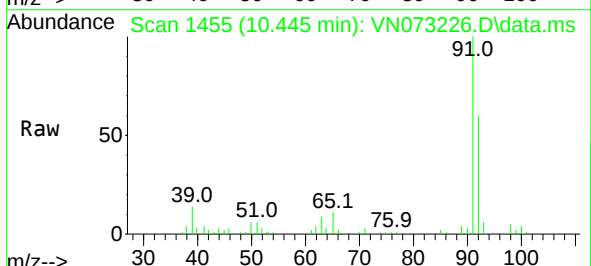




#62
4-Bromofluorobenzene
Concen: 54.998 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.001 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 95 Resp: 267966
Ion Ratio Lower Upper
95 100
174 73.8 0.0 167.6
176 71.9 0.0 163.4

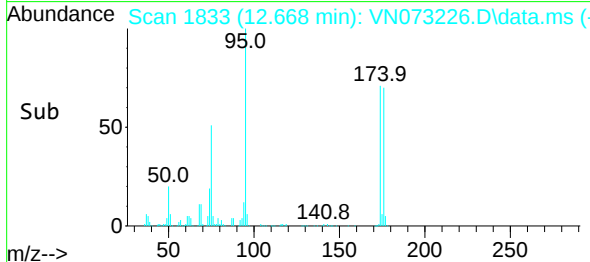

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1665
Delta R.T. 0.000 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 117 Resp: 510852
Ion Ratio Lower Upper
117 100
82 57.2 44.2 66.2
119 32.5 25.4 38.0

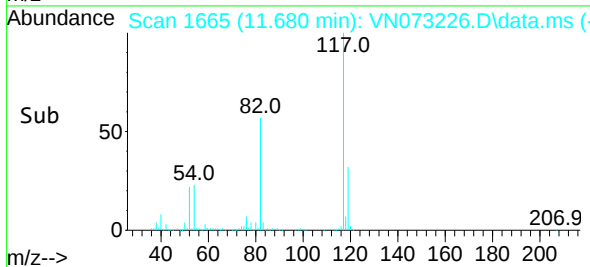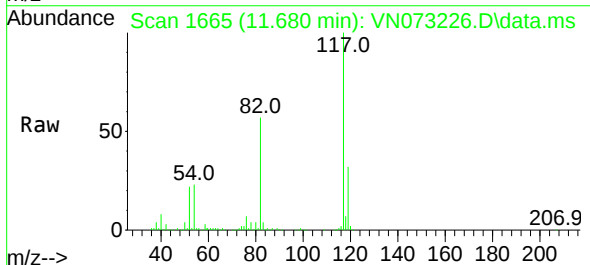



#67

Ethyl Benzene

Concen: 18.768 ug/l

RT: 11.780 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Instrument :

MSVOA_N

ClientSampleId :





MW-4

Tgt Ion: 91 Resp: 393664

Ion Ratio Lower Upper

91 100

106 32.0 24.9 37.3

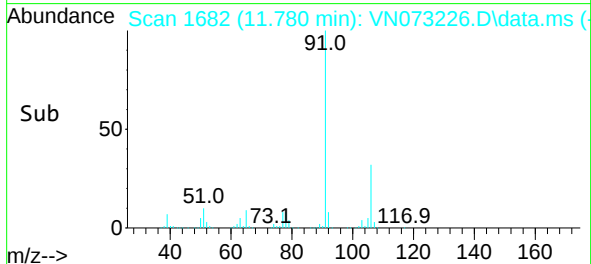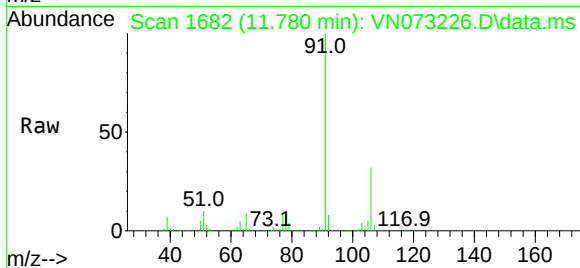

#68

m/p-Xylenes

Concen: 41.823 ug/l

RT: 11.892 min Scan# 1701

Delta R.T. -0.000 min

Lab File: VN073226.D




Acq: 29 Jun 2022 03:06


Tgt Ion: 106 Resp: 331072

Ion Ratio Lower Upper

106 100

91 204.1 158.9 238.3


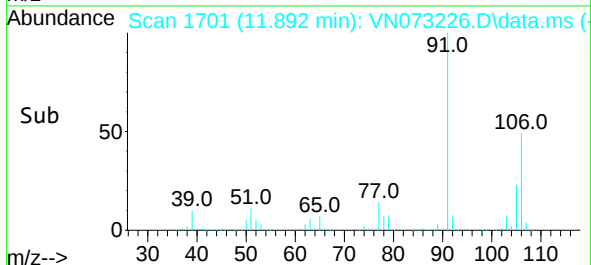

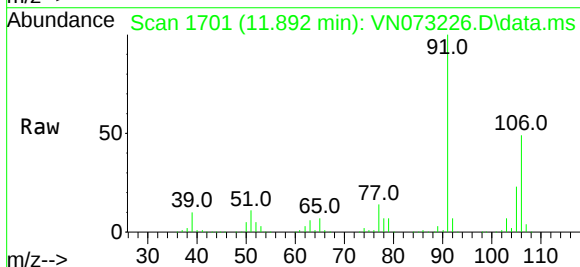




#69
o-Xylene
Concen: 9.746 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. -0.000 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:106 Resp: 78761
Ion Ratio Lower Upper
106 100
91 216.0 106.0 318.0

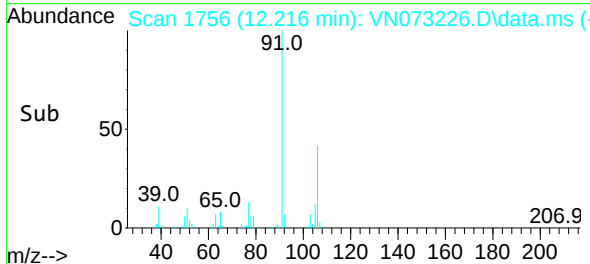

#70
Styrene
Concen: 0.334 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. -0.018 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion:104 Resp: 4164
Ion Ratio Lower Upper
104 100
78 279.5 39.5 59.3#
103 266.5 44.0 66.0#

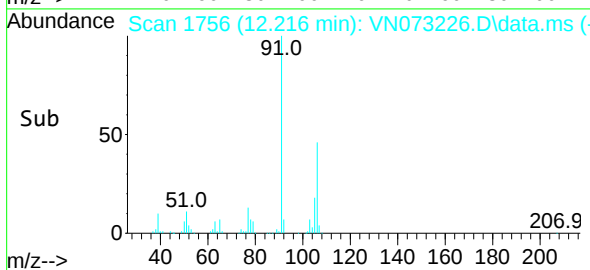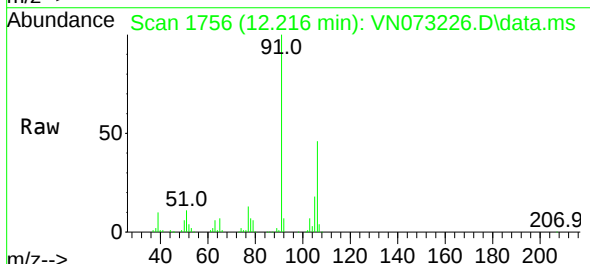



#71

Bromoform

Concen: 0.323 ug/l

RT: 12.668 min Scan# 1833

Delta R.T. 0.270 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Instrument :





MSVOA_N

ClientSampleId :

MW-4

Tgt Ion:173 Resp: 1005

Ion	Ratio	Lower	Upper
173	100		
175	1184.0	24.6	73.6#
254	0.0	0.1	0.1#

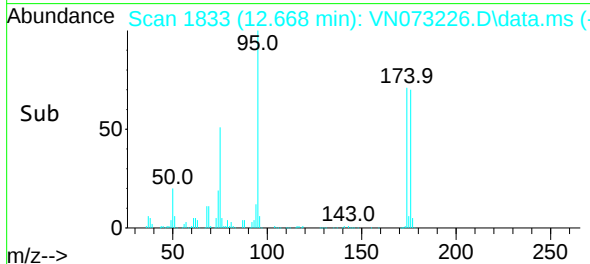

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.610 min Scan# 1993




Delta R.T. -0.000 min


Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Tgt Ion:152 Resp: 256882

Ion	Ratio	Lower	Upper
152	100		
115	62.1	28.9	86.7
150	156.3	0.0	356.2


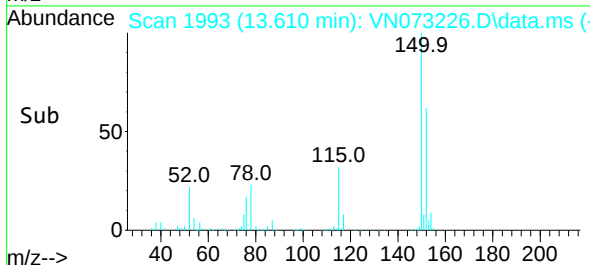

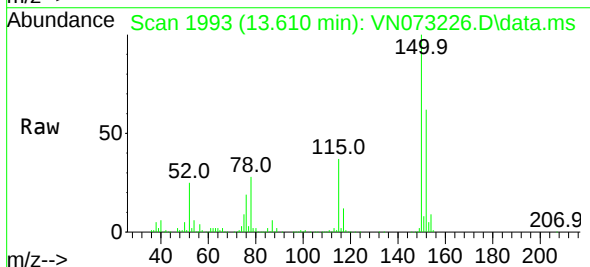




#73
Isopropylbenzene
Concen: 1.883 ug/l
RT: 12.515 min Scan# 1833
Delta R.T. -0.001 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:105 Resp: 41771
Ion Ratio Lower Upper
105 100
120 26.5 13.5 40.4

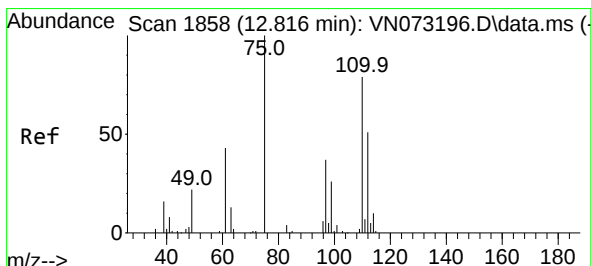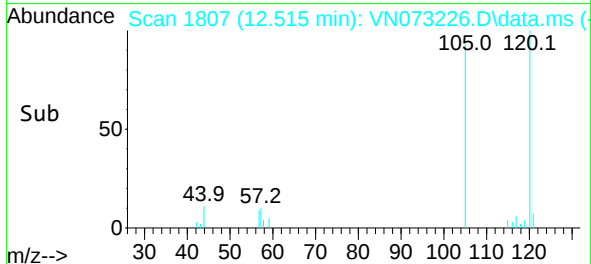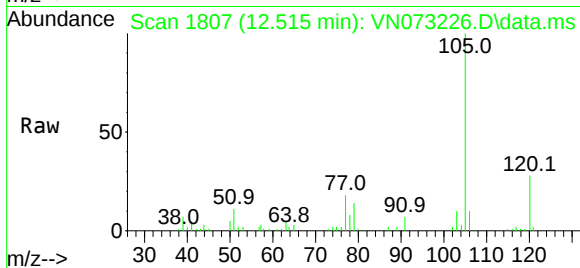

#76
1,2,3-Trichloropropane
Concen: 20.941 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.148 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 75 Resp: 140661
Ion Ratio Lower Upper
75 100
77 1.1 98.5 295.5#

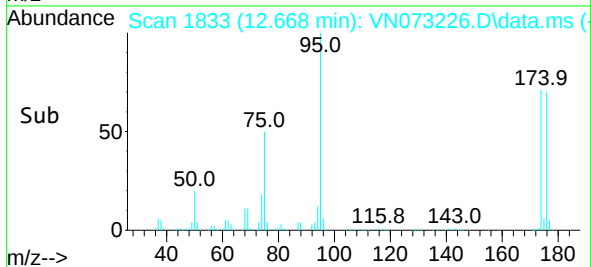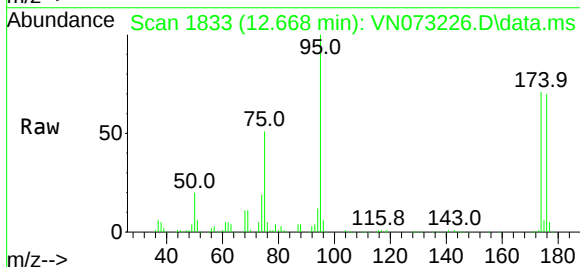



#78

n-propylbenzene

Concen: 3.729 ug/l

RT: 12.857 min Scan# 1865

Delta R.T. -0.000 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Instrument :

MSVOA_N

ClientSampleId :





MW-4

Tgt Ion: 91 Resp: 91904

Ion Ratio Lower Upper

91 100

120 21.9 11.9 35.5

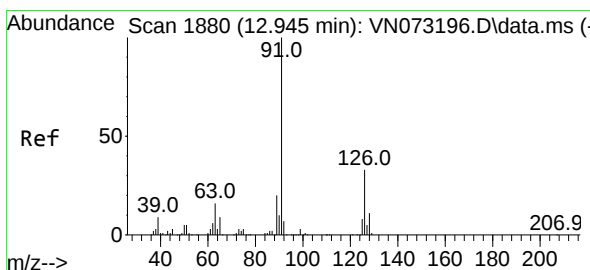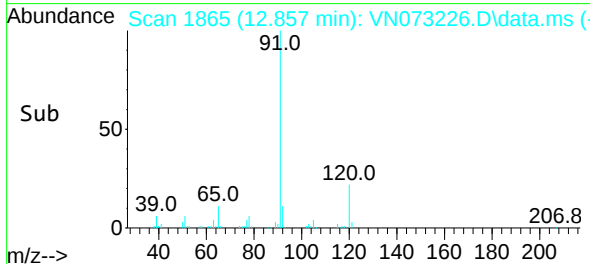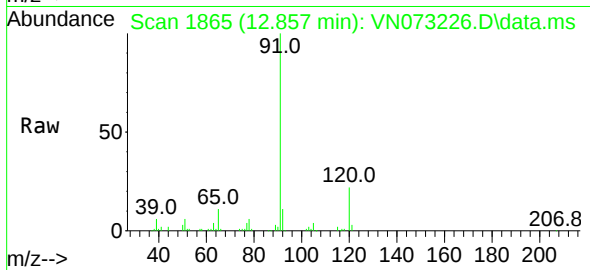

#79

2-Chlorotoluene

Concen: 1.710 ug/l

RT: 12.921 min Scan# 1876

Delta R.T. -0.024 min

Lab File: VN073226.D




Acq: 29 Jun 2022 03:06


Tgt Ion: 91 Resp: 26675

Ion Ratio Lower Upper

91 100

126 0.0 17.3 51.9#

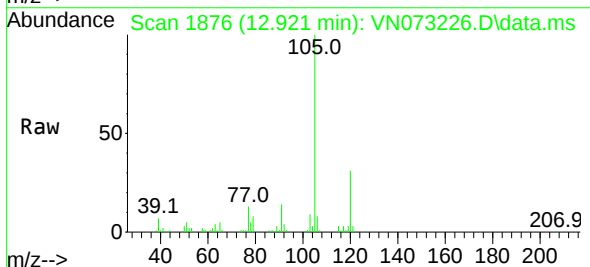



#80

1,3,5-Trimethylbenzene

Concen: 7.245 ug/l

RT: 12.998 min Scan# 1889

Delta R.T. -0.000 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06

Instrument :

MSVOA_N

ClientSampleId :





MW-4

Tgt Ion:105 Resp: 131003

Ion Ratio Lower Upper

105 100

120 48.8 24.9 74.7



#81

trans-1,4-Dichloro-2-butene

Concen: 57.430 ug/l

RT: 12.668 min Scan# 1833

Delta R.T. 0.105 min

Lab File: VN073226.D

Acq: 29 Jun 2022 03:06




Tgt Ion: 75 Resp: 140661


Ion Ratio Lower Upper

75 100

53 0.0 78.0 117.0#

89 0.0 37.2 55.8#


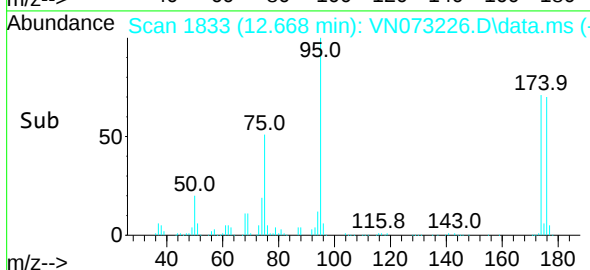






#82
4-Chlorotoluene
Concen: 0.988 ug/l
RT: 12.998 min Scan# 11
Delta R.T. -0.041 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion: 91 Resp: 14920
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

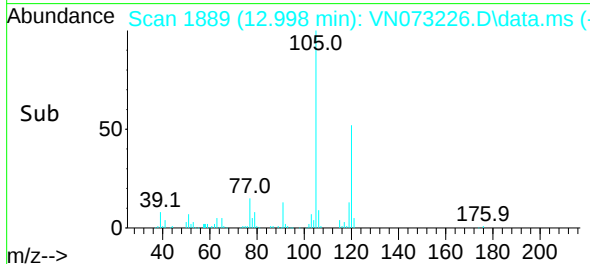

#83
tert-Butylbenzene
Concen: 3.882 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. 0.047 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 119 Resp: 62919
Ion Ratio Lower Upper
119 100
91 88.1 31.6 94.8
134 0.0 13.7 41.1#


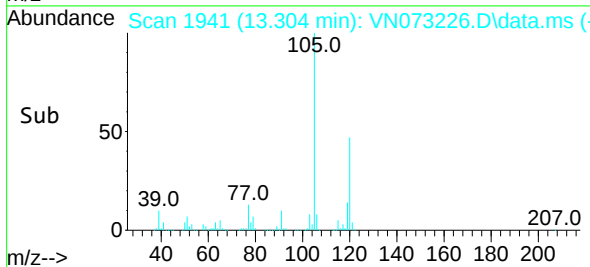

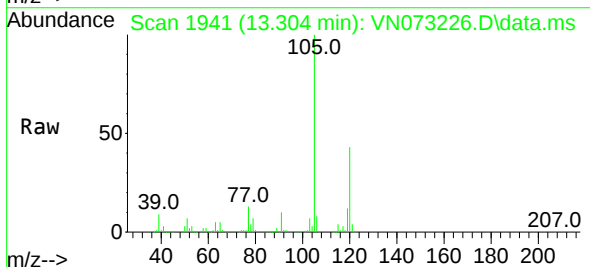


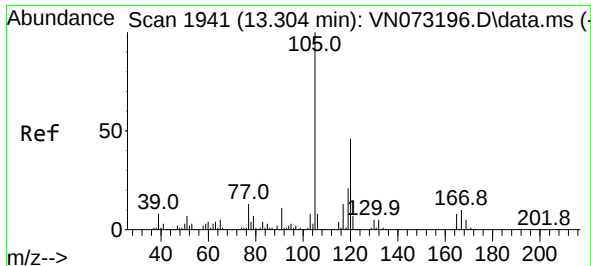

#84
 1,2,4-Trimethylbenzene
 Concen: 29.115 ug/l
 RT: 13.304 min Scan# 1941
 Delta R.T. -0.000 min
 Lab File: VN073226.D
 Acq: 29 Jun 2022 03:06




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-4


Tgt Ion:105 Resp: 525581
 Ion Ratio Lower Upper
 105 100
 120 45.0 23.3 69.8

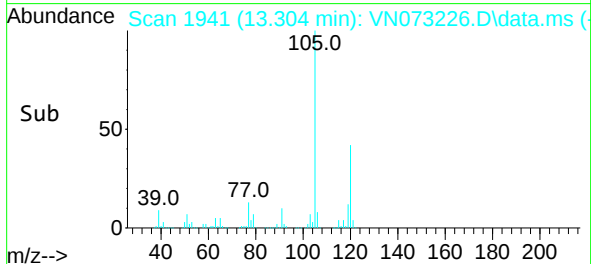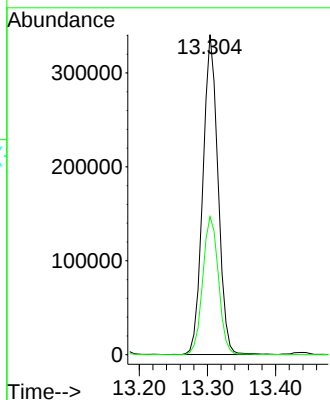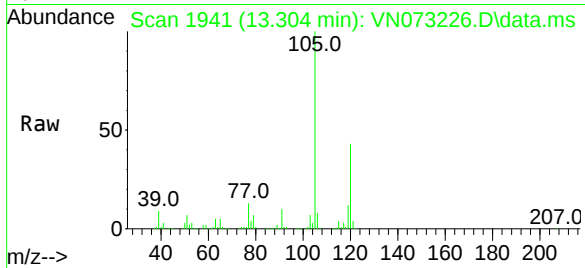

#85
 sec-Butylbenzene
 Concen: 24.147 ug/l
 RT: 13.304 min Scan# 1941
 Delta R.T. -0.135 min
 Lab File: VN073226.D
 Acq: 29 Jun 2022 03:06

Tgt Ion:105 Resp: 525581
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#


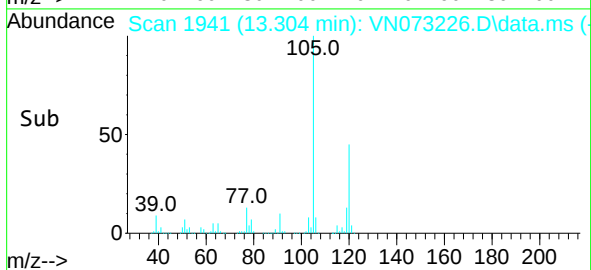
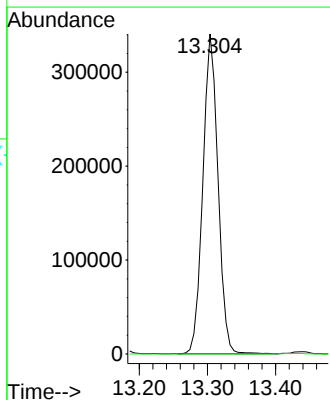
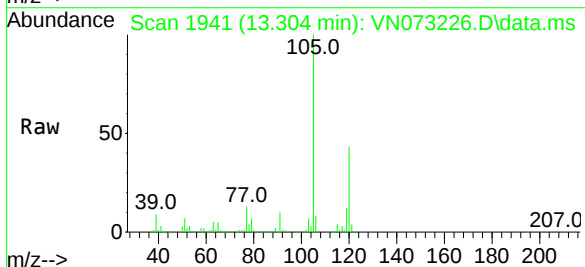




#86
p-Isopropyltoluene
Concen: 0.292 ug/l
RT: 13.498 min Scan# 1983
Delta R.T. -0.053 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06




Instrument :
MSVOA_N
ClientSampleId :
MW-4


Tgt Ion:119 Resp: 5143
Ion Ratio Lower Upper
119 100
134 25.9 13.3 39.8
91 0.0 11.3 33.9#

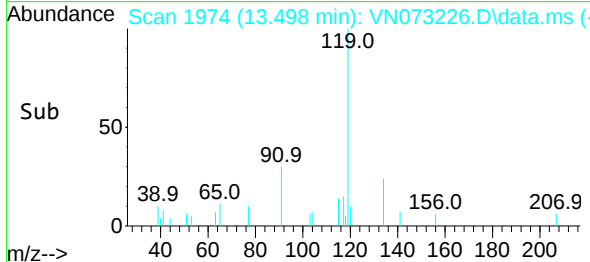

#89
n-Butylbenzene
Concen: 1.711 ug/l
RT: 13.810 min Scan# 2027
Delta R.T. -0.070 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion: 91 Resp: 25064
Ion Ratio Lower Upper
91 100
92 15.0 26.9 80.7#
134 13.4 13.6 40.8#


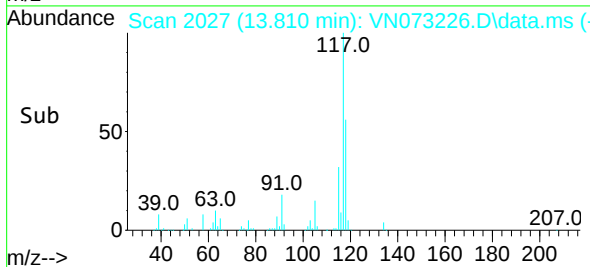

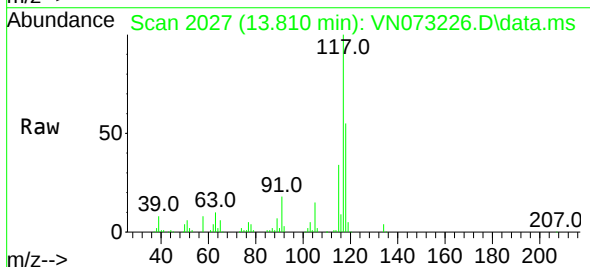




#90
Hexachloroethane
Concen: 1.204 ug/l
RT: 14.151 min Scan# 2085
Delta R.T. 0.006 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Instrument :
MSVOA_N
ClientSampleId :
MW-4

Tgt Ion:117 Resp: 3946
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

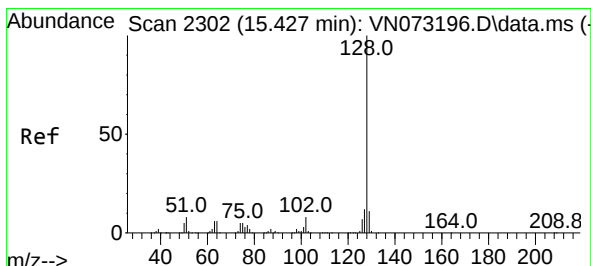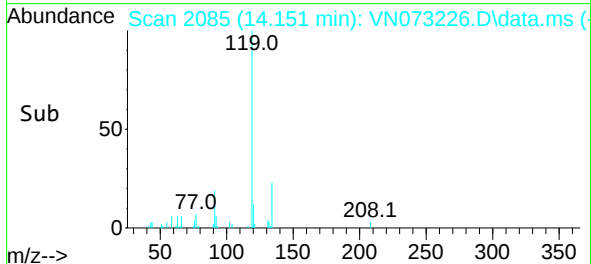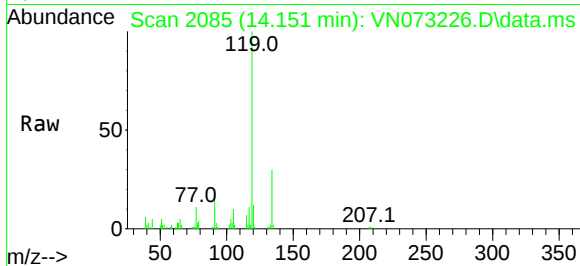

#95
Naphthalene
Concen: 6.493 ug/l
RT: 15.433 min Scan# 2303
Delta R.T. 0.006 min
Lab File: VN073226.D
Acq: 29 Jun 2022 03:06

Tgt Ion:128 Resp: 128553
Ion Ratio Lower Upper
128 100
127 12.5 10.3 15.5
129 11.4 8.6 13.0

