
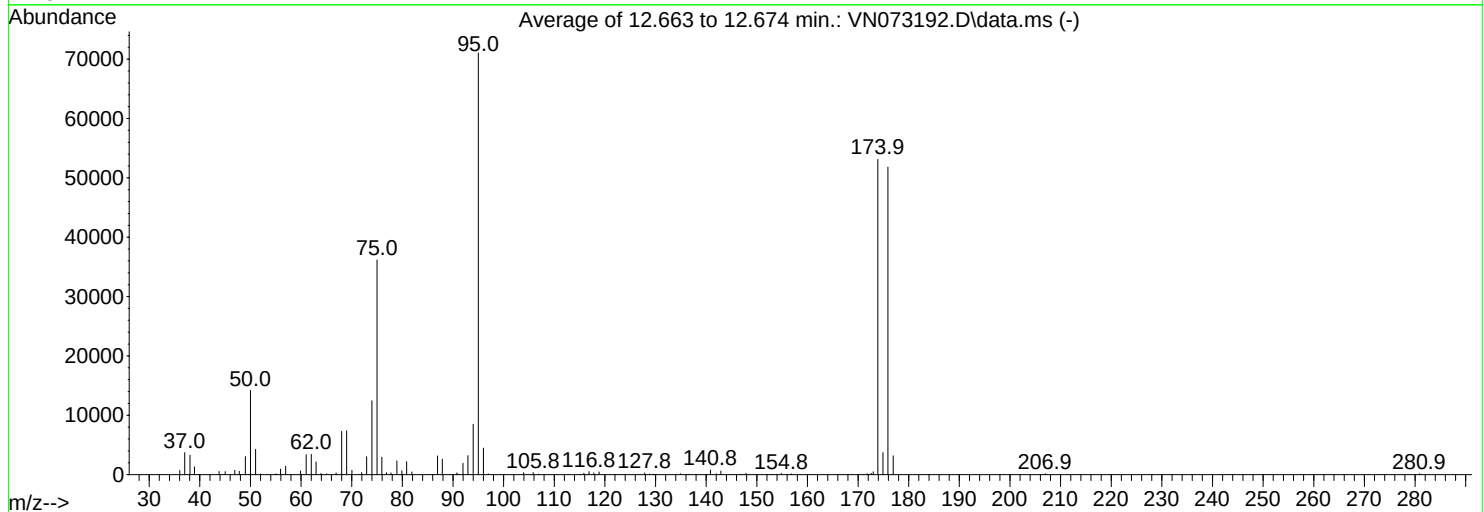


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062822\
 Data File : VN073192.D
 Acq On : 28 Jun 2022 08:58
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Title : SW846 8260
 Last Update : Wed Jun 29 01:54:03 2022

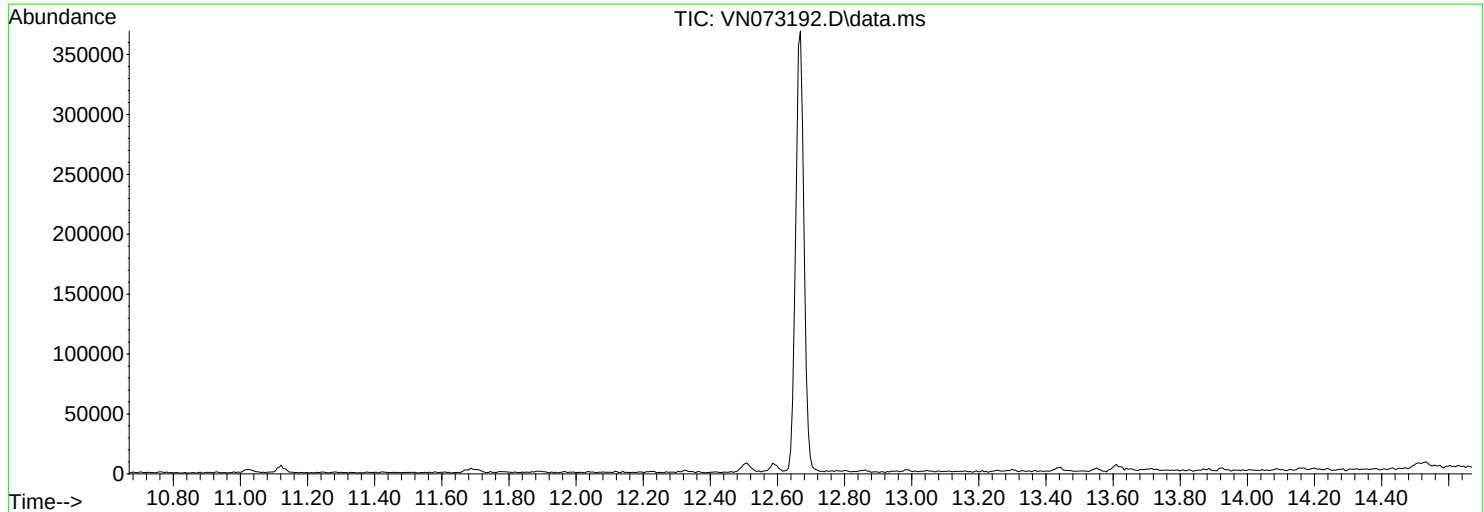

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	14207	PASS
75	95	30	60	50.9	36179	PASS
95	95	100	100	100.0	71061	PASS
96	95	5	9	6.3	4476	PASS
173	174	0.00	2	0.9	483	PASS
174	95	50	100	74.7	53104	PASS
175	174	5	9	7.0	3724	PASS
176	174	95	101	97.6	51803	PASS
177	176	5	9	6.2	3192	PASS