

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062823\
 Data File : VN078439.D
 Acq On : 28 Jun 2023 14:15
 Operator : JC\MD
 Sample : 03429-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-COMP-0627

Quant Time: Jun 29 05:20:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 07 05:05:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	481042	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	887944	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	844564	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	269462	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.589	65	322686	50.312	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 100.620%			
35) Dibromofluoromethane	8.177	113	311895	55.553	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 111.100%			
50) Toluene-d8	10.571	98	1070098	49.441	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 98.880%			
62) 4-Bromofluorobenzene	12.853	95	350824	52.140	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 104.280%			
Target Compounds						Qvalue
3) Chloromethane	2.365	50	1336	Below Cal	#	42
5) Bromomethane	2.971	94	2589	0.481	ug/l	93
6) Chloroethane	3.130	64	1151	0.237	ug/l #	43
11) Tert butyl alcohol	5.530	59	4235	4.782	ug/l #	84
13) Acrolein	4.201	56	385	0.394	ug/l #	16
16) Acetone	4.442	43	293938	159.220	ug/l	98
18) Methyl Acetate	5.048	43	4344	0.511	ug/l #	60
20) Methylene Chloride	5.295	84	23299	3.819	ug/l	93
25) 2-Butanone	7.494	43	154975	54.589	ug/l #	87
29) Tetrahydrofuran	7.847	42	5198	2.739	ug/l #	33
31) Cyclohexane	8.224	56	11621	1.412	ug/l #	35
36) 1,1-Dichloropropene	8.230	75	40756	5.061	ug/l #	48
37) Ethyl Acetate	7.571	43	76352	12.137	ug/l	98
38) Carbon Tetrachloride	8.230	117	53380	6.278	ug/l #	16
41) Methacrylonitrile	7.847	41	3368	0.988	ug/l #	37
42) 1,2-Dichloroethane	8.689	62	2072	0.251	ug/l #	73
43) Isopropyl Acetate	8.694	43	320078	26.603	ug/l #	85
48) Methyl methacrylate	9.671	41	8025	1.589	ug/l #	3
49) 1,4-Dioxane	9.712	88	206	1.941	ug/l #	30
51) 4-Methyl-2-Pentanone	10.453	43	590379	93.184	ug/l	92
54) cis-1,3-Dichloropropene	10.365	75	118659	12.594	ug/l #	68
57) 1,3-Dichloropropane	11.212	76	14032	1.448	ug/l #	42
59) 2-Hexanone	11.177	43	259055	58.723	ug/l #	19
71) Bromoform	12.853	173	1979	0.461	ug/l #	1
74) N-amyl acetate	12.500	43	2468	0.294	ug/l #	46
75) 1,1,2,2-Tetrachloroethane	12.941	83	171	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.853	75	184667	28.989	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	184667	89.064	ug/l #	15
94) Hexachlorobutadiene	15.506	225	61	Below Cal	#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062823\
Data File : VN078439.D
Acq On : 28 Jun 2023 14:15
Operator : JC\MD
Sample : 03429-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627

Quant Time: Jun 29 05:20:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 07 05:05:00 2023
Response via : Initial Calibration

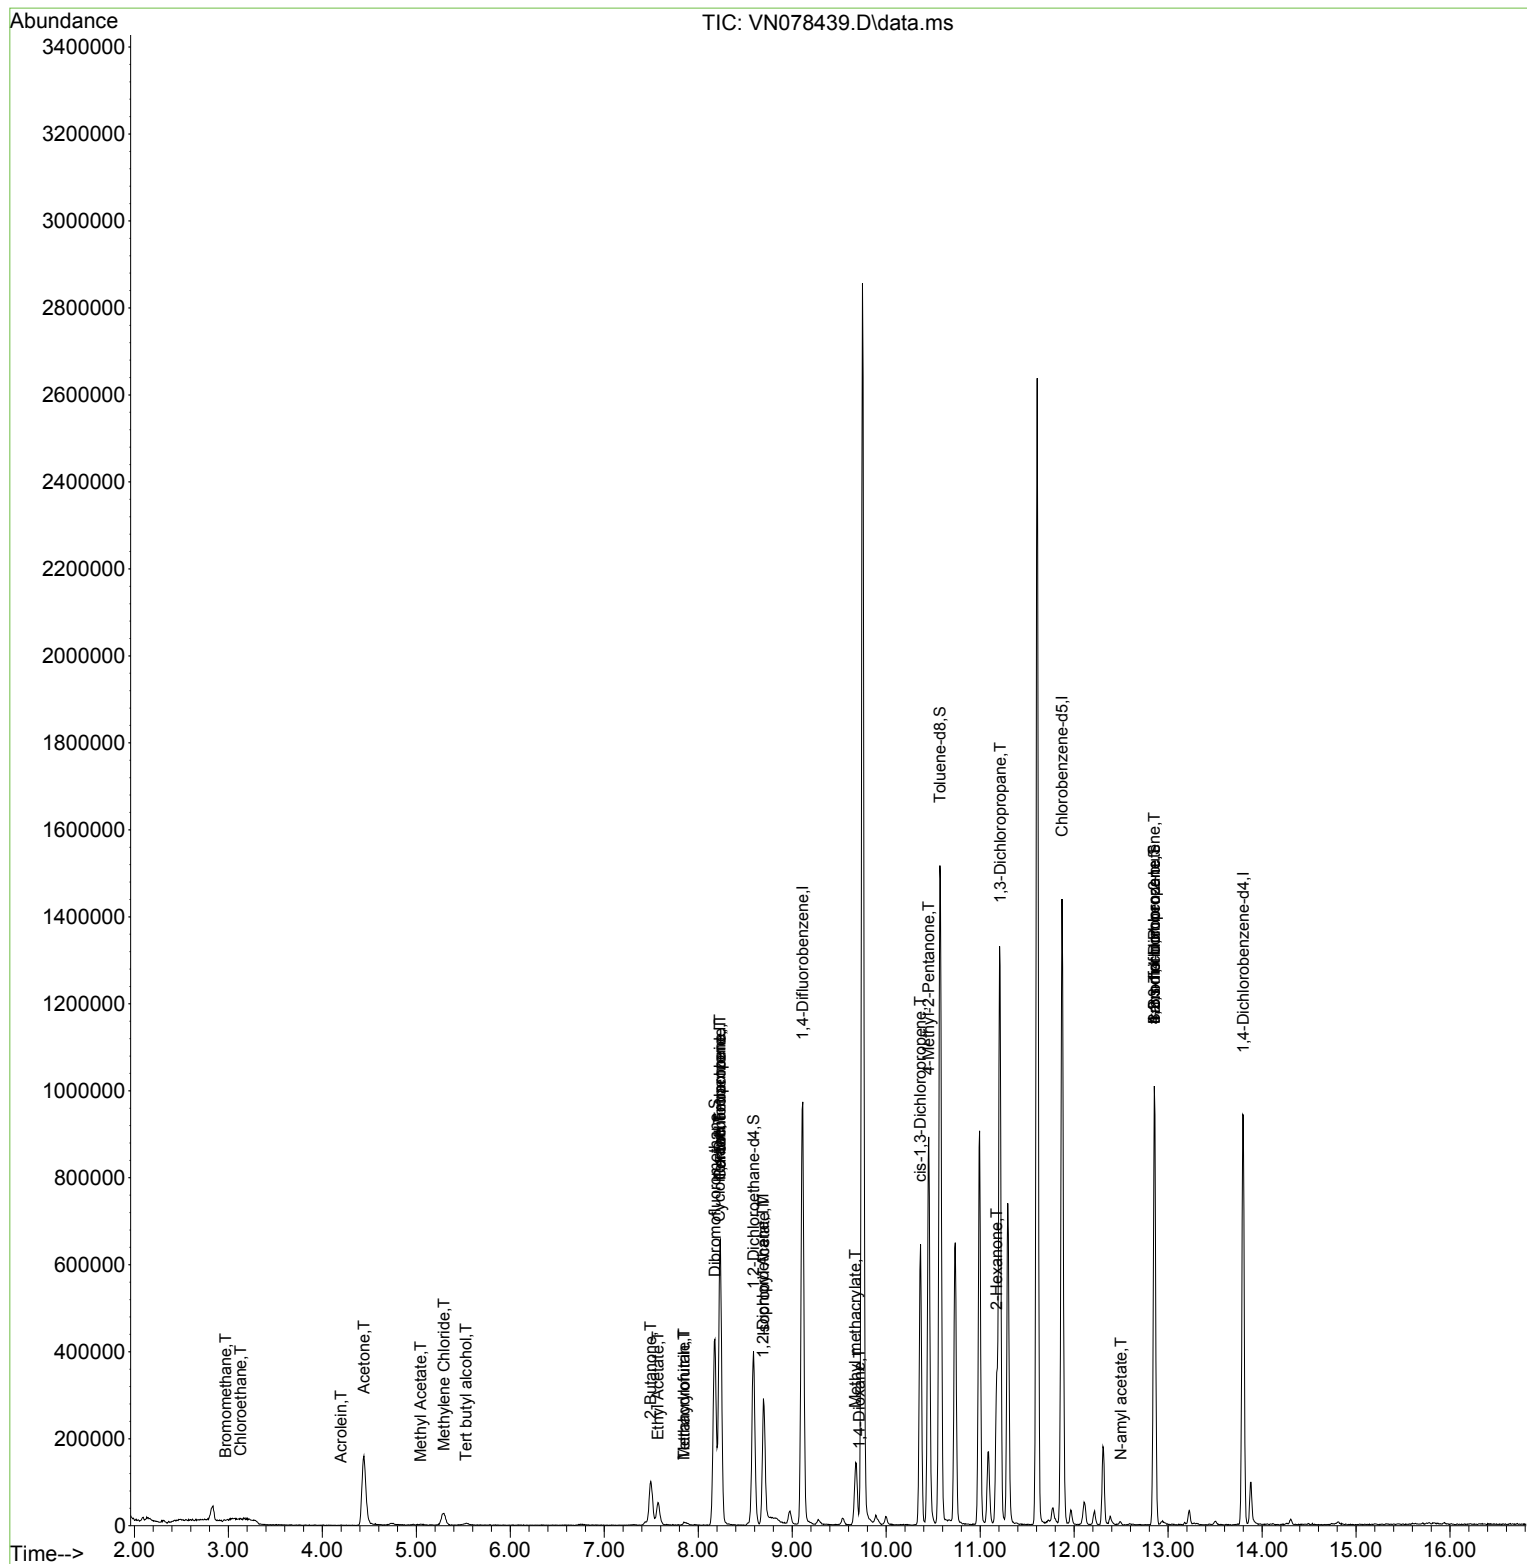



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 11

Delta R.T. -0.005 min

Lab File: VN078439.D

Acq: 28 Jun 2023 14:15

Instrument :

MSVOA_N

ClientSampleId :





SB-COMP-0627

Tgt Ion:168 Resp: 481042

Ion Ratio Lower Upper

168 100

99 59.8 53.0 79.6

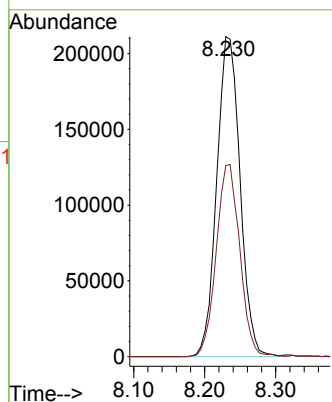

#3

Chloromethane

Concen: Below Cal

RT: 2.365 min Scan# 70

Delta R.T. -0.006 min

Lab File: VN078439.D




Acq: 28 Jun 2023 14:15


Tgt Ion: 50 Resp: 1336

Ion Ratio Lower Upper

50 100

52 0.0 26.5 39.7#


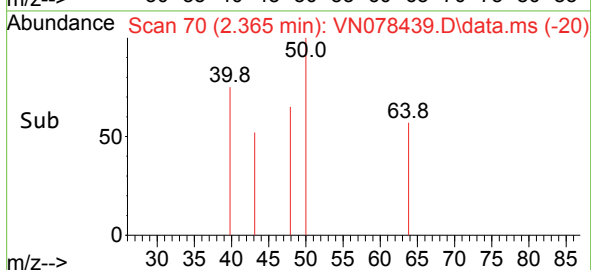






#5
Bromomethane
Concen: 0.481 ug/l
RT: 2.971 min Scan# 11
Delta R.T. 0.018 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 94 Resp: 2589
Ion Ratio Lower Upper
94 100
96 84.7 73.1 109.7

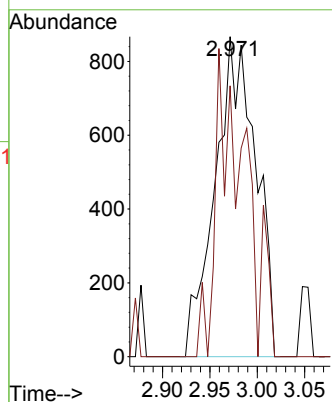

#6
Chloroethane
Concen: 0.237 ug/l
RT: 3.130 min Scan# 200
Delta R.T. 0.006 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion: 64 Resp: 1151
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#



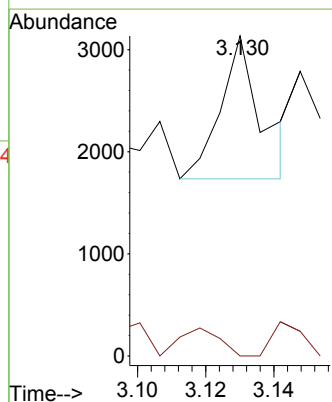





#11
Tert butyl alcohol
Concen: 4.782 ug/l
RT: 5.530 min Scan# 609
Delta R.T. -0.006 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 59 Resp: 4235
Ion Ratio Lower Upper
59 100
57 4.3 8.2 12.4#

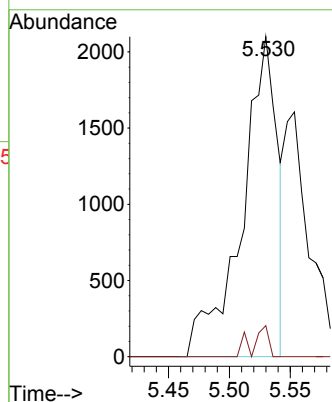

#13
Acrolein
Concen: 0.394 ug/l
RT: 4.201 min Scan# 382
Delta R.T. 0.012 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion: 56 Resp: 385
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#


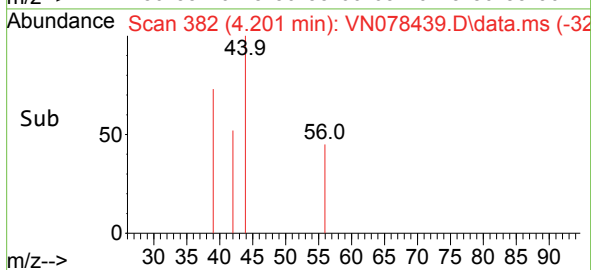
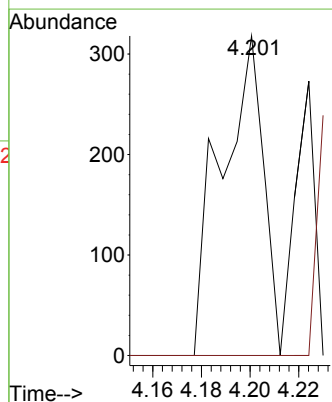





#16
Acetone
Concen: 159.220 ug/l
RT: 4.442 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 43 Resp: 293938
Ion Ratio Lower Upper
43 100
58 36.0 28.0 42.0

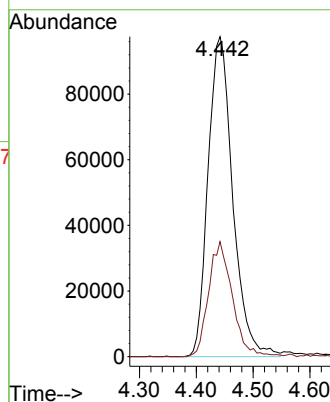

#18
Methyl Acetate
Concen: 0.511 ug/l
RT: 5.048 min Scan# 526
Delta R.T. 0.012 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15


Tgt Ion: 43 Resp: 4344
Ion Ratio Lower Upper
43 100
74 10.0 26.2 39.4#

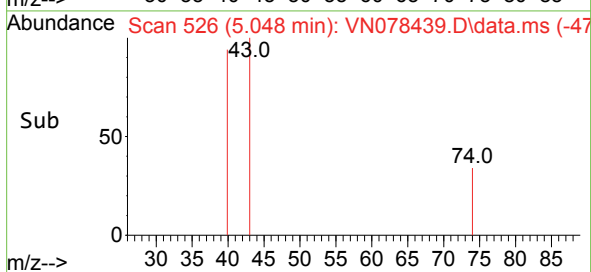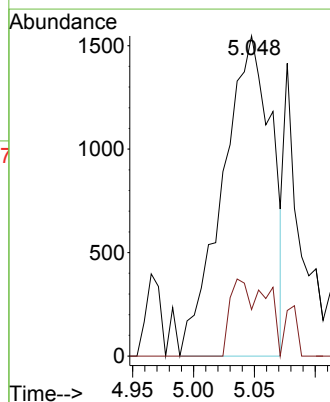






#20
Methylene Chloride
Concen: 3.819 ug/l
RT: 5.295 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627







Tgt Ion:	84	Resp:	23299
Ion	Ratio	Lower	Upper
84	100		
49	107.1	79.7	119.5
51	28.4	25.2	37.8
86	71.4	53.3	79.9



#25
2-Butanone
Concen: 54.589 ug/l
RT: 7.494 min Scan# 942
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion:	43	Resp:	154975
Ion	Ratio	Lower	Upper
43	100		
72	29.8	30.2	45.2#

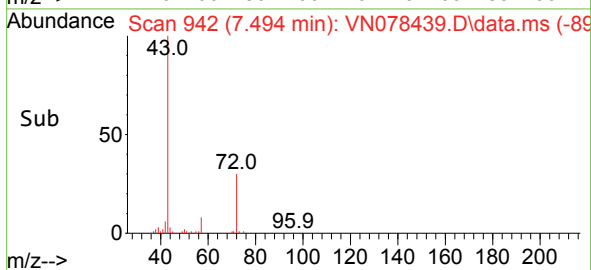



#29

Tetrahydrofuran

Concen: 2.739 ug/l

RT: 7.847 min Scan# 1002

Delta R.T. 0.000 min

Lab File: VN078439.D

Acq: 28 Jun 2023 14:15

Instrument :

MSVOA_N

ClientSampleId :

SB-COMP-0627





Tgt Ion: 42 Resp: 5198

Ion Ratio Lower Upper

42 100

72 0.0 49.8 74.6#

71 19.9 47.4 71.2#



#31

Cyclohexane

Concen: 1.412 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.041 min

Lab File: VN078439.D

Acq: 28 Jun 2023 14:15




Tgt Ion: 56 Resp: 11621


Ion Ratio Lower Upper

56 100

69 112.8 26.8 40.2#

84 143.2 81.8 122.6#









#33
1,2-Dichloroethane-d4
Concen: 50.312 ug/l
RT: 8.589 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 65 Resp: 322686
Ion Ratio Lower Upper
65 100
67 52.5 0.0 106.6

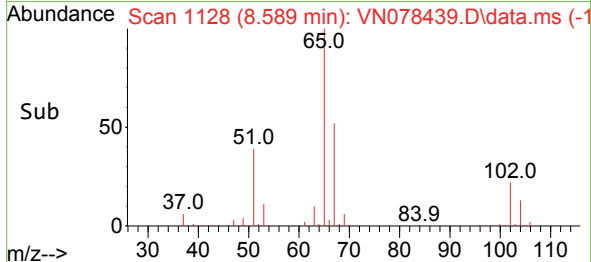

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.112 min Scan# 1217
Delta R.T. 0.006 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion: 114 Resp: 887944
Ion Ratio Lower Upper
114 100
63 18.2 0.0 36.4
88 14.9 0.0 30.6




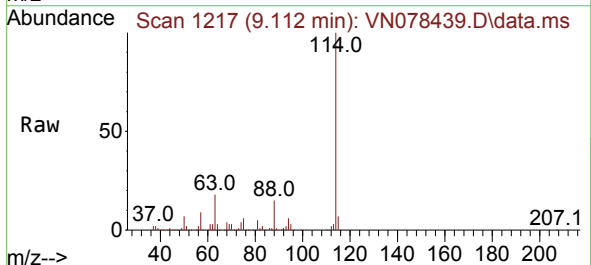




#35
 Dibromofluoromethane
 Concen: 55.553 ug/l
 RT: 8.177 min Scan# 1058
 Delta R.T. 0.000 min
 Lab File: VN078439.D
 Acq: 28 Jun 2023 14:15




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-COMP-0627


Tgt Ion:113 Resp: 311895
 Ion Ratio Lower Upper
 113 100
 111 103.8 82.6 123.8
 192 16.8 12.7 19.1

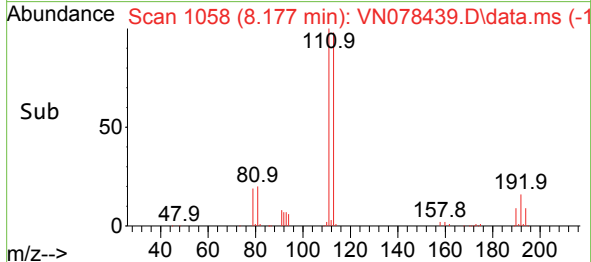

#36
 1,1-Dichloropropene
 Concen: 5.061 ug/l
 RT: 8.230 min Scan# 1067
 Delta R.T. -0.147 min
 Lab File: VN078439.D
 Acq: 28 Jun 2023 14:15

Tgt Ion: 75 Resp: 40756
 Ion Ratio Lower Upper
 75 100
 110 9.4 19.1 57.3#
 77 0.0 25.0 37.4#


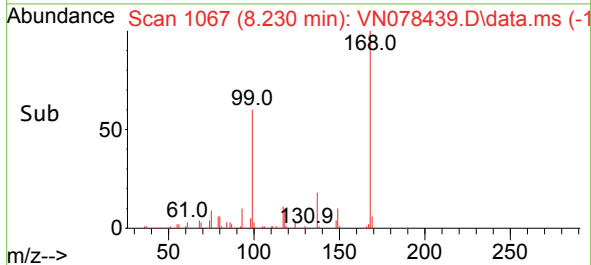






#37
Ethyl Acetate
Concen: 12.137 ug/l
RT: 7.571 min Scan# 91
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 43 Resp: 76352
Ion Ratio Lower Upper
43 100
61 16.2 13.2 19.8
70 12.4 11.3 16.9



#38
Carbon Tetrachloride
Concen: 6.278 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.141 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion: 117 Resp: 53380
Ion Ratio Lower Upper
117 100
119 5.0 77.3 115.9#
121 0.0 23.3 34.9#


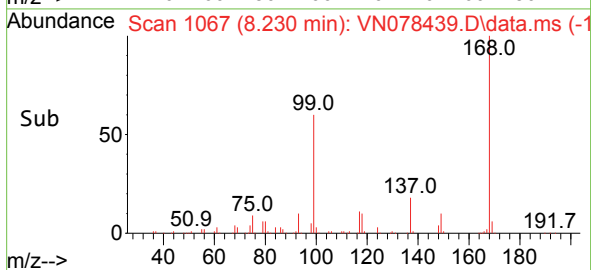






#41
Methacrylonitrile
Concen: 0.988 ug/l
RT: 7.847 min Scan# 1100
Delta R.T. 0.065 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion:	41	Resp:	3368
Ion	Ratio	Lower	Upper
41	100		
39	52.8	42.6	64.0
67	0.0	77.5	116.3#
52	0.0	28.9	43.3#

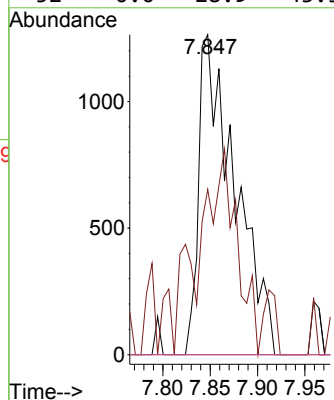

#42
1,2-Dichloroethane
Concen: 0.251 ug/l
RT: 8.689 min Scan# 1145
Delta R.T. 0.012 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion:	62	Resp:	2072
Ion	Ratio	Lower	Upper
62	100		
98	0.0	0.0	19.8



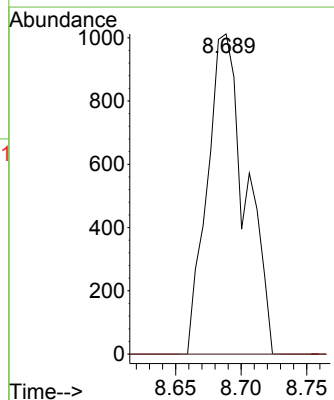



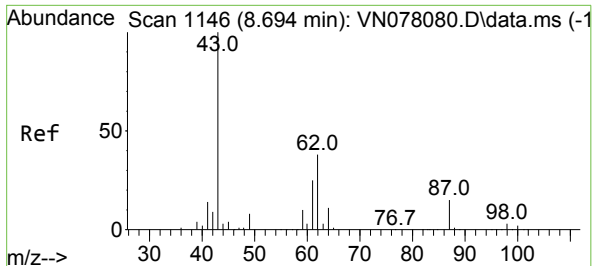

#43
Isopropyl Acetate
Concen: 26.603 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 43 Resp: 320078
Ion Ratio Lower Upper
43 100
61 20.0 24.7 37.1#
87 14.8 14.6 21.8

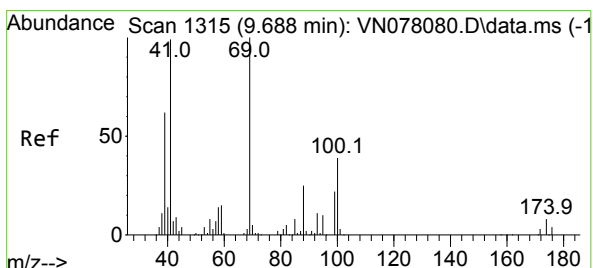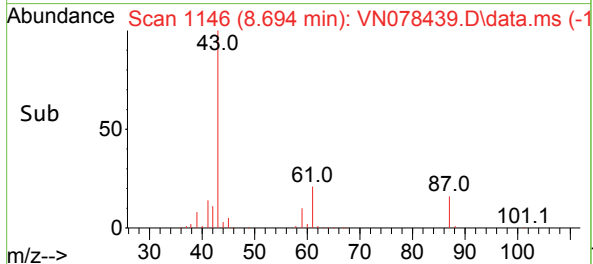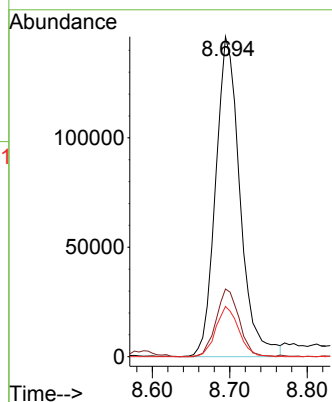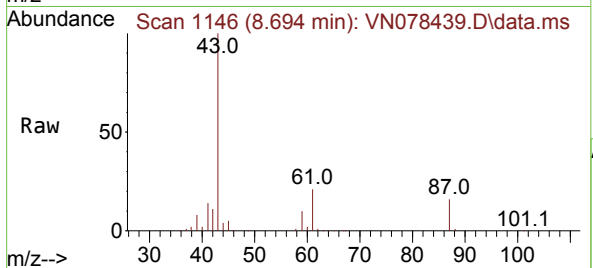

#48
Methyl methacrylate
Concen: 1.589 ug/l
RT: 9.671 min Scan# 1312
Delta R.T. -0.017 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion: 41 Resp: 8025
Ion Ratio Lower Upper
41 100
69 0.8 90.4 135.6#
39 0.0 54.6 81.8#


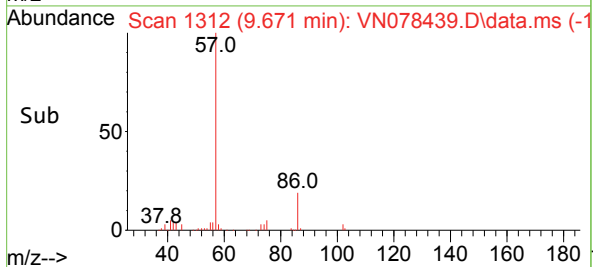
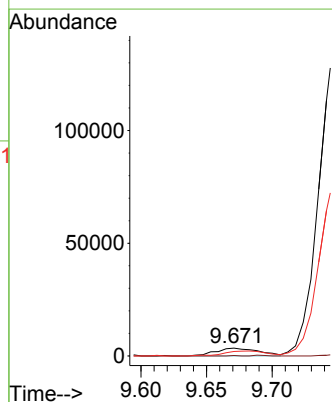
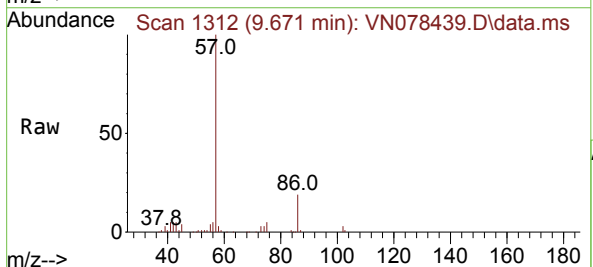




#49
1,4-Dioxane
Concen: 1.941 ug/l
RT: 9.712 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 88 Resp: 206
Ion Ratio Lower Upper
88 100
43 0.0 17.0 25.6#
58 0.0 47.0 70.4#

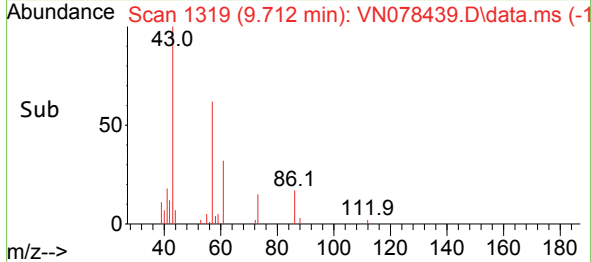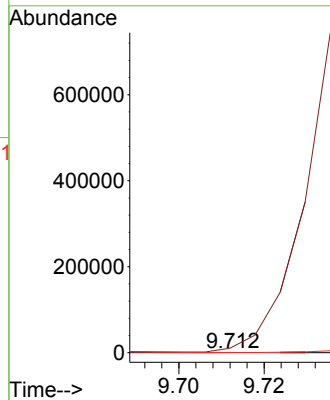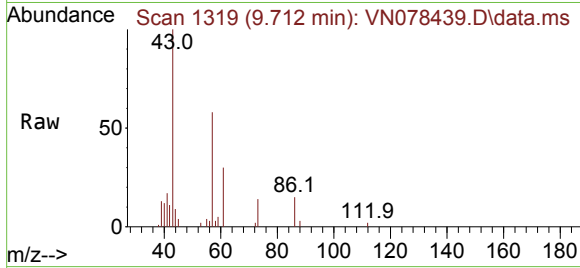

#50
Toluene-d8
Concen: 49.441 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15


Tgt Ion: 98 Resp: 1070098
Ion Ratio Lower Upper
98 100
100 64.0 52.0 78.0

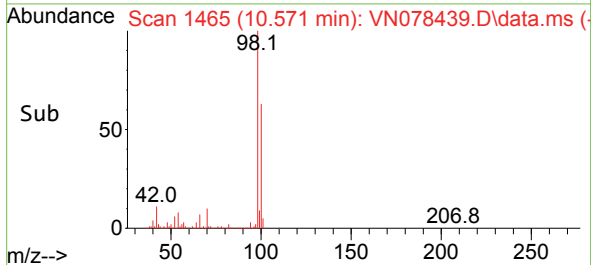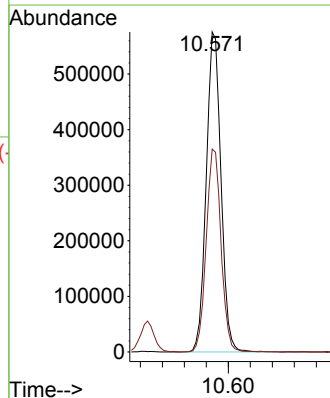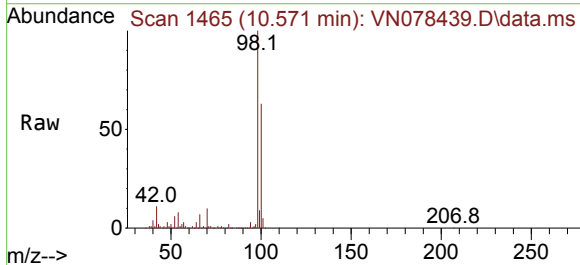



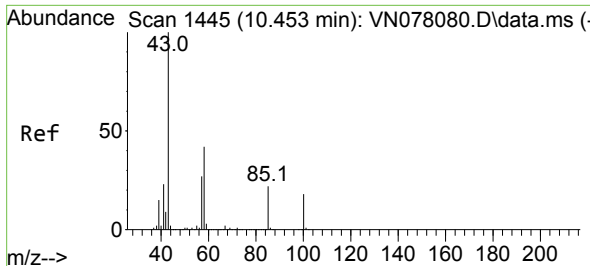


#51
4-Methyl-2-Pentanone
Concen: 93.184 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627



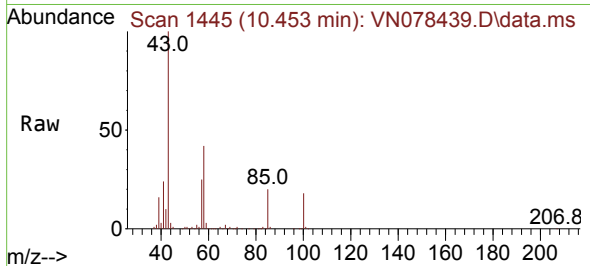



Tgt Ion: 43 Resp: 590379
Ion Ratio Lower Upper
43 100
58 40.2 36.6 54.8

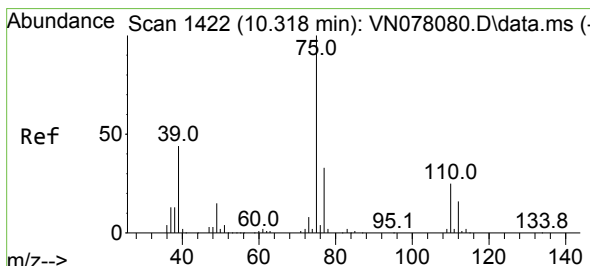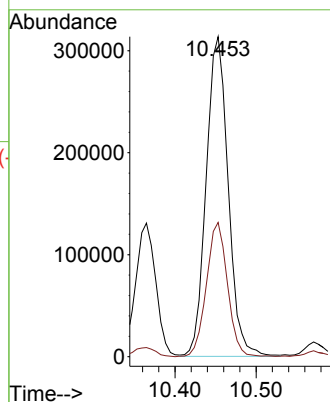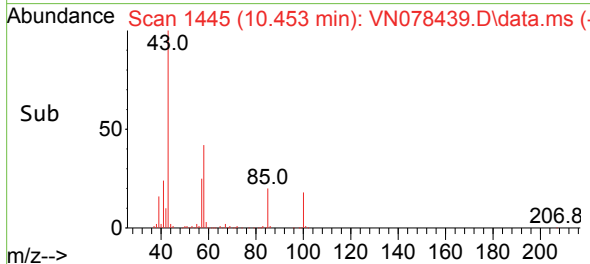

#54
cis-1,3-Dichloropropene
Concen: 12.594 ug/l
RT: 10.365 min Scan# 1430
Delta R.T. 0.047 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion: 75 Resp: 118659
Ion Ratio Lower Upper
75 100
77 0.7 26.1 39.1#
39 32.4 31.6 47.4

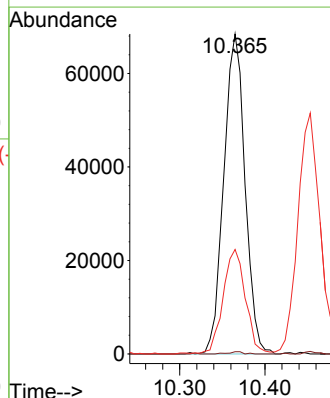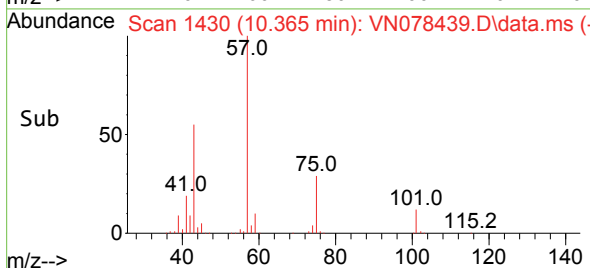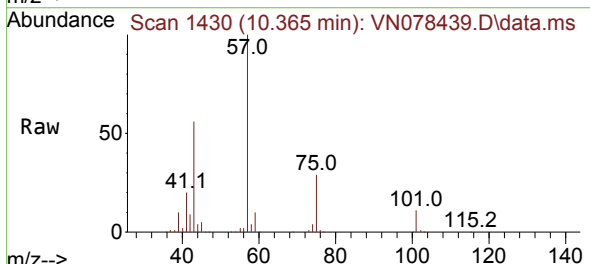

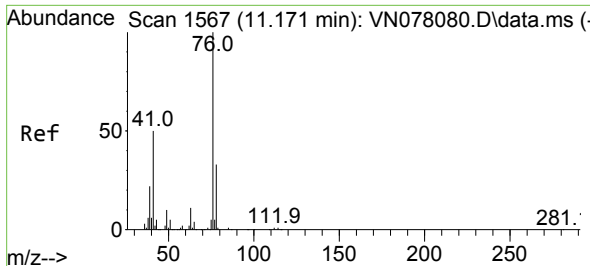

#57

1,3-Dichloropropane

Concen: 1.448 ug/l

RT: 11.212 min Scan# 11

Delta R.T. 0.041 min

Lab File: VN078439.D

Acq: 28 Jun 2023 14:15

Instrument :

MSVOA_N

ClientSampleId :





SB-COMP-0627

Tgt Ion: 76 Resp: 14032

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

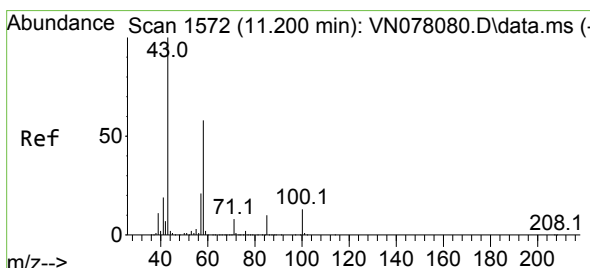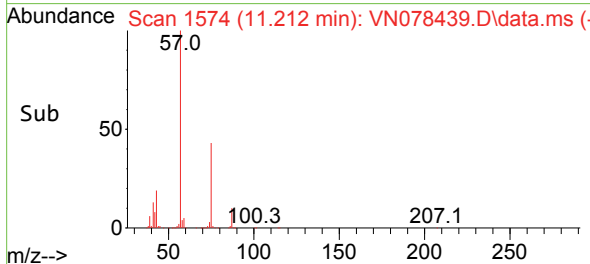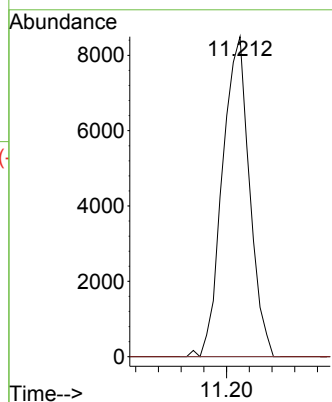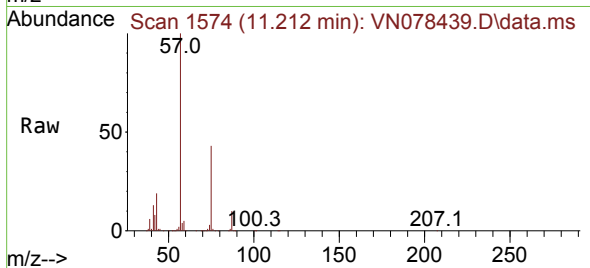

#59

2-Hexanone

Concen: 58.723 ug/l

RT: 11.177 min Scan# 1568

Delta R.T. -0.023 min

Lab File: VN078439.D




Acq: 28 Jun 2023 14:15


Tgt Ion: 43 Resp: 259055

Ion Ratio Lower Upper

43 100

58 0.0 31.7 95.1#


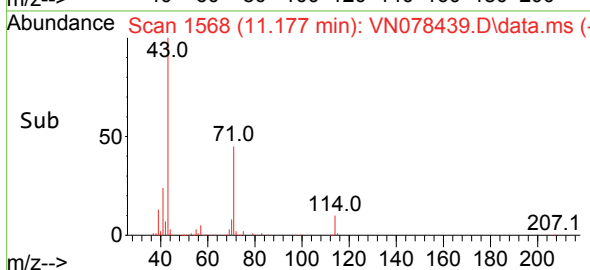

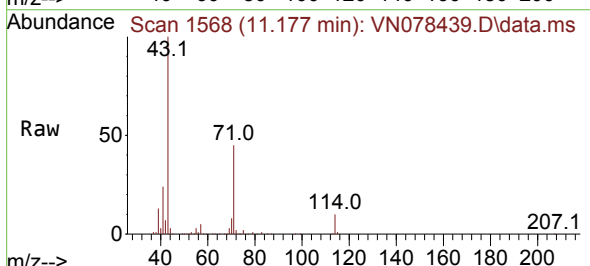


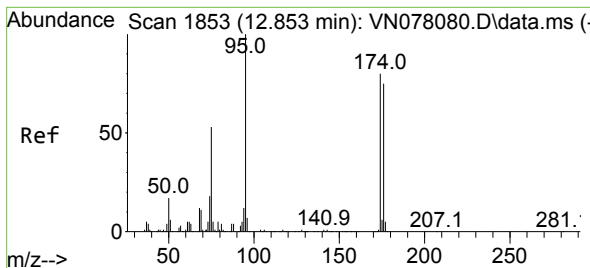

#62
4-Bromofluorobenzene
Concen: 52.140 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 95 Resp: 350824
Ion Ratio Lower Upper
95 100
174 76.7 0.0 143.8
176 72.3 0.0 135.8

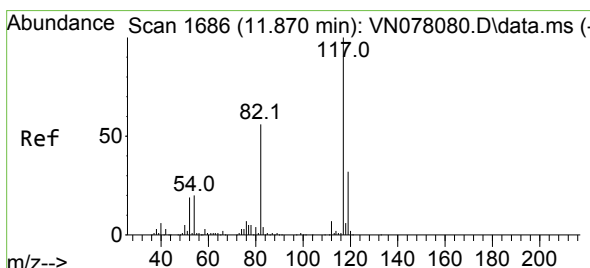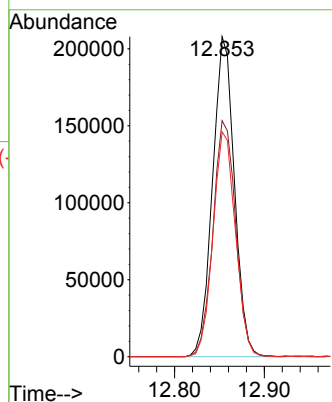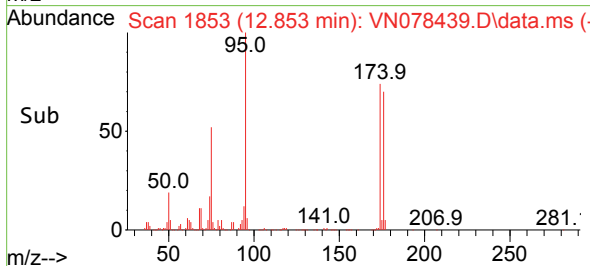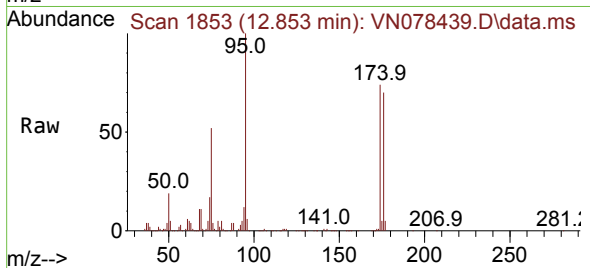

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion: 117 Resp: 844564
Ion Ratio Lower Upper
117 100
82 55.0 44.0 66.0
119 32.2 25.6 38.4



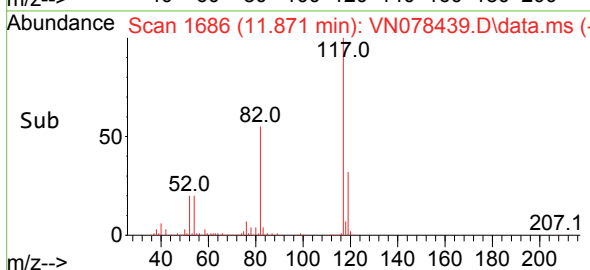
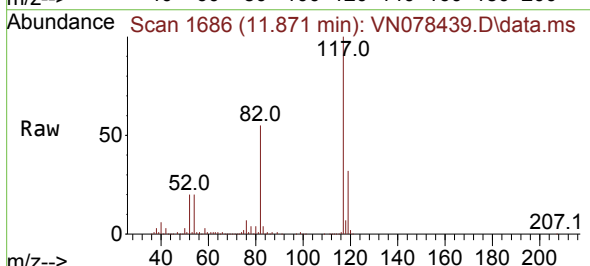


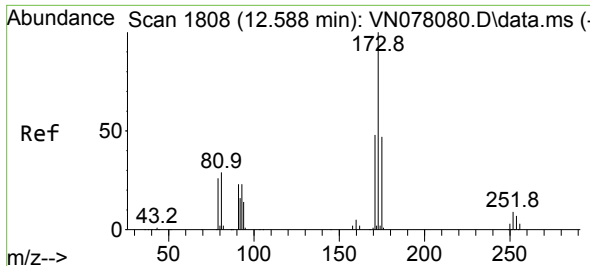

#71
Bromoform
Concen: 0.461 ug/l
RT: 12.853 min Scan# 1808
Delta R.T. 0.265 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion:173 Resp: 1979
Ion Ratio Lower Upper
173 100
175 903.3 24.3 73.0#
254 0.0 0.0 0.0

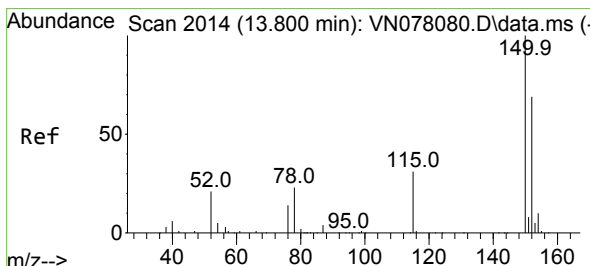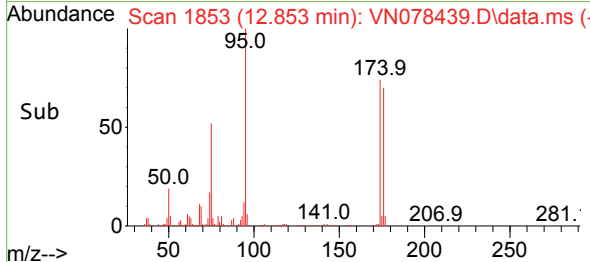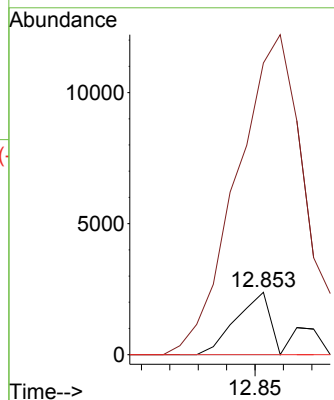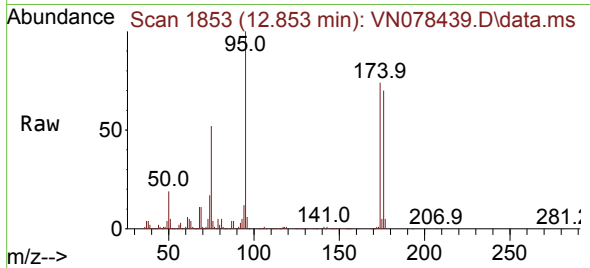

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion:152 Resp: 269462
Ion Ratio Lower Upper
152 100
115 59.0 32.3 96.8
150 153.8 0.0 355.8


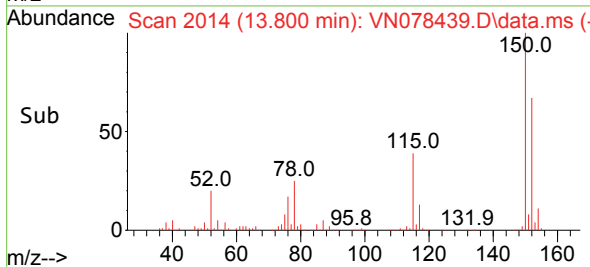
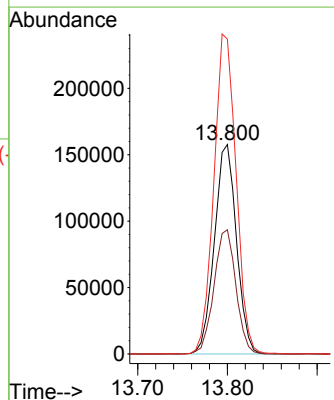
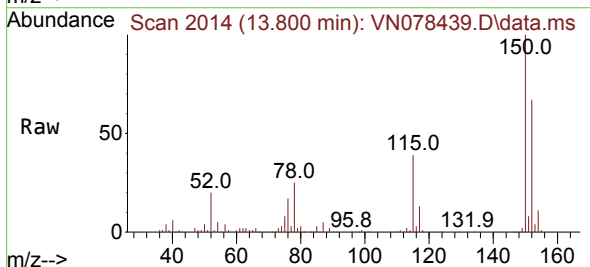




#74
N-amy1 acetate
Concen: 0.294 ug/l
RT: 12.500 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion:	43	Resp:	2468
Ion	Ratio	Lower	Upper
43	100		
70	0.0	43.4	65.2#
55	21.9	21.4	32.0
61	0.0	22.8	34.2#

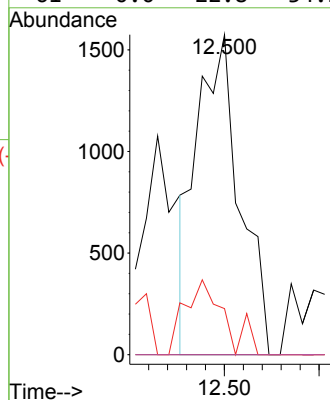

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.941 min Scan# 1868
Delta R.T. 0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Tgt Ion:	83	Resp:	171
Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.0	15.0#
85	390.1	31.9	95.7#


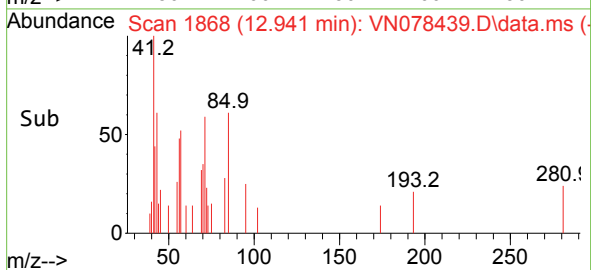
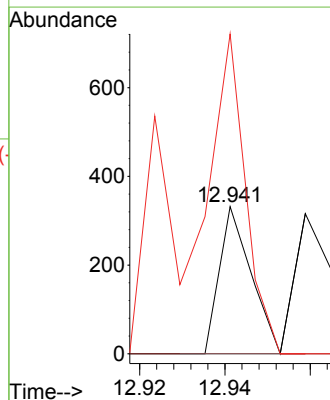





#76
1,2,3-Trichloropropane
Concen: 28.989 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15




Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627


Tgt Ion: 75 Resp: 184667
Ion Ratio Lower Upper
75 100
77 1.3 84.5 253.5#

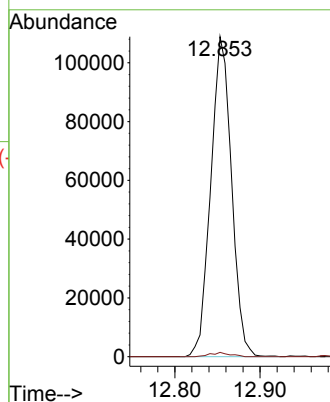

#81
trans-1,4-Dichloro-2-butene
Concen: 89.064 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15


Tgt Ion: 75 Resp: 184667
Ion Ratio Lower Upper
75 100
53 0.2 67.4 101.2#
89 0.1 38.8 58.2#

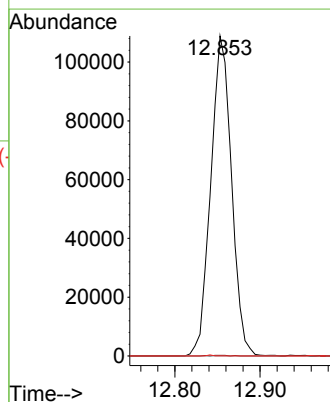



#94
Hexachlorobutadiene
Concen: Below Cal
RT: 15.506 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN078439.D
Acq: 28 Jun 2023 14:15

Instrument :
MSVOA_N
ClientSampleId :
SB-COMP-0627

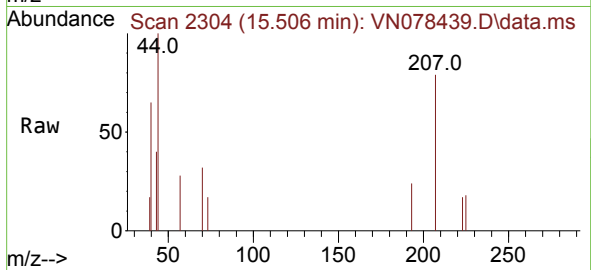

Tgt Ion:	225	Resp:	61
Ion	Ratio	Lower	Upper
225	100		
223	229.5	31.3	93.8#
227	0.0	31.9	95.9#

