


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062920\
 Data File : VN062204.D
 Acq On : 29 Jun 2020 21:44
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Title : SW846 8260
 Last Update : Wed Jun 24 15:33:00 2020

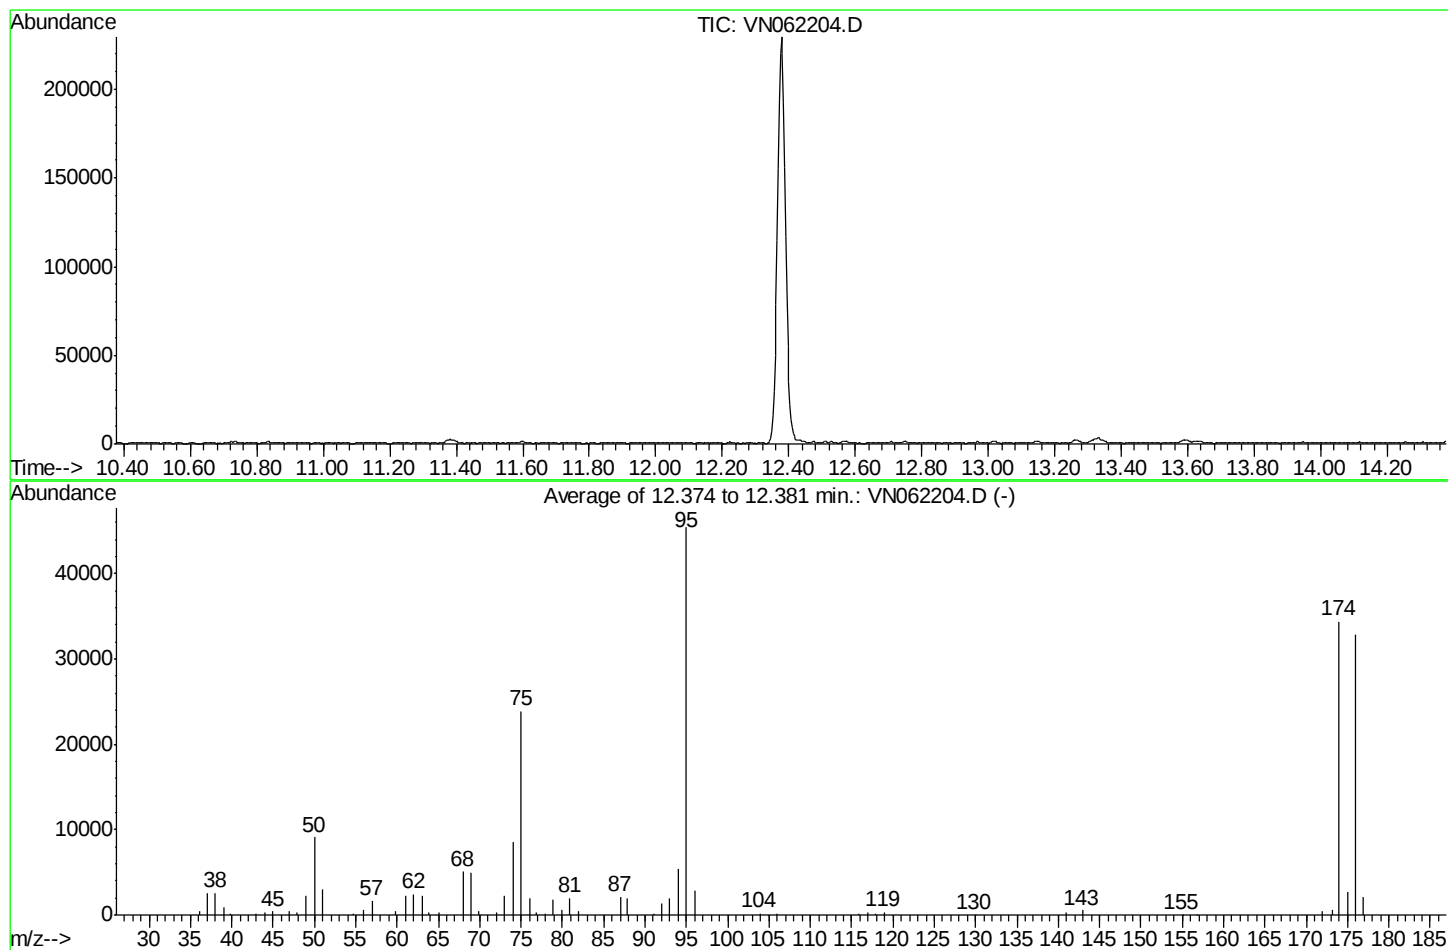

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	9089	PASS
75	95	30	60	52.6	23901	PASS
95	95	100	100	100.0	45416	PASS
96	95	5	9	6.4	2899	PASS
173	174	0.00	2	1.8	627	PASS
174	95	50	100	75.7	34365	PASS
175	174	5	9	7.7	2636	PASS
176	174	95	101	95.5	32832	PASS
177	176	5	9	6.5	2133	PASS