

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062921\
 Data File : VN067552.D
 Acq On : 29 Jun 2021 14:51
 Operator : JC/MD
 Sample : M2847-05
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jun 29 15:24:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062821W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 28 14:31:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	186659	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	353930	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	346621	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	136060	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	144161	56.432	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 112.860%			
35) Dibromofluoromethane	8.024	113	103722	47.268	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 94.540%			
50) Toluene-d8	10.443	98	482626	54.142	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 108.280%			
62) 4-Bromofluorobenzene	12.733	95	162992	52.347	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 104.700%			
Target Compounds						Qvalue
3) Chloromethane	2.309	50	800	0.344	ug/l #	43
5) Bromomethane	2.883	94	799	0.348	ug/l #	80
6) Chloroethane	3.237	64	623	0.286	ug/l #	67
11) Tert butyl alcohol	5.385	59	3509	9.202	ug/l	98
13) Acrolein	4.036	56	52	2.432	ug/l #	14
16) Acetone	4.296	43	17402	20.652	ug/l	96
17) Carbon Disulfide	4.524	76	8832	1.729	ug/l	99
20) Methylene Chloride	5.090	84	324	Below Cal	#	56
25) 2-Butanone	7.345	43	2867	2.206	ug/l	100
29) Tetrahydrofuran	7.595	42	14429	16.675	ug/l #	35
31) Cyclohexane	8.086	56	5274	Below Cal	#	22
36) 1,1-Dichloropropene	8.088	75	17674	5.531	ug/l #	52
37) Ethyl Acetate	7.597	43	96467	32.879	ug/l #	69
38) Carbon Tetrachloride	8.088	117	21638	6.322	ug/l #	16
40) Benzene	8.461	78	708704	73.254	ug/l	98
41) Methacrylonitrile	7.595	41	58486	39.987	ug/l #	47
42) 1,2-Dichloroethane	8.464	62	6645	1.990	ug/l #	79
45) 1,2-Dichloropropane	9.510	63	575	0.237	ug/l #	44
48) Methyl methacrylate	9.507	41	5001	2.279	ug/l #	50
51) 4-Methyl-2-Pentanone	10.333	43	4818	1.593	ug/l	99
52) Toluene	10.507	92	41745	6.604	ug/l	99
53) t-1,3-Dichloropropene	10.515	75	230	2.310	ug/l #	46
59) 2-Hexanone	11.092	43	1456	0.682	ug/l	91
67) Ethyl Benzene	11.848	91	6155	0.479	ug/l	95
68) m/p-Xylenes	11.956	106	3925	0.794	ug/l	92
69) o-Xylene	12.283	106	2113	0.432	ug/l	94
70) Styrene	12.299	104	16058	3.662	ug/l	89
74) N-amyl acetate	12.358	43	2417	0.644	ug/l #	48
76) 1,2,3-Trichloropropane	12.733	75	90521	33.192	ug/l #	100
80) 1,3,5-Trimethylbenzene	13.061	105	2503	0.267	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.733	75	90521	95.429	ug/l #	6
84) 1,2,4-Trimethylbenzene	13.369	105	7512	0.814	ug/l	98
90) Hexachloroethane	14.281	117	657	0.415	ug/l #	16
95) Naphthalene	15.507	128	29533	7.305	ug/l	98
96) 1,2,3-Trichlorobenzene	15.700	180	475	0.246	ug/l #	24

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062921\
Data File : VN067552.D
Acq On : 29 Jun 2021 14:51
Operator : JC/MD
Sample : M2847-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jun 29 15:24:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062821W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 28 14:31:03 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062921\
Data File : VN067552.D
Acq On : 29 Jun 2021 14:51
Operator : JC/MD
Sample : M2847-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jun 29 15:24:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062821W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 28 14:31:03 2021
Response via : Initial Calibration




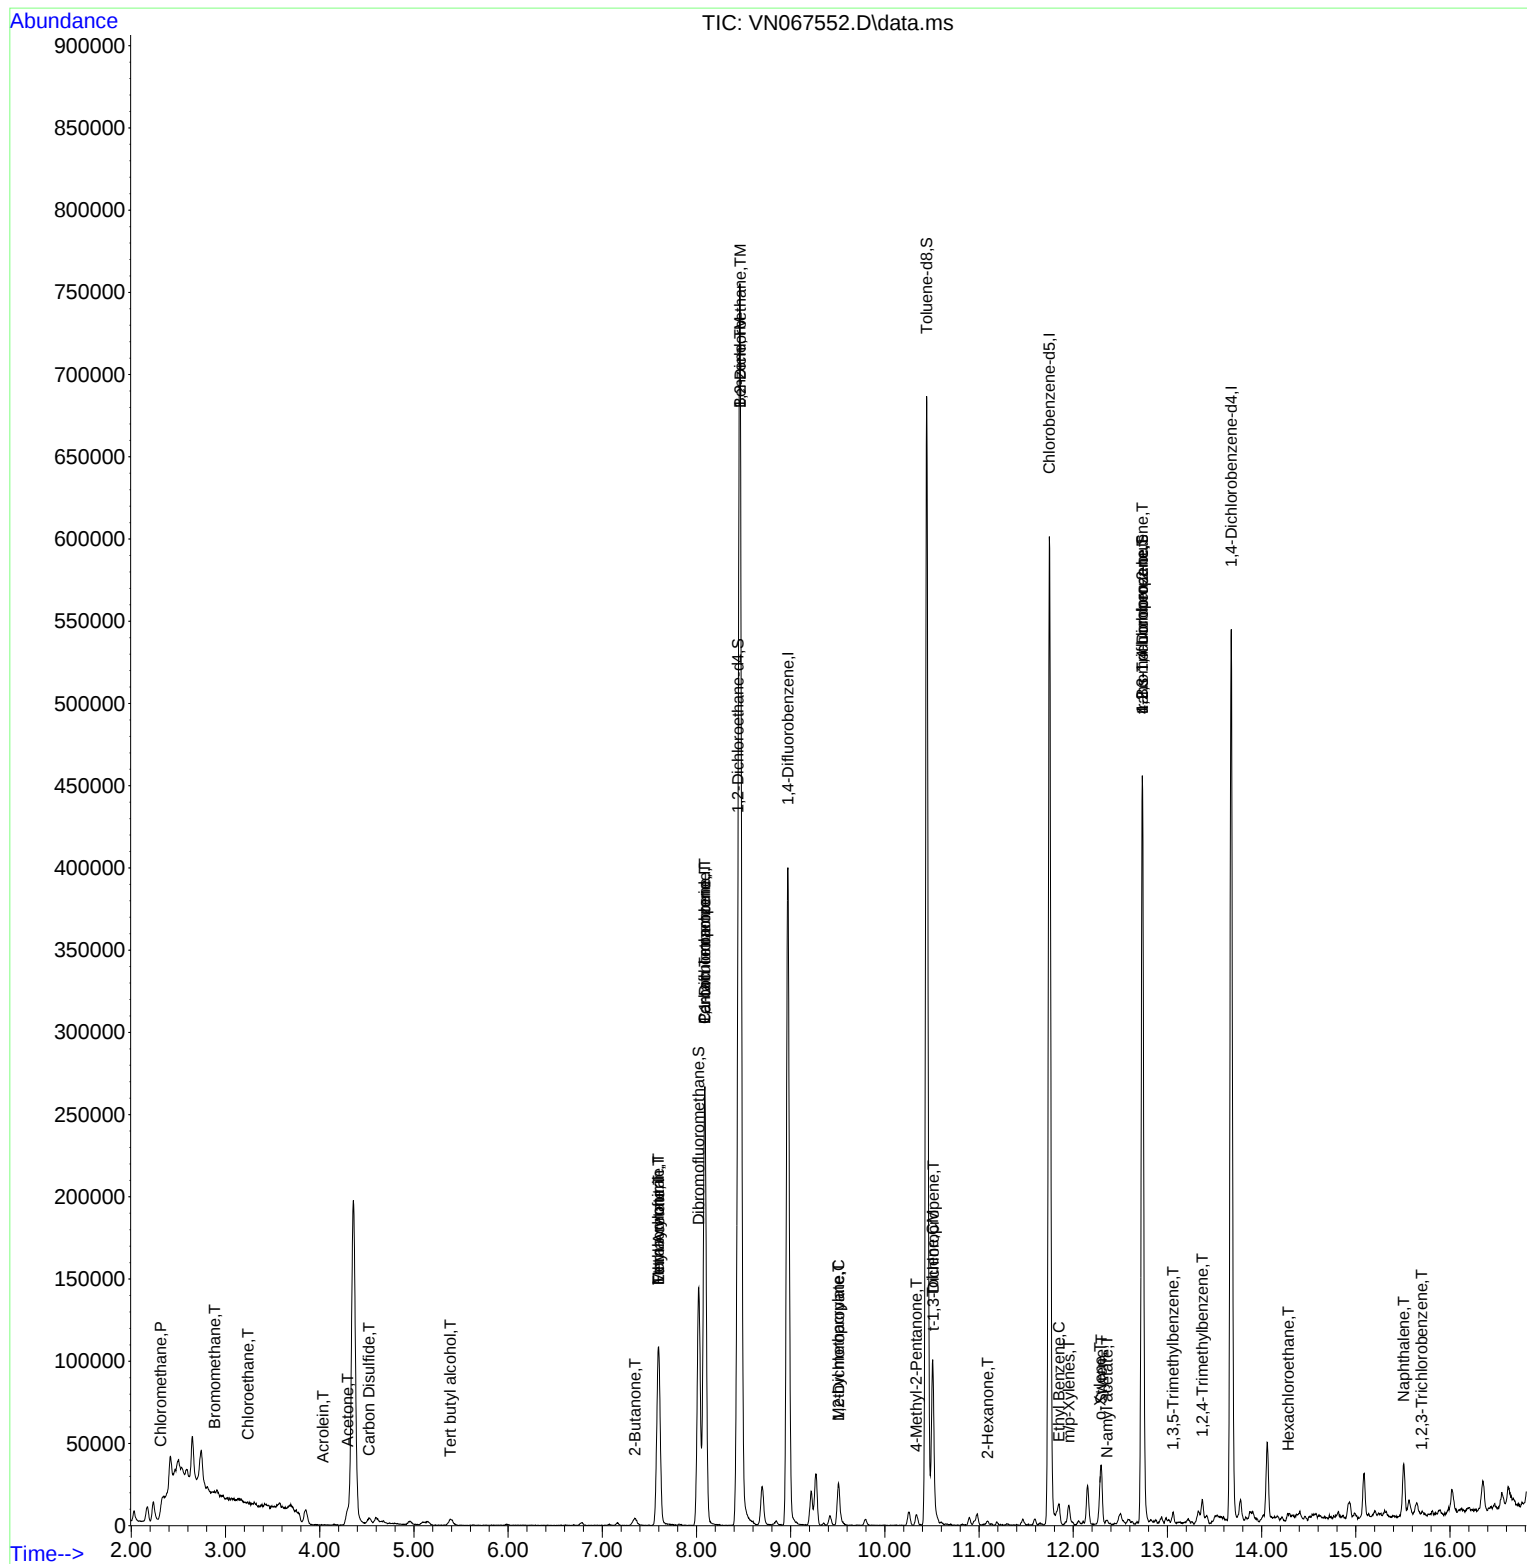




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN067528.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 186659
Ion Ratio Lower Upper
168 100
99 67.1 62.9 94.3



#3
Chloromethane
Concen: 0.344 ug/l
RT: 2.309 min Scan# 119
Delta R.T. 0.008 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 50 Resp: 800
Ion Ratio Lower Upper
50 100
52 0.0 25.6 38.4#


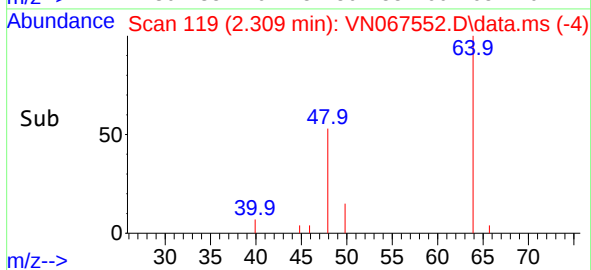






#5
Bromomethane
Concen: 0.348 ug/l
RT: 2.883 min Scan# 333
Delta R.T. 0.041 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 799
Ion Ratio Lower Upper
94 100
96 73.2 73.7 110.5#

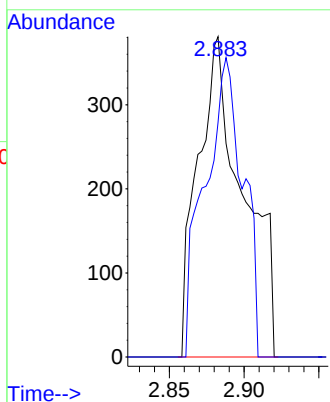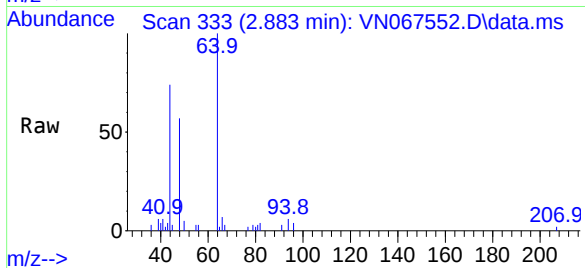

#6
Chloroethane
Concen: 0.286 ug/l
RT: 3.237 min Scan# 465
Delta R.T. 0.226 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 64 Resp: 623
Ion Ratio Lower Upper
64 100
66 12.7 24.7 37.1#

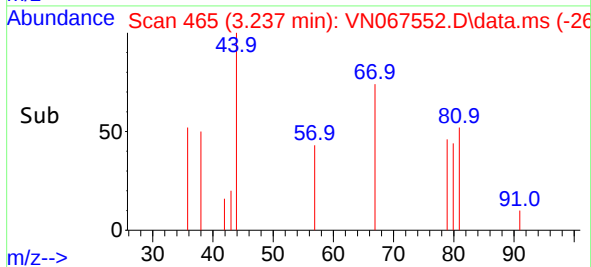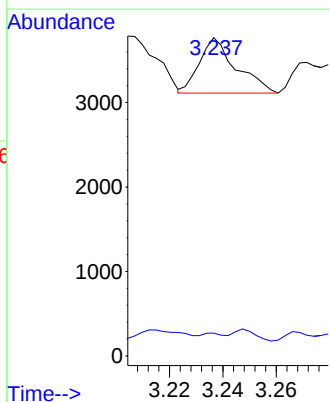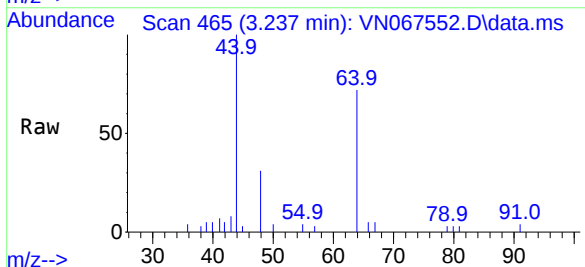







#11

Tert butyl alcohol
Concen: 9.202 ug/l
RT: 5.385 min Scan# 1266
Delta R.T. -0.008 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 3509
Ion Ratio Lower Upper
59 100
57 10.3 8.7 13.1

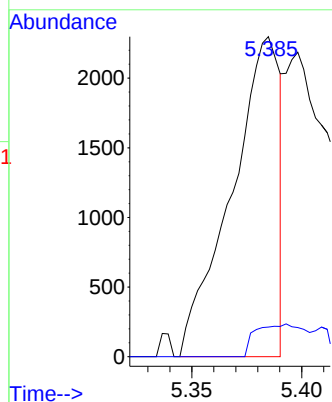


#13

Acrolein
Concen: 2.432 ug/l
RT: 4.036 min Scan# 763
Delta R.T. -0.002 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 56 Resp: 52
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.0#









#16
Acetone
Concen: 20.652 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.008 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 17402
Ion Ratio Lower Upper
43 100
58 28.5 21.2 31.8

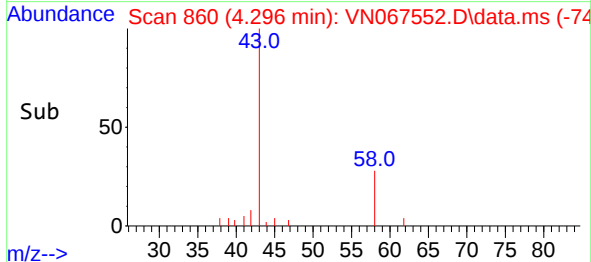

#17
Carbon Disulfide
Concen: 1.729 ug/l
RT: 4.524 min Scan# 945
Delta R.T. -0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 76 Resp: 8832
Ion Ratio Lower Upper
76 100
78 10.0 7.7 11.5


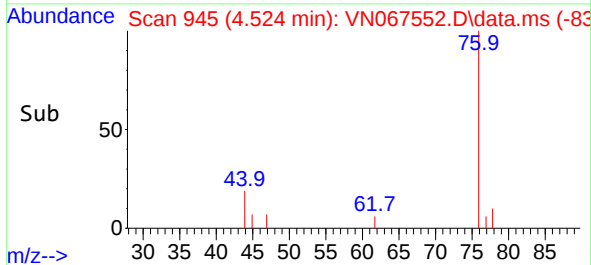

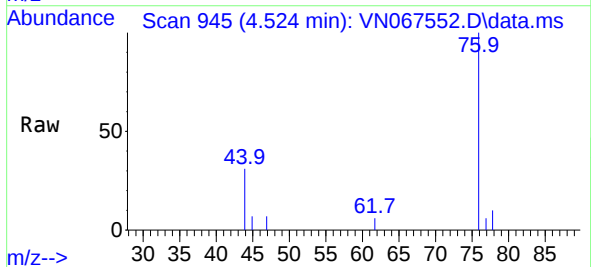




#25
2-Butanone
Concen: 2.206 ug/l
RT: 7.345 min Scan# 1997
Delta R.T. 0.005 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2867
Ion Ratio Lower Upper
43 100
72 24.6 19.7 29.5

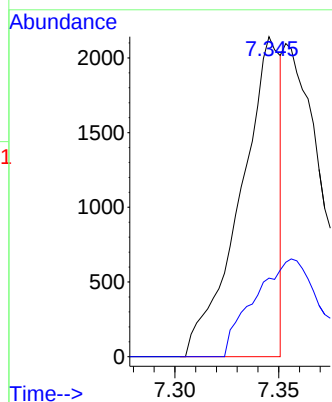

#29
Tetrahydrofuran
Concen: 16.675 ug/l
RT: 7.595 min Scan# 2090
Delta R.T. -0.094 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 42 Resp: 14429
Ion Ratio Lower Upper
42 100
72 0.0 32.8 49.2#
71 0.0 31.2 46.8#

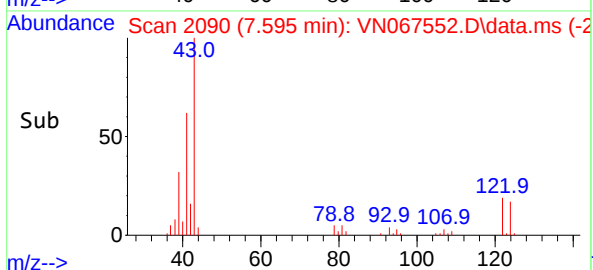







#33

1,2-Dichloroethane-d4
Concen: 56.432 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Instrument :
MSVOA_N
ClientSampleId :




Tgt Ion: 65 Resp: 144161
Ion Ratio Lower Upper
65 100
67 51.2 0.0 98.6




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 114 Resp: 353930
Ion Ratio Lower Upper
114 100
63 21.5 0.0 49.0
88 16.1 0.0 36.6









#35
Dibromofluoromethane
Concen: 47.268 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 103722
Ion Ratio Lower Upper
113 100
111 102.7 83.8 125.8
192 15.8 13.4 20.0

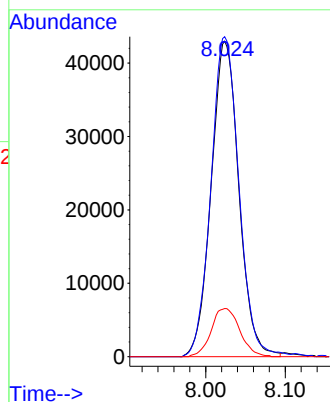

#36
1,1-Dichloropropene
Concen: 5.531 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 75 Resp: 17674
Ion Ratio Lower Upper
75 100
110 9.3 15.7 47.0#
77 0.0 24.6 37.0#

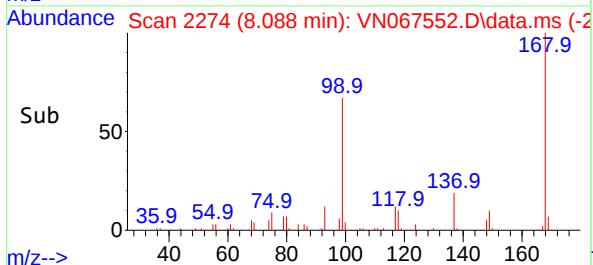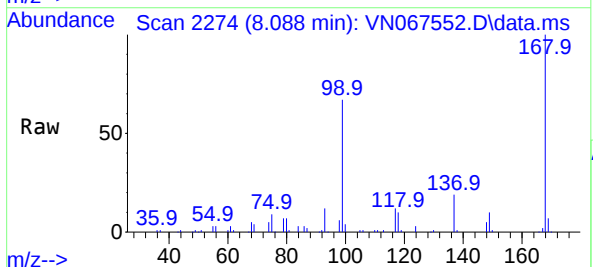



#37

Ethyl Acetate

Concen: 32.879 ug/l

RT: 7.597 min Scan# 2091





Delta R.T. 0.179 min

Lab File: VN067552.D

Acq: 29 Jun 2021 14:51

Tgt Ion:	43	Resp:	96467
Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.6	16.0#
70	0.0	8.1	12.1#

Instrument :
MSVOA_N
ClientSampled :



#38

Carbon Tetrachloride

Concen: 6.322 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.118 min

Lab File: VN067552.D

Acq: 29 Jun 2021 14:51

Tgt Ion:	117	Resp:	21638
Ion	Ratio	Lower	Upper
117	100		
119	4.3	75.4	113.2#
121	0.0	23.5	35.3#


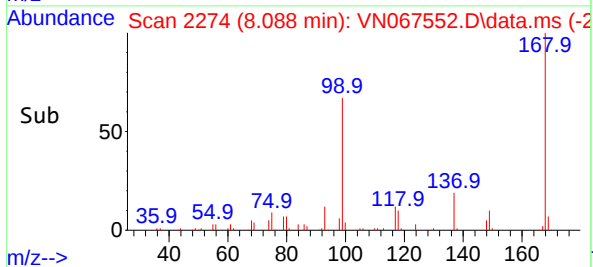

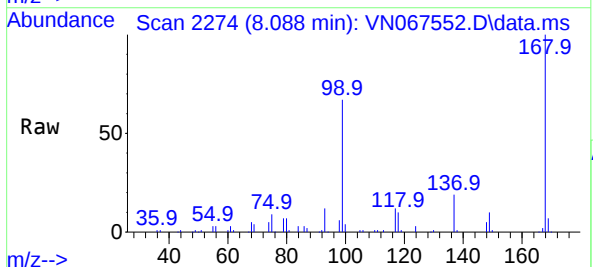




#40
Benzene
Concen: 73.254 ug/l
RT: 8.461 min Scan# 2413
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 78 Resp: 708704
Ion Ratio Lower Upper
78 100
77 24.6 18.9 28.3

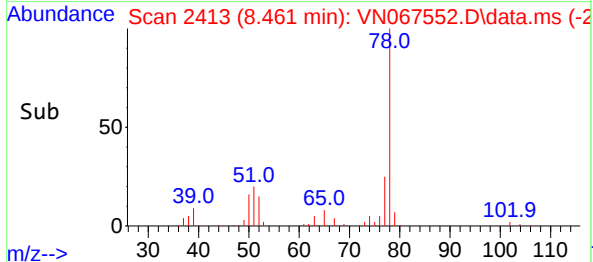

#41
Methacrylonitrile
Concen: 39.987 ug/l
RT: 7.595 min Scan# 2090
Delta R.T. -0.043 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 41 Resp: 58486
Ion Ratio Lower Upper
41 100
39 51.3 47.6 71.4
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#

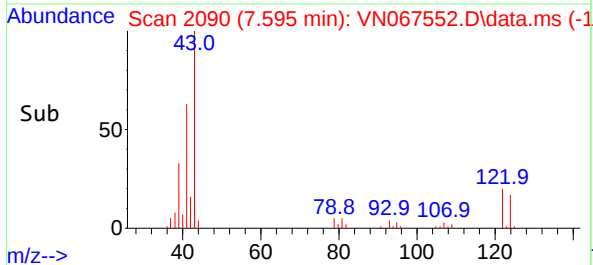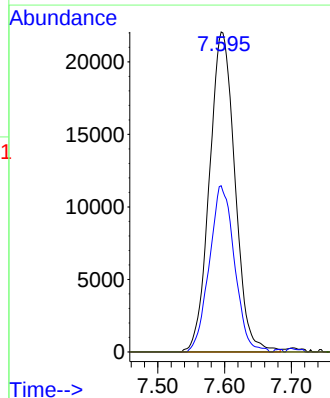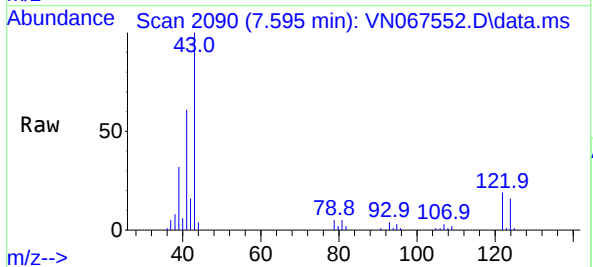







#42

1,2-Dichloroethane
Concen: 1.990 ug/l
RT: 8.464 min Scan# 2414
Delta R.T. -0.069 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 62 Resp: 6645
Ion Ratio Lower Upper
62 100
98 0.0 0.0 14.2




#45

1,2-Dichloropropane
Concen: 0.237 ug/l
RT: 9.510 min Scan# 2804
Delta R.T. 0.016 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 63 Resp: 575
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#


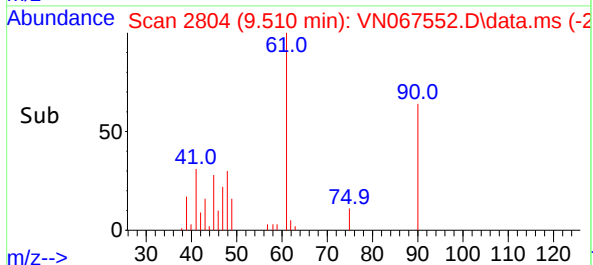

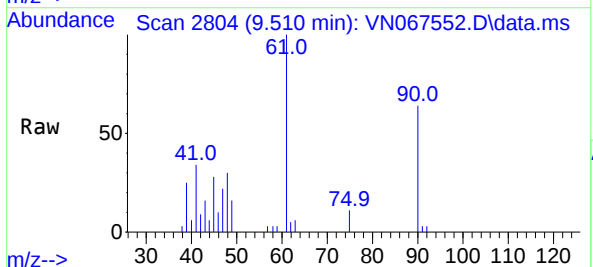




#48
Methyl methacrylate
Concen: 2.279 ug/l
RT: 9.507 min Scan# 2803
Delta R.T. -0.056 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 41 Resp: 5001
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 66.3 53.3 79.9

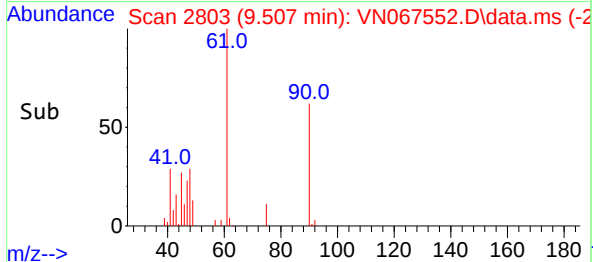

#50
Toluene-d8
Concen: 54.142 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 98 Resp: 482626
Ion Ratio Lower Upper
98 100
100 62.0 51.7 77.5


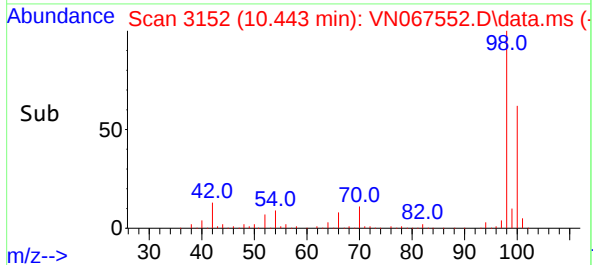

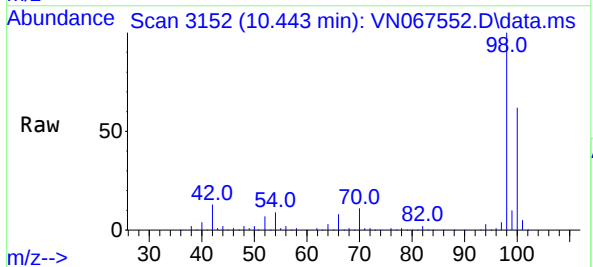




#51
4-Methyl-2-Pentanone
Concen: 1.593 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 4818
Ion Ratio Lower Upper
43 100
58 36.6 28.6 43.0

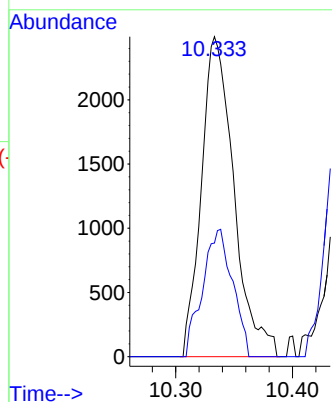

#52
Toluene
Concen: 6.604 ug/l
RT: 10.507 min Scan# 3176
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 92 Resp: 41745
Ion Ratio Lower Upper
92 100
91 176.0 139.6 209.4


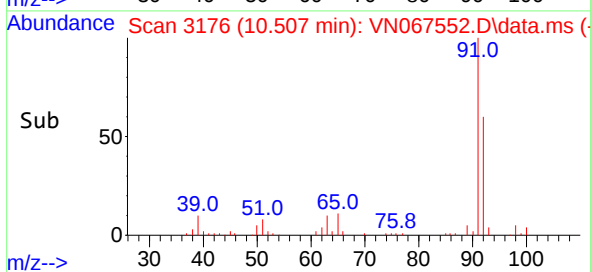
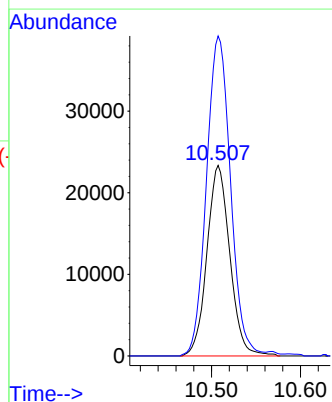





#53
t-1,3-Dichloropropene
Concen: 2.310 ug/l
RT: 10.515 min Scan# 3179
Delta R.T. -0.207 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 230
Ion Ratio Lower Upper
75 100
77 61.3 25.1 37.7#



#59
2-Hexanone
Concen: 0.682 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.003 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 43 Resp: 1456
Ion Ratio Lower Upper
43 100
58 55.8 24.7 74.1


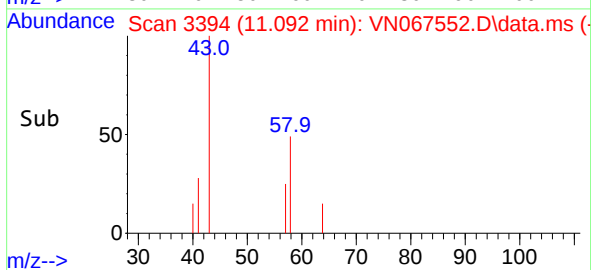






#62
4-Bromofluorobenzene
Concen: 52.347 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 162992
Ion Ratio Lower Upper
95 100
174 67.9 0.0 122.0
176 65.0 0.0 117.6

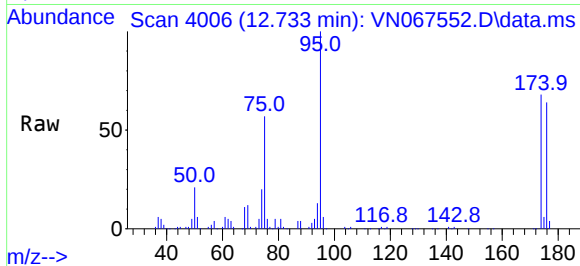

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 117 Resp: 346621
Ion Ratio Lower Upper
117 100
82 59.3 53.1 79.7
119 32.0 25.5 38.3




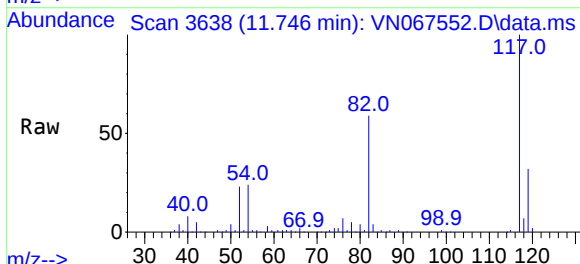




#67
Ethyl Benzene
Concen: 0.479 ug/l
RT: 11.848 min Scan# 3676
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 6155
Ion Ratio Lower Upper
91 100
106 32.1 23.4 35.0

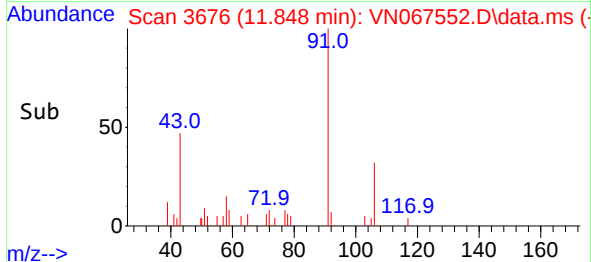

#68
m/p-Xylenes
Concen: 0.794 ug/l
RT: 11.956 min Scan# 3716
Delta R.T. -0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion:106 Resp: 3925
Ion Ratio Lower Upper
106 100
91 212.1 180.6 270.8


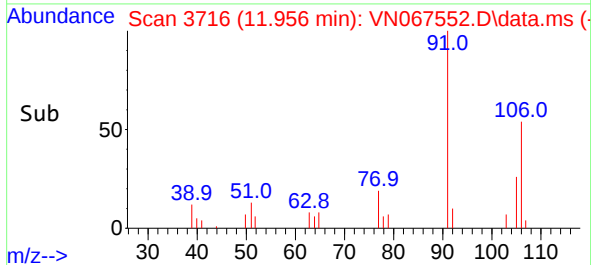

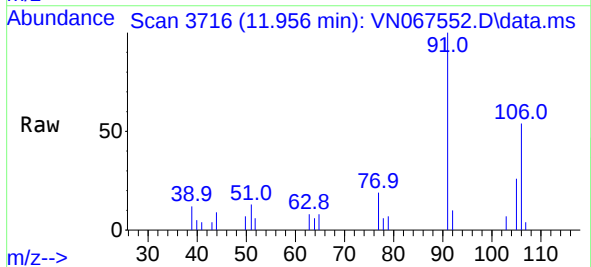




#69
o-Xylene
Concen: 0.432 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. -0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 2113
Ion Ratio Lower Upper
106 100
91 247.3 118.3 354.9



#70
Styrene
Concen: 3.662 ug/l
RT: 12.299 min Scan# 3844
Delta R.T. 0.003 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion:104 Resp: 16058
Ion Ratio Lower Upper
104 100
78 48.3 48.2 72.2
103 51.4 44.5 66.7



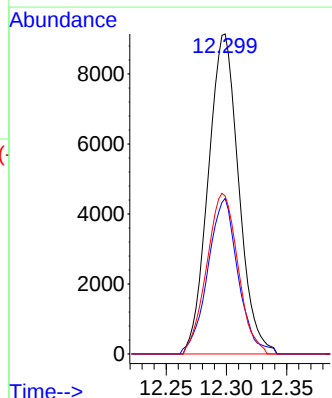





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 136060
Ion Ratio Lower Upper
152 100
115 63.5 36.1 108.5
150 159.1 0.0 351.8

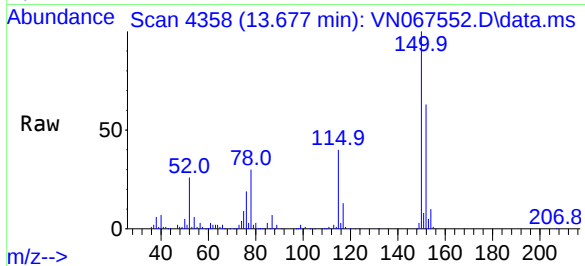

#74
N-ethyl acetate
Concen: 0.644 ug/l
RT: 12.358 min Scan# 3866
Delta R.T. -0.032 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 43 Resp: 2417
Ion Ratio Lower Upper
43 100
70 0.0 29.4 44.2#
55 2.2 17.0 25.4#
61 0.0 17.6 26.4#


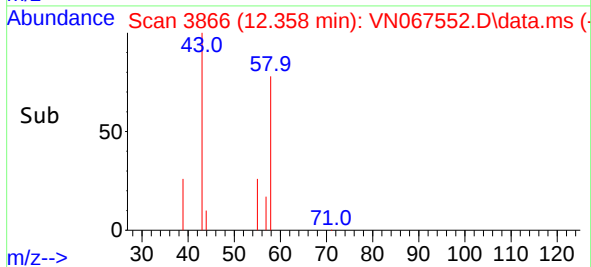
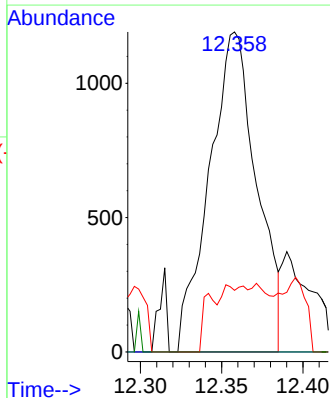
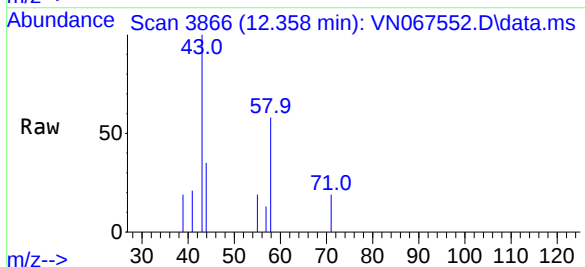




#76
1,2,3-Trichloropropane
Concen: 33.192 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.148 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 90521
Ion Ratio Lower Upper
75 100
77 1.3 0.0 0.0#

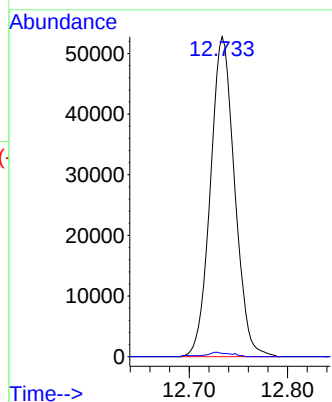

#80
1,3,5-Trimethylbenzene
Concen: 0.267 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion:105 Resp: 2503
Ion Ratio Lower Upper
105 100
120 42.3 22.2 66.6


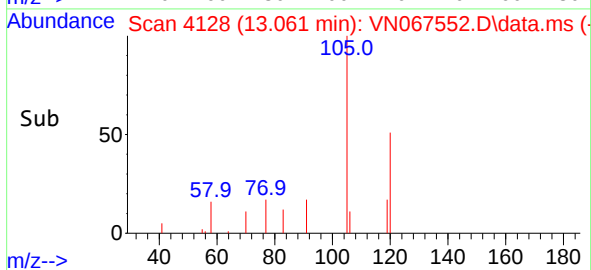
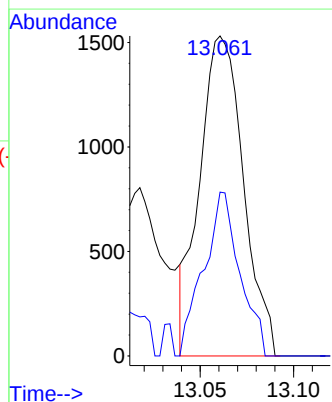





#81
trans-1,4-Dichloro-2-butene
Concen: 95.429 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 90521
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

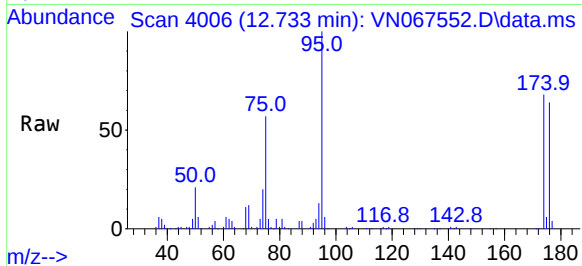

#84
1,2,4-Trimethylbenzene
Concen: 0.814 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51

Tgt Ion: 105 Resp: 7512
Ion Ratio Lower Upper
105 100
120 39.8 20.6 61.8


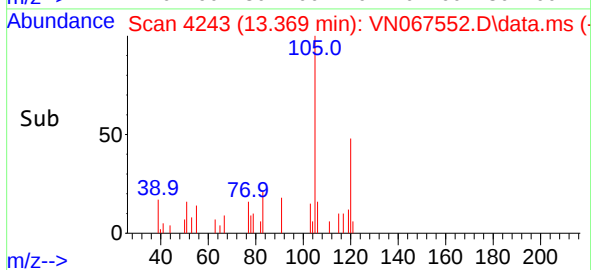

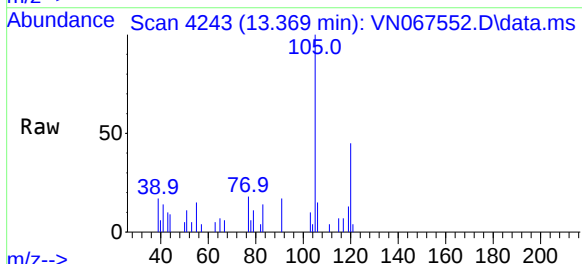




#90
Hexachloroethane
Concen: 0.415 ug/l
RT: 14.281 min Scan# 4583
Delta R.T. 0.067 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 657
Ion Ratio Lower Upper
117 100
201 0.0 33.5 100.5#

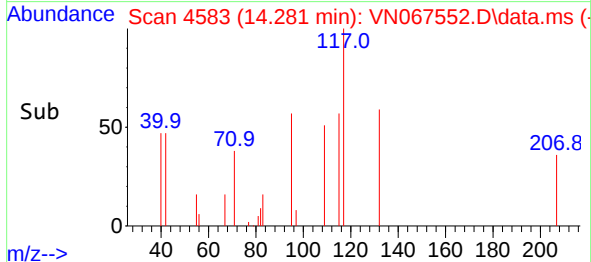

#95
Naphthalene
Concen: 7.305 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN067552.D
Acq: 29 Jun 2021 14:51


Tgt Ion:128 Resp: 29533
Ion Ratio Lower Upper
128 100
127 13.5 10.6 15.8
129 11.7 8.6 12.8

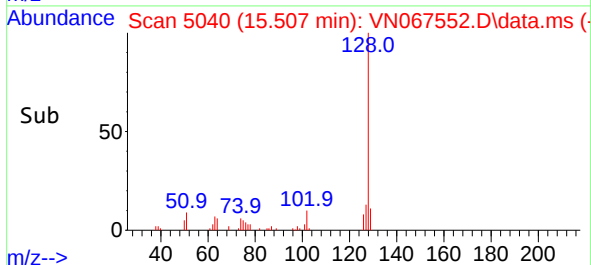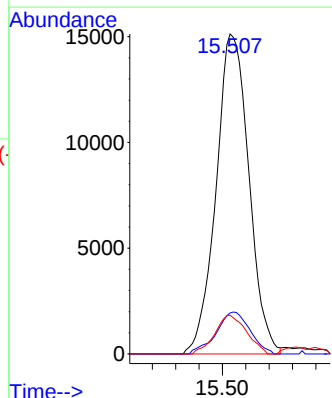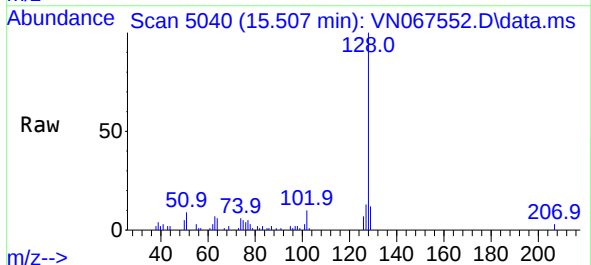



#96
 1,2,3-Trichlorobenzene
 Concen: 0.246 ug/l
 RT: 15.700 min Scan# 5112
 Delta R.T. -0.002 min
 Lab File: VN067552.D
 Acq: 29 Jun 2021 14:51

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:	180	Resp:	475
Ion	Ratio	Lower	Upper
180	100		
182	0.0	47.8	143.3#
145	47.8	18.2	54.6

