
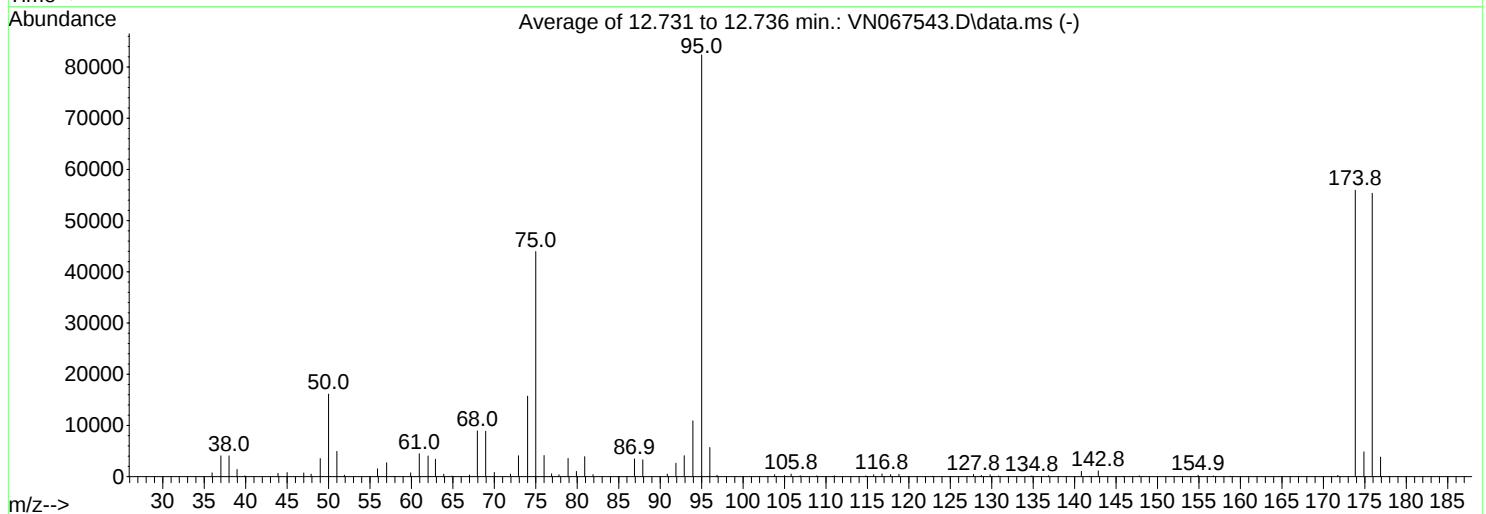


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062921\
 Data File : VN067543.D
 Acq On : 29 Jun 2021 9:17
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062821W.M
 Title : SW846 8260
 Last Update : Mon Jun 28 14:31:03 2021

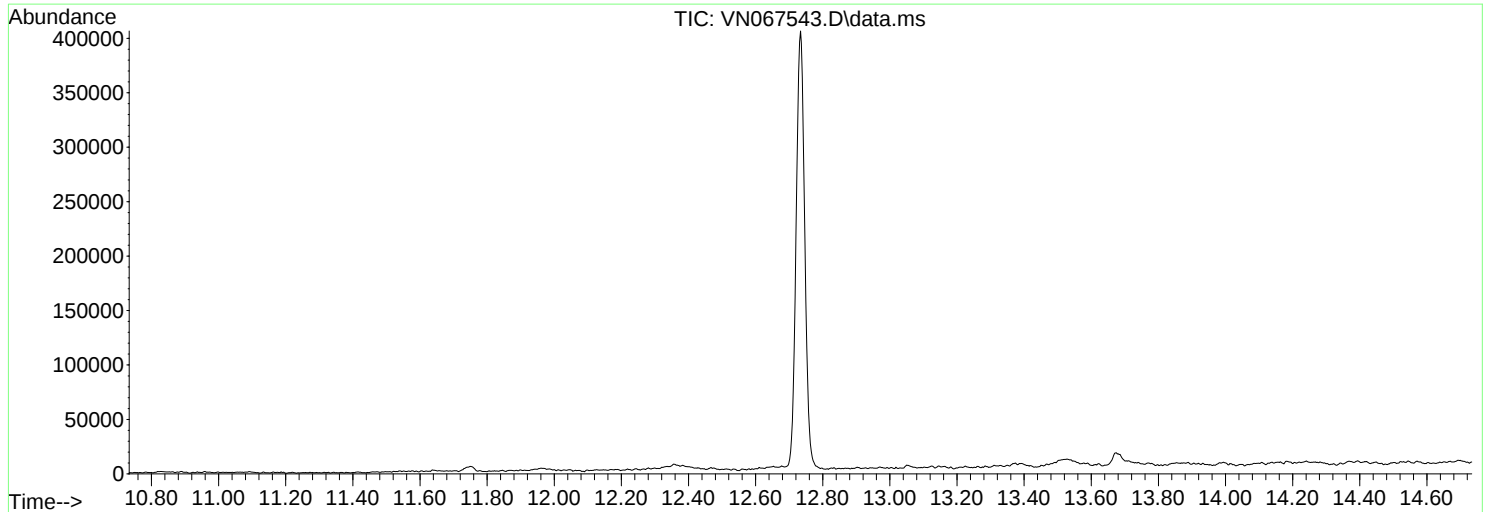

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3980

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	16122	PASS
75	95	30	60	53.4	43971	PASS
95	95	100	100	100.0	82381	PASS
96	95	5	9	6.9	5700	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.9	55936	PASS
175	174	5	9	8.6	4832	PASS
176	174	95	101	99.0	55363	PASS
177	176	5	9	6.9	3801	PASS