

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062922\
 Data File : VN073252.D
 Acq On : 29 Jun 2022 18:56
 Operator : JC\MD
 Sample : N3496-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Jun 30 07:01:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	322007	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	531165	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	502137	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	251221	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	200188	43.065	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.120%
35) Dibromofluoromethane	7.951	113	168697	47.737	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.480%
50) Toluene-d8	10.381	98	553232	44.078	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	88.160%
62) 4-Bromofluorobenzene	12.669	95	255465	52.964	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	105.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062922\
Data File : VN073252.D
Acq On : 29 Jun 2022 18:56
Operator : JC\MD
Sample : N3496-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Jun 30 07:01:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




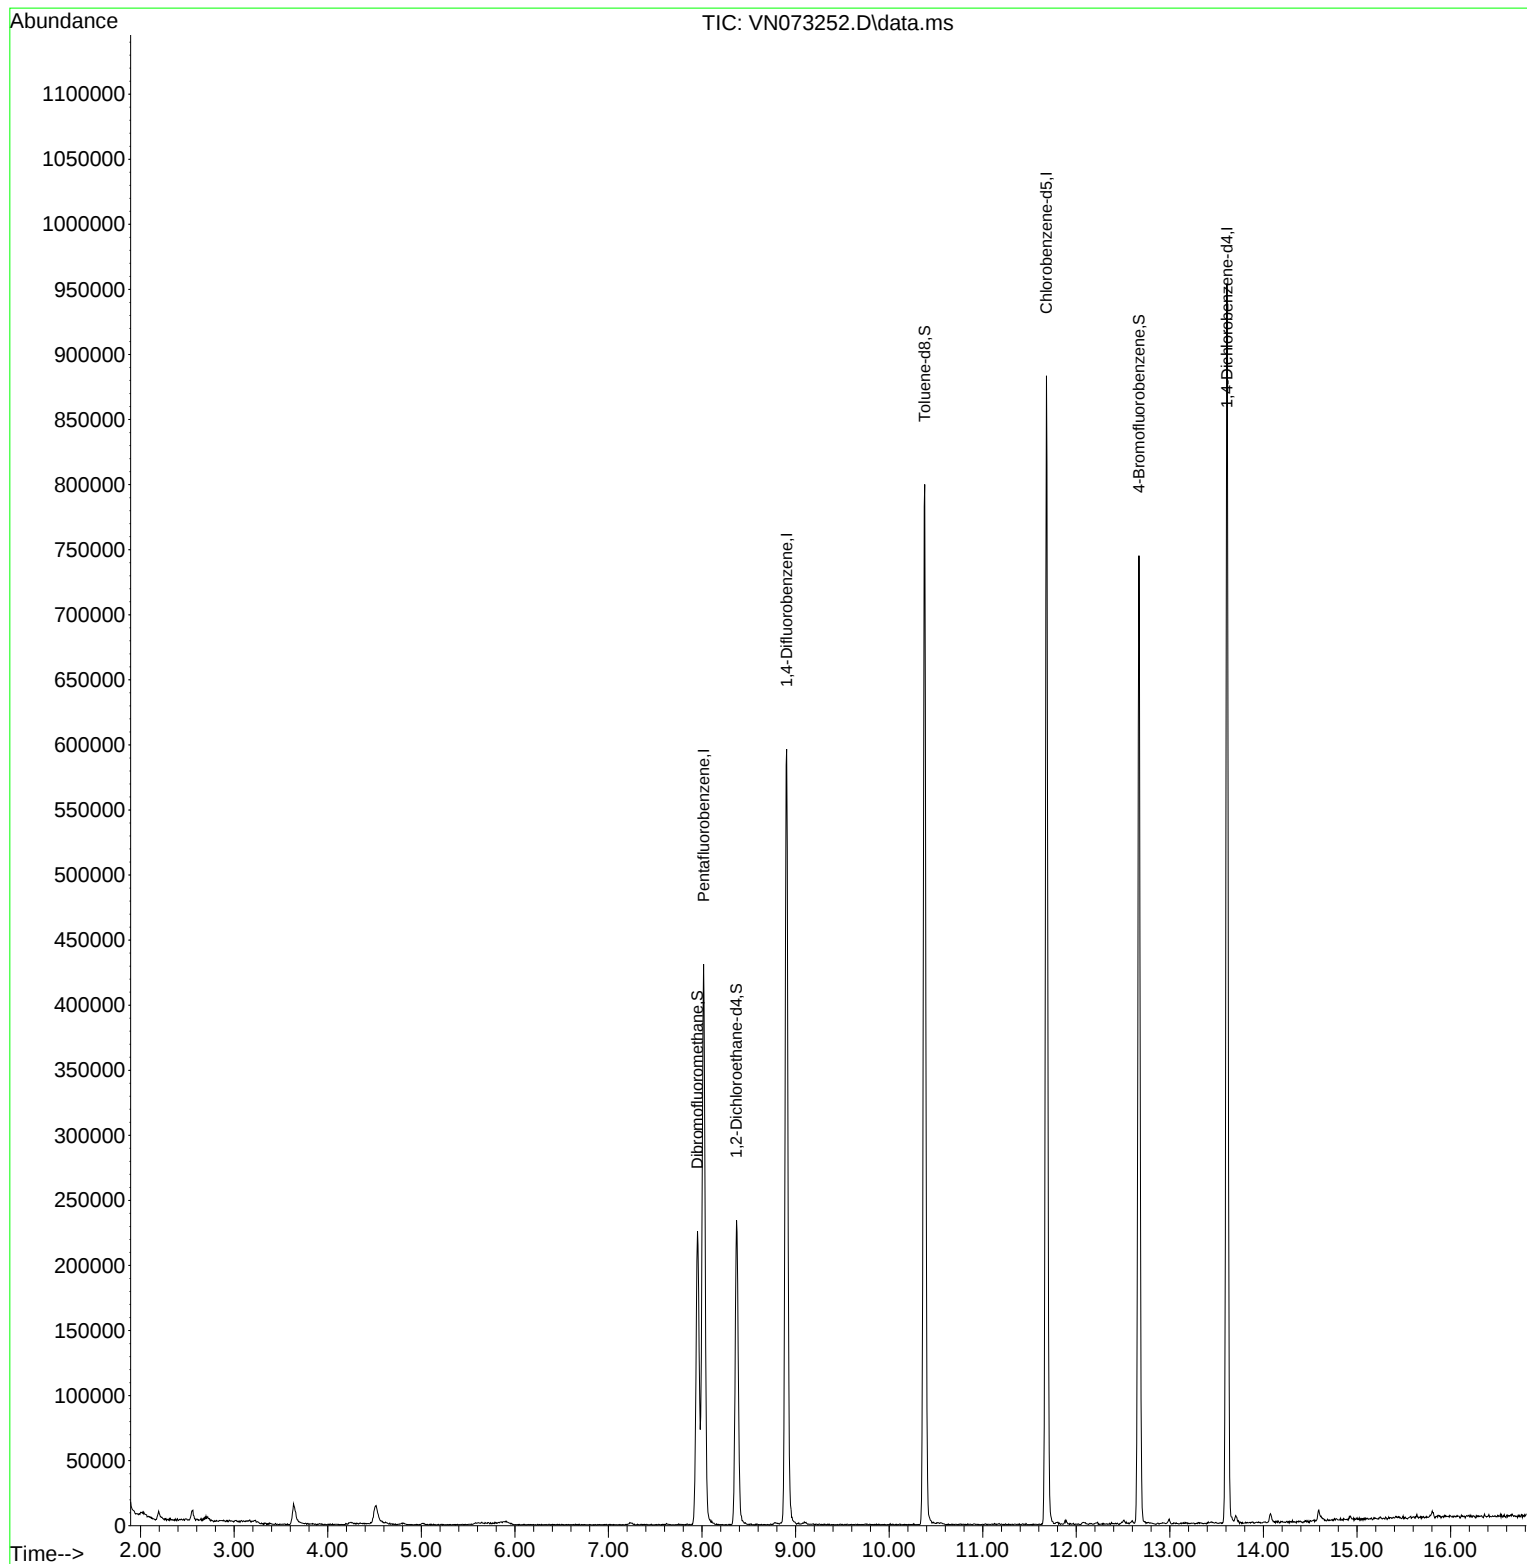


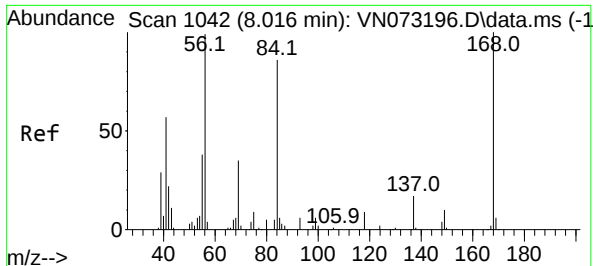

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073252.D
Acq: 29 Jun 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:168 Resp: 322007
Ion Ratio Lower Upper
168 100
99 61.0 42.3 63.5

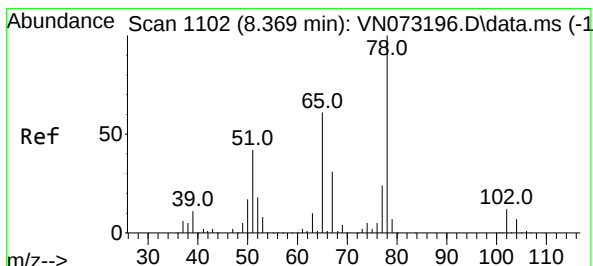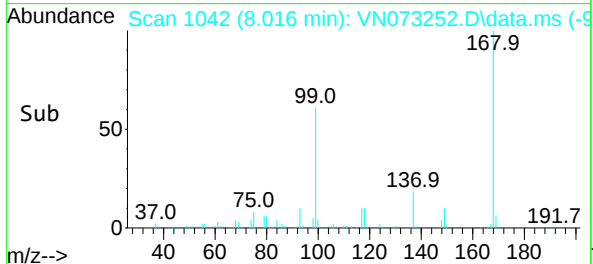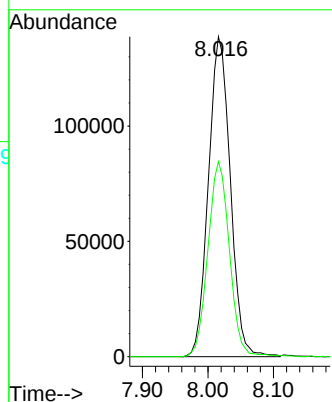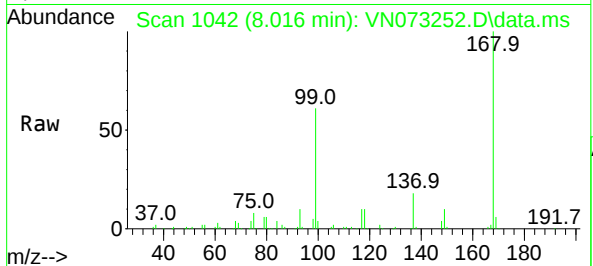

#33
1,2-Dichloroethane-d4
Concen: 43.065 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN073252.D
Acq: 29 Jun 2022 18:56

Tgt Ion: 65 Resp: 200188
Ion Ratio Lower Upper
65 100
67 52.2 0.0 104.8

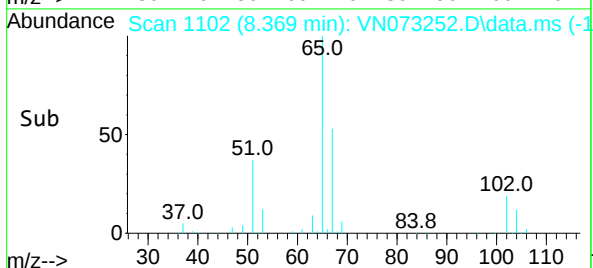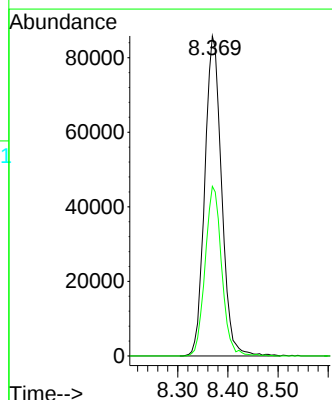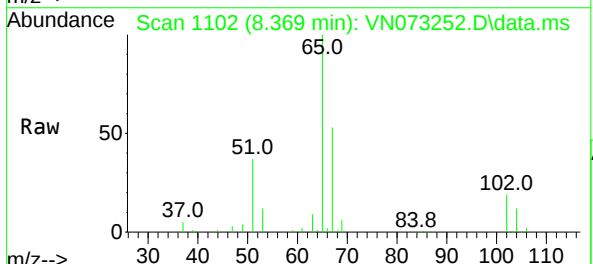



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1192

Delta R.T. 0.006 min

Lab File: VN073252.D

Acq: 29 Jun 2022 18:56

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-WATER-REF-4




Tgt Ion:114 Resp: 531165

Ion Ratio Lower Upper

114 100

63 20.8 0.0 40.0

88 15.5 0.0 32.6

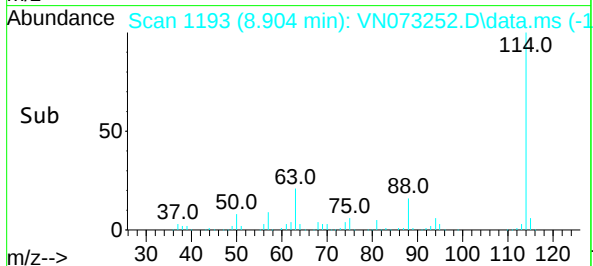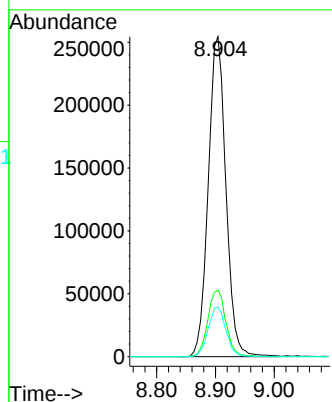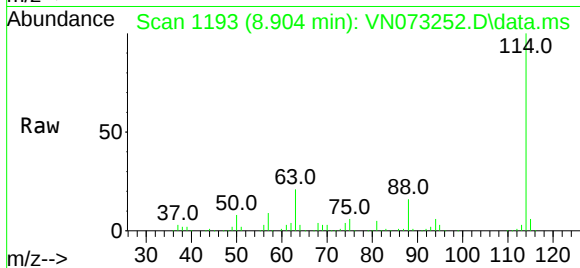

#35

Dibromofluoromethane

Concen: 47.737 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073252.D

Acq: 29 Jun 2022 18:56




Tgt Ion:113 Resp: 168697


Ion Ratio Lower Upper

113 100

111 102.0 81.4 122.0

192 19.1 17.0 25.6

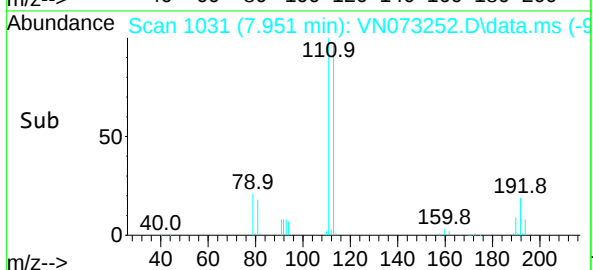
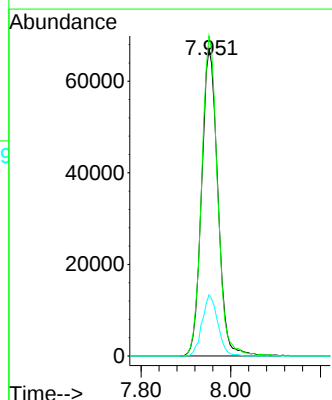
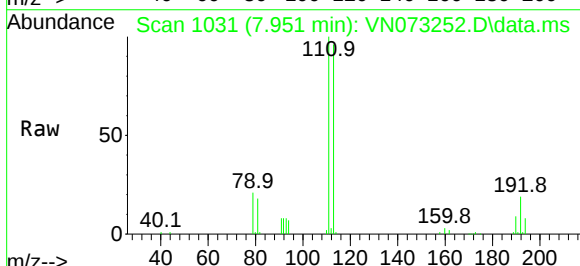


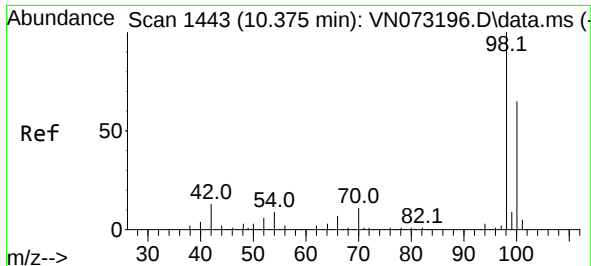

#50
Toluene-d8
Concen: 44.078 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.006 min
Lab File: VN073252.D
Acq: 29 Jun 2022 18:56




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 553232
Ion Ratio Lower Upper
98 100
100 65.5 52.6 78.8

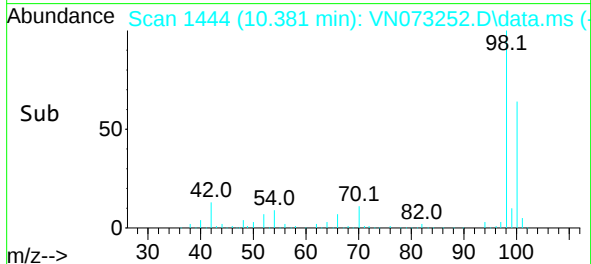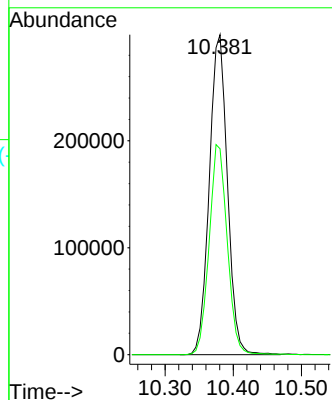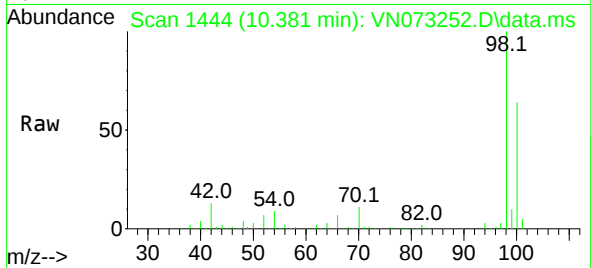

#62
4-Bromofluorobenzene
Concen: 52.964 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.000 min
Lab File: VN073252.D
Acq: 29 Jun 2022 18:56

Tgt Ion: 95 Resp: 255465
Ion Ratio Lower Upper
95 100
174 76.0 0.0 167.6
176 72.8 0.0 163.4


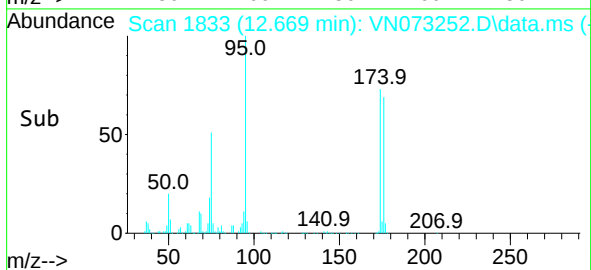
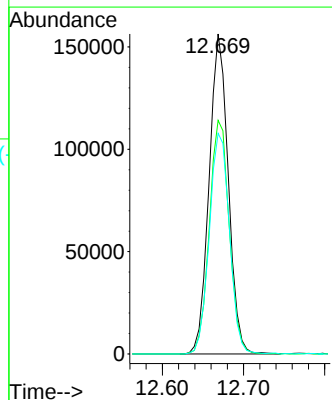
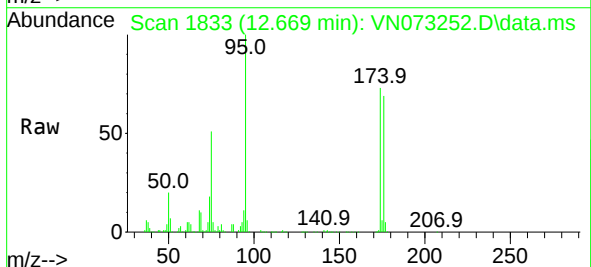


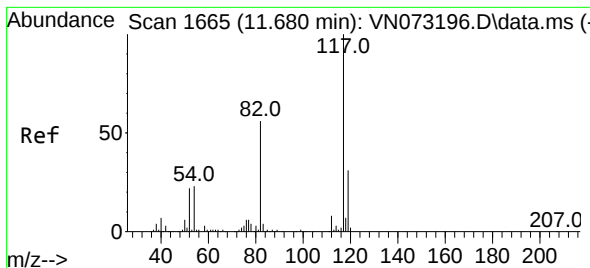

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1166
Delta R.T. 0.000 min
Lab File: VN073252.D
Acq: 29 Jun 2022 18:56

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 502137
Ion Ratio Lower Upper
117 100
82 55.3 44.2 66.2
119 32.5 25.4 38.0

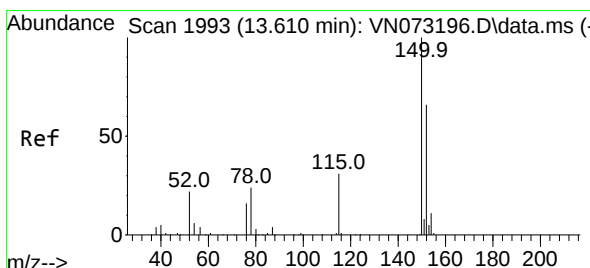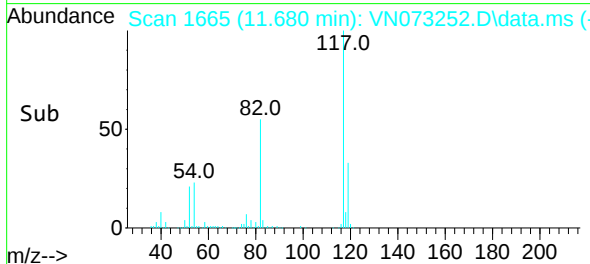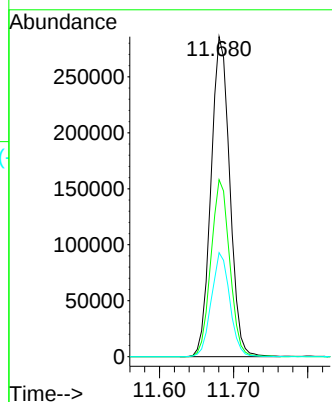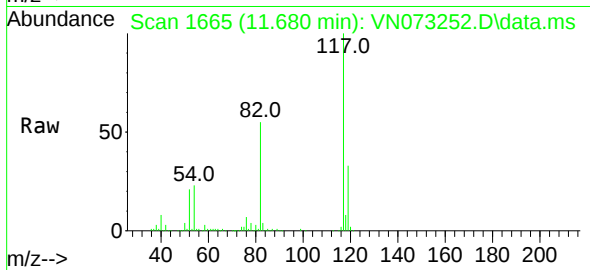

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN073252.D
Acq: 29 Jun 2022 18:56

Tgt Ion:152 Resp: 251221
Ion Ratio Lower Upper
152 100
115 59.8 28.9 86.7
150 156.7 0.0 356.2

