


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN063018\
Data File : VN049643.D
Acq On : 30 Jun 2018 9:36
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062918W.M
Title : SW846 8260
Last Update : Sat Jun 30 00:55:30 2018

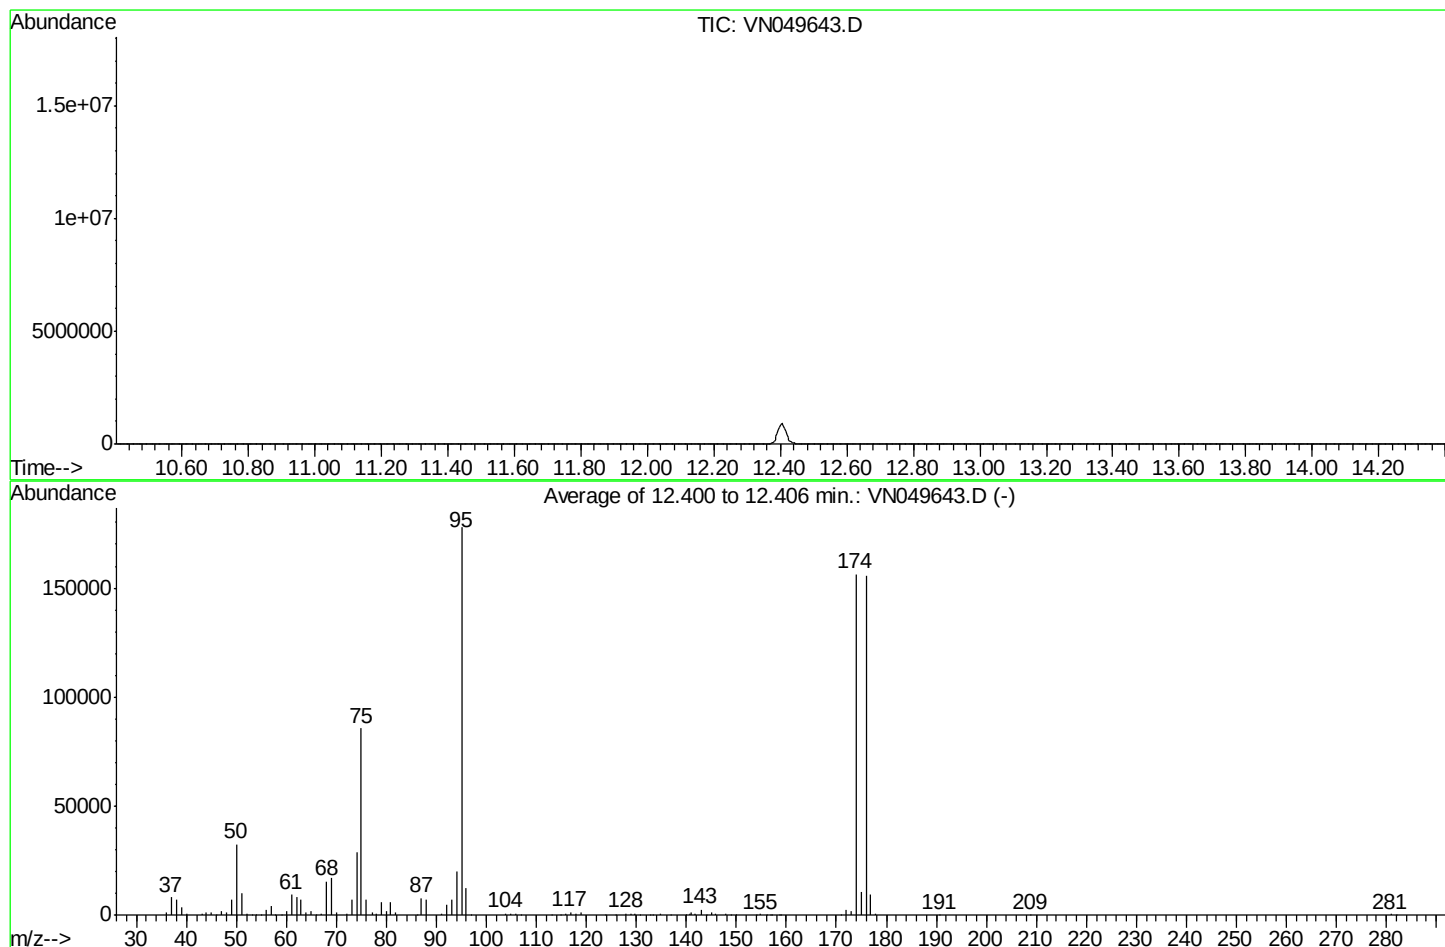

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3347

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	32461	PASS
75	95	30	60	48.1	85589	PASS
95	95	100	100	100.0	177813	PASS
96	95	5	9	6.8	12057	PASS
173	174	0.00	2	1.2	1817	PASS
174	95	50	100	88.0	156416	PASS
175	174	5	9	7.0	10881	PASS
176	174	95	101	99.5	155648	PASS
177	176	5	9	6.2	9674	PASS