

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN063020\
 Data File : VN062245.D
 Acq On : 30 Jun 2020 17:27
 Operator : JC/MD
 Sample : L3152-03
 Misc : 1.00u/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DRUM-COMP

Quant Time: Jul 01 03:37:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	183546	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	352554	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	321038	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	125769	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	139840	54.29	ug/l	0.00
Spiked Amount			Recovery	=	108.58%	
35) Dibromofluoromethane	7.54	113	110886	49.03	ug/l	0.00
Spiked Amount			Recovery	=	98.06%	
50) Toluene-d8	10.06	98	437935	48.44	ug/l	0.00
Spiked Amount			Recovery	=	96.88%	
62) 4-Bromofluorobenzene	12.38	95	135869	44.48	ug/l	0.00
Spiked Amount			Recovery	=	88.96%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.03	50	30	Below Cal	#	41
16) Acetone	3.76	43	61	Below Cal	#	40
18) Methyl Acetate	4.28	43	1008	0.492	ug/l	90
20) Methylene Chloride	4.49	84	3949	1.460	ug/l	94
29) Tetrahydrofuran	7.17	42	963	1.168	ug/l #	35
31) Cyclohexane	7.59	56	4602	1.293	ug/l #	62
36) 1,1-Dichloropropene	7.62	75	16095	4.542	ug/l #	45
38) Carbon Tetrachloride	7.62	117	18815	5.632	ug/l #	16
39) Methylcyclohexane	9.04	83	3306	0.851	ug/l #	83
41) Methacrylonitrile	7.18	41	584	0.429	ug/l #	16
43) Isopropyl Acetate	8.10	43	3355	0.701	ug/l #	58
48) Methyl methacrylate	9.10	41	821	0.383	ug/l #	19
52) Toluene	10.12	92	102804	15.599	ug/l	98
53) t-1,3-Dichloropropene	10.12	75	1167	0.291	ug/l #	1
71) Bromoform	12.38	173	1085	0.626	ug/l #	1
74) N-amyl acetate	12.07	43	131	3.377	ug/l #	38
76) 1,2,3-Trichloropropane	12.38	75	69472	23.465	ug/l #	100
79) 2-Chlorotoluene	12.64	91	1633	0.243	ug/l	82
80) 1,3,5-Trimethylbenzene	12.71	105	2423	0.307	ug/l	85
81) trans-1,4-Dichloro-2-buten	12.38	75	69472	68.526	ug/l #	13
82) 4-Chlorotoluene	12.75	91	1414	0.203	ug/l	83
84) 1,2,4-Trimethylbenzene	13.01	105	9993	1.268	ug/l	94
86) p-Isopropyltoluene	13.49	119	2476	0.317	ug/l	82
89) n-Butylbenzene	13.59	91	1745	0.268	ug/l #	77
90) Hexachloroethane	13.86	117	975	0.636	ug/l #	17
95) Naphthalene	15.10	128	11107	5.700	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1819

Delta R.T. -0.00 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27

Instrument :

MSVOA_N

ClientSampleId :


DRUM-COMP

Tot Ion:168 Resp: 183546

Ion Ratio Lower Upper

168 100

99 60.6 45.8 68.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.62

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#3

Chloromethane

Concen: Below Cal

RT: 2.03 min Scan# 80

Delta R.T. -0.00 min

Lab File: VN062245.D


Acq: 30 Jun 2020 17:27

Tgt Ion: 50 Resp: 30

Ion Ratio Lower Upper

50 100

52 0.0 27.0 40.6#



Abundance Ion 49.90 (49.60 to 50.60): VNO

Ion 51.90 (51.60 to 52.60): VNO

200


150


100

50

0

Time--> 2.02 2.03 2.04





#16

Acetone

Concen: Below Cal

RT: 3.76 min Scan# 618

Delta R.T. -0.01 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27

Instrument :

MSVOA_N

ClientSampleId :


DRUM-COMP

Tot Ion: 43 Resp: 61




Ion Ratio Lower Upper

43 100

58 0.0 27.5 41.3#



Abundance Ion 43.00 (42.70 to 43.70): VN062245.D (-529) (-)

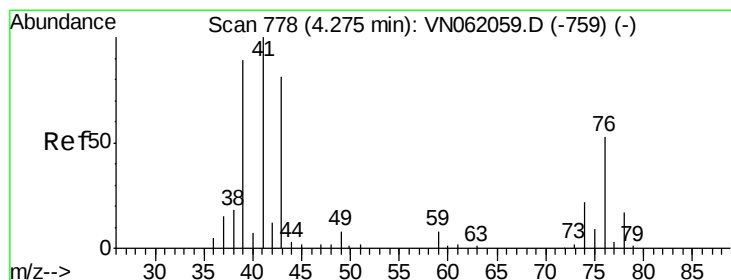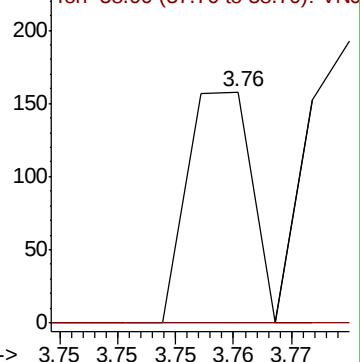

#18

Methyl Acetate

Concen: 0.492 ug/l

RT: 4.28 min Scan# 779

Delta R.T. 0.00 min

Lab File: VN062245.D


Acq: 30 Jun 2020 17:27

Tgt Ion: 43 Resp: 1008



Ion Ratio Lower Upper




43 100

74 23.4 22.9 34.3

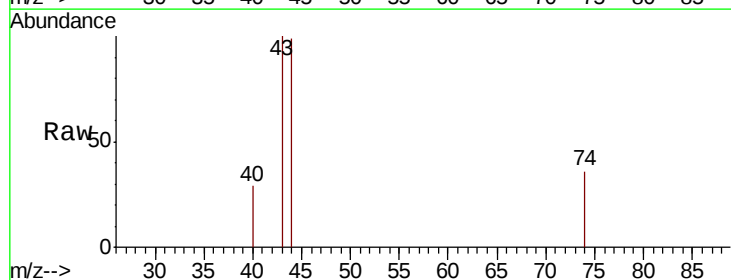

Abundance Ion 43.00 (42.70 to 43.70): VN062245.D (-685) (-)




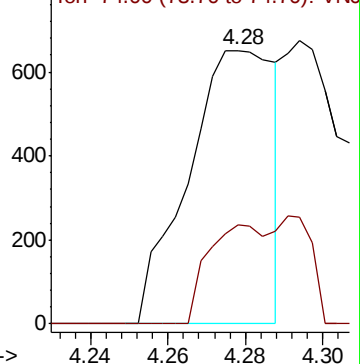


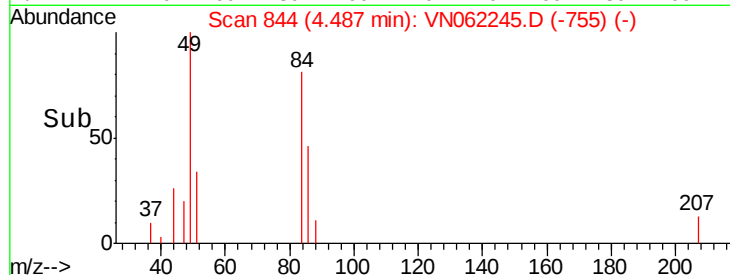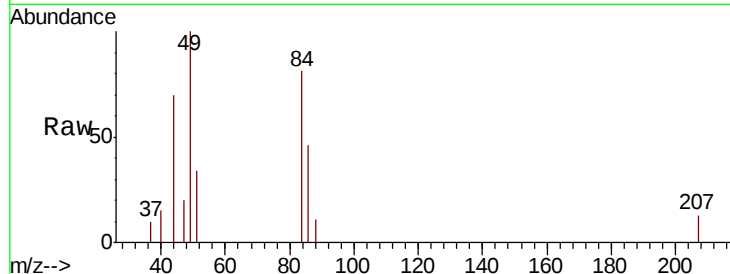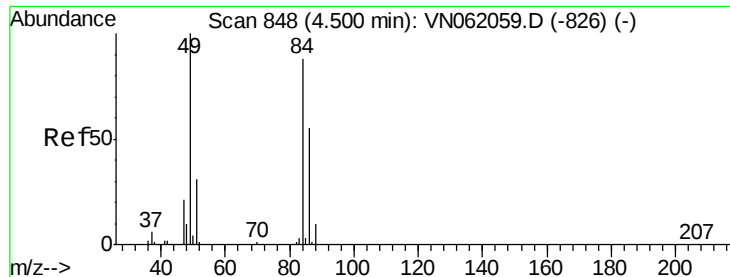

#20
Methvlene Chloride
Concen: 1.460 ug/l
RT: 4.49 min Scan# 844
Delta R.T. -0.01 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27


Instrument :
MSVOA_N
ClientSampleId :
DRUM-COMP


Tot Ion:	84	Resp:	3949
Ion	Ratio	Lower	Upper
84	100		
49	109.4	90.6	136.0
51	41.3	27.8	41.8
86	56.5	50.1	75.1

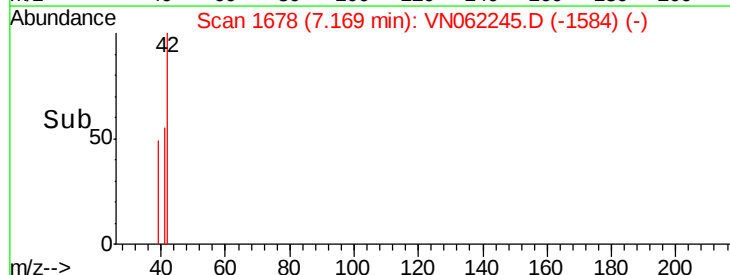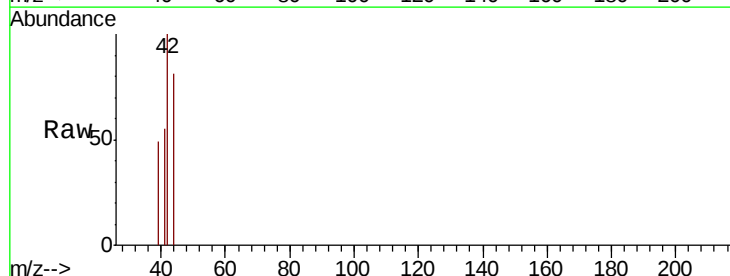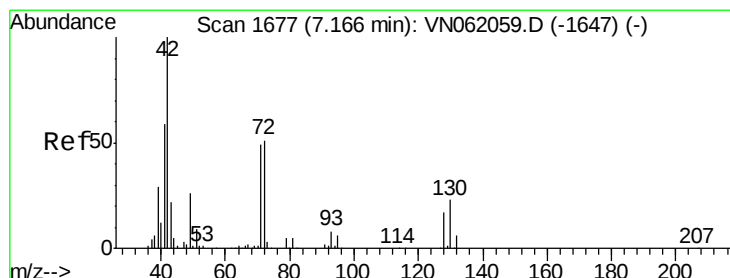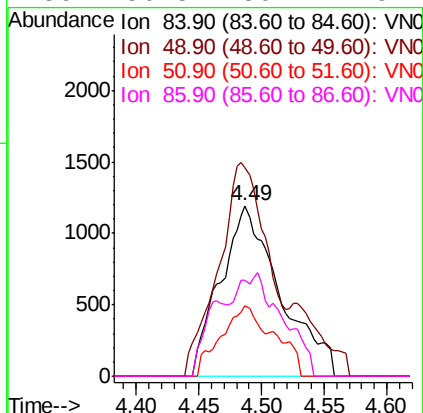

#29
Tetrahydrofuran
Concen: 1.168 ug/l
RT: 7.17 min Scan# 1678
Delta R.T. 0.00 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Tgt Ion:	42	Resp:	963
Ion	Ratio	Lower	Upper
42	100		
72	6.3	41.1	61.7#
71	3.0	38.2	57.4#




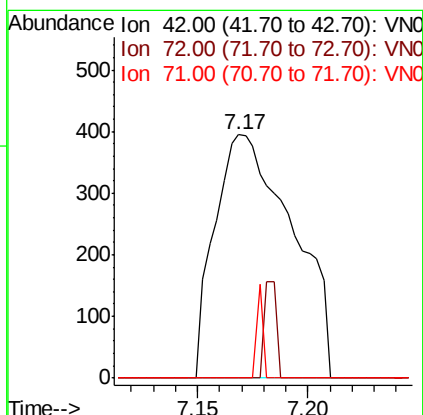




#31
Cyclohexane
Concen: 1.293 ug/l
RT: 7.59 min Scan# 1809
Delta R.T. -0.02 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27




Instrument :
MSVOA_N
ClientSampleId :
DRUM-COMP


Tot Ion: 56 Resp: 4602
Ion Ratio Lower Upper
56 100
69 41.0 28.0 42.0
84 48.5 76.1 114.1#

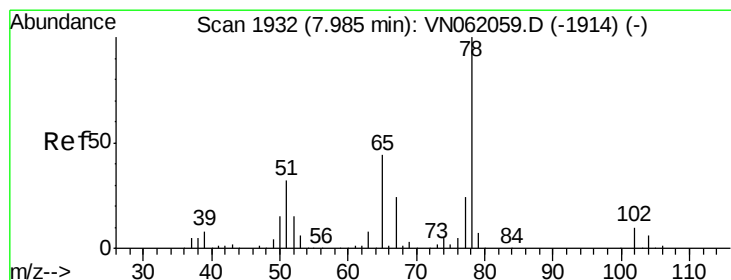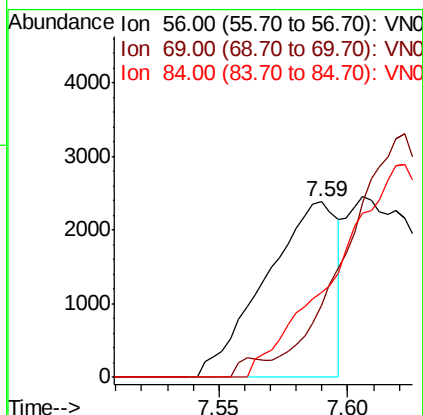

#33
1,2-Dichloroethane-d4
Concen: 54.291 ug/l
RT: 7.99 min Scan# 1932
Delta R.T. -0.00 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Tgt Ion: 65 Resp: 139840
Ion Ratio Lower Upper
65 100
67 51.4 0.0 106.2

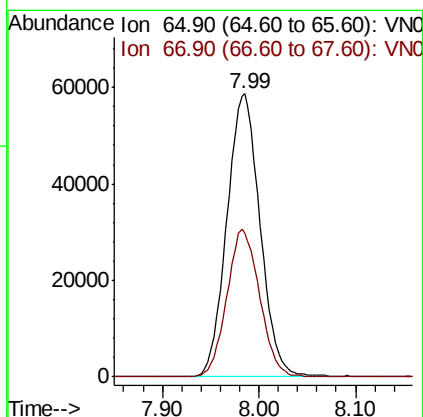


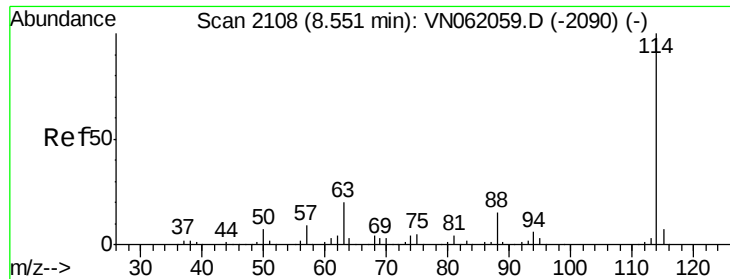




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2107
 Delta R.T. -0.00 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27

Instrument :
 MSVOA_N
 ClientSampleId :
 DRUM-COMP

Tot Ion:114 Resp: 352554
 Ion Ratio Lower Upper
 114 100
 63 20.1 0.0 39.2
 88 15.7 0.0 30.8

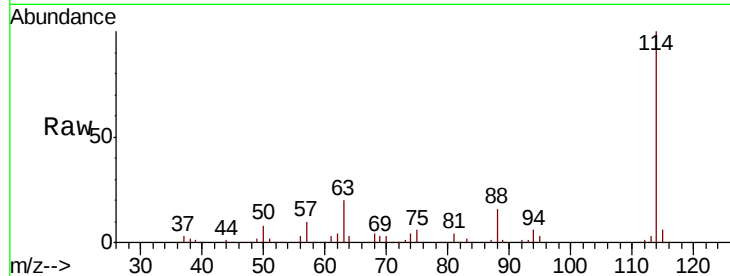


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

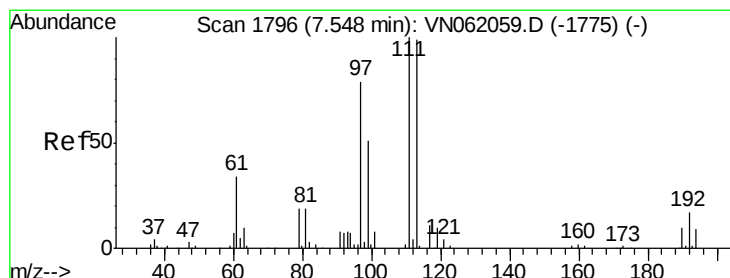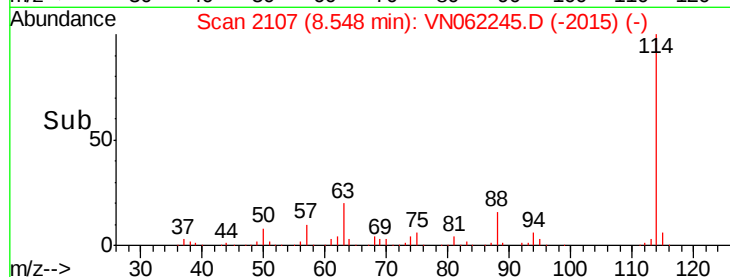
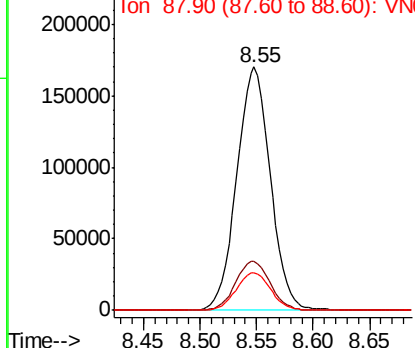



#35
 Dibromofluoromethane
 Concen: 49.026 ug/l
 RT: 7.54 min Scan# 1795
 Delta R.T. -0.00 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27

Tgt Ion:113 Resp: 110886
 Ion Ratio Lower Upper
 113 100
 111 102.6 82.2 123.4
 192 16.8 14.0 21.0

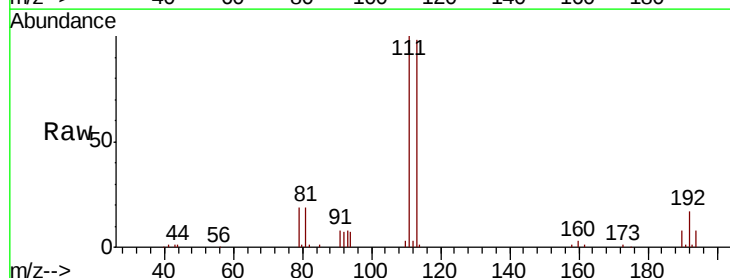

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



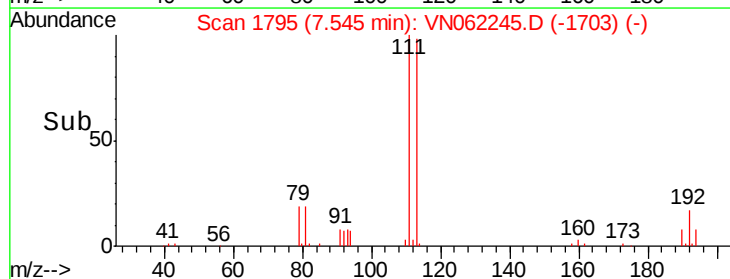
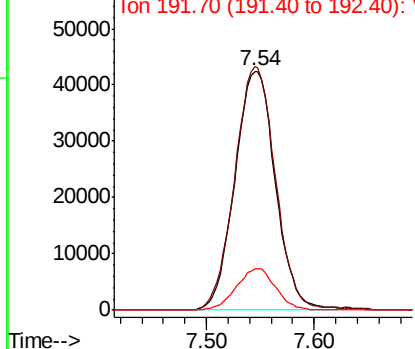




#36
 1,1-Dichloropropene
 Concen: 4.542 ug/l
 RT: 7.62 min Scan# 1818
 Delta R.T. -0.13 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27




Instrument :
 MSVOA_N
 ClientSampleId :
 DRUM-COMP


Tot Ion	Ratio	Lower	Upper
75	100		
110	4.1	17.9	53.8#
77	0.0	24.9	37.3#

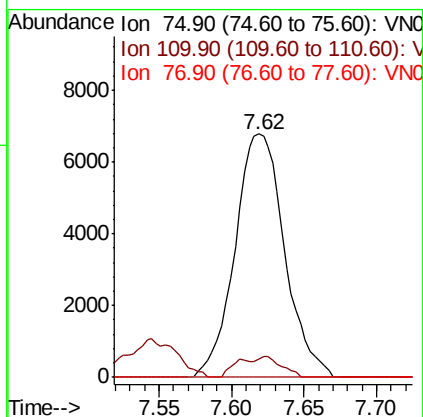

#38
 Carbon Tetrachloride
 Concen: 5.632 ug/l
 RT: 7.62 min Scan# 1819
 Delta R.T. -0.11 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27

Tgt Ion	Ratio	Lower	Upper
117	100		
119	6.4	78.2	117.2#
121	0.0	25.8	38.6#

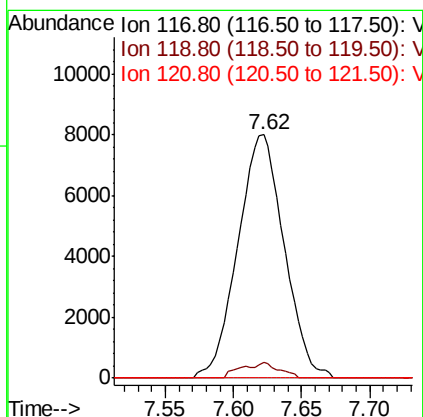







#39
Methylcyclohexane
Concen: 0.851 ug/l
RT: 9.04 min Scan# 2261
Delta R.T. -0.00 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Instrument :
MSVOA_N
ClientSampled :
DRUM-COMP

Tot Ion: 83 Resp: 3306
Ion Ratio Lower Upper
83 100
55 91.2 57.0 85.6#
98 45.0 39.0 58.6




Abundance Ion 83.00 (82.70 to 83.70): VN0
Ion 55.00 (54.70 to 55.70): VN0
Ion 98.00 (97.70 to 98.70): VN0


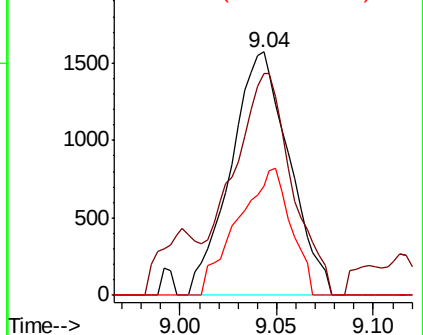



#41
Methacrylonitrile
Concen: 0.429 ug/l
RT: 7.18 min Scan# 1682
Delta R.T. 0.06 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Tgt Ion: 41 Resp: 584
Ion Ratio Lower Upper
41 100
39 5.5 44.2 66.2#
67 0.0 79.5 119.3#
52 0.0 32.3 48.5#



Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 39.00 (38.70 to 39.70): VN0
Ion 67.00 (66.70 to 67.70): VN0
Ion 52.00 (51.70 to 52.70): VN0

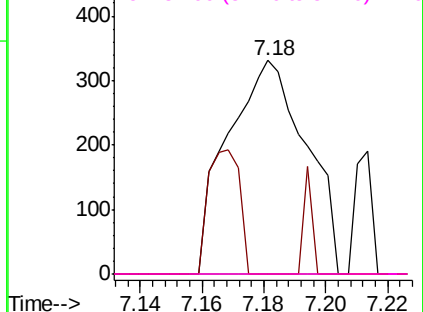



#43

Isopropyl Acetate

Concen: 0.701 ug/l

RT: 8.10 min Scan# 1969

Delta R.T. -0.02 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27

Instrument :

MSVOA_N

ClientSampleId :

DRUM-COMP


Tot Ion: 43 Resp: 3355

Ion Ratio Lower Upper

43 100

61 0.0 17.2 25.8#




87 0.0 12.1 18.1#



Abundance Ion 43.00 (42.70 to 43.70): VN062245.D (-1953) (-)

Ion 61.00 (60.70 to 61.70): VN062245.D (-1953) (-)

Ion 87.00 (86.70 to 87.70): VN062245.D (-1953) (-)

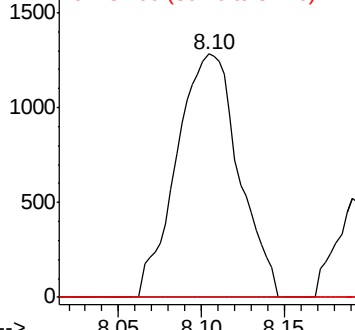

#48

Methyl methacrylate

Concen: 0.383 ug/l

RT: 9.10 min Scan# 2280

Delta R.T. -0.06 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27


Tgt Ion: 41 Resp: 821

Ion Ratio Lower Upper

41 100

69 0.0 80.7 121.1#



39 26.6 54.5 81.7#




Abundance Ion 41.00 (40.70 to 41.70): VN062245.D (-2287) (-)

Ion 69.00 (68.70 to 69.70): VN062245.D (-2287) (-)

Ion 39.00 (38.70 to 39.70): VN062245.D (-2287) (-)

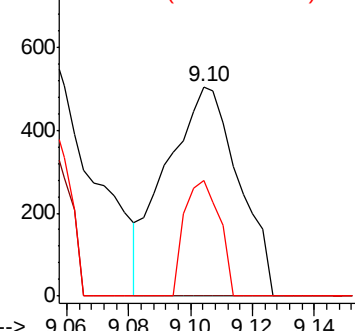



#50

Toluene-d8

Concen: 48.438 ug/l

RT: 10.06 min Scan# 2577

Delta R.T. -0.00 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27

Instrument :

MSVOA_N

ClientSampled :


DRUM-COMP

Tot Ion: 98 Resp: 437935




Ion Ratio Lower Upper

98 100

100 64.6 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VN062059.D (-2561) (-)

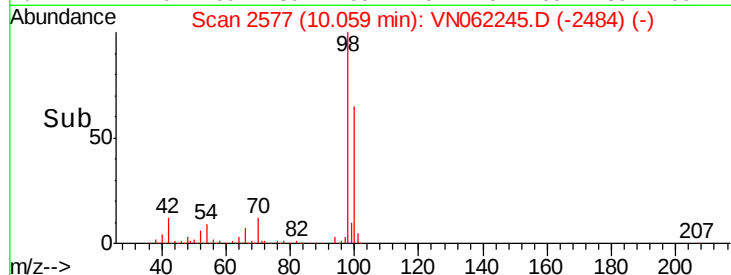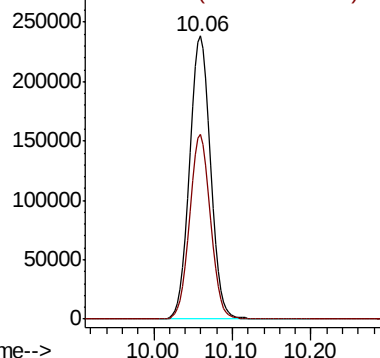

#52

Toluene

Concen: 15.599 ug/l

RT: 10.12 min Scan# 2597

Delta R.T. -0.00 min

Lab File: VN062245.D


Acq: 30 Jun 2020 17:27

Tgt Ion: 92 Resp: 102804



Ion Ratio Lower Upper


92 100

91 174.2 137.4 206.0



Abundance Ion 92.00 (91.70 to 92.70): VN062059.D (-2581) (-)

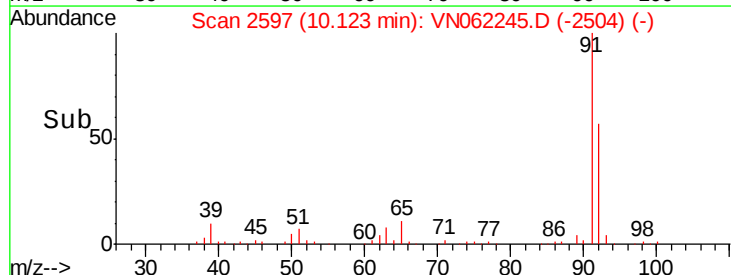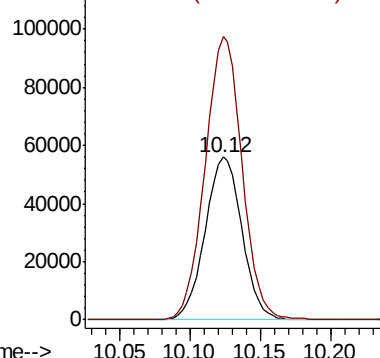



#53

t-1,3-Dichloropropene

Concen: 0.291 ug/l

RT: 10.12 min Scan# 2597

Delta R.T. -0.23 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27

Instrument :

MSVOA_N

ClientSampleId :





DRUM-COMP

Tot Ion: 75 Resp: 1167

Ion Ratio Lower Upper

75 100

77 142.9 25.5 38.3#

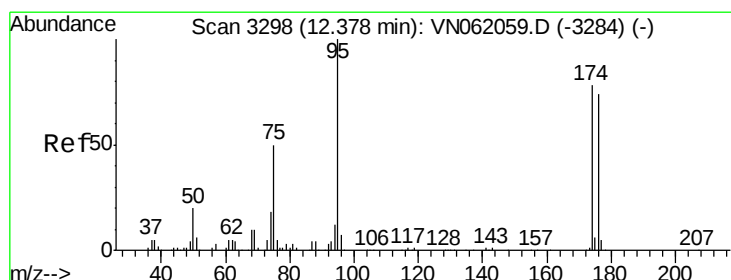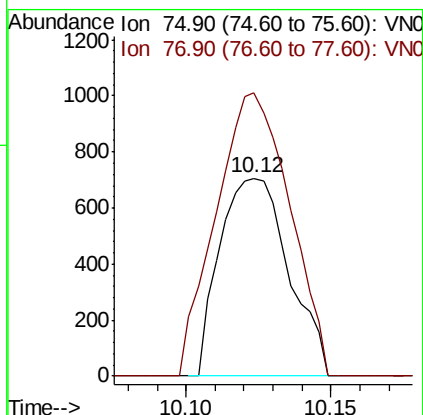

#62

4-Bromofluorobenzene

Concen: 44.480 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.00 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27




Tgt Ion: 95 Resp: 135869


Ion Ratio Lower Upper

95 100

174 75.7 0.0 154.8

176 70.7 0.0 147.4

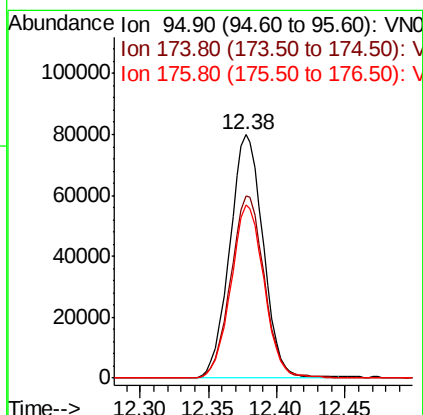







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. -0.00 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Instrument :
MSVOA_N
ClientSampleId :
DRUM-COMP

Tot Ion:117 Resp: 321038
Ion Ratio Lower Upper
117 100
82 57.7 43.8 65.8
119 31.0 25.2 37.8




Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V


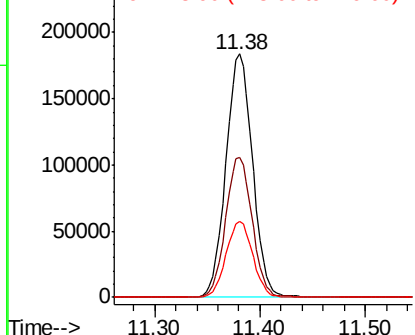



#71
Bromoform
Concen: 0.626 ug/l
RT: 12.38 min Scan# 3299
Delta R.T. 0.28 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Tgt Ion:173 Resp: 1085
Ion Ratio Lower Upper
173 100
175 597.7 24.7 74.1#
254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

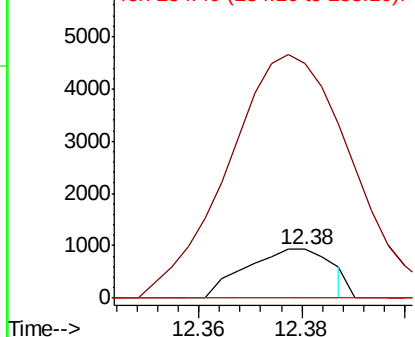



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27

Instrument :

MSVOA_N

ClientSampleId :

DRUM-COMP


Tot Ion:152 Resp: 125769

Ion Ratio Lower Upper

152 100

115 60.3 29.5 88.5




150 157.7 0.0 351.4



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

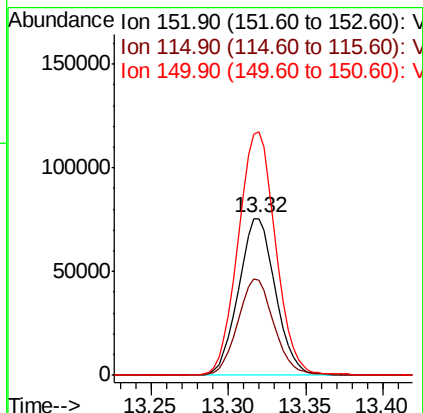

#74

N-ethyl acetate

Concen: 3.377 ug/l

RT: 12.07 min Scan# 3203

Delta R.T. 0.03 min

Lab File: VN062245.D

Acq: 30 Jun 2020 17:27

Tgt Ion: 43 Resp: 131


Ion Ratio Lower Upper

43 100

70 0.0 39.4 59.2#

55 0.0 21.7 32.5#

61 0.0 21.3 31.9#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V



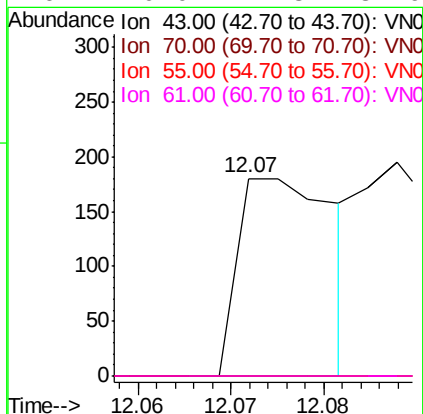





#76
 1,2,3-Trichloropropane
 Concen: 23.465 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. -0.15 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27




Instrument :
 MSVOA_N
 ClientSampleId :
 DRUM-COMP


Tot Ion: 75 Resp: 69472
 Ion Ratio Lower Upper
 75 100
 77 1.5 0.0 0.0#

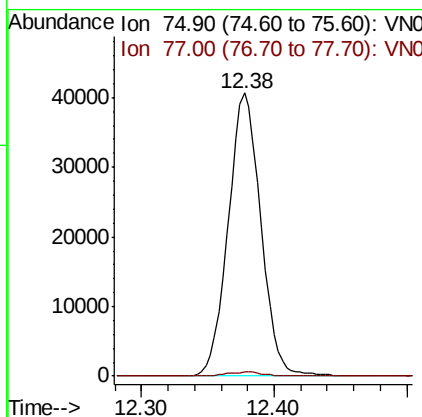

#79
 2-Chlorotoluene
 Concen: 0.243 ug/l
 RT: 12.64 min Scan# 3381
 Delta R.T. -0.00 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27

Tgt Ion: 91 Resp: 1633
 Ion Ratio Lower Upper
 91 100
 126 23.4 16.9 50.7



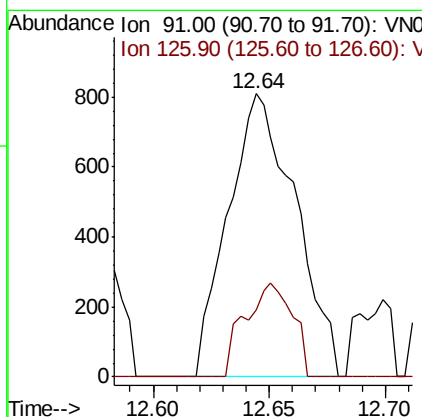





#80
 1,3,5-Trimethylbenzene
 Concen: 0.307 ug/l
 RT: 12.71 min Scan# 3401
 Delta R.T. -0.00 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27




Instrument :
 MSVOA_N
 ClientSampleId :
 DRUM-COMP


Tot Ion:105 Resp: 2423
 Ion Ratio Lower Upper
 105 100
 120 59.5 24.6 74.0

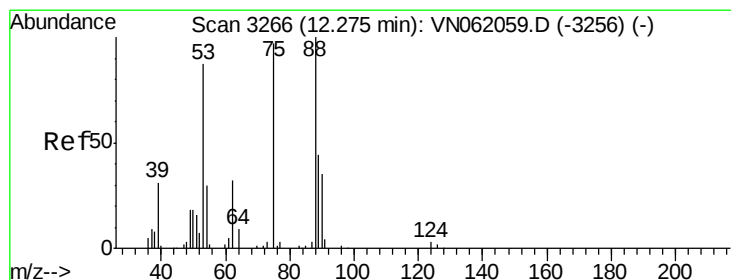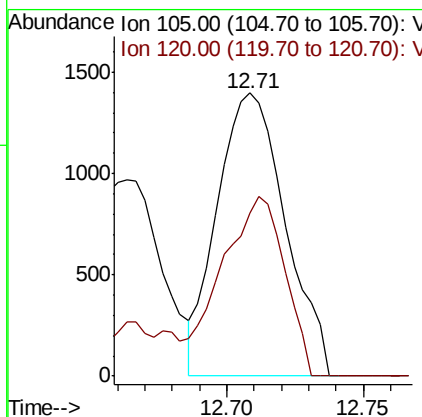

#81
 trans-1,4-Dichloro-2-butene
 Concen: 68.526 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. 0.10 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27

Tgt Ion: 75 Resp: 69472
 Ion Ratio Lower Upper
 75 100
 53 0.0 72.0 108.0#
 89 0.0 36.9 55.3#



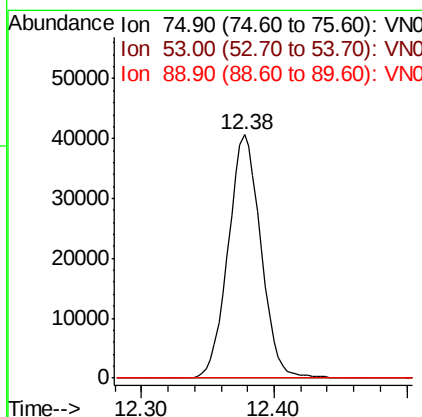





#82
4-Chlorotoluene
Concen: 0.203 ug/l
RT: 12.75 min Scan# 3413
Delta R.T. -0.00 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27




Instrument :
MSVOA_N
ClientSampleId :
DRUM-COMP


Tot Ion: 91 Resp: 1414
Ion Ratio Lower Upper
91 100
126 23.6 16.7 50.1

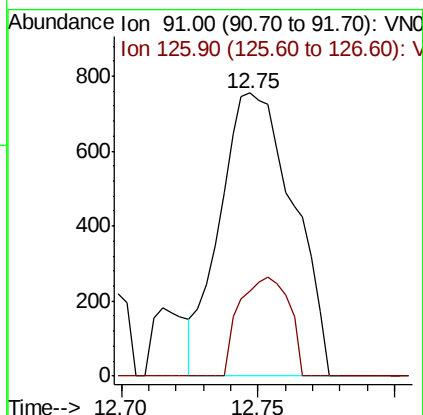

#84
1,2,4-Trimethylbenzene
Concen: 1.268 ug/l
RT: 13.01 min Scan# 3496
Delta R.T. -0.00 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Tgt Ion: 105 Resp: 9993
Ion Ratio Lower Upper
105 100
120 42.2 23.2 69.5


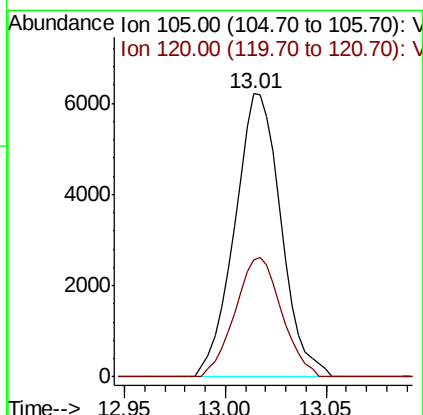






#86
 p-Isopropyltoluene
 Concen: 0.317 ug/l
 RT: 13.49 min Scan# 3643
 Delta R.T. 0.22 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27




Instrument :
 MSVOA_N
 ClientSampleId :
 DRUM-COMP


Tot Ion: 119 Resp: 2476
 Ion Ratio Lower Upper
 119 100
 134 36.3 13.0 39.0
 91 29.8 11.3 33.8

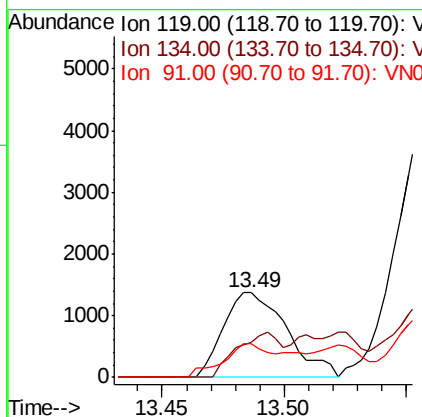

#89
 n-Butylbenzene
 Concen: 0.268 ug/l
 RT: 13.59 min Scan# 3675
 Delta R.T. -0.00 min
 Lab File: VN062245.D
 Acq: 30 Jun 2020 17:27

Tgt Ion: 91 Resp: 1745
 Ion Ratio Lower Upper
 91 100
 92 45.0 26.6 79.7
 134 0.0 12.3 36.9#



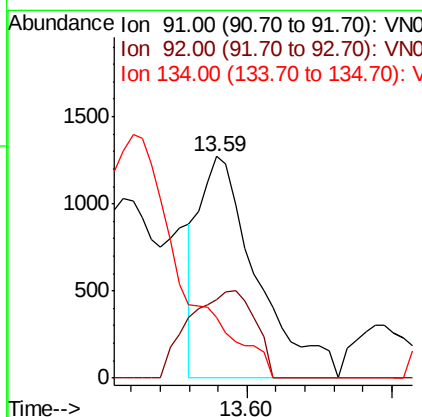





#90
Hexachloroethane
Concen: 0.636 ug/l
RT: 13.86 min Scan# 3759
Delta R.T. 0.01 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Instrument :
MSVOA_N
ClientSampleId :
DRUM-COMP

Tot Ion:117 Resp: 975
Ion Ratio Lower Upper
117 100
201 0.0 32.7 98.1#

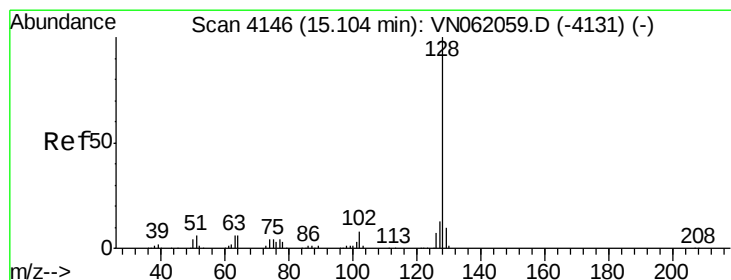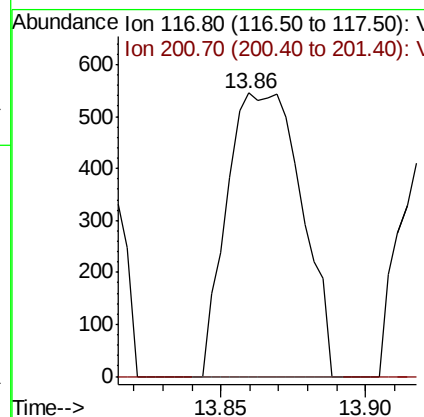

#95
Naphthalene
Concen: 5.700 ug/l
RT: 15.10 min Scan# 4146
Delta R.T. -0.00 min
Lab File: VN062245.D
Acq: 30 Jun 2020 17:27

Tgt Ion:128 Resp: 11107
Ion Ratio Lower Upper
128 100
127 13.6 10.5 15.7
129 11.9 8.6 13.0

