

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN063020\
 Data File : VN062271.D
 Acq On : 1 Jul 2020 5:07
 Operator : JC/MD
 Sample : L3153-14
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SP2-B

Quant Time: Jul 01 06:00:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	214721	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	438386	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	420252	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	149494	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	7.99	65	167091	55.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.90%	
35) Dibromofluoromethane	7.55	113	134289	47.75	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.50%	
50) Toluene-d8	10.06	98	562203	50.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.02%	
62) 4-Bromofluorobenzene	12.38	95	180256	47.46	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.92%	

Target Compounds


					Qvalue	
3) Chloromethane	2.03	50	289	Below Cal	#	41
8) Diethyl Ether	3.38	74	454	0.276	ug/l	78
11) Tert butyl alcohol	4.74	59	99	0.229	ug/l #	72
16) Acetone	3.78	43	91075	93.761	ug/l	94
18) Methyl Acetate	4.28	43	6767	2.825	ug/l #	67
20) Methylene Chloride	4.51	84	24917	8.829	ug/l	98
25) 2-Butanone	6.80	43	3964	2.691	ug/l	99
29) Tetrahydrofuran	7.17	42	238	0.247	ug/l #	46
31) Cyclohexane	7.63	56	5385	1.294	ug/l #	37
36) 1,1-Dichloropropene	7.63	75	19598	4.448	ug/l #	47
38) Carbon Tetrachloride	7.63	117	22797	5.488	ug/l #	16
43) Isopropyl Acetate	8.13	43	29407	4.944	ug/l	99
48) Methyl methacrylate	9.15	41	2263	0.849	ug/l #	6
51) 4-Methyl-2-Pentanone	9.95	43	5668	1.631	ug/l	93
54) cis-1,3-Dichloropropene	9.88	75	20154	3.793	ug/l #	68
56) Ethyl methacrylate	10.51	69	962	0.224	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	1210	0.218	ug/l #	42
59) 2-Hexanone	10.74	43	16965	6.760	ug/l #	54
71) Bromoform	12.38	173	1661	0.732	ug/l #	1
74) N-amyl acetate	12.07	43	130	3.372	ug/l #	38
76) 1,2,3-Trichloropropane	12.38	75	92902	26.399	ug/l #	100
78) n-propylbenzene	12.65	91	8202	0.620	ug/l #	53
79) 2-Chlorotoluene	12.65	91	8202	1.025	ug/l	94
81) trans-1,4-Dichloro-2-buten	12.38	75	92902	77.094	ug/l #	13
82) 4-Chlorotoluene	12.75	91	8039	0.971	ug/l	99
95) Naphthalene	15.10	128	69	4.004	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN063020\
Data File : VN062271.D
Acq On : 1 Jul 2020 5:07
Operator : JC/MD
Sample : L3153-14
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SP2-B

Quant Time: Jul 01 06:00:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 24 15:33:00 2020
Response via : Initial Calibration

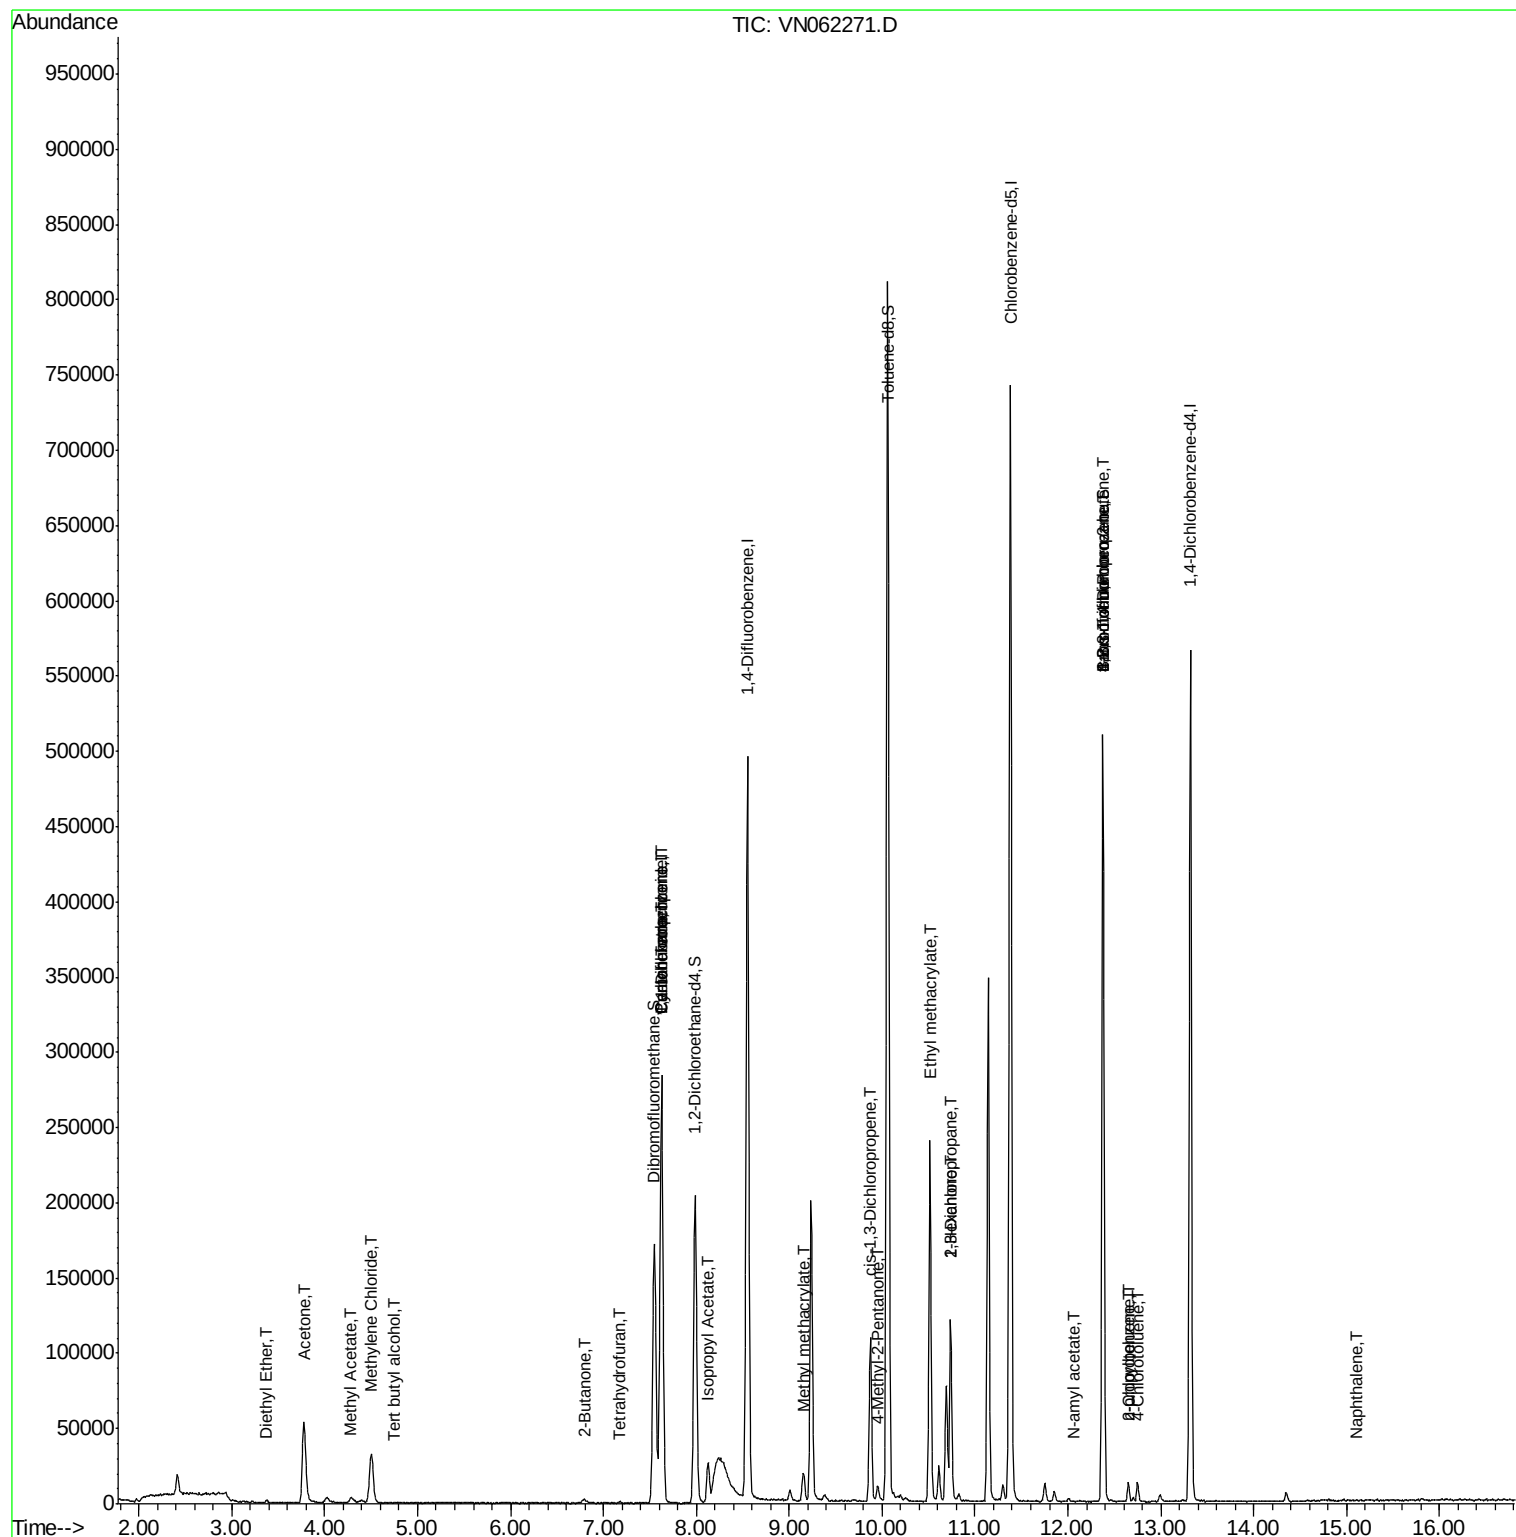



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062271.D

Acq: 1 Jul 2020 5:07

Instrument :

MSVOA_N

ClientSampled :


SP2-B

Tot Ion:168 Resp: 214721

Ion Ratio Lower Upper

168 100

99 62.6 45.8 68.8



Abundance Ion 167.90 (167.60 to 168.60): VN062271.D

Ion 98.90 (98.60 to 99.60): VN062271.D

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#3

Chloromethane

Concen: Below Cal

RT: 2.03 min Scan# 80

Delta R.T. -0.00 min

Lab File: VN062271.D


Acq: 1 Jul 2020 5:07

Tgt Ion: 50 Resp: 289

Ion Ratio Lower Upper

50 100

52 0.0 27.0 40.6#



Abundance Ion 49.90 (49.60 to 50.60): VN062271.D

Ion 51.90 (51.60 to 52.60): VN062271.D

2.03

300

250

200


150


100

50

0

Time--> 2.02 2.04 2.06





#8

Diethyl Ether

Concen: 0.276 ug/l

RT: 3.38 min Scan# 499

Delta R.T. 0.01 min

Lab File: VN062271.D

Acq: 1 Jul 2020 5:07

Instrument :

MSVOA_N

ClientSampleId :





SP2-B

Tot Ion: 74 Resp: 454

Ion Ratio Lower Upper

74 100

45 105.3 42.5 127.5

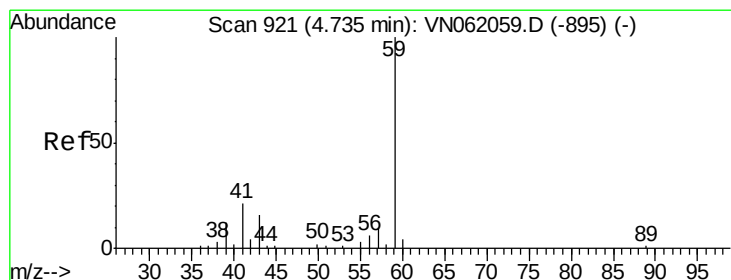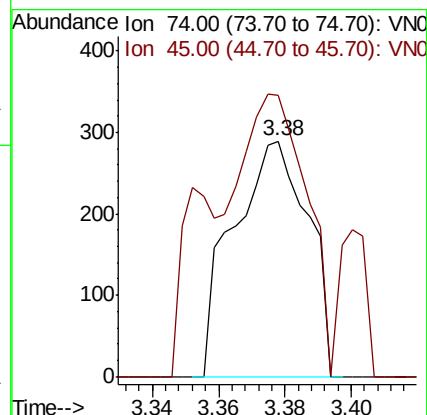

#11

Tert butyl alcohol

Concen: 0.229 ug/l

RT: 4.74 min Scan# 923

Delta R.T. 0.01 min

Lab File: VN062271.D




Acq: 1 Jul 2020 5:07


Tgt Ion: 59 Resp: 99

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#



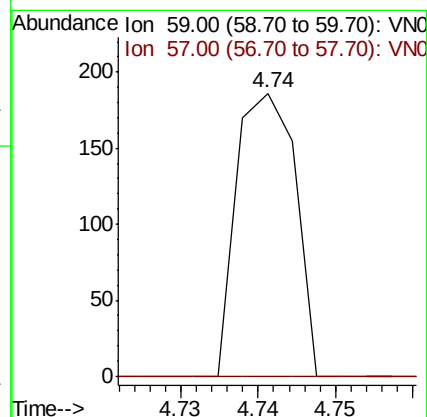





#16
 Acetone
 Concen: 93.761 ug/l
 RT: 3.78 min Scan# 623
 Delta R.T. 0.00 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07




Instrument :
 MSVOA_N
 ClientSampleId :
 SP2-B


Tot Ion: 43 Resp: 91075
 Ion Ratio Lower Upper
 43 100
 58 30.8 27.5 41.3

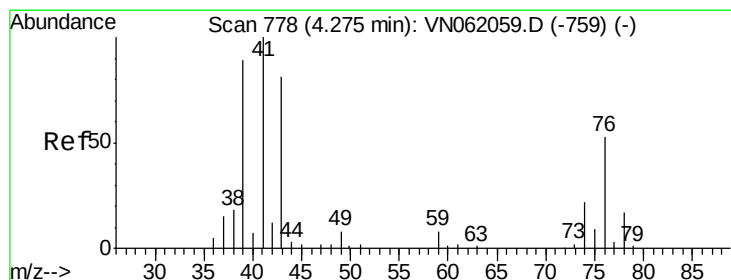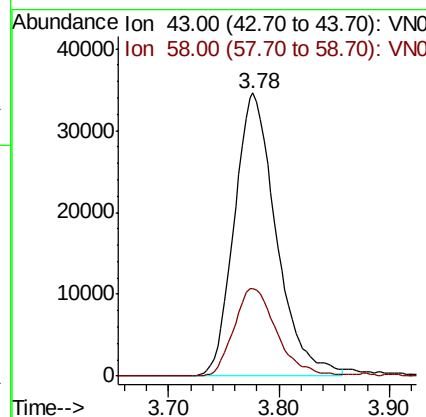

#18
 Methyl Acetate
 Concen: 2.825 ug/l
 RT: 4.28 min Scan# 781
 Delta R.T. 0.01 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07

Tgt Ion: 43 Resp: 6767
 Ion Ratio Lower Upper
 43 100
 74 10.9 22.9 34.3#

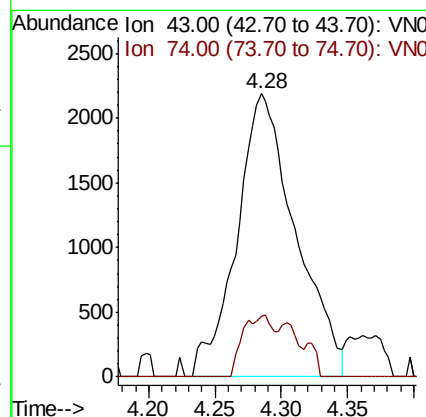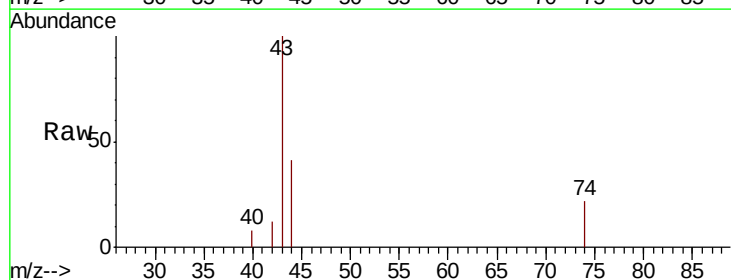







#20
Methvlene Chloride
Concen: 8.829 ug/l
RT: 4.51 min Scan# 850
Delta R.T. 0.01 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Instrument :
MSVOA_N
ClientSampled :
SP2-B

Tot Ion:	84	Resp:	24917
Ion	Ratio	Lower	Upper
84	100		
49	111.5	90.6	136.0
51	34.0	27.8	41.8
86	61.0	50.1	75.1

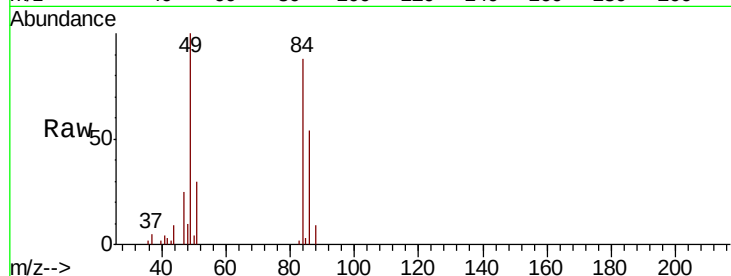


Abundance Ion 83.90 (83.60 to 84.60): VN0
Ion 48.90 (48.60 to 49.60): VN0
Ion 50.90 (50.60 to 51.60): VN0
Ion 85.90 (85.60 to 86.60): VN0


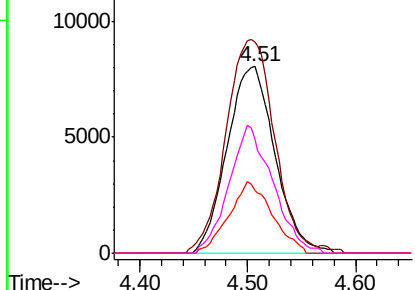



#25
2-Butanone
Concen: 2.691 ug/l
RT: 6.80 min Scan# 1563
Delta R.T. 0.02 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Tgt Ion:	43	Resp:	3964
Ion	Ratio	Lower	Upper
43	100		
72	31.8	24.8	37.2

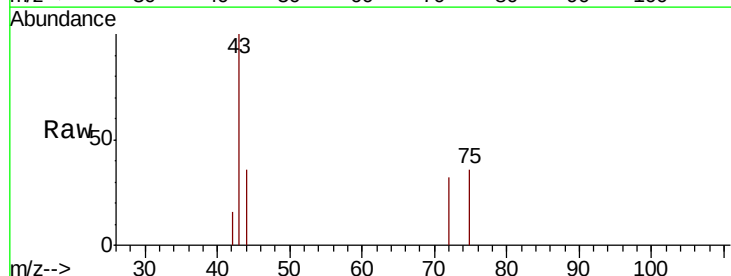

Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 72.00 (71.70 to 72.70): VN0




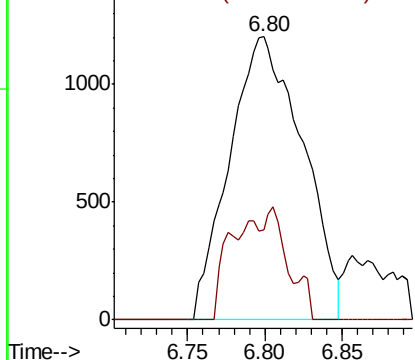




#29
Tetrahydrofuran
Concen: 0.247 ug/l
RT: 7.17 min Scan# 1677
Delta R.T. 0.00 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07




Instrument :
MSVOA_N
ClientSampled :
SP2-B


Tot Ion: 42 Resp: 238
Ion Ratio Lower Upper
42 100
72 78.2 41.1 61.7#
71 0.0 38.2 57.4#

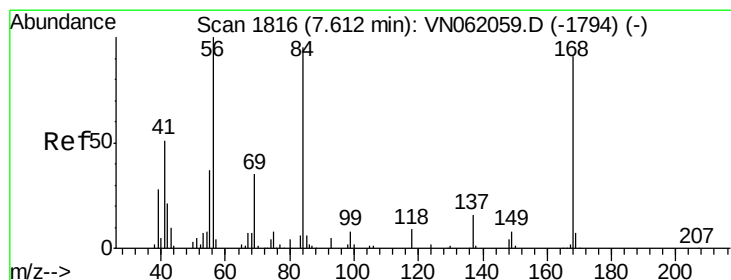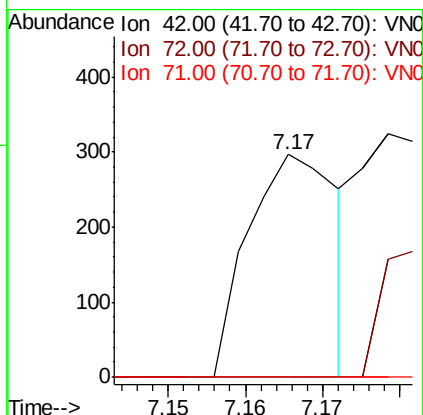

#31
Cyclohexane
Concen: 1.294 ug/l
RT: 7.63 min Scan# 1820
Delta R.T. 0.01 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Tgt Ion: 56 Resp: 5385
Ion Ratio Lower Upper
56 100
69 145.2 28.0 42.0#
84 110.9 76.1 114.1


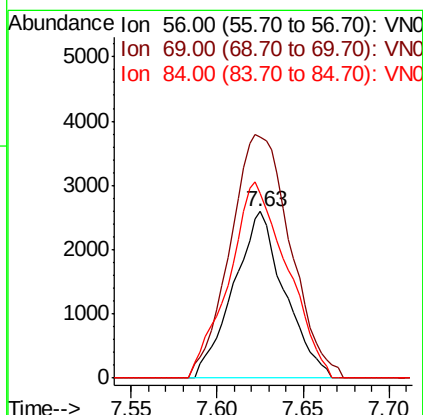




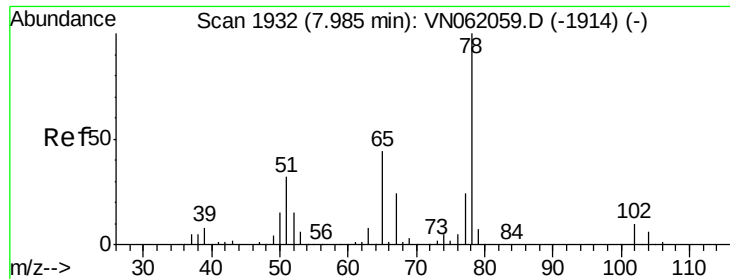

#33
 1,2-Dichloroethane-d4
 Concen: 55.452 ug/l
 RT: 7.99 min Scan# 1933
 Delta R.T. 0.00 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07




Instrument :
 MSVOA_N
 ClientSampled :
 SP2-B


Tot Ion: 65 Resp: 167091
 Ion Ratio Lower Upper
 65 100
 67 53.4 0.0 106.2

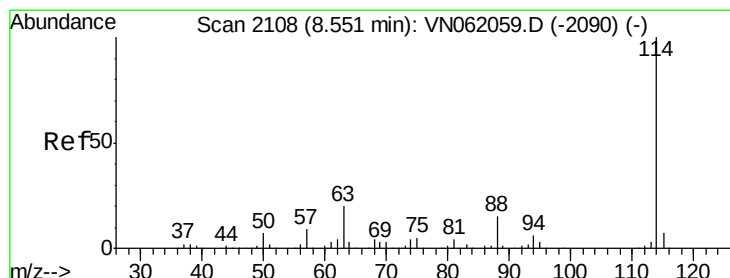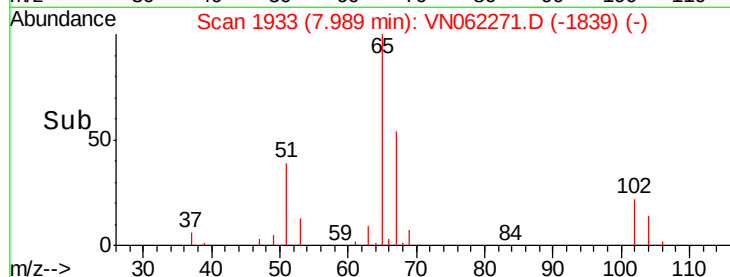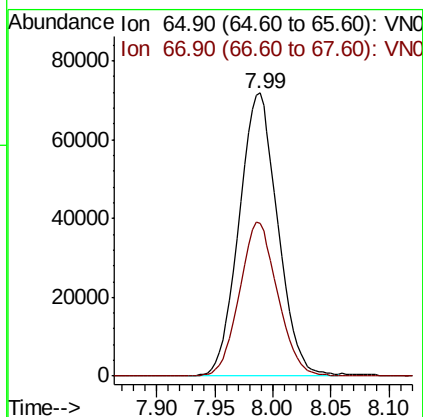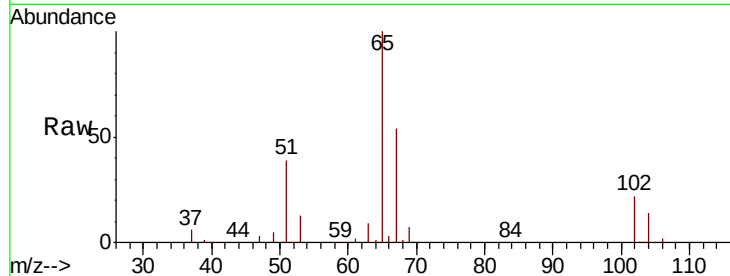

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. 0.00 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07

Tgt Ion: 114 Resp: 438386
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 39.2
 88 15.7 0.0 30.8


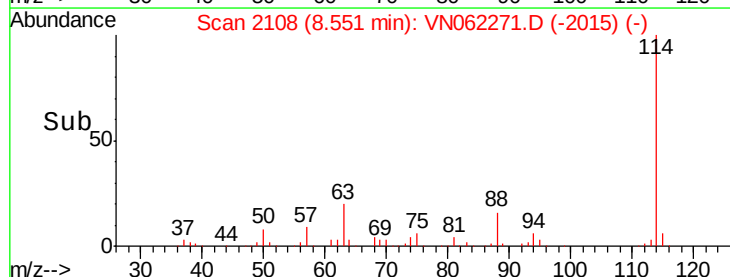
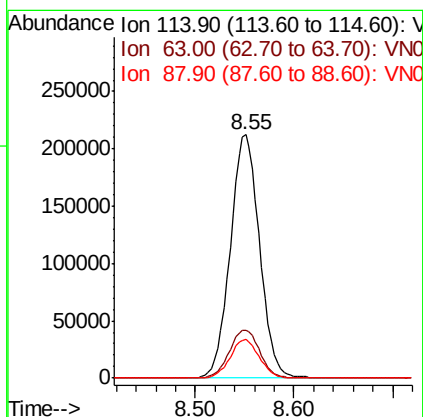
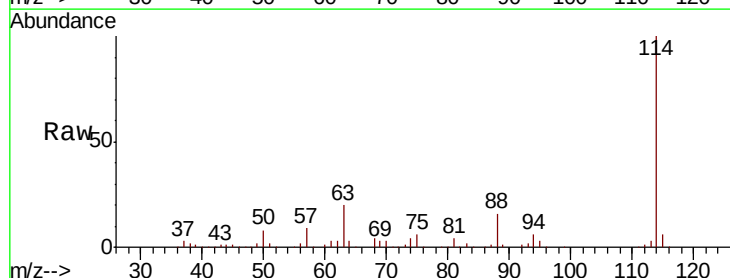


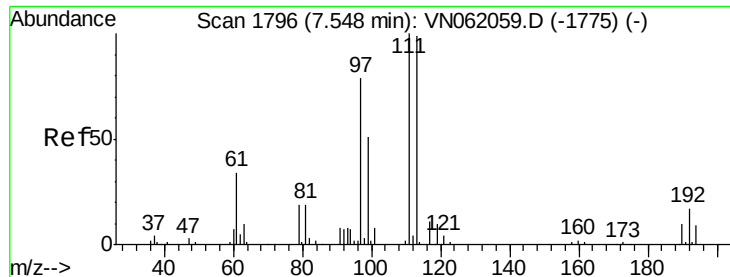

#35
 Dibromofluoromethane
 Concen: 47.748 ug/l
 RT: 7.55 min Scan# 1796
 Delta R.T. -0.00 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07




Instrument :
 MSVOA_N
 ClientSampleId :
 SP2-B


Tot Ion:113 Resp: 134289
 Ion Ratio Lower Upper
 113 100
 111 103.6 82.2 123.4
 192 16.9 14.0 21.0

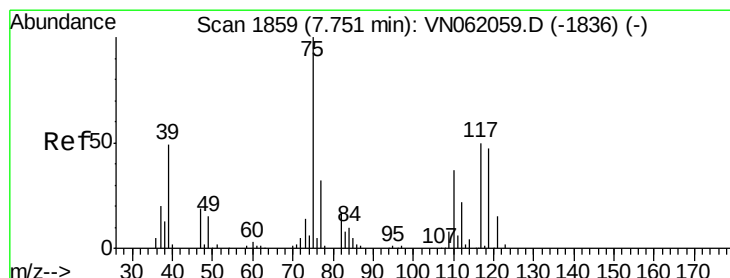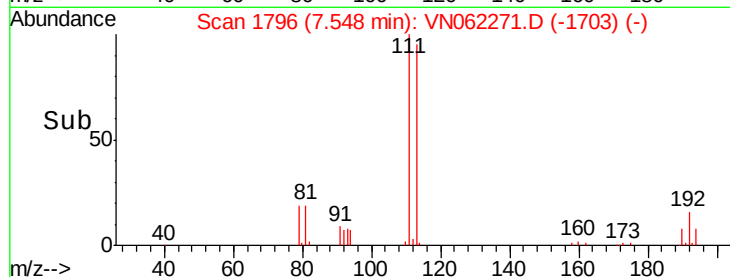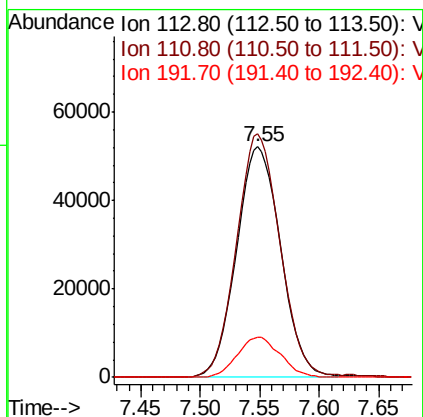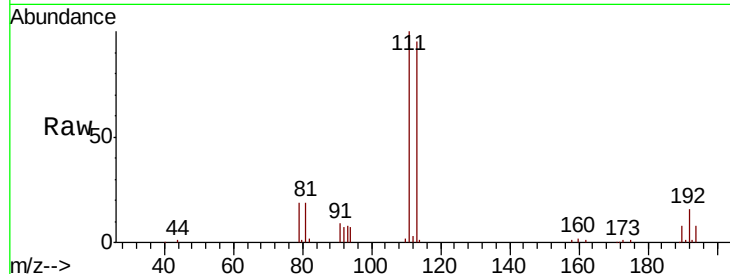

#36
 1,1-Dichloropropene
 Concen: 4.448 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.13 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07

Tgt Ion: 75 Resp: 19598
 Ion Ratio Lower Upper
 75 100
 110 6.8 17.9 53.8#
 77 0.0 24.9 37.3#

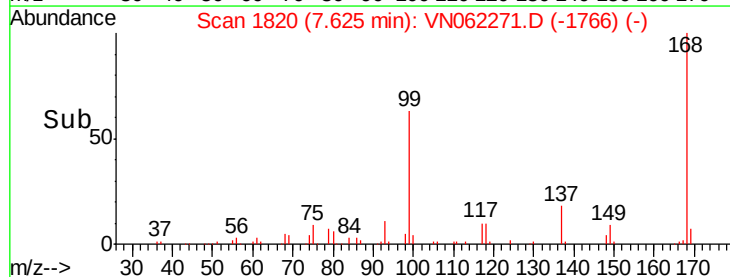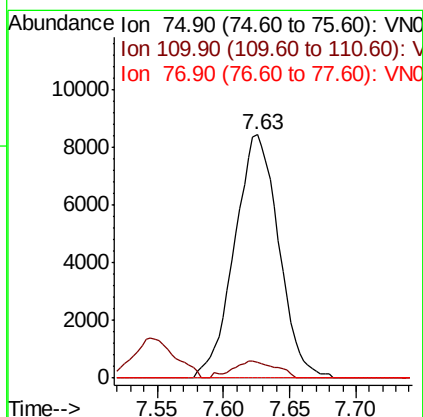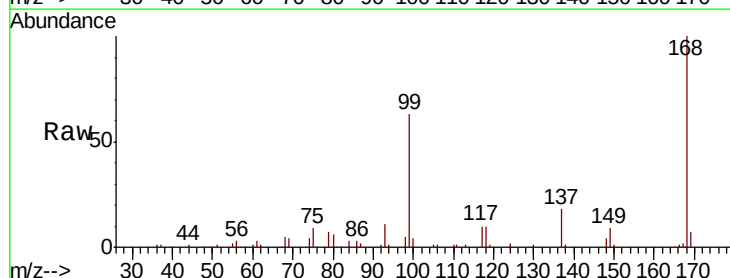







#38
Carbon Tetrachloride
Concen: 5.488 ug/l
RT: 7.63 min Scan# 1821
Delta R.T. -0.10 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Instrument :
MSVOA_N
ClientSampleId :
SP2-B

Tot Ion:117 Resp: 22797
Ion Ratio Lower Upper
117 100
119 6.7 78.2 117.2#
121 0.0 25.8 38.6#

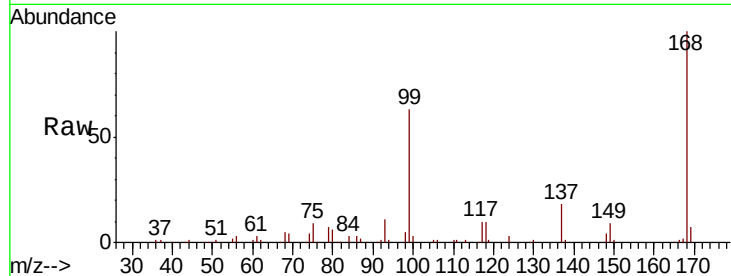


Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

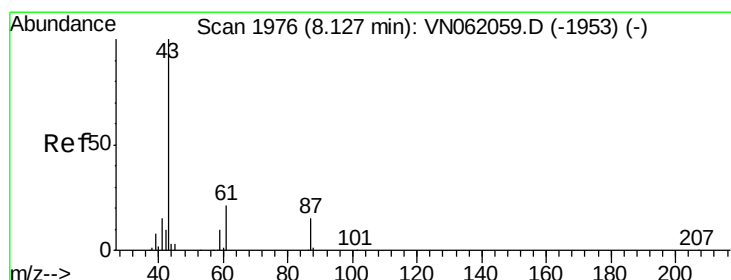
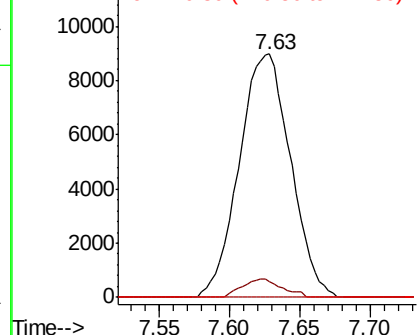



#43
Isopropyl Acetate
Concen: 4.944 ug/l
RT: 8.13 min Scan# 1977
Delta R.T. 0.00 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Tgt Ion: 43 Resp: 29407
Ion Ratio Lower Upper
43 100
61 22.3 17.2 25.8
87 14.7 12.1 18.1



Abundance Ion 43.00 (42.70 to 43.70): V
Ion 61.00 (60.70 to 61.70): V
Ion 87.00 (86.70 to 87.70): V

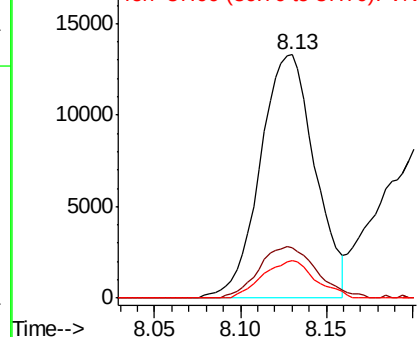







#48
Methvl methacrylate
Concen: 0.849 ug/l
RT: 9.15 min Scan# 2295
Delta R.T. -0.01 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Instrument :
MSVOA_N
ClientSampleId :
SP2-B

Tot Ion: 41 Resp: 2263
Ion Ratio Lower Upper
41 100
69 0.0 80.7 121.1#
39 0.0 54.5 81.7#

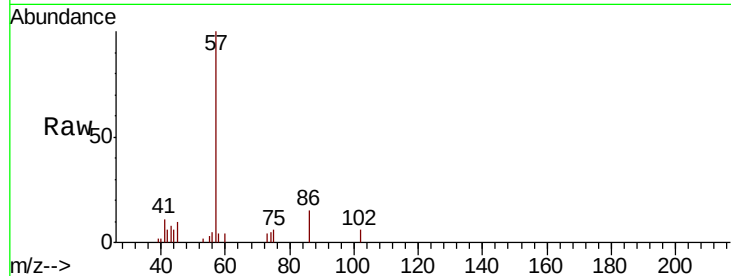


Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0


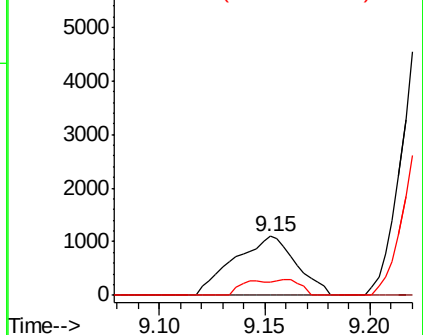



#50
Toluene-d8
Concen: 50.008 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. -0.00 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Tgt Ion: 98 Resp: 562203
Ion Ratio Lower Upper
98 100
100 64.9 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0



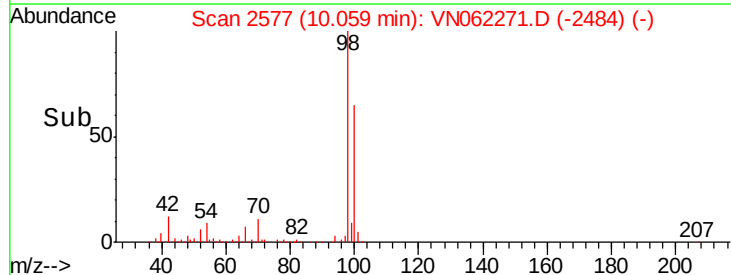
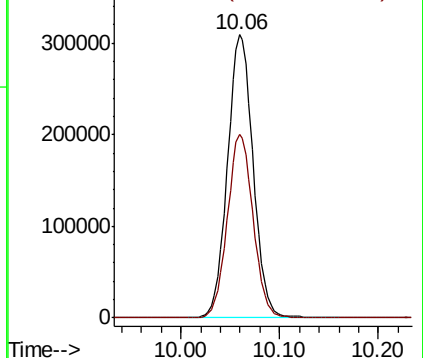




#51
 4-Methyl-2-Pentanone
 Concen: 1.631 ug/l
 RT: 9.95 min Scan# 2544
 Delta R.T. 0.00 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07




Instrument :
 MSVOA_N
 ClientSampled :
 SP2-B


Tot Ion: 43 Resp: 5668
 Ion Ratio Lower Upper
 43 100
 58 47.2 34.2 51.2

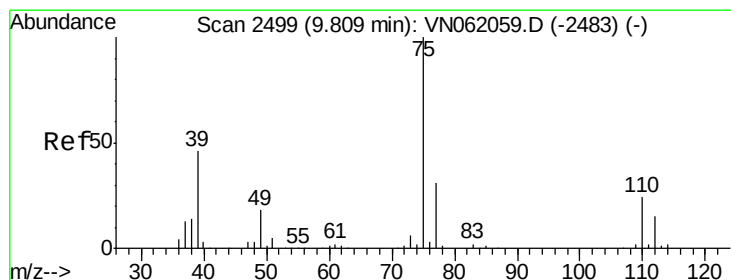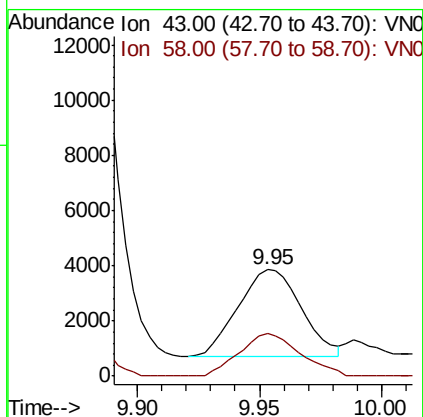

#54
 cis-1,3-Dichloropropene
 Concen: 3.793 ug/l
 RT: 9.88 min Scan# 2520
 Delta R.T. 0.07 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07

Tgt Ion: 75 Resp: 20154
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.6#
 39 36.4 36.9 55.3#

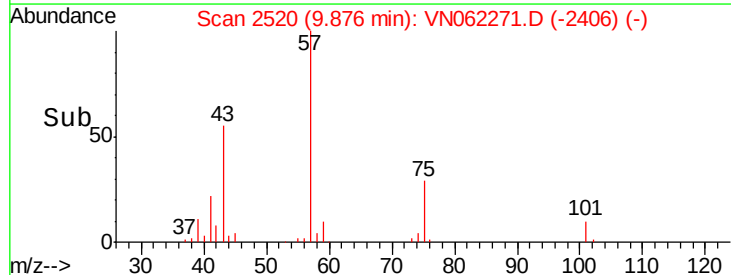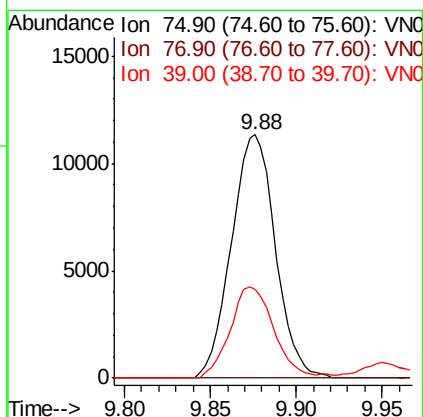



#56

Ethyl methacrylate

Concen: 0.224 ug/l

RT: 10.51 min Scan# 2717

Delta R.T. 0.11 min

Lab File: VN062271.D

Acq: 1 Jul 2020 5:07

Instrument :

MSVOA_N

ClientSampled :

SP2-B


Tot Ion: 69 Resp: 962

Ion Ratio Lower Upper

69 100

41 4809.9 46.6 70.0#




39 2186.2 31.0 46.4#

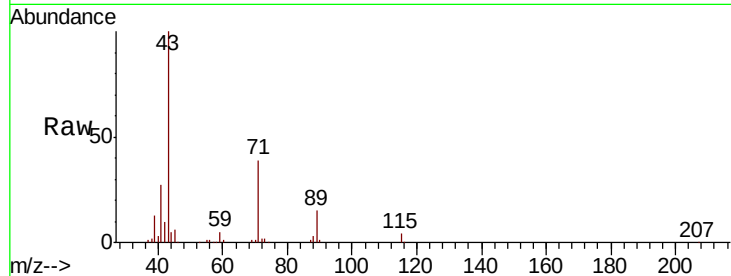

Abundance Ion 69.00 (68.70 to 69.70): VN062271.D (-2669) (-)

Ion 41.00 (40.70 to 41.70): VN062271.D (-2669) (-)

Ion 39.00 (38.70 to 39.70): VN062271.D (-2669) (-)

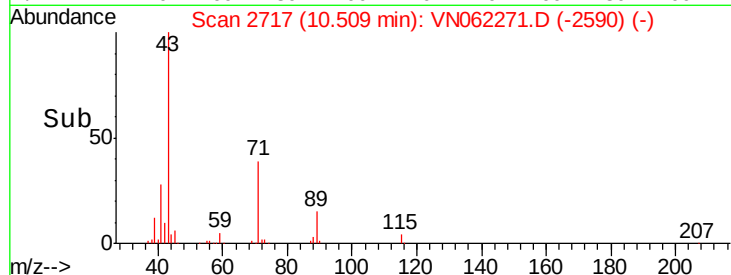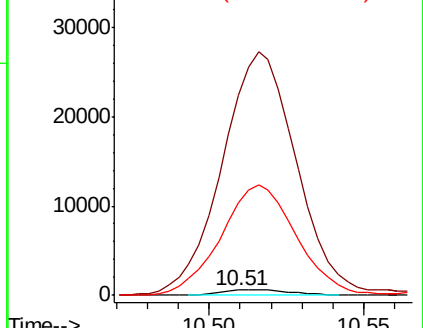

#57

1,3-Dichloropropane

Concen: 0.218 ug/l

RT: 10.74 min Scan# 2789

Delta R.T. 0.06 min

Lab File: VN062271.D


Acq: 1 Jul 2020 5:07

Tgt Ion: 76 Resp: 1210

Ion Ratio Lower Upper



76 100


78 0.0 25.8 38.8#



Abundance Ion 75.90 (75.60 to 76.60): VN062271.D (-2676) (-)

Ion 77.90 (77.60 to 78.60): VN062271.D (-2676) (-)




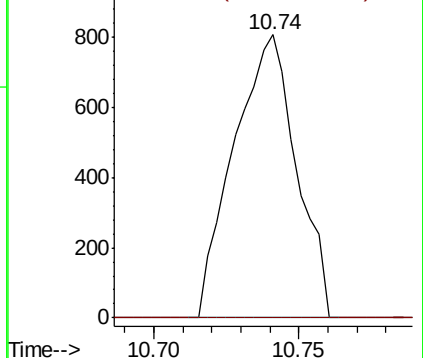




#59
2-Hexanone
Concen: 6.760 ug/l
RT: 10.74 min Scan# 2788
Delta R.T. 0.02 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07




Instrument :
MSVOA_N
ClientSampled :
SP2-B


Tot Ion: 43 Resp: 16965
Ion Ratio Lower Upper
43 100
58 24.2 29.5 88.5#

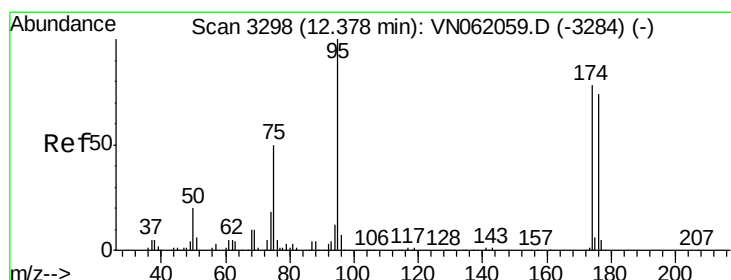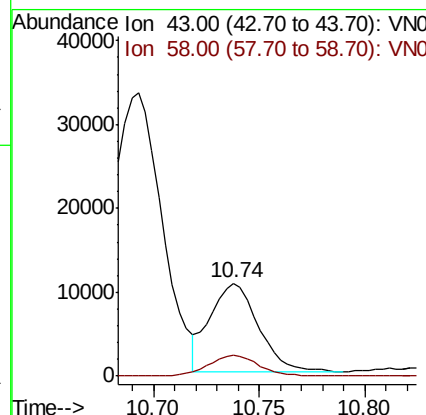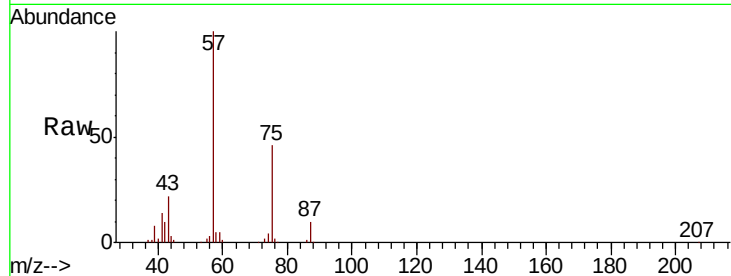

#62
4-Bromofluorobenzene
Concen: 47.457 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.00 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Tgt Ion: 95 Resp: 180256
Ion Ratio Lower Upper
95 100
174 72.3 0.0 154.8
176 69.5 0.0 147.4

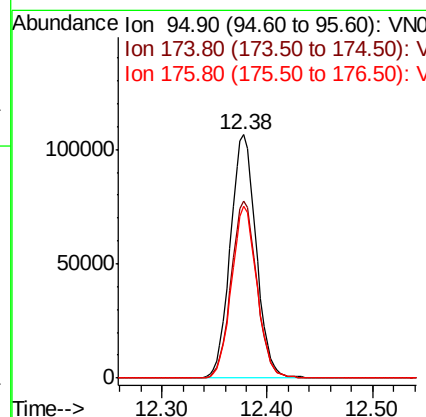







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. 0.00 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Instrument :
MSVOA_N
ClientSampleId :
SP2-B

Tot Ion:117 Resp: 420252
Ion Ratio Lower Upper
117 100
82 58.0 43.8 65.8
119 31.4 25.2 37.8

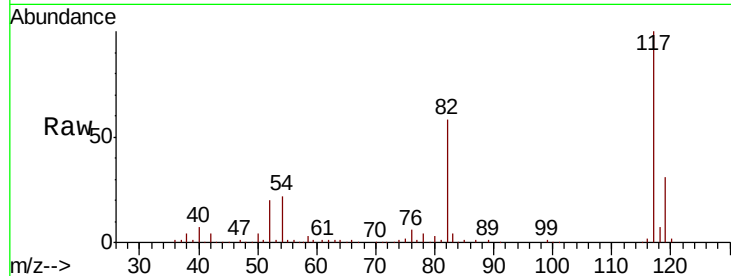


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V


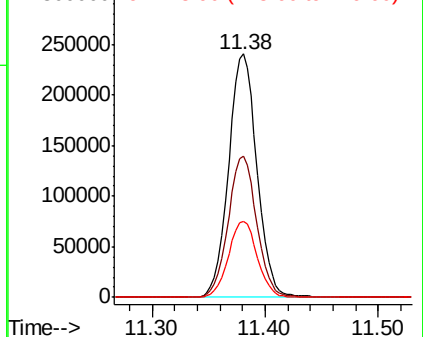



#71
Bromoform
Concen: 0.732 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.28 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Tgt Ion:173 Resp: 1661
Ion Ratio Lower Upper
173 100
175 492.9 24.7 74.1#
254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

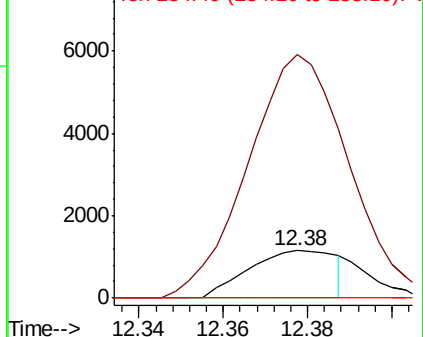



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062271.D

Acq: 1 Jul 2020 5:07

Instrument :

MSVOA_N

ClientSampled :

SP2-B


Tot Ion:152 Resp: 149494

Ion Ratio Lower Upper

152 100

115 60.1 29.5 88.5




150 156.4 0.0 351.4

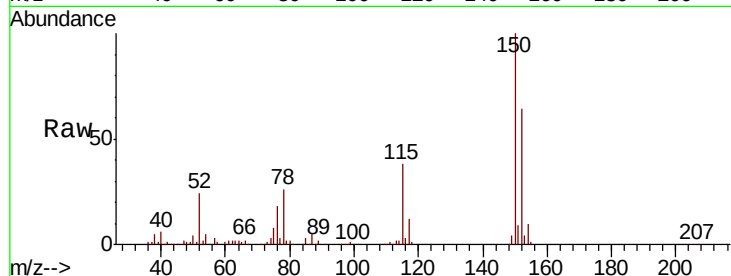

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

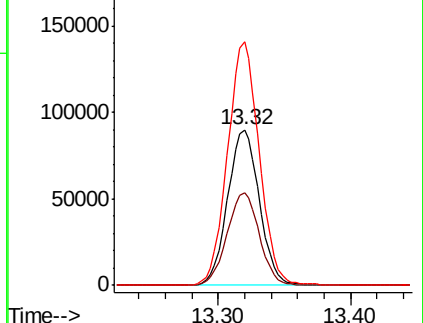

#74

N-ethyl acetate

Concen: 3.372 ug/l

RT: 12.07 min Scan# 3201

Delta R.T. 0.02 min

Lab File: VN062271.D

Acq: 1 Jul 2020 5:07

Tgt Ion: 43 Resp: 130


Ion Ratio Lower Upper

43 100

70 0.0 39.4 59.2#

55 0.0 21.7 32.5#

61 0.0 21.3 31.9#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V

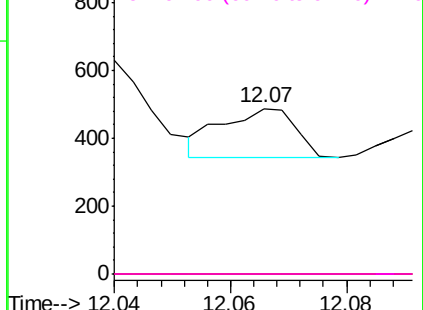

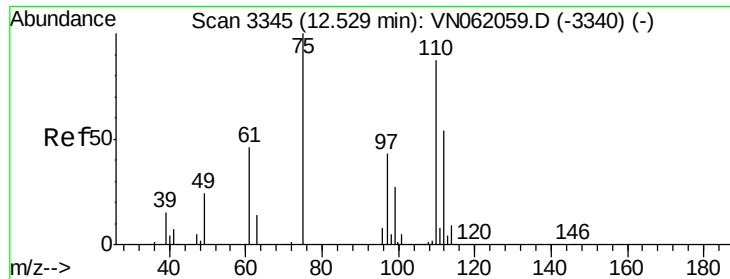

#76

1,2,3-Trichloropropane

Concen: 26.399 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.15 min

Lab File: VN062271.D

Acq: 1 Jul 2020 5:07

Instrument :

MSVOA_N

ClientSampled :


SP2-B

Tot Ion: 75 Resp: 92902

Ion Ratio Lower Upper




75 100

77 1.2 0.0 0.0#

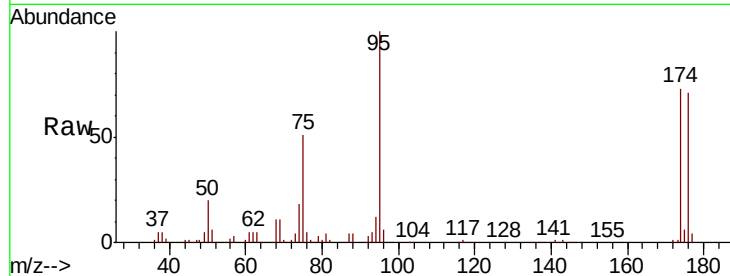

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

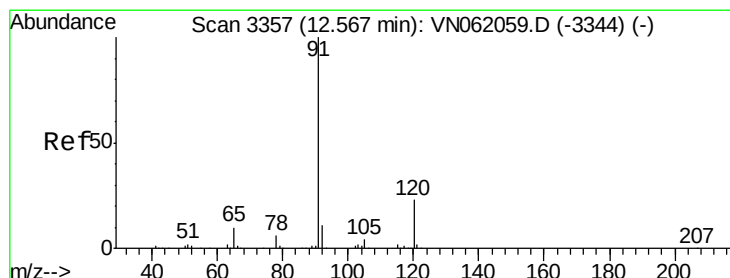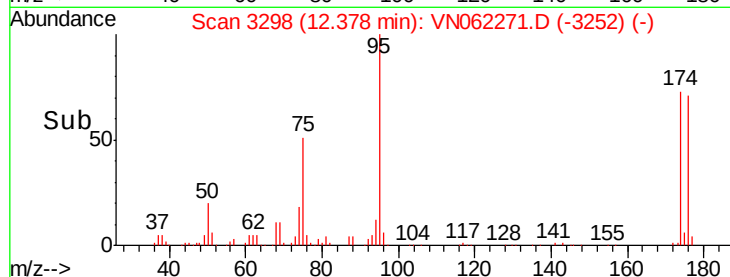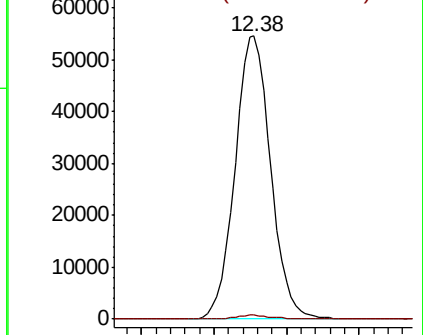

#78

n-propylbenzene

Concen: 0.620 ug/l

RT: 12.65 min Scan# 3383

Delta R.T. 0.08 min

Lab File: VN062271.D


Acq: 1 Jul 2020 5:07

Tgt Ion: 91 Resp: 8202

Ion Ratio Lower Upper



91 100


120 0.0 11.4 34.1#

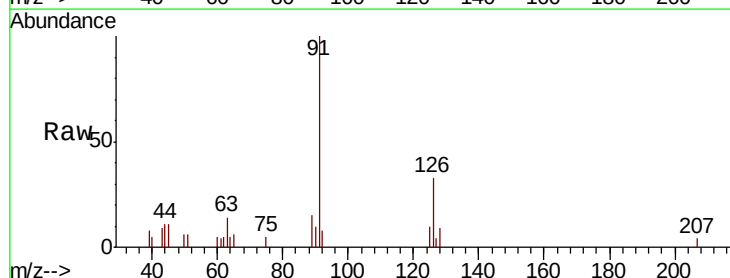

Abundance Ion 91.00 (90.70 to 91.70): VN0

Ion 120.00 (119.70 to 120.70): V



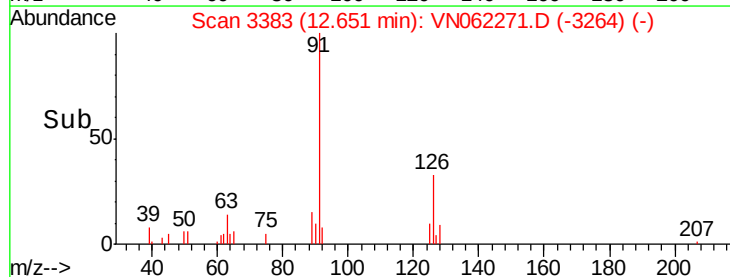
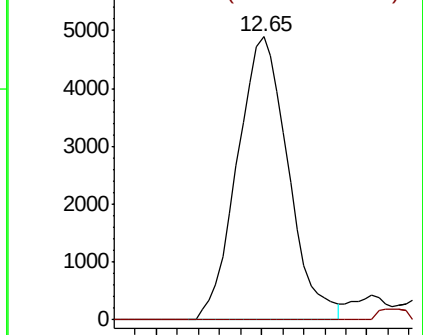




#79
 2-Chlorotoluene
 Concen: 1.025 ug/l
 RT: 12.65 min Scan# 3383
 Delta R.T. 0.00 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07




Instrument :
 MSVOA_N
 ClientSampled :
 SP2-B


Tot Ion: 91 Resp: 8202
 Ion Ratio Lower Upper
 91 100
 126 30.3 16.9 50.7

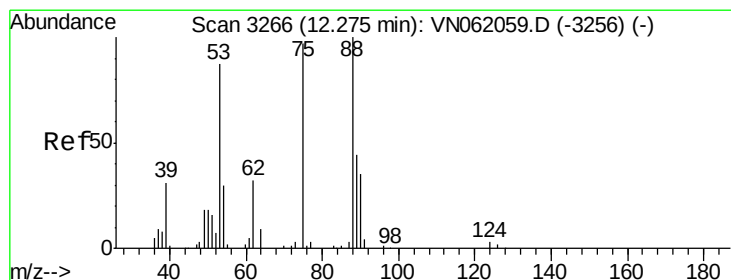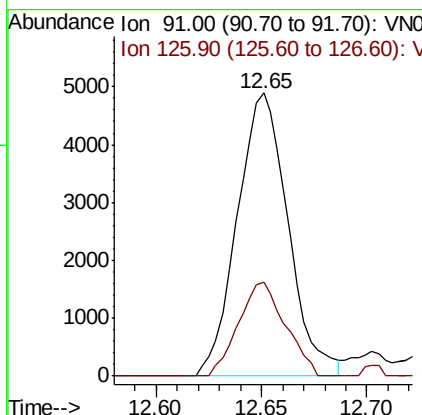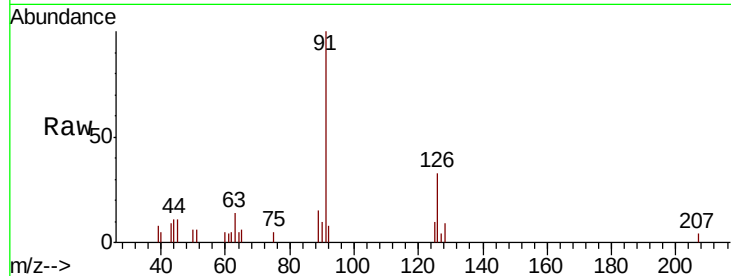

#81
 trans-1,4-Dichloro-2-butene
 Concen: 77.094 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. 0.10 min
 Lab File: VN062271.D
 Acq: 1 Jul 2020 5:07

Tgt Ion: 75 Resp: 92902
 Ion Ratio Lower Upper
 75 100
 53 0.0 72.0 108.0#
 89 0.0 36.9 55.3#



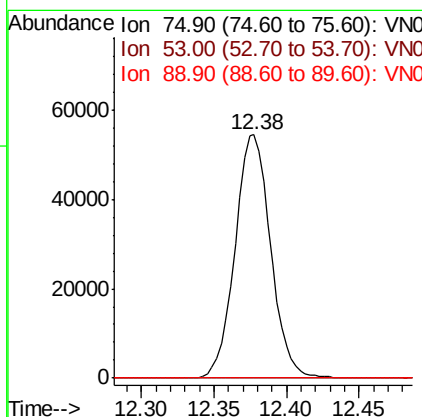



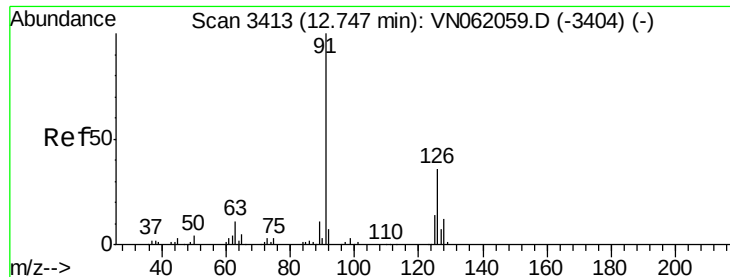

#82
4-Chlorotoluene
Concen: 0.971 ug/l
RT: 12.75 min Scan# 3414
Delta R.T. 0.00 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Instrument :
MSVOA_N
ClientSampled :
SP2-B

Tot Ion: 91 Resp: 8039
Ion Ratio Lower Upper
91 100
126 34.2 16.7 50.1

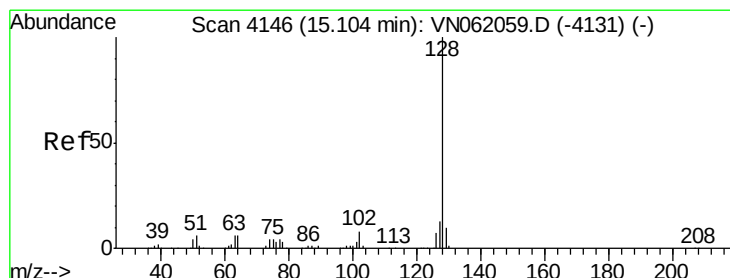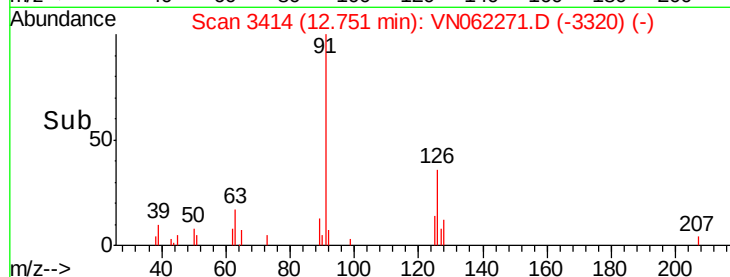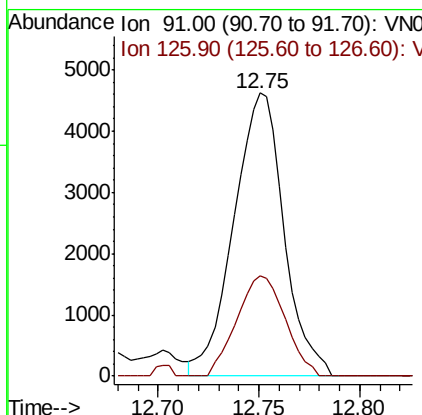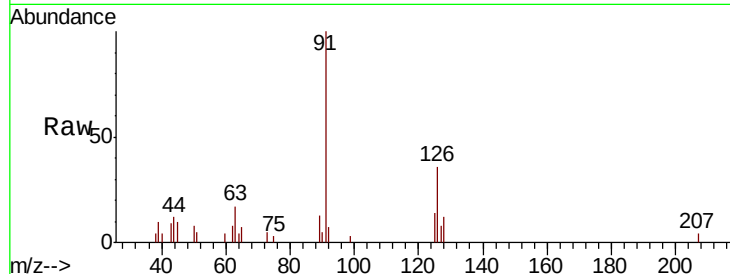

#95
Naphthalene
Concen: 4.004 ug/l
RT: 15.10 min Scan# 4146
Delta R.T. 0.00 min
Lab File: VN062271.D
Acq: 1 Jul 2020 5:07

Tgt Ion: 128 Resp: 69
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 0.0 8.6 13.0#

