

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN063020\
 Data File : VN062272.D
 Acq On : 1 Jul 2020 5:31
 Operator : JC/MD
 Sample : L3153-17
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SP2-C

Quant Time: Jul 01 06:01:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	201480	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	413539	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	407964	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	145409	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	159369	56.37	ug/l	0.00
Spiked Amount			Recovery	=	112.74%	
35) Dibromofluoromethane	7.55	113	125837	47.43	ug/l	0.00
Spiked Amount			Recovery	=	94.86%	
50) Toluene-d8	10.06	98	537788	50.71	ug/l	0.00
Spiked Amount			Recovery	=	101.42%	
62) 4-Bromofluorobenzene	12.38	95	174256	48.63	ug/l	0.00
Spiked Amount			Recovery	=	97.26%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.03	50	189	Below Cal	#	41
8) Diethyl Ether	3.38	74	479	0.310	ug/l #	7
16) Acetone	3.78	43	66347	71.871	ug/l	95
18) Methyl Acetate	4.28	43	6080	2.705	ug/l #	78
20) Methylene Chloride	4.50	84	26535	10.050	ug/l	95
25) 2-Butanone	6.80	43	3457	2.501	ug/l #	75
29) Tetrahydrofuran	7.16	42	306	0.338	ug/l #	28
31) Cyclohexane	7.63	56	5059	1.295	ug/l #	17
36) 1,1-Dichloropropene	7.63	75	18211	4.381	ug/l #	48
38) Carbon Tetrachloride	7.63	117	20788	5.305	ug/l #	16
41) Methacrylonitrile	7.17	41	474	0.297	ug/l #	27
43) Isopropyl Acetate	8.13	43	34735	6.191	ug/l	97
48) Methyl methacrylate	9.14	41	2748	1.092	ug/l #	15
51) 4-Methyl-2-Pentanone	9.95	43	5725	1.746	ug/l	95
54) cis-1,3-Dichloropropene	9.87	75	21897	4.369	ug/l #	71
56) Ethyl methacrylate	10.52	69	1005	0.248	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	1910	0.365	ug/l #	42
59) 2-Hexanone	10.73	43	22306	9.423	ug/l #	51
71) Bromoform	12.38	173	1412	0.641	ug/l #	1
74) N-amyl acetate	12.07	43	120	3.370	ug/l #	38
76) 1,2,3-Trichloropropane	12.38	75	89655	26.192	ug/l #	100
79) 2-Chlorotoluene	12.65	91	6106	0.784	ug/l	93
81) trans-1,4-Dichloro-2-buten	12.38	75	89655	76.489	ug/l #	13
82) 4-Chlorotoluene	12.75	91	5957	0.740	ug/l	96
95) Naphthalene	15.11	128	161	4.016	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN063020\
Data File : VN062272.D
Acq On : 1 Jul 2020 5:31
Operator : JC/MD
Sample : L3153-17
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SP2-C

Quant Time: Jul 01 06:01:09 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 24 15:33:00 2020
Response via : Initial Calibration

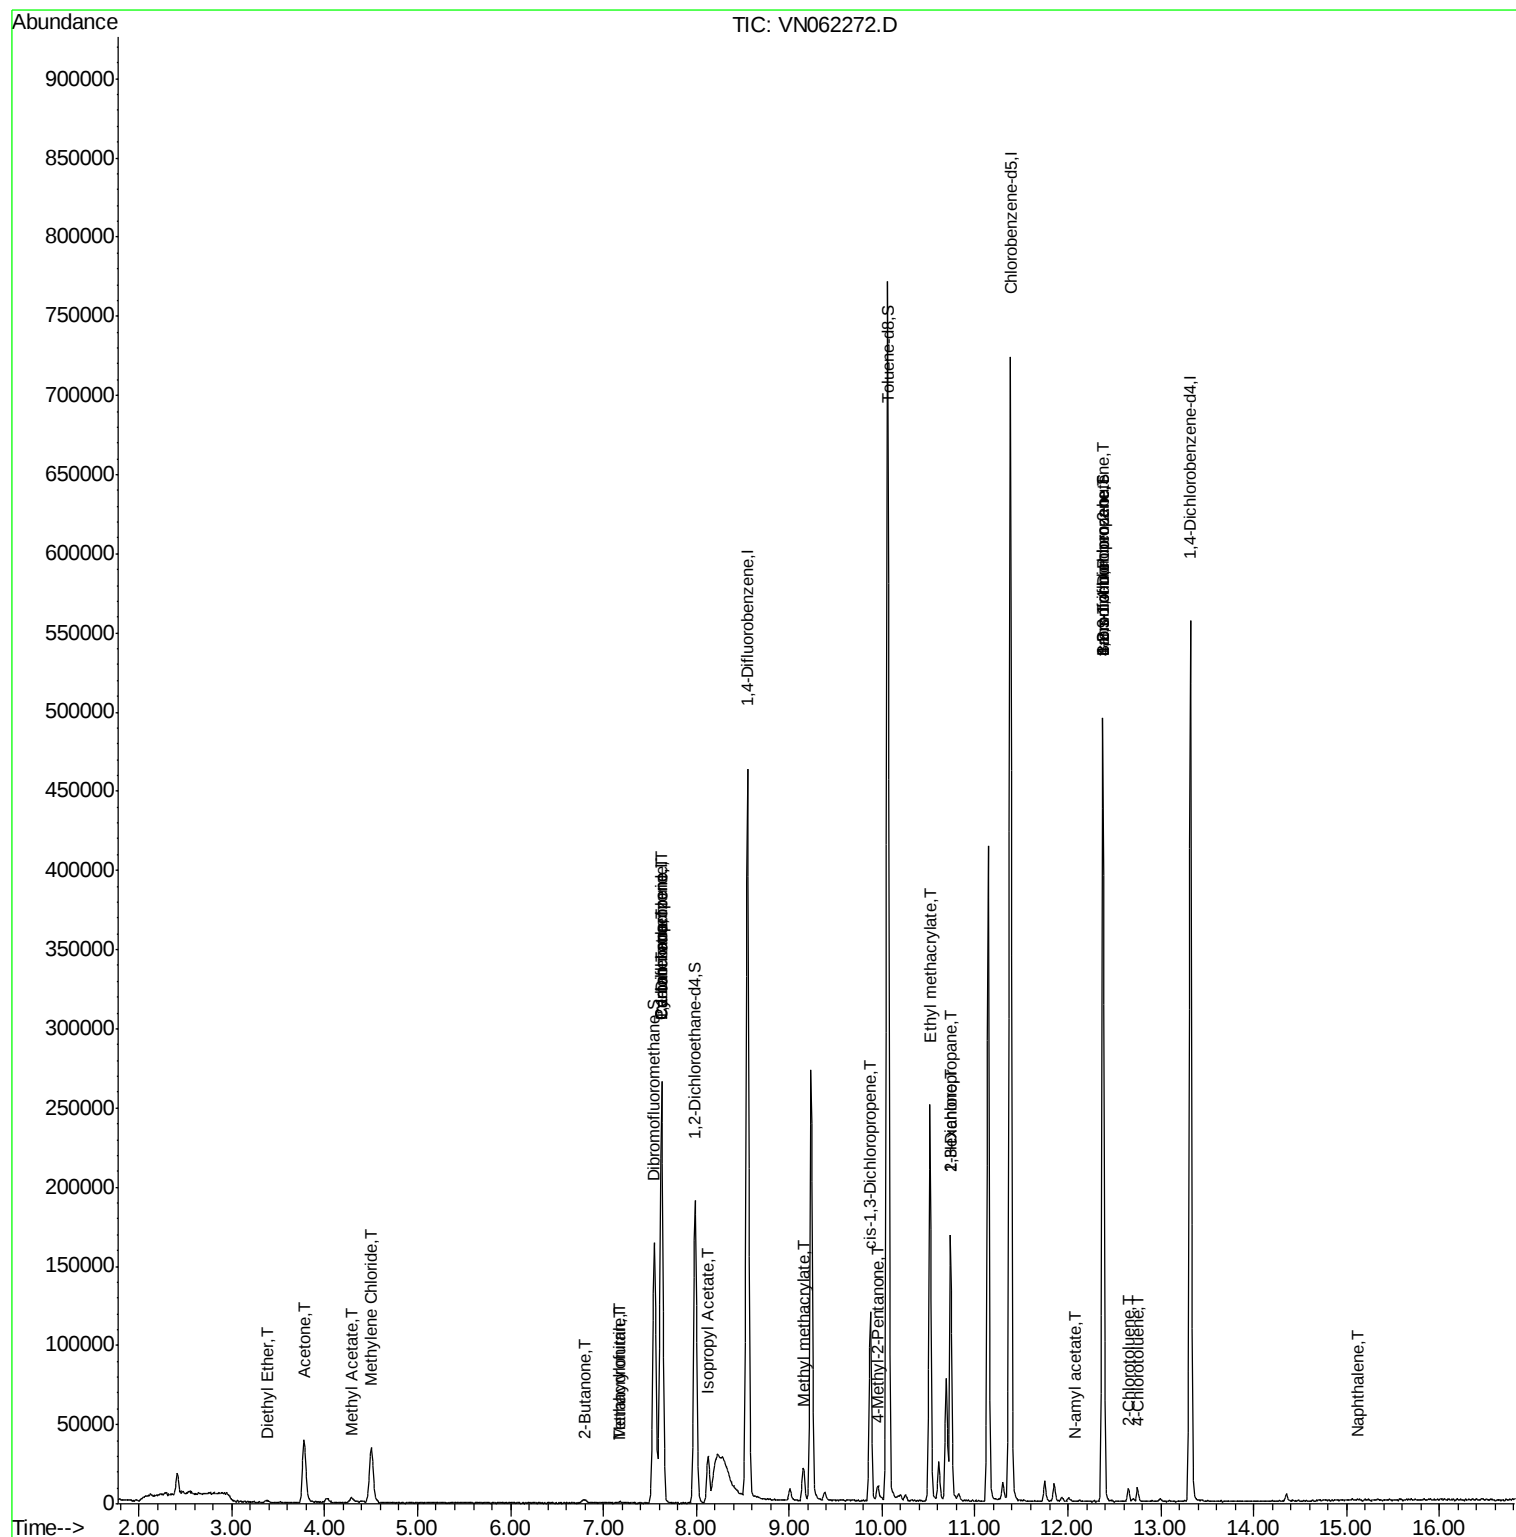



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062272.D

Acq: 1 Jul 2020 5:31

Instrument :

MSVOA_N

ClientSampled :


SP2-C

Tot Ion:168 Resp: 201480

Ion Ratio Lower Upper




168 100

99 62.3 45.8 68.8

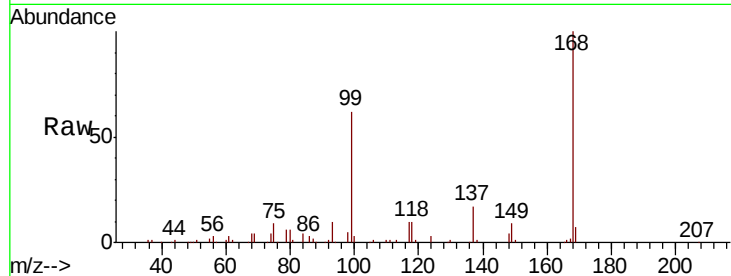

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

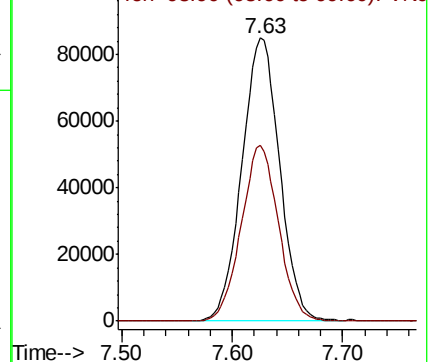

#3

Chloromethane

Concen: Below Cal

RT: 2.03 min Scan# 81

Delta R.T. 0.00 min

Lab File: VN062272.D


Acq: 1 Jul 2020 5:31

Tgt Ion: 50 Resp: 189

Ion Ratio Lower Upper



50 100


52 0.0 27.0 40.6#



Abundance Ion 49.90 (49.60 to 50.60): VN

Ion 51.90 (51.60 to 52.60): VN

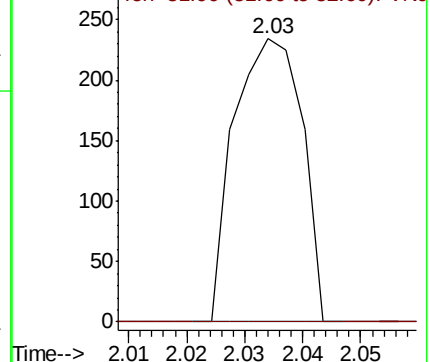

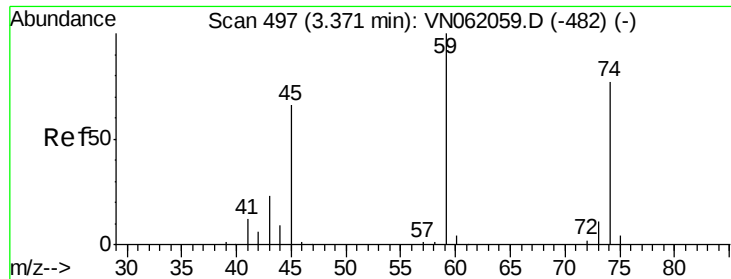

#8

Diethyl Ether

Concen: 0.310 ug/l

RT: 3.38 min Scan# 501

Delta R.T. 0.01 min

Lab File: VN062272.D

Acq: 1 Jul 2020 5:31

Instrument :

MSVOA_N

ClientSampleId :





SP2-C

Tot Ion: 74 Resp: 479

Ion Ratio Lower Upper

74 100

45 0.0 42.5 127.5#

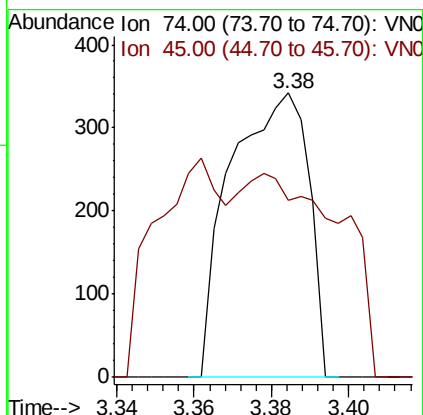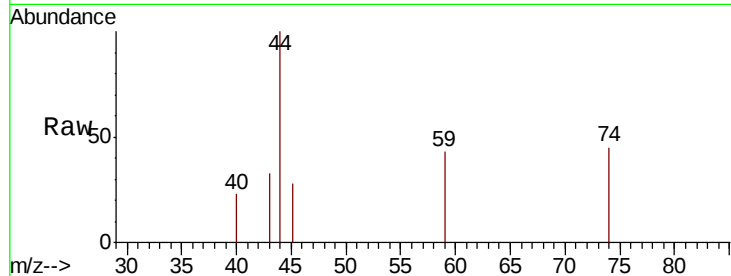

#16

Acetone

Concen: 71.871 ug/l

RT: 3.78 min Scan# 623

Delta R.T. 0.00 min

Lab File: VN062272.D




Acq: 1 Jul 2020 5:31

Tgt Ion: 43 Resp: 66347

Ion Ratio Lower Upper

43 100

58 31.4 27.5 41.3


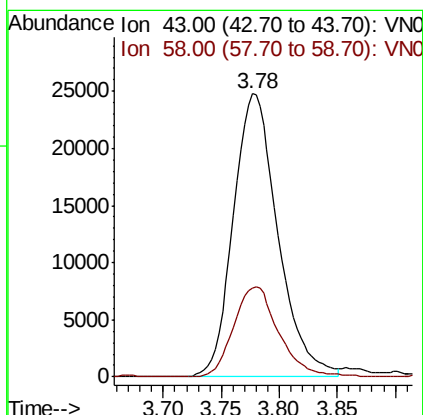






#18
Methyl Acetate
Concen: 2.705 ug/l
RT: 4.28 min Scan# 781
Delta R.T. 0.01 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31




Instrument :
MSVOA_N
ClientSampleId :
SP2-C


Tot Ion: 43 Resp: 6080
Ion Ratio Lower Upper
43 100
74 17.2 22.9 34.3#

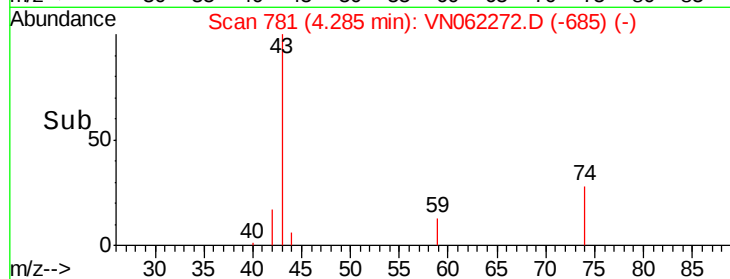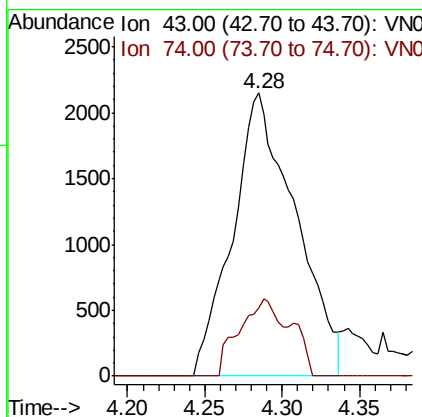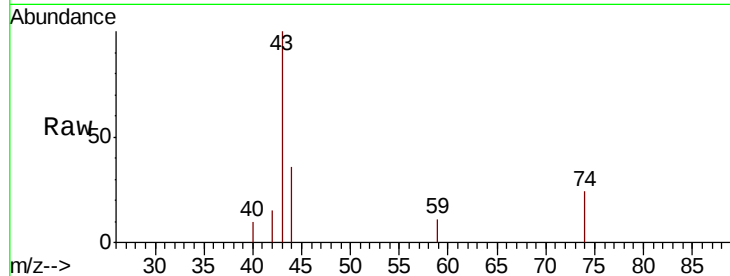

#20
Methylene Chloride
Concen: 10.050 ug/l
RT: 4.50 min Scan# 849
Delta R.T. 0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Tgt Ion: 84 Resp: 26535
Ion Ratio Lower Upper
84 100
49 121.5 90.6 136.0
51 37.0 27.8 41.8
86 61.1 50.1 75.1


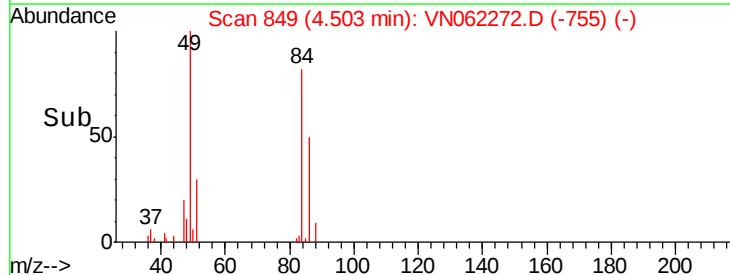
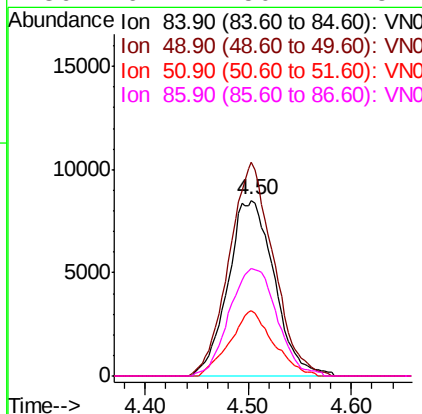



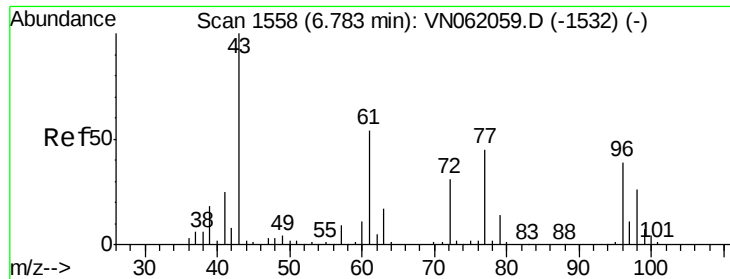

#25
2-Butanone
Concen: 2.501 ug/l
RT: 6.80 min Scan# 1562
Delta R.T. 0.01 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31




Instrument :
MSVOA_N
ClientSampled :
SP2-C


Tot Ion: 43 Resp: 3457
Ion Ratio Lower Upper
43 100
72 17.4 24.8 37.2#

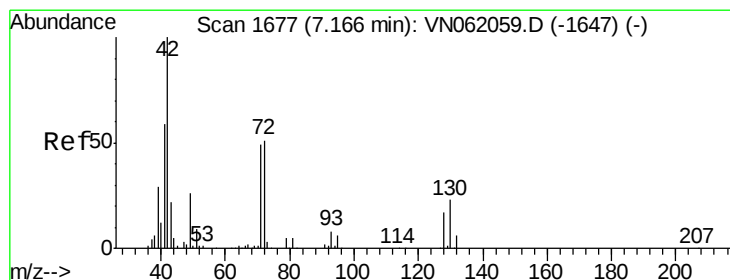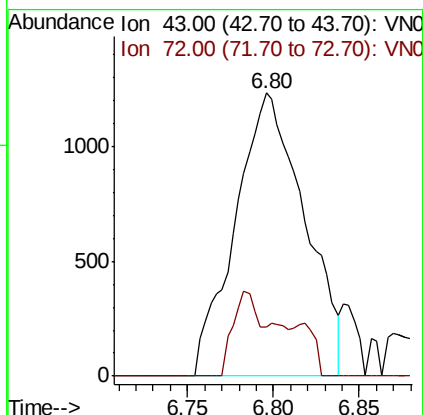

#29
Tetrahydrofuran
Concen: 0.338 ug/l
RT: 7.16 min Scan# 1676
Delta R.T. -0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Tgt Ion: 42 Resp: 306
Ion Ratio Lower Upper
42 100
72 0.0 41.1 61.7#
71 0.0 38.2 57.4#

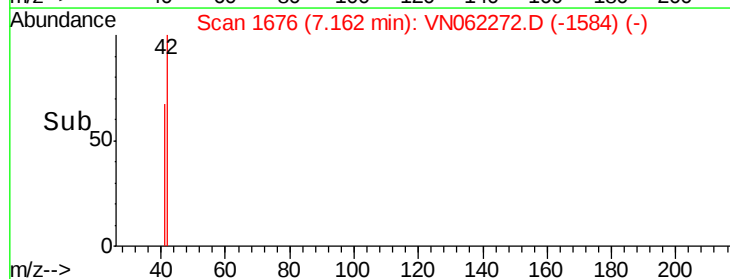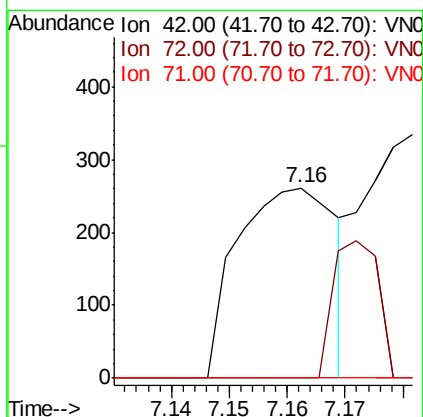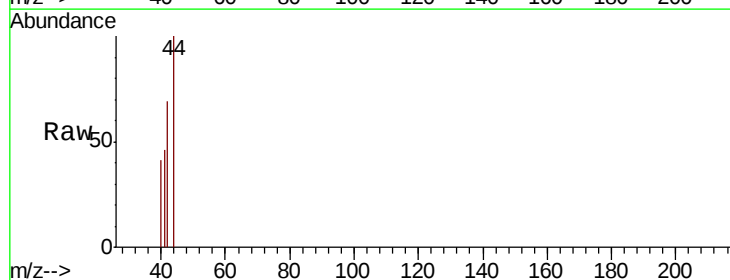

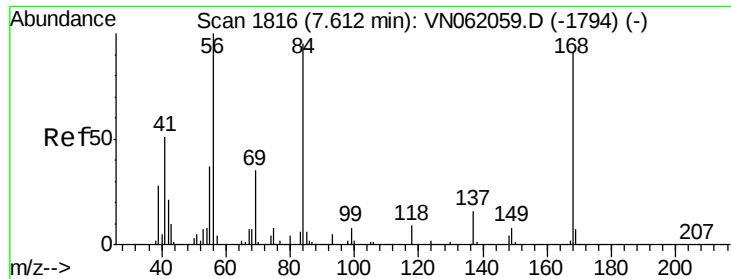

#31

Cyclohexane

Concen: 1.295 ug/l

RT: 7.63 min Scan# 1821

Delta R.T. 0.02 min

Lab File: VN062272.D

Acq: 1 Jul 2020 5:31

Instrument :

MSVOA_N

ClientSampleId :

SP2-C


Tot Ion: 56 Resp: 5059

Ion Ratio Lower Upper

56 100

69 151.0 28.0 42.0#




84 133.8 76.1 114.1#

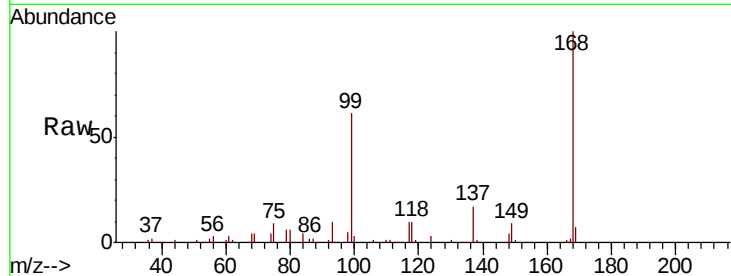

Abundance Ion 56.00 (55.70 to 56.70): VN062272.D (-1723) (-)

Ion 69.00 (68.70 to 69.70): VN062272.D (-1723) (-)

Ion 84.00 (83.70 to 84.70): VN062272.D (-1723) (-)

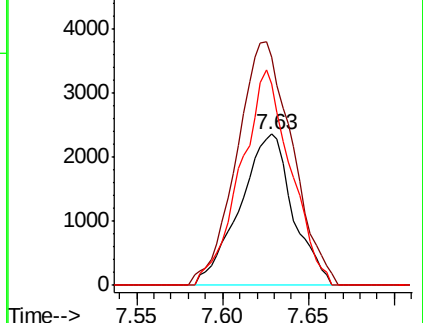

#33

1,2-Dichloroethane-d4

Concen: 56.365 ug/l

RT: 7.99 min Scan# 1932

Delta R.T. 0.00 min

Lab File: VN062272.D


Acq: 1 Jul 2020 5:31

Tgt Ion: 65 Resp: 159369

Ion Ratio Lower Upper



65 100


67 53.1 0.0 106.2



Abundance Ion 64.90 (64.60 to 65.60): VN062272.D (-1839) (-)

Ion 66.90 (66.60 to 67.60): VN062272.D (-1839) (-)

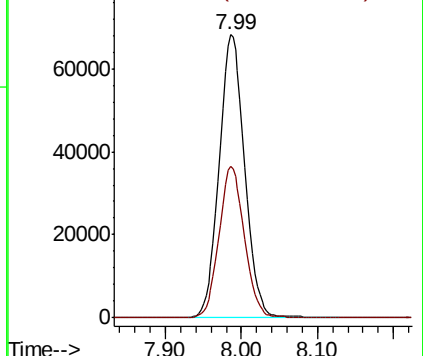


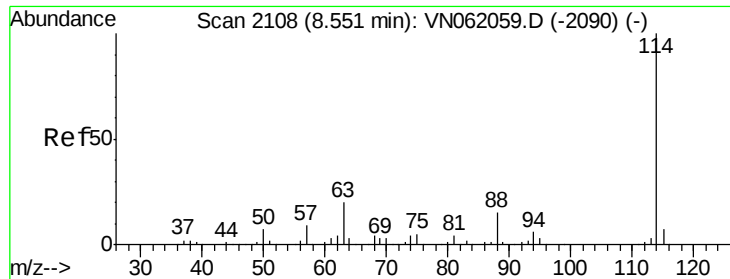




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.55 min Scan# 2108
Delta R.T. 0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Instrument :
MSVOA_N
ClientSampled :
SP2-C

Tot Ion:114 Resp: 413539
Ion Ratio Lower Upper
114 100
63 21.1 0.0 39.2
88 15.6 0.0 30.8

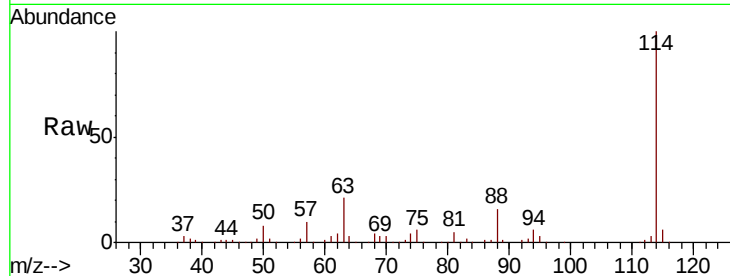


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN

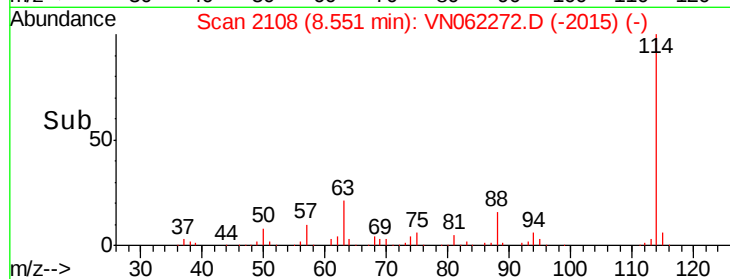
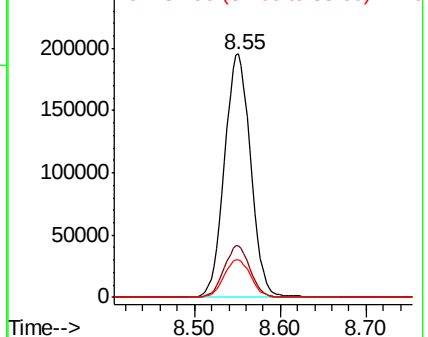



#35
Dibromofluoromethane
Concen: 47.431 ug/l
RT: 7.55 min Scan# 1796
Delta R.T. -0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Tgt Ion:113 Resp: 125837
Ion Ratio Lower Upper
113 100
111 103.9 82.2 123.4
192 16.9 14.0 21.0



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V




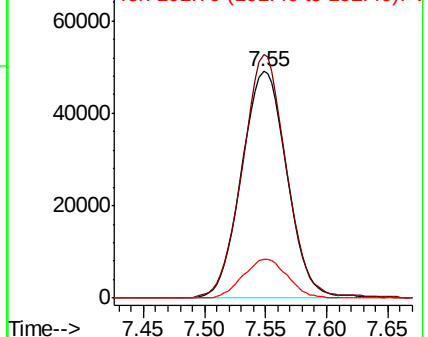


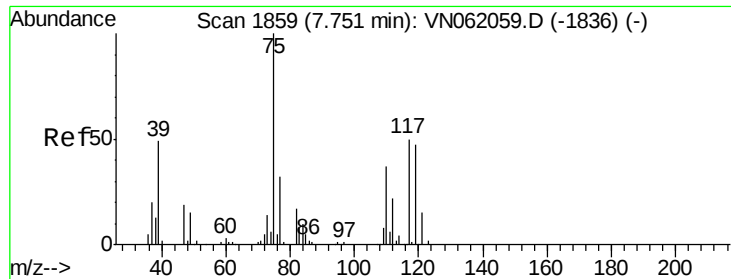

#36
 1,1-Dichloropropene
 Concen: 4.381 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.13 min
 Lab File: VN062272.D
 Acq: 1 Jul 2020 5:31




Instrument :
 MSVOA_N
 ClientSampleID :
 SP2-C


Tot Ion	Ratio	Lower	Upper
75	100		
110	7.1	17.9	53.8#
77	0.0	24.9	37.3#

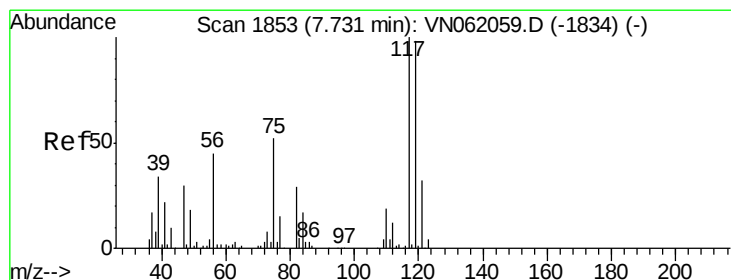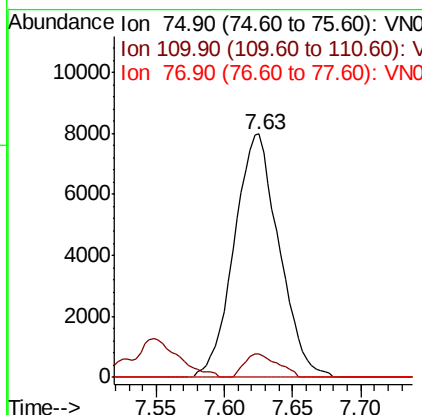

#38
 Carbon Tetrachloride
 Concen: 5.305 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.11 min
 Lab File: VN062272.D
 Acq: 1 Jul 2020 5:31

Tgt Ion	Ratio	Lower	Upper
117	100		
119	6.2	78.2	117.2#
121	0.0	25.8	38.6#



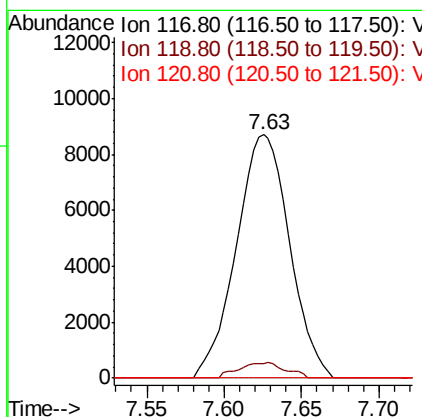





#41
Methacrylonitrile
Concen: 0.297 ug/l
RT: 7.17 min Scan# 1679
Delta R.T. 0.05 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31




Instrument :
MSVOA_N
ClientSampleID :
SP2-C


Tot Ion: 41 Resp: 474
Ion Ratio Lower Upper
41 100
39 32.7 44.2 66.2#
67 0.0 79.5 119.3#
52 0.0 32.3 48.5#

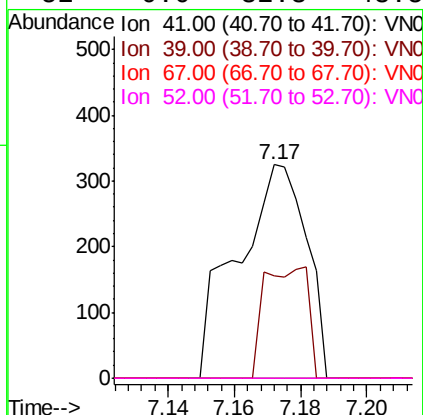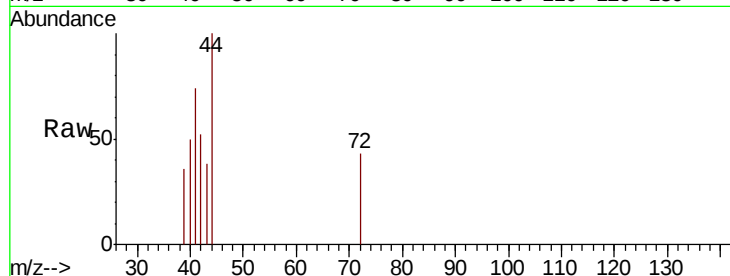

#43
Isopropyl Acetate
Concen: 6.191 ug/l
RT: 8.13 min Scan# 1976
Delta R.T. -0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Tgt Ion: 43 Resp: 34735
Ion Ratio Lower Upper
43 100
61 20.6 17.2 25.8
87 13.0 12.1 18.1

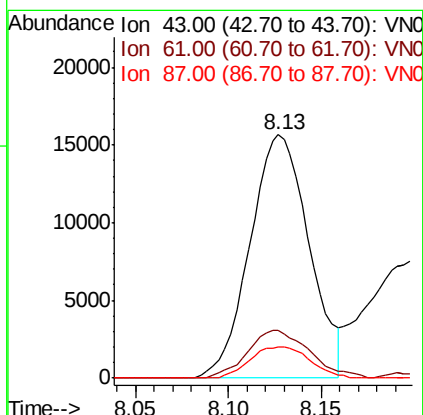







#48
Methvl methacrylate
Concen: 1.092 ug/l
RT: 9.14 min Scan# 2292
Delta R.T. -0.02 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Instrument :
MSVOA_N
ClientSampleId :
SP2-C

Tot Ion: 41 Resp: 2748
Ion Ratio Lower Upper
41 100
69 0.0 80.7 121.1#
39 18.7 54.5 81.7#

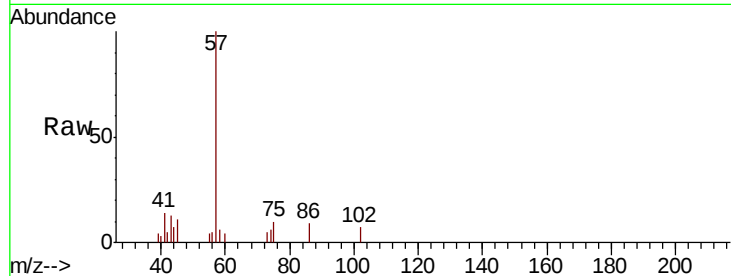


Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0


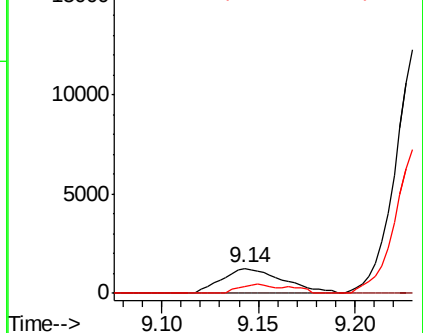



#50
Toluene-d8
Concen: 50.710 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. -0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Tgt Ion: 98 Resp: 537788
Ion Ratio Lower Upper
98 100
100 65.1 51.2 76.8

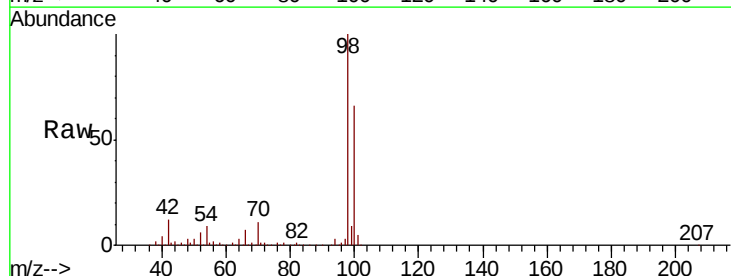

Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0



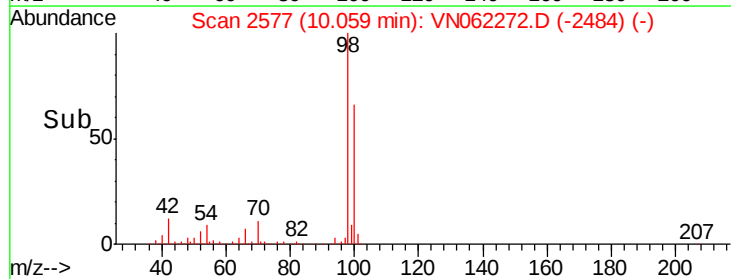
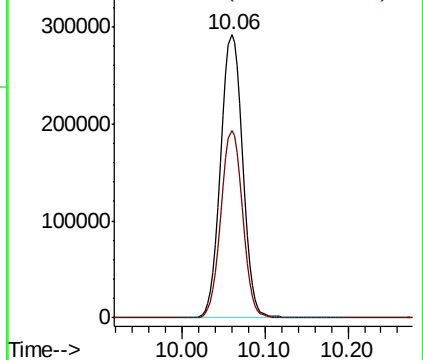


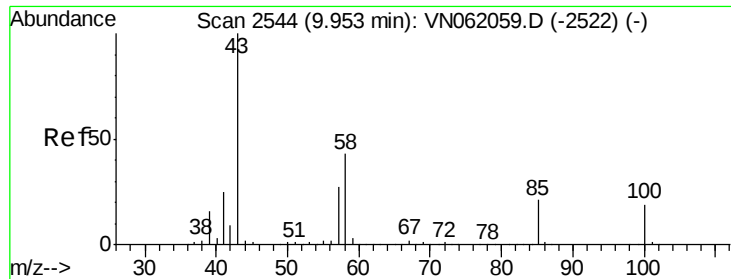

#51
4-Methyl-2-Pentanone
Concen: 1.746 ug/l
RT: 9.95 min Scan# 2543
Delta R.T. -0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31




Instrument :
MSVOA_N
ClientSampled :
SP2-C


Tot Ion: 43 Resp: 5725
Ion Ratio Lower Upper
43 100
58 46.0 34.2 51.2

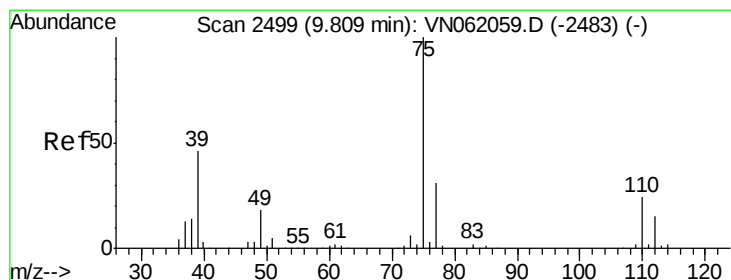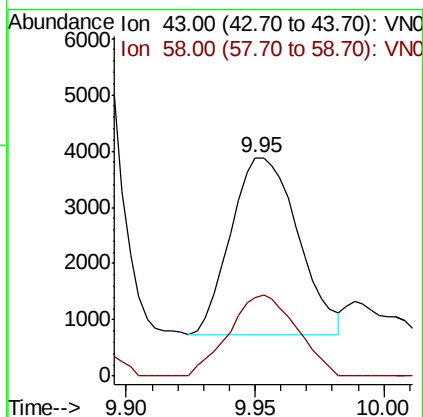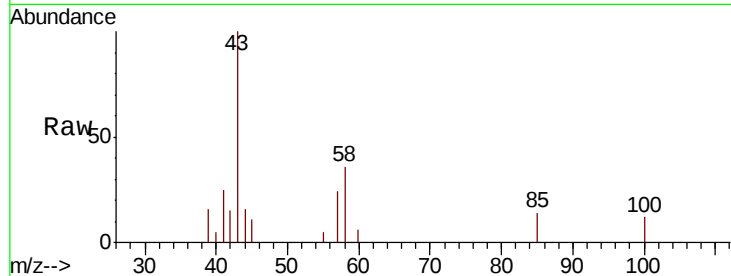

#54
cis-1,3-Dichloropropene
Concen: 4.369 ug/l
RT: 9.87 min Scan# 2519
Delta R.T. 0.06 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Tgt Ion: 75 Resp: 21897
Ion Ratio Lower Upper
75 100
77 0.0 25.0 37.6#
39 38.9 36.9 55.3

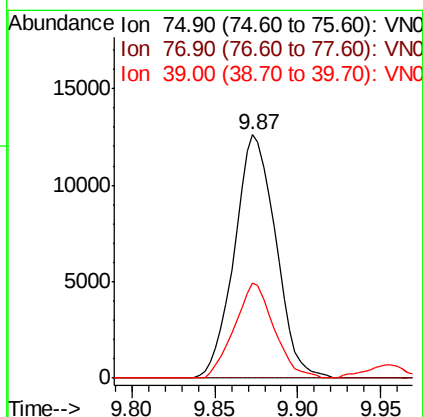

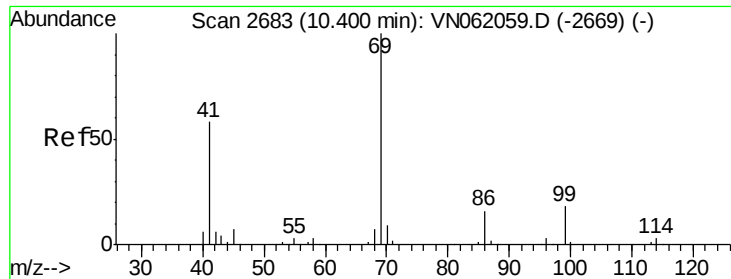

#56

Ethyl methacrylate

Concen: 0.248 ug/l

RT: 10.52 min Scan# 2719

Delta R.T. 0.12 min

Lab File: VN062272.D

Acq: 1 Jul 2020 5:31

Instrument :

MSVOA_N

ClientSampleId :

SP2-C


Tot Ion: 69 Resp: 1005

Ion Ratio Lower Upper

69 100

41 4854.8 46.6 70.0#




39 2205.8 31.0 46.4#

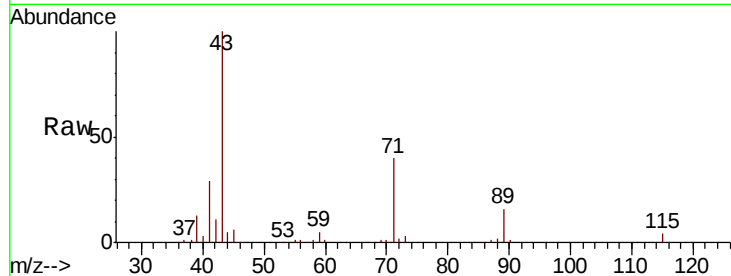

Abundance Ion 69.00 (68.70 to 69.70): VN062059.D (-2669) (-)

Ion 41.00 (40.70 to 41.70): VN062059.D (-2669) (-)

Ion 39.00 (38.70 to 39.70): VN062059.D (-2669) (-)

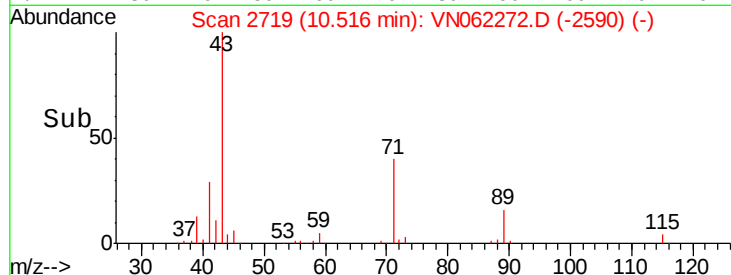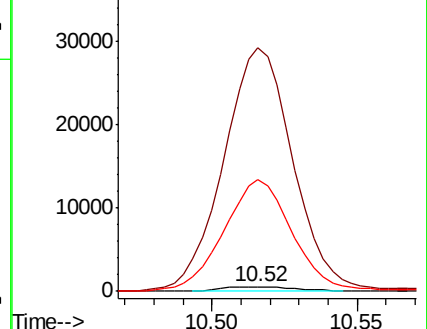

#57

1,3-Dichloropropane

Concen: 0.365 ug/l

RT: 10.74 min Scan# 2788

Delta R.T. 0.06 min

Lab File: VN062272.D


Acq: 1 Jul 2020 5:31

Tgt Ion: 76 Resp: 1910

Ion Ratio Lower Upper



76 100


78 0.0 25.8 38.8#



Abundance Ion 75.90 (75.60 to 76.60): VN062059.D (-2754) (-)

Ion 77.90 (77.60 to 78.60): VN062059.D (-2754) (-)




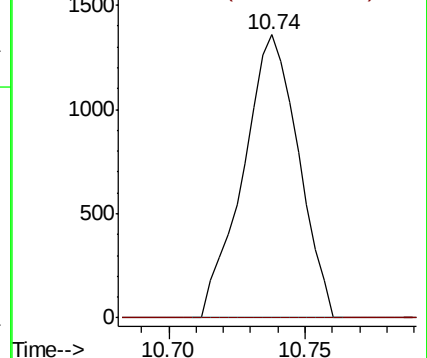




#59
2-Hexanone
Concen: 9.423 ug/l
RT: 10.73 min Scan# 2787
Delta R.T. 0.01 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31




Instrument :
MSVOA_N
ClientSampleId :
SP2-C


Tot Ion: 43 Resp: 22306
Ion Ratio Lower Upper
43 100
58 22.1 29.5 88.5#

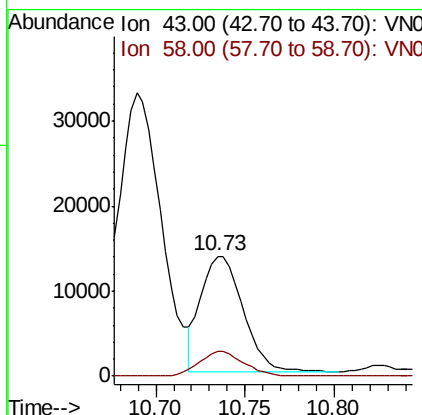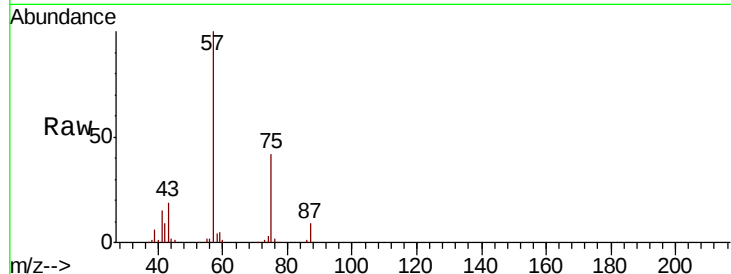

#62
4-Bromofluorobenzene
Concen: 48.634 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Tgt Ion: 95 Resp: 174256
Ion Ratio Lower Upper
95 100
174 72.5 0.0 154.8
176 69.9 0.0 147.4

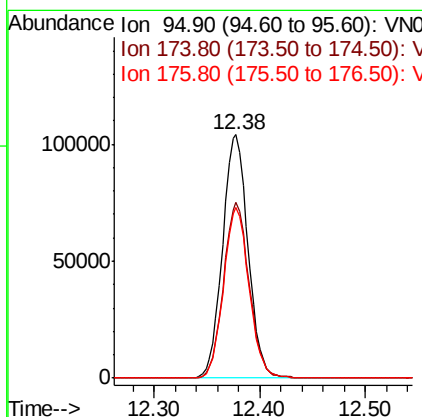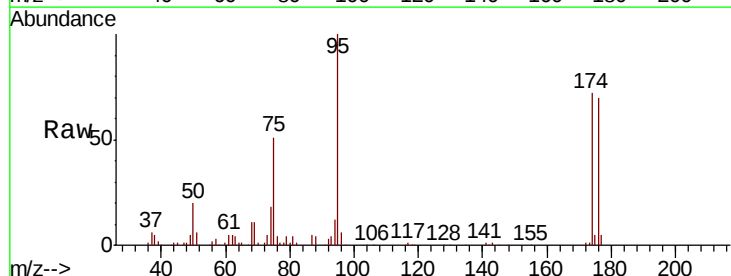


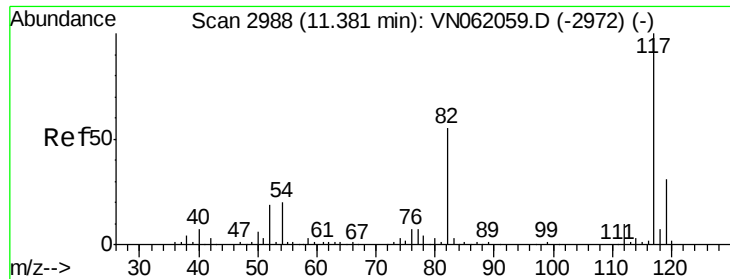




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. 0.00 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Instrument :
MSVOA_N
ClientSampleId :
SP2-C

Tot Ion:117 Resp: 407964
Ion Ratio Lower Upper
117 100
82 56.4 43.8 65.8
119 31.0 25.2 37.8

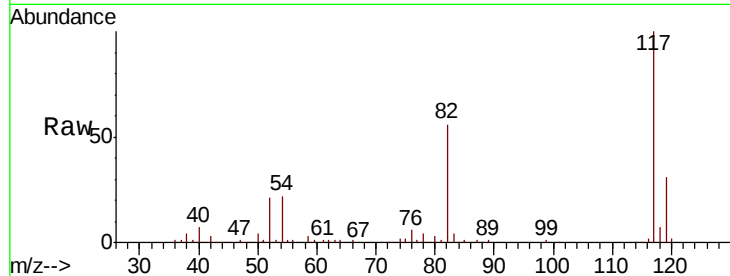


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V


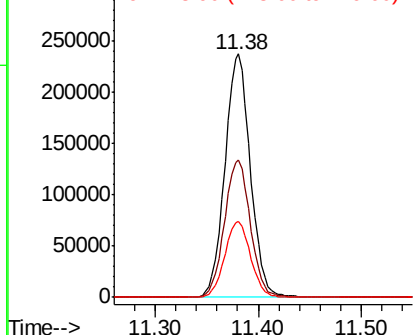



#71
Bromoform
Concen: 0.641 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.28 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Tgt Ion:173 Resp: 1412
Ion Ratio Lower Upper
173 100
175 570.8 24.7 74.1#
254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

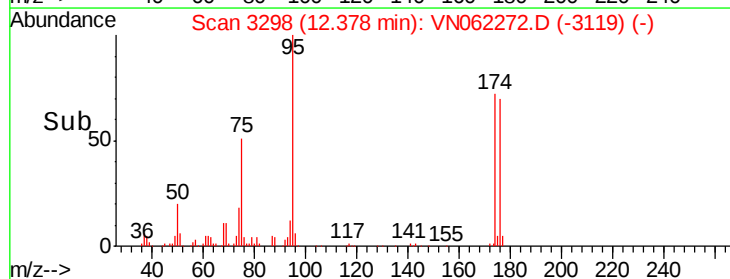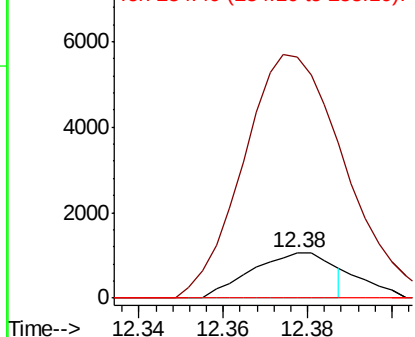

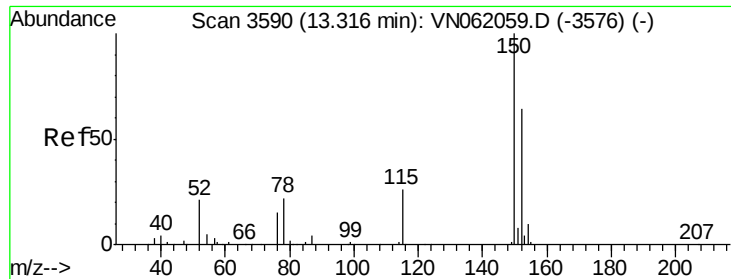

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062272.D

Acq: 1 Jul 2020 5:31

Instrument :

MSVOA_N

ClientSampleId :

SP2-C


Tot Ion:152 Resp: 145409

Ion Ratio Lower Upper

152 100

115 60.8 29.5 88.5




150 158.1 0.0 351.4



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

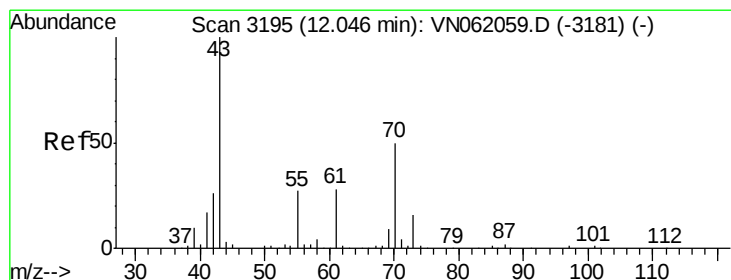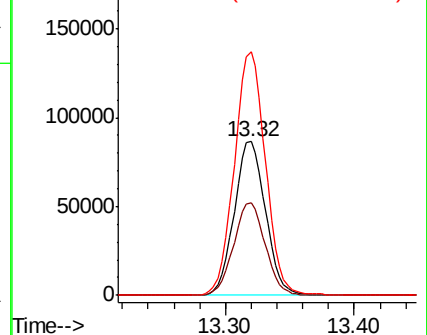

#74

N-ethyl acetate

Concen: 3.370 ug/l

RT: 12.07 min Scan# 3202

Delta R.T. 0.02 min

Lab File: VN062272.D

Acq: 1 Jul 2020 5:31

Tgt Ion: 43 Resp: 120


Ion Ratio Lower Upper

43 100

70 0.0 39.4 59.2#

55 0.0 21.7 32.5#

61 0.0 21.3 31.9#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V

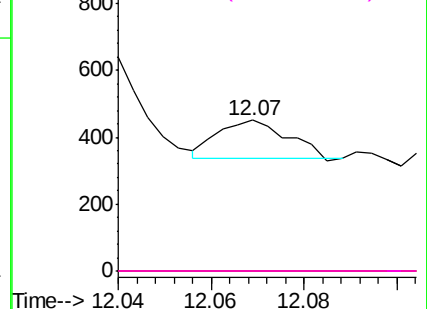

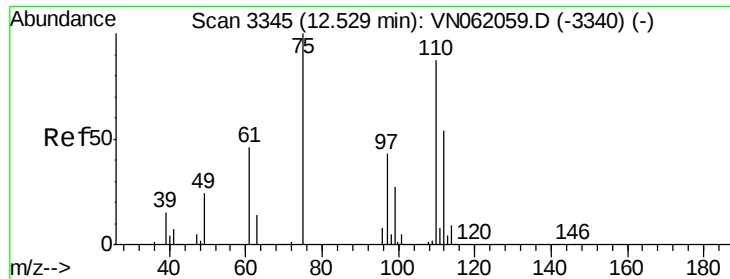

#76

1,2,3-Trichloropropane

Concen: 26.192 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.15 min

Lab File: VN062272.D

Acq: 1 Jul 2020 5:31

Instrument :

MSVOA_N

ClientSampled :


SP2-C

Tot Ion: 75 Resp: 89655

Ion Ratio Lower Upper




75 100

77 1.0 0.0 0.0#

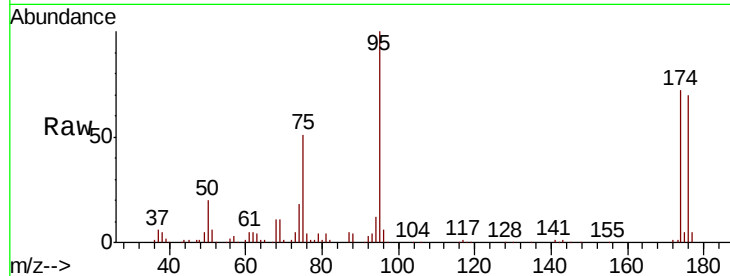

Abundance Ion 74.90 (74.60 to 75.60): VN062272.D (-3298) (-)

Ion 77.00 (76.70 to 77.70): VN062272.D (-3298) (-)

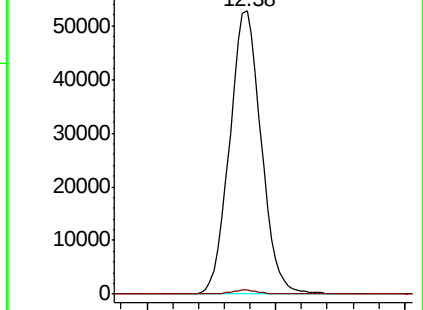

#79

2-Chlorotoluene

Concen: 0.784 ug/l

RT: 12.65 min Scan# 3383

Delta R.T. 0.00 min

Lab File: VN062272.D


Acq: 1 Jul 2020 5:31

Tgt Ion: 91 Resp: 6106

Ion Ratio Lower Upper



91 100


126 29.9 16.9 50.7



Abundance Ion 91.00 (90.70 to 91.70): VN062272.D (-3383) (-)

Ion 125.90 (125.60 to 126.60): VN062272.D (-3383) (-)

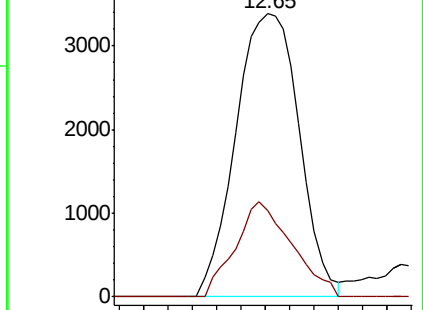

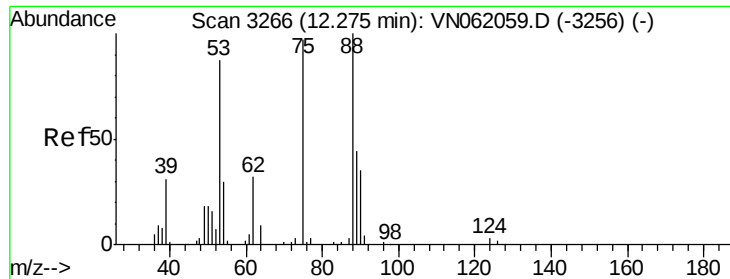

#81

trans-1,4-Dichloro-2-butene

Concen: 76.489 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.10 min

Lab File: VN062272.D

Acq: 1 Jul 2020 5:31

Instrument :

MSVOA_N

ClientSampleId :

SP2-C


Tot Ion: 75 Resp: 89655

Ion Ratio Lower Upper

75 100

53 0.0 72.0 108.0#




89 0.0 36.9 55.3#

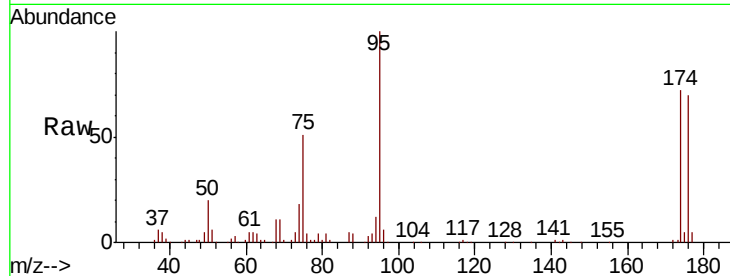

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0

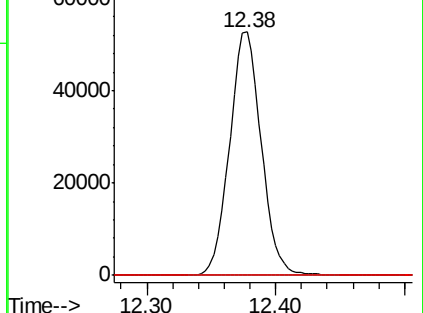

#82

4-Chlorotoluene

Concen: 0.740 ug/l

RT: 12.75 min Scan# 3414

Delta R.T. 0.00 min

Lab File: VN062272.D


Acq: 1 Jul 2020 5:31

Tgt Ion: 91 Resp: 5957

Ion Ratio Lower Upper



91 100


126 31.0 16.7 50.1



Abundance Ion 91.00 (90.70 to 91.70): VN0

Ion 125.90 (125.60 to 126.60): V

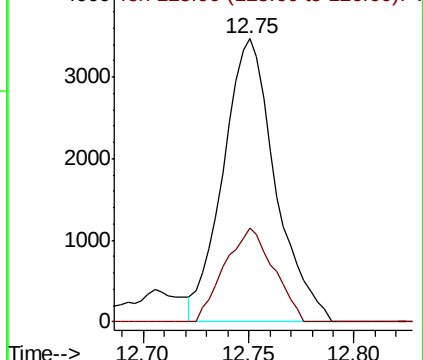


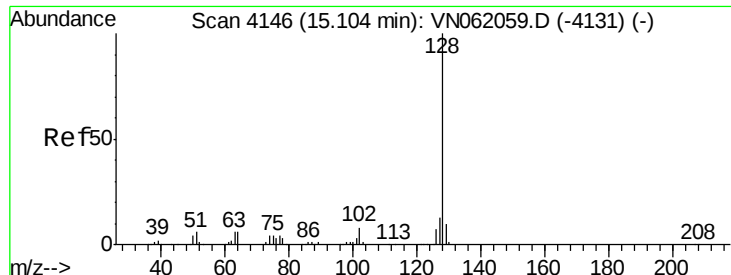

#95
Naphthalene
Concen: 4.016 ug/l
RT: 15.11 min Scan# 4149
Delta R.T. 0.01 min
Lab File: VN062272.D
Acq: 1 Jul 2020 5:31

Instrument :
MSVOA_N
ClientSampleId :
SP2-C

Tot Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.5	15.7#
129	0.0	8.6	13.0#

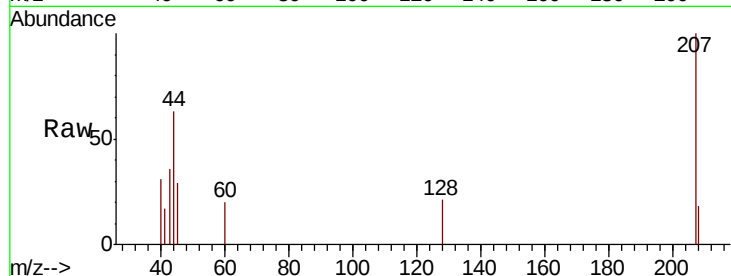

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

