

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN063020\
 Data File : VN062248.D
 Acq On : 30 Jun 2020 18:39
 Operator : JC/MD
 Sample : L3170-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1R

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.137	105	113	121	rBV2	15819	23457	1.83%	0.362%
2	2.407	190	197	213	rBV4	10470	19179	1.50%	0.296%
3	2.947	353	365	382	rVB	45566	95099	7.43%	1.466%
4	4.024	684	700	717	rBV3	8083	22851	1.78%	0.352%
5	4.992	978	1001	1029	rBV2	20973	76766	6.00%	1.184%
6	7.548	1777	1796	1808	rBV	157545	394179	30.78%	6.078%
7	7.625	1808	1820	1844	rVB2	254662	608696	47.54%	9.386%
8	7.989	1911	1933	1953	rBV	184814	424693	33.17%	6.549%
9	8.551	2090	2108	2126	rBV	426551	881712	68.86%	13.596%
10	10.059	2559	2577	2603	rBV	701312	1280436	100.00%	19.744%
11	11.381	2974	2988	3015	rBV	640040	1119743	87.45%	17.266%
12	12.378	3284	3298	3317	rBV	437842	734365	57.35%	11.324%
13	13.320	3578	3591	3611	rBV	481099	803932	62.79%	12.397%


Sum of corrected areas: 6485108

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN063020\
Data File : VN062248.D
Acq On : 30 Jun 2020 18:39
Operator : JC/MD
Sample : L3170-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1R

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

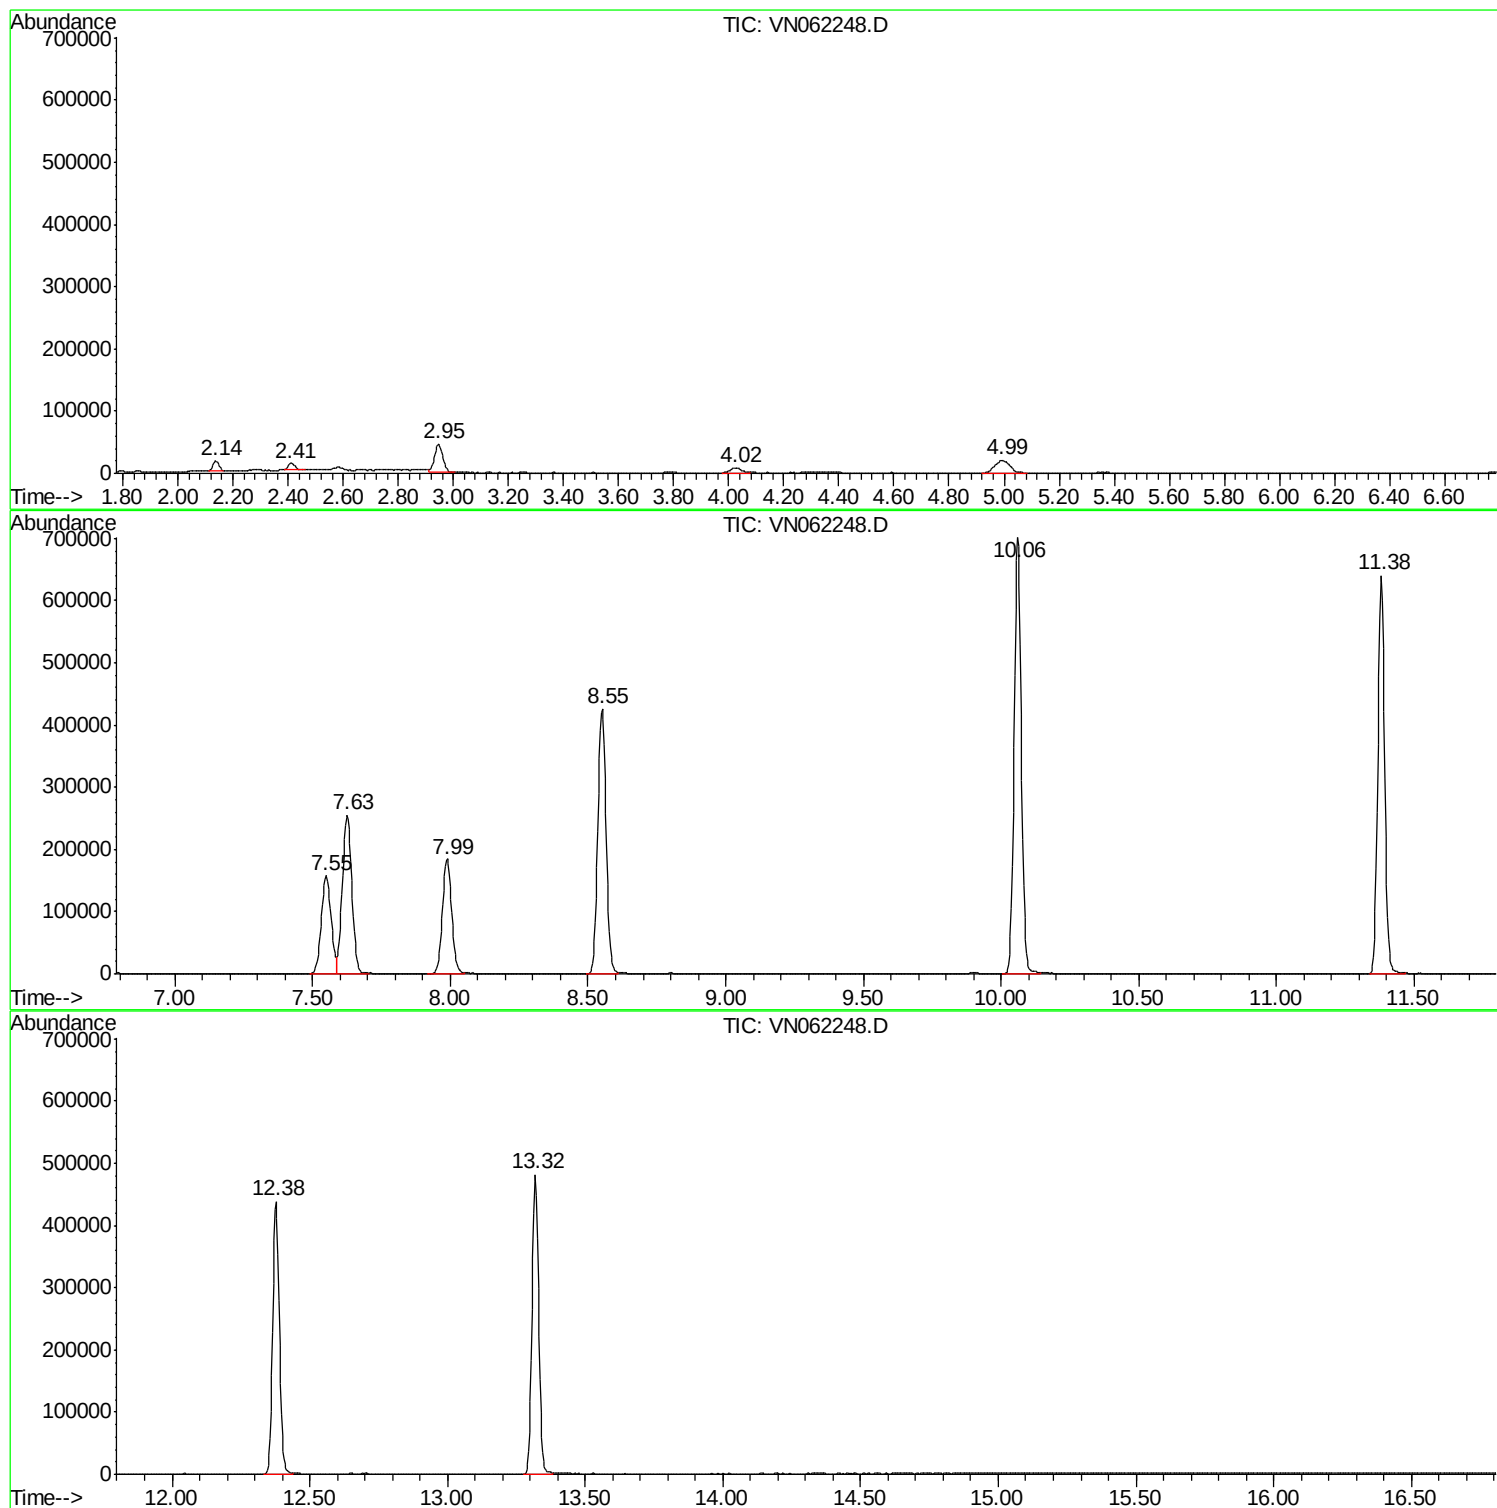

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN063020\
Data File : VN062248.D
Acq On : 30 Jun 2020 18:39
Operator : JC/MD
Sample : L3170-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :
MW-1R










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.95	7.81 ug/l	95099	Pentafluorobenzene	7.63

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Fluorodichloromethane	102	CHCl2F	000075-43-4	95
2		Ethyl 2-butyrate	112	C6H10O2	004341-76-8	9
3		1-Hexyne	82	C6H10	000693-02-7	7
4		Chlorine dioxide	67	ClO2	010049-04-4	5
5		Methanamine, N,N-difluoro-	67	CH3F2N	000753-58-2	4

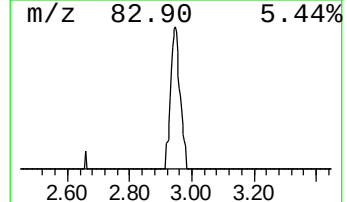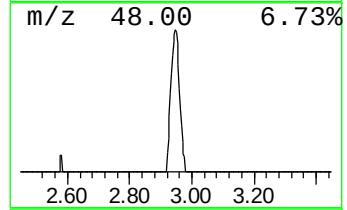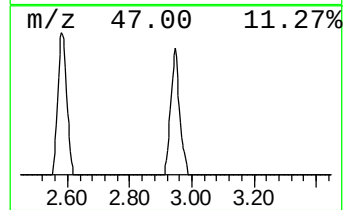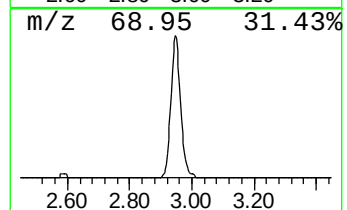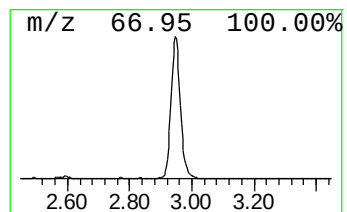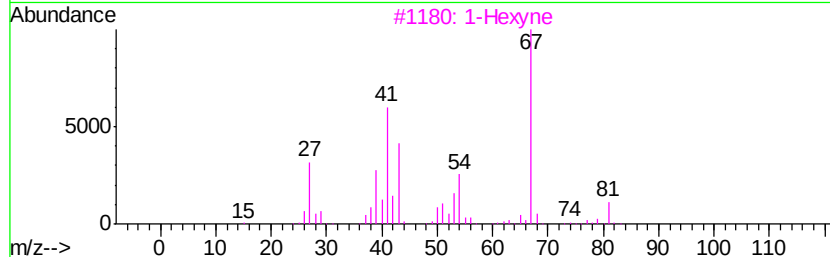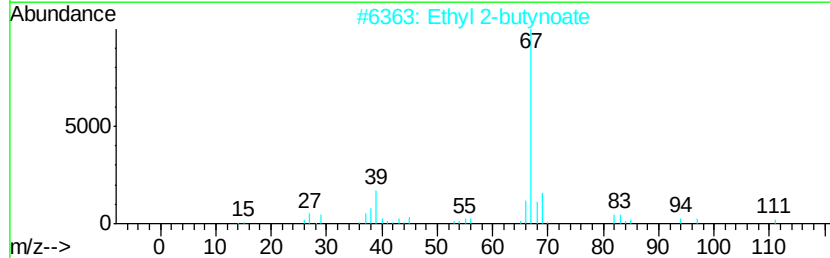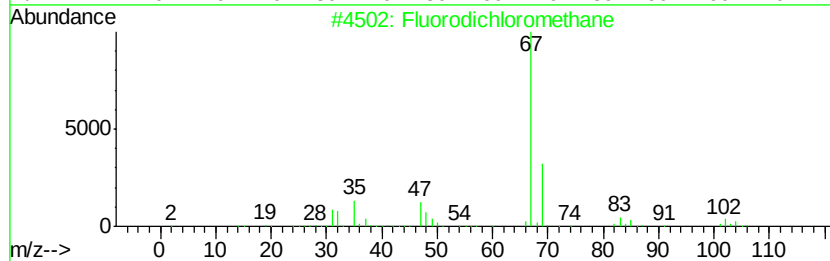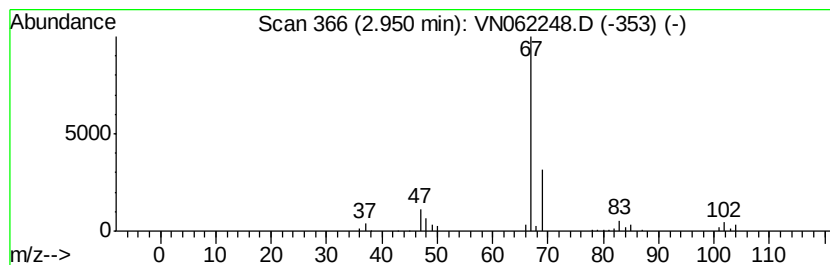

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN063020\
Data File : VN062248.D
Acq On : 30 Jun 2020 18:39
Operator : JC/MD
Sample : L3170-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1R

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichloromet...	2.95	7.8	ug/l	95099	1	7.63	608696	50.0