

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN063020\
 Data File : VN062252.D
 Acq On : 30 Jun 2020 20:16
 Operator : JC/MD
 Sample : L3170-07
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-8

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.796	3	7	22	rVB	101534	131319	6.24%	1.479%
2	2.005	59	72	89	rBV	1507856	2104513	100.00%	23.708%
3	2.417	194	200	211	rVB5	17609	29728	1.41%	0.335%
4	4.018	683	698	723	rBV4	19232	57410	2.73%	0.647%
5	4.995	974	1002	1029	rVB2	103010	376993	17.91%	4.247%
6	7.548	1778	1796	1808	rBV2	154642	386267	18.35%	4.351%
7	7.625	1808	1820	1838	rVB	248385	582539	27.68%	6.563%
8	7.989	1913	1933	1953	rBV2	179729	426757	20.28%	4.808%
9	8.551	2092	2108	2130	rBV	412351	868939	41.29%	9.789%
10	10.059	2562	2577	2591	rBV	674969	1235613	58.71%	13.920%
11	10.124	2591	2597	2613	rVB	15731	30357	1.44%	0.342%
12	11.381	2974	2988	3011	rBV	609938	1073133	50.99%	12.089%
13	11.590	3040	3053	3066	rVB2	13910	26380	1.25%	0.297%
14	11.927	3148	3158	3174	rBV5	11149	24580	1.17%	0.277%
15	12.378	3285	3298	3319	rBV	428265	715842	34.01%	8.064%
16	13.320	3577	3591	3608	rBV	477220	806374	38.32%	9.084%


Sum of corrected areas: 8876744

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN063020\
Data File : VN062252.D
Acq On : 30 Jun 2020 20:16
Operator : JC/MD
Sample : L3170-07
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

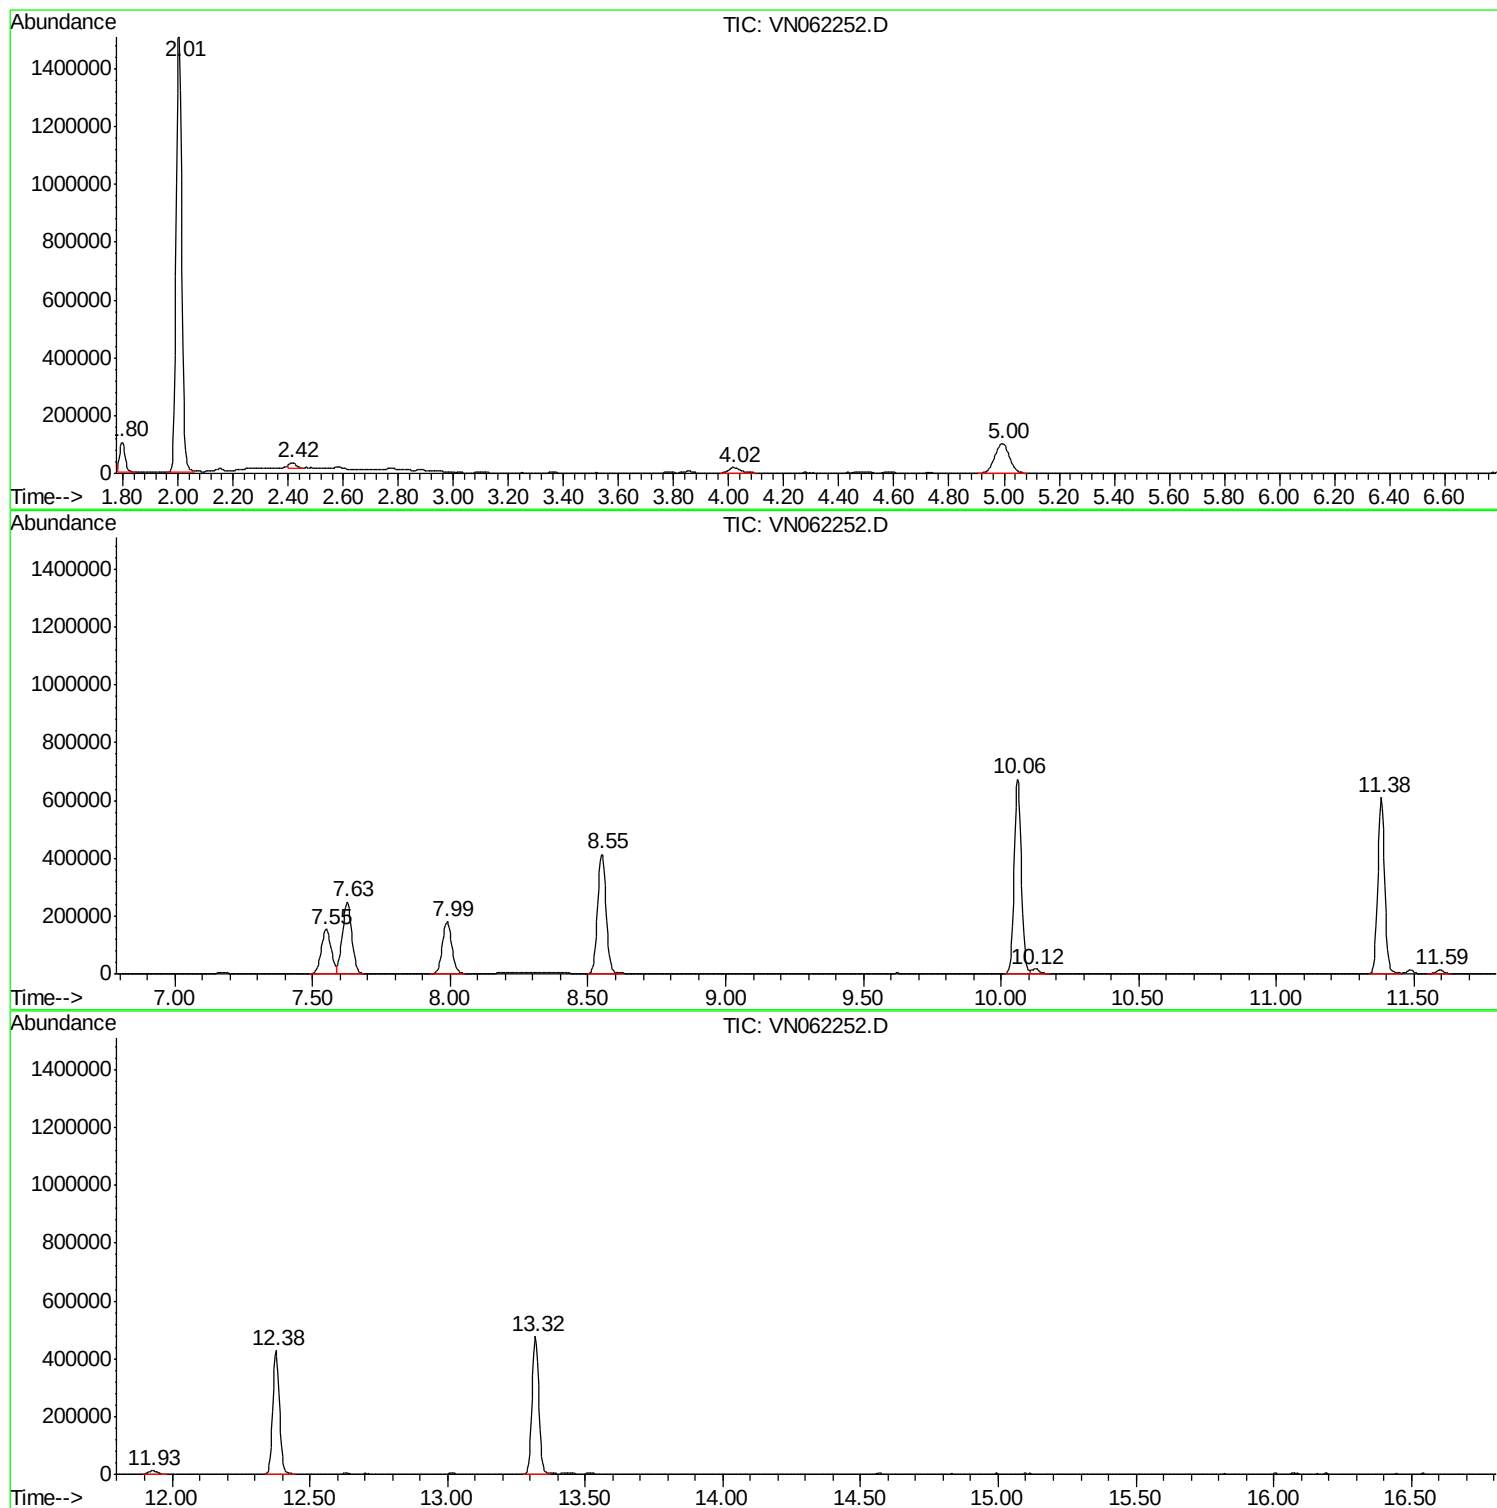

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN063020\
Data File : VN062252.D
Acq On : 30 Jun 2020 20:16
Operator : JC/MD
Sample : L3170-07
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-8










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,1-difluoro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.80	11.27 ug/l	131319	Pentafluorobenzene	7.63

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	91
2		Propiolonitrile	51	C3HN	001070-71-9	3
3		Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	2
4		Difluoromethane	52	CH2F2	000075-10-5	1
5		2-Chloroethanol	80	C2H5ClO	000107-07-3	1

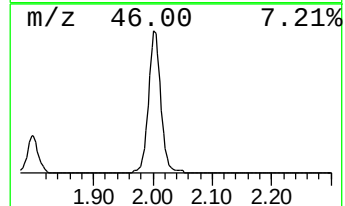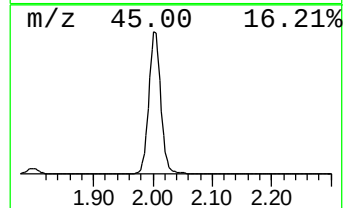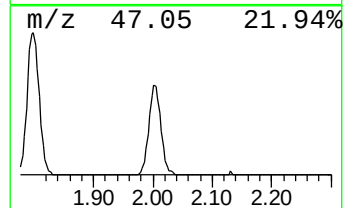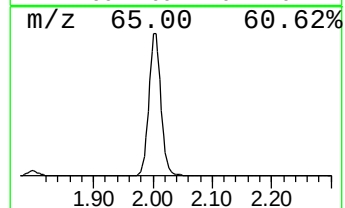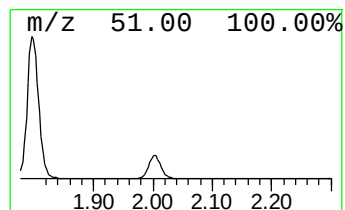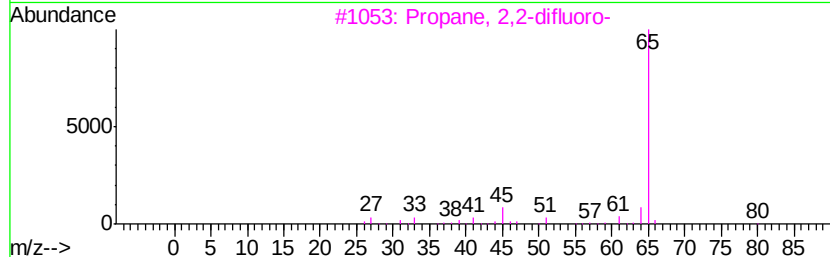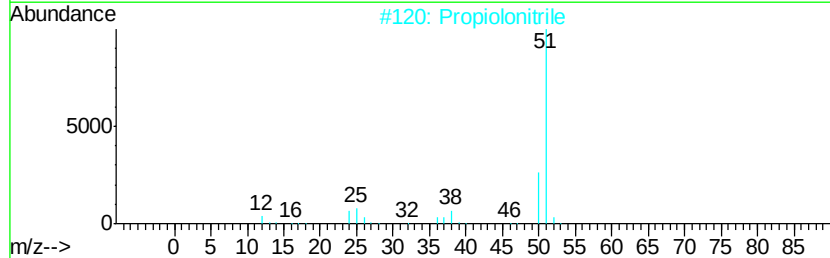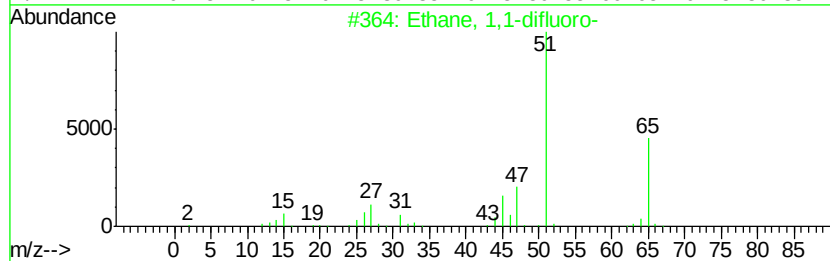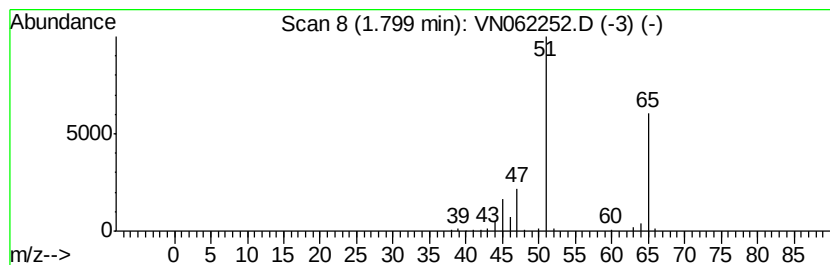

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN063020\
Data File : VN062252.D
Acq On : 30 Jun 2020 20:16
Operator : JC/MD
Sample : L3170-07
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-8










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethane, 1-chloro-1,1-difluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.01	180.63 ug/l	2104510	Pentafluorobenzene	7.63

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3	Ethane, 1-chloro-1,1-difluoro-	100	C2H3ClF2	000075-68-3	83
2		Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	43
3		Benzene, 1-nitro-2-(p-methylphen...	247	C13H10FN03	028987-57-7	1

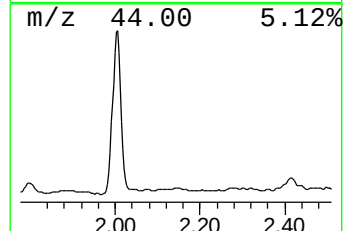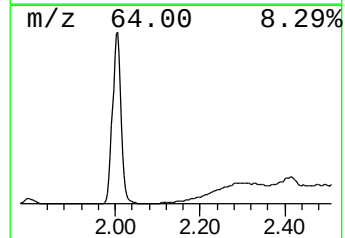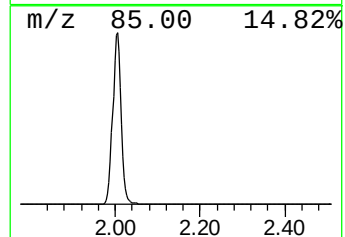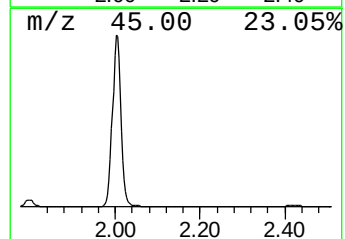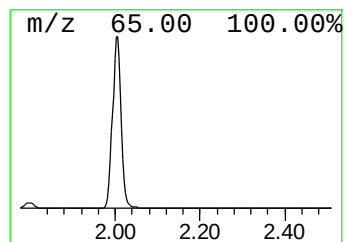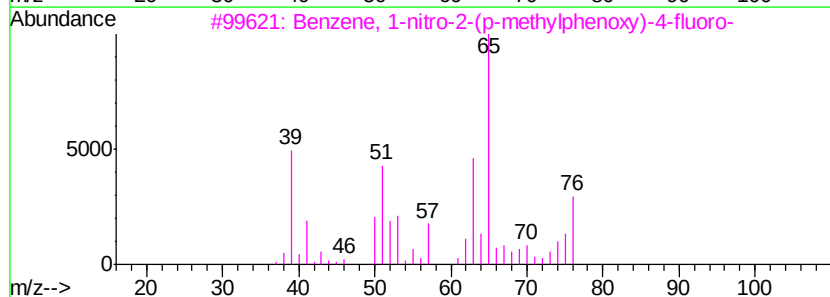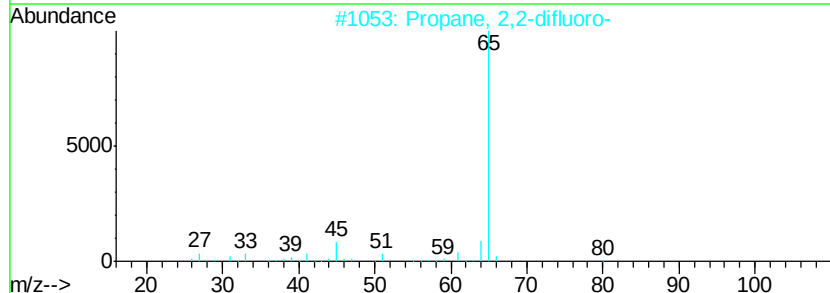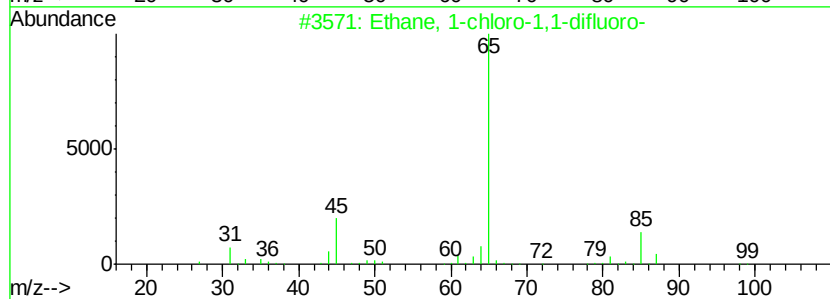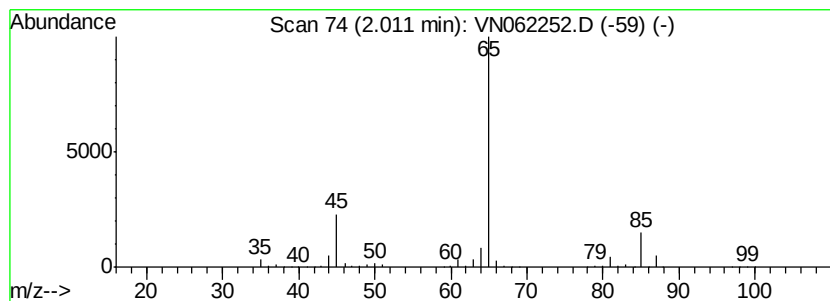

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN063020\
Data File : VN062252.D
Acq On : 30 Jun 2020 20:16
Operator : JC/MD
Sample : L3170-07
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,1-diflu...	1.80	11.3	ug/l	131319	1	7.63	582539	50.0
Ethane, 1-chloro-...	2.01	180.6	ug/l	2104510	1	7.63	582539	50.0