
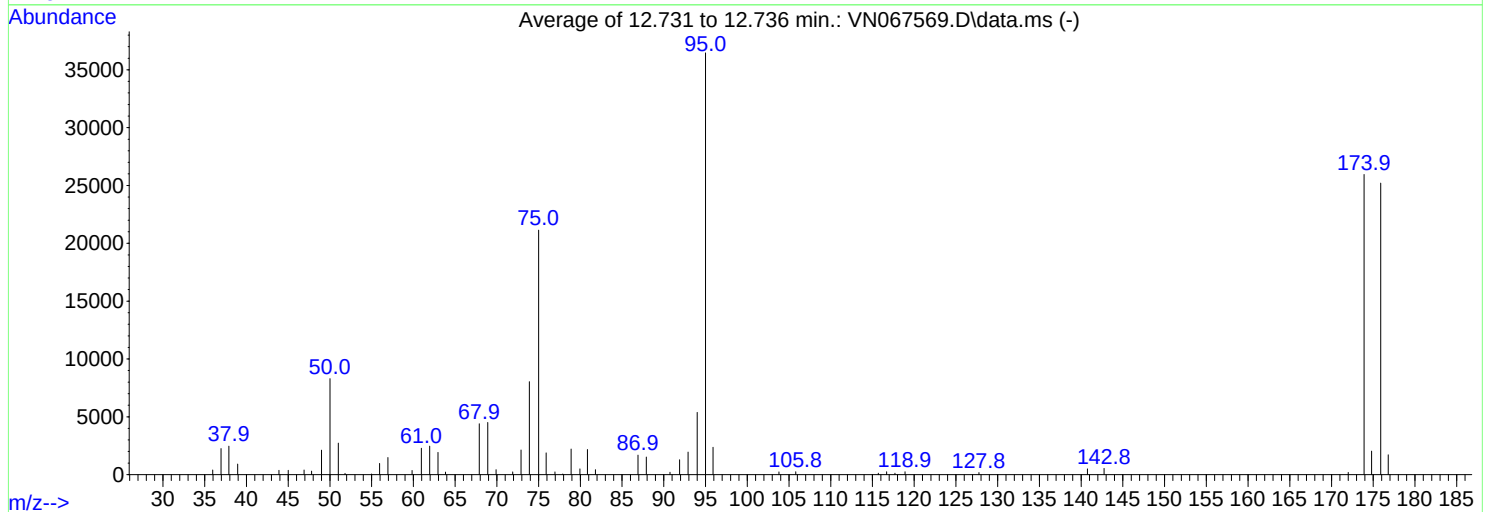


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN063021\
 Data File : VN067569.D
 Acq On : 30 Jun 2021 10:08
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062821W.M
 Title : SW846 8260
 Last Update : Mon Jun 28 14:31:03 2021

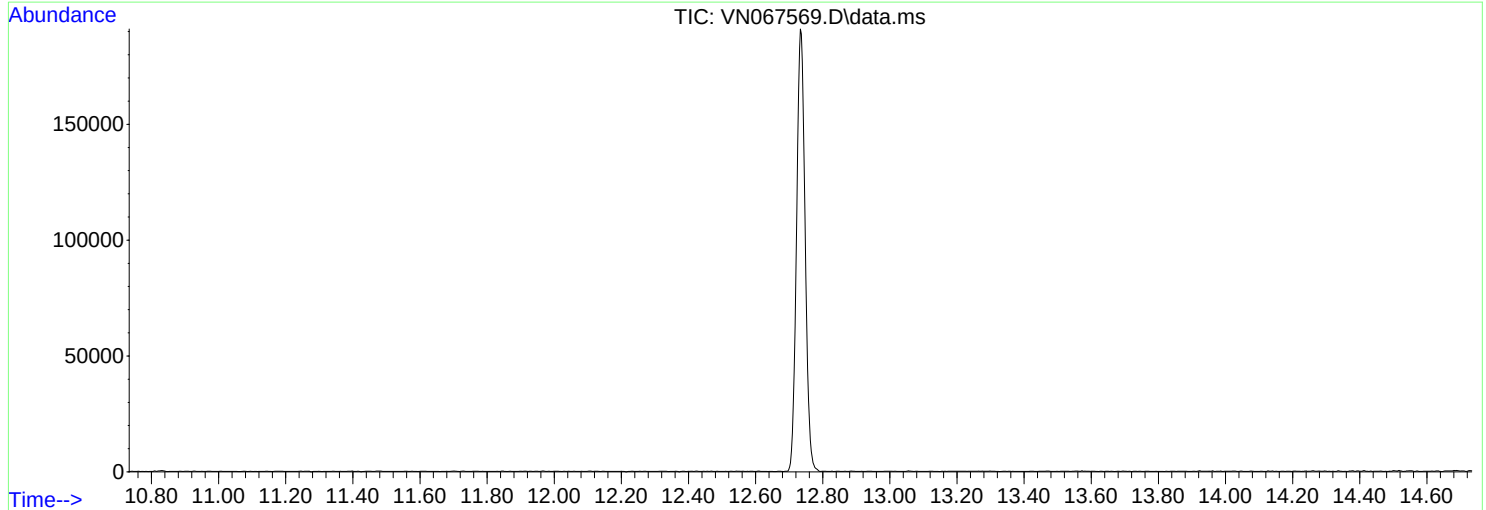

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	8305	PASS
75	95	30	60	58.0	21144	PASS
95	95	100	100	100.0	36467	PASS
96	95	5	9	6.5	2367	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.2	25955	PASS
175	174	5	9	7.8	2028	PASS
176	174	95	101	97.1	25200	PASS
177	176	5	9	6.8	1718	PASS