

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN063022\  
Data File : VN073265.D  
Acq On : 30 Jun 2022 14:59  
Operator : JC\MD  
Sample : N3554-04  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
152140-SPC-01-50

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M

Title : SW846 8260

Signal : TIC: VN073265.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 7.951       | 1021          | 1031        | 1036         | rBV      | 214117         | 512083        | 36.00%          | 6.085%        |
| 2         | 8.016       | 1036          | 1042        | 1055         | rVB      | 397195         | 908975        | 63.89%          | 10.801%       |
| 3         | 8.369       | 1091          | 1102        | 1117         | rBV      | 229727         | 518125        | 36.42%          | 6.157%        |
| 4         | 8.904       | 1181          | 1193        | 1207         | rBV      | 564523         | 1181454       | 83.05%          | 14.039%       |
| 5         | 10.380      | 1435          | 1444        | 1453         | rBV      | 775371         | 1422596       | 100.00%         | 16.905%       |
| 6         | 11.680      | 1657          | 1665        | 1678         | rBV      | 805941         | 1422648       | 100.00%         | 16.905%       |
| 7         | 12.669      | 1826          | 1833        | 1847         | rVB      | 655400         | 1095456       | 77.00%          | 13.017%       |
| 8         | 13.610      | 1986          | 1993        | 2001         | rBV      | 828186         | 1354097       | 95.18%          | 16.091%       |


Sum of corrected areas: 8415434

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN063022\  
Data File : VN073265.D  
Acq On : 30 Jun 2022 14:59  
Operator : JC\MD  
Sample : N3554-04  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
152140-SPC-01-50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

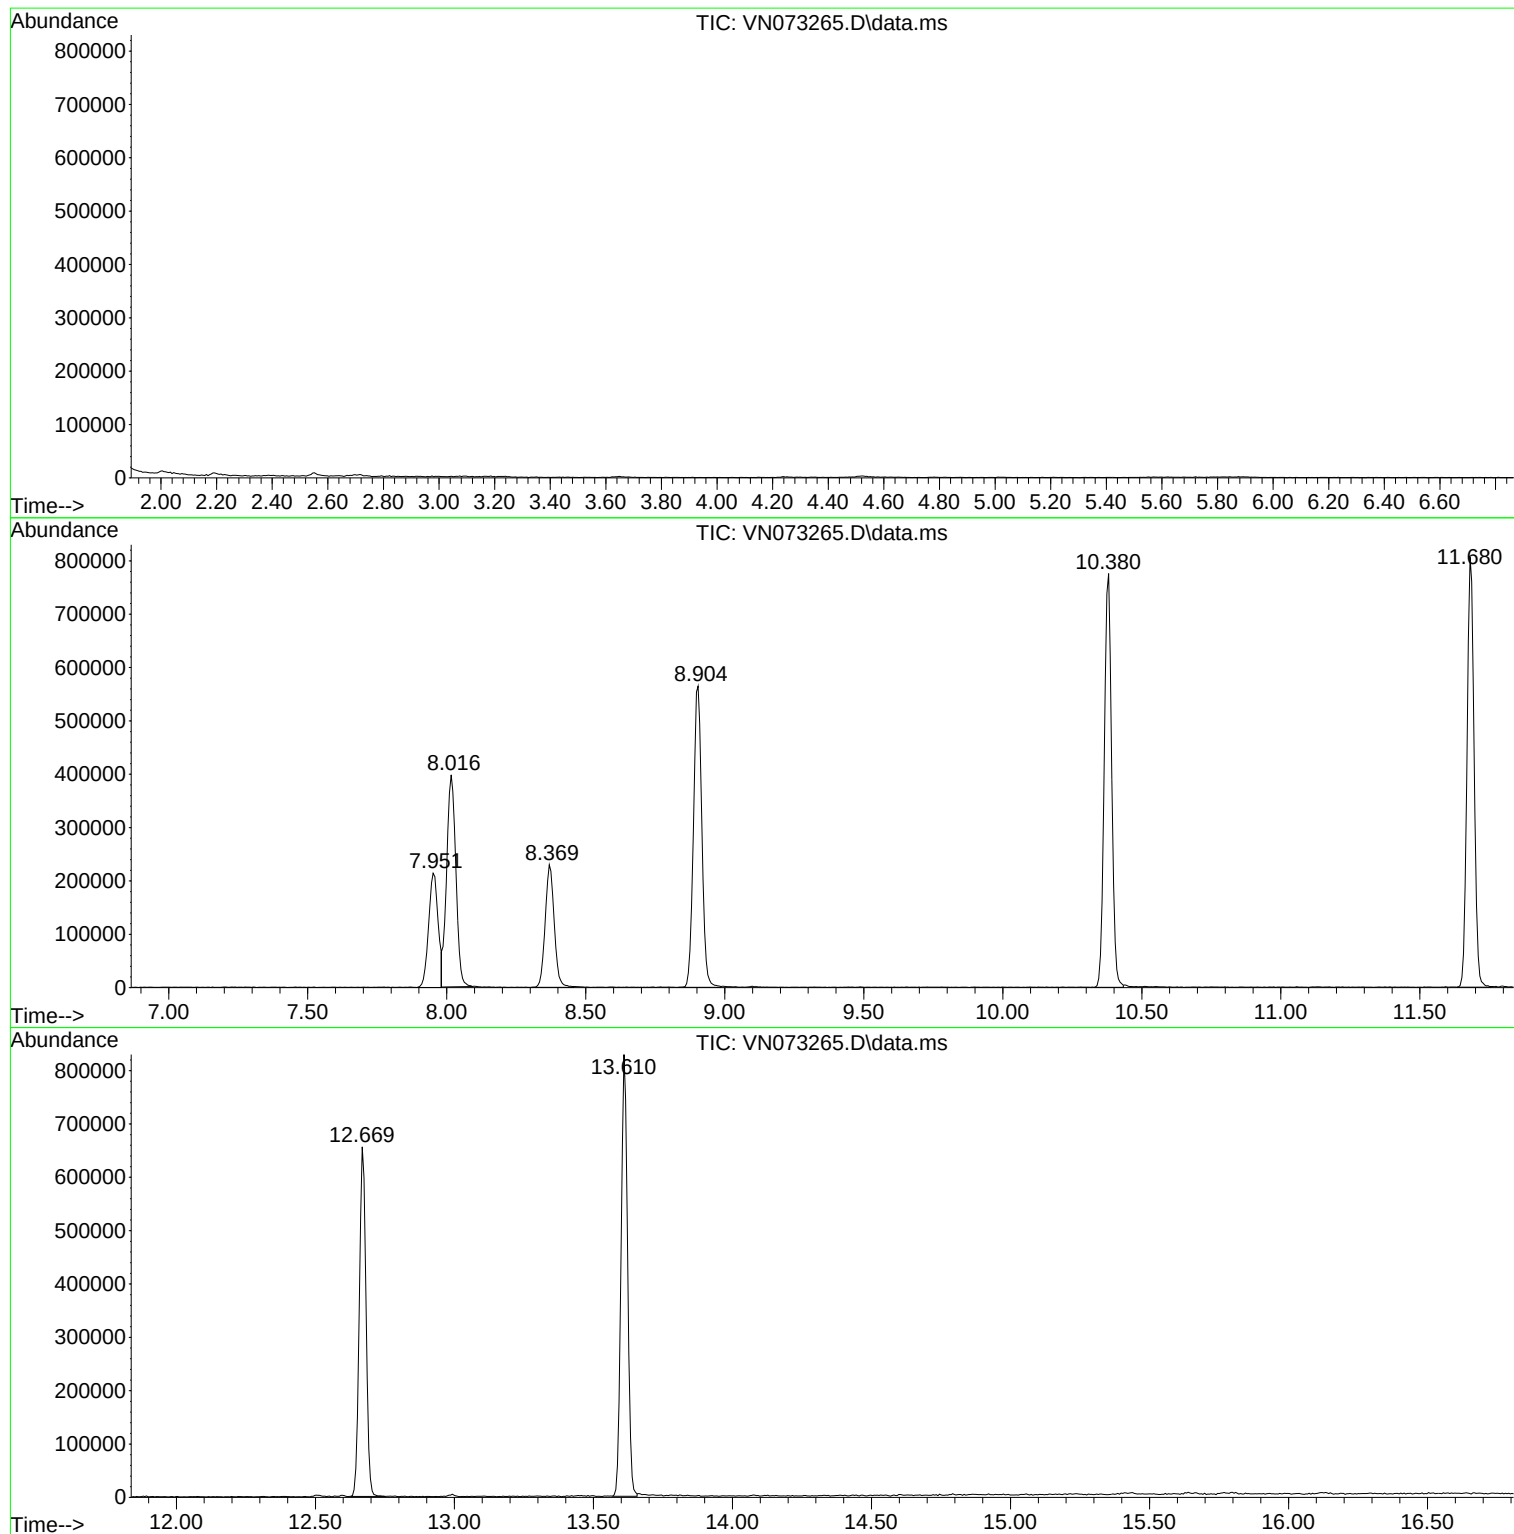

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN063022\  
Data File : VN073265.D  
Acq On : 30 Jun 2022 14:59  
Operator : JC\MD  
Sample : N3554-04  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
152140-SPC-01-50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN063022\  
Data File : VN073265.D  
Acq On : 30 Jun 2022 14:59  
Operator : JC\MD  
Sample : N3554-04  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
152140-SPC-01-50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |