


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN070119\
 Data File : VN056563.D
 Acq On : 1 Jul 2019 11:26
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
 Title : SW846 8260
 Last Update : Fri Jun 21 03:45:40 2019

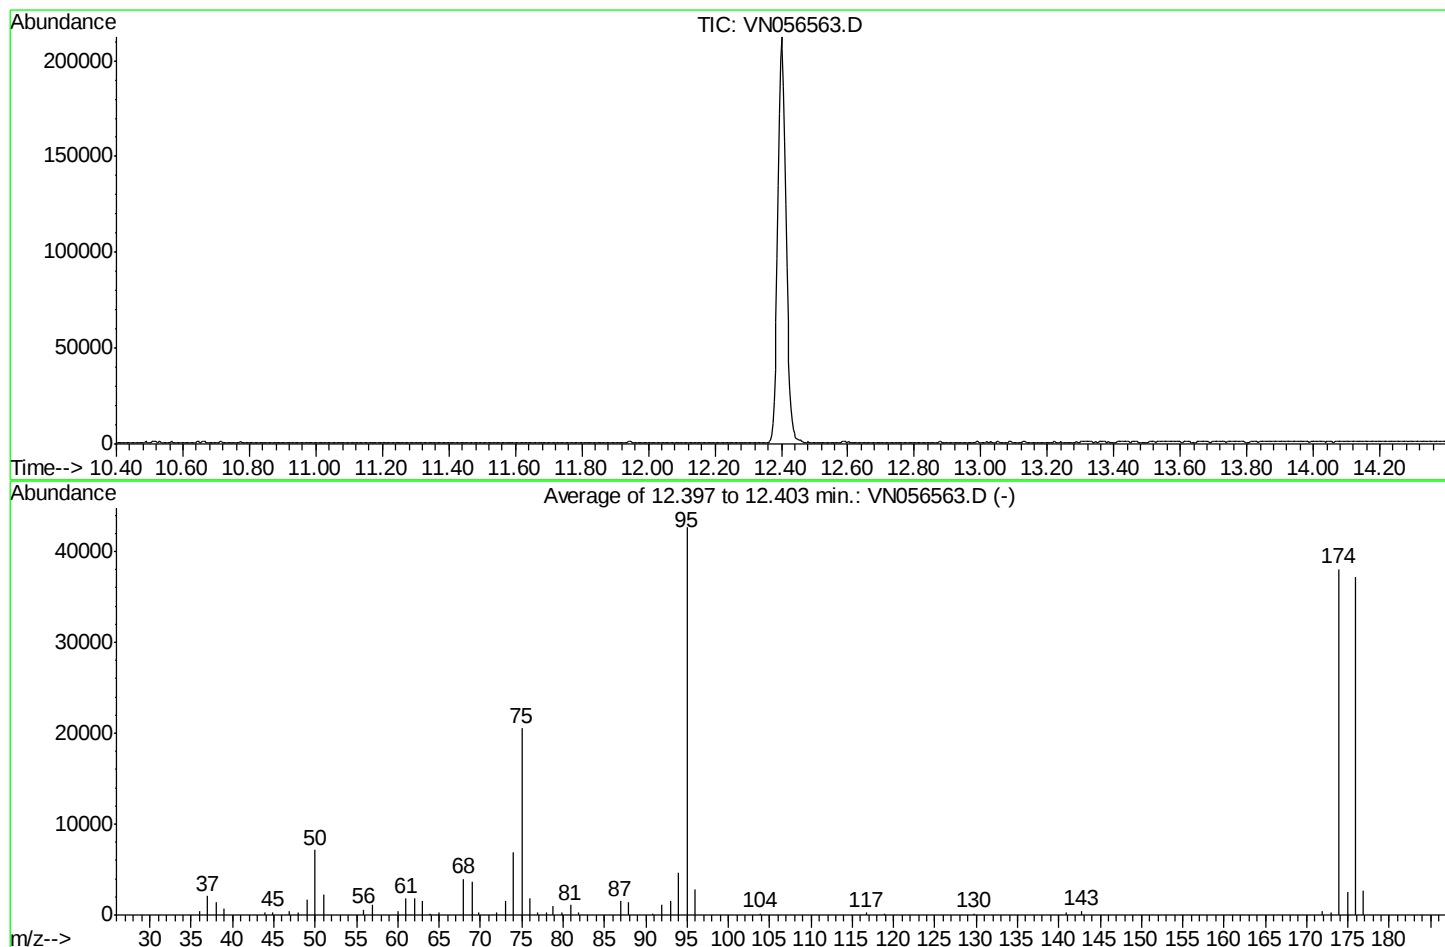

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	7167	PASS
75	95	30	60	48.2	20560	PASS
95	95	100	100	100.0	42656	PASS
96	95	5	9	6.5	2759	PASS
173	174	0.00	2	0.8	286	PASS
174	95	50	100	89.3	38082	PASS
175	174	5	9	6.8	2589	PASS
176	174	95	101	97.8	37234	PASS
177	176	5	9	7.1	2652	PASS