

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070120\
 Data File : VN062287.D
 Acq On : 1 Jul 2020 13:14
 Operator : JC/MD
 Sample : L3170-06DL 5X
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-7DL

Quant Time: Jul 02 06:52:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	191347	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	376805	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	358279	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	125148	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	7.99	65	153769	57.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	114.52%	
35) Dibromofluoromethane	7.55	113	120781	49.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.92%	
50) Toluene-d8	10.06	98	485589	50.25	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.50%	
62) 4-Bromofluorobenzene	12.38	95	153958	47.16	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.32%	

Target Compounds


						Qvalue
3) Chloromethane	2.03	50	428	Below Cal	#	41
11) Tert butyl alcohol	4.73	59	136038	352.850	ug/l	100
15) Acrylonitrile	5.00	53	7211	6.864	ug/l #	37
16) Acetone	3.78	43	584	Below Cal	#	40
17) Carbon Disulfide	4.01	76	1898	0.352	ug/l #	75
18) Methyl Acetate	4.27	43	610	0.286	ug/l #	46
19) Methyl tert-butyl Ether	4.99	73	555353	79.102	ug/l	99
20) Methylene Chloride	4.50	84	2278	0.710	ug/l	91
22) Diisopropyl ether	5.90	45	8560	1.257	ug/l #	97
23) Vinyl Acetate	5.91	43	5283	0.950	ug/l #	68
31) Cyclohexane	7.62	56	4853	1.308	ug/l #	1
36) 1,1-Dichloropropene	7.63	75	17137	4.525	ug/l #	48
38) Carbon Tetrachloride	7.63	117	19916	5.578	ug/l #	16
42) 1,2-Dichloroethane	8.09	62	998	0.256	ug/l #	73
43) Isopropyl Acetate	8.09	43	1050	0.205	ug/l #	58
51) 4-Methyl-2-Pentanone	9.95	43	825	0.276	ug/l #	33
59) 2-Hexanone	10.73	43	1021	0.473	ug/l #	44
71) Bromoform	12.37	173	1355	0.700	ug/l #	1
74) N-amyl acetate	12.05	43	662	3.516	ug/l #	41
76) 1,2,3-Trichloropropane	12.38	75	79404	26.952	ug/l #	100
79) 2-Chlorotoluene	12.75	91	1476	0.220	ug/l	80
81) trans-1,4-Dichloro-2-buten	12.38	75	79404	78.711	ug/l #	13
82) 4-Chlorotoluene	12.75	91	1476	0.213	ug/l	81
93) 1,2,4-Trichlorobenzene	14.89	180	772	0.432	ug/l #	76
95) Naphthalene	15.11	128	3027	4.462	ug/l #	90
96) 1,2,3-Trichlorobenzene	15.29	180	944	0.516	ug/l #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN070120\
Data File : VN062287.D
Acq On : 1 Jul 2020 13:14
Operator : JC/MD
Sample : L3170-06DL 5X
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-7DL

Quant Time: Jul 02 06:52:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 24 15:33:00 2020
Response via : Initial Calibration

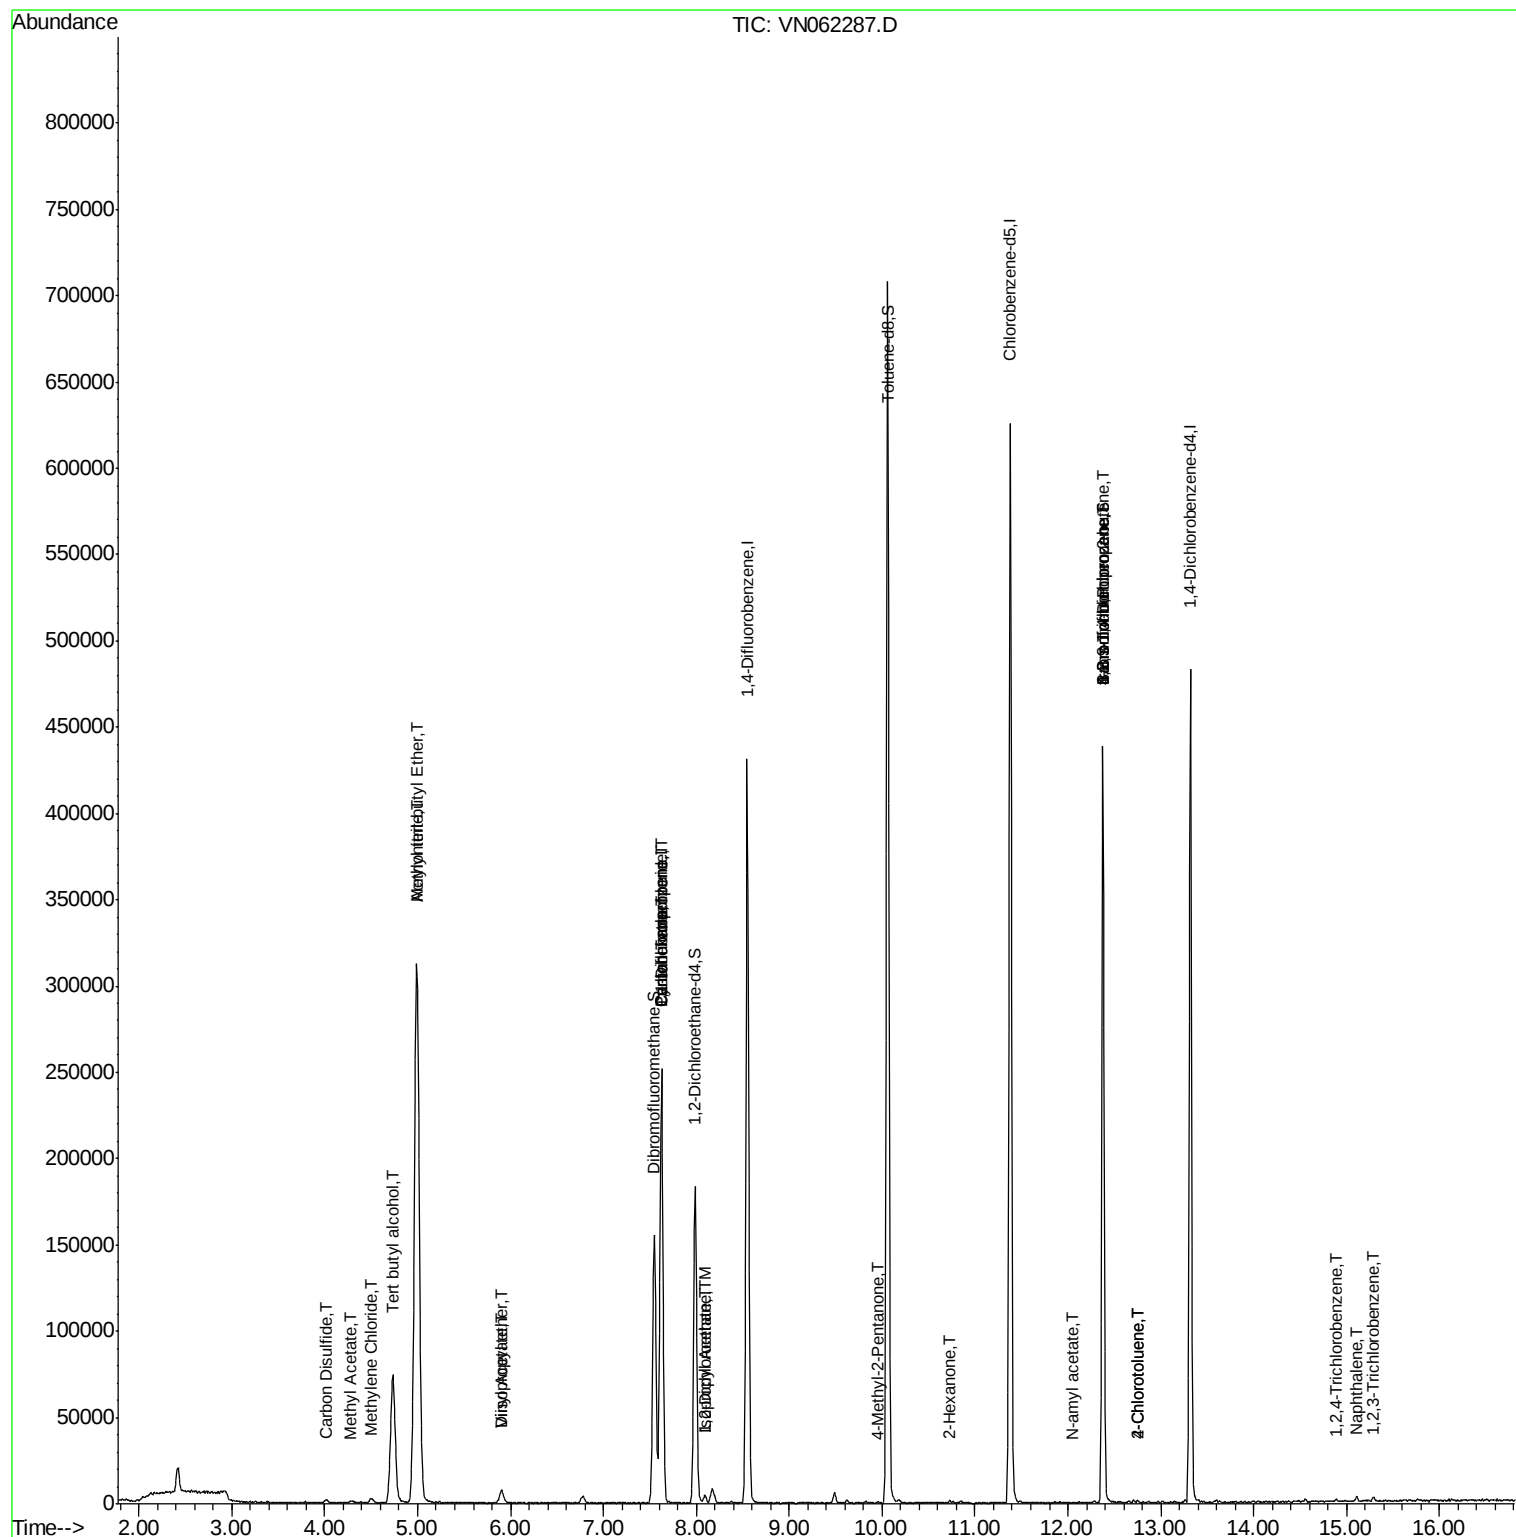



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14

Instrument :

MSVOA_N

ClientSampleId :


MW-7DL

Tot Ion:168 Resp: 191347

Ion Ratio Lower Upper




168 100

99 61.6 45.8 68.8



Abundance Ion 167.90 (167.60 to 168.60): VN062287.D

Ion 98.90 (98.60 to 99.60): VN062287.D

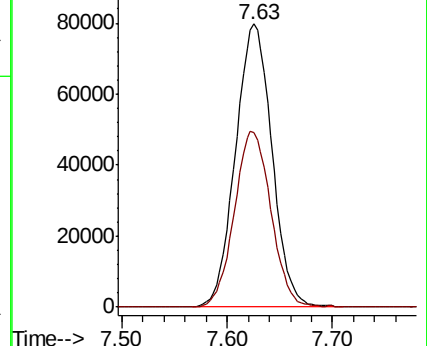

#3

Chloromethane

Concen: Below Cal

RT: 2.03 min Scan# 81

Delta R.T. 0.00 min

Lab File: VN062287.D


Acq: 1 Jul 2020 13:14

Tgt Ion: 50 Resp: 428

Ion Ratio Lower Upper



50 100


52 0.0 27.0 40.6#



Abundance Ion 49.90 (49.60 to 50.60): VN062287.D

Ion 51.90 (51.60 to 52.60): VN062287.D

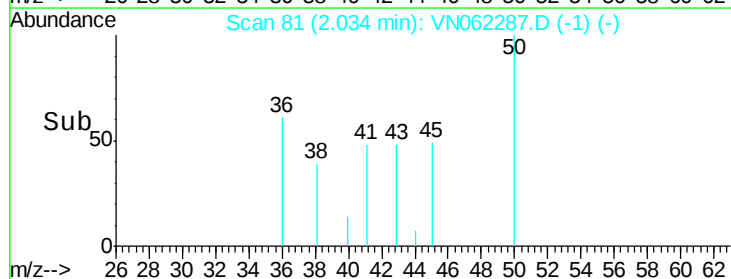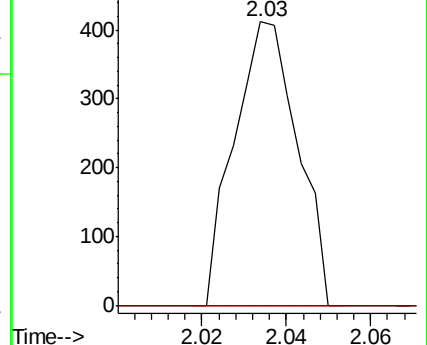




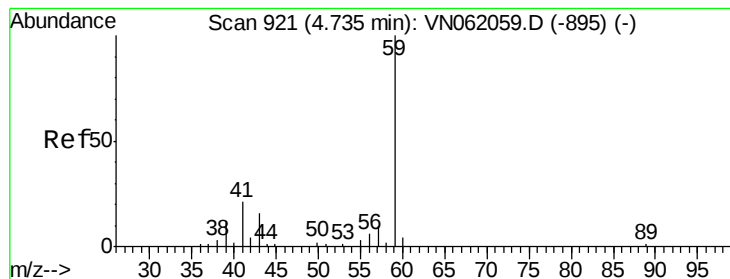


#11

Tert butyl alcohol
 Concen: 352.850 ug/l
 RT: 4.73 min Scan# 921
 Delta R.T. -0.00 min
 Lab File: VN062287.D
 Acq: 1 Jul 2020 13:14

Instrument :
 MSVOA_N
 ClientSampled :
 MW-7DL




Tot Ion: 59 Resp: 136038
 Ion Ratio Lower Upper
 59 100
 57 10.3 8.3 12.5

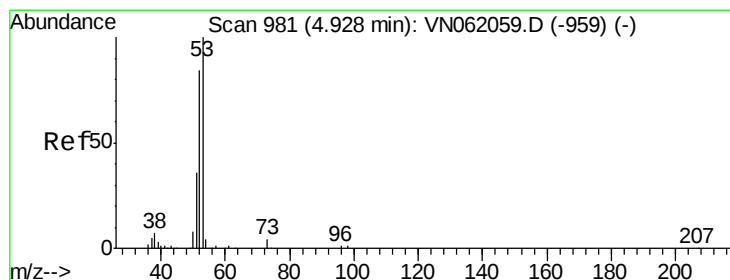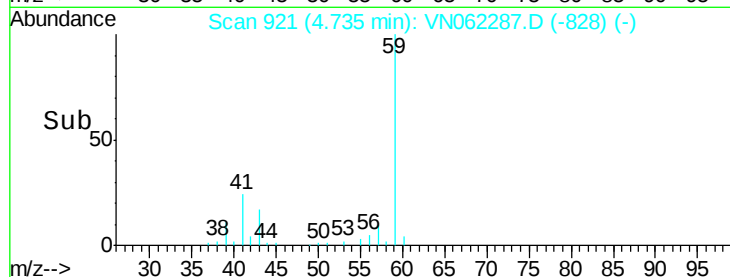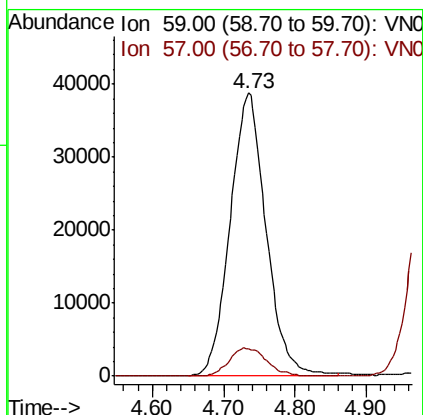


#15

Acrylonitrile
 Concen: 6.864 ug/l
 RT: 5.00 min Scan# 1002
 Delta R.T. 0.07 min
 Lab File: VN062287.D
 Acq: 1 Jul 2020 13:14

Tgt Ion: 53 Resp: 7211
 Ion Ratio Lower Upper
 53 100
 52 3.1 66.2 99.4#
 51 39.2 28.9 43.3


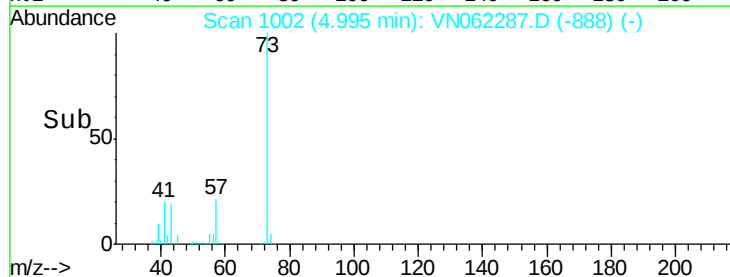
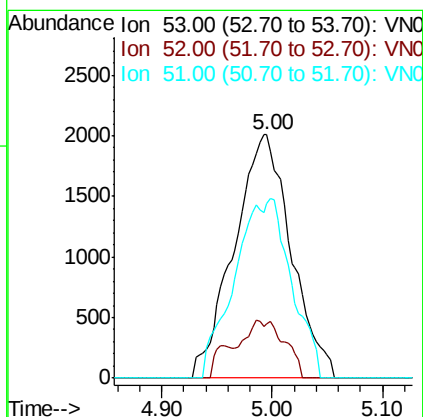



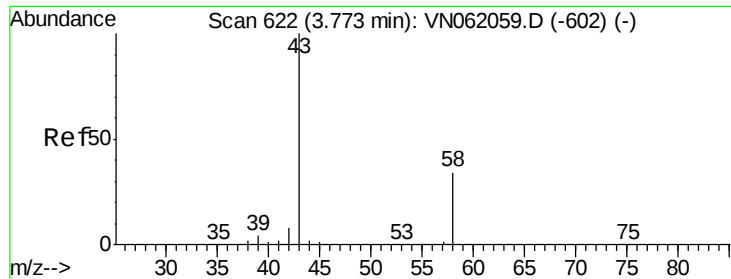

#16
Acetone
Concen: Below Cal
RT: 3.78 min Scan# 623
Delta R.T. 0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14




Instrument :
MSVOA_N
ClientSampleId :
MW-7DL


Tot Ion: 43 Resp: 584
Ion Ratio Lower Upper
43 100
58 0.0 27.5 41.3#

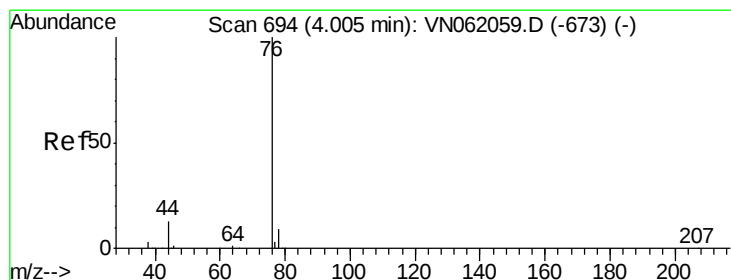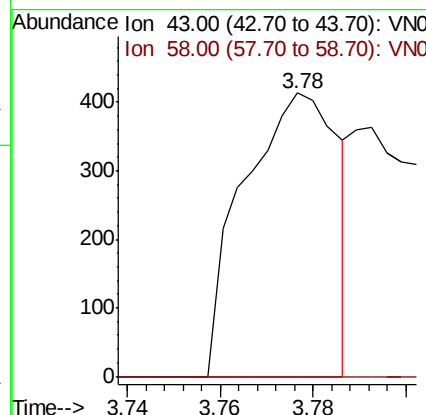

#17
Carbon Disulfide
Concen: 0.352 ug/l
RT: 4.01 min Scan# 696
Delta R.T. 0.01 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14

Tgt Ion: 76 Resp: 1898
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


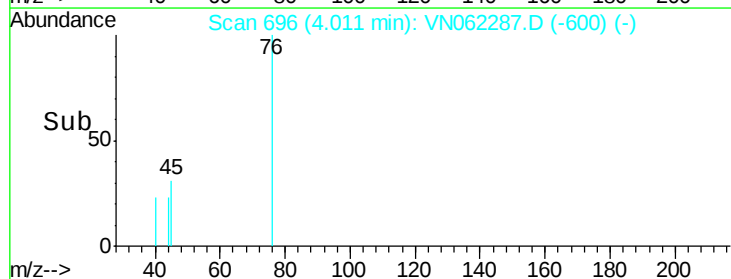
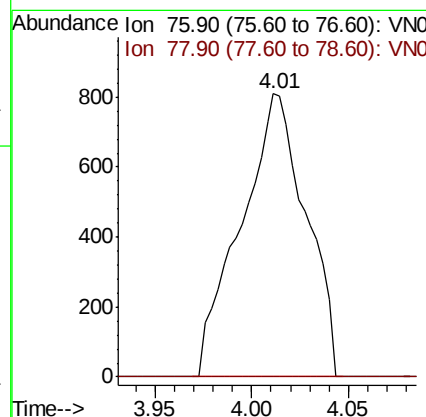
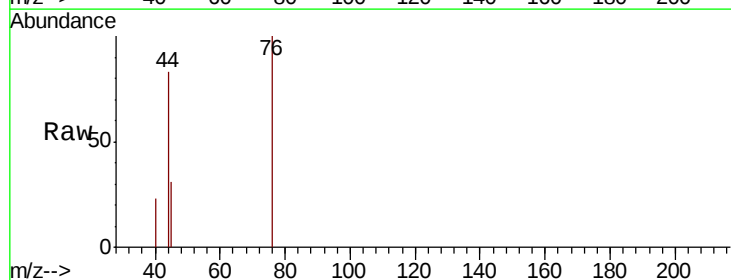


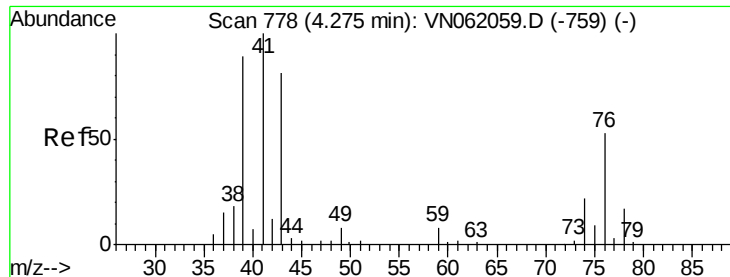

#18
Methyl Acetate
Concen: 0.286 ug/l
RT: 4.27 min Scan# 777
Delta R.T. -0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14




Instrument :
MSVOA_N
ClientSampled :
MW-7DL




Tot Ion: 43 Resp: 610
Ion Ratio Lower Upper
43 100
74 0.0 22.9 34.3#

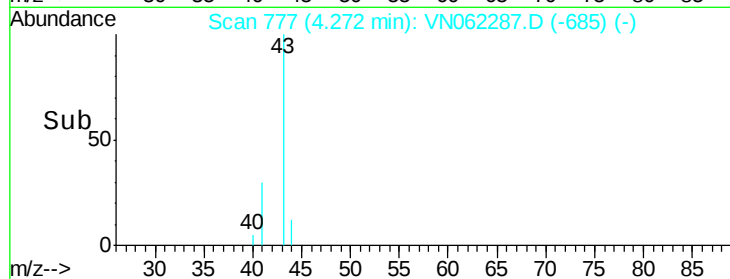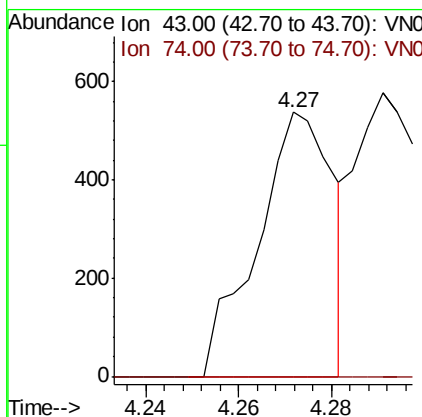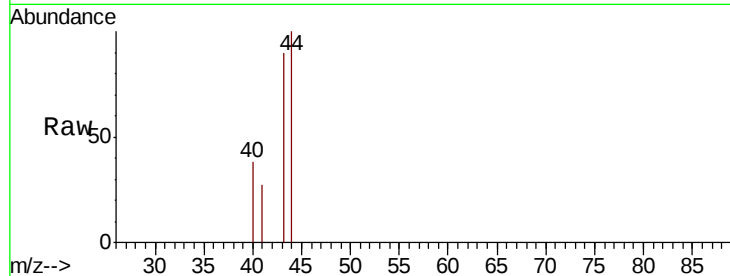

#19
Methyl tert-butyl Ether
Concen: 79.102 ug/l
RT: 4.99 min Scan# 1001
Delta R.T. 0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14

Tgt Ion: 73 Resp: 555353
Ion Ratio Lower Upper
73 100
57 21.1 16.6 24.8


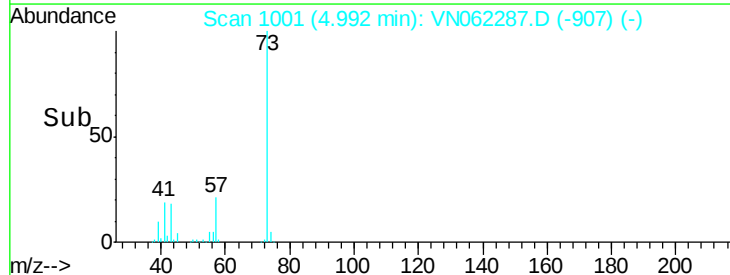
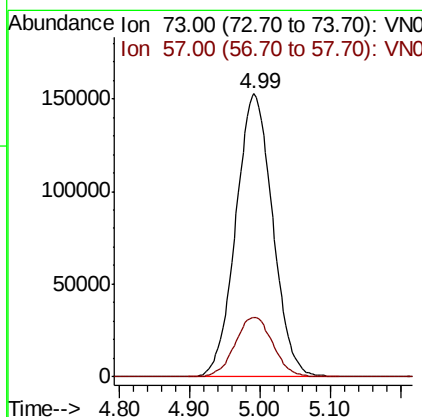



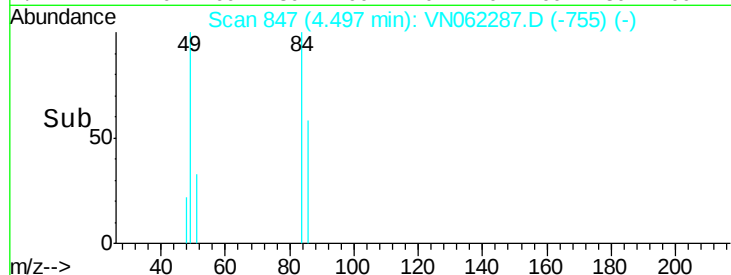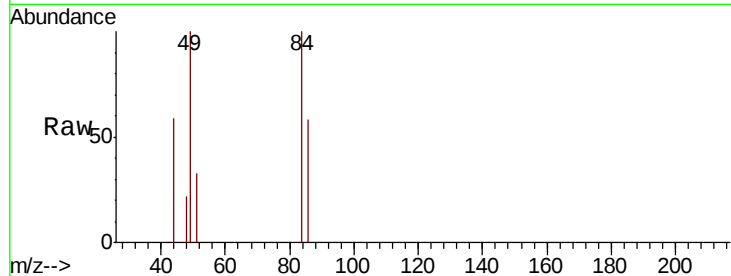

#20
Methvlene Chloride
Concen: 0.710 ug/l
RT: 4.50 min Scan# 847
Delta R.T. -0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14


Instrument :
MSVOA_N
ClientSampled :
MW-7DL


Tot Ion:	84	Resp:	2278
Ion	Ratio	Lower	Upper
84	100		
49	99.5	90.6	136.0
51	32.7	27.8	41.8
86	58.5	50.1	75.1

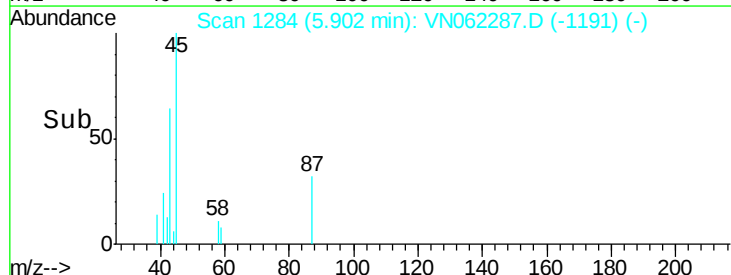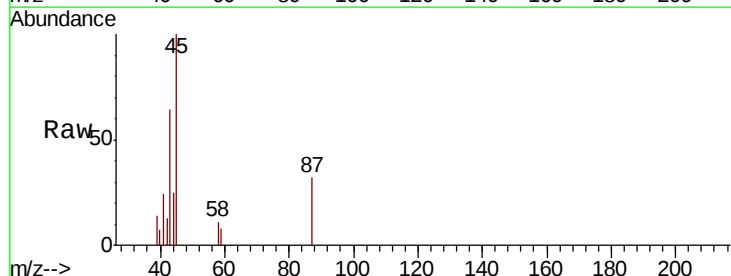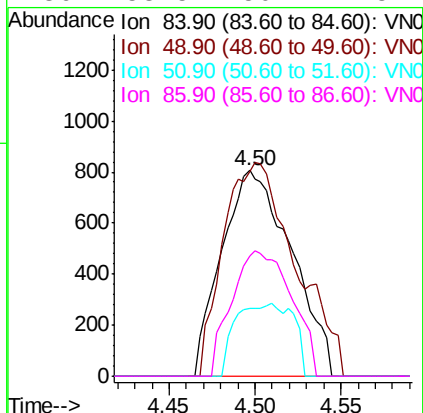

#22
Diisopropyl ether
Concen: 1.257 ug/l
RT: 5.90 min Scan# 1284
Delta R.T. -0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14

Tgt Ion:	45	Resp:	8560
Ion	Ratio	Lower	Upper
45	100		
43	63.6	49.7	74.5
87	32.0	25.9	38.9
59	8.4	10.6	16.0#

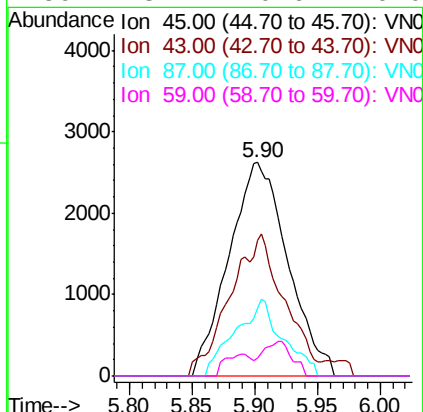



#23

Vinyl Acetate

Concen: 0.950 ug/l

RT: 5.91 min Scan# 1285

Delta R.T. 0.06 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14

Instrument :

MSVOA_N

ClientSampleId :


MW-7DL

Tot Ion: 43 Resp: 5283

Ion Ratio Lower Upper




43 100

86 0.0 10.1 15.1#



Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 86.00 (85.70 to 86.70): VNO

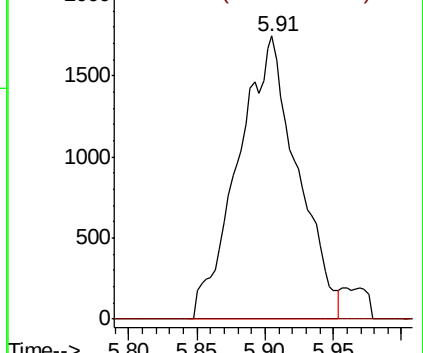

#31

Cyclohexane

Concen: 1.308 ug/l

RT: 7.62 min Scan# 1819

Delta R.T. 0.01 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14


Tgt Ion: 56 Resp: 4853

Ion Ratio Lower Upper

56 100

69 177.8 28.0 42.0#



84 144.4 76.1 114.1#




Abundance Ion 56.00 (55.70 to 56.70): VNO

Ion 69.00 (68.70 to 69.70): VNO

Ion 84.00 (83.70 to 84.70): VNO




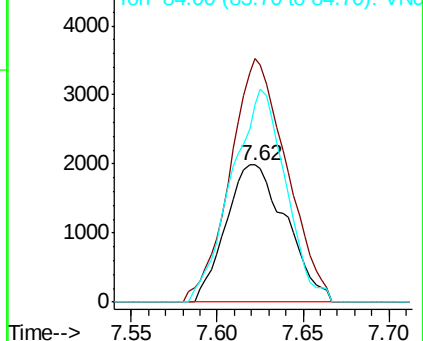


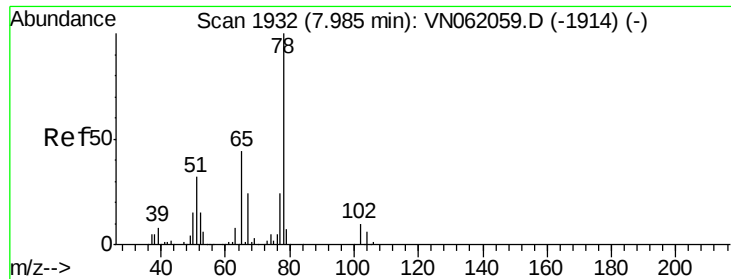

#33
 1,2-Dichloroethane-d4
 Concen: 57.265 ug/l
 RT: 7.99 min Scan# 1933
 Delta R.T. 0.00 min
 Lab File: VN062287.D
 Acq: 1 Jul 2020 13:14




Instrument :
 MSVOA_N
 ClientSampled :
 MW-7DL


Tot Ion: 65 Resp: 153769
 Ion Ratio Lower Upper
 65 100
 67 52.3 0.0 106.2

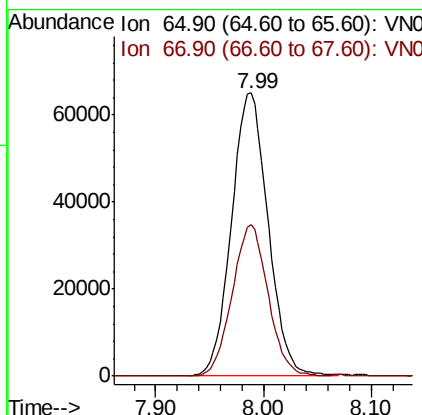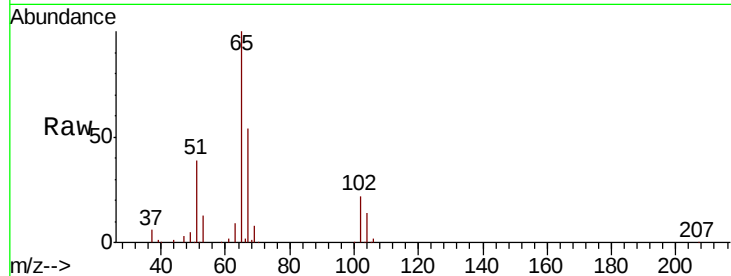

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. -0.00 min
 Lab File: VN062287.D
 Acq: 1 Jul 2020 13:14

Tgt Ion: 114 Resp: 376805
 Ion Ratio Lower Upper
 114 100
 63 21.1 0.0 39.2
 88 16.1 0.0 30.8


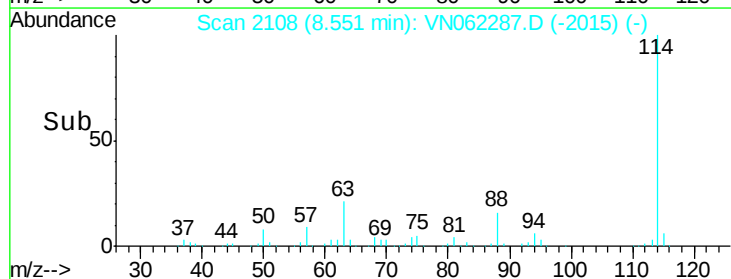
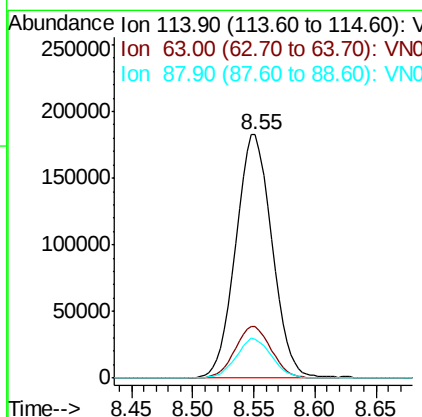



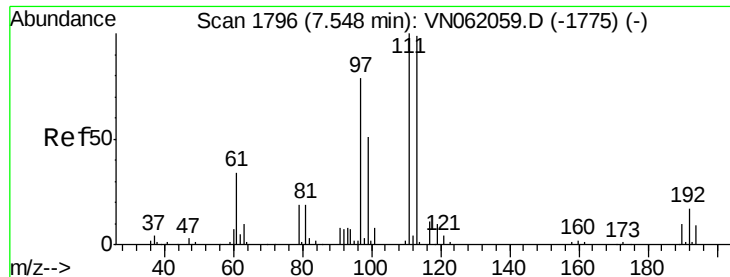

#35
Dibromofluoromethane
Concen: 49.964 ug/l
RT: 7.55 min Scan# 1796
Delta R.T. -0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14




Instrument :
MSVOA_N
ClientSampleId :
MW-7DL


Tot Ion:113 Resp: 120781
Ion Ratio Lower Upper
113 100
111 104.0 82.2 123.4
192 16.4 14.0 21.0

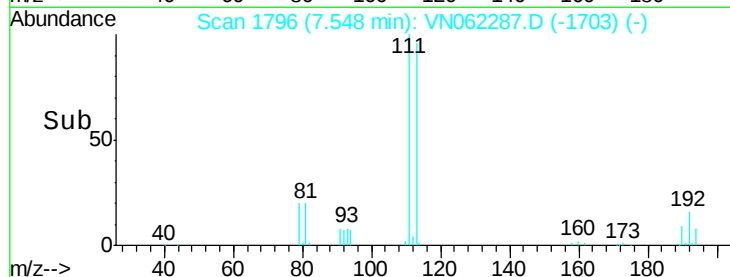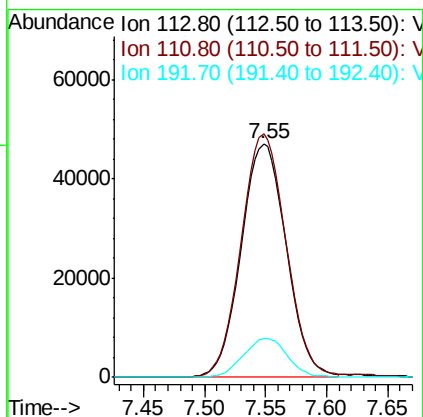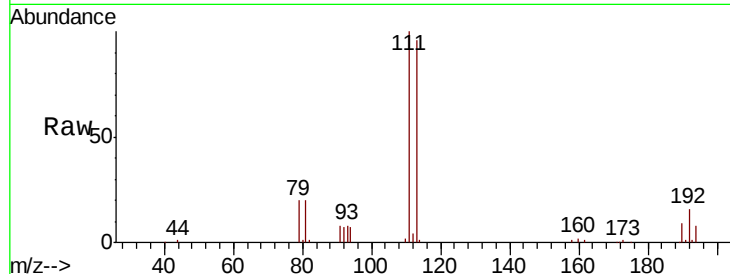

#36
1,1-Dichloropropene
Concen: 4.525 ug/l
RT: 7.63 min Scan# 1820
Delta R.T. -0.13 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14

Tgt Ion: 75 Resp: 17137
Ion Ratio Lower Upper
75 100
110 7.3 17.9 53.8#
77 0.0 24.9 37.3#

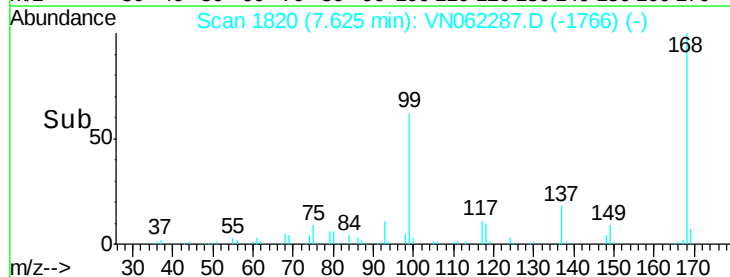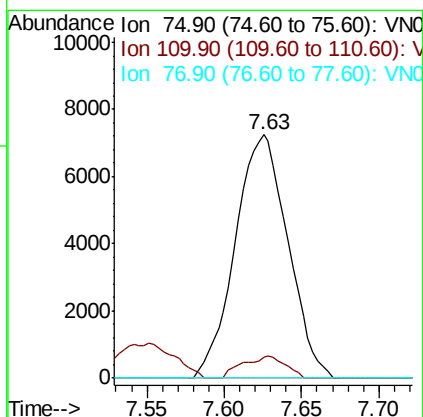

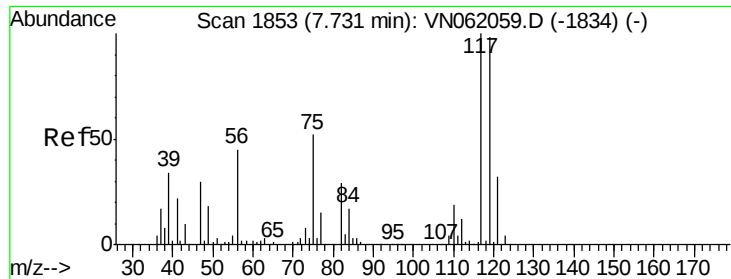

#38

Carbon Tetrachloride

Concen: 5.578 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.11 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14

Instrument :

MSVOA_N

ClientSampled :

MW-7DL


Tot Ion:117 Resp: 19916

Ion Ratio Lower Upper

117 100

119 6.5 78.2 117.2#




121 0.0 25.8 38.6#

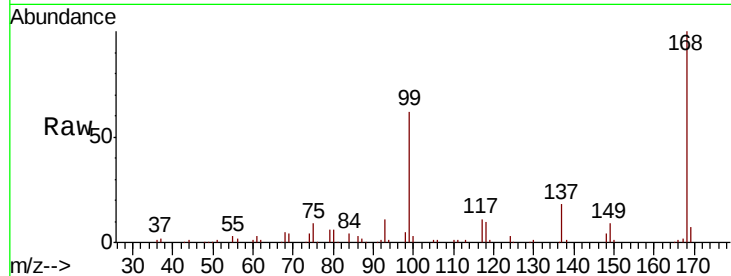

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

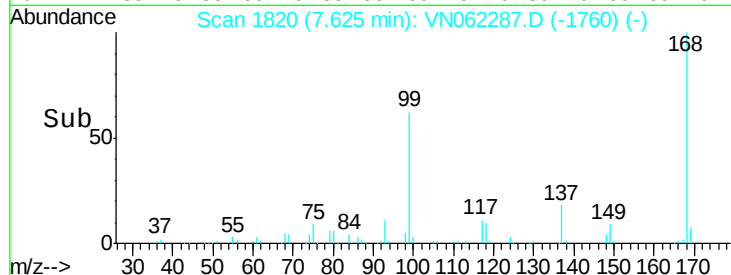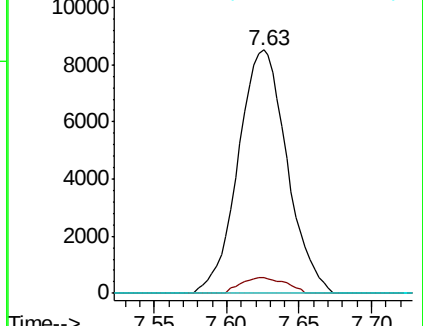

#42

1,2-Dichloroethane

Concen: 0.256 ug/l

RT: 8.09 min Scan# 1965

Delta R.T. 0.01 min

Lab File: VN062287.D


Acq: 1 Jul 2020 13:14

Tgt Ion: 62 Resp: 998

Ion Ratio Lower Upper



62 100


98 0.0 0.0 19.8



Abundance Ion 61.90 (61.60 to 62.60): V

Ion 97.90 (97.60 to 98.60): V



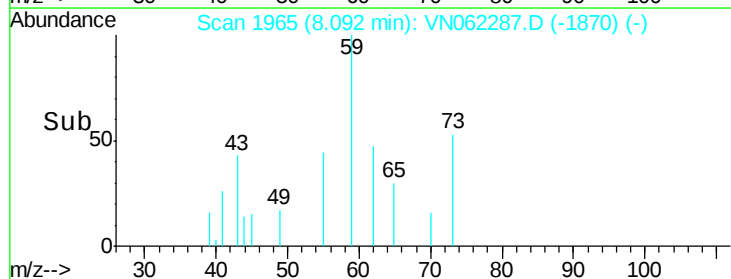
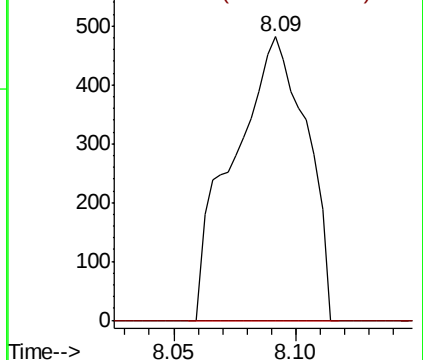




#43
Isopropyl Acetate
Concen: 0.205 ug/l
RT: 8.09 min Scan# 1966
Delta R.T. -0.03 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14




Instrument :
MSVOA_N
ClientSampleId :
MW-7DL


Tot Ion: 43 Resp: 1050
Ion Ratio Lower Upper
43 100
61 0.0 17.2 25.8#
87 0.0 12.1 18.1#

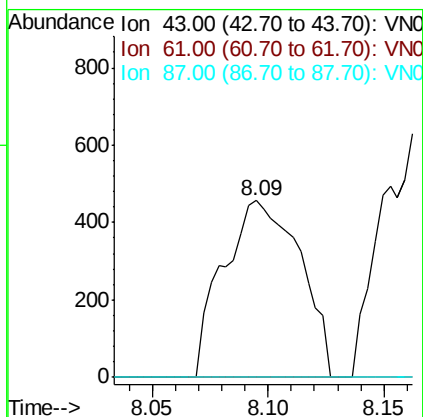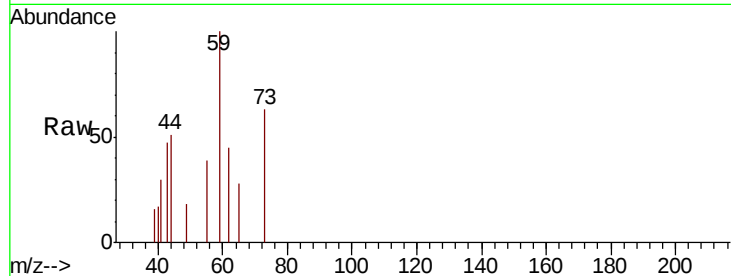

#50
Toluene-d8
Concen: 50.252 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. -0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14

Tgt Ion: 98 Resp: 485589
Ion Ratio Lower Upper
98 100
100 64.5 51.2 76.8

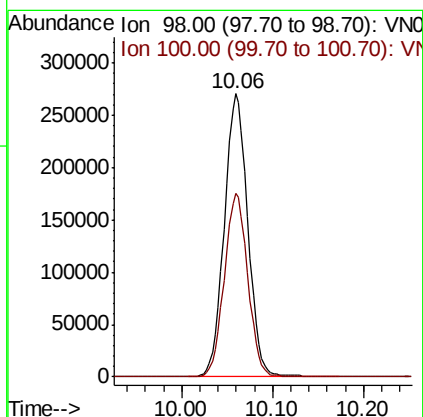

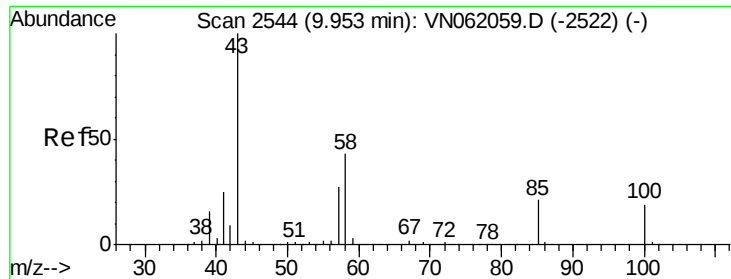

#51

4-Methyl-2-Pentanone

Concen: 0.276 ug/l

RT: 9.95 min Scan# 2544

Delta R.T. -0.00 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14

Instrument :

MSVOA_N

ClientSampled :





MW-7DL

Tot Ion: 43 Resp: 825

Ion Ratio Lower Upper

43 100

58 0.0 34.2 51.2#

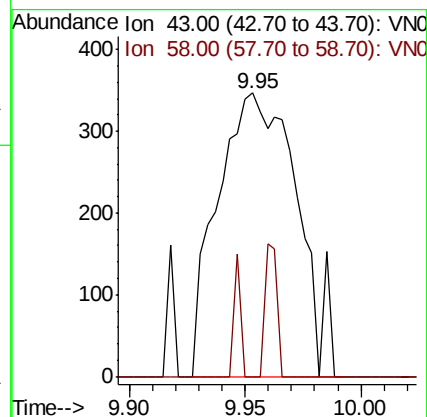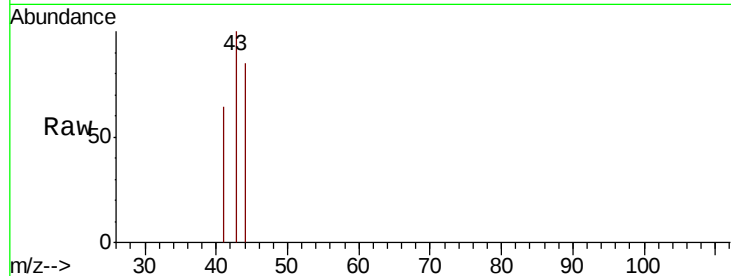

#59

2-Hexanone

Concen: 0.473 ug/l

RT: 10.73 min Scan# 2786

Delta R.T. 0.01 min

Lab File: VN062287.D




Acq: 1 Jul 2020 13:14


Tgt Ion: 43 Resp: 1021

Ion Ratio Lower Upper

43 100

58 16.8 29.5 88.5#

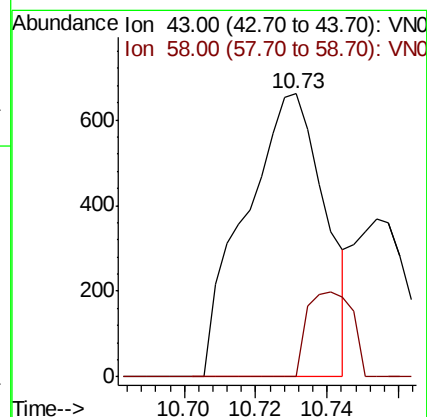



#62

4-Bromofluorobenzene

Concen: 47.158 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.00 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14

Instrument :

MSVOA_N

ClientSampleId :

MW-7DL


Tot Ion: 95 Resp: 153958

Ion Ratio Lower Upper

95 100

174 71.7 0.0 154.8




176 69.4 0.0 147.4

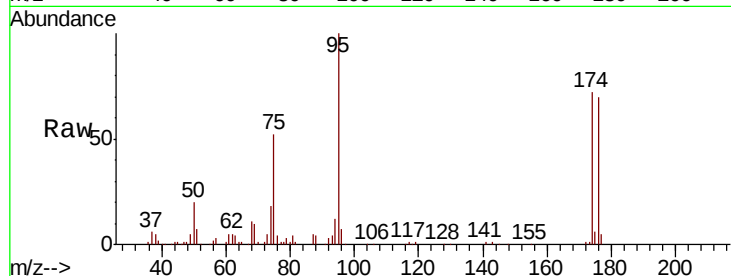

Abundance Ion 94.90 (94.60 to 95.60): VN062287.D (-3205) (-)

Ion 173.80 (173.50 to 174.50): VN062287.D (-3205) (-)

Ion 175.80 (175.50 to 176.50): VN062287.D (-3205) (-)

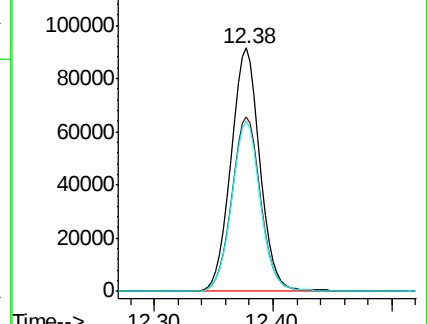

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2987

Delta R.T. -0.00 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14


Tgt Ion: 117 Resp: 358279

Ion Ratio Lower Upper

117 100

82 58.4 43.8 65.8



119 32.0 25.2 37.8




Abundance Ion 116.90 (116.60 to 117.60): VN062287.D (-2895) (-)

Ion 82.00 (81.70 to 82.70): VN062287.D (-2895) (-)

Ion 118.90 (118.60 to 119.60): VN062287.D (-2895) (-)




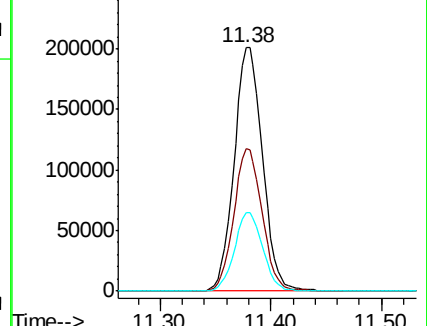




#71
Bromoform
Concen: 0.700 ug/l
RT: 12.37 min Scan# 3297
Delta R.T. 0.27 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14




Instrument :
MSVOA_N
ClientSampled :
MW-7DL


Tot Ion:173 Resp: 1355
Ion Ratio Lower Upper
173 100
175 564.1 24.7 74.1#
254 0.0 0.0 0.0

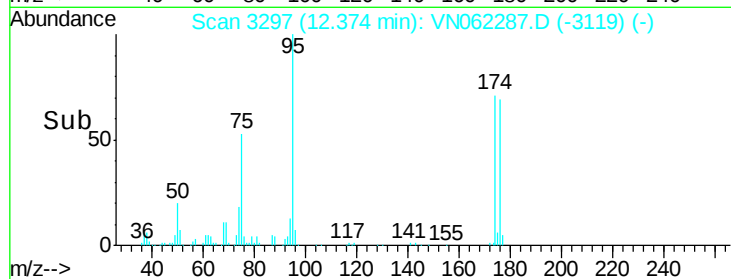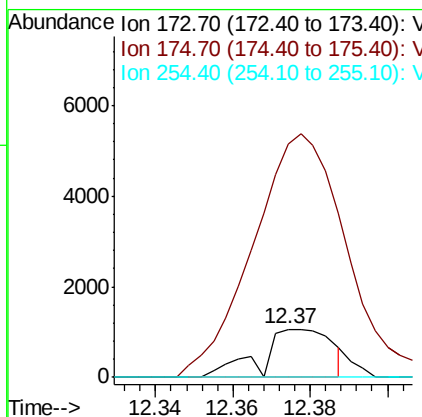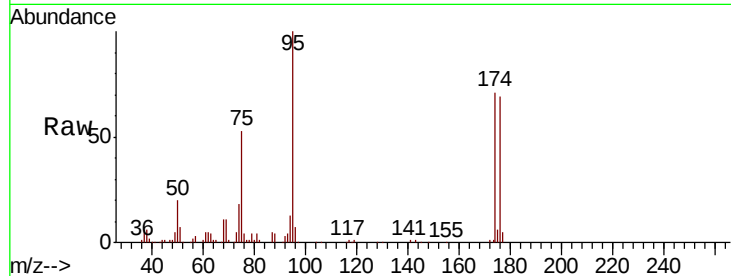

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3591
Delta R.T. 0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14

Tgt Ion:152 Resp: 125148
Ion Ratio Lower Upper
152 100
115 61.9 29.5 88.5
150 161.3 0.0 351.4

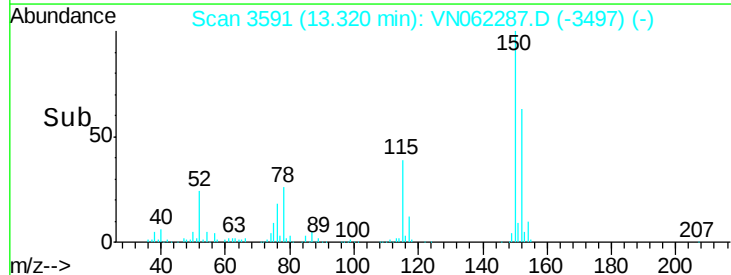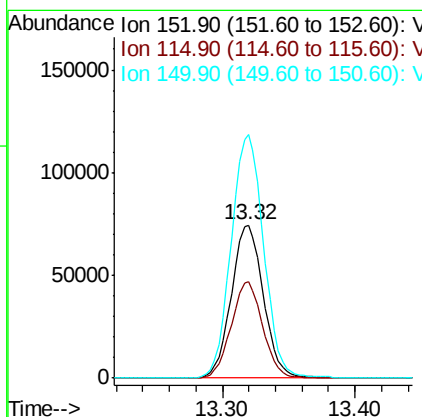

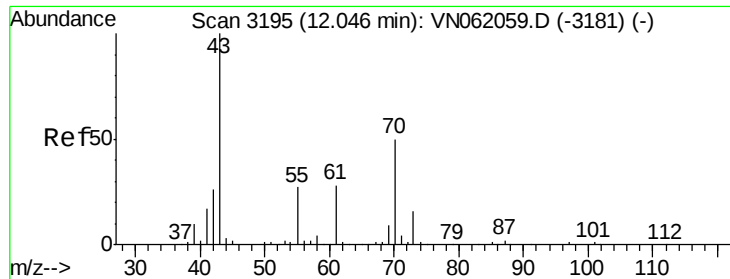

#74

N-amvl acetate

Concen: 3.516 ug/l

RT: 12.05 min Scan# 3196

Delta R.T. 0.00 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14

Instrument :

MSVOA_N

ClientSampled :

MW-7DL

Tot Ion: 43 Resp: 662


Ion Ratio Lower Upper

43 100

70 4.4 39.4 59.2#

55 0.0 21.7 32.5#

61 0.0 21.3 31.9#

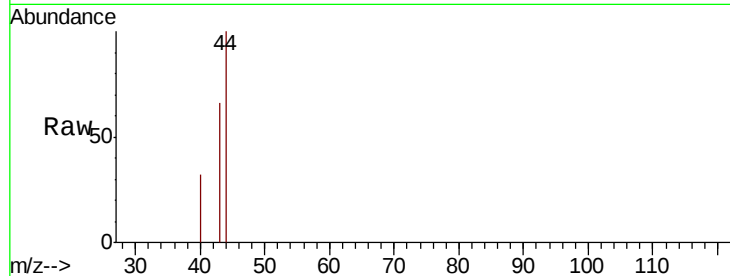


Abundance Ion 43.00 (42.70 to 43.70): VN0



Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

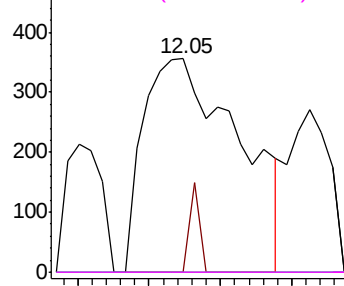

Time-->

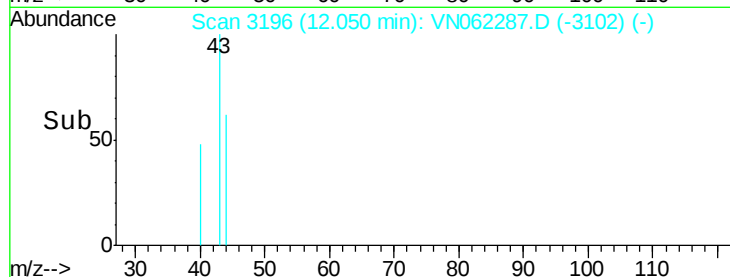

#76

1,2,3-Trichloropropane

Concen: 26.952 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.15 min

Lab File: VN062287.D


Acq: 1 Jul 2020 13:14

Tgt Ion: 75 Resp: 79404

Ion Ratio Lower Upper


75 100

77 1.2 0.0 0.0#





Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

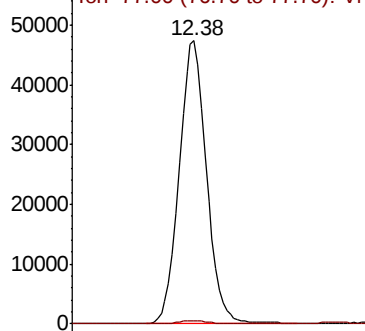

Time-->




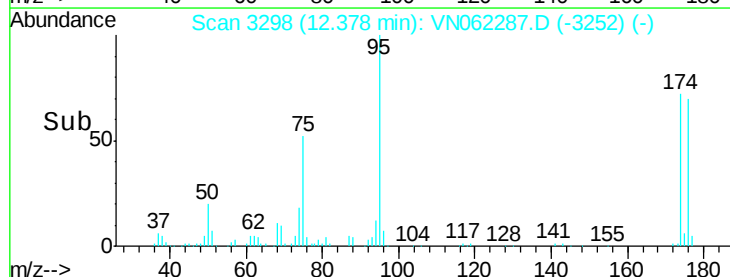


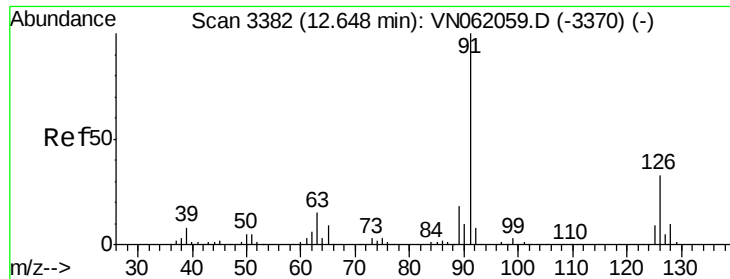

#79
 2-Chlorotoluene
 Concen: 0.220 ug/l
 RT: 12.75 min Scan# 3413
 Delta R.T. 0.10 min
 Lab File: VN062287.D
 Acq: 1 Jul 2020 13:14




Instrument :
 MSVOA_N
 ClientSampled :
 MW-7DL


Tot Ion: 91 Resp: 1476
 Ion Ratio Lower Upper
 91 100
 126 22.6 16.9 50.7

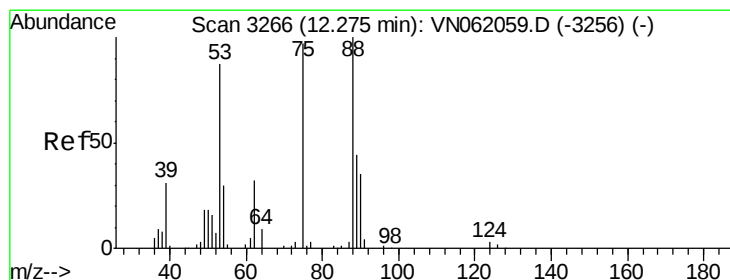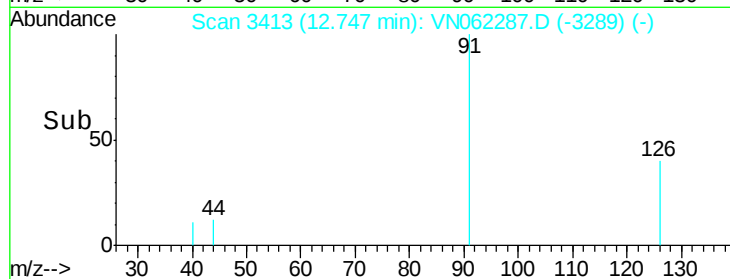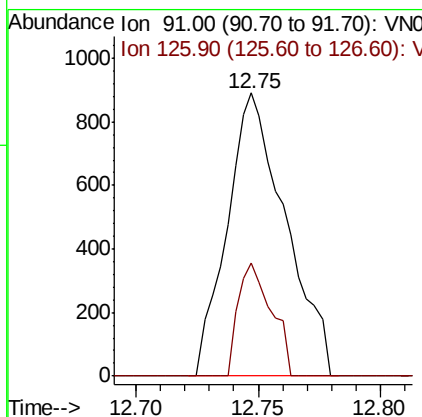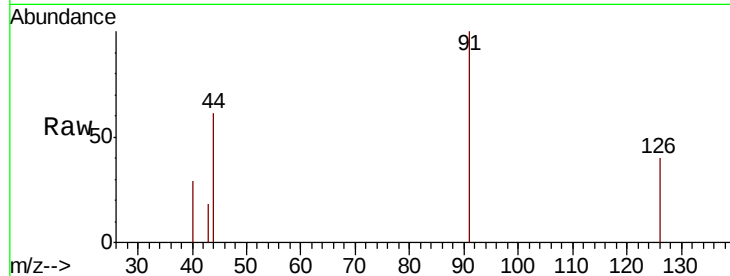

#81
 trans-1,4-Dichloro-2-butene
 Concen: 78.711 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. 0.10 min
 Lab File: VN062287.D
 Acq: 1 Jul 2020 13:14

Tgt Ion: 75 Resp: 79404
 Ion Ratio Lower Upper
 75 100
 53 0.0 72.0 108.0#
 89 0.0 36.9 55.3#

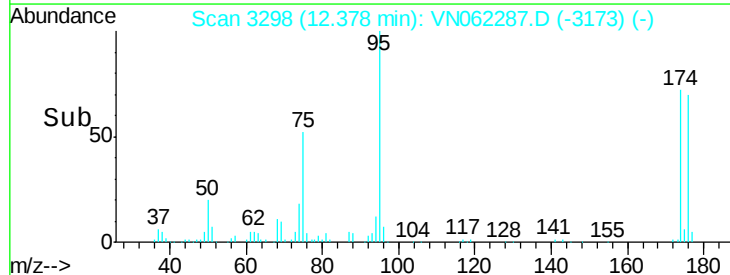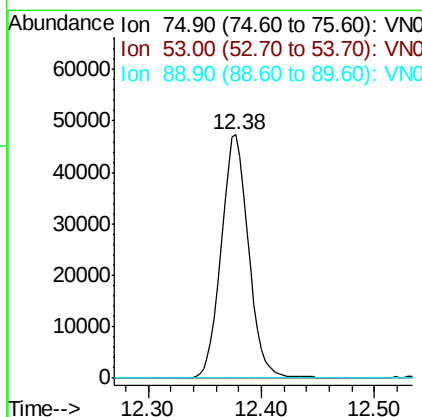

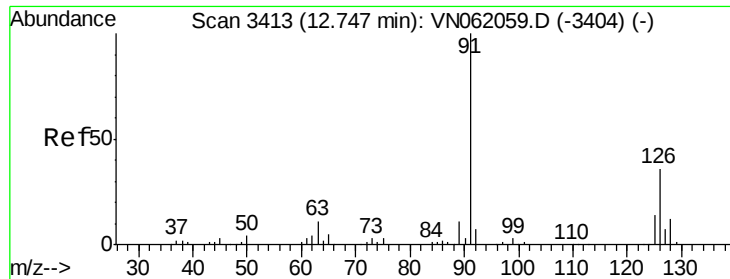

#82

4-Chlorotoluene

Concen: 0.213 ug/l

RT: 12.75 min Scan# 3413

Delta R.T. -0.00 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14

Instrument :

MSVOA_N

ClientSampled :


MW-7DL

Tot Ion: 91 Resp: 1476

Ion Ratio Lower Upper




91 100

126 22.6 16.7 50.1

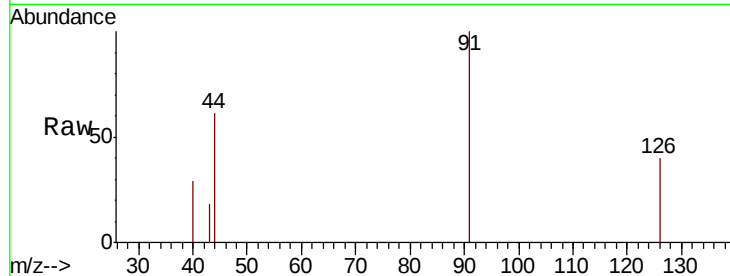

Abundance Ion 91.00 (90.70 to 91.70): VN062059.D (-3404) (-)

Ion 125.90 (125.60 to 126.60): VN062059.D (-3404) (-)

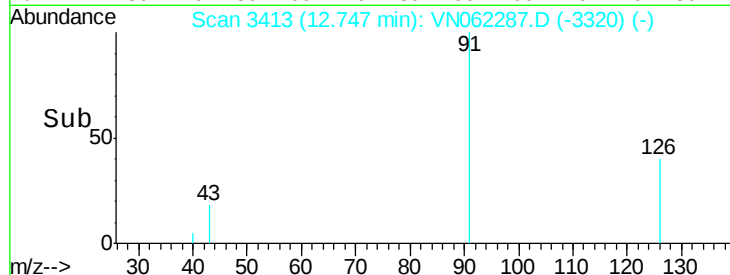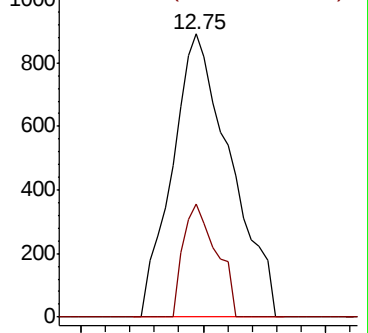

#93

1,2,4-Trichlorobenzene

Concen: 0.432 ug/l

RT: 14.89 min Scan# 4078

Delta R.T. 0.00 min

Lab File: VN062287.D

Acq: 1 Jul 2020 13:14


Tgt Ion: 180 Resp: 772

Ion Ratio Lower Upper

180 100

182 108.5 48.0 144.2



145 0.0 16.0 48.0#




Abundance Ion 179.80 (179.50 to 180.50): VN062059.D (-4064) (-)

Ion 181.80 (181.50 to 182.50): VN062059.D (-4064) (-)

Ion 144.80 (144.50 to 145.50): VN062059.D (-4064) (-)



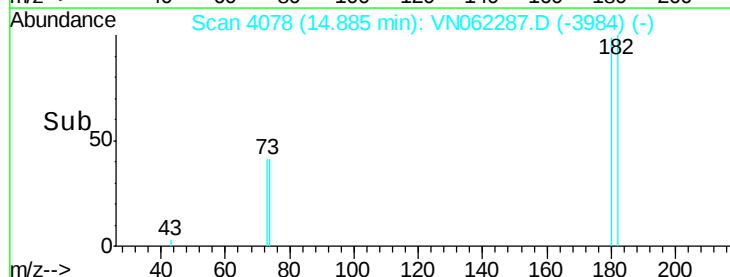
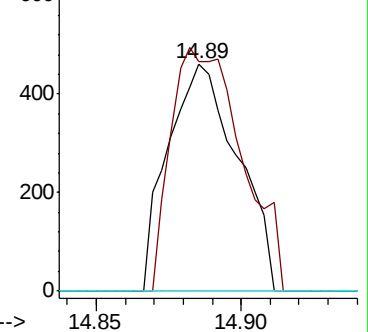




#95
Naphthalene
Concen: 4.462 ug/l
RT: 15.11 min Scan# 4147
Delta R.T. 0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14

Instrument :
MSVOA_N
ClientSampleId :
MW-7DL

Tot Ion:128 Resp: 3027
Ion Ratio Lower Upper
128 100
127 8.2 10.5 15.7#
129 7.9 8.6 13.0#

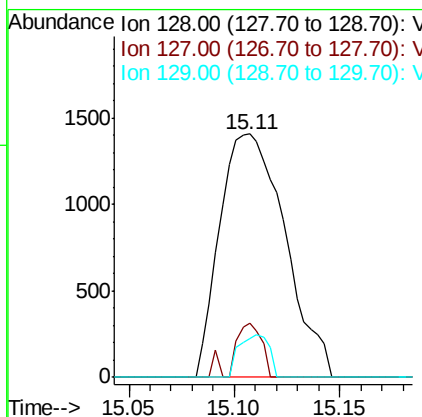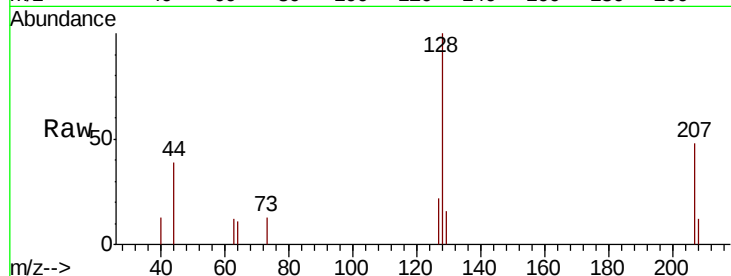

#96
1,2,3-Trichlorobenzene
Concen: 0.516 ug/l
RT: 15.29 min Scan# 4203
Delta R.T. 0.00 min
Lab File: VN062287.D
Acq: 1 Jul 2020 13:14

Tgt Ion:180 Resp: 944
Ion Ratio Lower Upper
180 100
182 103.8 46.8 140.4
145 3.4 16.4 49.2#

