

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070120\
 Data File : VN062318.D
 Acq On : 2 Jul 2020 3:32
 Operator : JC/MD
 Sample : PB129873ZHE#04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB129873ZHE#04

Quant Time: Jul 02 06:59:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	196005	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	420341	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	406137	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	135994	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	7.99	65	163510	59.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	118.90%	
35) Dibromofluoromethane	7.55	113	130981	48.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.14%	
50) Toluene-d8	10.06	98	546497	50.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.40%	
62) 4-Bromofluorobenzene	12.38	95	172487	47.36	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.72%	

Target Compounds


						Qvalue
3) Chloromethane	2.03	50	446	Below Cal	#	76
11) Tert butyl alcohol	4.70	59	891	2.256	ug/l #	72
16) Acetone	3.78	43	12573	10.685	ug/l	96
17) Carbon Disulfide	4.01	76	970	0.201	ug/l #	75
18) Methyl Acetate	4.28	43	5651	2.584	ug/l	92
20) Methylene Chloride	4.50	84	7785	2.879	ug/l	92
25) 2-Butanone	6.79	43	2604	1.937	ug/l #	81
29) Tetrahydrofuran	7.18	42	873	0.991	ug/l #	56
31) Cyclohexane	7.62	56	5036	1.325	ug/l #	13
36) 1,1-Dichloropropene	7.63	75	18595	4.401	ug/l #	48
38) Carbon Tetrachloride	7.62	117	20864	5.238	ug/l #	15
43) Isopropyl Acetate	8.13	43	71248	12.493	ug/l	98
45) 1,2-Dichloropropane	9.23	63	1858	0.585	ug/l #	43
48) Methyl methacrylate	9.15	41	4024	1.574	ug/l #	6
49) 1,4-Dioxane	9.24	88	96	1.693	ug/l #	1
51) 4-Methyl-2-Pentanone	9.95	43	8240	2.473	ug/l	90
54) cis-1,3-Dichloropropene	9.88	75	33663	6.608	ug/l #	69
56) Ethyl methacrylate	10.51	69	1562	0.379	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	6033	1.135	ug/l #	42
59) 2-Hexanone	10.74	43	82081	34.113	ug/l #	50
71) Bromoform	12.37	173	1595	0.727	ug/l #	1
74) N-amyl acetate	12.00	43	2070	3.842	ug/l #	38
76) 1,2,3-Trichloropropane	12.38	75	88705	27.708	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	5595	0.656	ug/l	99
81) trans-1,4-Dichloro-2-buten	12.38	75	88705	80.918	ug/l #	13
95) Naphthalene	15.12	128	172	4.019	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN070120\
Data File : VN062318.D
Acq On : 2 Jul 2020 3:32
Operator : JC/MD
Sample : PB129873ZHE#04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB129873ZHE#04

Quant Time: Jul 02 06:59:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 24 15:33:00 2020
Response via : Initial Calibration

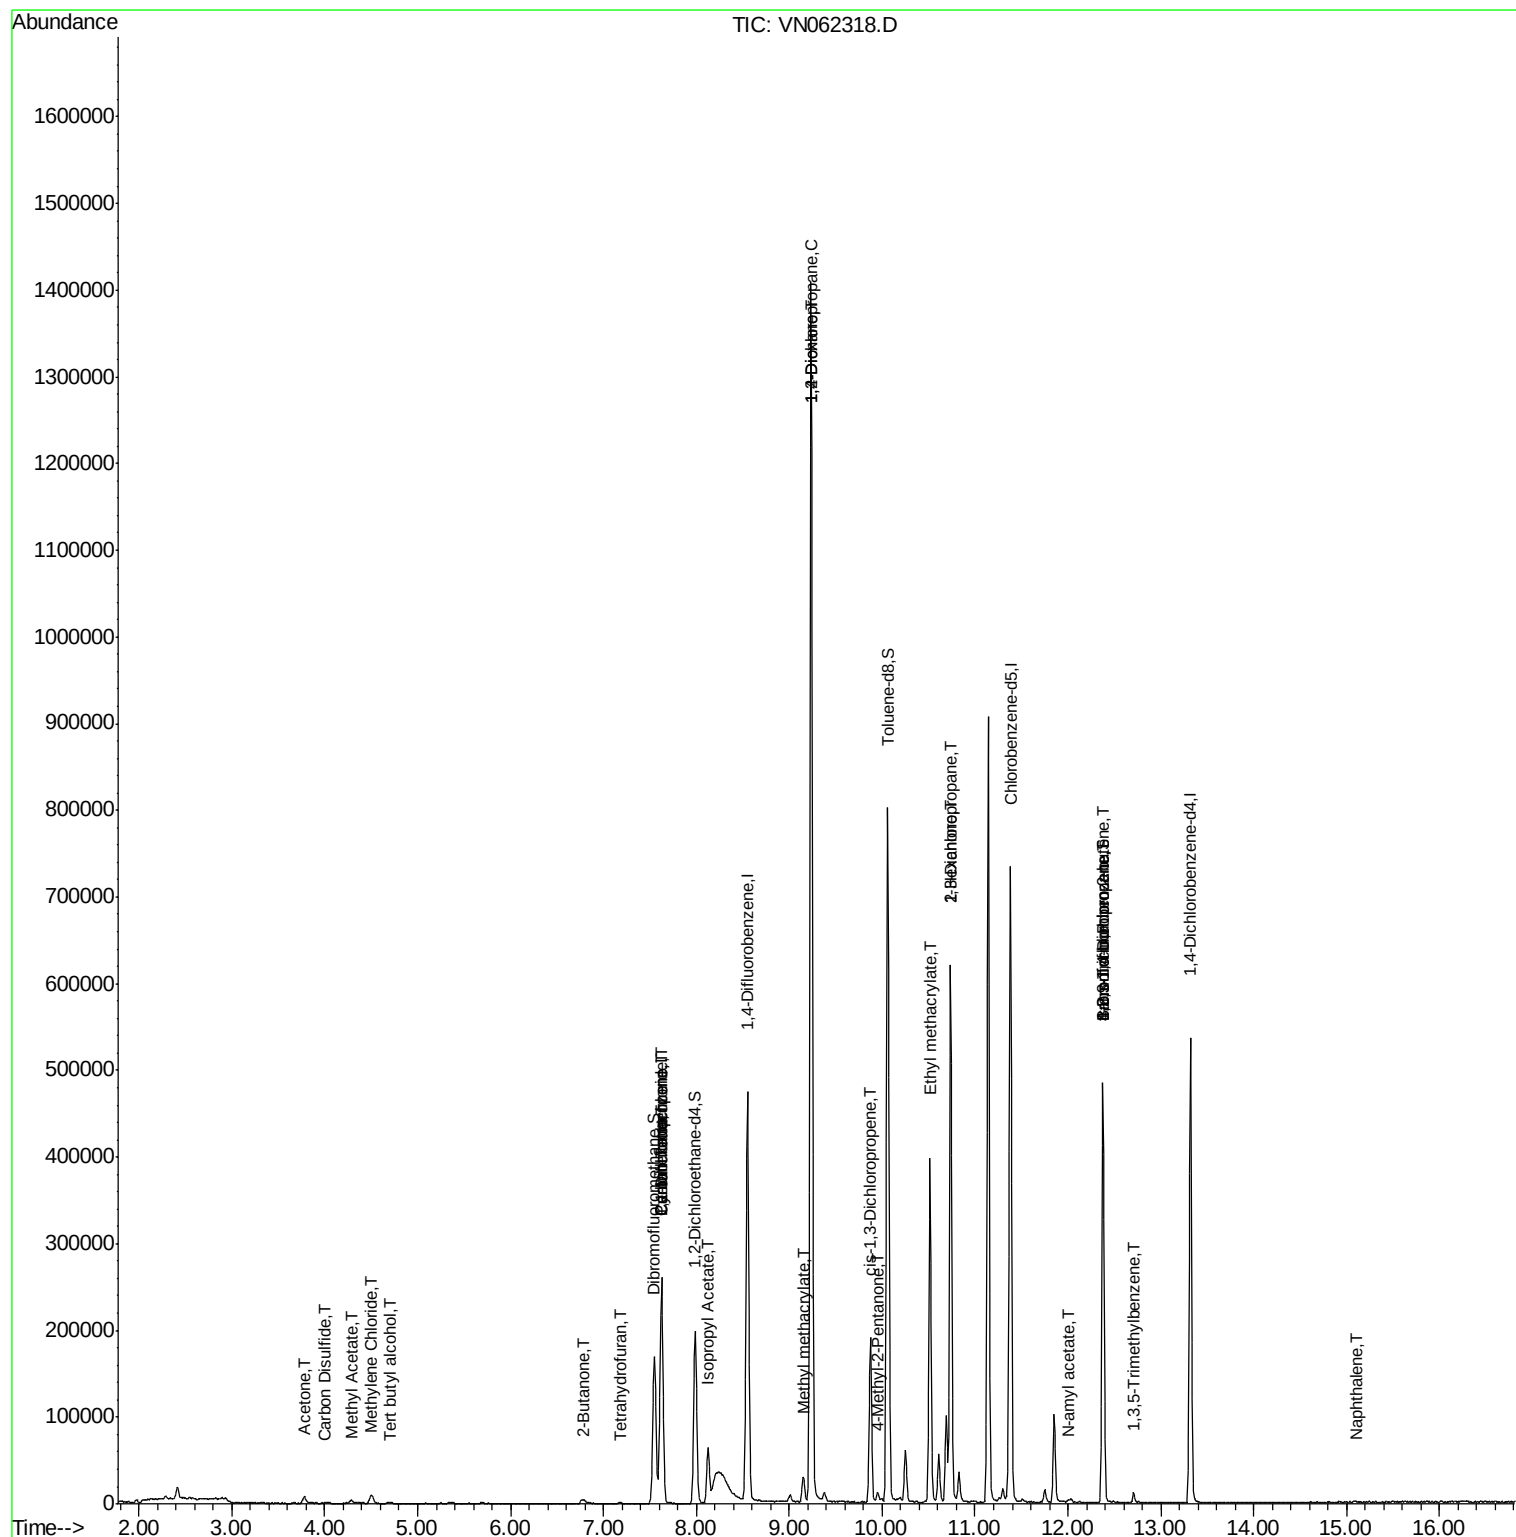

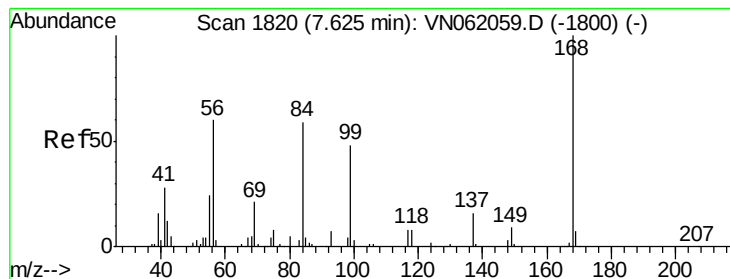

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32

Instrument :

MSVOA_N

ClientSampleId :


PB129873ZHE#04

Tot Ion:168 Resp: 196005

Ion Ratio Lower Upper

168 100

99 63.5 45.8 68.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#3

Chloromethane

Concen: Below Cal

RT: 2.03 min Scan# 81

Delta R.T. 0.00 min

Lab File: VN062318.D


Acq: 2 Jul 2020 3:32

Tgt Ion: 50 Resp: 446

Ion Ratio Lower Upper

50 100

52 47.7 27.0 40.6#



Abundance Ion 49.90 (49.60 to 50.60): VN

Ion 51.90 (51.60 to 52.60): VN

2.03

400


300


200

100

0

Time--> 2.00 2.02 2.04 2.06






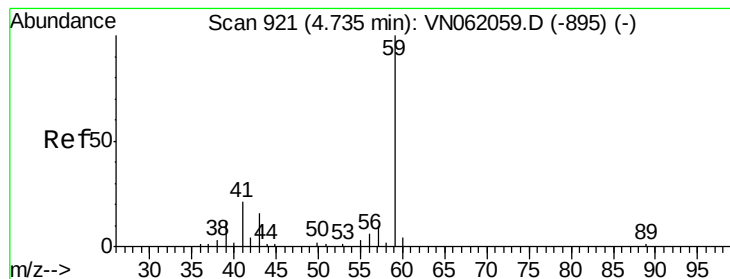


#11

Tert butyl alcohol
 Concen: 2.256 ug/l
 RT: 4.70 min Scan# 909
 Delta R.T. -0.04 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32

Instrument :
 MSVOA_N
 ClientSampleId :
 PB129873ZHE#04




Tot Ion: 59 Resp: 891
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.3 12.5#

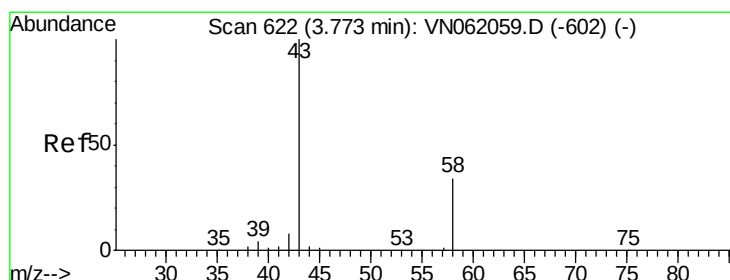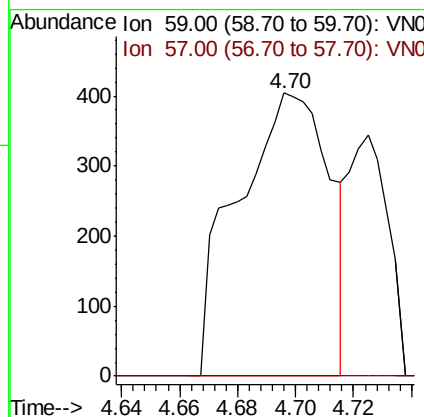


#16

Acetone
 Concen: 10.685 ug/l
 RT: 3.78 min Scan# 624
 Delta R.T. 0.01 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32

Tgt Ion: 43 Resp: 12573
 Ion Ratio Lower Upper
 43 100
 58 37.0 27.5 41.3

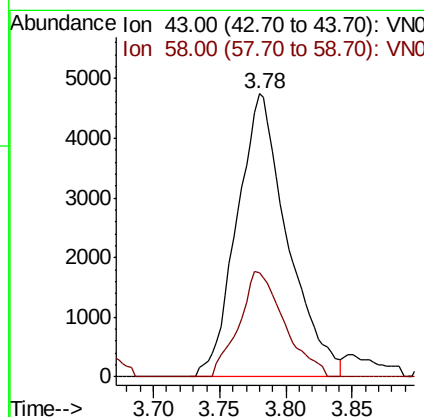



#17

Carbon Disulfide

Concen: 0.201 ug/l

RT: 4.01 min Scan# 695

Delta R.T. 0.00 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32

Instrument :

MSVOA_N

ClientSampleId :


PB129873ZHE#04

Tot Ion: 76 Resp: 970




Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#



Abundance Ion 75.90 (75.60 to 76.60): VN062059.D (-673) (-)

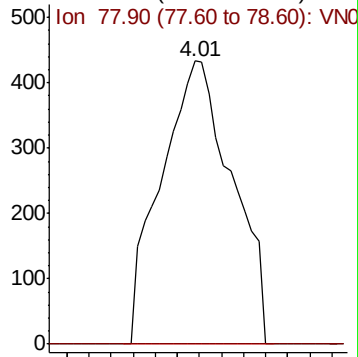

#18

Methyl Acetate

Concen: 2.584 ug/l

RT: 4.28 min Scan# 781

Delta R.T. 0.01 min

Lab File: VN062318.D


Acq: 2 Jul 2020 3:32

Tgt Ion: 43 Resp: 5651



Ion Ratio Lower Upper


43 100

74 24.3 22.9 34.3



Abundance Ion 43.00 (42.70 to 43.70): VN062059.D (-759) (-)

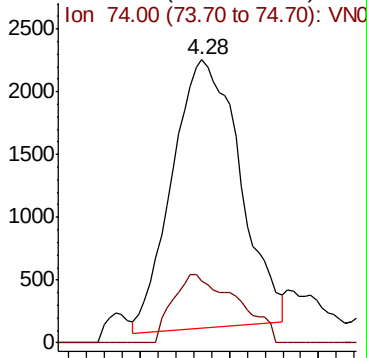







#20
Methvlene Chloride
Concen: 2.879 ug/l
RT: 4.50 min Scan# 849
Delta R.T. 0.00 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32

Instrument :
MSVOA_N
ClientSampleId :
PB129873ZHE#04

Tot Ion:	84	Resp:	7785
Ion	Ratio	Lower	Upper
84	100		
49	104.6	90.6	136.0
51	35.5	27.8	41.8
86	71.9	50.1	75.1

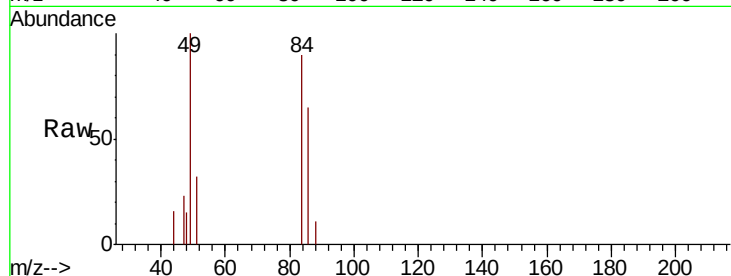


Abundance Ion 83.90 (83.60 to 84.60): VN0
Ion 48.90 (48.60 to 49.60): VN0
Ion 50.90 (50.60 to 51.60): VN0
Ion 85.90 (85.60 to 86.60): VN0


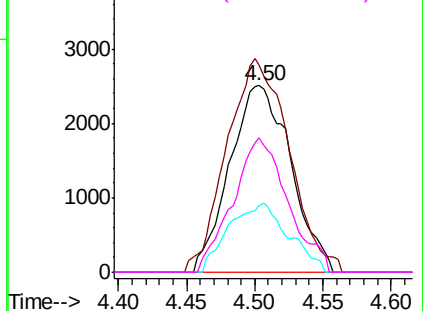



#25
2-Butanone
Concen: 1.937 ug/l
RT: 6.79 min Scan# 1561
Delta R.T. 0.01 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32

Tgt Ion:	43	Resp:	2604
Ion	Ratio	Lower	Upper
43	100		
72	20.4	24.8	37.2#



Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 72.00 (71.70 to 72.70): VN0




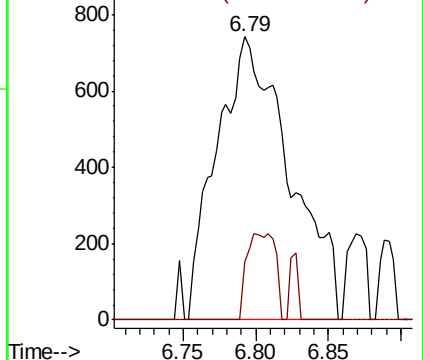


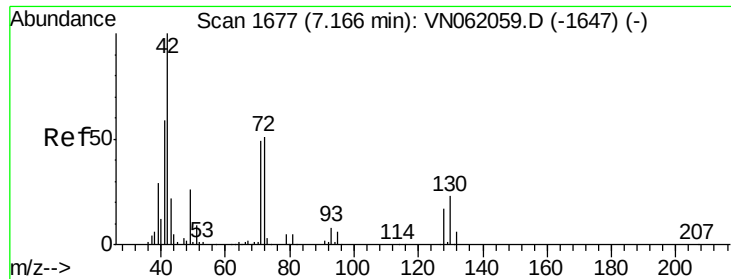

#29
Tetrahydrofuran
Concen: 0.991 ug/l
RT: 7.18 min Scan# 1681
Delta R.T. 0.01 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32




Instrument :
MSVOA_N
ClientSampleId :
PB129873ZHE#04


Tot Ion: 42 Resp: 873
Ion Ratio Lower Upper
42 100
72 20.2 41.1 61.7#
71 18.6 38.2 57.4#

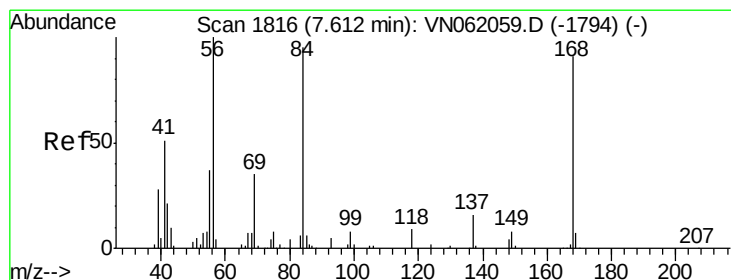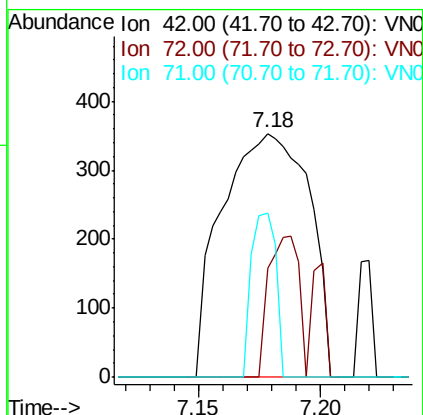

#31
Cyclohexane
Concen: 1.325 ug/l
RT: 7.62 min Scan# 1819
Delta R.T. 0.01 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32

Tgt Ion: 56 Resp: 5036
Ion Ratio Lower Upper
56 100
69 144.2 28.0 42.0#
84 143.9 76.1 114.1#


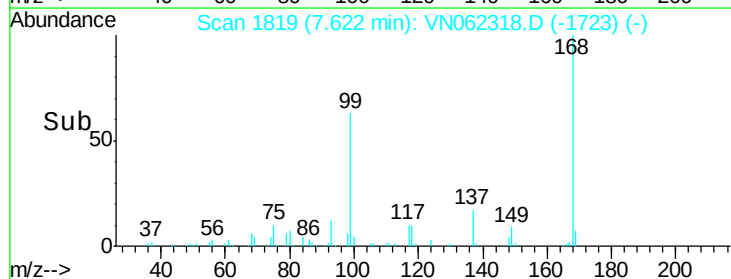
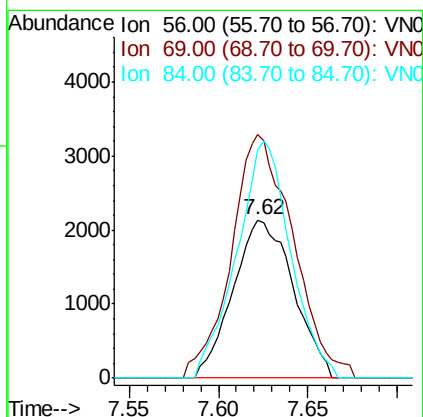
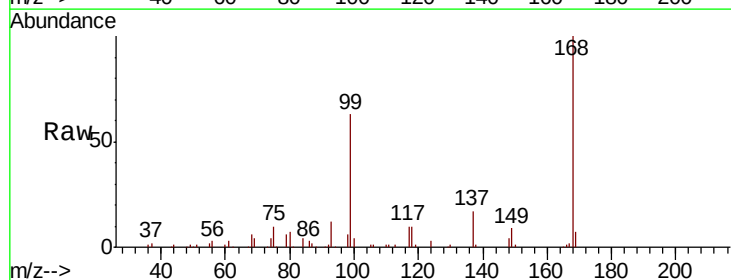


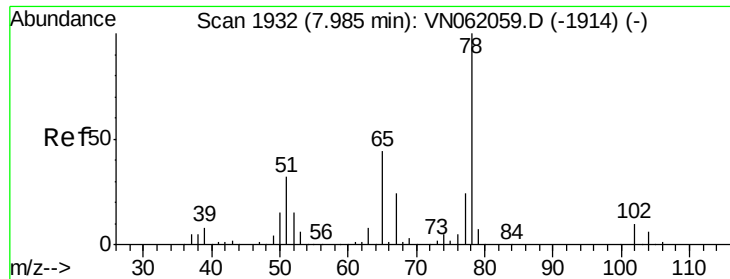

#33
 1,2-Dichloroethane-d4
 Concen: 59.445 ug/l
 RT: 7.99 min Scan# 1933
 Delta R.T. 0.00 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129873ZHE#04


Tot Ion: 65 Resp: 163510
 Ion Ratio Lower Upper
 65 100
 67 52.8 0.0 106.2

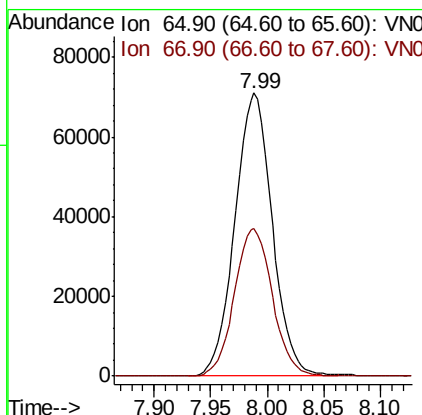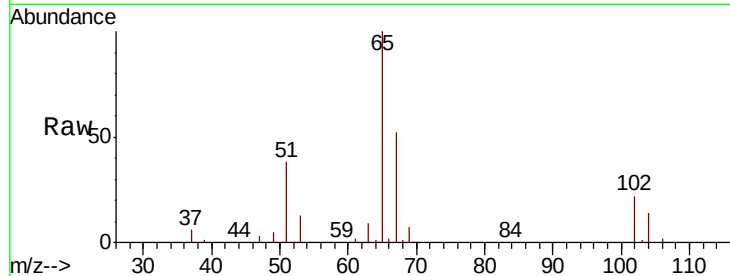

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. -0.00 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32

Tgt Ion: 114 Resp: 420341
 Ion Ratio Lower Upper
 114 100
 63 21.0 0.0 39.2
 88 15.6 0.0 30.8


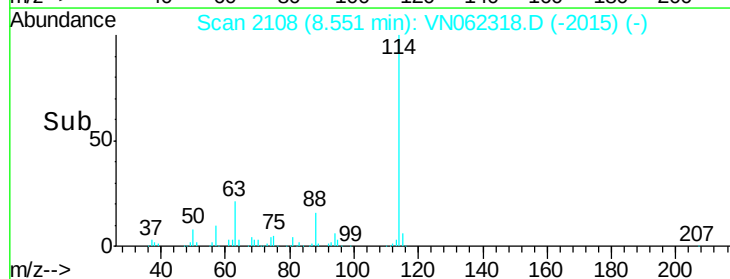
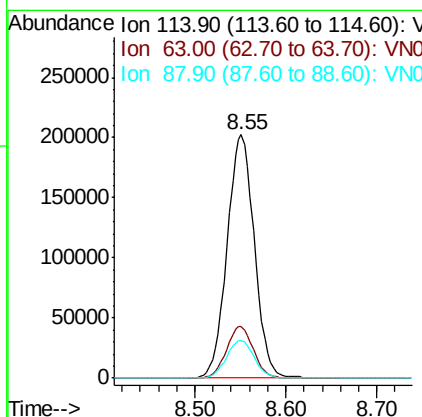





#35
 Dibromofluoromethane
 Concen: 48.571 ug/l
 RT: 7.55 min Scan# 1796
 Delta R.T. -0.00 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129873ZHE#04


Tot Ion:113 Resp: 130981
 Ion Ratio Lower Upper
 113 100
 111 103.9 82.2 123.4
 192 16.2 14.0 21.0

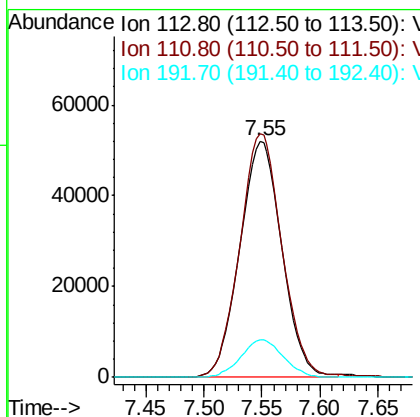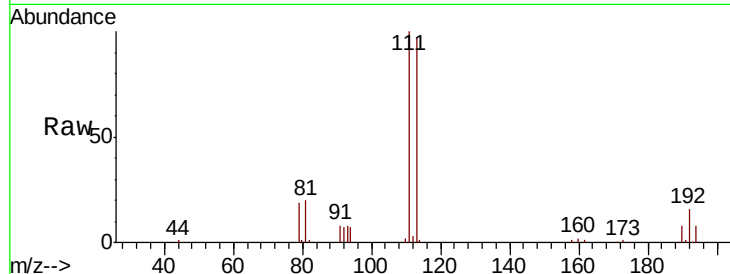

#36
 1,1-Dichloropropene
 Concen: 4.401 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.13 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32

Tgt Ion: 75 Resp: 18595
 Ion Ratio Lower Upper
 75 100
 110 8.1 17.9 53.8#
 77 0.0 24.9 37.3#

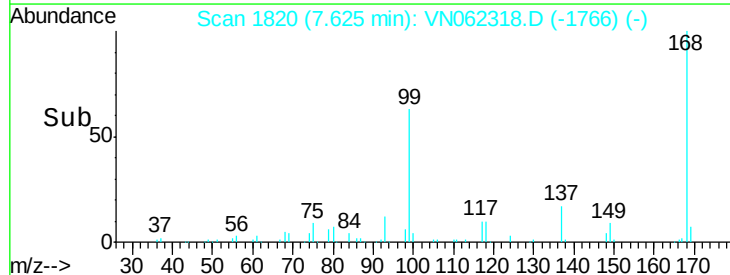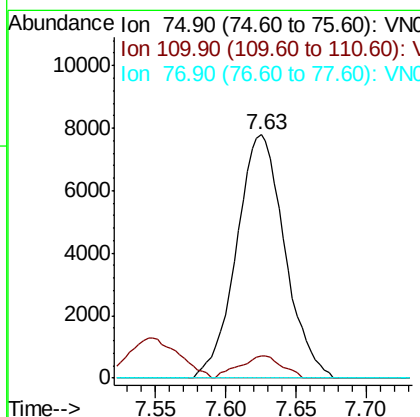

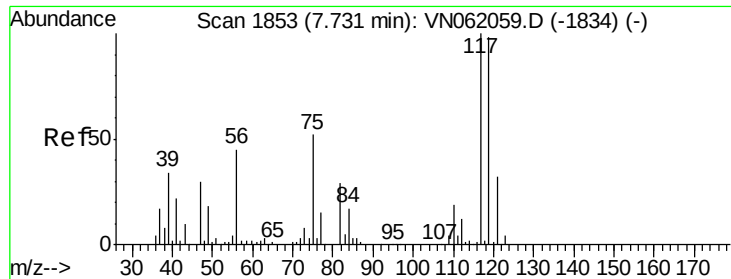

#38

Carbon Tetrachloride

Concen: 5.238 ug/l

RT: 7.62 min Scan# 1819

Delta R.T. -0.11 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32

Instrument :

MSVOA_N

ClientSampleId :

PB129873ZHE#04


Tot Ion:117 Resp: 20864

Ion Ratio Lower Upper

117 100

119 5.0 78.2 117.2#




121 0.0 25.8 38.6#

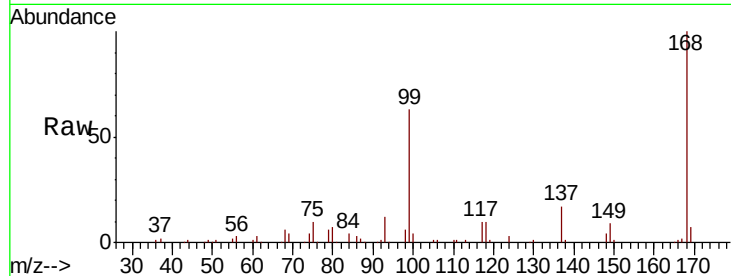

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

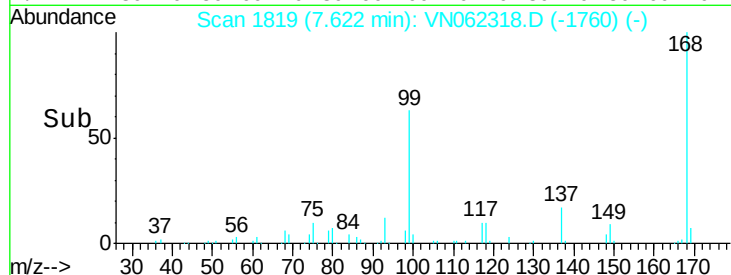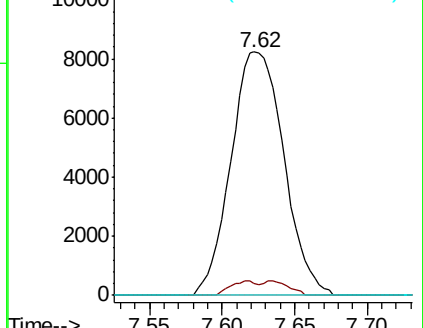

#43

Isopropyl Acetate

Concen: 12.493 ug/l

RT: 8.13 min Scan# 1976

Delta R.T. -0.00 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32


Tgt Ion: 43 Resp: 71248

Ion Ratio Lower Upper

43 100

61 21.2 17.2 25.8



87 13.8 12.1 18.1




Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0




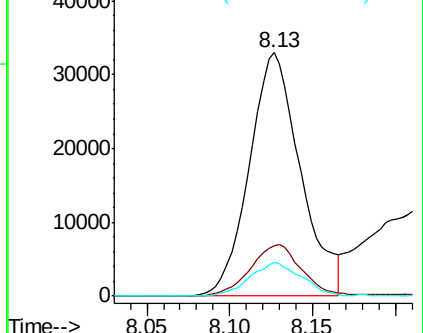


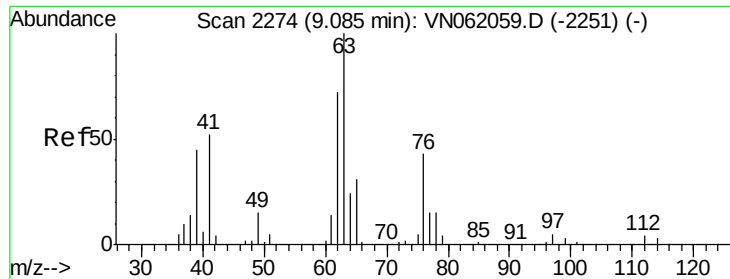

#45
 1,2-Dichloropropane
 Concen: 0.585 ug/l
 RT: 9.23 min Scan# 2320
 Delta R.T. 0.15 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129873ZHE#04


Tot Ion: 63 Resp: 1858
 Ion Ratio Lower Upper
 63 100
 65 0.0 25.0 37.4#

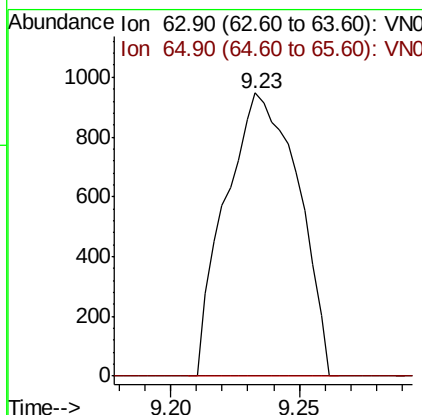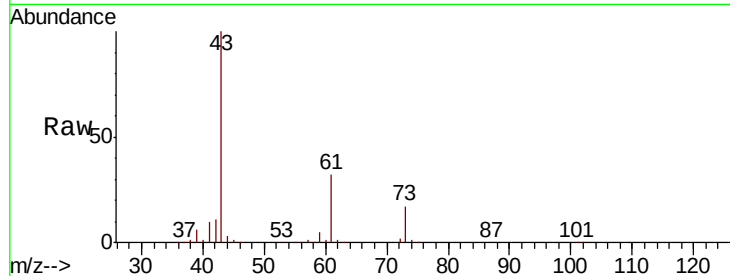

#48
 Methyl methacrylate
 Concen: 1.574 ug/l
 RT: 9.15 min Scan# 2294
 Delta R.T. -0.02 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32

Tgt Ion: 41 Resp: 4024
 Ion Ratio Lower Upper
 41 100
 69 0.0 80.7 121.1#
 39 0.0 54.5 81.7#

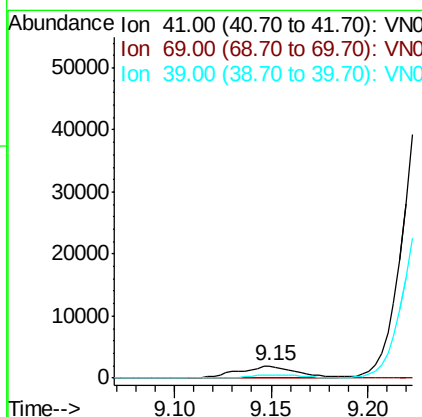



#49

1,4-Dioxane

Concen: 1.693 ug/l

RT: 9.24 min Scan# 2323

Delta R.T. 0.08 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32

Instrument :

MSVOA_N

ClientSampleId :

PB129873ZHE#04


Tot Ion: 88 Resp: 96

Ion Ratio Lower Upper

88 100

43 1362678.1 22.0 33.0#


58 7087.5 49.2 73.8#





Abundance Ion 88.00 (87.70 to 88.70): VN062318.D (-2206) (-)

Ion 43.00 (42.70 to 43.70): VN062318.D (-2206) (-)

Ion 58.00 (57.70 to 58.70): VN062318.D (-2206) (-)

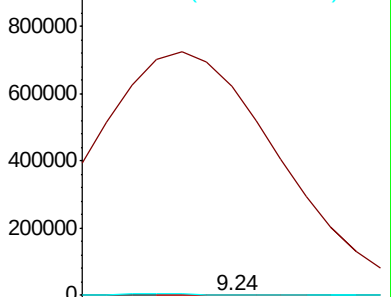

Time-->



#50

Toluene-d8

Concen: 50.697 ug/l

RT: 10.06 min Scan# 2577

Delta R.T. -0.00 min

Lab File: VN062318.D


Acq: 2 Jul 2020 3:32

Tgt Ion: 98 Resp: 546497

Ion Ratio Lower Upper


98 100

100 64.7 51.2 76.8





Abundance Ion 98.00 (97.70 to 98.70): VN062318.D (-2484) (-)

Ion 100.00 (99.70 to 100.70): VN062318.D (-2484) (-)

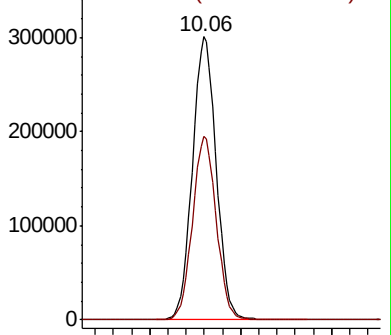

Time-->




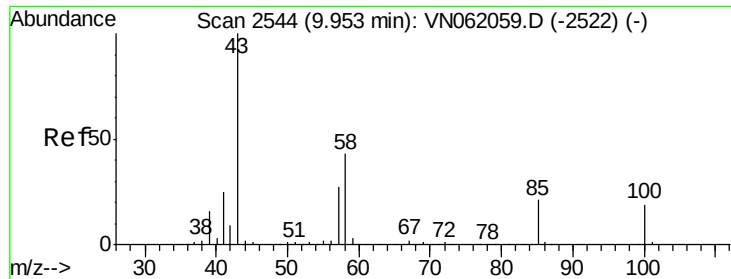




#51
4-Methyl-2-Pentanone
Concen: 2.473 ug/l
RT: 9.95 min Scan# 2544
Delta R.T. -0.00 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32

Instrument :
MSVOA_N
ClientSampleId :
PB129873ZHE#04

Tot Ion: 43 Resp: 8240
Ion Ratio Lower Upper
43 100
58 36.0 34.2 51.2

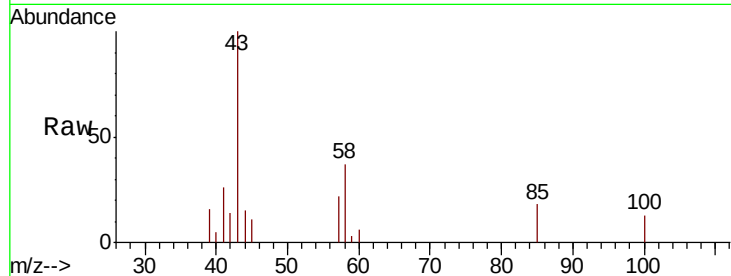


Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 58.00 (57.70 to 58.70): VN0

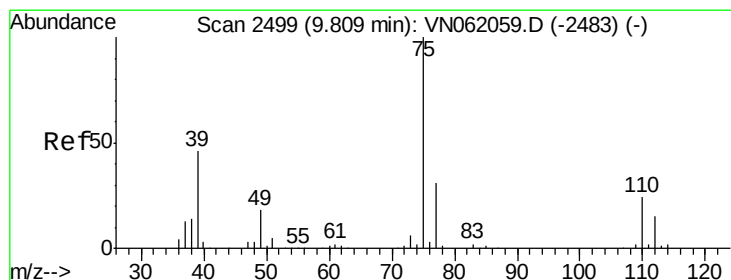
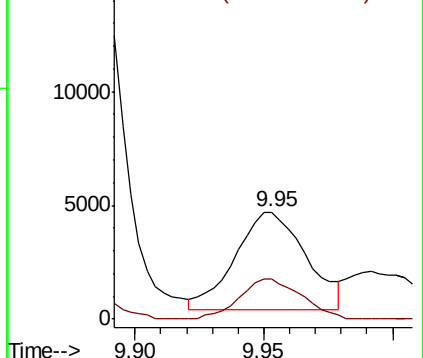



#54
cis-1,3-Dichloropropene
Concen: 6.608 ug/l
RT: 9.88 min Scan# 2520
Delta R.T. 0.07 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32

Tgt Ion: 75 Resp: 33663
Ion Ratio Lower Upper
75 100
77 0.0 25.0 37.6#
39 37.0 36.9 55.3



Abundance Ion 74.90 (74.60 to 75.60): VN0
Ion 76.90 (76.60 to 77.60): VN0
Ion 39.00 (38.70 to 39.70): VN0

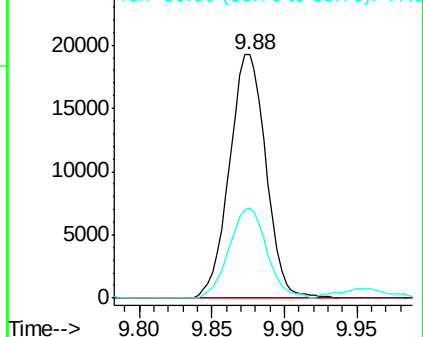

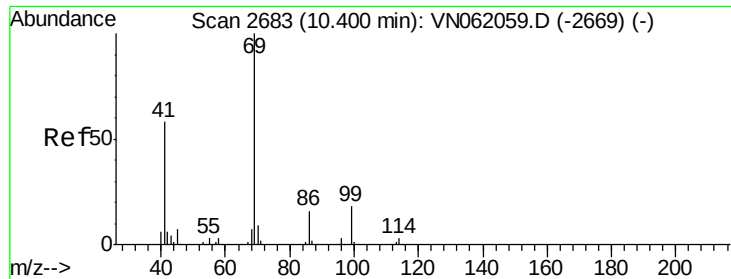

#56

Ethyl methacrylate

Concen: 0.379 ug/l

RT: 10.51 min Scan# 2718

Delta R.T. 0.11 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32

Instrument :

MSVOA_N

ClientSampleId :

PB129873ZHE#04





Tot Ion: 69 Resp: 1562

Ion Ratio Lower Upper

69 100

41 4865.6 46.6 70.0#

39 2283.9 31.0 46.4#

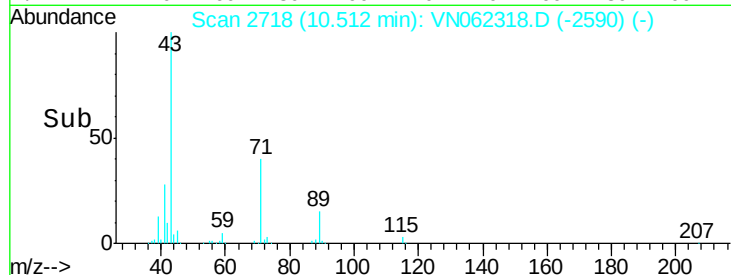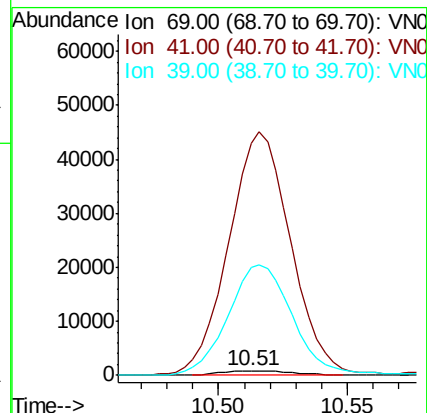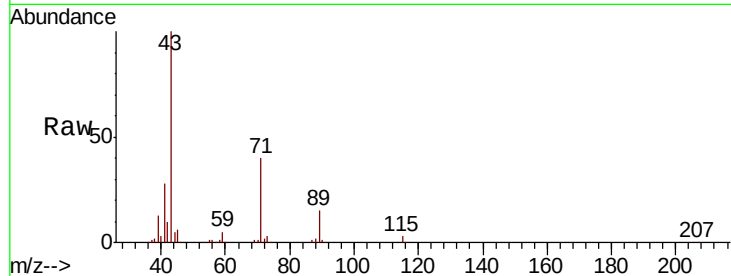

#57

1,3-Dichloropropane

Concen: 1.135 ug/l

RT: 10.74 min Scan# 2789

Delta R.T. 0.06 min

Lab File: VN062318.D




Acq: 2 Jul 2020 3:32


Tgt Ion: 76 Resp: 6033

Ion Ratio Lower Upper

76 100

78 0.0 25.8 38.8#



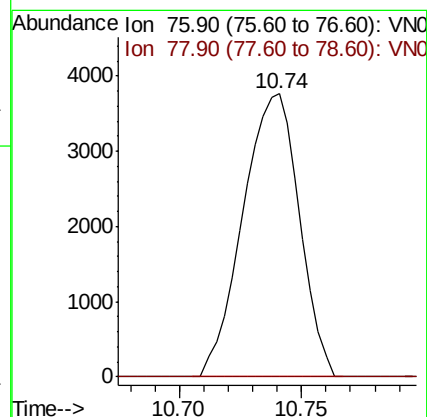



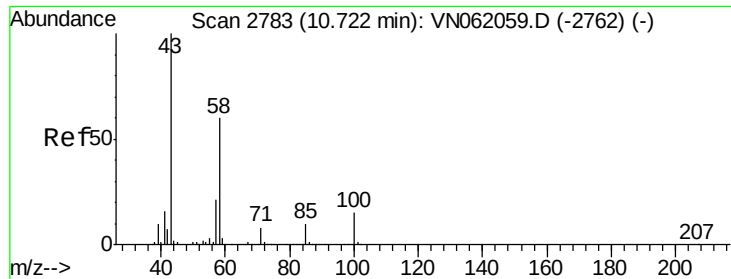

#59
2-Hexanone
Concen: 34.113 ug/l
RT: 10.74 min Scan# 2788
Delta R.T. 0.02 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32




Instrument :
MSVOA_N
ClientSampleId :
PB129873ZHE#04


Tot Ion: 43 Resp: 82081
Ion Ratio Lower Upper
43 100
58 21.6 29.5 88.5#

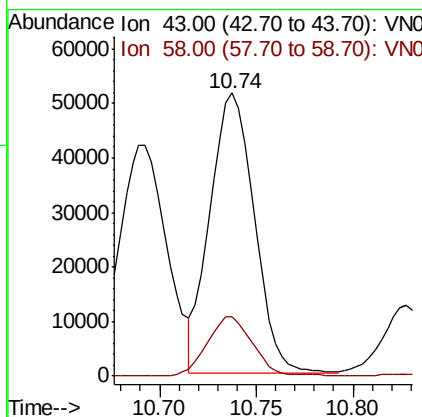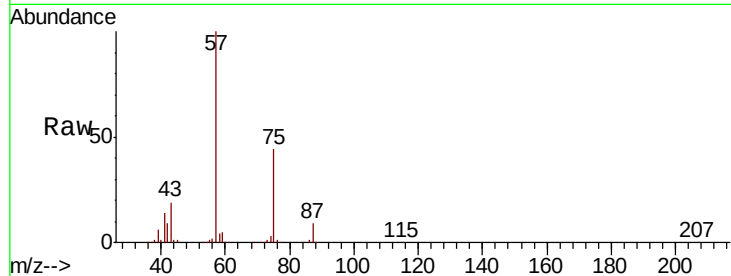

#62
4-Bromofluorobenzene
Concen: 47.361 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.00 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32

Tgt Ion: 95 Resp: 172487
Ion Ratio Lower Upper
95 100
174 71.1 0.0 154.8
176 67.9 0.0 147.4

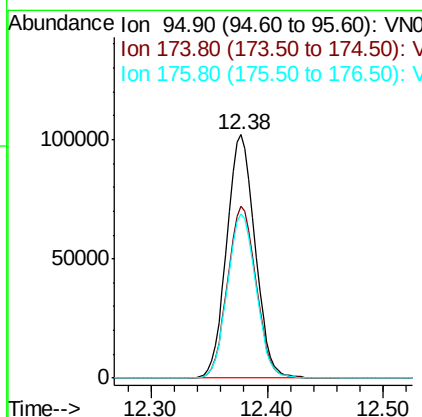


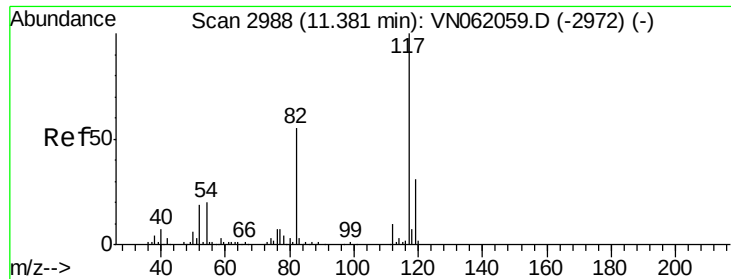




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. -0.00 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32

Instrument :
MSVOA_N
ClientSampleId :
PB129873ZHE#04

Tot Ion:117 Resp: 406137
Ion Ratio Lower Upper
117 100
82 58.4 43.8 65.8
119 32.1 25.2 37.8

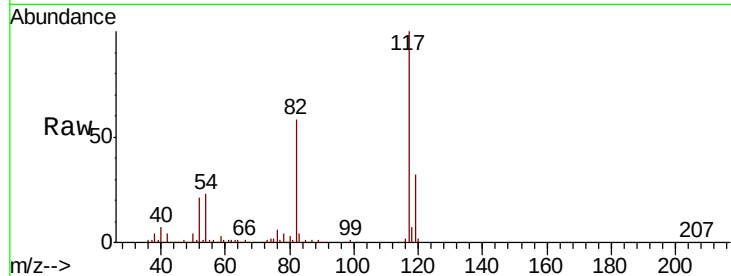


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

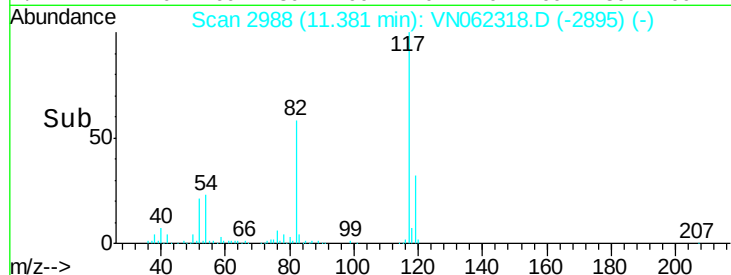
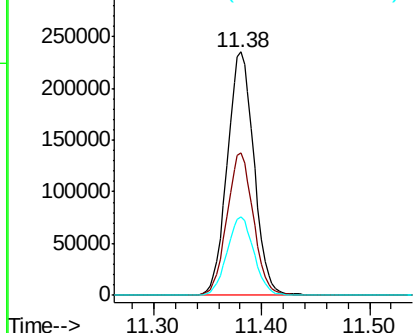



#71
Bromoform
Concen: 0.727 ug/l
RT: 12.37 min Scan# 3297
Delta R.T. 0.27 min
Lab File: VN062318.D
Acq: 2 Jul 2020 3:32

Tgt Ion:173 Resp: 1595
Ion Ratio Lower Upper
173 100
175 479.7 24.7 74.1#
254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

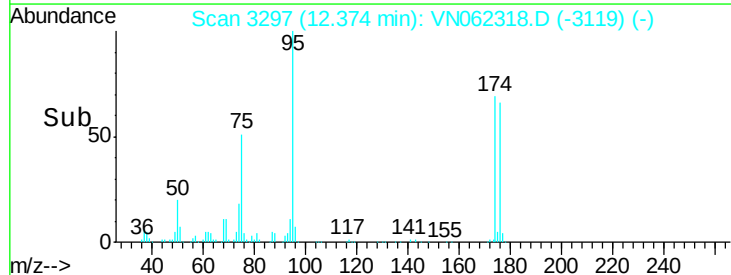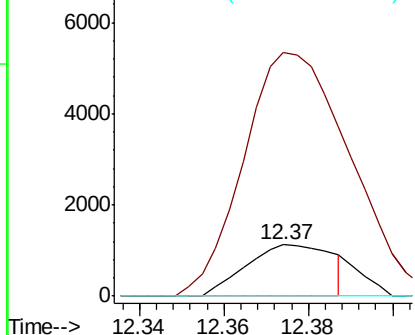

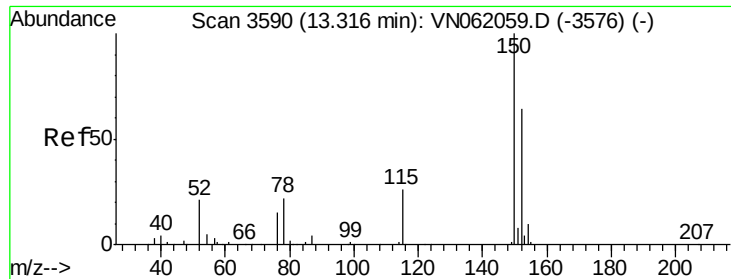

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32

Instrument :

MSVOA_N

ClientSampleId :

PB129873ZHE#04


Tot Ion:152 Resp: 135994

Ion Ratio Lower Upper

152 100

115 63.2 29.5 88.5




150 161.5 0.0 351.4

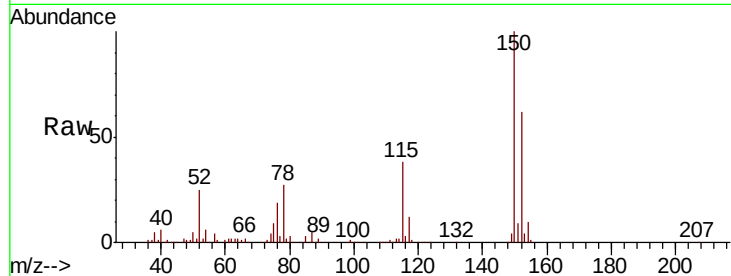

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

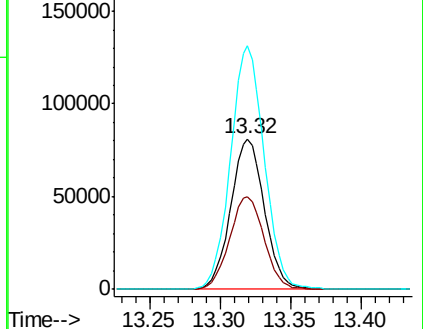

#74

N-ethyl acetate

Concen: 3.842 ug/l

RT: 12.00 min Scan# 3182

Delta R.T. -0.04 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32

Tgt Ion: 43 Resp: 2070


Ion Ratio Lower Upper

43 100

70 0.0 39.4 59.2#

55 0.0 21.7 32.5#

61 0.0 21.3 31.9#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V




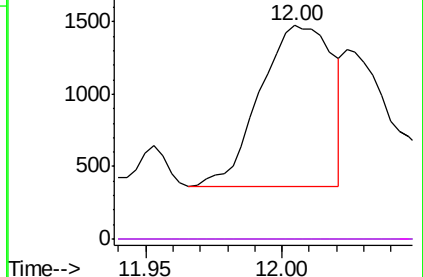


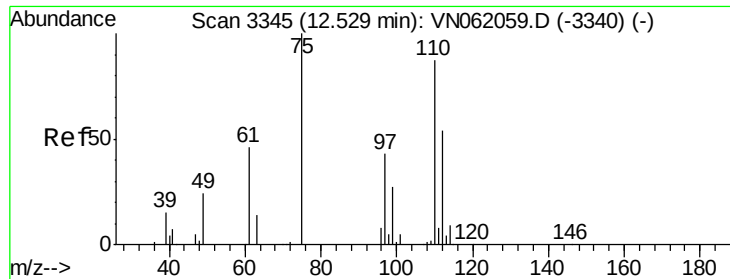

#76
 1,2,3-Trichloropropane
 Concen: 27.708 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. -0.15 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129873ZHE#04


Tot Ion: 75 Resp: 88705
 Ion Ratio Lower Upper
 75 100
 77 1.2 0.0 0.0#

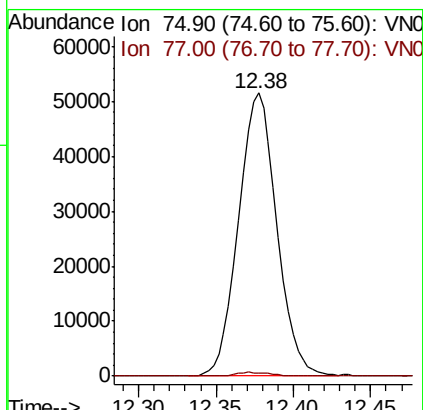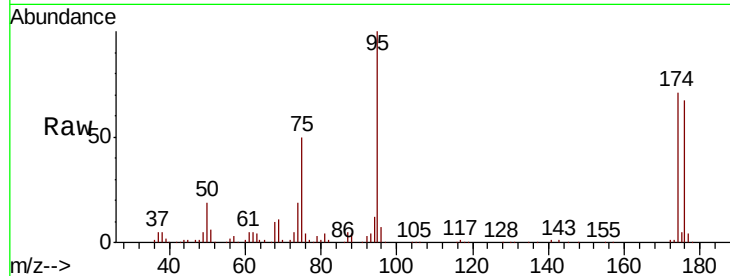

#80
 1,3,5-Trimethylbenzene
 Concen: 0.656 ug/l
 RT: 12.71 min Scan# 3401
 Delta R.T. -0.00 min
 Lab File: VN062318.D
 Acq: 2 Jul 2020 3:32

Tgt Ion: 105 Resp: 5595
 Ion Ratio Lower Upper
 105 100
 120 49.7 24.6 74.0

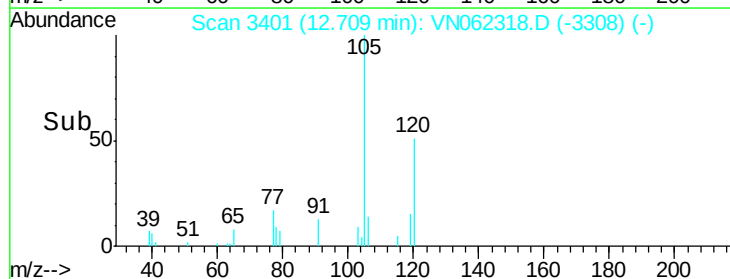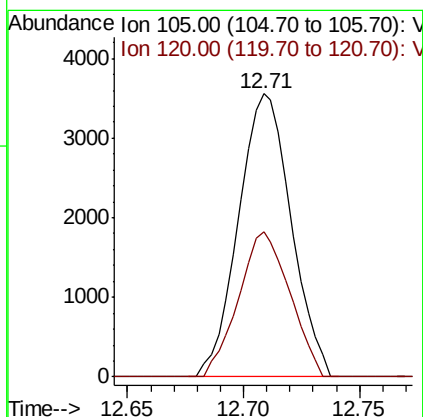

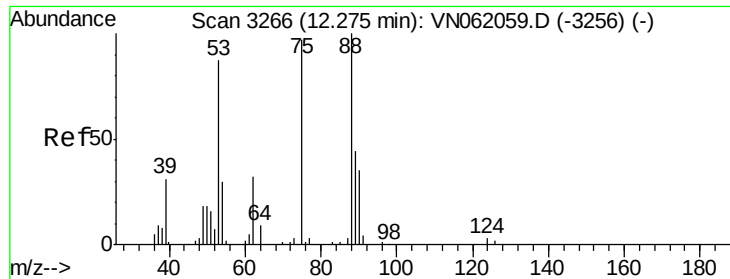

#81

trans-1,4-Dichloro-2-butene

Concen: 80.918 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.10 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32

Instrument :

MSVOA_N

ClientSampleId :

PB129873ZHE#04


Tot Ion: 75 Resp: 88705

Ion Ratio Lower Upper

75 100

53 0.0 72.0 108.0#




89 0.0 36.9 55.3#

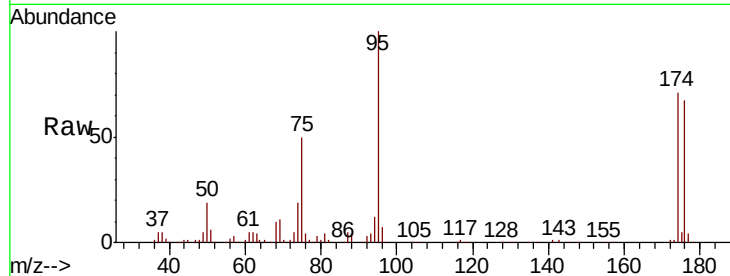

Abundance Ion 74.90 (74.60 to 75.60): VN062318.D (-3173) (-)

Ion 53.00 (52.70 to 53.70): VN062318.D (-3173) (-)

Ion 88.90 (88.60 to 89.60): VN062318.D (-3173) (-)

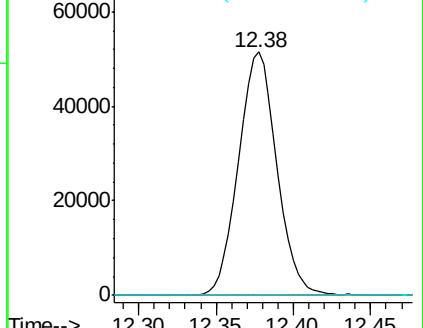

#95

Naphthalene

Concen: 4.019 ug/l

RT: 15.12 min Scan# 4150

Delta R.T. 0.01 min

Lab File: VN062318.D

Acq: 2 Jul 2020 3:32


Tgt Ion: 128 Resp: 172

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.6 13.0#



Abundance Ion 128.00 (127.70 to 128.70): VN062318.D (-4053) (-)

Ion 127.00 (126.70 to 127.70): VN062318.D (-4053) (-)

Ion 129.00 (128.70 to 129.70): VN062318.D (-4053) (-)

