

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN070120\
 Data File : VN062331.D
 Acq On : 2 Jul 2020 8:46
 Operator : JC/MD
 Sample : L3171-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CHASSIS-WASH

Quant Time: Jul 02 11:08:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	192176	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	403030	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	397395	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	159150	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	160950	59.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	119.36%	
35) Dibromofluoromethane	7.55	113	127626	49.36	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.72%	
50) Toluene-d8	10.06	98	537122	51.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.94%	
62) 4-Bromofluorobenzene	12.38	95	181063	51.85	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.70%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.03	50	432	Below Cal	#	86
11) Tert butyl alcohol	4.71	59	789	2.038	ug/l #	72
16) Acetone	3.78	43	84279	97.083	ug/l	99
18) Methyl Acetate	4.28	43	5845	2.726	ug/l	97
20) Methylene Chloride	4.51	84	62012	24.939	ug/l	94
25) 2-Butanone	6.79	43	32367	24.554	ug/l	99
29) Tetrahydrofuran	7.15	42	286	0.331	ug/l #	28
31) Cyclohexane	7.63	56	5039	1.352	ug/l #	4
36) 1,1-Dichloropropene	7.63	75	18559	4.581	ug/l #	48
37) Ethyl Acetate	6.79	43	32367	9.649	ug/l #	67
38) Carbon Tetrachloride	7.63	117	20740	5.430	ug/l #	16
41) Methacrylonitrile	7.16	41	746	0.480	ug/l #	14
43) Isopropyl Acetate	8.13	43	11545	2.111	ug/l	98
48) Methyl methacrylate	9.14	41	4016	1.638	ug/l #	20
51) 4-Methyl-2-Pentanone	9.95	43	141399	44.257	ug/l	97
54) cis-1,3-Dichloropropene	9.87	75	15110	3.093	ug/l #	76
56) Ethyl methacrylate	10.33	69	6345	1.605	ug/l #	44
59) 2-Hexanone	10.73	43	11927	5.170	ug/l	69
71) Bromoform	12.37	173	1478	0.689	ug/l #	1
74) N-amyl acetate	12.00	43	4595	4.289	ug/l #	43
75) 1,1,2,2-Tetrachloroethane	12.54	83	2782	0.679	ug/l #	25
76) 1,2,3-Trichloropropane	12.37	75	93362	24.920	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.37	75	93362	72.775	ug/l #	14
95) Naphthalene	15.11	128	187	4.018	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN070120\
Data File : VN062331.D
Acq On : 2 Jul 2020 8:46
Operator : JC/MD
Sample : L3171-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHASSIS-WASH

Quant Time: Jul 02 11:08:41 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 24 15:33:00 2020
Response via : Initial Calibration

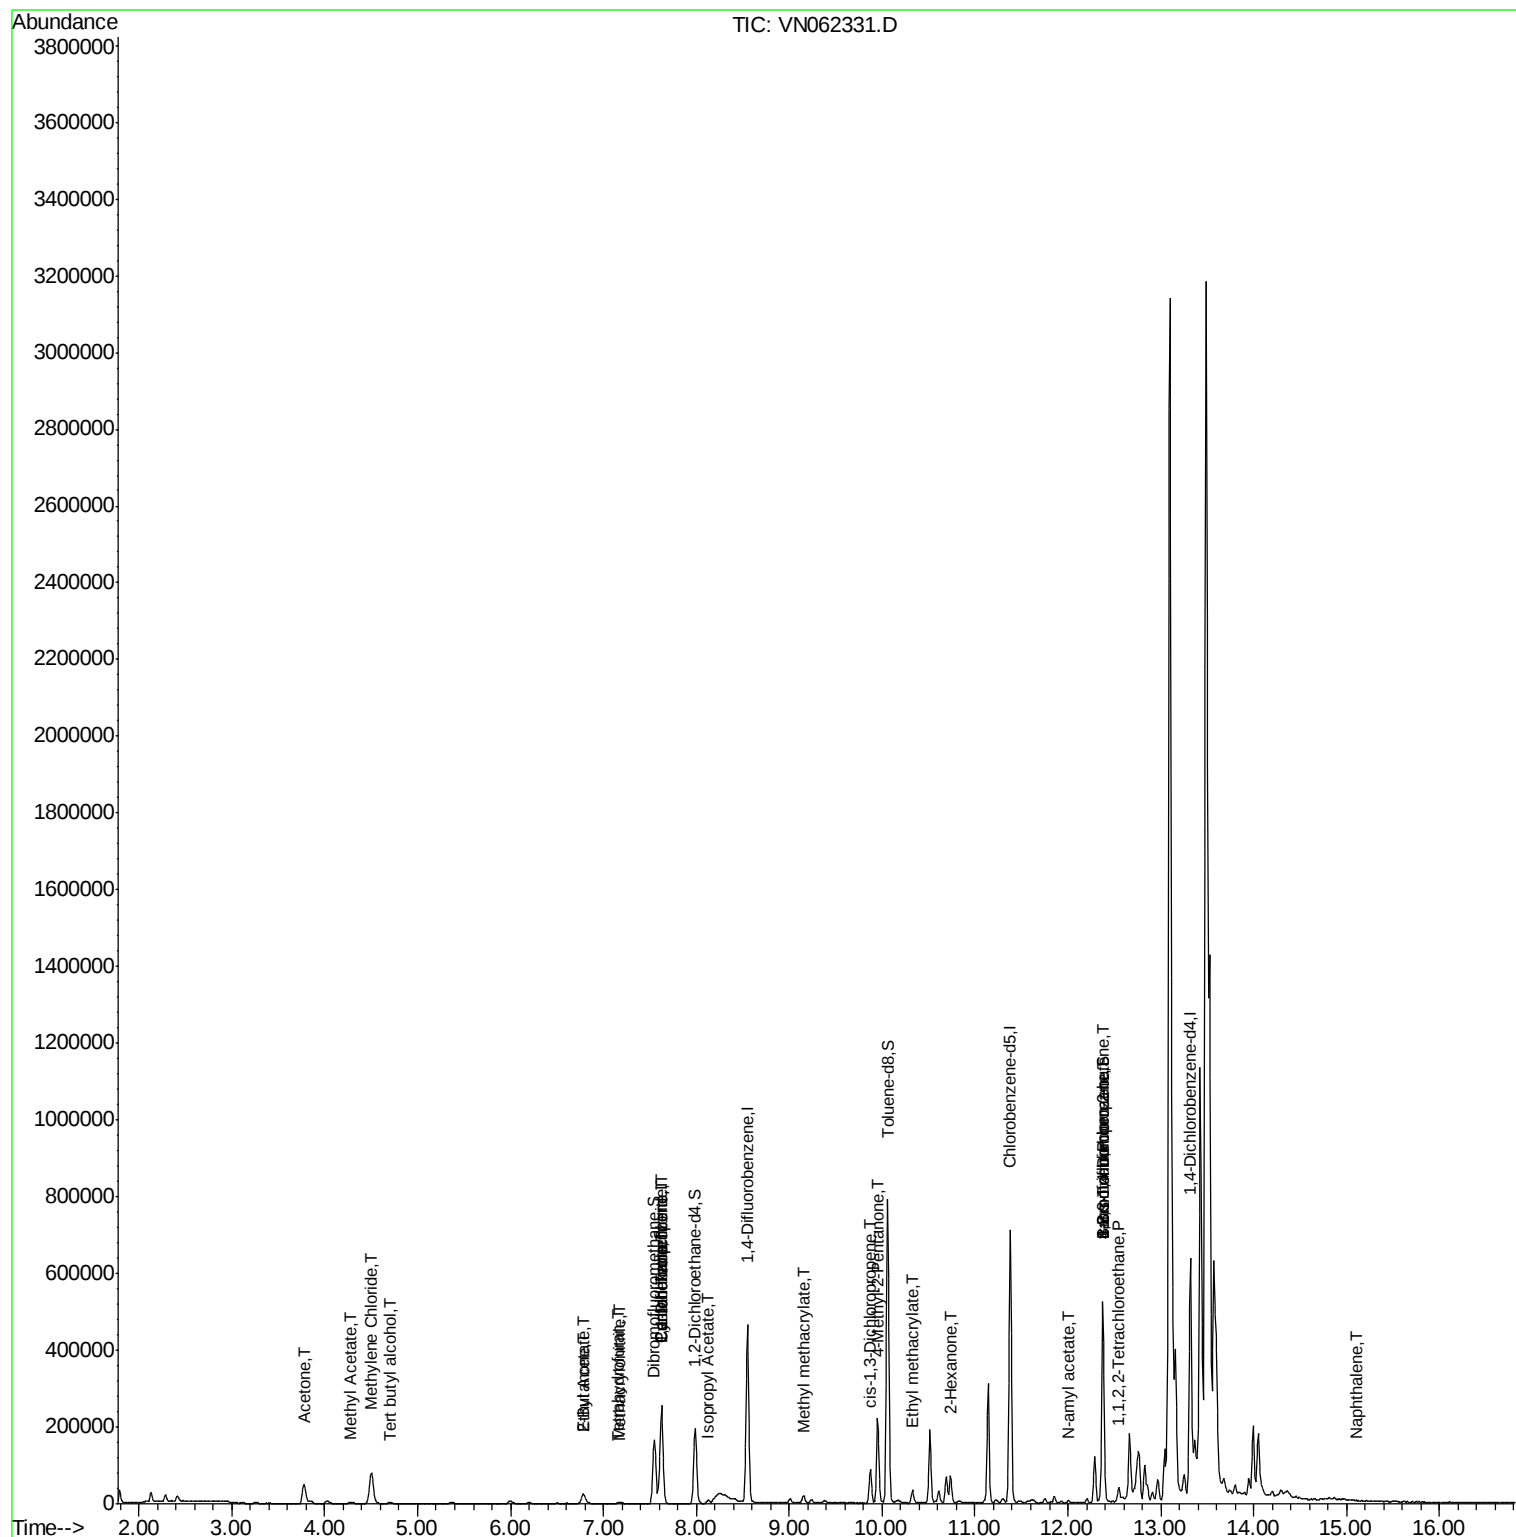



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Instrument :

MSVOA_N

ClientSampleId :


CHASSIS-WASH

Tgt Ion:168 Resp: 192176

Ion Ratio Lower Upper




168 100

99 62.6 45.8 68.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

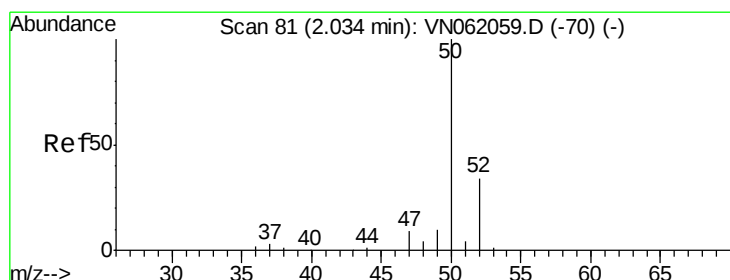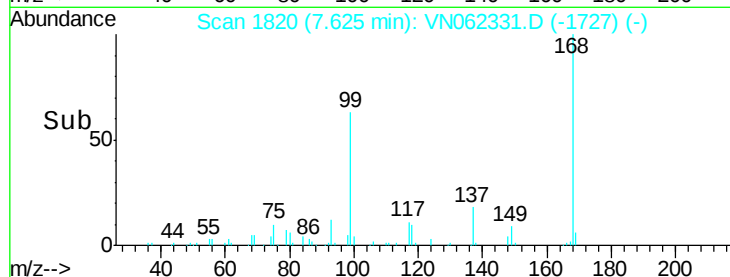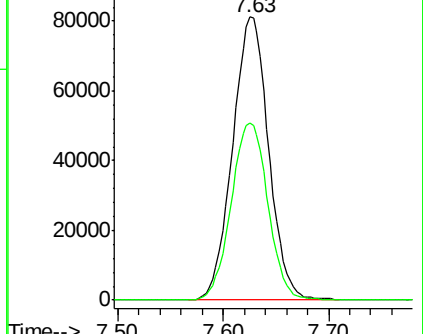

#3

Chloromethane

Concen: Below Cal

RT: 2.03 min Scan# 81

Delta R.T. 0.00 min

Lab File: VN062331.D


Acq: 2 Jul 2020 8:46

Tgt Ion: 50 Resp: 432

Ion Ratio Lower Upper



50 100


52 41.5 27.0 40.6#

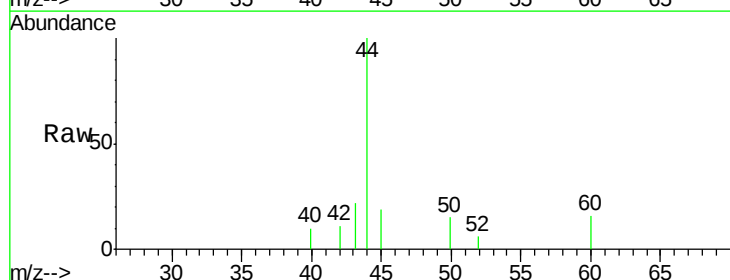

Abundance Ion 49.90 (49.60 to 50.60): VNO

Ion 51.90 (51.60 to 52.60): VNO

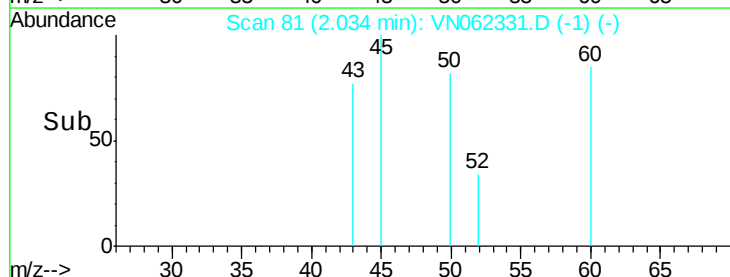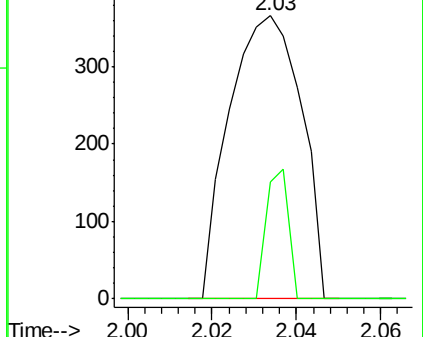




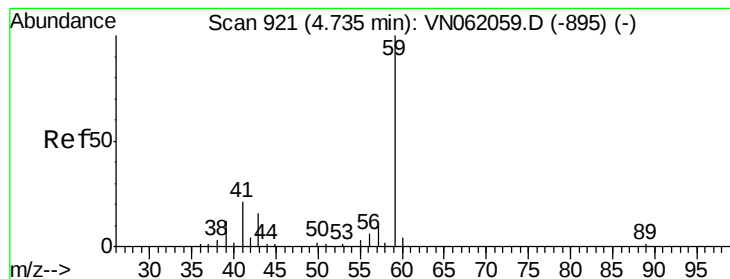


#11

Tert butyl alcohol
 Concen: 2.038 ug/l
 RT: 4.71 min Scan# 912
 Delta R.T. -0.03 min
 Lab File: VN062331.D
 Acq: 2 Jul 2020 8:46

Instrument :
 MSVOA_N
 ClientSampleId :
 CHASSIS-WASH




Tgt Ion: 59 Resp: 789
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.3 12.5#

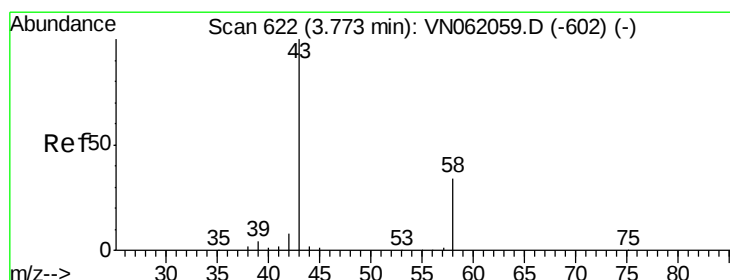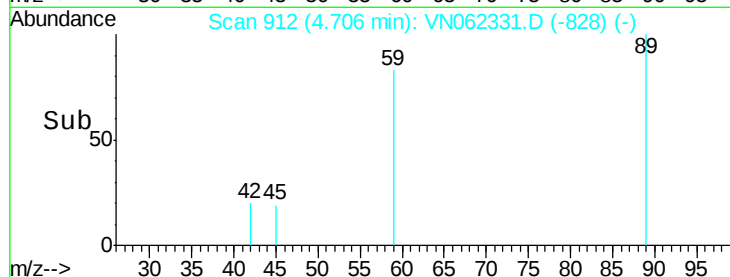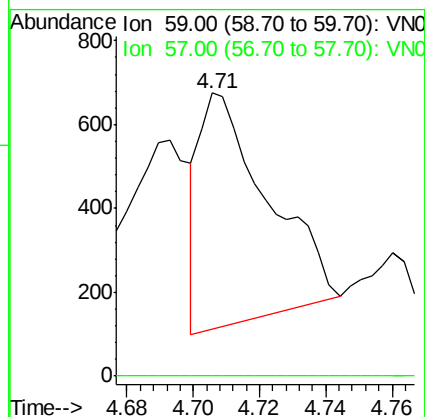


#16

Acetone
 Concen: 97.083 ug/l
 RT: 3.78 min Scan# 623
 Delta R.T. 0.00 min
 Lab File: VN062331.D
 Acq: 2 Jul 2020 8:46

Tgt Ion: 43 Resp: 84279
 Ion Ratio Lower Upper
 43 100
 58 33.6 27.5 41.3

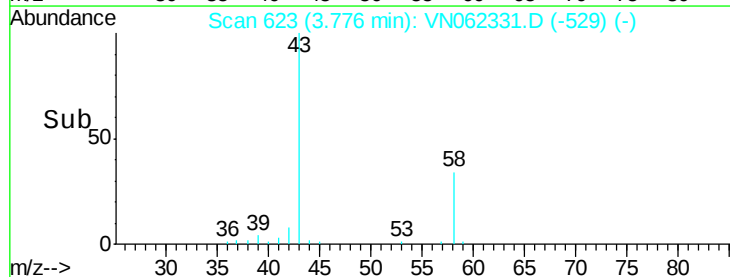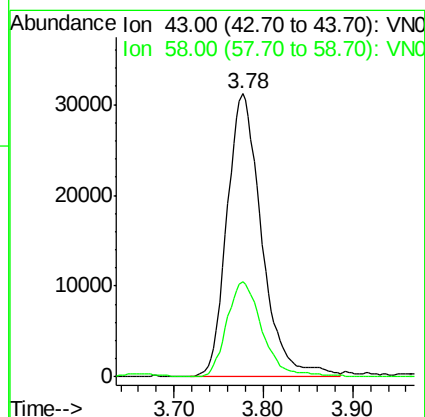

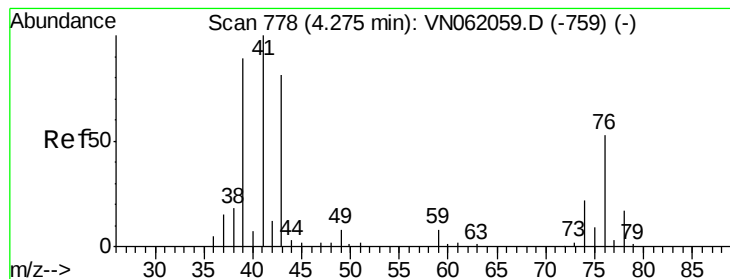

#18

Methyl Acetate

Concen: 2.726 ug/l

RT: 4.28 min Scan# 781

Delta R.T. 0.01 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Instrument :

MSVOA_N

ClientSampleId :


CHASSIS-WASH

Tgt Ion: 43 Resp: 5845

Ion Ratio Lower Upper




43 100

74 26.9 22.9 34.3



Abundance Ion 43.00 (42.70 to 43.70): VN062059.D (-759) (-)

Ion 74.00 (73.70 to 74.70): VN062059.D (-759) (-)

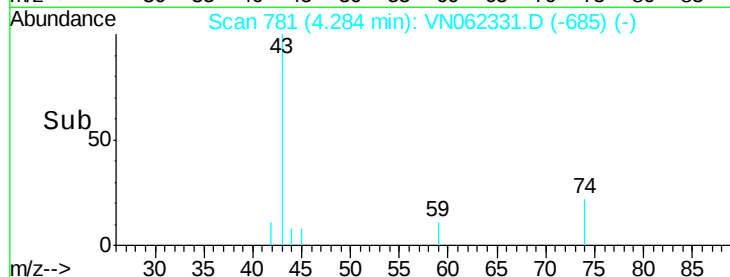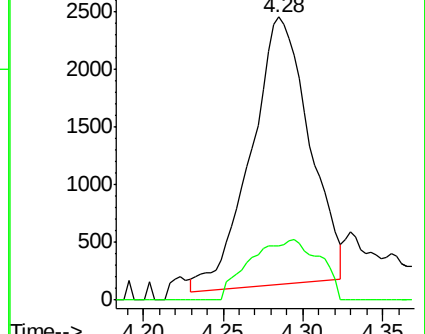

#20

Methylene Chloride

Concen: 24.939 ug/l

RT: 4.51 min Scan# 850

Delta R.T. 0.01 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Tgt Ion: 84 Resp: 62012


Ion Ratio Lower Upper

84 100

49 120.7 90.6 136.0

51 36.0 27.8 41.8

86 58.8 50.1 75.1






Abundance Ion 83.90 (83.60 to 84.60): VN062059.D (-826) (-)

Ion 48.90 (48.60 to 49.60): VN062059.D (-826) (-)

Ion 50.90 (50.60 to 51.60): VN062059.D (-826) (-)

Ion 85.90 (85.60 to 86.60): VN062059.D (-826) (-)

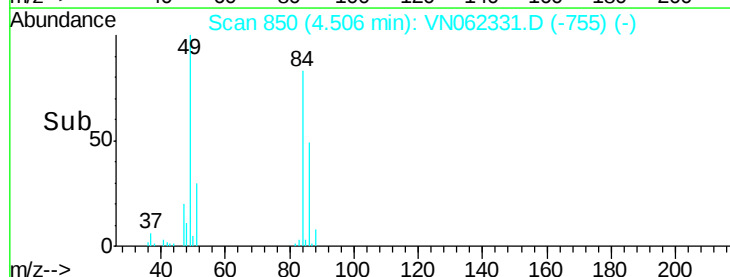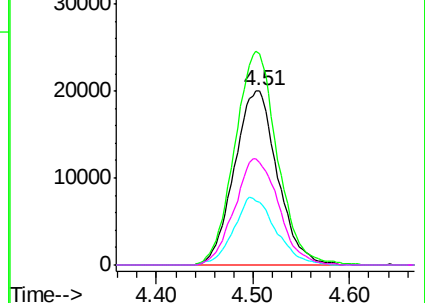

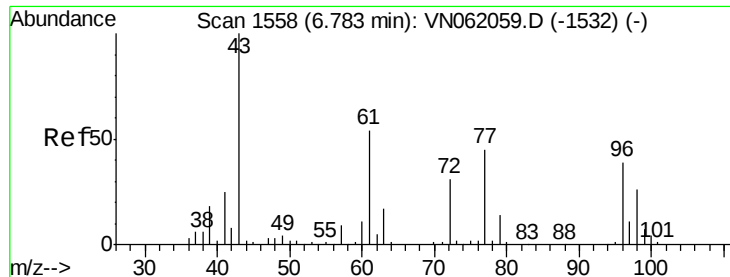

#25

2-Butanone

Concen: 24.554 ug/l

RT: 6.79 min Scan# 1561

Delta R.T. 0.01 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Instrument :

MSVOA_N

ClientSampleId :


CHASSIS-WASH

Tgt Ion: 43 Resp: 32367




Ion Ratio Lower Upper

43 100

72 31.3 24.8 37.2

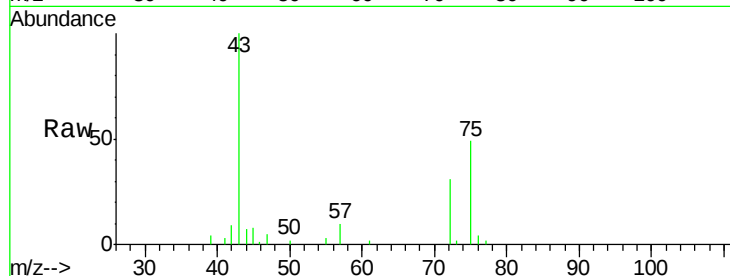

Abundance Ion 43.00 (42.70 to 43.70): VN062059.D (-1532) (-)

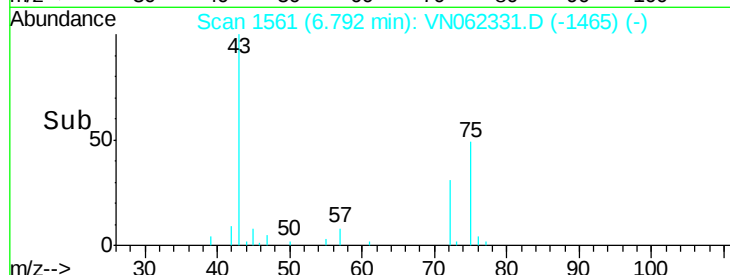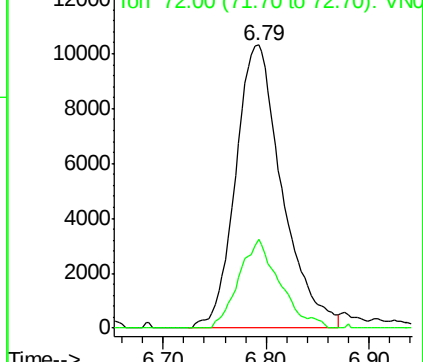

#29

Tetrahydrofuran

Concen: 0.331 ug/l

RT: 7.15 min Scan# 1672

Delta R.T. -0.02 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46


Tgt Ion: 42 Resp: 286

Ion Ratio Lower Upper



42 100


72 0.0 41.1 61.7#

71 0.0 38.2 57.4#



Abundance Ion 42.00 (41.70 to 42.70): VN062059.D (-1647) (-)

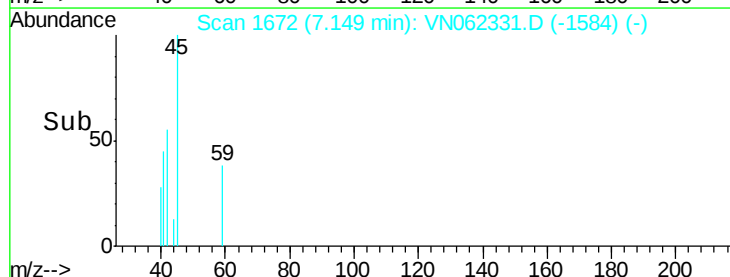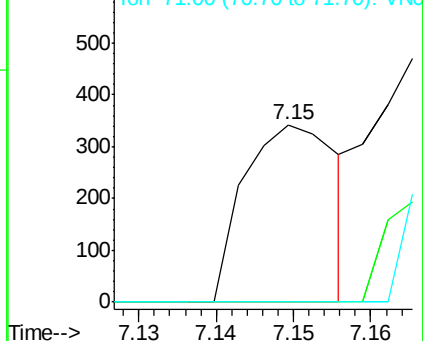

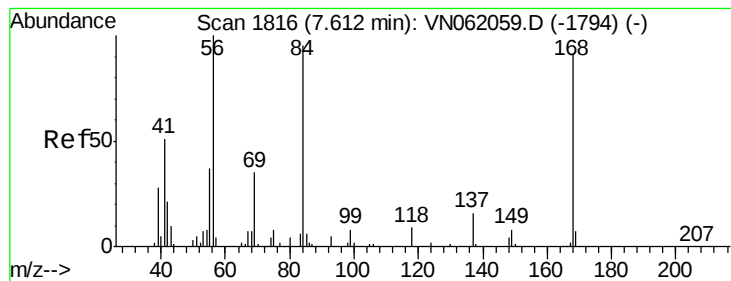

#31

Cyclohexane

Concen: 1.352 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.01 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Instrument :

MSVOA_N

ClientSampleId :

CHASSIS-WASH


Tgt Ion: 56 Resp: 5039

Ion Ratio Lower Upper

56 100

69 160.8 28.0 42.0#




84 145.7 76.1 114.1#



Abundance Ion 56.00 (55.70 to 56.70): VN062331.D (-1723) (-)

Ion 69.00 (68.70 to 69.70): VN062331.D (-1723) (-)

Ion 84.00 (83.70 to 84.70): VN062331.D (-1723) (-)

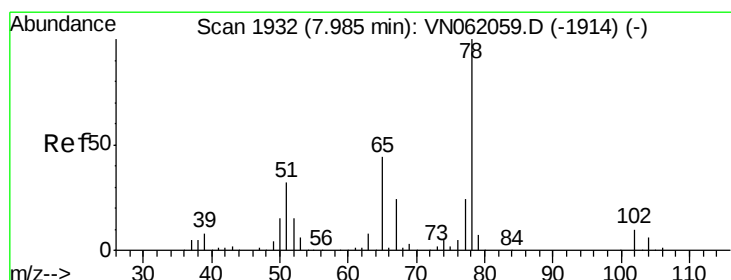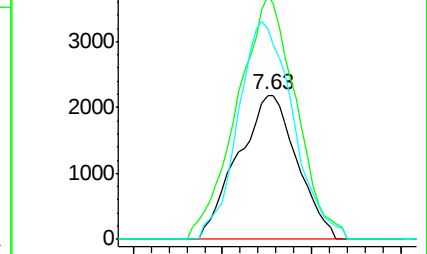

#33

1,2-Dichloroethane-d4

Concen: 59.680 ug/l

RT: 7.99 min Scan# 1933

Delta R.T. 0.00 min

Lab File: VN062331.D


Acq: 2 Jul 2020 8:46

Tgt Ion: 65 Resp: 160950

Ion Ratio Lower Upper



65 100


67 52.8 0.0 106.2



Abundance Ion 64.90 (64.60 to 65.60): VN062331.D (-1839) (-)

Ion 66.90 (66.60 to 67.60): VN062331.D (-1839) (-)

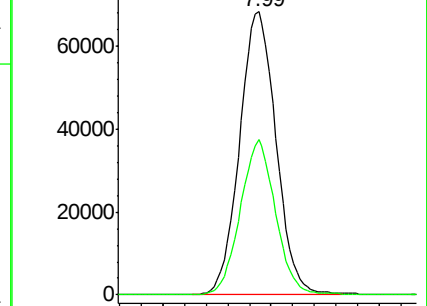







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.55 min Scan# 2108
Delta R.T. -0.00 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46

Instrument :
MSVOA_N
ClientSampleId :
CHASSIS-WASH

Tgt Ion:114 Resp: 403030
Ion Ratio Lower Upper
114 100
63 20.7 0.0 39.2
88 15.9 0.0 30.8




Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN


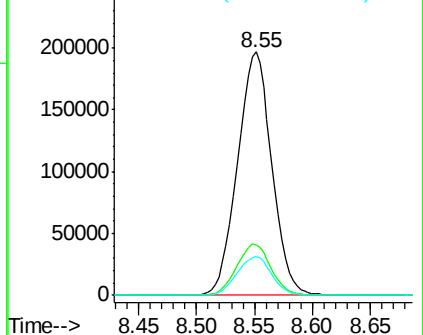



#35
Dibromofluoromethane
Concen: 49.360 ug/l
RT: 7.55 min Scan# 1797
Delta R.T. 0.00 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46

Tgt Ion:113 Resp: 127626
Ion Ratio Lower Upper
113 100
111 103.0 82.2 123.4
192 17.1 14.0 21.0



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V




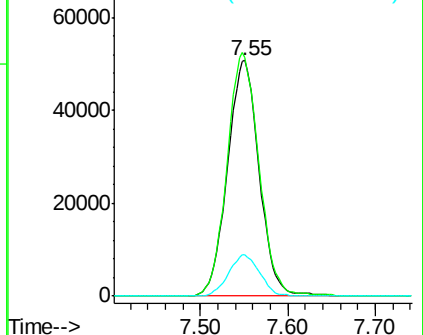


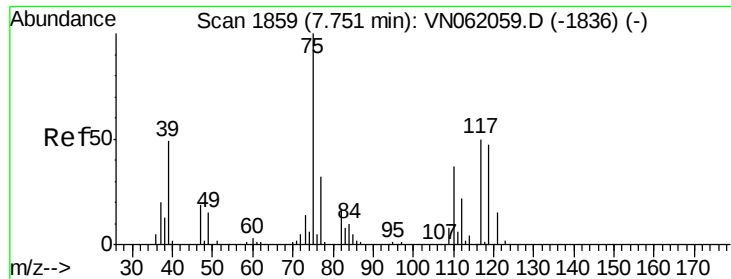

#36
 1,1-Dichloropropene
 Concen: 4.581 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.13 min
 Lab File: VN062331.D
 Acq: 2 Jul 2020 8:46




Instrument :
 MSVOA_N
 ClientSampleId :
 CHASSIS-WASH


Tgt Ion: 75 Resp: 18559
 Ion Ratio Lower Upper
 75 100
 110 7.4 17.9 53.8#
 77 0.0 24.9 37.3#

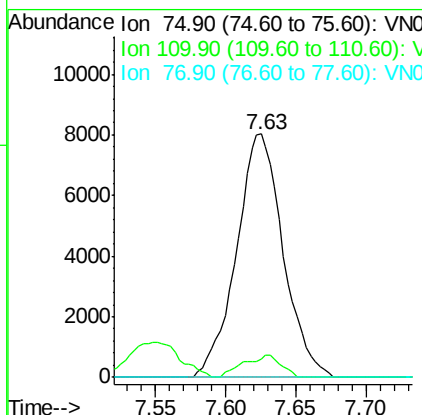

#37
 Ethyl Acetate
 Concen: 9.649 ug/l
 RT: 6.79 min Scan# 1561
 Delta R.T. -0.09 min
 Lab File: VN062331.D
 Acq: 2 Jul 2020 8:46

Tgt Ion: 43 Resp: 32367
 Ion Ratio Lower Upper
 43 100
 61 0.8 12.0 18.0#
 70 0.0 9.6 14.4#

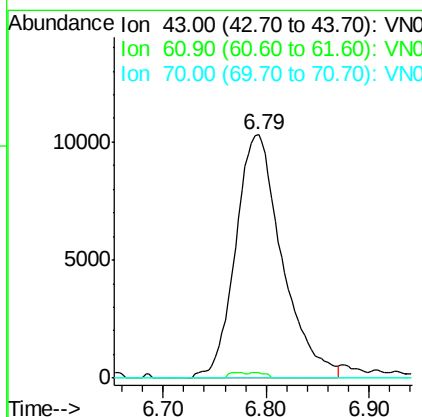



#38

Carbon Tetrachloride

Concen: 5.430 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.11 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Instrument :

MSVOA_N

ClientSampleId :

CHASSIS-WASH


Tgt Ion:117 Resp: 20740

Ion Ratio Lower Upper

117 100

119 5.6 78.2 117.2#




121 0.0 25.8 38.6#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

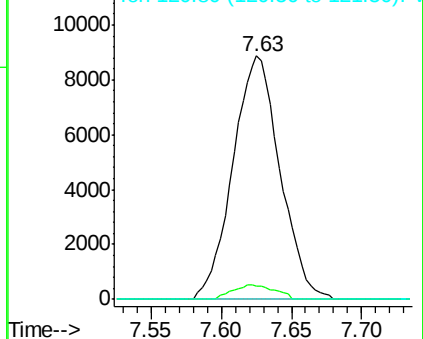

#41

Methacrylonitrile

Concen: 0.480 ug/l

RT: 7.16 min Scan# 1676

Delta R.T. 0.04 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Tgt Ion: 41 Resp: 746


Ion Ratio Lower Upper

41 100

39 0.0 44.2 66.2#

67 0.0 79.5 119.3#

52 0.0 32.3 48.5#






Abundance Ion 41.00 (40.70 to 41.70): V

Ion 39.00 (38.70 to 39.70): V

Ion 67.00 (66.70 to 67.70): V

Ion 52.00 (51.70 to 52.70): V




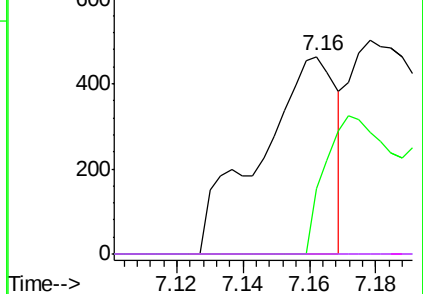




#43
Isopropyl Acetate
Concen: 2.111 ug/l
RT: 8.13 min Scan# 1977
Delta R.T. 0.00 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46




Instrument :
MSVOA_N
ClientSampleId :
CHASSIS-WASH


Tgt Ion: 43 Resp: 11545
Ion Ratio Lower Upper
43 100
61 21.1 17.2 25.8
87 13.4 12.1 18.1

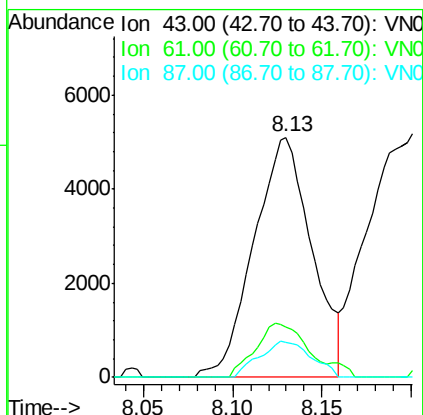

#48
Methyl methacrylate
Concen: 1.638 ug/l
RT: 9.14 min Scan# 2292
Delta R.T. -0.02 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46

Tgt Ion: 41 Resp: 4016
Ion Ratio Lower Upper
41 100
69 0.0 80.7 121.1#
39 27.4 54.5 81.7#



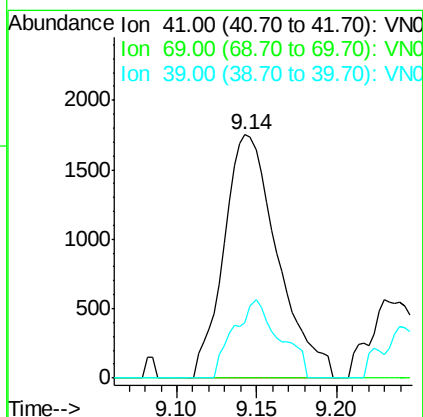





#50
Toluene-d8
Concen: 51.968 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. -0.00 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46




Instrument :
MSVOA_N
ClientSampleId :
CHASSIS-WASH


Tgt Ion: 98 Resp: 537122
Ion Ratio Lower Upper
98 100
100 64.8 51.2 76.8

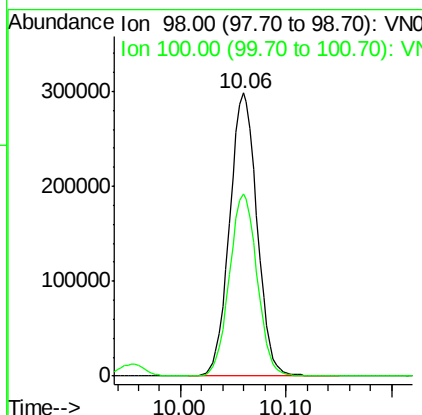

#51
4-Methyl-2-Pentanone
Concen: 44.257 ug/l
RT: 9.95 min Scan# 2544
Delta R.T. -0.00 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46

Tgt Ion: 43 Resp: 141399
Ion Ratio Lower Upper
43 100
58 40.5 34.2 51.2



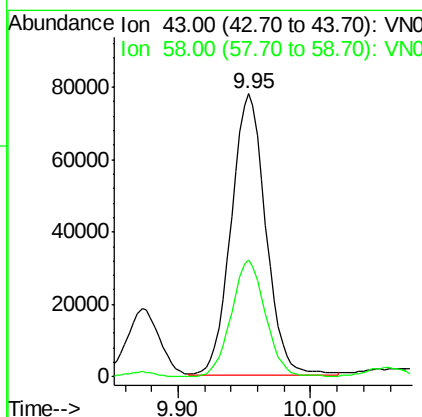



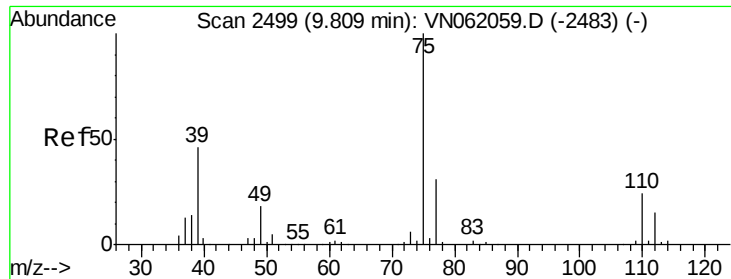

#54
 cis-1,3-Dichloropropene
 Concen: 3.093 ug/l
 RT: 9.87 min Scan# 2519
 Delta R.T. 0.06 min
 Lab File: VN062331.D
 Acq: 2 Jul 2020 8:46




Instrument :
 MSVOA_N
 ClientSampleId :
 CHASSIS-WASH


Tgt Ion: 75 Resp: 15110
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.6#
 39 44.5 36.9 55.3

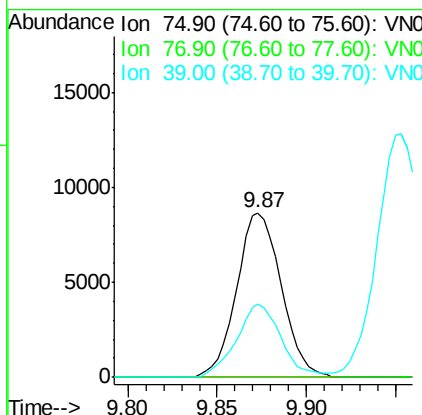

#56
 Ethyl methacrylate
 Concen: 1.605 ug/l
 RT: 10.33 min Scan# 2661
 Delta R.T. -0.07 min
 Lab File: VN062331.D
 Acq: 2 Jul 2020 8:46

Tgt Ion: 69 Resp: 6345
 Ion Ratio Lower Upper
 69 100
 41 110.9 46.6 70.0#
 39 59.2 31.0 46.4#



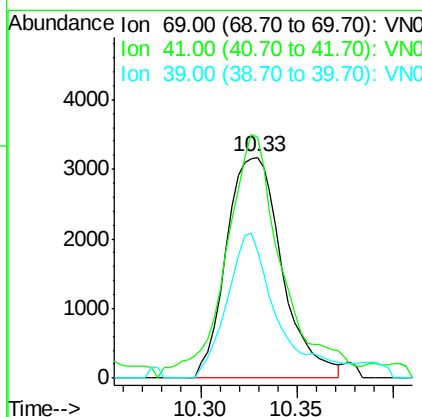





#59
2-Hexanone
Concen: 5.170 ug/l
RT: 10.73 min Scan# 2787
Delta R.T. 0.01 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46




Instrument :
MSVOA_N
ClientSampleId :
CHASSIS-WASH


Tgt Ion: 43 Resp: 11927
Ion Ratio Lower Upper
43 100
58 35.4 29.5 88.5

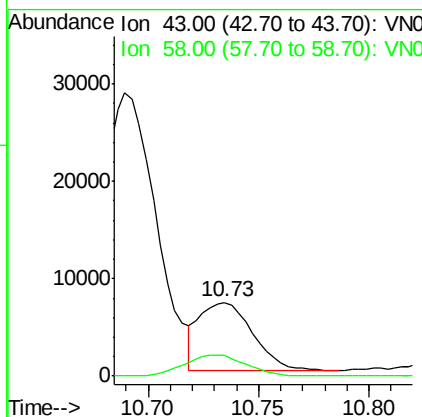

#62
4-Bromofluorobenzene
Concen: 51.851 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.00 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46

Tgt Ion: 95 Resp: 181063
Ion Ratio Lower Upper
95 100
174 70.9 0.0 154.8
176 68.5 0.0 147.4



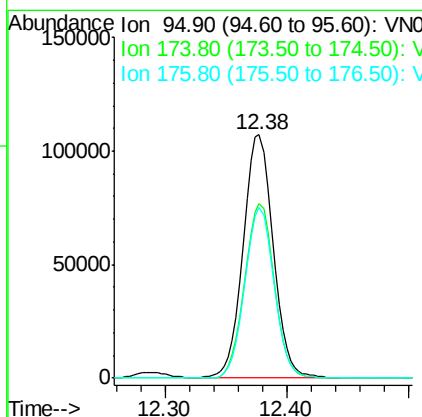





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. -0.00 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46




Instrument :
MSVOA_N
ClientSampleId :
CHASSIS-WASH


Tgt Ion:117 Resp: 397395
Ion Ratio Lower Upper
117 100
82 58.7 43.8 65.8
119 32.2 25.2 37.8

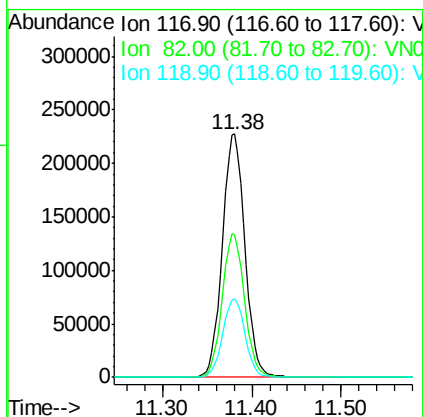

#71
Bromoform
Concen: 0.689 ug/l
RT: 12.37 min Scan# 3297
Delta R.T. 0.27 min
Lab File: VN062331.D
Acq: 2 Jul 2020 8:46

Tgt Ion:173 Resp: 1478
Ion Ratio Lower Upper
173 100
175 598.0 24.7 74.1#
254 0.0 0.0 0.0

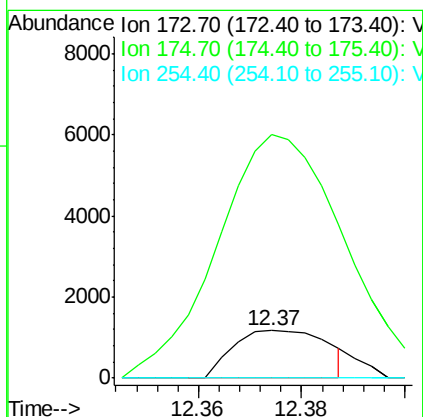

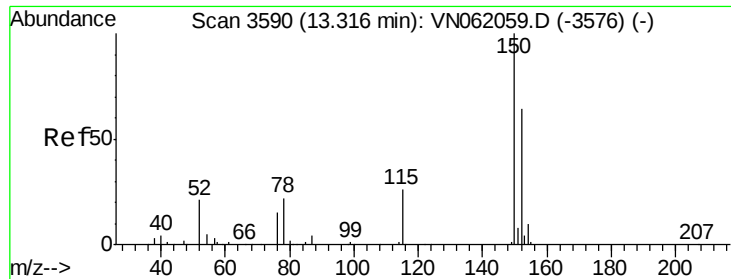

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3590

Delta R.T. -0.00 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Instrument :

MSVOA_N

ClientSampleId :

CHASSIS-WASH


Tgt Ion:152 Resp: 159150

Ion Ratio Lower Upper

152 100

115 62.2 29.5 88.5




150 157.8 0.0 351.4



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

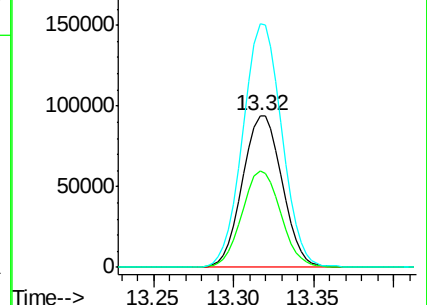

#74

N-ethyl acetate

Concen: 4.289 ug/l

RT: 12.00 min Scan# 3181

Delta R.T. -0.04 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Tgt Ion: 43 Resp: 4595


Ion Ratio Lower Upper

43 100

70 0.0 39.4 59.2#

55 9.5 21.7 32.5#

61 0.0 21.3 31.9#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V

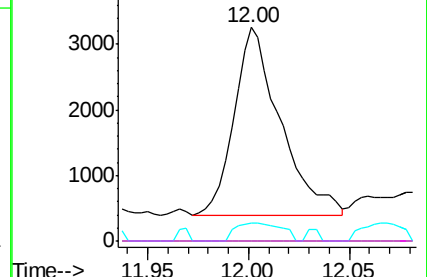



#75

1,1,2,2-Tetrachloroethane

Concen: 0.679 ug/l

RT: 12.54 min Scan# 3350

Delta R.T. 0.07 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Instrument :

MSVOA_N

ClientSampleId :

CHASSIS-WASH


Tgt Ion: 83 Resp: 2782

Ion Ratio Lower Upper

83 100

131 0.0 4.8 14.4#

85 0.0 32.4 97.0#




Abundance Ion 82.90 (82.60 to 83.60): VN062331.D (-3236) (-)

Ion 130.80 (130.50 to 131.50): VN062331.D (-3236) (-)

Ion 84.90 (84.60 to 85.60): VN062331.D (-3236) (-)

Time-->




Abundance

Ion 82.90 (82.60 to 83.60): VN062331.D (-3236) (-)

Ion 130.80 (130.50 to 131.50): VN062331.D (-3236) (-)

Ion 84.90 (84.60 to 85.60): VN062331.D (-3236) (-)

Time-->



#76

1,2,3-Trichloropropane

Concen: 24.920 ug/l

RT: 12.37 min Scan# 3297

Delta R.T. -0.15 min

Lab File: VN062331.D


Acq: 2 Jul 2020 8:46

Tgt Ion: 75 Resp: 93362

Ion Ratio Lower Upper

75 100


77 1.5 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN062331.D (-3252) (-)

Ion 77.00 (76.70 to 77.70): VN062331.D (-3252) (-)

Time-->




Abundance

Ion 74.90 (74.60 to 75.60): VN062331.D (-3252) (-)

Ion 77.00 (76.70 to 77.70): VN062331.D (-3252) (-)

Time-->

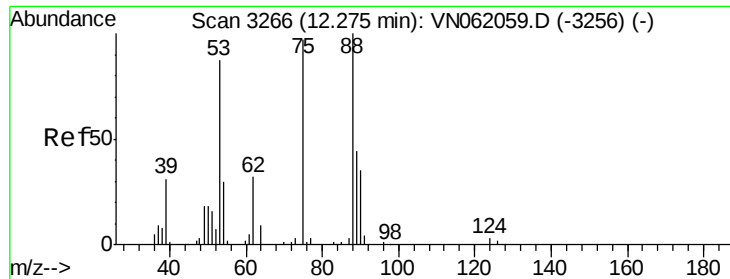

#81

trans-1,4-Dichloro-2-butene

Concen: 72.775 ug/l

RT: 12.37 min Scan# 3297

Delta R.T. 0.10 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46

Instrument :

MSVOA_N

ClientSampleId :

CHASSIS-WASH


Tgt Ion: 75 Resp: 93362

Ion Ratio Lower Upper

75 100

53 0.6 72.0 108.0#




89 0.0 36.9 55.3#

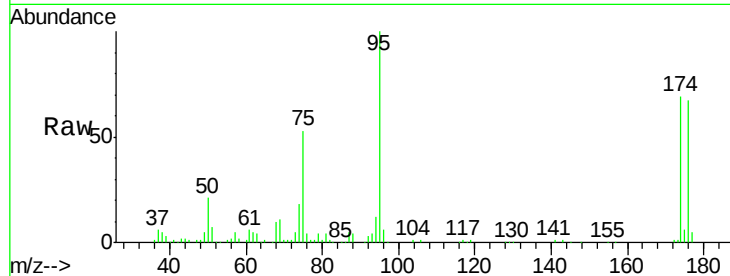

Abundance Ion 74.90 (74.60 to 75.60): VN062331.D (-3173) (-)

Ion 53.00 (52.70 to 53.70): VN062331.D (-3173) (-)

Ion 88.90 (88.60 to 89.60): VN062331.D (-3173) (-)

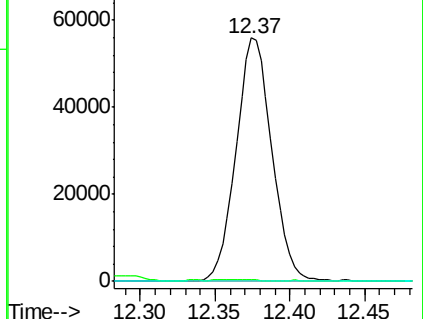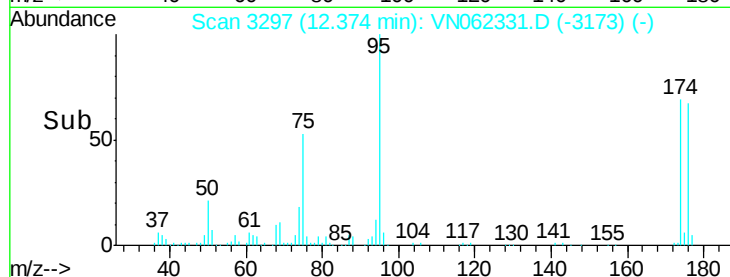

#95

Naphthalene

Concen: 4.018 ug/l

RT: 15.11 min Scan# 4147

Delta R.T. 0.00 min

Lab File: VN062331.D

Acq: 2 Jul 2020 8:46


Tgt Ion: 128 Resp: 187

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.6 13.0#



Abundance Ion 128.00 (127.70 to 128.70): VN062331.D (-4053) (-)

Ion 127.00 (126.70 to 127.70): VN062331.D (-4053) (-)

Ion 129.00 (128.70 to 129.70): VN062331.D (-4053) (-)

