

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN070120\
 Data File : VN062333.D
 Acq On : 2 Jul 2020 9:34
 Operator : JC/MD
 Sample : L3171-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAIM-SYSTEM

Quant Time: Jul 02 11:09:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	195797	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	408676	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	405236	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	152850	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	165797	60.34	ug/l	0.00
Spiked Amount 50.000			Recovery =	120.68%		
35) Dibromofluoromethane	7.55	113	131896	50.31	ug/l	0.00
Spiked Amount 50.000			Recovery =	100.62%		
50) Toluene-d8	10.06	98	534064	50.96	ug/l	0.00
Spiked Amount 50.000			Recovery =	101.92%		
62) 4-Bromofluorobenzene	12.38	95	173859	49.10	ug/l	0.00
Spiked Amount 50.000			Recovery =	98.20%		


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.03	50	413	Below Cal	#	41
11) Tert butyl alcohol	4.73	59	362	0.918	ug/l #	72
16) Acetone	3.78	43	157473	181.475	ug/l	96
17) Carbon Disulfide	4.01	76	10457	1.673	ug/l	97
18) Methyl Acetate	4.29	43	10735	4.915	ug/l #	89
20) Methylene Chloride	4.50	84	33124	12.972	ug/l	99
25) 2-Butanone	6.80	43	13031	9.703	ug/l	98
28) Bromochloromethane	7.33	49	9043	4.644	ug/l #	11
29) Tetrahydrofuran	7.17	42	915	1.040	ug/l #	50
30) Chloroform	7.33	83	109048	23.882	ug/l	99
31) Cyclohexane	7.63	56	5241	1.381	ug/l #	11
36) 1,1-Dichloropropene	7.62	75	18350	4.467	ug/l #	47
37) Ethyl Acetate	6.80	43	13031	3.831	ug/l #	66
38) Carbon Tetrachloride	7.63	117	20617	5.324	ug/l #	16
41) Methacrylonitrile	7.17	41	619	0.393	ug/l #	24
43) Isopropyl Acetate	8.13	43	11098	2.001	ug/l #	92
48) Methyl methacrylate	9.14	41	2135	0.859	ug/l #	34
51) 4-Methyl-2-Pentanone	9.95	43	19589	6.047	ug/l	99
52) Toluene	10.12	92	5252	0.687	ug/l	97
54) cis-1,3-Dichloropropene	9.88	75	6336	1.279	ug/l #	74
59) 2-Hexanone	10.69	43	62957	26.912	ug/l #	21
71) Bromoform	12.37	173	602	0.275	ug/l #	1
74) N-amyl acetate	12.01	43	2853	3.954	ug/l #	40
76) 1,2,3-Trichloropropane	12.37	75	89634	24.911	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.37	75	89634	72.749	ug/l #	13
86) p-Isopropyltoluene	13.26	119	36673	3.859	ug/l	91
95) Naphthalene	15.10	128	29	3.999	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN070120\
Data File : VN062333.D
Acq On : 2 Jul 2020 9:34
Operator : JC/MD
Sample : L3171-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM

Quant Time: Jul 02 11:09:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 24 15:33:00 2020
Response via : Initial Calibration

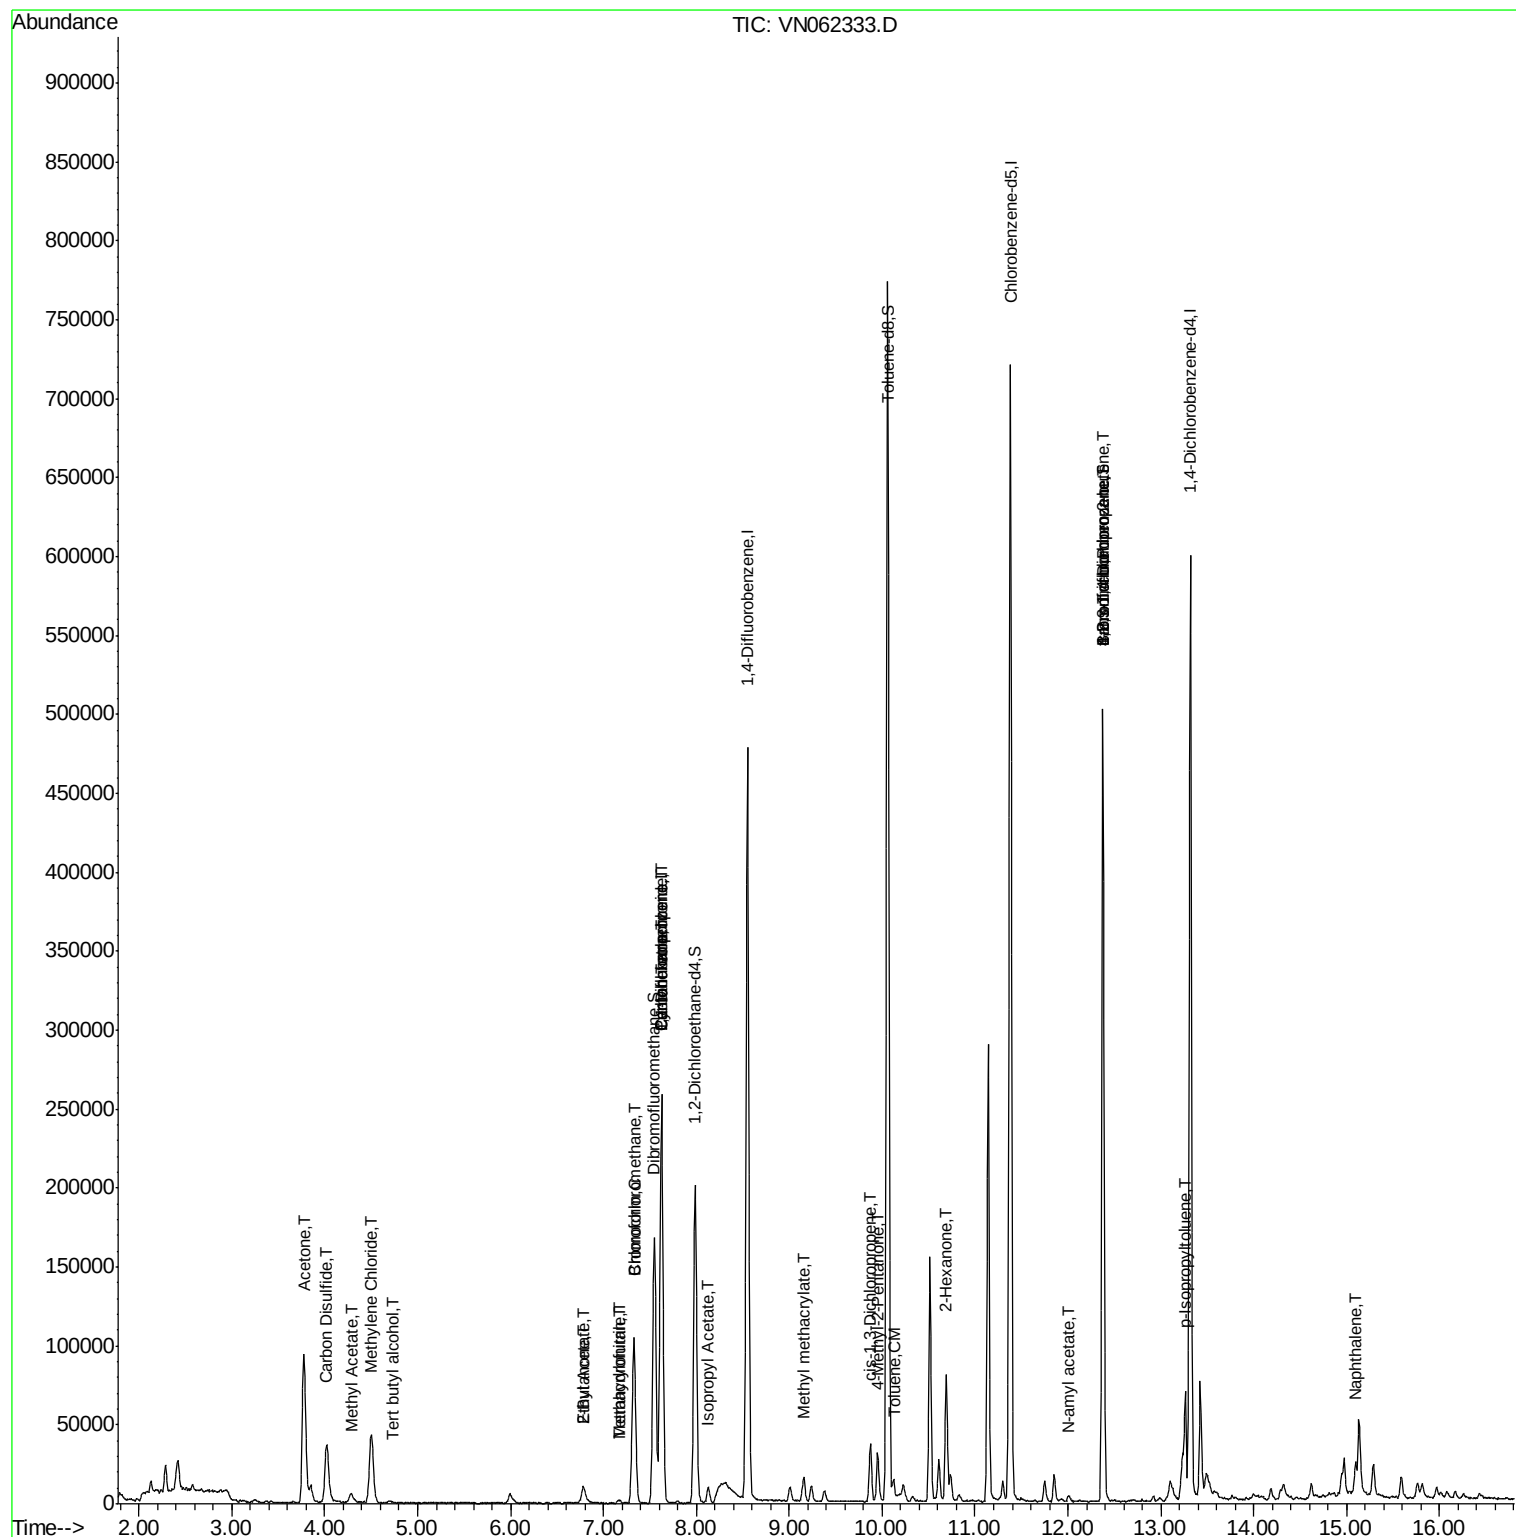

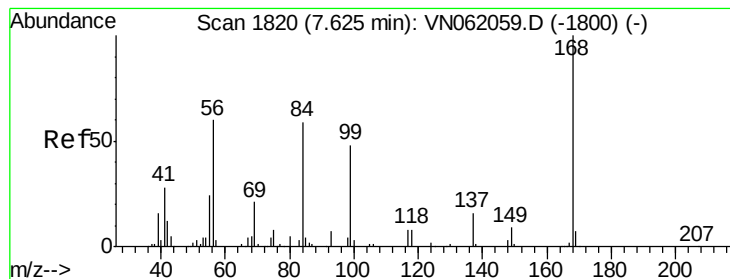

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062333.D

Acq: 2 Jul 2020 9:34


Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM

Tgt Ion:168 Resp: 195797

Ion Ratio Lower Upper




168 100

99 64.2 45.8 68.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

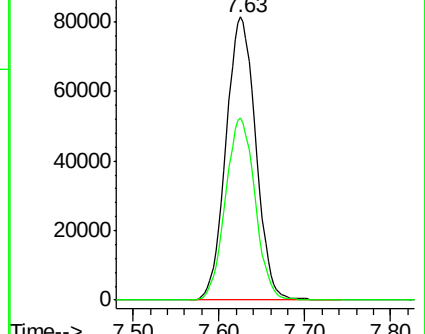

#3

Chloromethane

Concen: Below Cal

RT: 2.03 min Scan# 80

Delta R.T. -0.00 min

Lab File: VN062333.D


Acq: 2 Jul 2020 9:34

Tgt Ion: 50 Resp: 413

Ion Ratio Lower Upper



50 100


52 0.0 27.0 40.6#



Abundance Ion 49.90 (49.60 to 50.60): VNO

Ion 51.90 (51.60 to 52.60): VNO

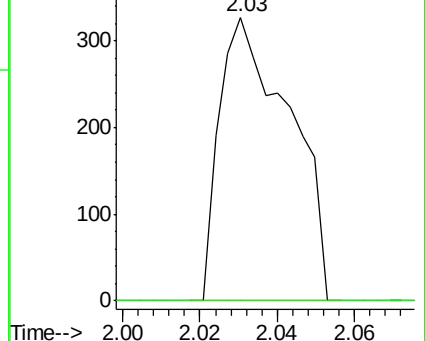




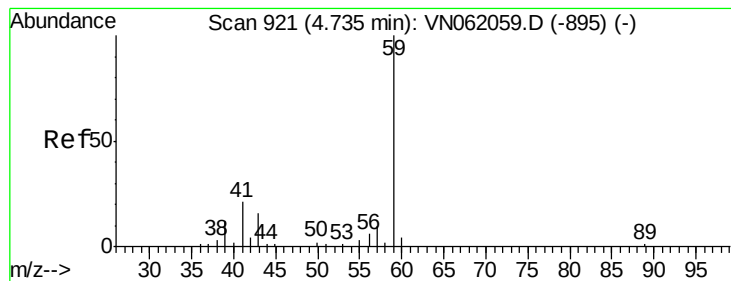


#11

Tert butyl alcohol
 Concen: 0.918 ug/l
 RT: 4.73 min Scan# 920
 Delta R.T. -0.00 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34

Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAIM-SYSTEM




Tgt Ion: 59 Resp: 362
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.3 12.5#

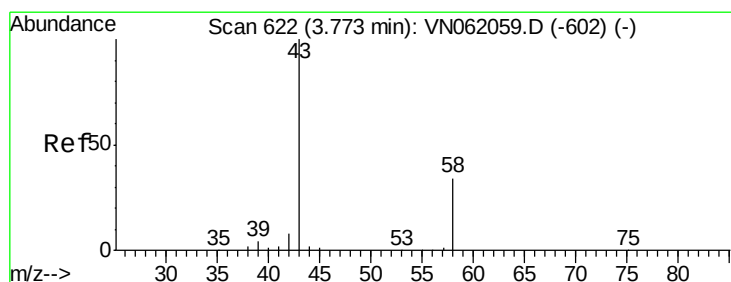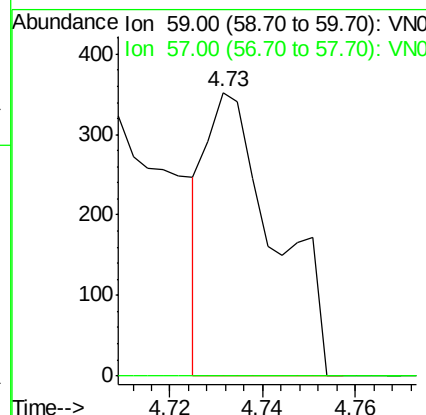


#16

Acetone
 Concen: 181.475 ug/l
 RT: 3.78 min Scan# 623
 Delta R.T. 0.00 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34

Tgt Ion: 43 Resp: 157473
 Ion Ratio Lower Upper
 43 100
 58 32.2 27.5 41.3

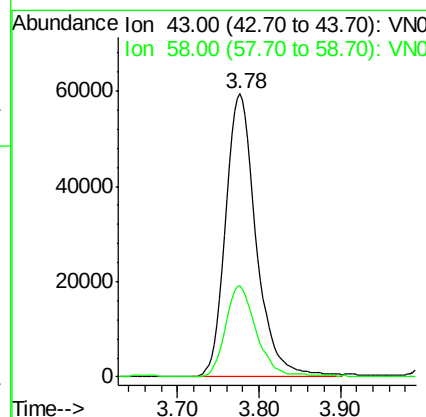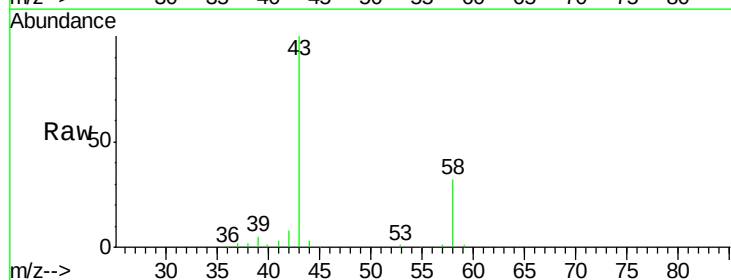



#17

Carbon Disulfide

Concen: 1.673 ug/l

RT: 4.01 min Scan# 695

Delta R.T. 0.00 min

Lab File: VN062333.D

Acq: 2 Jul 2020 9:34

Instrument :

MSVOA_N

ClientSampleId :


RECLAIM-SYSTEM

Tgt Ion: 76 Resp: 10457

Ion Ratio Lower Upper




76 100

78 8.0 7.2 10.8



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

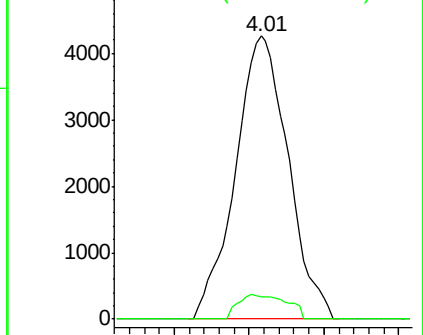

#18

Methyl Acetate

Concen: 4.915 ug/l

RT: 4.29 min Scan# 782

Delta R.T. 0.01 min

Lab File: VN062333.D


Acq: 2 Jul 2020 9:34

Tgt Ion: 43 Resp: 10735

Ion Ratio Lower Upper



43 100


74 22.5 22.9 34.3#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 74.00 (73.70 to 74.70): VN0

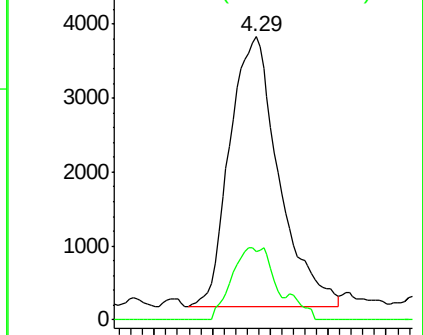




#20
Methylene Chloride
Concen: 12.972 ug/l
RT: 4.50 min Scan# 849
Delta R.T. 0.00 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34

Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM

Tgt Ion:	84	Resp:	33124
Ion	Ratio	Lower	Upper
84	100		
49	113.4	90.6	136.0
51	37.1	27.8	41.8
86	63.3	50.1	75.1






Abundance Ion 83.90 (83.60 to 84.60): VN062059.D (-826) (-)

Ion 48.90 (48.60 to 49.60): VN062059.D (-826) (-)


Ion 50.90 (50.60 to 51.60): VN062059.D (-826) (-)

Ion 85.90 (85.60 to 86.60): VN062059.D (-826) (-)

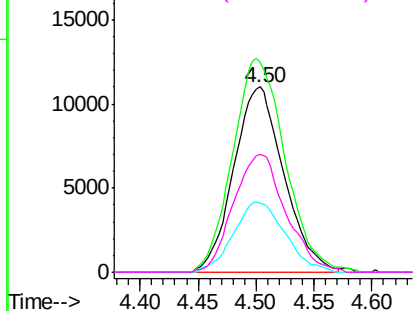



#25
2-Butanone
Concen: 9.703 ug/l
RT: 6.80 min Scan# 1562
Delta R.T. 0.01 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34


Tgt Ion:	43	Resp:	13031
Ion	Ratio	Lower	Upper
43	100		
72	30.0	24.8	37.2



Abundance Ion 43.00 (42.70 to 43.70): VN062059.D (-1532) (-)

Ion 72.00 (71.70 to 72.70): VN062059.D (-1532) (-)




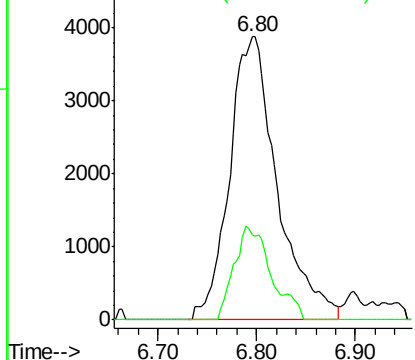




#28
 Bromochloromethane
 Concen: 4.644 ug/l
 RT: 7.33 min Scan# 1727
 Delta R.T. 0.18 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34




Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAIM-SYSTEM


Tgt Ion: 49 Resp: 9043
 Ion Ratio Lower Upper
 49 100
 129 0.0 0.0 4.4
 130 0.0 65.5 98.3#

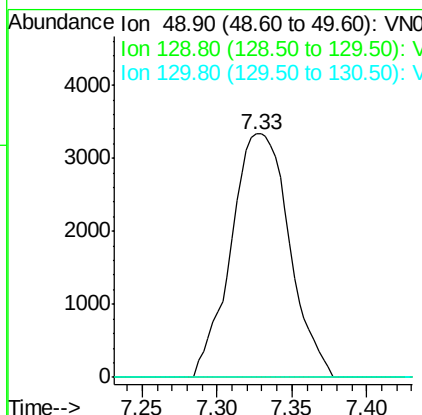

#29
 Tetrahydrofuran
 Concen: 1.040 ug/l
 RT: 7.17 min Scan# 1679
 Delta R.T. 0.01 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34

Tgt Ion: 42 Resp: 915
 Ion Ratio Lower Upper
 42 100
 72 12.8 41.1 61.7#
 71 17.4 38.2 57.4#



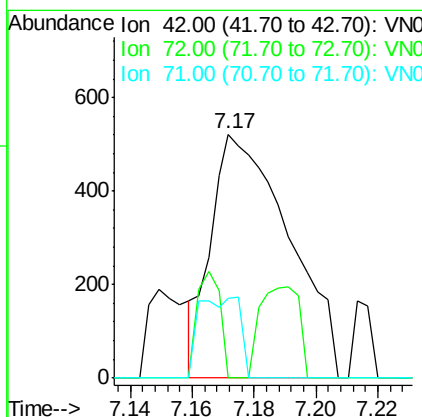





#30
Chloroform
Concen: 23.882 ug/l
RT: 7.33 min Scan# 1728
Delta R.T. -0.00 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34




Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM


Tgt Ion: 83 Resp: 109048
Ion Ratio Lower Upper
83 100
85 66.0 52.3 78.5

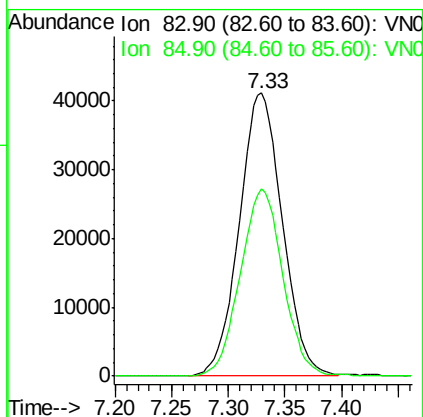

#31
Cyclohexane
Concen: 1.381 ug/l
RT: 7.63 min Scan# 1821
Delta R.T. 0.02 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34

Tgt Ion: 56 Resp: 5241
Ion Ratio Lower Upper
56 100
69 162.8 28.0 42.0#
84 135.2 76.1 114.1#



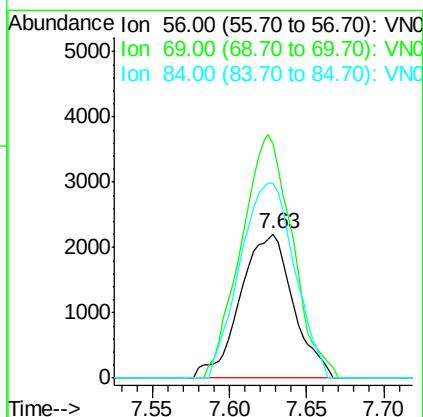



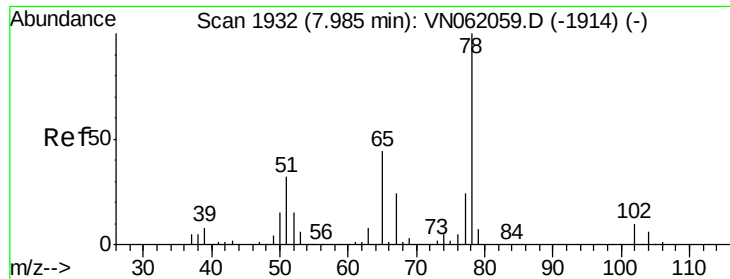

#33
 1,2-Dichloroethane-d4
 Concen: 60.341 ug/l
 RT: 7.99 min Scan# 1933
 Delta R.T. 0.00 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34




Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAIM-SYSTEM


Tgt Ion: 65 Resp: 165797
 Ion Ratio Lower Upper
 65 100
 67 52.9 0.0 106.2

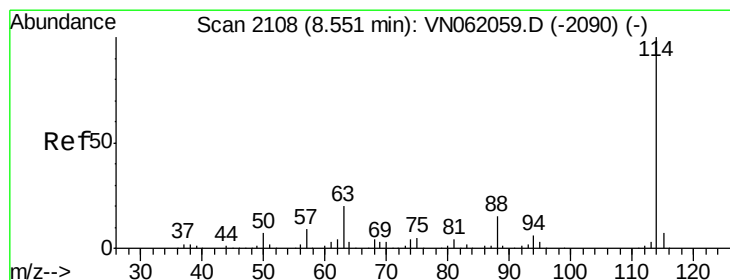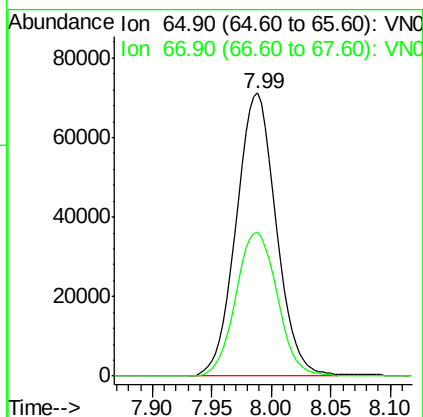

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. -0.00 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34

Tgt Ion: 114 Resp: 408676
 Ion Ratio Lower Upper
 114 100
 63 20.9 0.0 39.2
 88 16.4 0.0 30.8



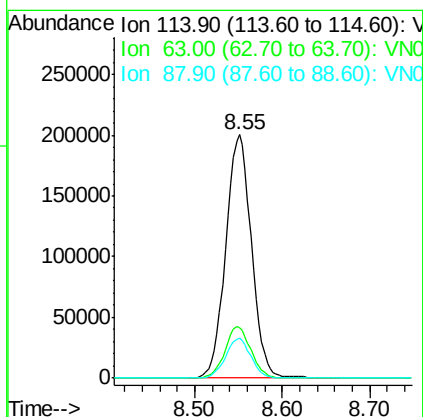





#35
 Dibromofluoromethane
 Concen: 50.306 ug/l
 RT: 7.55 min Scan# 1796
 Delta R.T. -0.00 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34




Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAIM-SYSTEM


Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.1	82.2	123.4
192	16.9	14.0	21.0

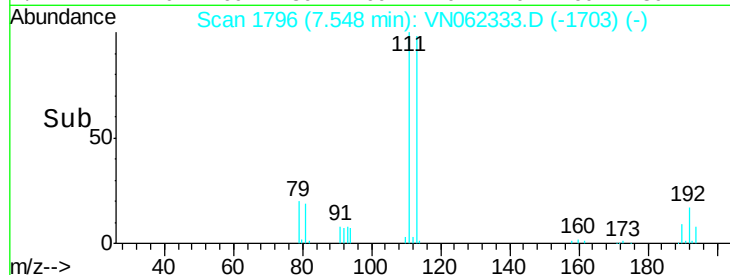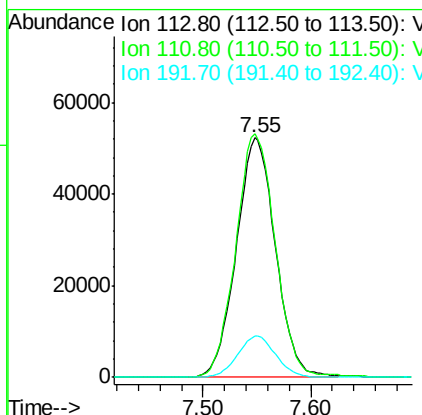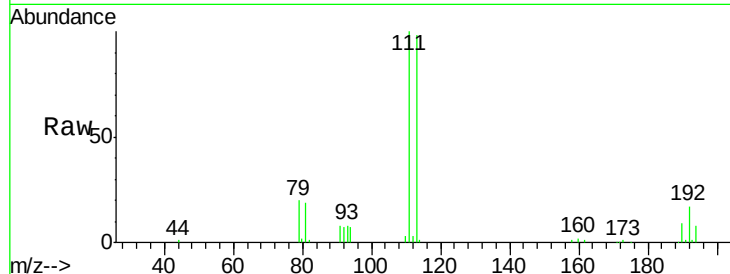

#36
 1,1-Dichloropropene
 Concen: 4.467 ug/l
 RT: 7.62 min Scan# 1819
 Delta R.T. -0.13 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34

Tgt Ion	Ratio	Lower	Upper
75	100		
110	6.4	17.9	53.8#
77	0.0	24.9	37.3#



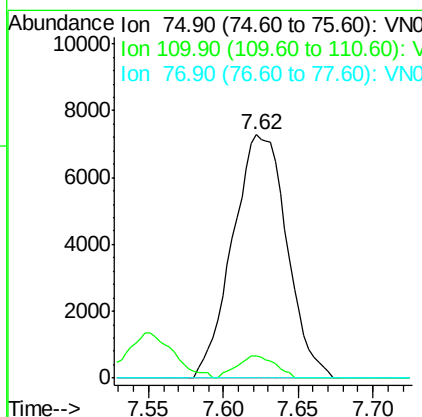
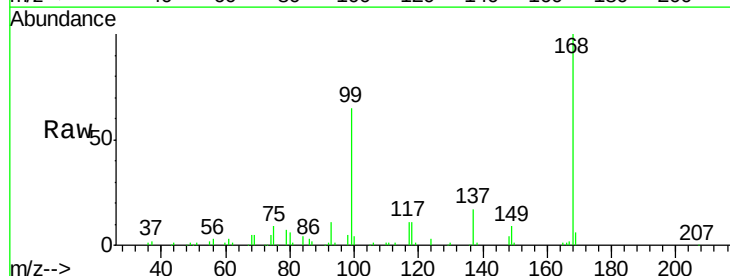




#37
Ethyl Acetate
 Concen: 3.831 ug/l
 RT: 6.80 min Scan# 1562
 Delta R.T. -0.08 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34




Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAIM-SYSTEM


Tgt Ion: 43 Resp: 13031
 Ion Ratio Lower Upper
 43 100
 61 0.0 12.0 18.0#
 70 0.0 9.6 14.4#

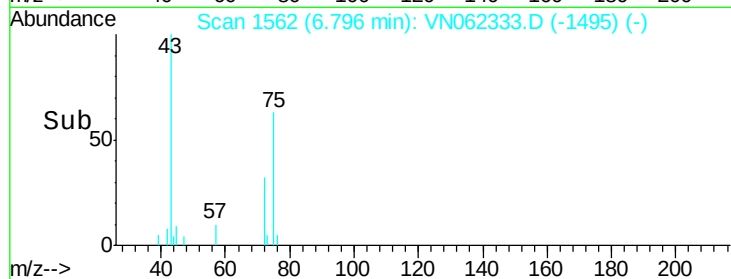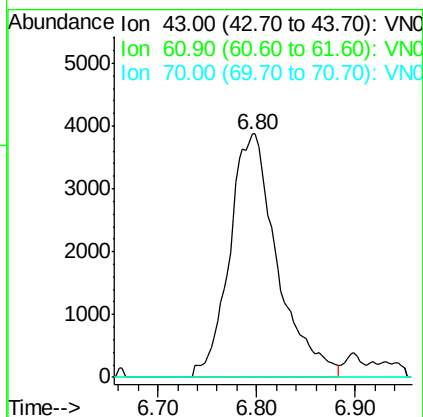

#38
Carbon Tetrachloride
 Concen: 5.324 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.11 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34

Tgt Ion: 117 Resp: 20617
 Ion Ratio Lower Upper
 117 100
 119 5.8 78.2 117.2#
 121 0.0 25.8 38.6#



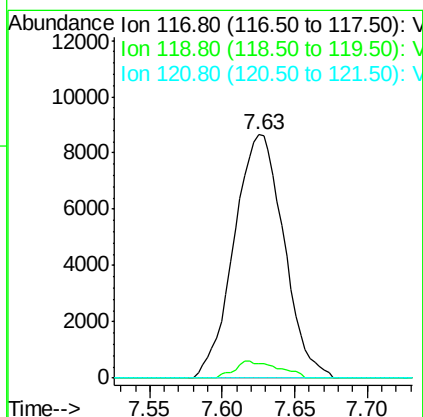





#41
Methacrylonitrile
Concen: 0.393 ug/l
RT: 7.17 min Scan# 1678
Delta R.T. 0.04 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34




Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM


Tgt Ion: 41 Resp: 619
Ion Ratio Lower Upper
41 100
39 25.2 44.2 66.2#
67 0.0 79.5 119.3#
52 0.0 32.3 48.5#

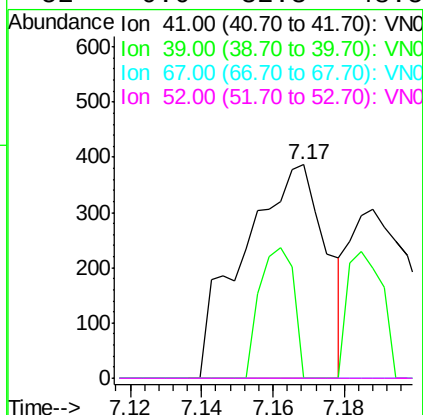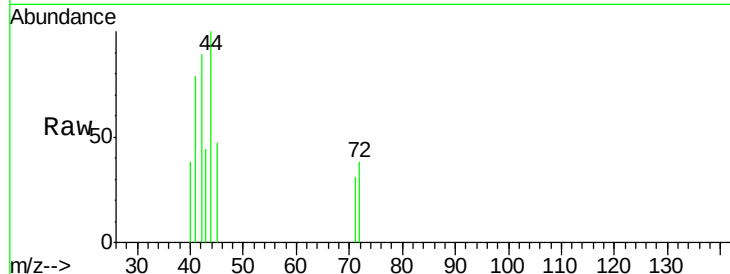

#43
Isopropyl Acetate
Concen: 2.001 ug/l
RT: 8.13 min Scan# 1977
Delta R.T. 0.00 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34

Tgt Ion: 43 Resp: 11098
Ion Ratio Lower Upper
43 100
61 17.9 17.2 25.8
87 11.5 12.1 18.1#


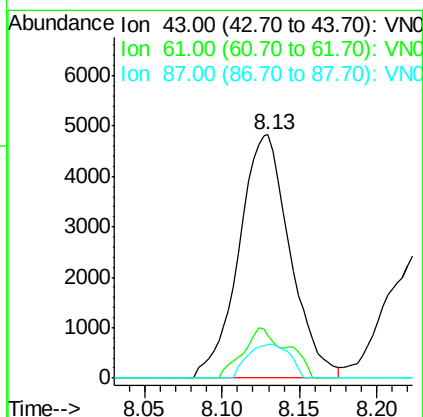






#48
Methyl methacrylate
Concen: 0.859 ug/l
RT: 9.14 min Scan# 2291
Delta R.T. -0.03 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34




Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM


Tgt Ion: 41 Resp: 2135
Ion Ratio Lower Upper
41 100
69 0.0 80.7 121.1#
39 55.3 54.5 81.7

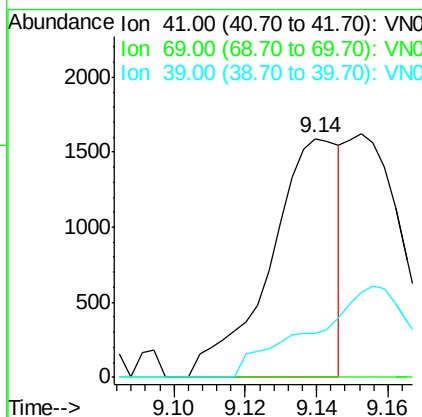

#50
Toluene-d8
Concen: 50.958 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. -0.00 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34

Tgt Ion: 98 Resp: 534064
Ion Ratio Lower Upper
98 100
100 65.2 51.2 76.8

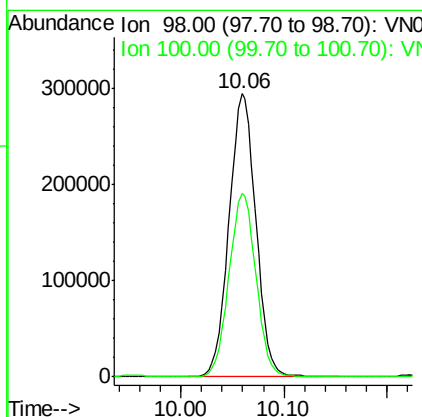

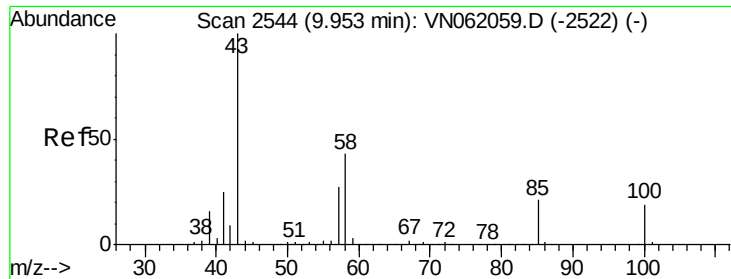

#51

4-Methyl-2-Pentanone

Concen: 6.047 ug/l

RT: 9.95 min Scan# 2544

Delta R.T. -0.00 min

Lab File: VN062333.D

Acq: 2 Jul 2020 9:34


Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM

Tgt Ion: 43 Resp: 19589

Ion Ratio Lower Upper




43 100

58 41.8 34.2 51.2



Abundance Ion 43.00 (42.70 to 43.70): VN062059.D (-2522) (-)

Ion 58.00 (57.70 to 58.70): VN062059.D (-2522) (-)

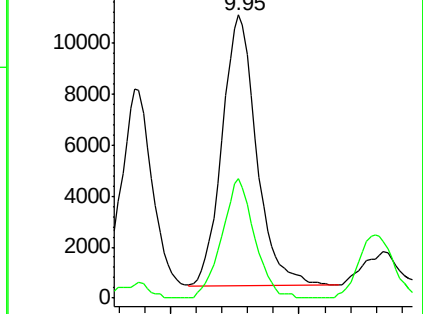

#52

Toluene

Concen: 0.687 ug/l

RT: 10.12 min Scan# 2596

Delta R.T. -0.00 min

Lab File: VN062333.D


Acq: 2 Jul 2020 9:34

Tgt Ion: 92 Resp: 5252

Ion Ratio Lower Upper



92 100


91 167.1 137.4 206.0



Abundance Ion 92.00 (91.70 to 92.70): VN062059.D (-2581) (-)

Ion 91.00 (90.70 to 91.70): VN062059.D (-2581) (-)




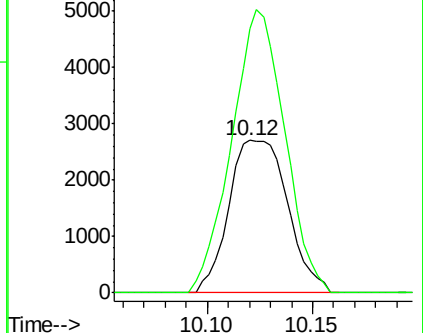


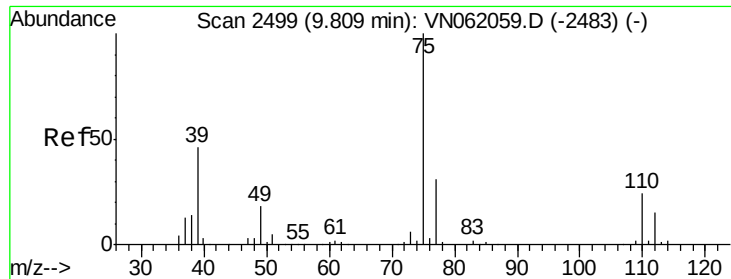

#54
 cis-1,3-Dichloropropene
 Concen: 1.279 ug/l
 RT: 9.88 min Scan# 2520
 Delta R.T. 0.07 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34




Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAIM-SYSTEM


Tgt Ion: 75 Resp: 6336
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.6#
 39 49.0 36.9 55.3

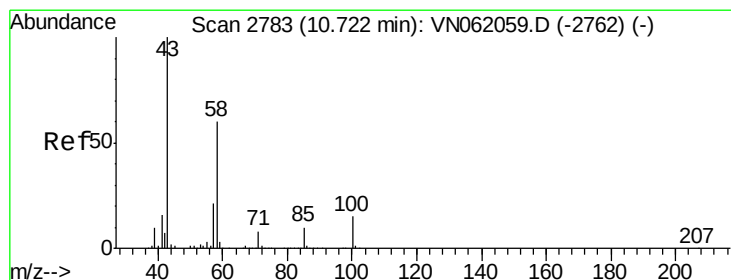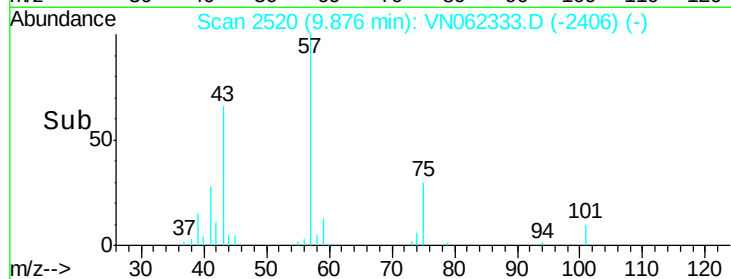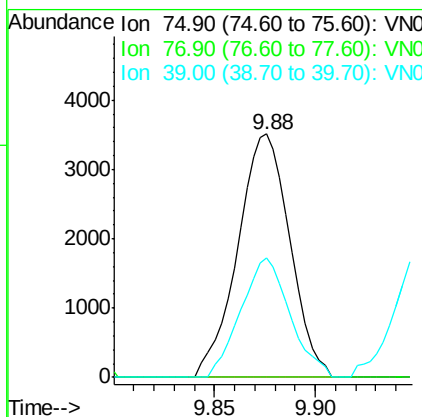

#59
 2-Hexanone
 Concen: 26.912 ug/l
 RT: 10.69 min Scan# 2773
 Delta R.T. -0.03 min
 Lab File: VN062333.D
 Acq: 2 Jul 2020 9:34

Tgt Ion: 43 Resp: 62957
 Ion Ratio Lower Upper
 43 100
 58 0.0 29.5 88.5#



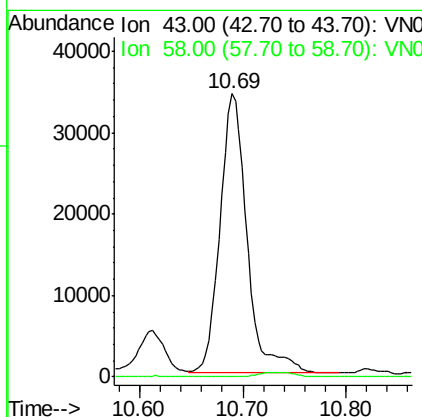





#62
4-Bromofluorobenzene
Concen: 49.100 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.00 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34




Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM


Tgt Ion: 95 Resp: 173859
Ion Ratio Lower Upper
95 100
174 72.2 0.0 154.8
176 67.7 0.0 147.4

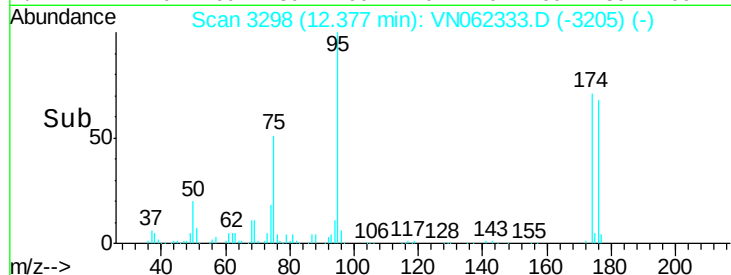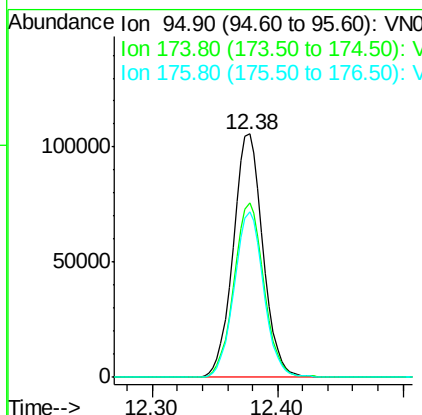

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. -0.00 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34

Tgt Ion: 117 Resp: 405236
Ion Ratio Lower Upper
117 100
82 59.0 43.8 65.8
119 31.9 25.2 37.8

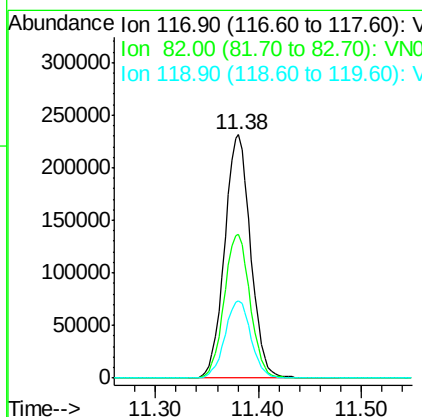



#71

Bromoform

Concen: 0.275 ug/l

RT: 12.37 min Scan# 3296

Delta R.T. 0.27 min

Lab File: VN062333.D

Acq: 2 Jul 2020 9:34

Instrument :

MSVOA_N

ClientSampleId :

RECLAIM-SYSTEM


Tgt Ion:173 Resp: 602

Ion Ratio Lower Upper

173 100

175 1315.9 24.7 74.1#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

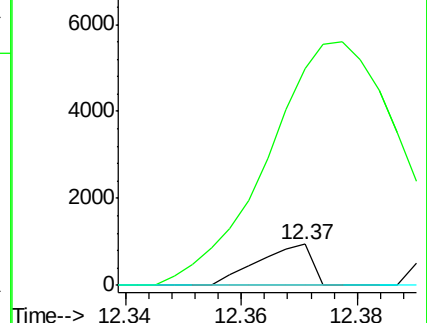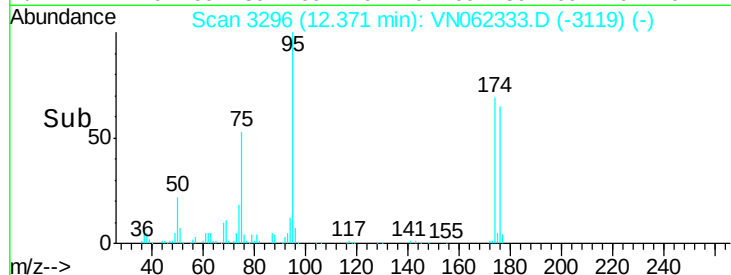

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062333.D

Acq: 2 Jul 2020 9:34


Tgt Ion:152 Resp: 152850

Ion Ratio Lower Upper

152 100

115 60.5 29.5 88.5



150 160.2 0.0 351.4




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

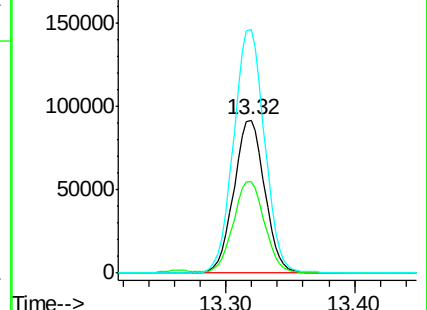

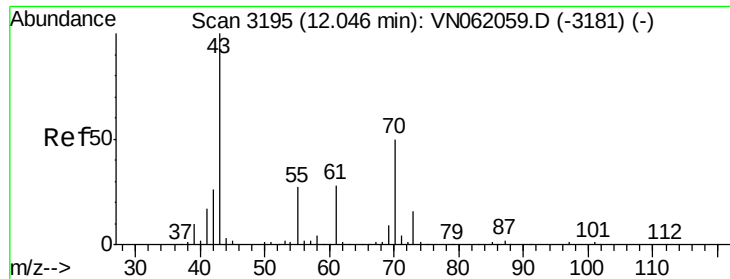

#74

N-amyI acetate

Concen: 3.954 ug/l

RT: 12.01 min Scan# 3183

Delta R.T. -0.04 min

Lab File: VN062333.D

Acq: 2 Jul 2020 9:34

Instrument :

MSVOA_N

ClientSampleId :

RECLAIM-SYSTEM

Tgt Ion: 43 Resp: 2853





Ion Ratio Lower Upper

43 100

70 0.0 39.4 59.2#

55 3.8 21.7 32.5#

61 0.0 21.3 31.9#

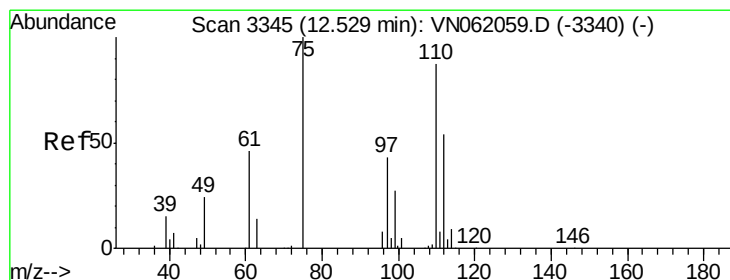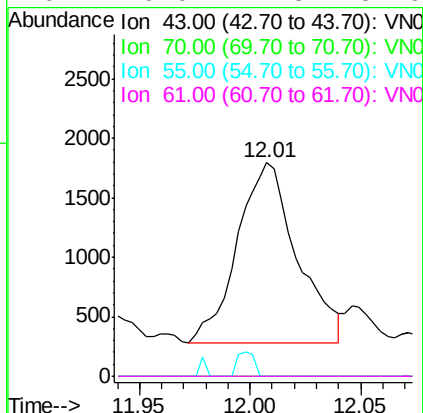

#76

1,2,3-Trichloropropane

Concen: 24.911 ug/l

RT: 12.37 min Scan# 3297

Delta R.T. -0.15 min

Lab File: VN062333.D




Acq: 2 Jul 2020 9:34


Tgt Ion: 75 Resp: 89634

Ion Ratio Lower Upper

75 100

77 1.3 0.0 0.0#

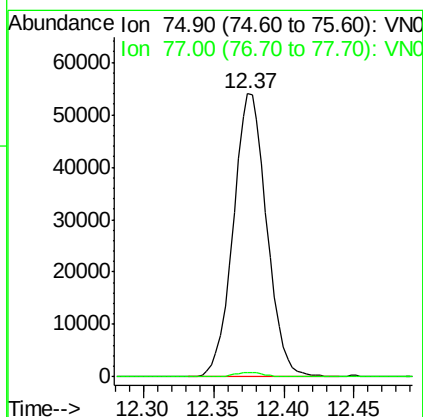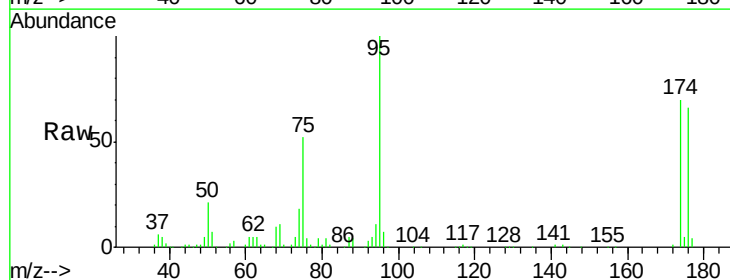

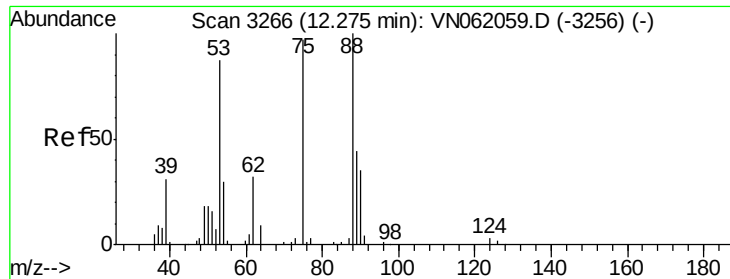

#81

trans-1,4-Dichloro-2-butene

Concen: 72.749 ug/l

RT: 12.37 min Scan# 3297

Delta R.T. 0.10 min

Lab File: VN062333.D

Acq: 2 Jul 2020 9:34

Instrument :

MSVOA_N

ClientSampleId :

RECLAIM-SYSTEM


Tgt Ion: 75 Resp: 89634

Ion Ratio Lower Upper

75 100

53 0.0 72.0 108.0#




89 0.0 36.9 55.3#

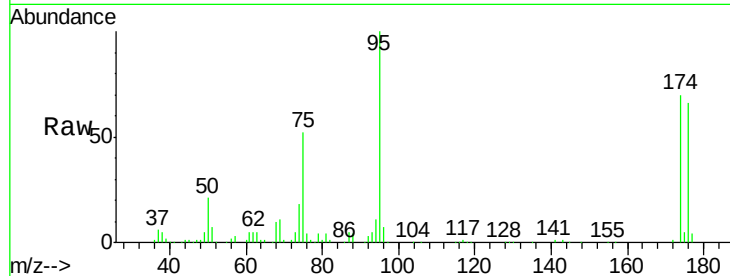

Abundance Ion 74.90 (74.60 to 75.60): VN062333.D (-3173) (-)

Ion 53.00 (52.70 to 53.70): VN062333.D (-3173) (-)

Ion 88.90 (88.60 to 89.60): VN062333.D (-3173) (-)

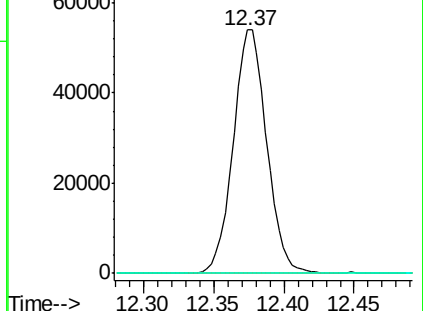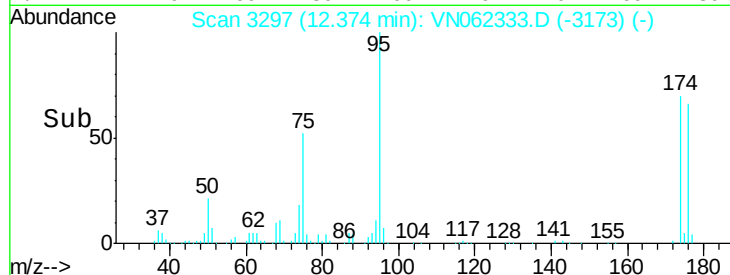

#86

p-Isopropyltoluene

Concen: 3.859 ug/l

RT: 13.26 min Scan# 3574

Delta R.T. -0.00 min

Lab File: VN062333.D

Acq: 2 Jul 2020 9:34


Tgt Ion: 119 Resp: 36673

Ion Ratio Lower Upper

119 100

134 25.8 13.0 39.0



91 31.3 11.3 33.8




Abundance Ion 119.00 (118.70 to 119.70): VN062333.D (-3481) (-)

Ion 134.00 (133.70 to 134.70): VN062333.D (-3481) (-)

Ion 91.00 (90.70 to 91.70): VN062333.D (-3481) (-)

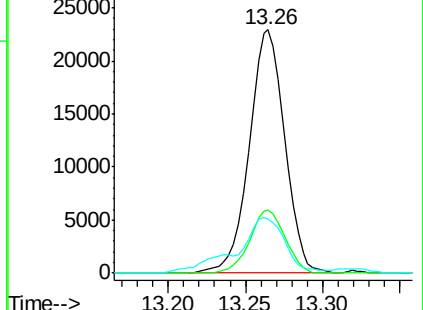




#95
Naphthalene
Concen: 3.999 ug/l
RT: 15.10 min Scan# 4145
Delta R.T. -0.00 min
Lab File: VN062333.D
Acq: 2 Jul 2020 9:34

Instrument :
MSVOA_N
ClientSampleId :
RECLAIM-SYSTEM

Tgt Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.5	15.7#
129	0.0	8.6	13.0#



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

