


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN070120\
Data File : VN062281.D
Acq On : 1 Jul 2020 10:17
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Title : SW846 8260
Last Update : Wed Jun 24 15:33:00 2020

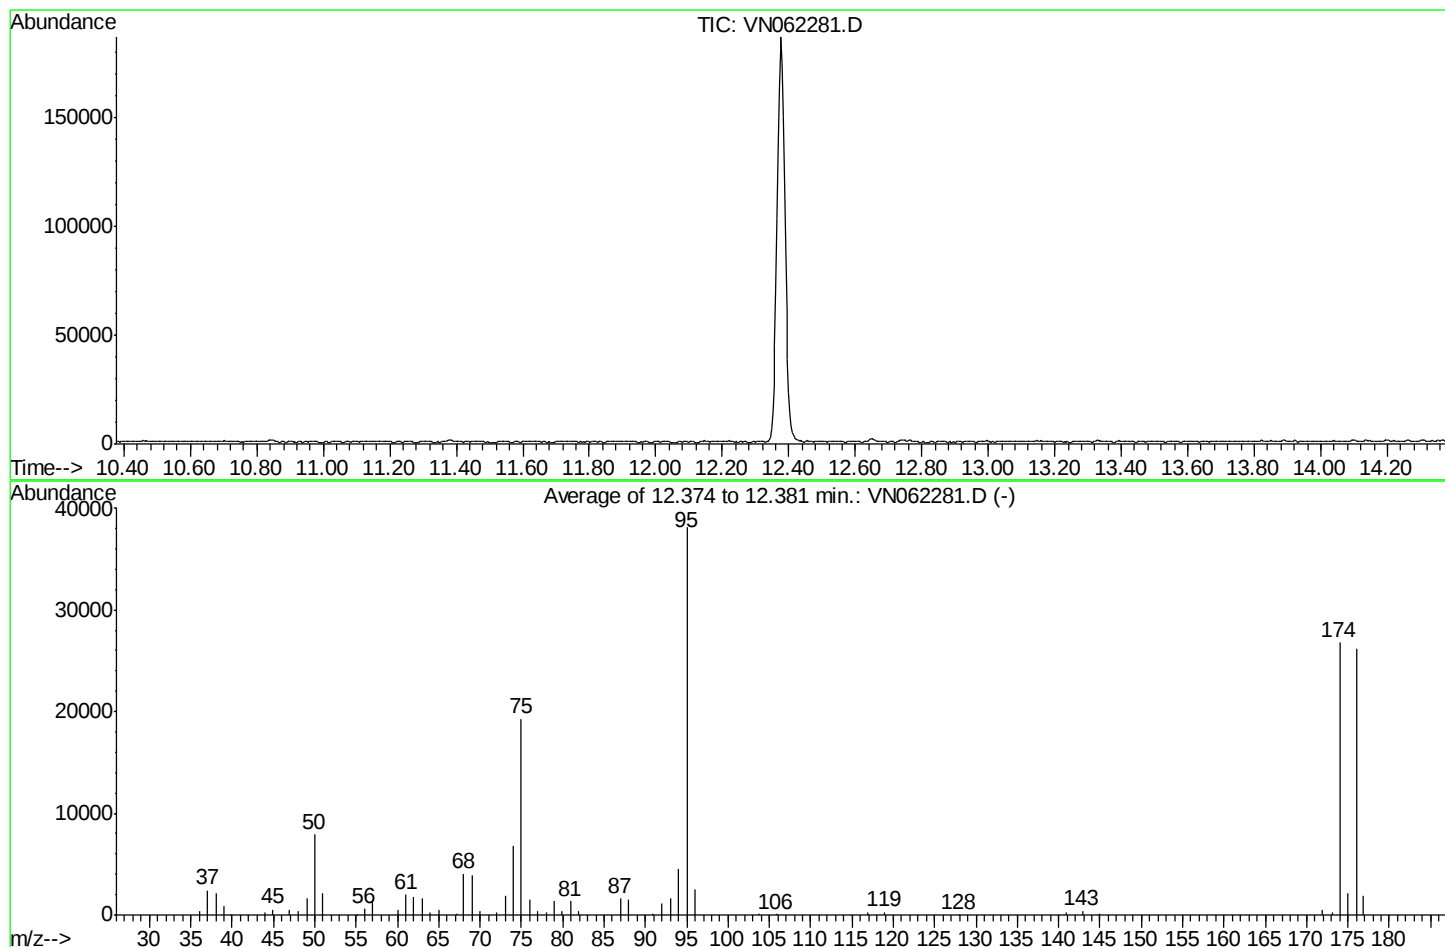

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3283

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	7893	PASS
75	95	30	60	50.6	19298	PASS
95	95	100	100	100.0	38117	PASS
96	95	5	9	6.5	2461	PASS
173	174	0.00	2	1.0	270	PASS
174	95	50	100	70.3	26784	PASS
175	174	5	9	8.2	2202	PASS
176	174	95	101	97.7	26178	PASS
177	176	5	9	7.0	1836	PASS