
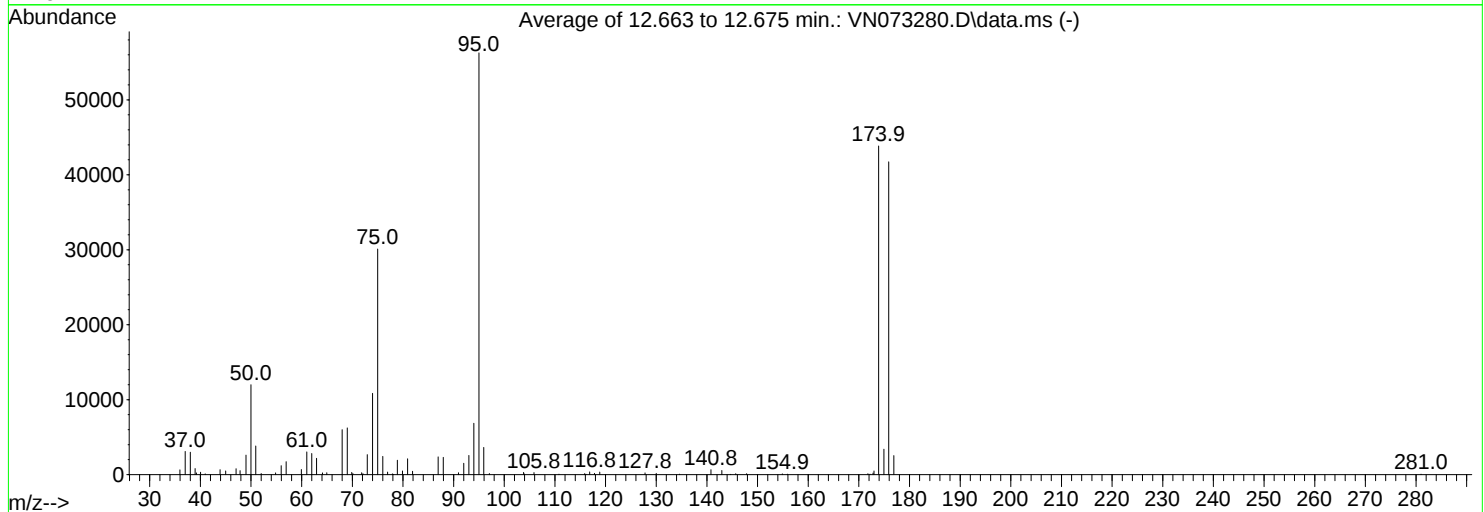


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070122\
Data File : VN073280.D
Acq On : 01 Jul 2022 07:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 01:54:03 2022

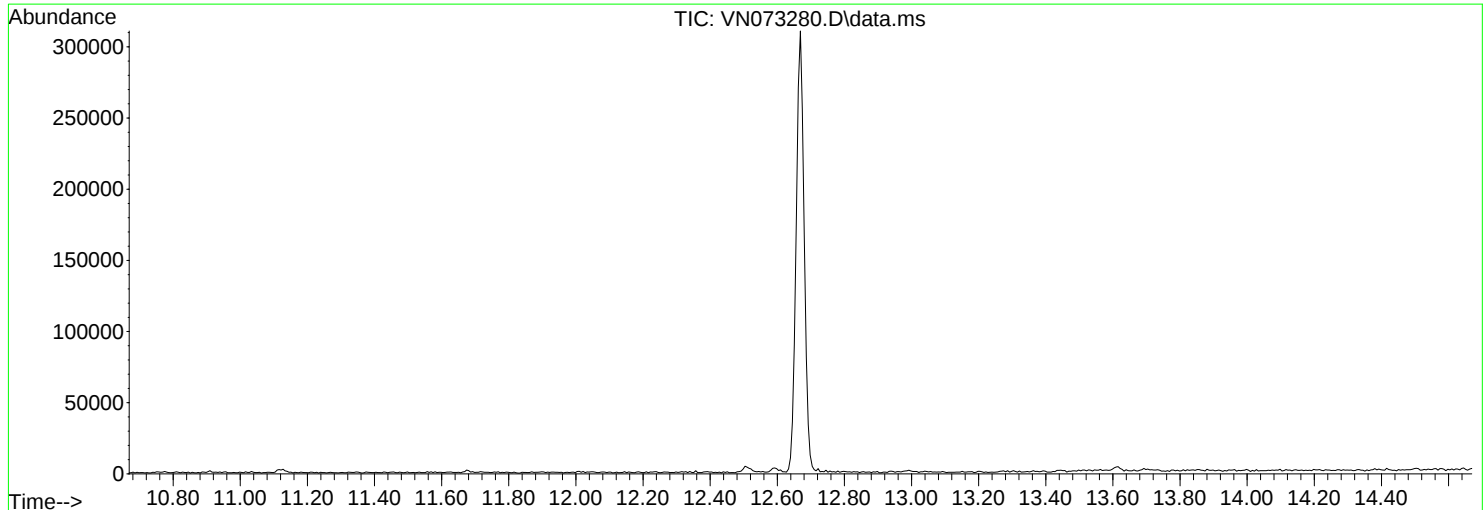

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	11992	PASS
75	95	30	60	53.5	30101	PASS
95	95	100	100	100.0	56269	PASS
96	95	5	9	6.4	3627	PASS
173	174	0.00	2	1.1	483	PASS
174	95	50	100	77.9	43845	PASS
175	174	5	9	7.7	3395	PASS
176	174	95	101	95.2	41731	PASS
177	176	5	9	6.1	2548	PASS