


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070124\
Data File : VN082753.D
Acq On : 01 Jul 2024 09:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062724W.M
Title : SW846 8260
Last Update : Fri Jun 28 06:02:21 2024

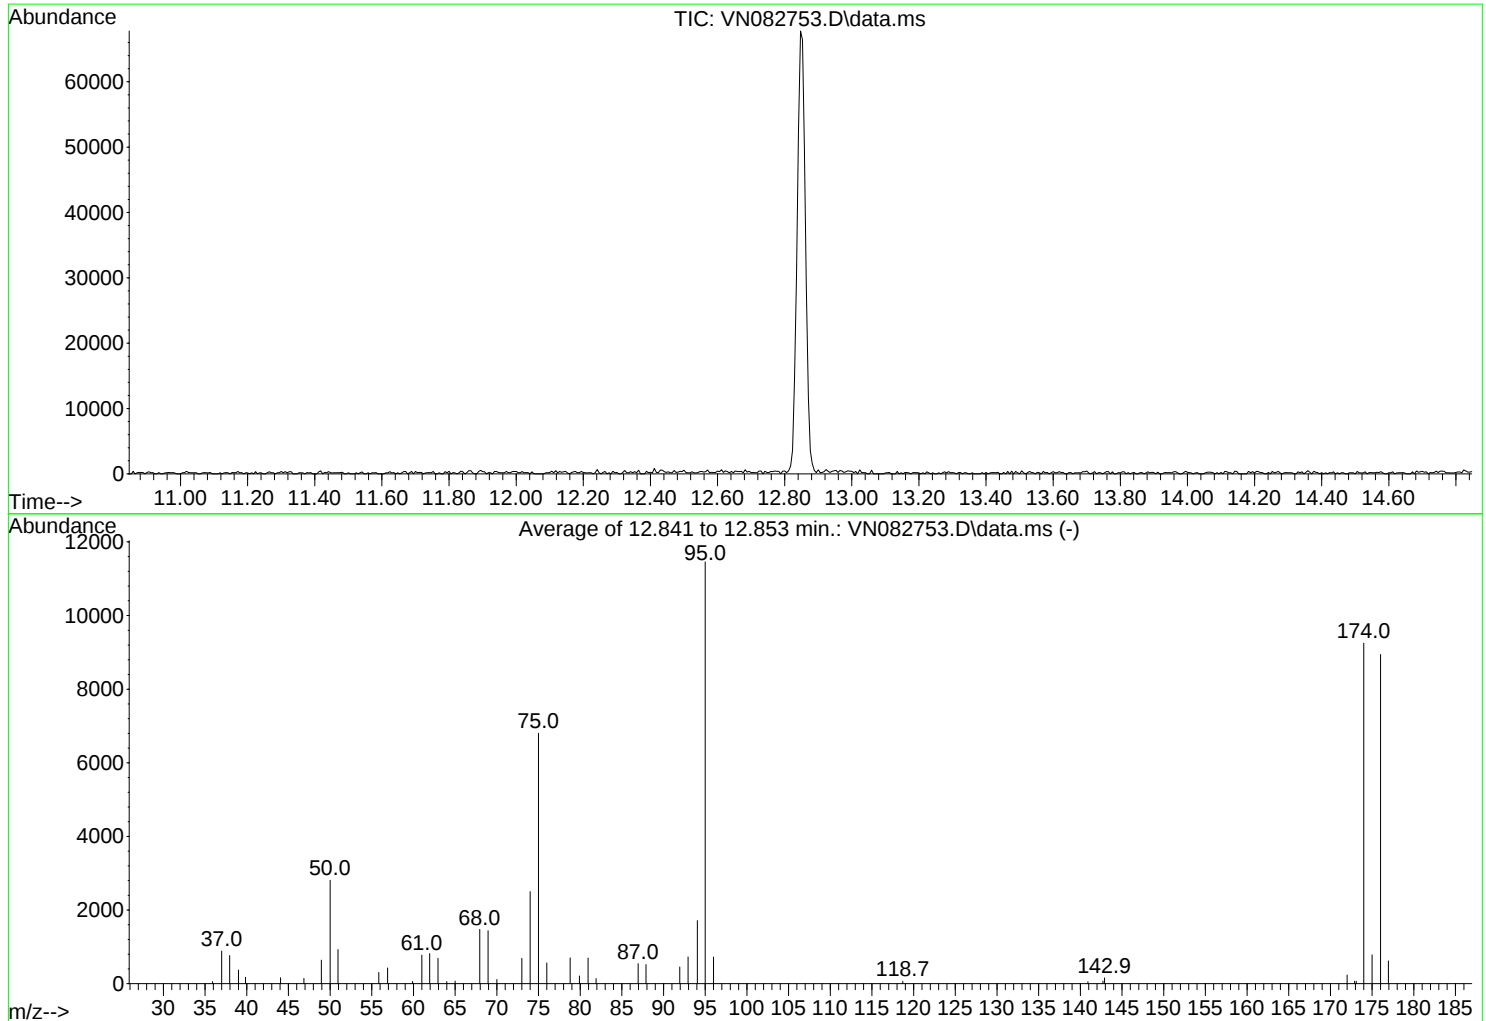

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	2809	PASS
75	95	30	60	59.4	6803	PASS
95	95	100	100	100.0	11459	PASS
96	95	5	9	6.3	720	PASS
173	174	0.00	2	0.7	67	PASS
174	95	50	100	80.7	9251	PASS
175	174	5	9	8.5	782	PASS
176	174	95	101	96.6	8941	PASS
177	176	5	9	6.9	616	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	57	56.90	427	74.00	2498	94.05	1711
37.00	886	59.90	62	75.00	6803	95.00	1145
37.95	765	61.00	773	76.00	560	96.00	72
39.00	370	61.95	816	78.80	699	118.70	6
39.85	174	62.95	685	79.90	209	140.90	52
44.05	162	64.00	57	80.95	695	142.70	69
46.85	142	65.00	68	81.90	141	142.90	156
48.95	641	67.95	1472	86.95	543	172.00	237
50.00	2809	68.95	1440	87.90	517	172.90	65
50.95	926	70.00	111	91.95	453	173.10	67
55.85	306	73.00	687	92.95	726	174.00	9251

Average of 12.841 to 12.853 min.: VN082753.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.00	782						
176.00	8941						
176.95	616						

Instrument :

MSVOA_N

ClientSampleId :

BFB