
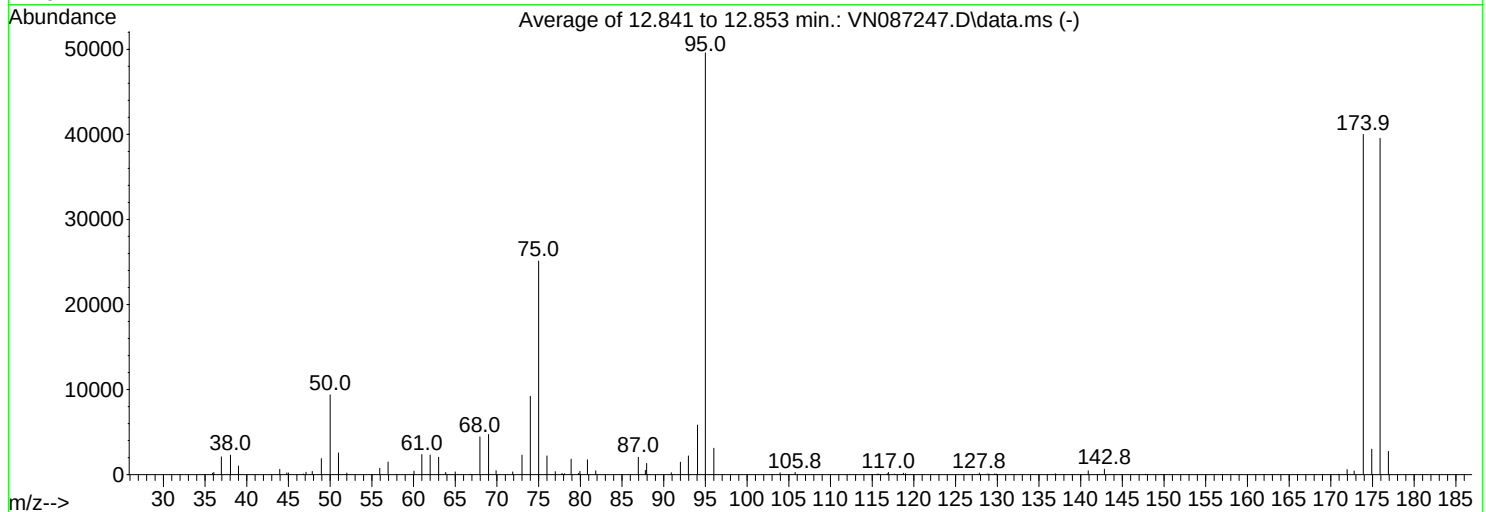


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070125\
Data File : VN087247.D
Acq On : 01 Jul 2025 08:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
Title : SW846 8260
Last Update : Tue Jul 01 03:15:00 2025

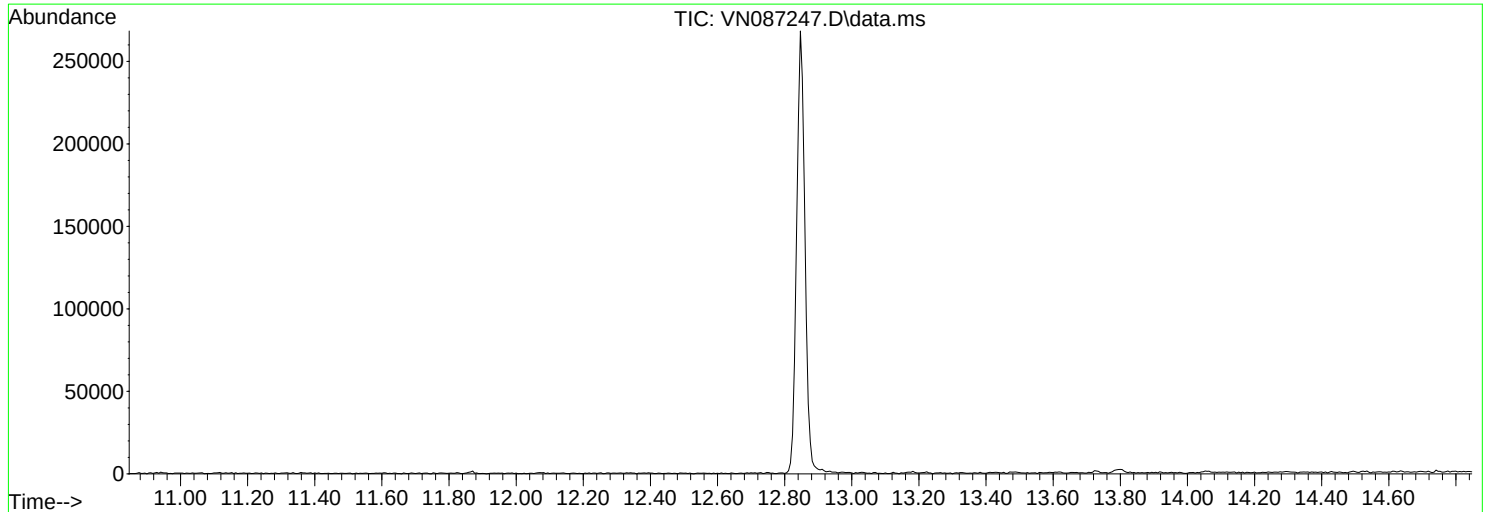

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	9389	PASS
75	95	30	60	50.6	25101	PASS
95	95	100	100	100.0	49581	PASS
96	95	5	9	6.3	3105	PASS
173	174	0.00	2	1.1	425	PASS
174	95	50	100	80.6	39981	PASS
175	174	5	9	7.5	2999	PASS
176	174	95	101	98.9	39528	PASS
177	176	5	9	6.9	2725	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	179	48.95	1890	63.85	263	77.00	351
36.05	265	50.00	9389	65.00	329	77.80	161
36.95	2097	51.00	2551	66.80	63	78.10	111
38.05	2293	52.00	191	67.95	4430	78.90	182
39.00	1010	55.95	763	69.00	4722	79.80	151
43.95	612	56.95	1482	69.90	464	79.95	391
44.80	206	57.90	53	71.90	312	80.85	1755
45.00	200	60.05	414	73.00	2303	81.85	460
46.80	69	61.00	2370	74.00	9212	86.95	2059
47.10	285	62.00	2323	75.00	25101	87.80	501
47.85	383	63.00	2050	76.00	2194	87.95	1319

Average of 12.841 to 12.853 min.: VN087247.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	224	116.95	260	142.85	638		
92.00	1466	117.70	70	147.80	59		
92.95	2200	118.75	169	170.90	52		
94.05	5829	119.00	118	171.95	596		
95.00	49581	127.85	184	172.80	425		
96.00	3105	128.80	73	173.90	39981		
103.95	231	129.00	71	174.90	2999		
105.75	262	129.70	88	175.90	39528		
115.60	76	129.90	68	176.90	2725		
115.80	75	136.95	114				
116.80	113	140.90	447				

Instrument :

MSVOA_N

ClientSampleId :

BFB