


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN070218\
 Data File : VN049660.D
 Acq On : 2 Jul 2018 9:42
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062918W.M
 Title : SW846 8260
 Last Update : Sat Jun 30 00:55:30 2018

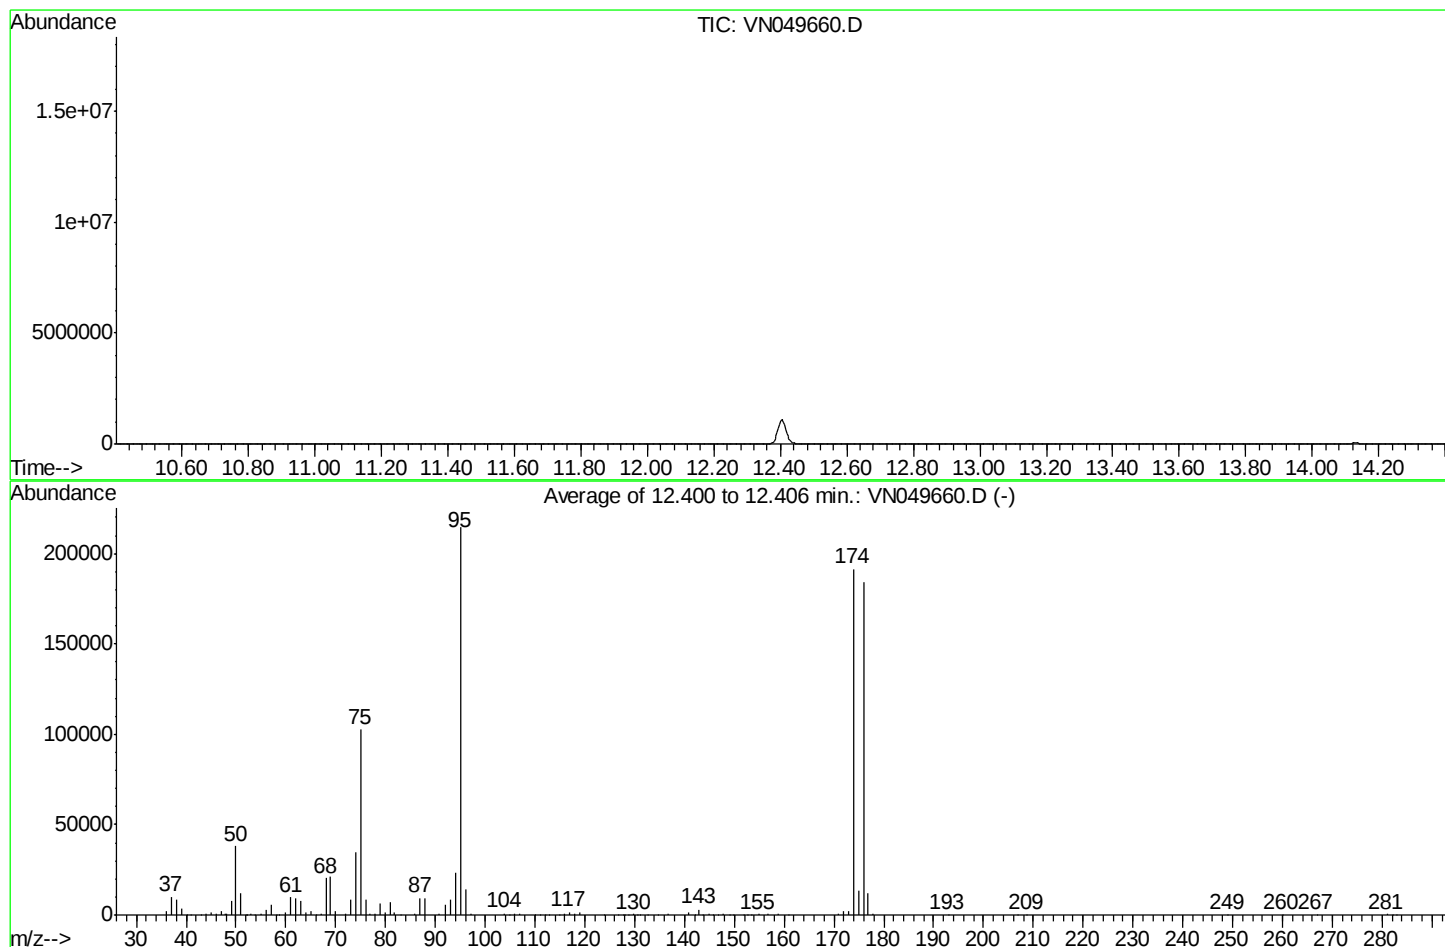

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3347

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	38016	PASS
75	95	30	60	47.8	102472	PASS
95	95	100	100	100.0	214506	PASS
96	95	5	9	6.7	14362	PASS
173	174	0.00	2	1.3	2474	PASS
174	95	50	100	89.2	191296	PASS
175	174	5	9	6.9	13133	PASS
176	174	95	101	96.2	184042	PASS
177	176	5	9	6.6	12104	PASS