

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070220\
 Data File : VN062345.D
 Acq On : 2 Jul 2020 20:06
 Operator : JC/MD
 Sample : PB129917ZHE#03
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 03 00:36:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	125994	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	260824	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	255504	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	86817	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	105627	59.74	ug/l	0.00
Spiked Amount			Recovery	=	119.48%	
35) Dibromofluoromethane	7.55	113	83272	49.76	ug/l	0.00
Spiked Amount			Recovery	=	99.52%	
50) Toluene-d8	10.06	98	343760	51.39	ug/l	0.00
Spiked Amount			Recovery	=	102.78%	
62) 4-Bromofluorobenzene	12.38	95	107636	47.63	ug/l	0.00
Spiked Amount			Recovery	=	95.26%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.03	50	160	Below Cal	#	41
11) Tert butyl alcohol	4.68	59	292	1.150	ug/l #	72
16) Acetone	3.78	43	8656	11.736	ug/l	99
18) Methyl Acetate	4.29	43	2460	1.750	ug/l	95
20) Methylene Chloride	4.50	84	5757	3.345	ug/l	98
25) 2-Butanone	6.80	43	1812	2.097	ug/l	93
29) Tetrahydrofuran	7.17	42	573	1.012	ug/l #	28
31) Cyclohexane	7.62	56	3498	1.432	ug/l #	2
36) 1,1-Dichloropropene	7.62	75	11756	4.484	ug/l #	47
37) Ethyl Acetate	6.80	43	1812	0.835	ug/l #	66
38) Carbon Tetrachloride	7.63	117	13166	5.327	ug/l #	14
43) Isopropyl Acetate	8.13	43	47573	13.443	ug/l	98
45) 1,2-Dichloropropane	9.24	63	1103	0.560	ug/l #	43
48) Methyl methacrylate	9.14	41	2915	1.837	ug/l #	6
51) 4-Methyl-2-Pentanone	9.95	43	3841	1.858	ug/l #	85
54) cis-1,3-Dichloropropene	9.88	75	22953	7.261	ug/l #	67
56) Ethyl methacrylate	10.52	69	1045	0.409	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	4441	1.346	ug/l #	42
59) 2-Hexanone	10.74	43	56857	38.082	ug/l #	49
74) N-amyl acetate	12.01	43	1213	3.801	ug/l #	38
76) 1,2,3-Trichloropropane	12.38	75	57037	27.908	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	2178	0.400	ug/l	99
81) trans-1,4-Dichloro-2-buten	12.38	75	57037	81.502	ug/l #	13
95) Naphthalene	15.11	128	528	4.112	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN070220\
Data File : VN062345.D
Acq On : 2 Jul 2020 20:06
Operator : JC/MD
Sample : PB129917ZHE#03
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :

Quant Time: Jul 03 00:36:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 24 15:33:00 2020
Response via : Initial Calibration

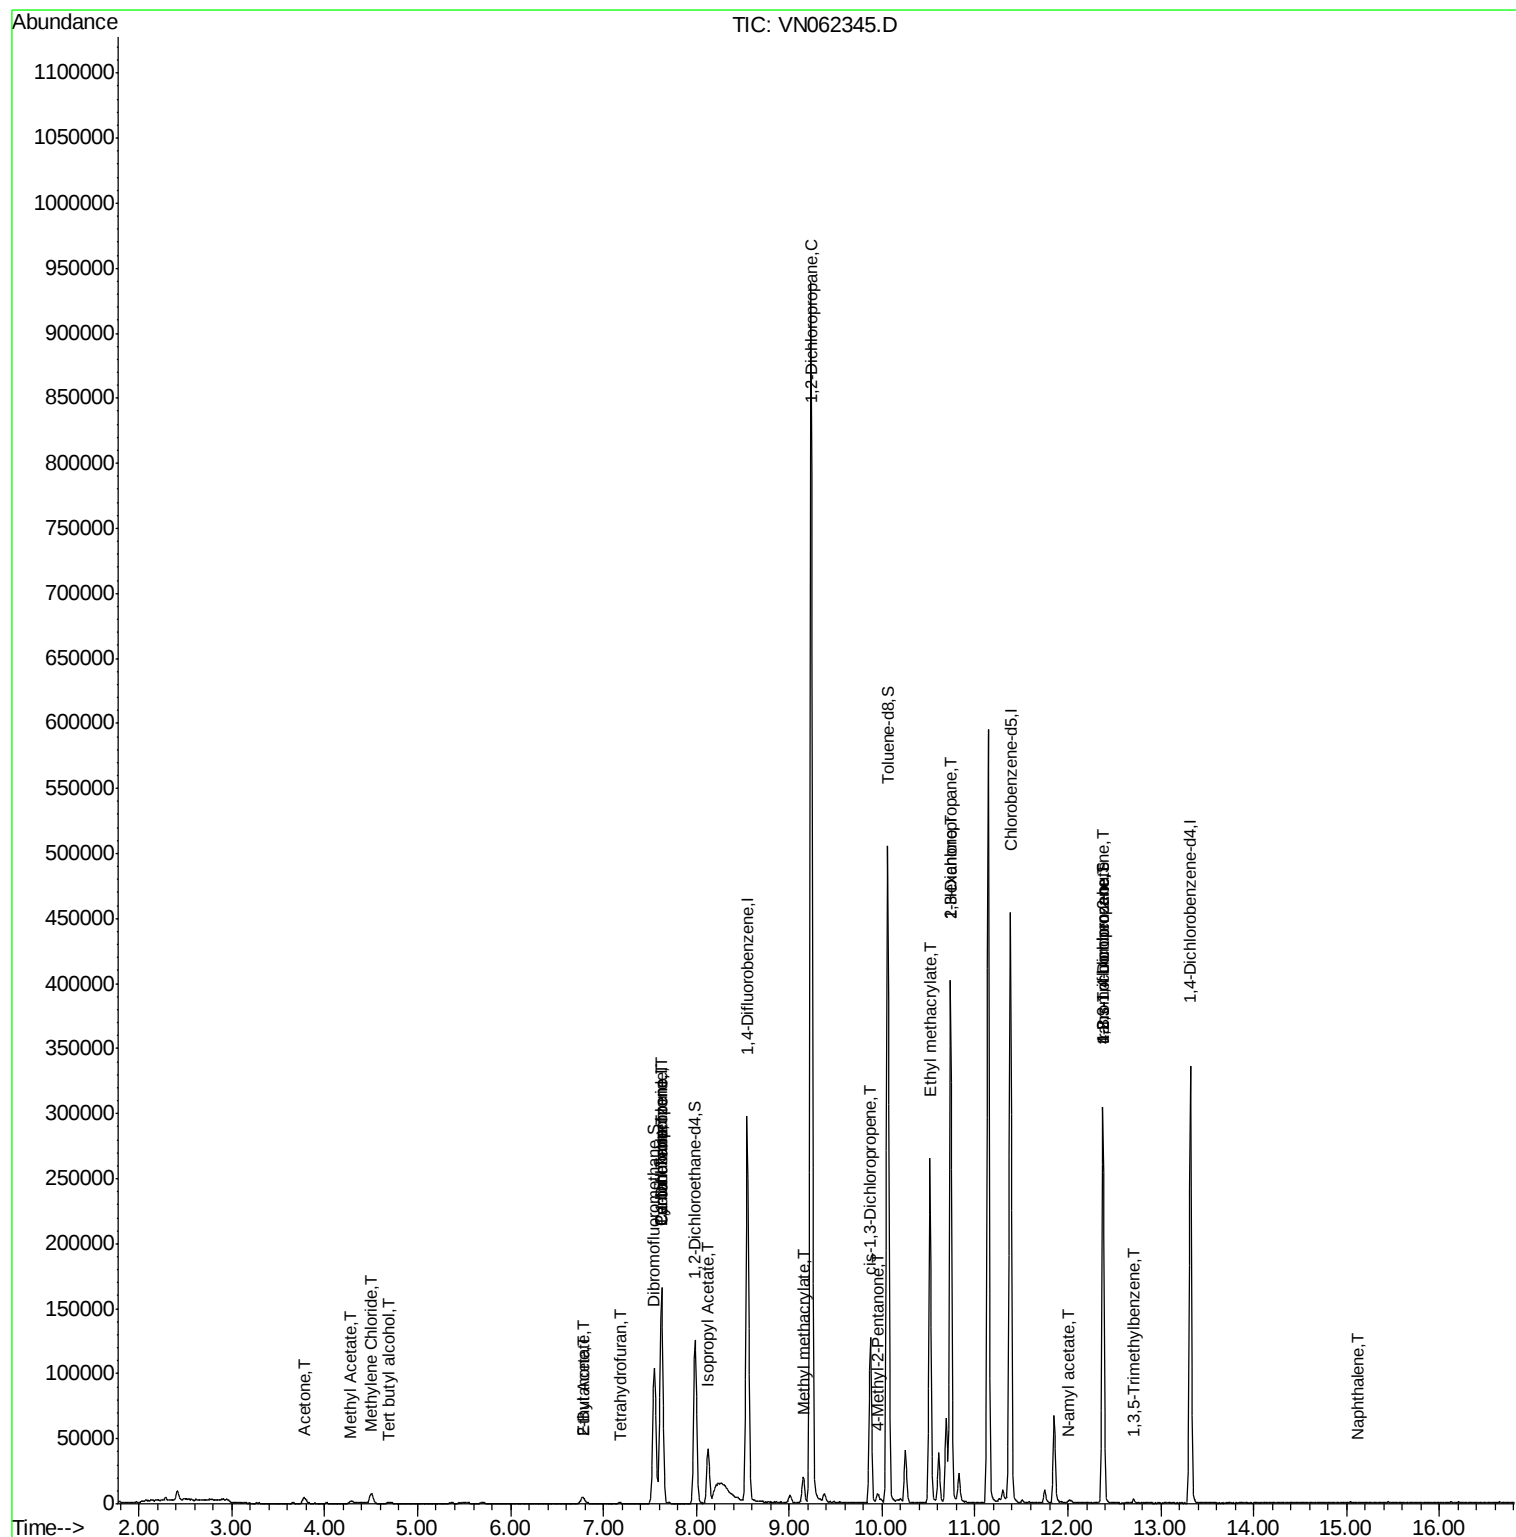

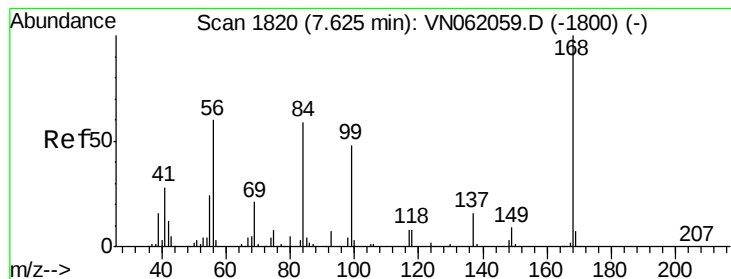

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.00 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06

Instrument :

MSVOA_N


ClientSampled :

Tot Ion:168 Resp: 125994

Ion Ratio Lower Upper

168 100

99 61.7 45.8 68.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

60000

50000

40000

30000

20000

10000



0

7.50

7.60

7.70

Time-->

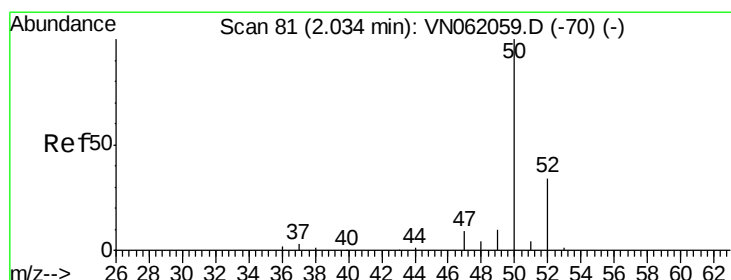

#3

Chloromethane

Concen: Below Cal

RT: 2.03 min Scan# 81

Delta R.T. 0.00 min

Lab File: VN062345.D


Acq: 2 Jul 2020 20:06

Tgt Ion: 50 Resp: 160

Ion Ratio Lower Upper

50 100

52 0.0 27.0 40.6#

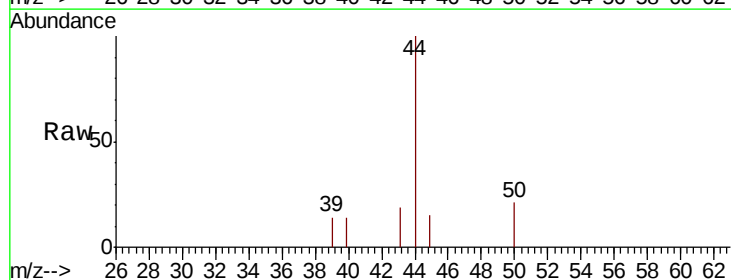

Abundance Ion 49.90 (49.60 to 50.60): VN

Ion 51.90 (51.60 to 52.60): VN

2.03

250

200

150

100

50

0

2.01


2.02


2.03

2.04

2.05

Time-->







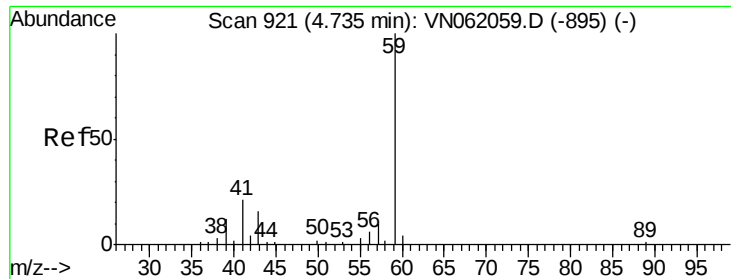

#11
Tert butyl alcohol
Concen: 1.150 ug/l
RT: 4.68 min Scan# 904
Delta R.T. -0.05 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 59 Resp: 292
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

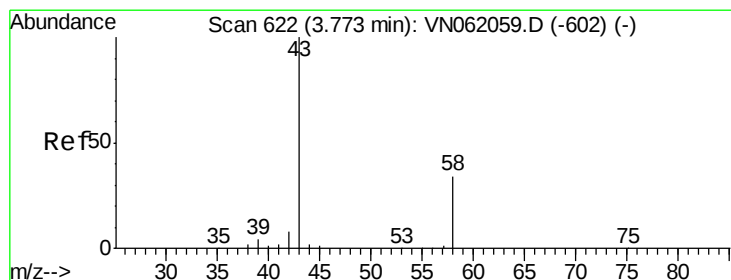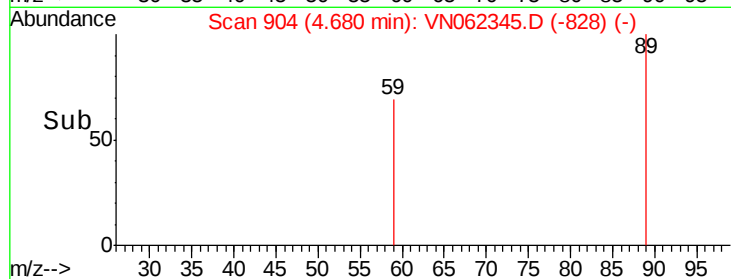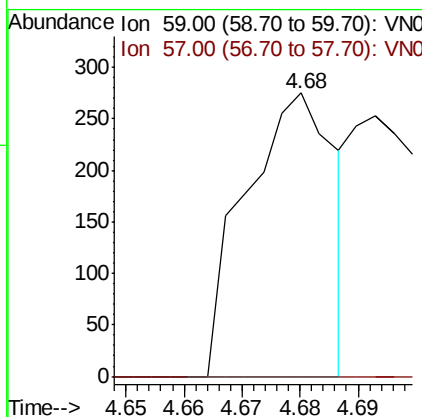

#16
Acetone
Concen: 11.736 ug/l
RT: 3.78 min Scan# 624
Delta R.T. 0.01 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06

Tgt Ion: 43 Resp: 8656
Ion Ratio Lower Upper
43 100
58 34.0 27.5 41.3


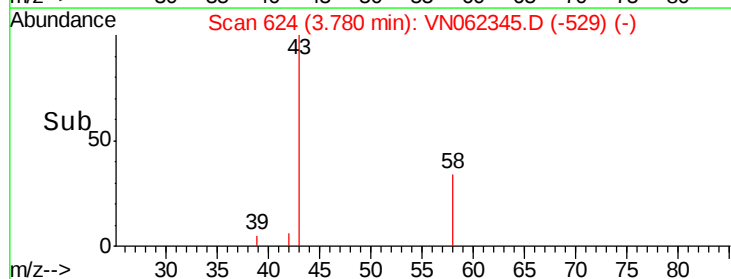
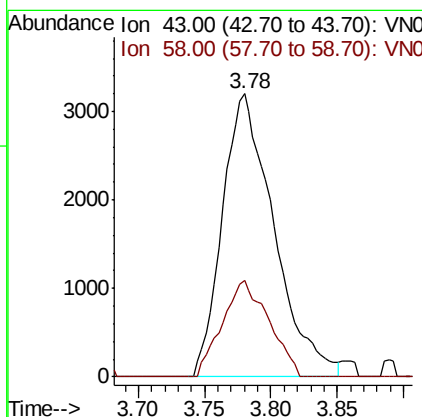
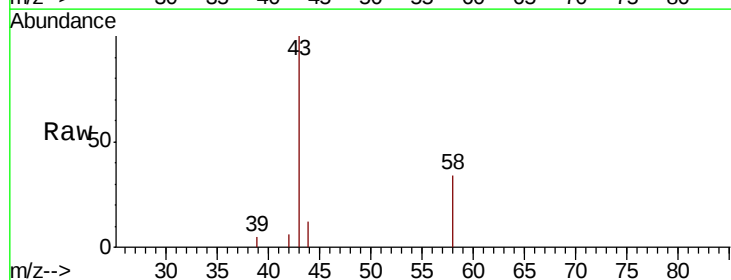


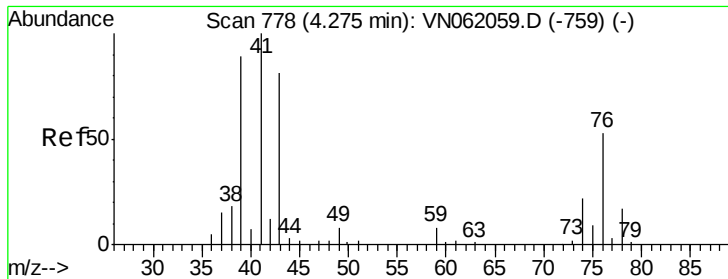

#18
Methyl Acetate
Concen: 1.750 ug/l
RT: 4.29 min Scan# 783
Delta R.T. 0.02 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 43 Resp: 2460
Ion Ratio Lower Upper
43 100
74 26.0 22.9 34.3

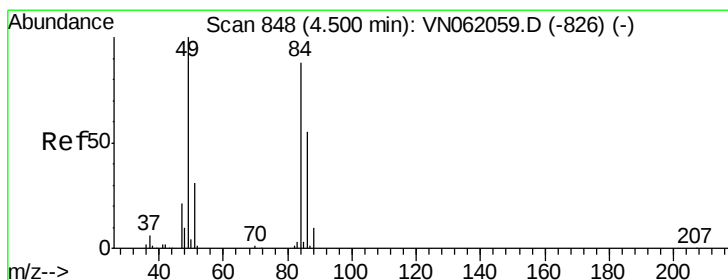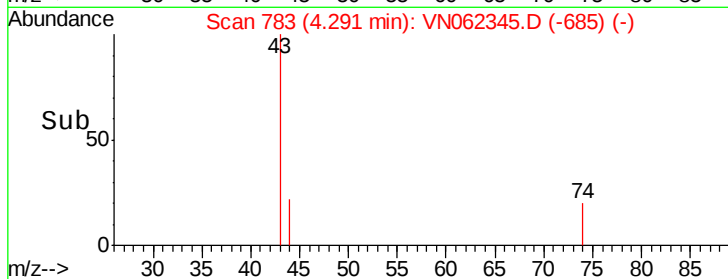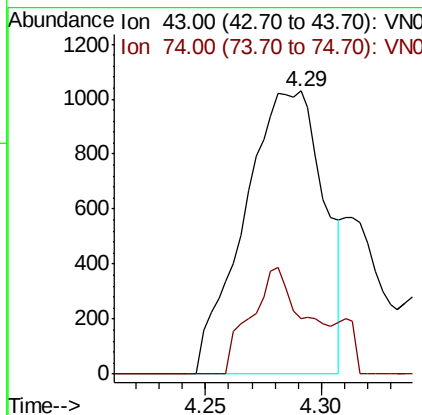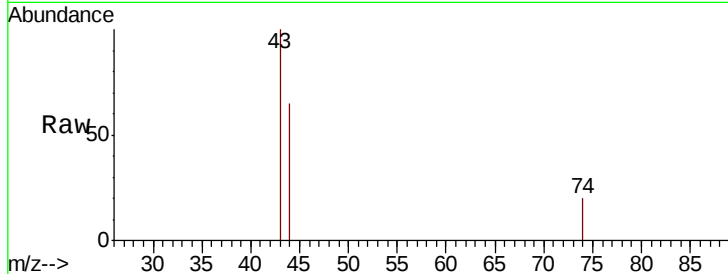

#20
Methylene Chloride
Concen: 3.345 ug/l
RT: 4.50 min Scan# 848
Delta R.T. 0.00 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06

Tgt Ion: 84 Resp: 5757
Ion Ratio Lower Upper
84 100
49 110.5 90.6 136.0
51 33.2 27.8 41.8
86 61.5 50.1 75.1

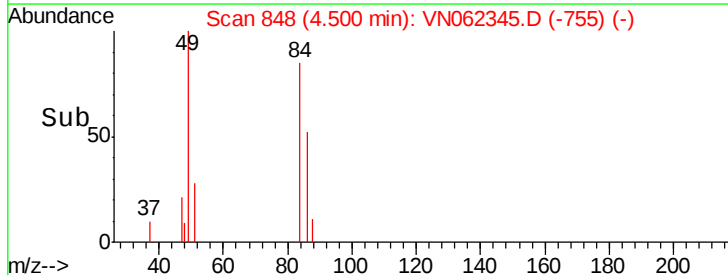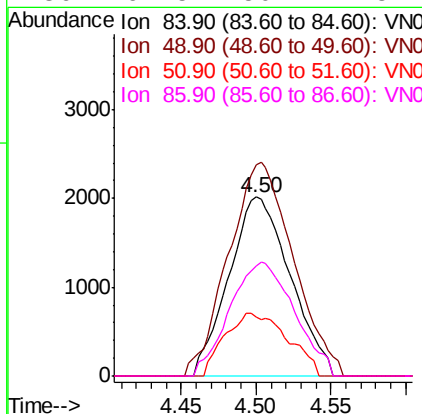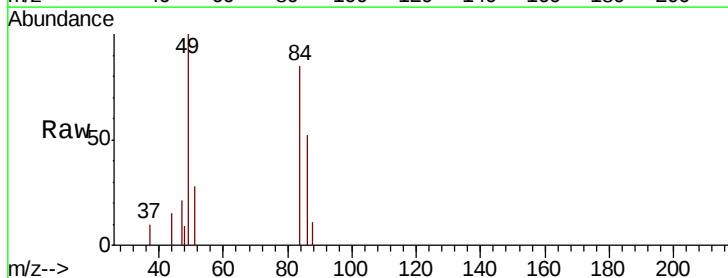



#25

2-Butanone

Concen: 2.097 ug/l

RT: 6.80 min Scan# 1562

Delta R.T. 0.01 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06





Instrument :
MSVOA_N
ClientSampled :

Tot Ion: 43 Resp: 1812

Ion Ratio Lower Upper

43 100

72 27.1 24.8 37.2

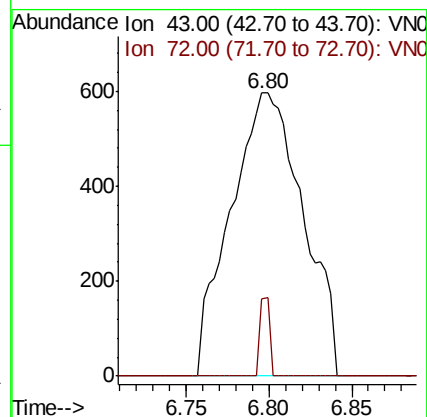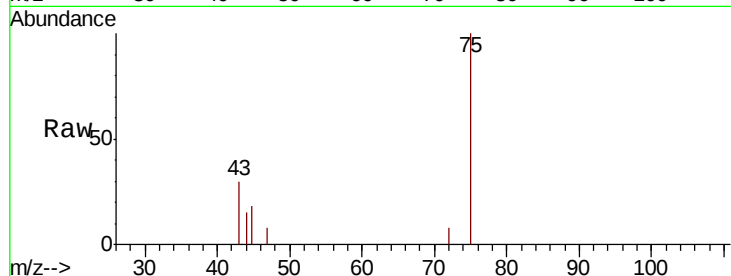

#29

Tetrahydrofuran

Concen: 1.012 ug/l

RT: 7.17 min Scan# 1678

Delta R.T. 0.00 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06




Tgt Ion: 42 Resp: 573


Ion Ratio Lower Upper

42 100

72 0.0 41.1 61.7#

71 0.0 38.2 57.4#

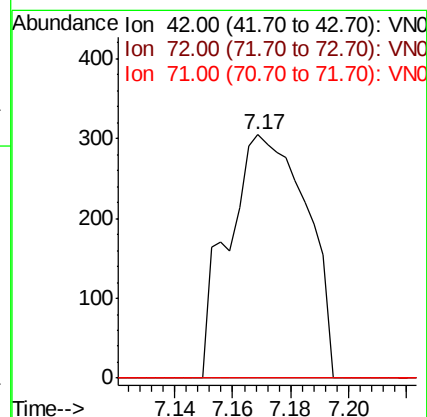

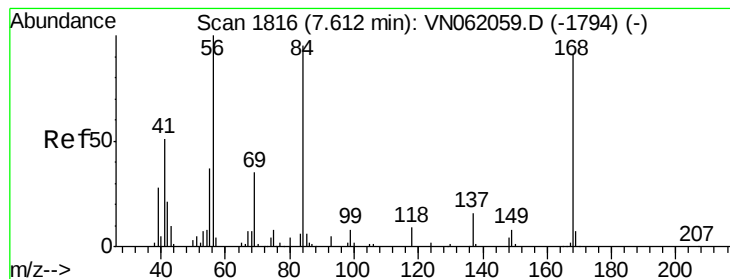

#31

Cyclohexane

Concen: 1.432 ug/l

RT: 7.62 min Scan# 1816

Delta R.T. 0.01 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06

Instrument :

MSVOA_N

ClientSampled :


Tot Ion: 56 Resp: 3498

Ion Ratio Lower Upper

56 100

69 156.9 28.0 42.0#




84 150.9 76.1 114.1#

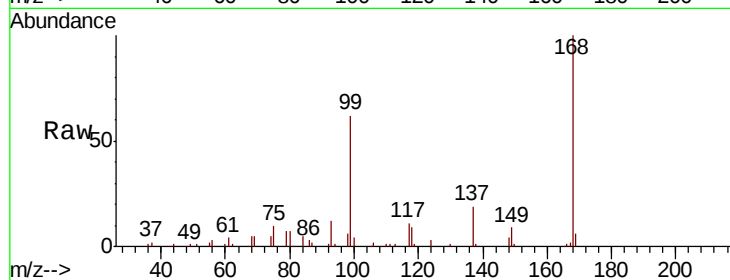

Abundance Ion 56.00 (55.70 to 56.70): VN062345.D (-1794) (-)

Ion 69.00 (68.70 to 69.70): VN062345.D (-1794) (-)

Ion 84.00 (83.70 to 84.70): VN062345.D (-1794) (-)

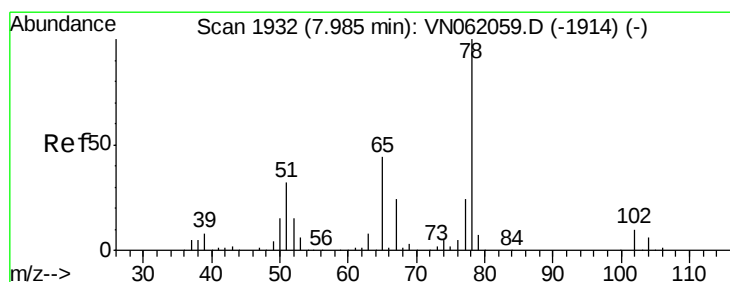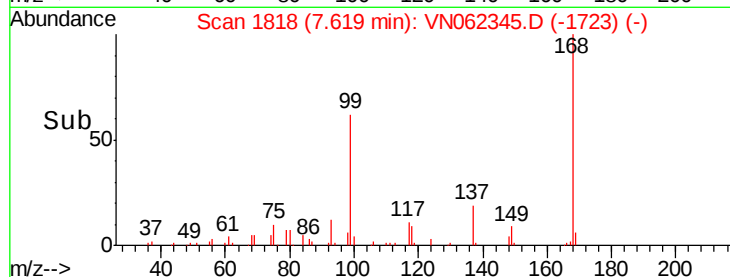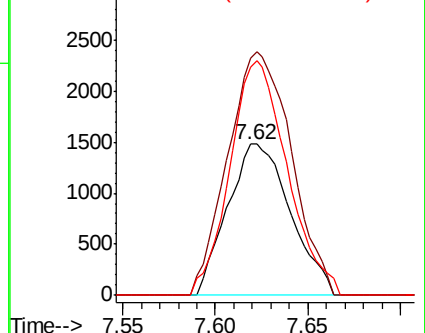

#33

1,2-Dichloroethane-d4

Concen: 59.740 ug/l

RT: 7.99 min Scan# 1932

Delta R.T. 0.00 min

Lab File: VN062345.D


Acq: 2 Jul 2020 20:06

Tgt Ion: 65 Resp: 105627

Ion Ratio Lower Upper



65 100


67 52.7 0.0 106.2

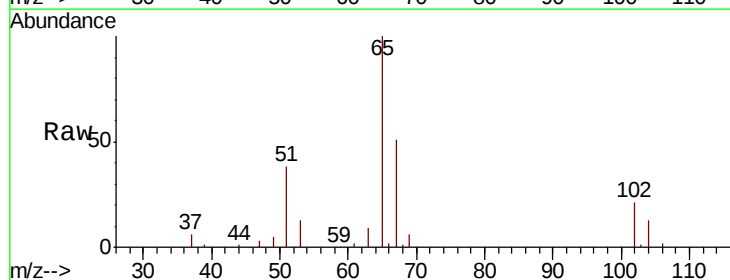

Abundance Ion 64.90 (64.60 to 65.60): VN062345.D (-1839) (-)

Ion 66.90 (66.60 to 67.60): VN062345.D (-1839) (-)

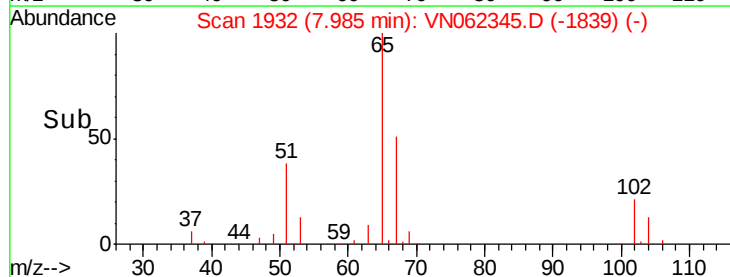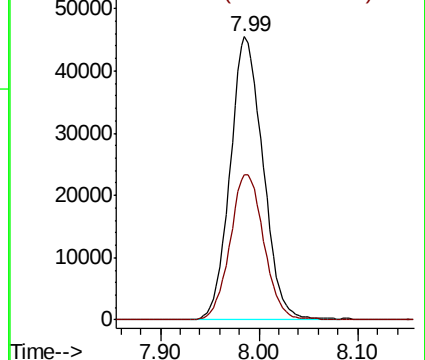

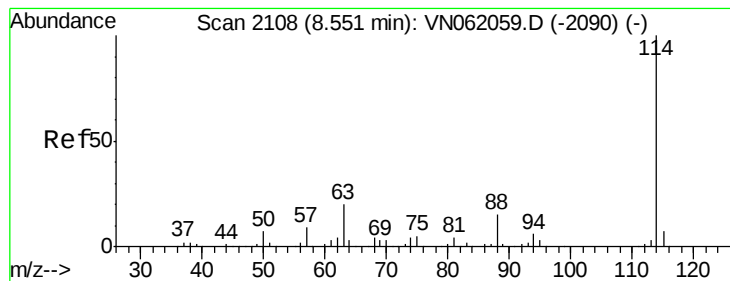

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2108

Delta R.T. 0.00 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:114 Resp: 260824

Ion Ratio Lower Upper

114 100

63 21.0 0.0 39.2




88 16.1 0.0 30.8

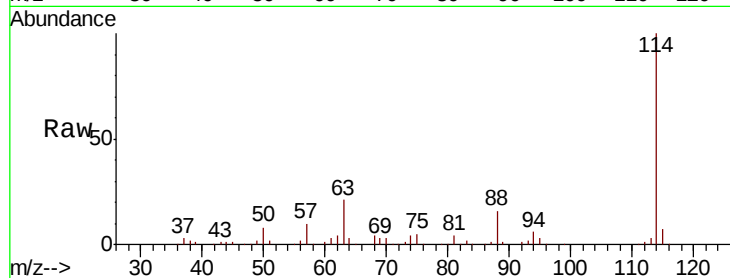

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

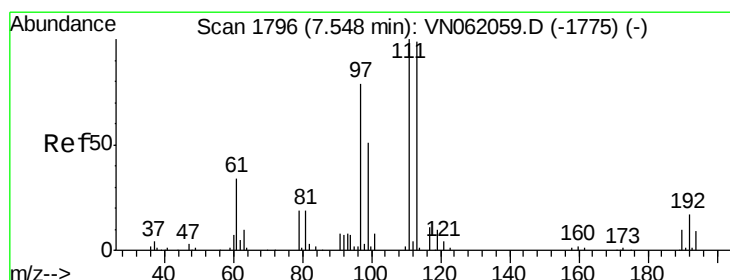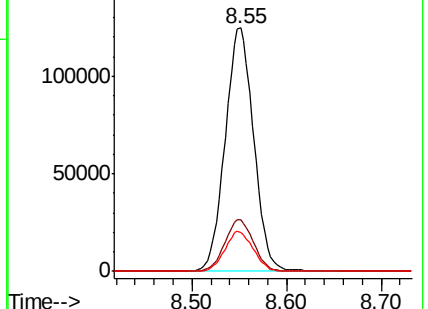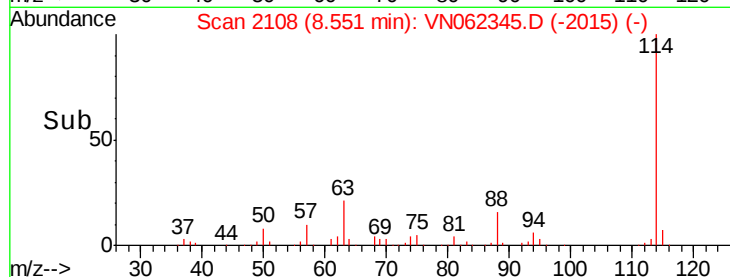

#35

Dibromofluoromethane

Concen: 49.765 ug/l

RT: 7.55 min Scan# 1796

Delta R.T. 0.00 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06


Tgt Ion:113 Resp: 83272

Ion Ratio Lower Upper

113 100

111 101.9 82.2 123.4



192 16.7 14.0 21.0

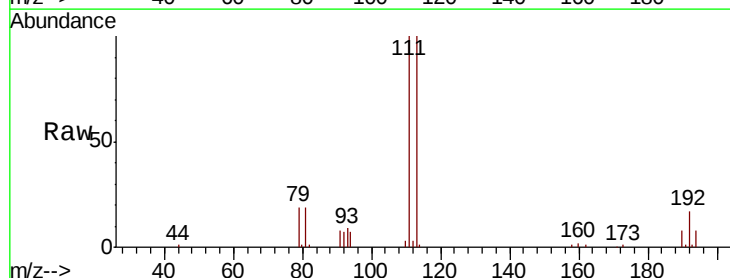


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

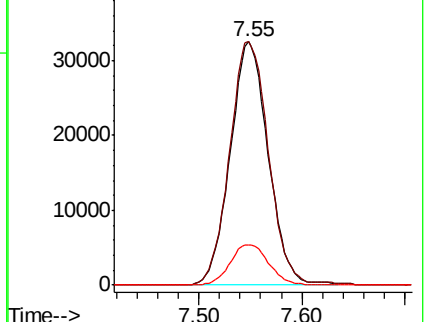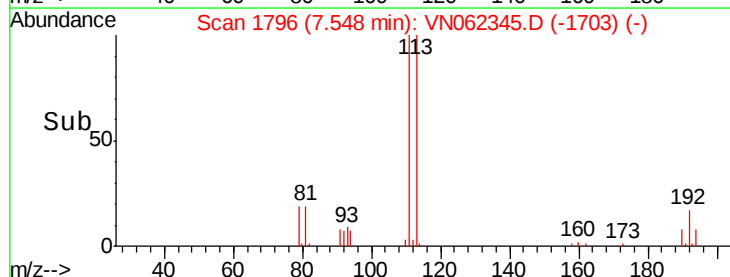

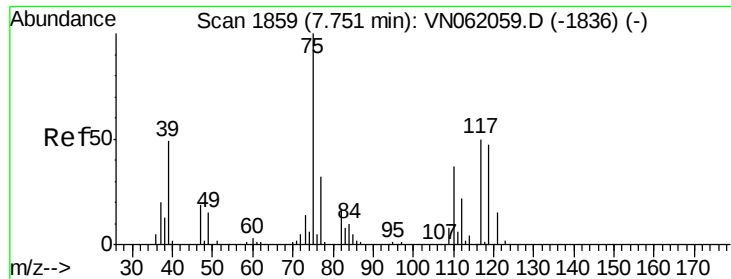

#36

1,1-Dichloropropene

Concen: 4.484 ug/l

RT: 7.62 min Scan# 1818

Delta R.T. -0.13 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06

Instrument :

MSVOA_N

ClientSampled :


Tot Ion: 75 Resp: 11756

Ion Ratio Lower Upper

75 100

110 7.0 17.9 53.8#




77 0.0 24.9 37.3#

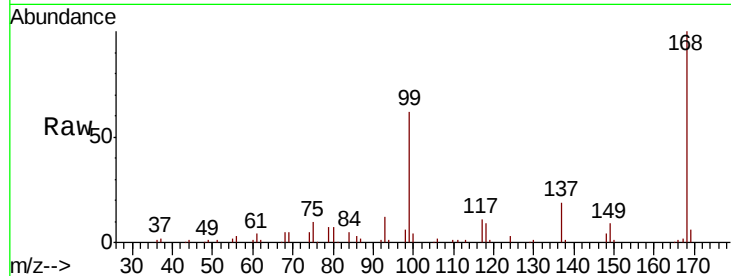

Abundance Ion 74.90 (74.60 to 75.60): VN062059.D (-1836) (-)

Ion 109.90 (109.60 to 110.60): VN062059.D (-1836) (-)

Ion 76.90 (76.60 to 77.60): VN062059.D (-1836) (-)

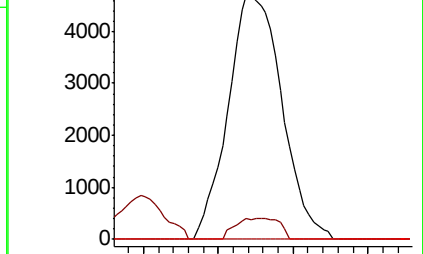

#37

Ethyl Acetate

Concen: 0.835 ug/l

RT: 6.80 min Scan# 1562

Delta R.T. -0.08 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06


Tgt Ion: 43 Resp: 1812

Ion Ratio Lower Upper

43 100

61 0.0 12.0 18.0#



70 0.0 9.6 14.4#




Abundance Ion 43.00 (42.70 to 43.70): VN062059.D (-1576) (-)

Ion 60.90 (60.60 to 61.60): VN062059.D (-1576) (-)

Ion 70.00 (69.70 to 70.70): VN062059.D (-1576) (-)

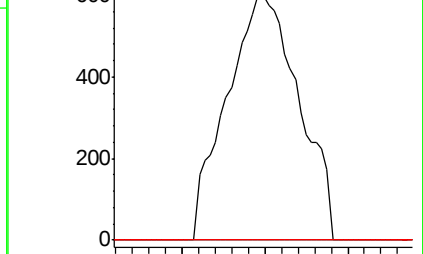


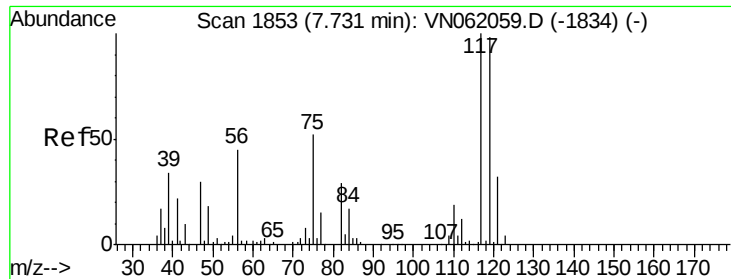




#38
Carbon Tetrachloride
Concen: 5.327 ug/l
RT: 7.63 min Scan# 1820
Delta R.T. -0.11 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06

Instrument :
MSVOA_N
ClientSampled :

Tot Ion:117 Resp: 13166
Ion Ratio Lower Upper
117 100
119 4.1 78.2 117.2#
121 0.0 25.8 38.6#

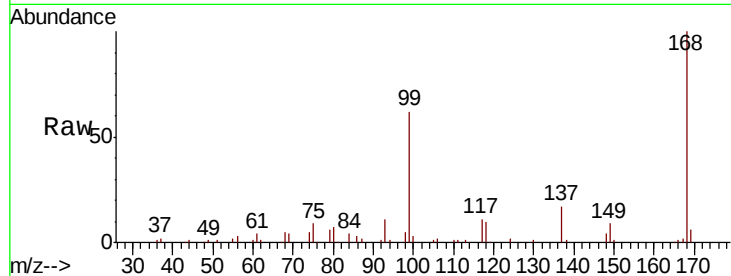


Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V


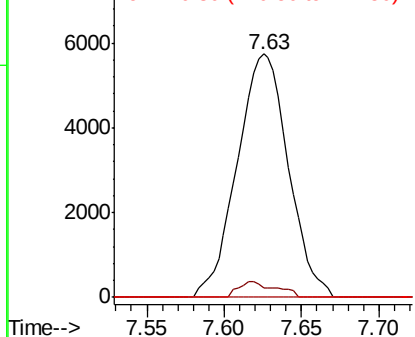



#43
Isopropyl Acetate
Concen: 13.443 ug/l
RT: 8.13 min Scan# 1976
Delta R.T. 0.00 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06

Tgt Ion: 43 Resp: 47573
Ion Ratio Lower Upper
43 100
61 21.1 17.2 25.8
87 14.1 12.1 18.1



Abundance Ion 43.00 (42.70 to 43.70): V
Ion 61.00 (60.70 to 61.70): V
Ion 87.00 (86.70 to 87.70): V




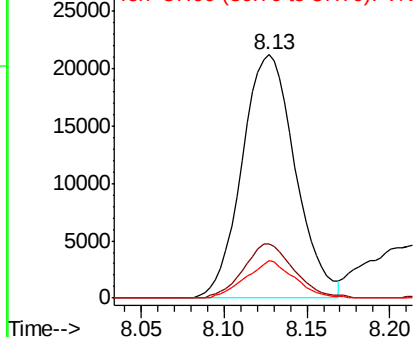


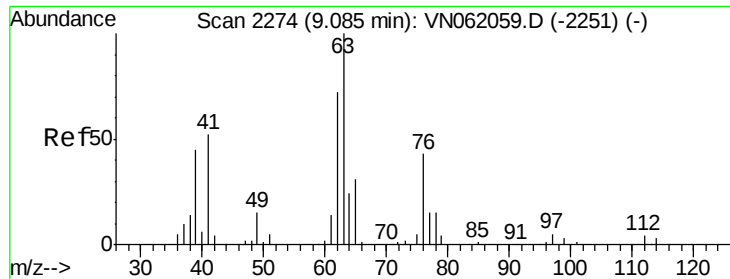

#45
 1,2-Dichloropropane
 Concen: 0.560 ug/l
 RT: 9.24 min Scan# 2323
 Delta R.T. 0.16 min
 Lab File: VN062345.D
 Acq: 2 Jul 2020 20:06




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion: 63 Resp: 1103
 Ion Ratio Lower Upper
 63 100
 65 0.0 25.0 37.4#

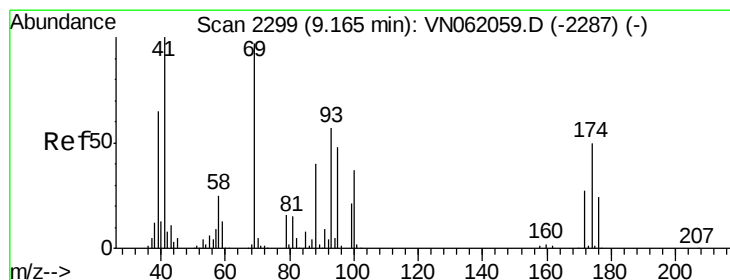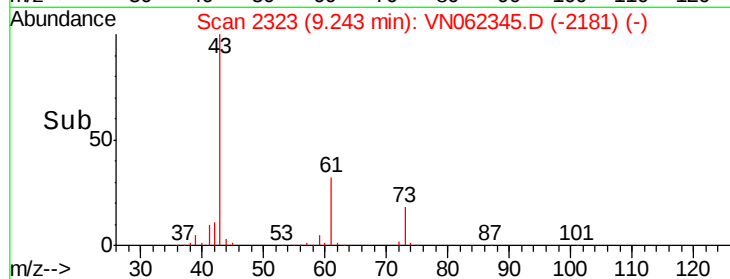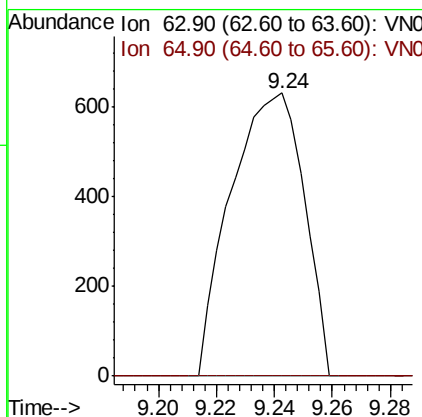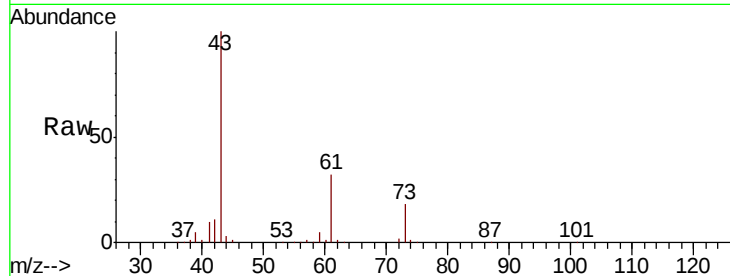

#48
 Methyl methacrylate
 Concen: 1.837 ug/l
 RT: 9.14 min Scan# 2292
 Delta R.T. -0.02 min
 Lab File: VN062345.D
 Acq: 2 Jul 2020 20:06

Tgt Ion: 41 Resp: 2915
 Ion Ratio Lower Upper
 41 100
 69 0.0 80.7 121.1#
 39 0.0 54.5 81.7#

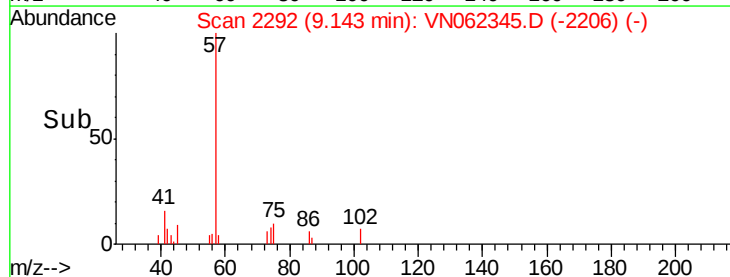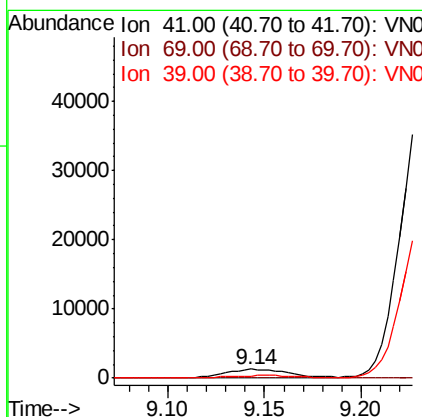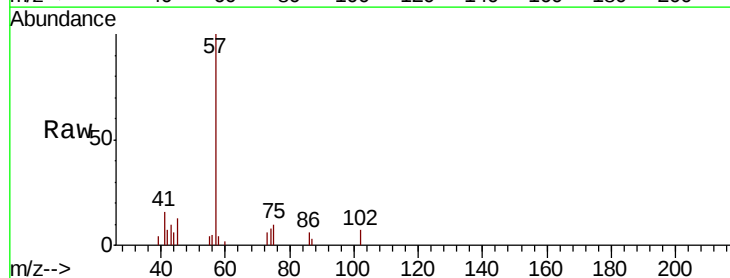



#50

Toluene-d8

Concen: 51.393 ug/l

RT: 10.06 min Scan# 2577

Delta R.T. 0.00 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 98 Resp: 343760

Ion Ratio Lower Upper


98 100

100 65.0 51.2 76.8


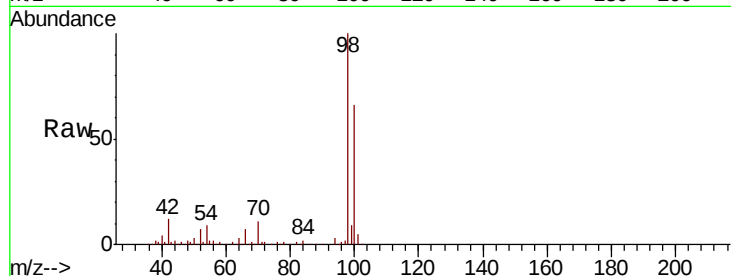


Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

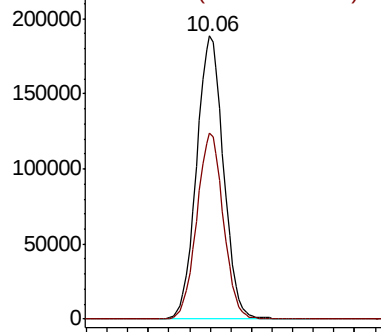

Time-->



#51

4-Methyl-2-Pentanone

Concen: 1.858 ug/l

RT: 9.95 min Scan# 2544

Delta R.T. 0.00 min

Lab File: VN062345.D


Acq: 2 Jul 2020 20:06

Tgt Ion: 43 Resp: 3841

Ion Ratio Lower Upper


43 100

58 52.0 34.2 51.2#





Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

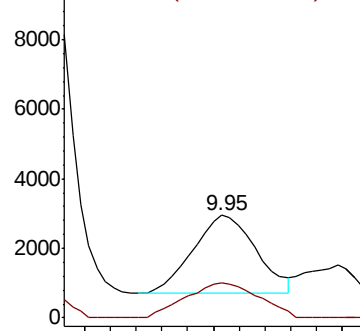

Time-->




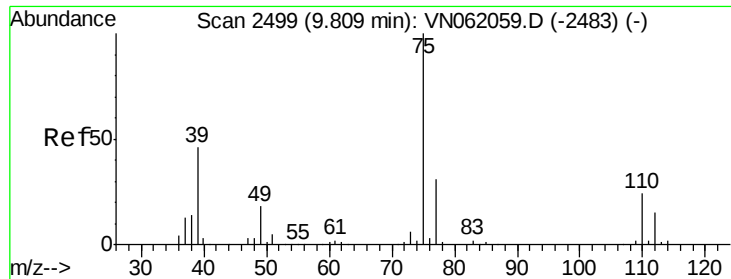




#54
 cis-1,3-Dichloropropene
 Concen: 7.261 ug/l
 RT: 9.88 min Scan# 2520
 Delta R.T. 0.07 min
 Lab File: VN062345.D
 Acq: 2 Jul 2020 20:06

Instrument :
 MSVOA_N
 ClientSampleId :

Tot Ion: 75 Resp: 22953
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.6#
 39 35.4 36.9 55.3#

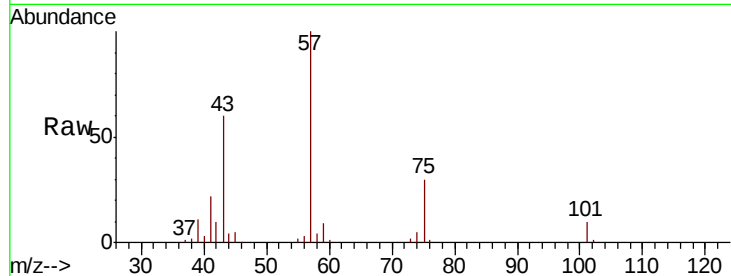


Abundance Ion 74.90 (74.60 to 75.60): VNO
 Ion 76.90 (76.60 to 77.60): VNO
 Ion 39.00 (38.70 to 39.70): VNO

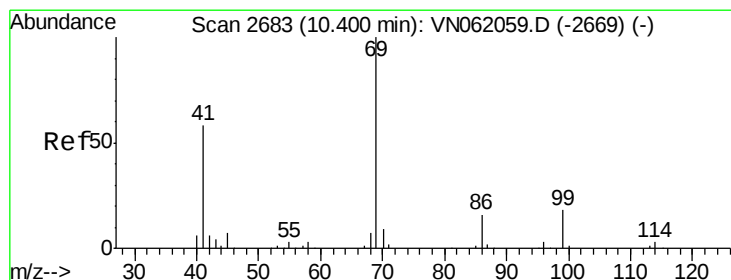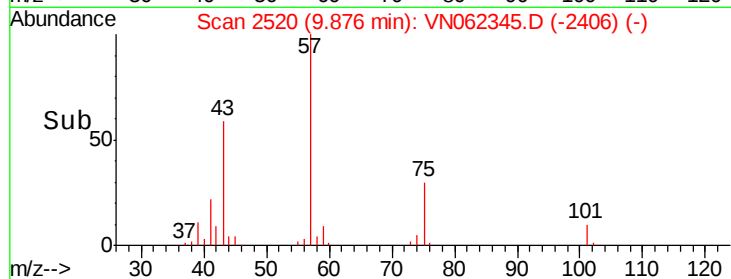
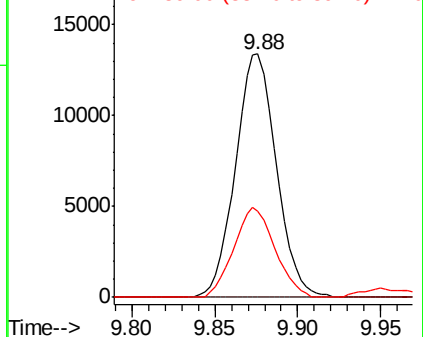



#56
 Ethyl methacrylate
 Concen: 0.409 ug/l
 RT: 10.52 min Scan# 2720
 Delta R.T. 0.12 min
 Lab File: VN062345.D
 Acq: 2 Jul 2020 20:06

Tgt Ion: 69 Resp: 1045
 Ion Ratio Lower Upper
 69 100
 41 4907.9 46.6 70.0#
 39 2296.3 31.0 46.4#



Abundance Ion 69.00 (68.70 to 69.70): VNO
 Ion 41.00 (40.70 to 41.70): VNO
 Ion 39.00 (38.70 to 39.70): VNO

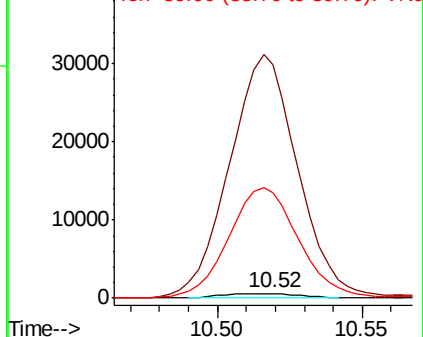

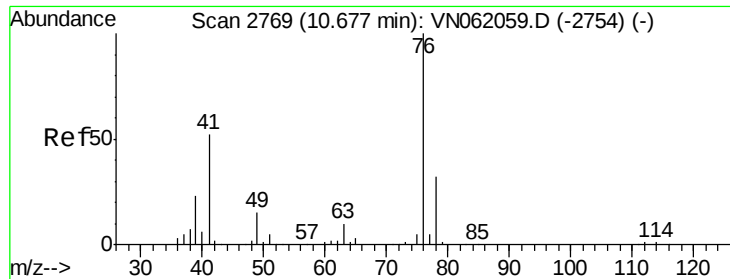

#57

1,3-Dichloropropane

Concen: 1.346 ug/l

RT: 10.74 min Scan# 2788

Delta R.T. 0.06 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 76 Resp: 4441

Ion Ratio Lower Upper




76 100

78 0.0 25.8 38.8#

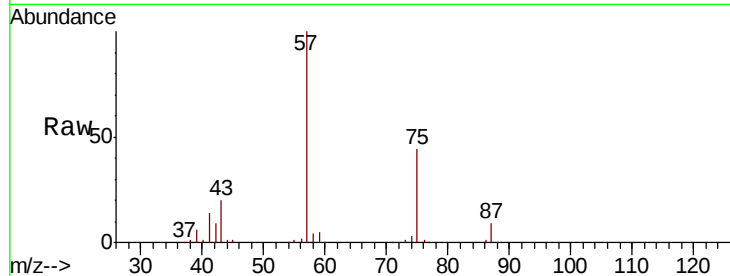

Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

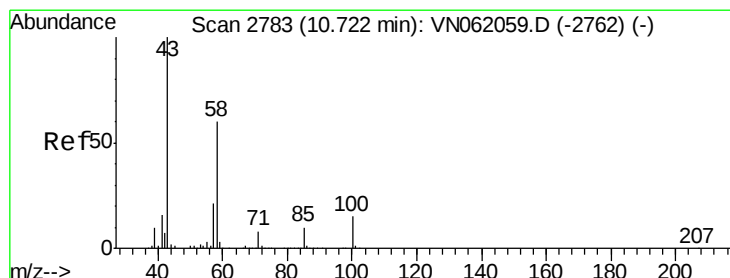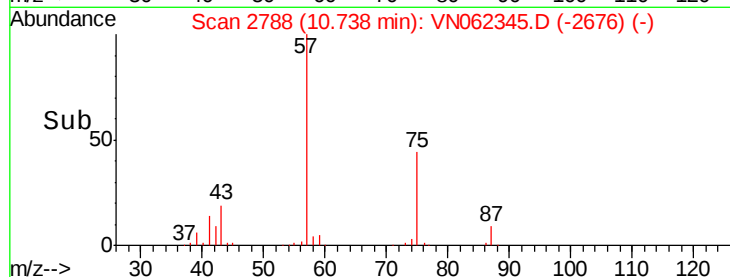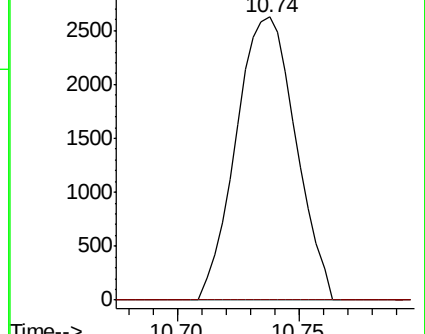

#59

2-Hexanone

Concen: 38.082 ug/l

RT: 10.74 min Scan# 2788

Delta R.T. 0.02 min

Lab File: VN062345.D


Acq: 2 Jul 2020 20:06

Tgt Ion: 43 Resp: 56857

Ion Ratio Lower Upper



43 100


58 20.5 29.5 88.5#

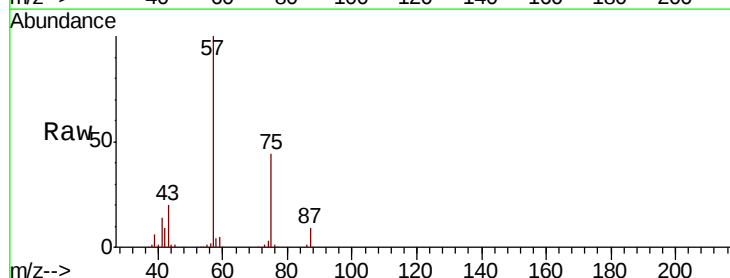

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

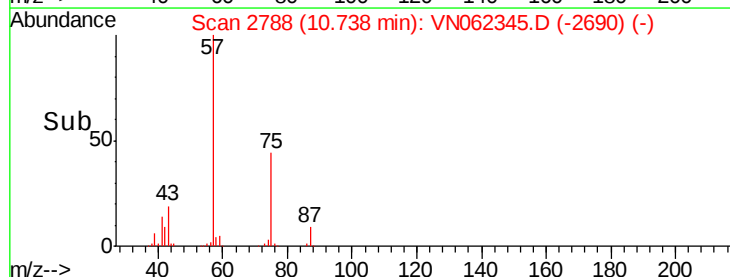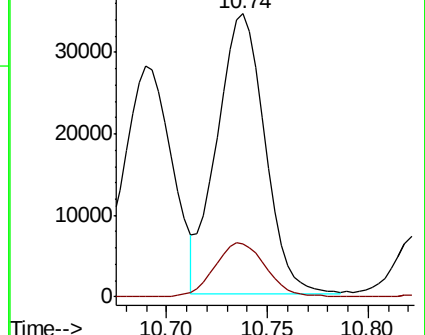




#62
4-Bromofluorobenzene
Concen: 47.630 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.00 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06

Instrument :
MSVOA_N
ClientSampled :

Tot Ion	95	Resp	107636
Ion Ratio	Lower	Upper	
95	100		
174	72.7	0.0	154.8
176	68.5	0.0	147.4



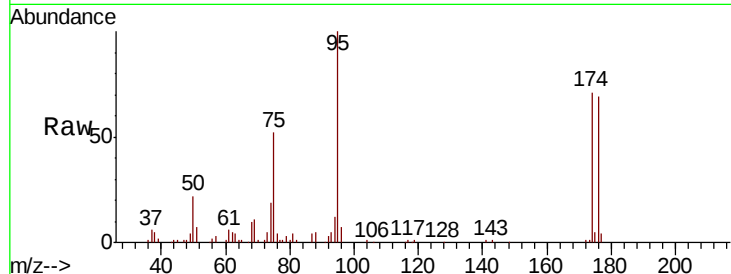


Abundance

Ion 94.90 (94.60 to 95.60): VN062059.D (-3284) (-)


Ion 173.80 (173.50 to 174.50): VN062059.D (-3284) (-)

Ion 175.80 (175.50 to 176.50): VN062059.D (-3284) (-)

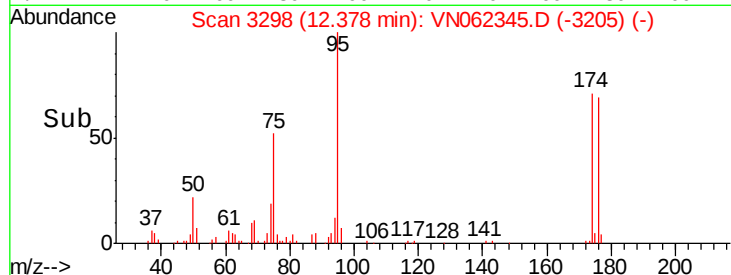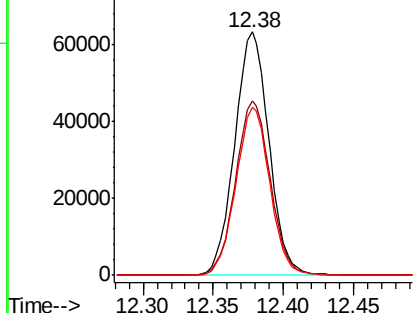

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. 0.00 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06

Tgt Ion	117	Resp	255504
Ion Ratio	Lower	Upper	
117	100		
82	59.0	43.8	65.8
119	31.8	25.2	37.8


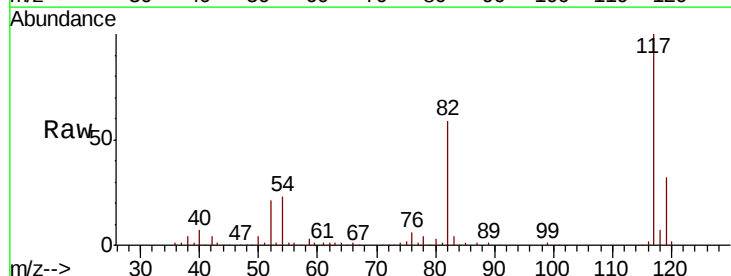



Abundance

Ion 116.90 (116.60 to 117.60): VN062059.D (-2972) (-)

Ion 82.00 (81.70 to 82.70): VN062059.D (-2972) (-)

Ion 118.90 (118.60 to 119.60): VN062059.D (-2972) (-)

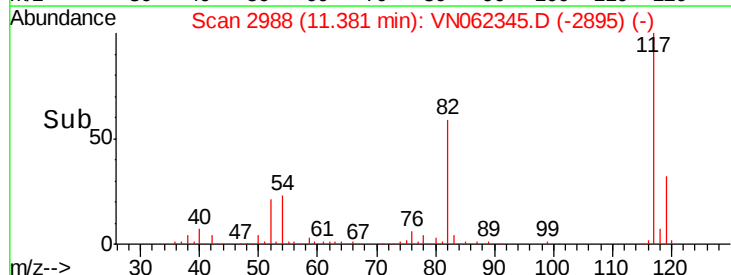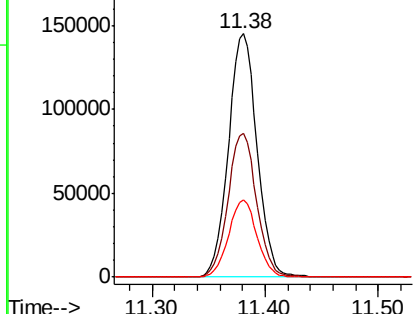



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:152 Resp: 86817

Ion Ratio Lower Upper

152 100

115 61.3 29.5 88.5




150 157.1 0.0 351.4



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

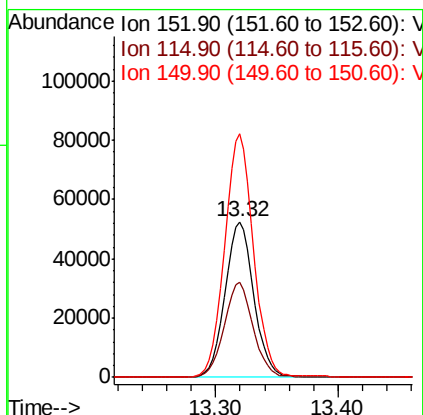

#74

N-ethyl acetate

Concen: 3.801 ug/l

RT: 12.01 min Scan# 3183

Delta R.T. -0.04 min

Lab File: VN062345.D

Acq: 2 Jul 2020 20:06

Tgt Ion: 43 Resp: 1213


Ion Ratio Lower Upper

43 100

70 0.0 39.4 59.2#

55 0.0 21.7 32.5#

61 0.0 21.3 31.9#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V



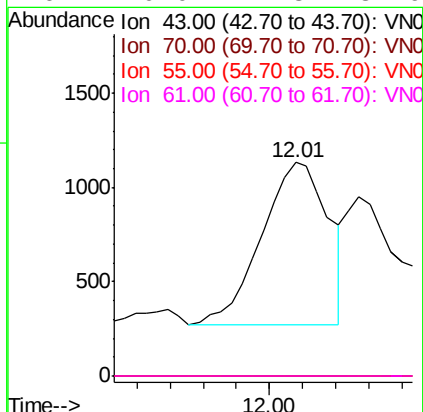



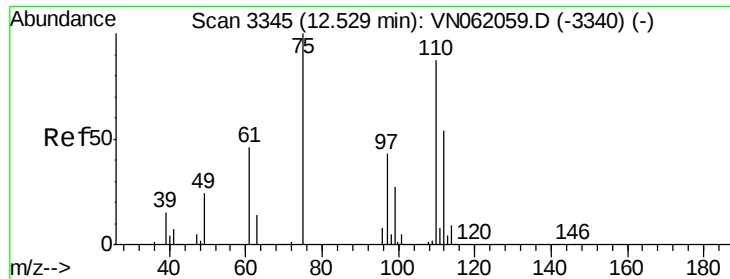

#76
 1,2,3-Trichloropropane
 Concen: 27.908 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. -0.15 min
 Lab File: VN062345.D
 Acq: 2 Jul 2020 20:06




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 75 Resp: 57037
 Ion Ratio Lower Upper
 75 100
 77 1.1 0.0 0.0#

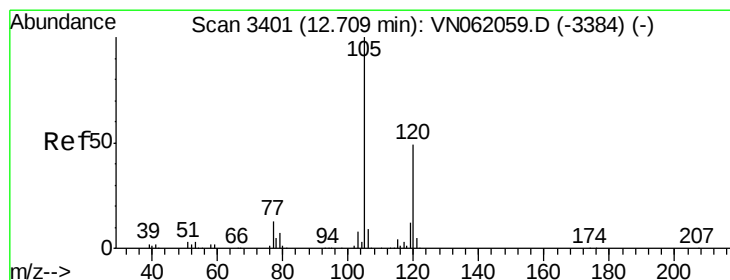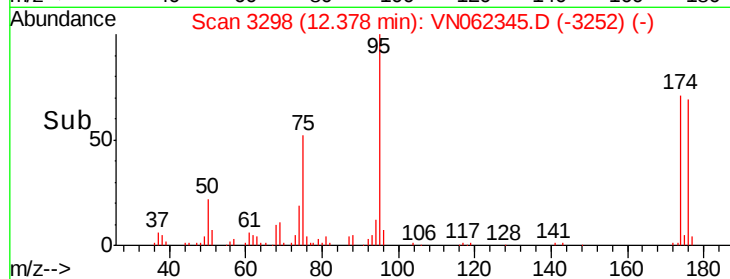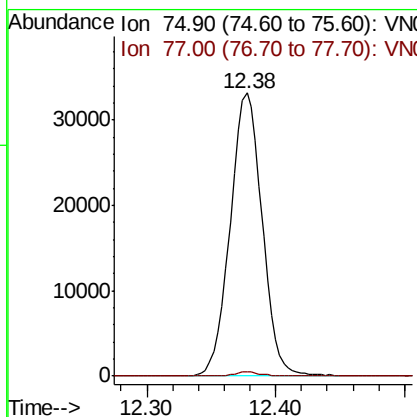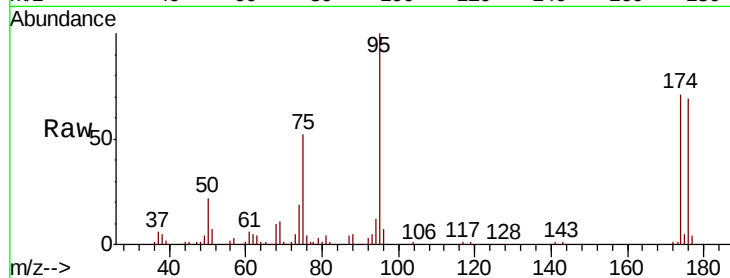

#80
 1,3,5-Trimethylbenzene
 Concen: 0.400 ug/l
 RT: 12.71 min Scan# 3401
 Delta R.T. 0.00 min
 Lab File: VN062345.D
 Acq: 2 Jul 2020 20:06

Tgt Ion:105 Resp: 2178
 Ion Ratio Lower Upper
 105 100
 120 48.8 24.6 74.0

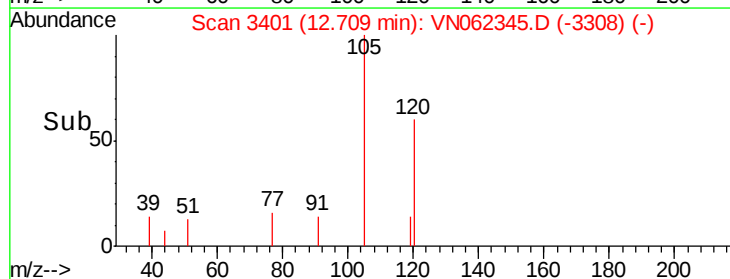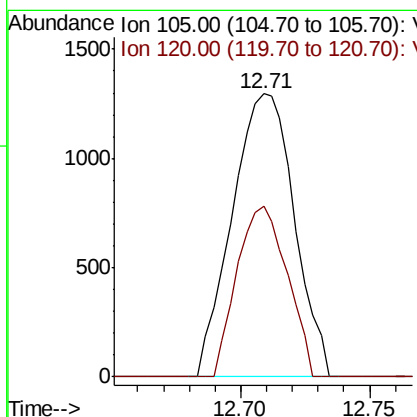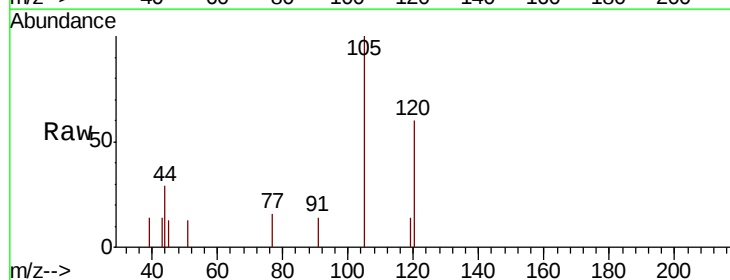


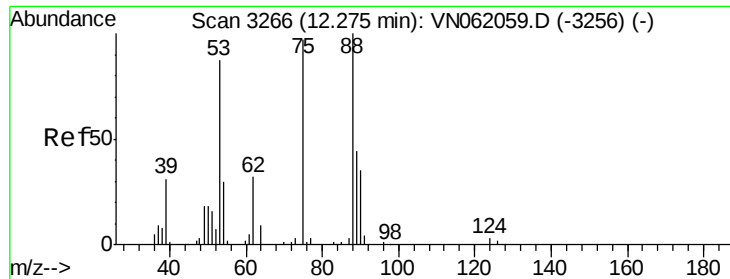




#81
trans-1,4-Dichloro-2-butene
Concen: 81.502 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.10 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06

Instrument :
MSVOA_N
ClientSampleId :

Tot Ion: 75 Resp: 57037
Ion Ratio Lower Upper
75 100
53 0.0 72.0 108.0#
89 0.0 36.9 55.3#

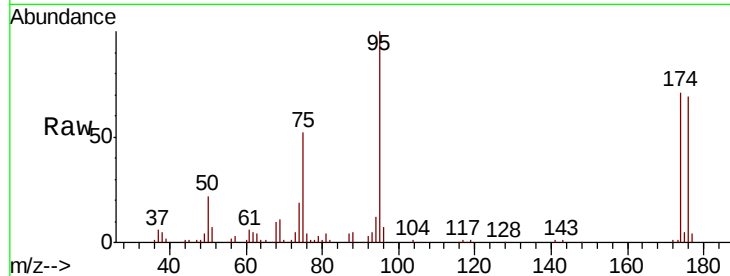


Abundance Ion 74.90 (74.60 to 75.60): VN0
Ion 53.00 (52.70 to 53.70): VN0
Ion 88.90 (88.60 to 89.60): VN0

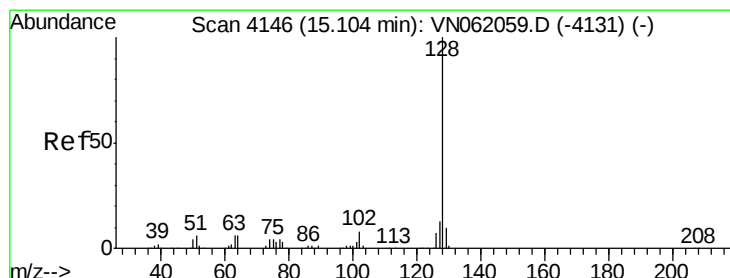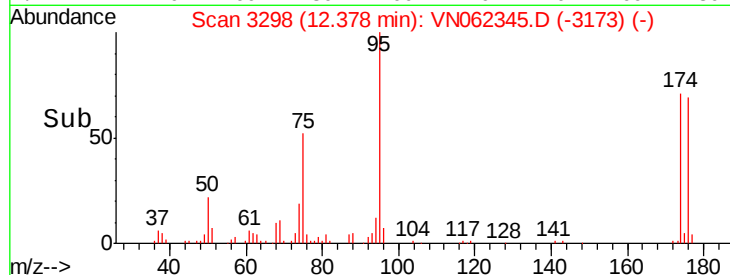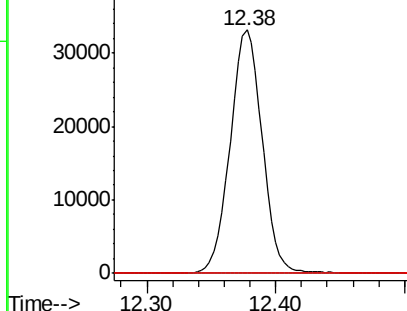

#95
Naphthalene
Concen: 4.112 ug/l
RT: 15.11 min Scan# 4149
Delta R.T. 0.01 min
Lab File: VN062345.D
Acq: 2 Jul 2020 20:06

Tgt Ion: 128 Resp: 528
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 0.0 8.6 13.0#

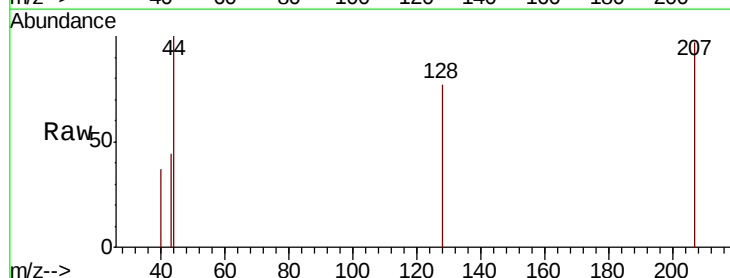

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

