


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070220\
 Data File : VN062335.D
 Acq On : 2 Jul 2020 14:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Title : SW846 8260
 Last Update : Wed Jun 24 15:33:00 2020

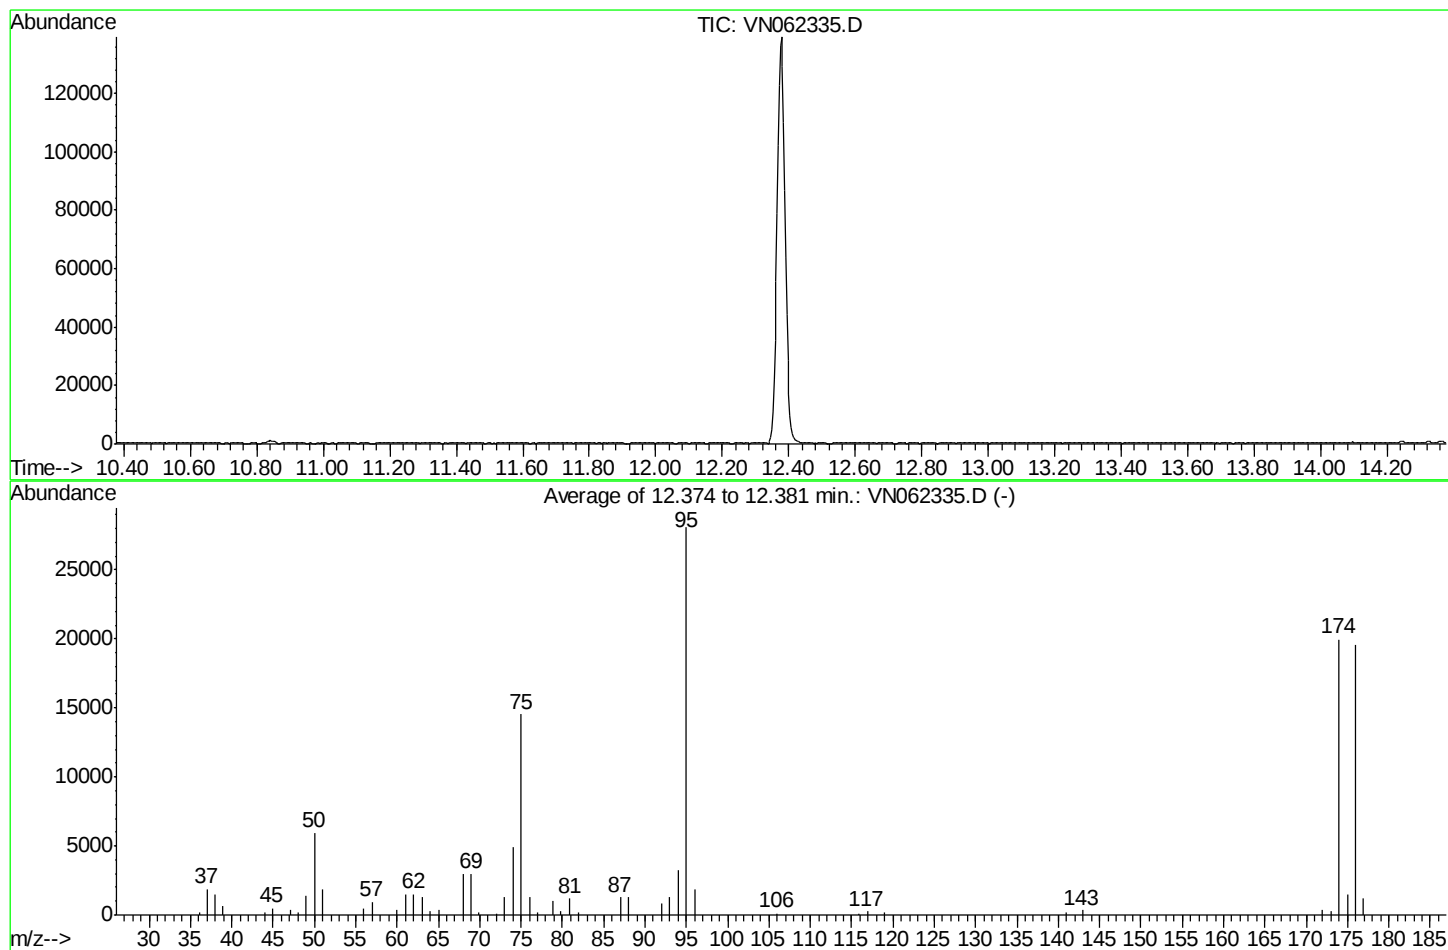

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	5964	PASS
75	95	30	60	51.8	14543	PASS
95	95	100	100	100.0	28080	PASS
96	95	5	9	6.7	1889	PASS
173	174	0.00	2	1.3	250	PASS
174	95	50	100	71.1	19978	PASS
175	174	5	9	7.6	1509	PASS
176	174	95	101	97.9	19552	PASS
177	176	5	9	6.2	1216	PASS