

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070221\
 Data File : VN067625.D
 Acq On : 2 Jul 2021 18:42
 Operator : JC/MD
 Sample : M2896-08
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FS-04

Quant Time: Jul 05 05:04:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 02 12:55:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	399700	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	740202	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	718945	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	279768	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	289819	48.456	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	96.920%		
35) Dibromofluoromethane	8.024	113	217297	47.463	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	94.920%		
50) Toluene-d8	10.446	98	919615	47.593	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	95.180%		
62) 4-Bromofluorobenzene	12.733	95	321087	46.580	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	93.160%		
Target Compounds						Qvalue
3) Chloromethane	2.303	50	1452	0.265	ug/l #	73
11) Tert butyl alcohol	5.387	59	528	0.644	ug/l #	71
13) Acrolein	4.044	56	386	0.570	ug/l #	35
16) Acetone	4.296	43	85088	44.873	ug/l	97
17) Carbon Disulfide	4.518	76	2101	0.208	ug/l #	74
18) Methyl Acetate	4.872	43	8230	1.704	ug/l	98
20) Methylene Chloride	5.095	84	35166	7.439	ug/l	91
25) 2-Butanone	7.343	43	23357	7.634	ug/l	99
29) Tetrahydrofuran	7.710	42	3201	1.571	ug/l #	65
31) Cyclohexane	8.094	56	10322	1.248	ug/l #	48
36) 1,1-Dichloropropene	8.091	75	35243	5.048	ug/l #	52
37) Ethyl Acetate	7.343	43	23357	3.487	ug/l #	73
38) Carbon Tetrachloride	8.088	117	43760	6.219	ug/l #	16
43) Isopropyl Acetate	8.566	43	46053	3.942	ug/l #	90
48) Methyl methacrylate	9.550	41	12968	2.523	ug/l #	12
49) 1,4-Dioxane	9.622	88	307	3.368	ug/l #	1
51) 4-Methyl-2-Pentanone	10.336	43	11586	1.622	ug/l #	85
52) Toluene	10.510	92	10110	0.733	ug/l	98
53) t-1,3-Dichloropropene	10.722	75	49	1.725	ug/l #	43
54) cis-1,3-Dichloropropene	10.247	75	77561	9.463	ug/l #	59
57) 1,3-Dichloropropane	11.095	76	38979	4.433	ug/l #	43
59) 2-Hexanone	11.095	43	578743	115.575	ug/l #	54
60) Dibromochloromethane	11.489	129	316	2.095	ug/l #	11
70) Styrene	12.293	104	811	1.388	ug/l #	81
74) N-ethyl acetate	12.350	43	6180	0.755	ug/l #	53
76) 1,2,3-Trichloropropane	12.733	75	177108	31.653	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.733	75	177108	95.448	ug/l #	7
84) 1,2,4-Trimethylbenzene	13.372	105	4932	0.269	ug/l	96
89) n-Butylbenzene	13.943	91	3270	0.224	ug/l #	78
92) 1,2-Dibromo-3-Chloropr...	14.592	75	245	0.222	ug/l #	16
95) Naphthalene	15.509	128	35997	6.980	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070221\
Data File : VN067625.D
Acq On : 2 Jul 2021 18:42
Operator : JC/MD
Sample : M2896-08
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FS-04


Quant Time: Jul 05 05:04:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 02 12:55:54 2021
Response via : Initial Calibration

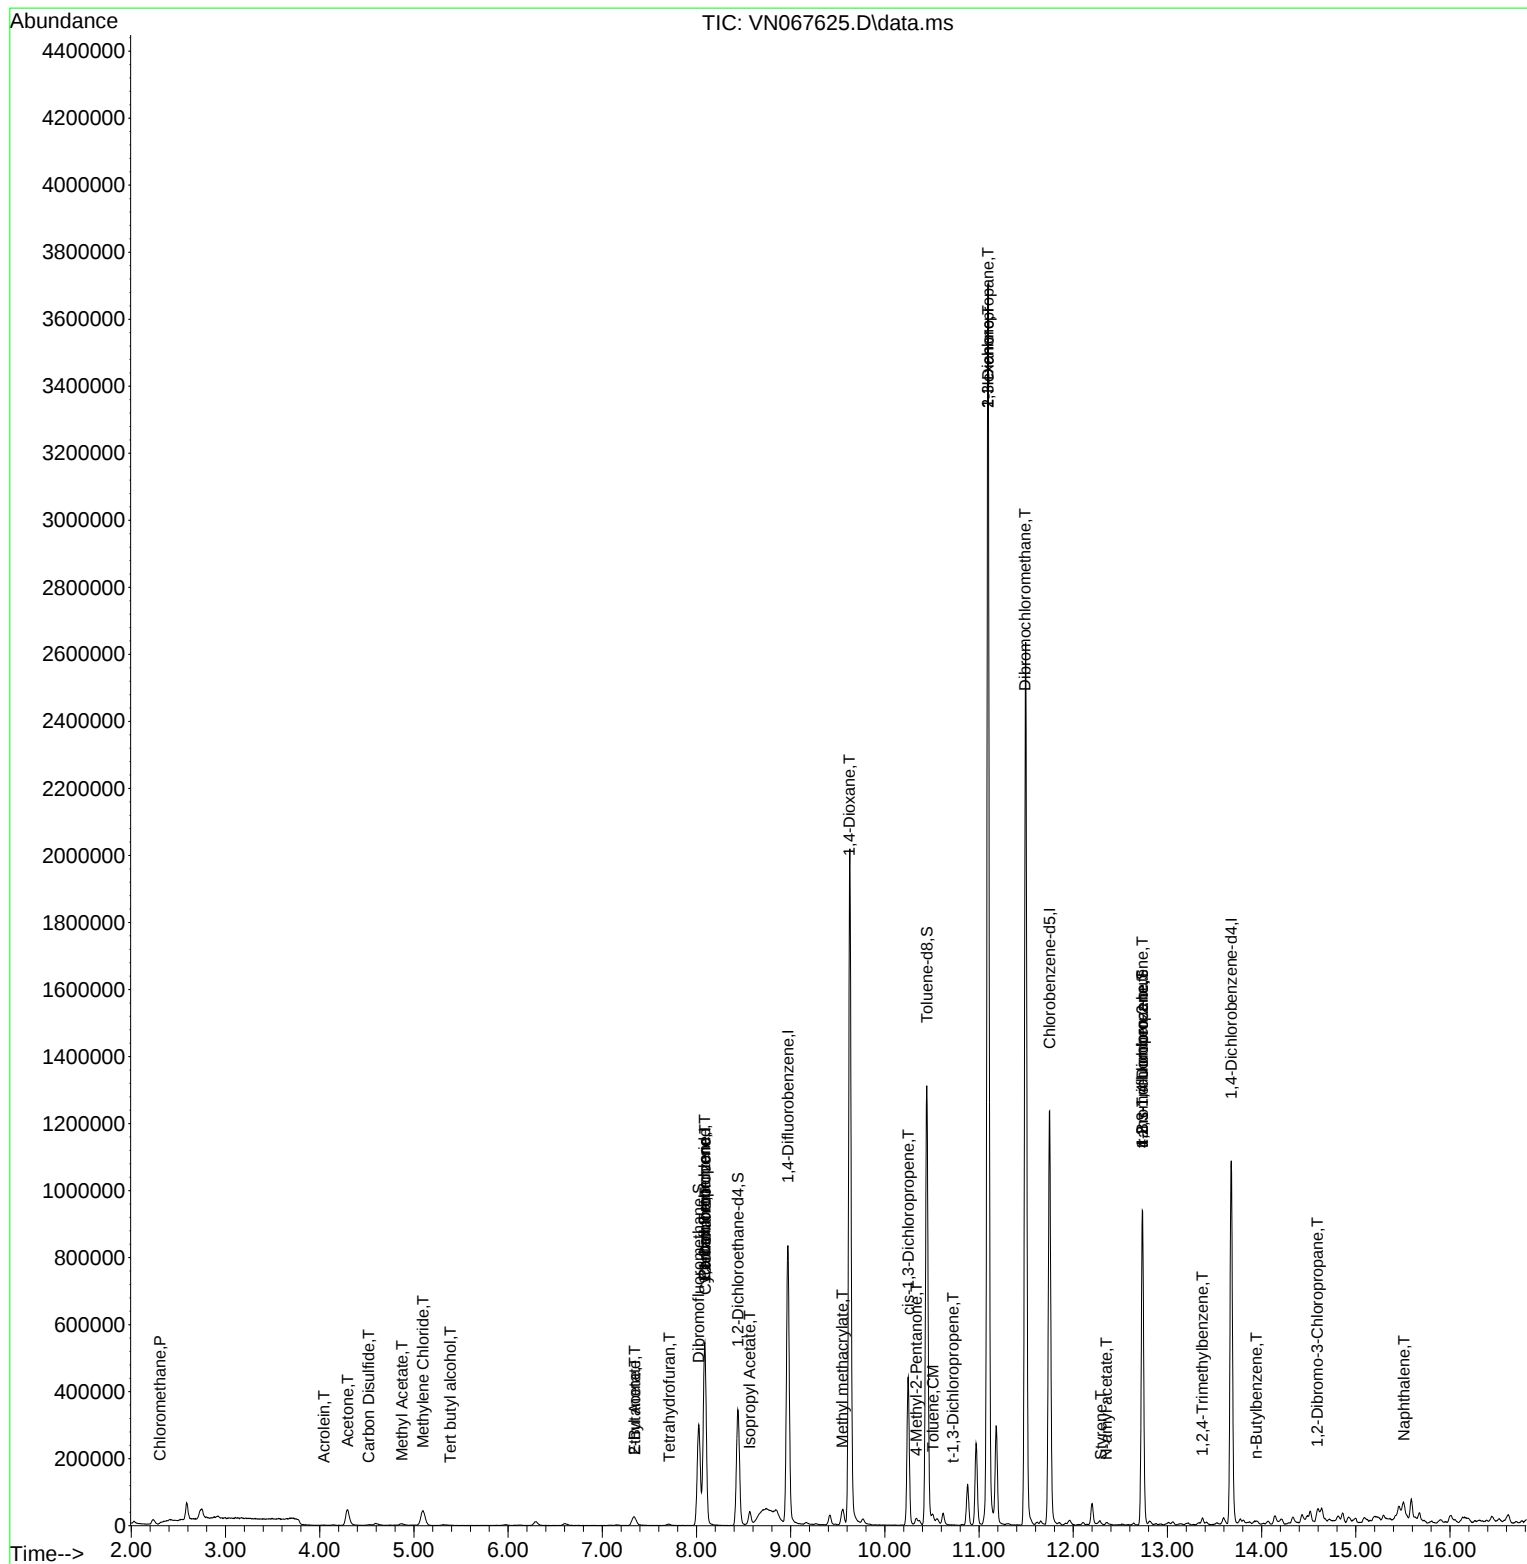






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Instrument :
MSVOA_N
ClientSampleId :
FS-04







Tgt Ion:168 Resp: 399700
Ion Ratio Lower Upper
168 100
99 63.1 62.9 94.3

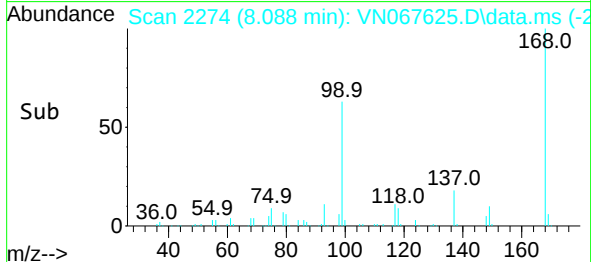

#3
Chloromethane
Concen: 0.265 ug/l
RT: 2.303 min Scan# 117
Delta R.T. 0.002 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 50 Resp: 1452
Ion Ratio Lower Upper
50 100
52 16.9 25.6 38.4#






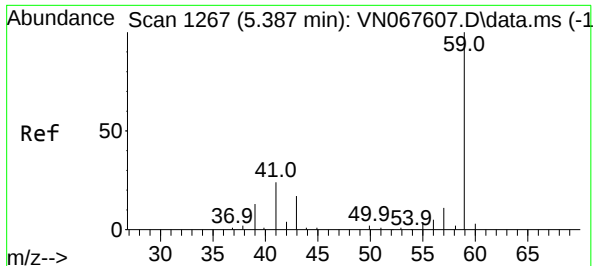


#11

Tert butyl alcohol
Concen: 0.644 ug/l
RT: 5.387 min Scan# 1267
Delta R.T. 0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Instrument :
MSVOA_N
ClientSampled :
FS-04




Tgt Ion: 59 Resp: 528
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

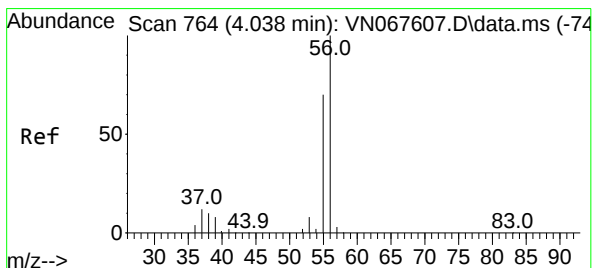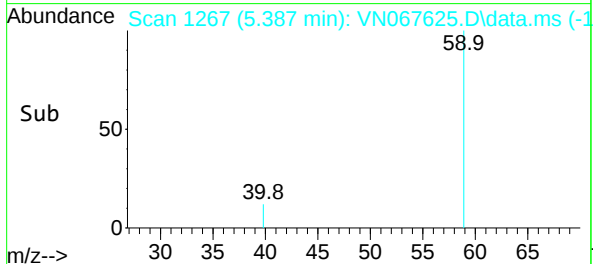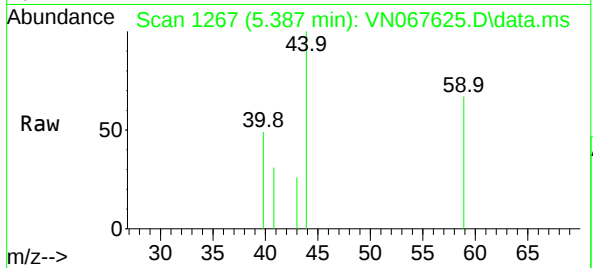


#13

Acrolein
Concen: 0.570 ug/l
RT: 4.044 min Scan# 766
Delta R.T. 0.006 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 56 Resp: 386
Ion Ratio Lower Upper
56 100
55 125.9 57.4 86.0#


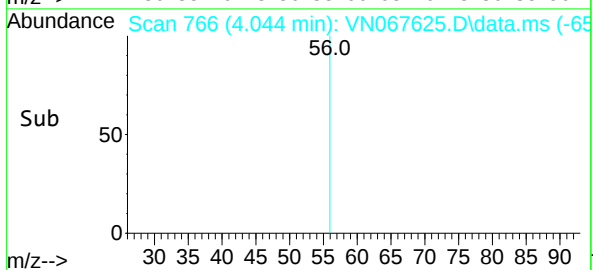

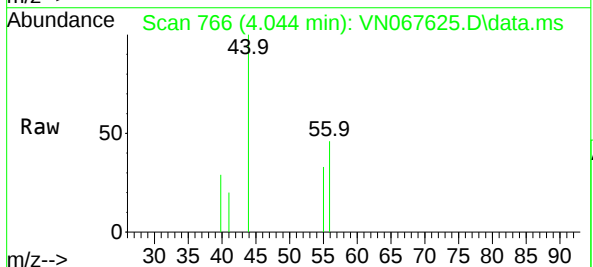




#16
Acetone
Concen: 44.873 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.005 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 43 Resp: 85088
Ion Ratio Lower Upper
43 100
58 28.2 21.2 31.8

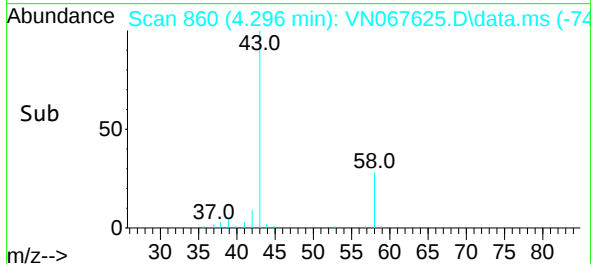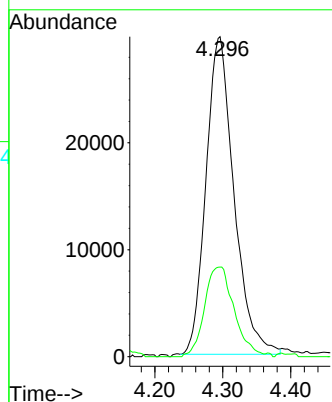

#17
Carbon Disulfide
Concen: 0.208 ug/l
RT: 4.518 min Scan# 943
Delta R.T. -0.003 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 76 Resp: 2101
Ion Ratio Lower Upper
76 100
78 0.0 7.7 11.5#



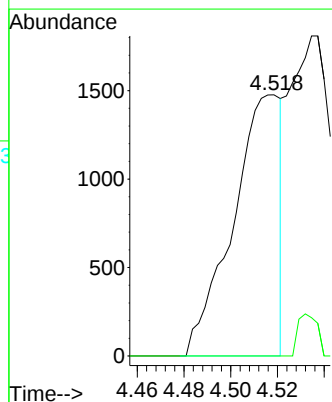



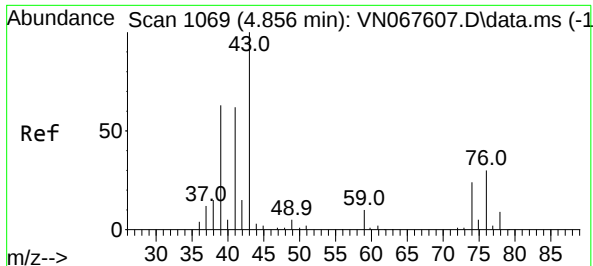

#18
Methyl Acetate
Concen: 1.704 ug/l
RT: 4.872 min Scan# 1075
Delta R.T. 0.016 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 43 Resp: 8230
Ion Ratio Lower Upper
43 100
74 20.7 17.4 26.0

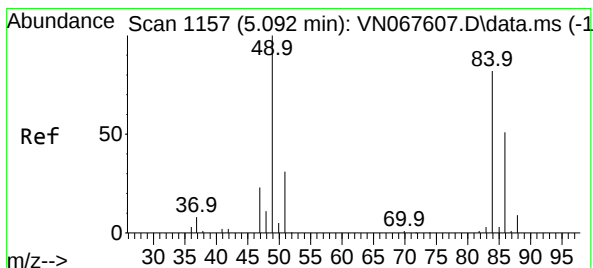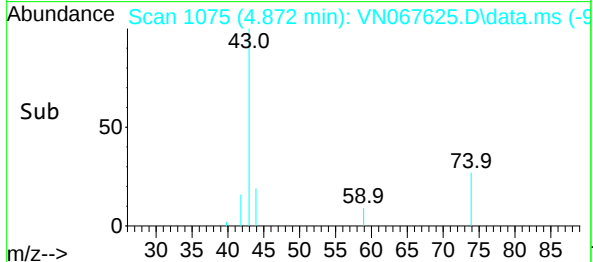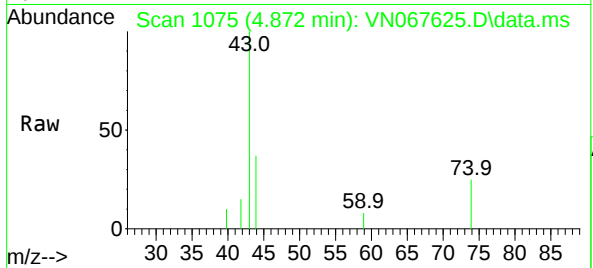

#20
Methylene Chloride
Concen: 7.439 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.003 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 84 Resp: 35166
Ion Ratio Lower Upper
84 100
49 123.2 110.9 166.3
51 40.5 32.6 49.0
86 58.3 51.6 77.4


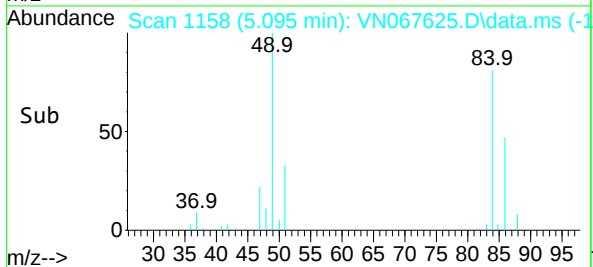
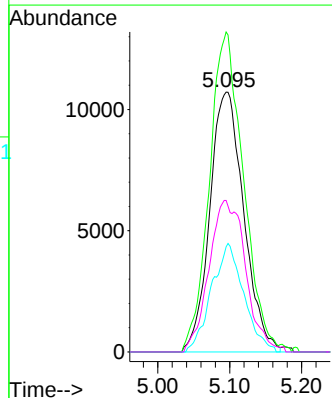
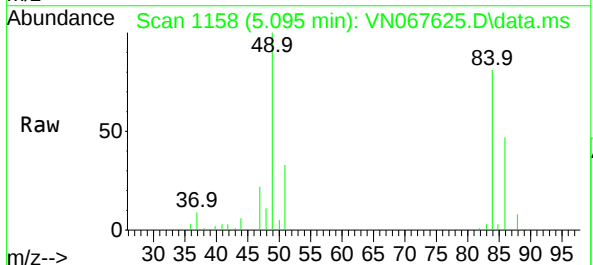


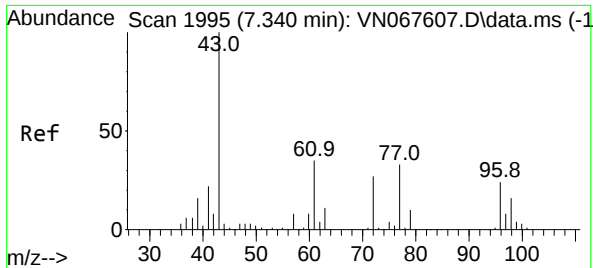

#25
2-Butanone
Concen: 7.634 ug/l
RT: 7.343 min Scan# 1996
Delta R.T. 0.003 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 43 Resp: 23357
Ion Ratio Lower Upper
43 100
72 24.0 19.7 29.5

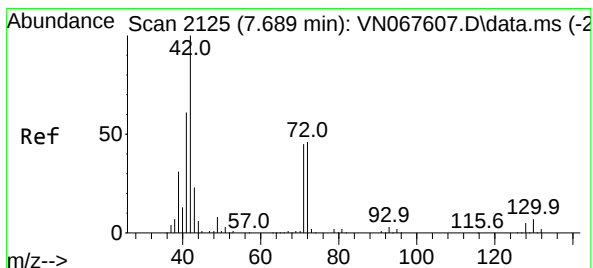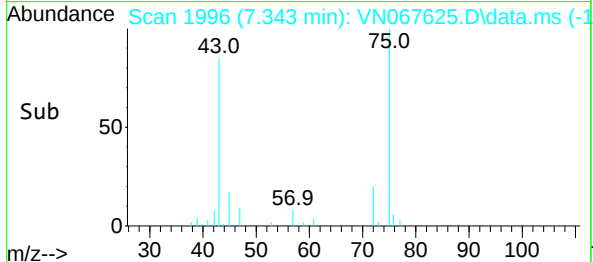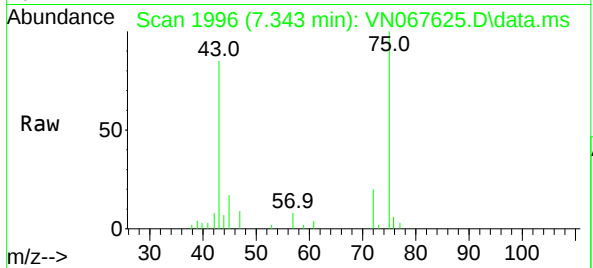

#29
Tetrahydrofuran
Concen: 1.571 ug/l
RT: 7.710 min Scan# 2133
Delta R.T. 0.021 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42


Tgt Ion: 42 Resp: 3201
Ion Ratio Lower Upper
42 100
72 22.6 32.8 49.2#
71 13.5 31.2 46.8#

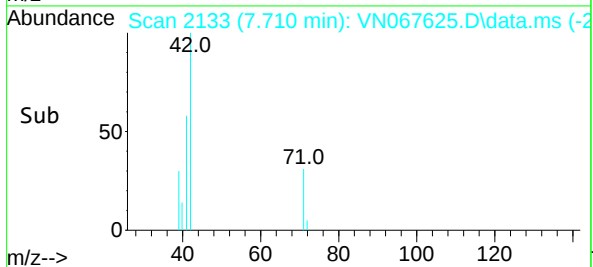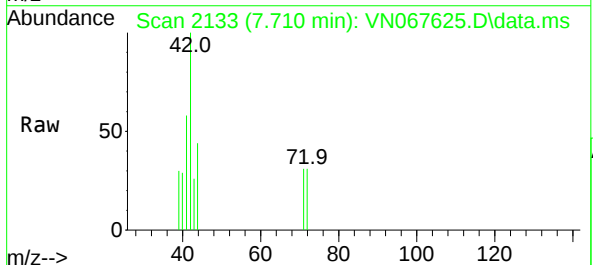






#31
Cyclohexane
Concen: 1.248 ug/l
RT: 8.094 min Scan# 2276
Delta R.T. -0.002 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Instrument :
MSVOA_N
ClientSampled :
FS-04







Tgt Ion: 56 Resp: 10322
Ion Ratio Lower Upper
56 100
69 118.5 27.3 40.9#
84 91.2 64.9 97.3

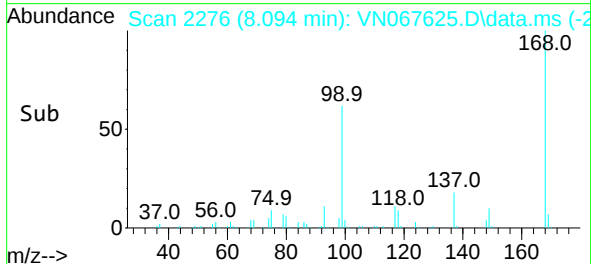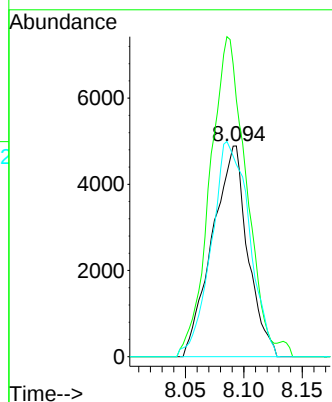

#33
1,2-Dichloroethane-d4
Concen: 48.456 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 65 Resp: 289819
Ion Ratio Lower Upper
65 100
67 51.0 0.0 98.6



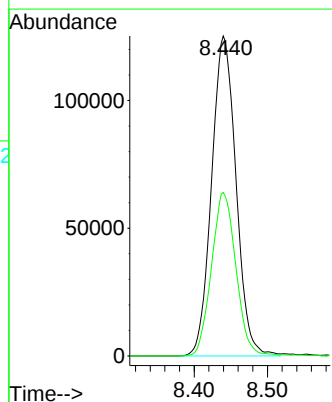





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. -0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampleId :
FS-04


Tgt Ion:114	Resp: 740202
Ion Ratio	Lower Upper
114 100	
63 20.8	0.0 49.0
88 15.1	0.0 36.6

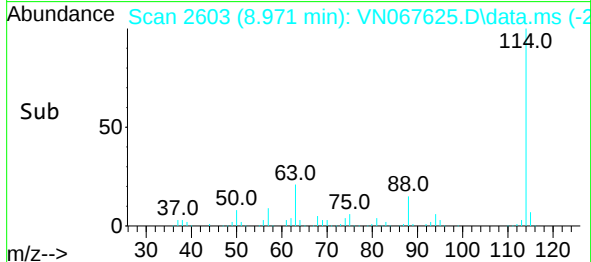

#35
Dibromofluoromethane
Concen: 47.463 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42


Tgt Ion:113	Resp: 217297		
Ion	Ratio	Lower	Upper
113	100		
111	102.2	83.8	125.8
192	16.2	13.4	20.0

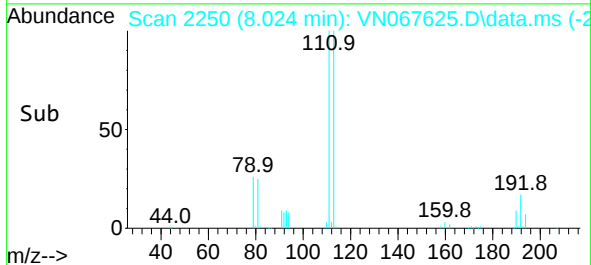






#36
1,1-Dichloropropene
Concen: 5.048 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.131 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Instrument :
MSVOA_N
ClientSampled :
FS-04







Tgt Ion: 75 Resp: 35243
Ion Ratio Lower Upper
75 100
110 9.1 15.7 47.0#
77 0.0 24.6 37.0#

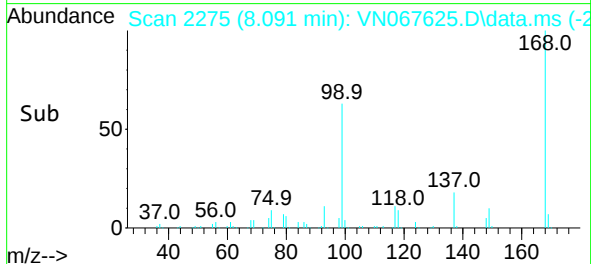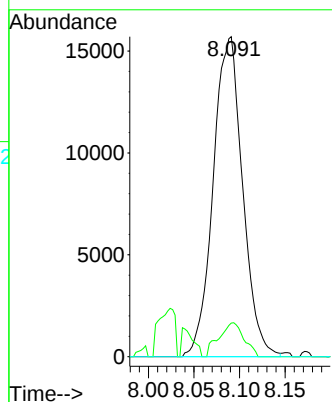

#37
Ethyl Acetate
Concen: 3.487 ug/l
RT: 7.343 min Scan# 1996
Delta R.T. -0.072 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42


Tgt Ion: 43 Resp: 23357
Ion Ratio Lower Upper
43 100
61 2.5 10.6 16.0#
70 0.0 8.1 12.1#








#38
Carbon Tetrachloride
Concen: 6.219 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Instrument :
MSVOA_N
ClientSampled :
FS-04







Tgt Ion:117 Resp: 43760
Ion Ratio Lower Upper
117 100
119 4.5 75.4 113.2#
121 0.0 23.5 35.3#

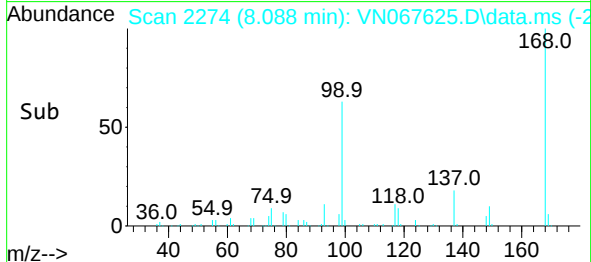

#43
Isopropyl Acetate
Concen: 3.942 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. -0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 43 Resp: 46053
Ion Ratio Lower Upper
43 100
61 17.6 19.0 28.4#
87 13.6 9.5 14.3




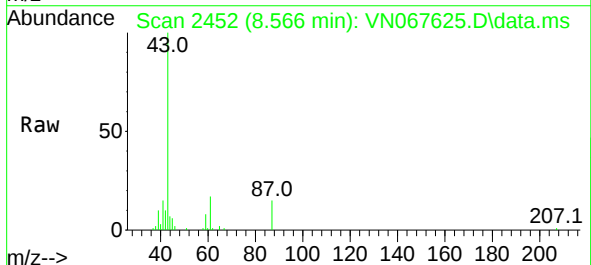




#48
Methyl methacrylate
Concen: 2.523 ug/l
RT: 9.550 min Scan# 2819
Delta R.T. -0.013 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 41 Resp: 12968
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

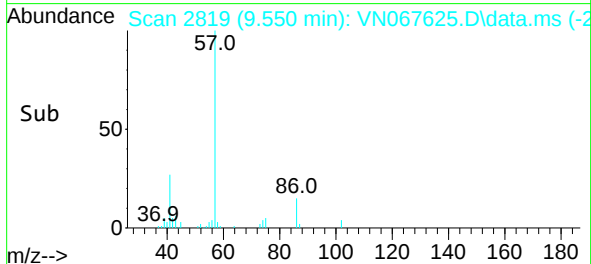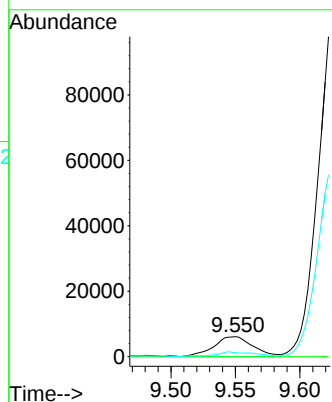

#49
1,4-Dioxane
Concen: 3.368 ug/l
RT: 9.622 min Scan# 2846
Delta R.T. 0.051 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 88 Resp: 307
Ion Ratio Lower Upper
88 100
43 651159.0 28.8 43.2#
58 2451.5 60.4 90.6#



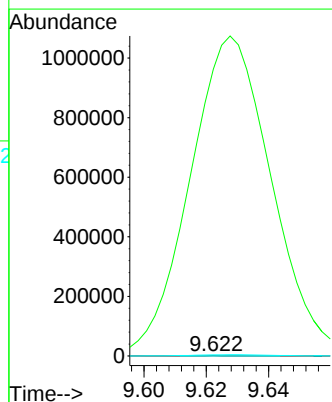





#50
Toluene-d8
Concen: 47.593 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 98 Resp: 919615
Ion Ratio Lower Upper
98 100
100 63.7 51.7 77.5

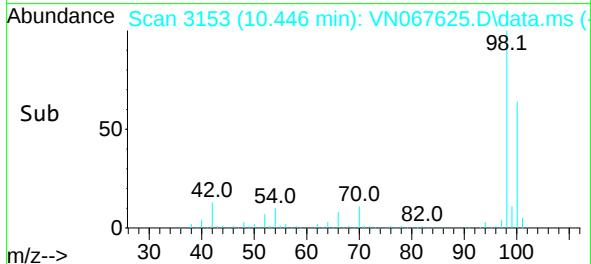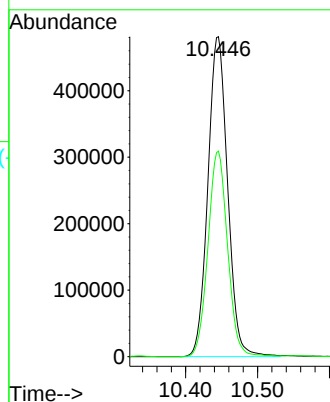

#51
4-Methyl-2-Pentanone
Concen: 1.622 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. -0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 43 Resp: 11586
Ion Ratio Lower Upper
43 100
58 44.5 28.6 43.0#



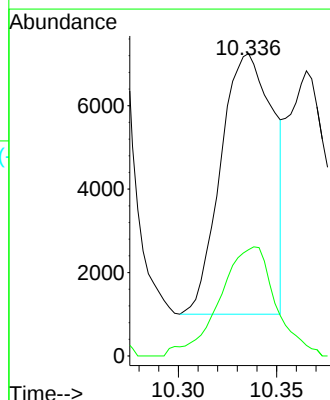





#52
Toluene
Concen: 0.733 ug/l
RT: 10.510 min Scan# 3177
Delta R.T. 0.003 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 92 Resp: 10110
Ion Ratio Lower Upper
92 100
91 177.9 139.6 209.4

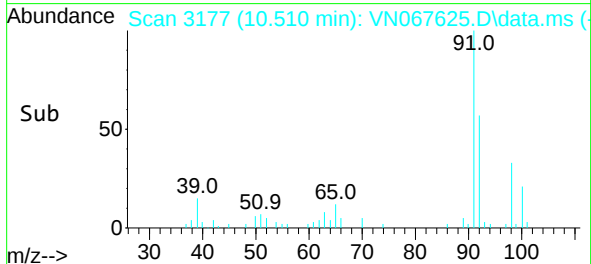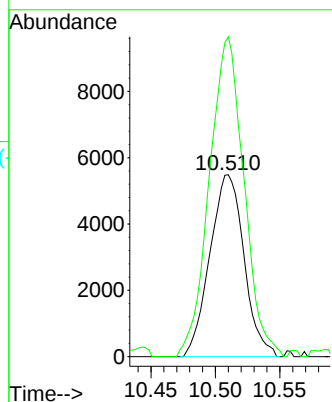

#53
t-1,3-Dichloropropene
Concen: 1.725 ug/l
RT: 10.722 min Scan# 3256
Delta R.T. -0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 75 Resp: 49
Ion Ratio Lower Upper
75 100
77 0.0 25.1 37.7#



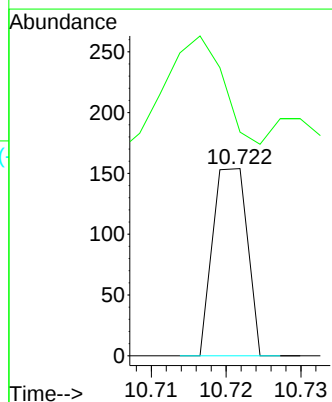



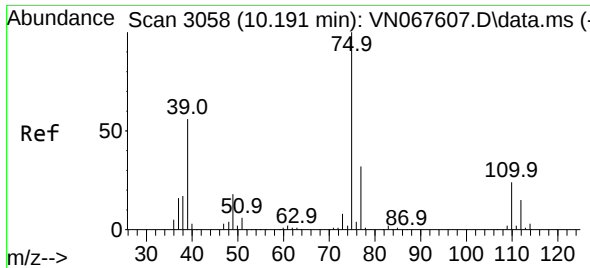

#54
cis-1,3-Dichloropropene
Concen: 9.463 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 75 Resp: 77561
Ion Ratio Lower Upper
75 100
77 0.7 24.6 37.0#
39 36.6 50.7 76.1#

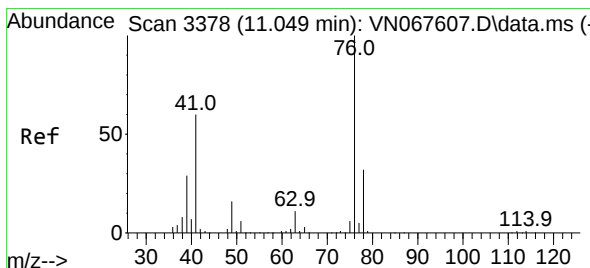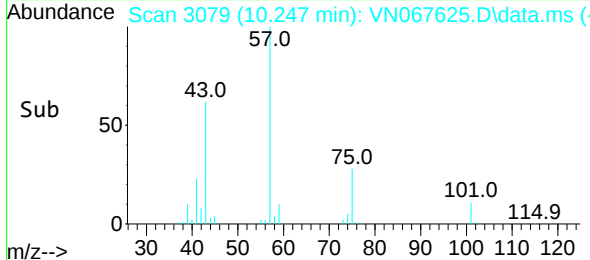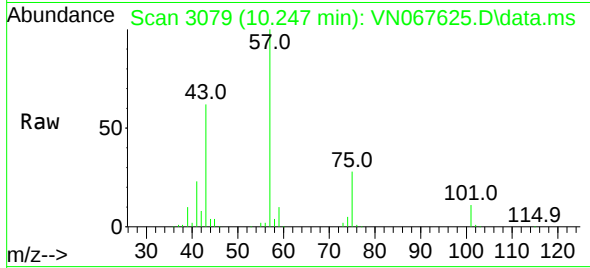

#57
1,3-Dichloropropane
Concen: 4.433 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.046 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 76 Resp: 38979
Ion Ratio Lower Upper
76 100
78 0.2 25.7 38.5#


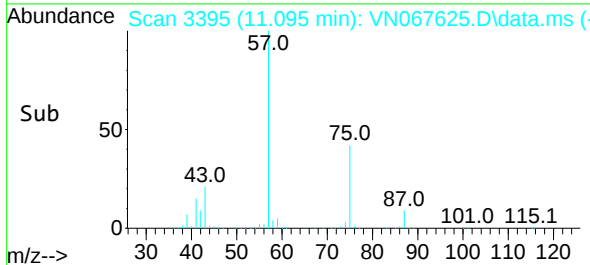

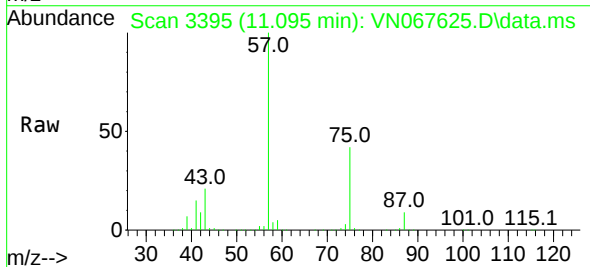




#59
2-Hexanone
Concen: 115.575 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.006 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 43 Resp: 578743
Ion Ratio Lower Upper
43 100
58 18.1 24.7 74.1#

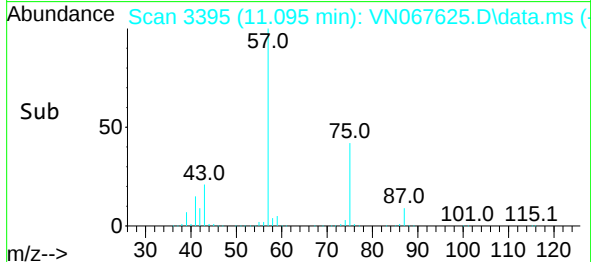

#60
Dibromochloromethane
Concen: 2.095 ug/l
RT: 11.489 min Scan# 3542
Delta R.T. 0.247 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion:129 Resp: 316
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#




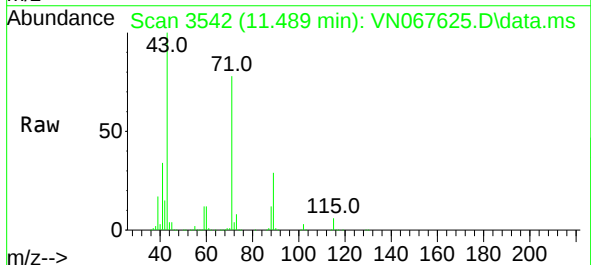




#62
4-Bromofluorobenzene
Concen: 46.580 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 95 Resp: 321087
Ion Ratio Lower Upper
95 100
174 73.1 0.0 122.0
176 70.3 0.0 117.6

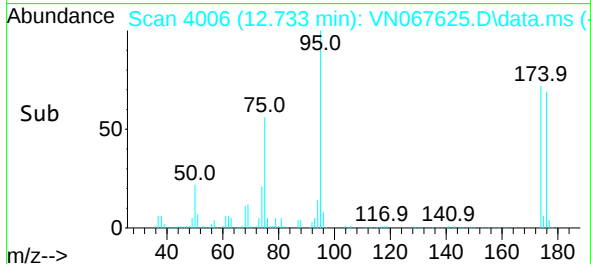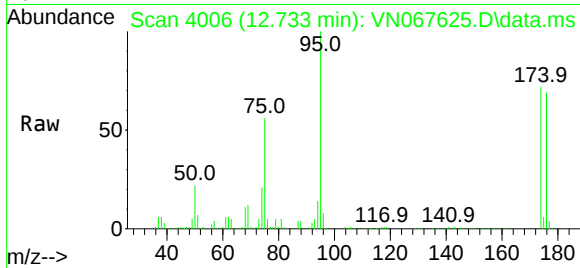

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion: 117 Resp: 718945
Ion Ratio Lower Upper
117 100
82 55.2 53.1 79.7
119 32.1 25.5 38.3




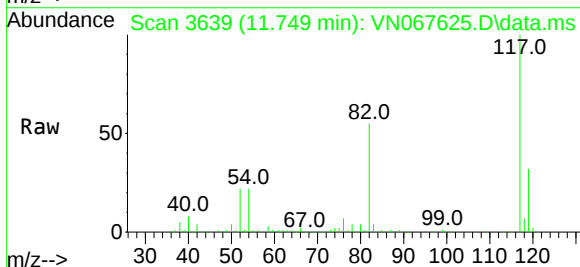




#70
Styrene
Concen: 1.388 ug/l
RT: 12.293 min Scan# 3842
Delta R.T. -0.006 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion:104 Resp: 811
Ion Ratio Lower Upper
104 100
78 49.9 48.2 72.2
103 73.2 44.5 66.7#

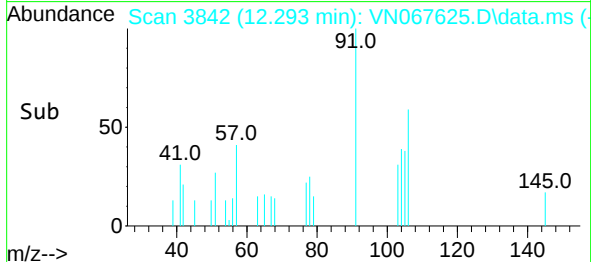

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion:152 Resp: 279768
Ion Ratio Lower Upper
152 100
115 63.0 36.1 108.5
150 159.1 0.0 351.8




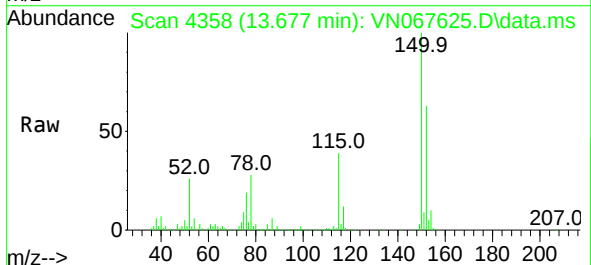




#74
N-amy1 acetate
Concen: 0.755 ug/l
RT: 12.350 min Scan# 3863
Delta R.T. -0.040 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion:	43	Resp:	6180
Ion	Ratio	Lower	Upper
43	100		
70	0.0	29.4	44.2#
55	11.0	17.0	25.4#
61	0.0	17.6	26.4#

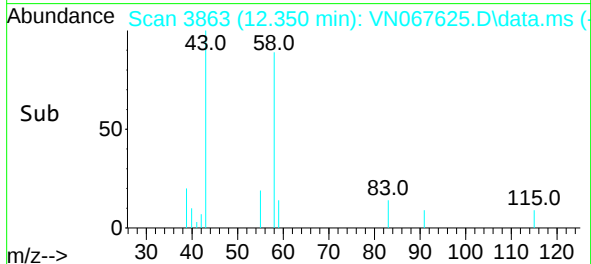

#76
1,2,3-Trichloropropane
Concen: 31.653 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion:	75	Resp:	177108
Ion	Ratio	Lower	Upper
75	100		
77	0.7	0.0	0.0#









#81
trans-1,4-Dichloro-2-butene
Concen: 95.448 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampled :
FS-04


Tgt Ion: 75 Resp: 177108
Ion Ratio Lower Upper
75 100
53 1.5 87.6 131.4#
89 0.0 37.8 56.8#

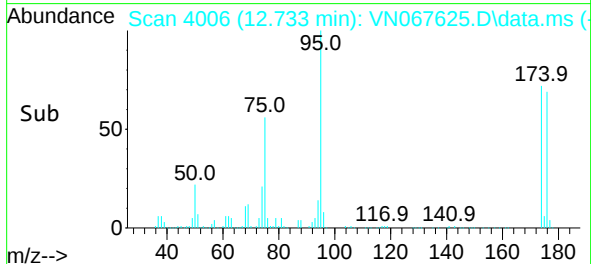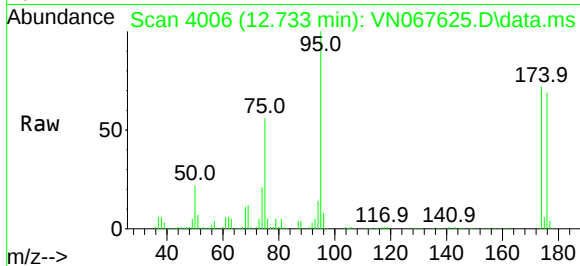

#84
1,2,4-Trimethylbenzene
Concen: 0.269 ug/l
RT: 13.372 min Scan# 4244
Delta R.T. -0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Tgt Ion:105 Resp: 4932
Ion Ratio Lower Upper
105 100
120 44.0 20.6 61.8




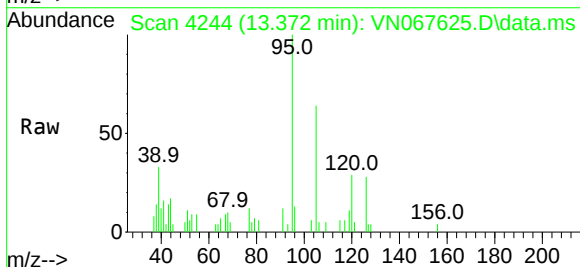


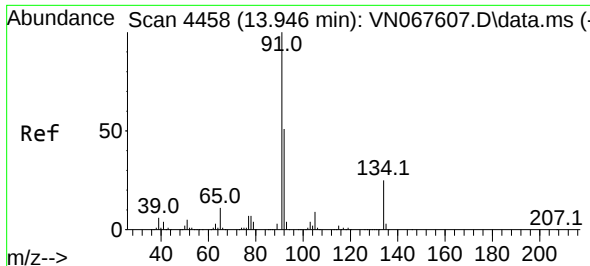

#89
n-Butylbenzene
Concen: 0.224 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. -0.003 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42




Instrument :
MSVOA_N
ClientSampleId :
FS-04


Tgt Ion: 91 Resp: 3270
Ion Ratio Lower Upper
91 100
92 43.5 25.7 77.1
134 0.0 11.2 33.6#

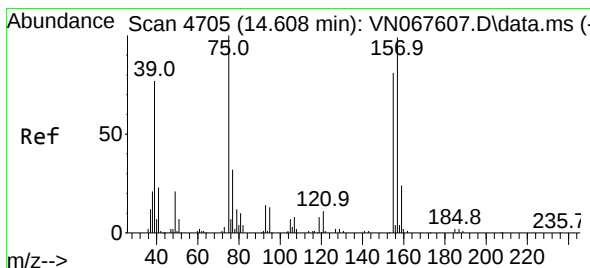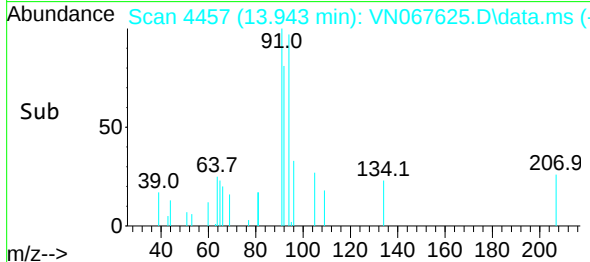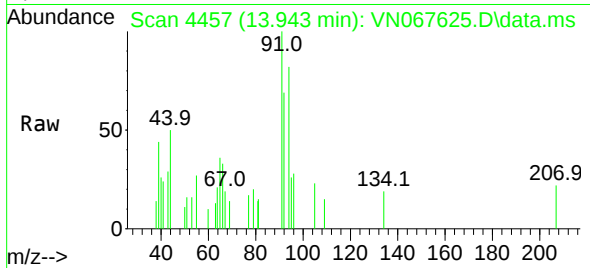

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.222 ug/l
RT: 14.592 min Scan# 4699
Delta R.T. -0.016 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42


Tgt Ion: 75 Resp: 245
Ion Ratio Lower Upper
75 100
155 0.0 29.8 89.5#
157 0.0 37.6 112.8#

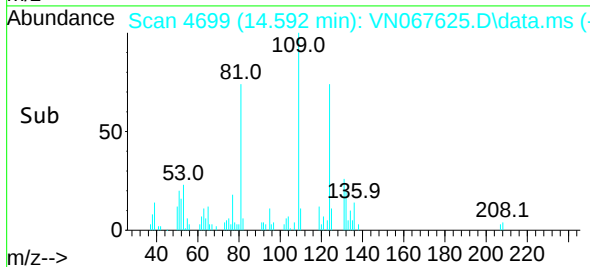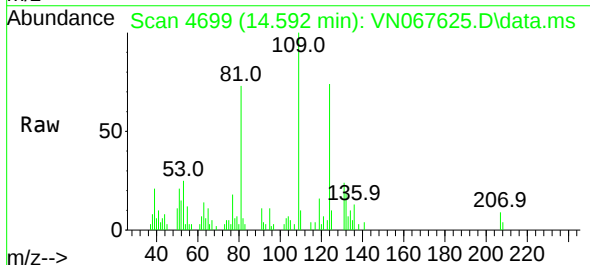



#95
Naphthalene
Concen: 6.980 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.000 min
Lab File: VN067625.D
Acq: 2 Jul 2021 18:42

Instrument :
MSVOA_N
ClientSampleId :
FS-04



Tgt Ion:128 Resp: 35997
Ion Ratio Lower Upper
128 100
127 13.7 10.6 15.8
129 11.9 8.6 12.8

