


t-1,3-Dichloropropene

Response Ratio

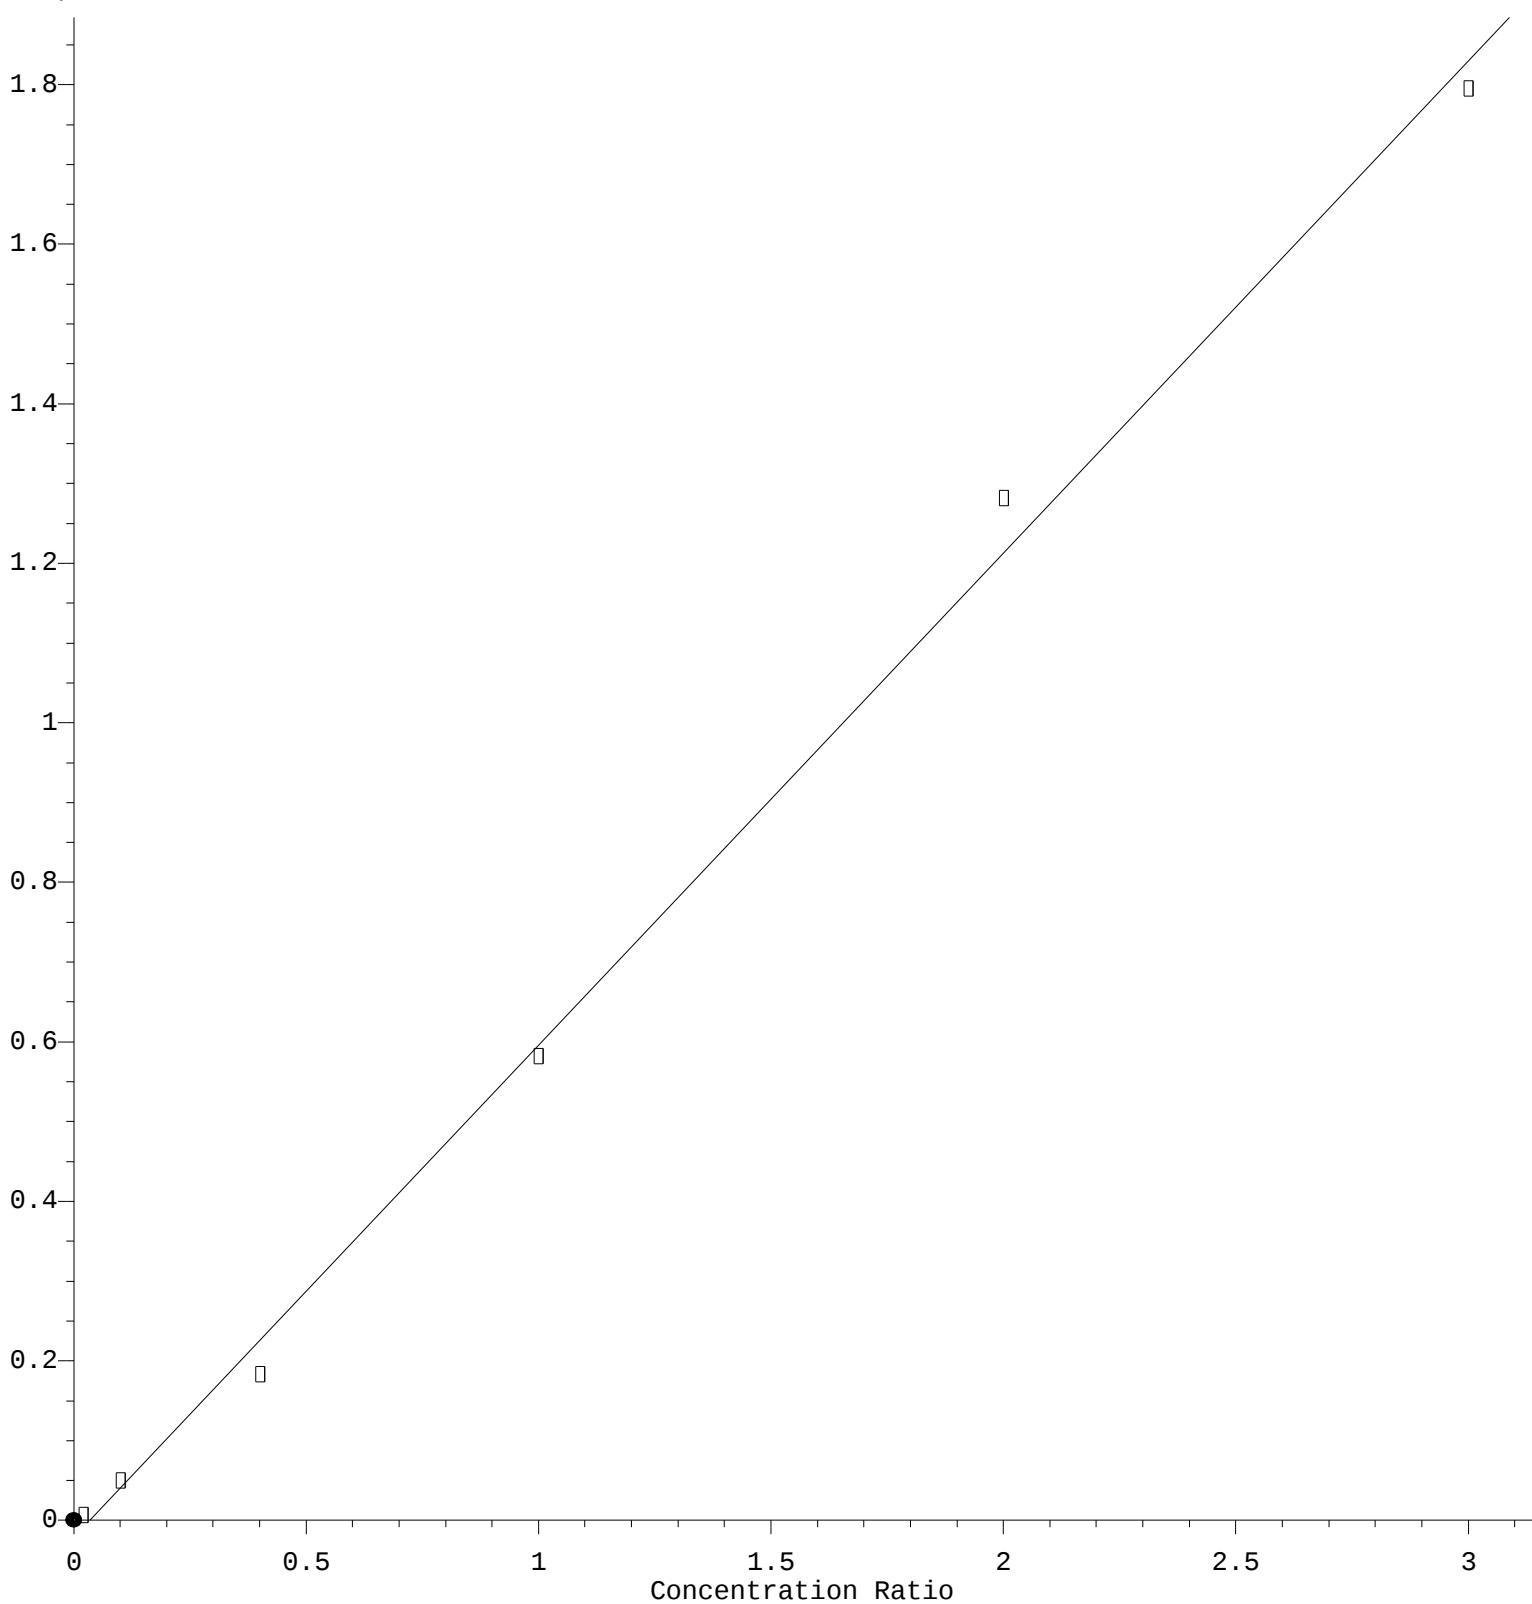

$$\text{Response} = 6.171\text{e-}001 * \text{Amt} - 2.122\text{e-}002$$


Coef of Det (r^2) = 0.996960 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070221W.M

Calibration Table Last Updated: Fri Jul 02 12:55:54 2021

2-Chloroethyl Vinyl ether

Response Ratio

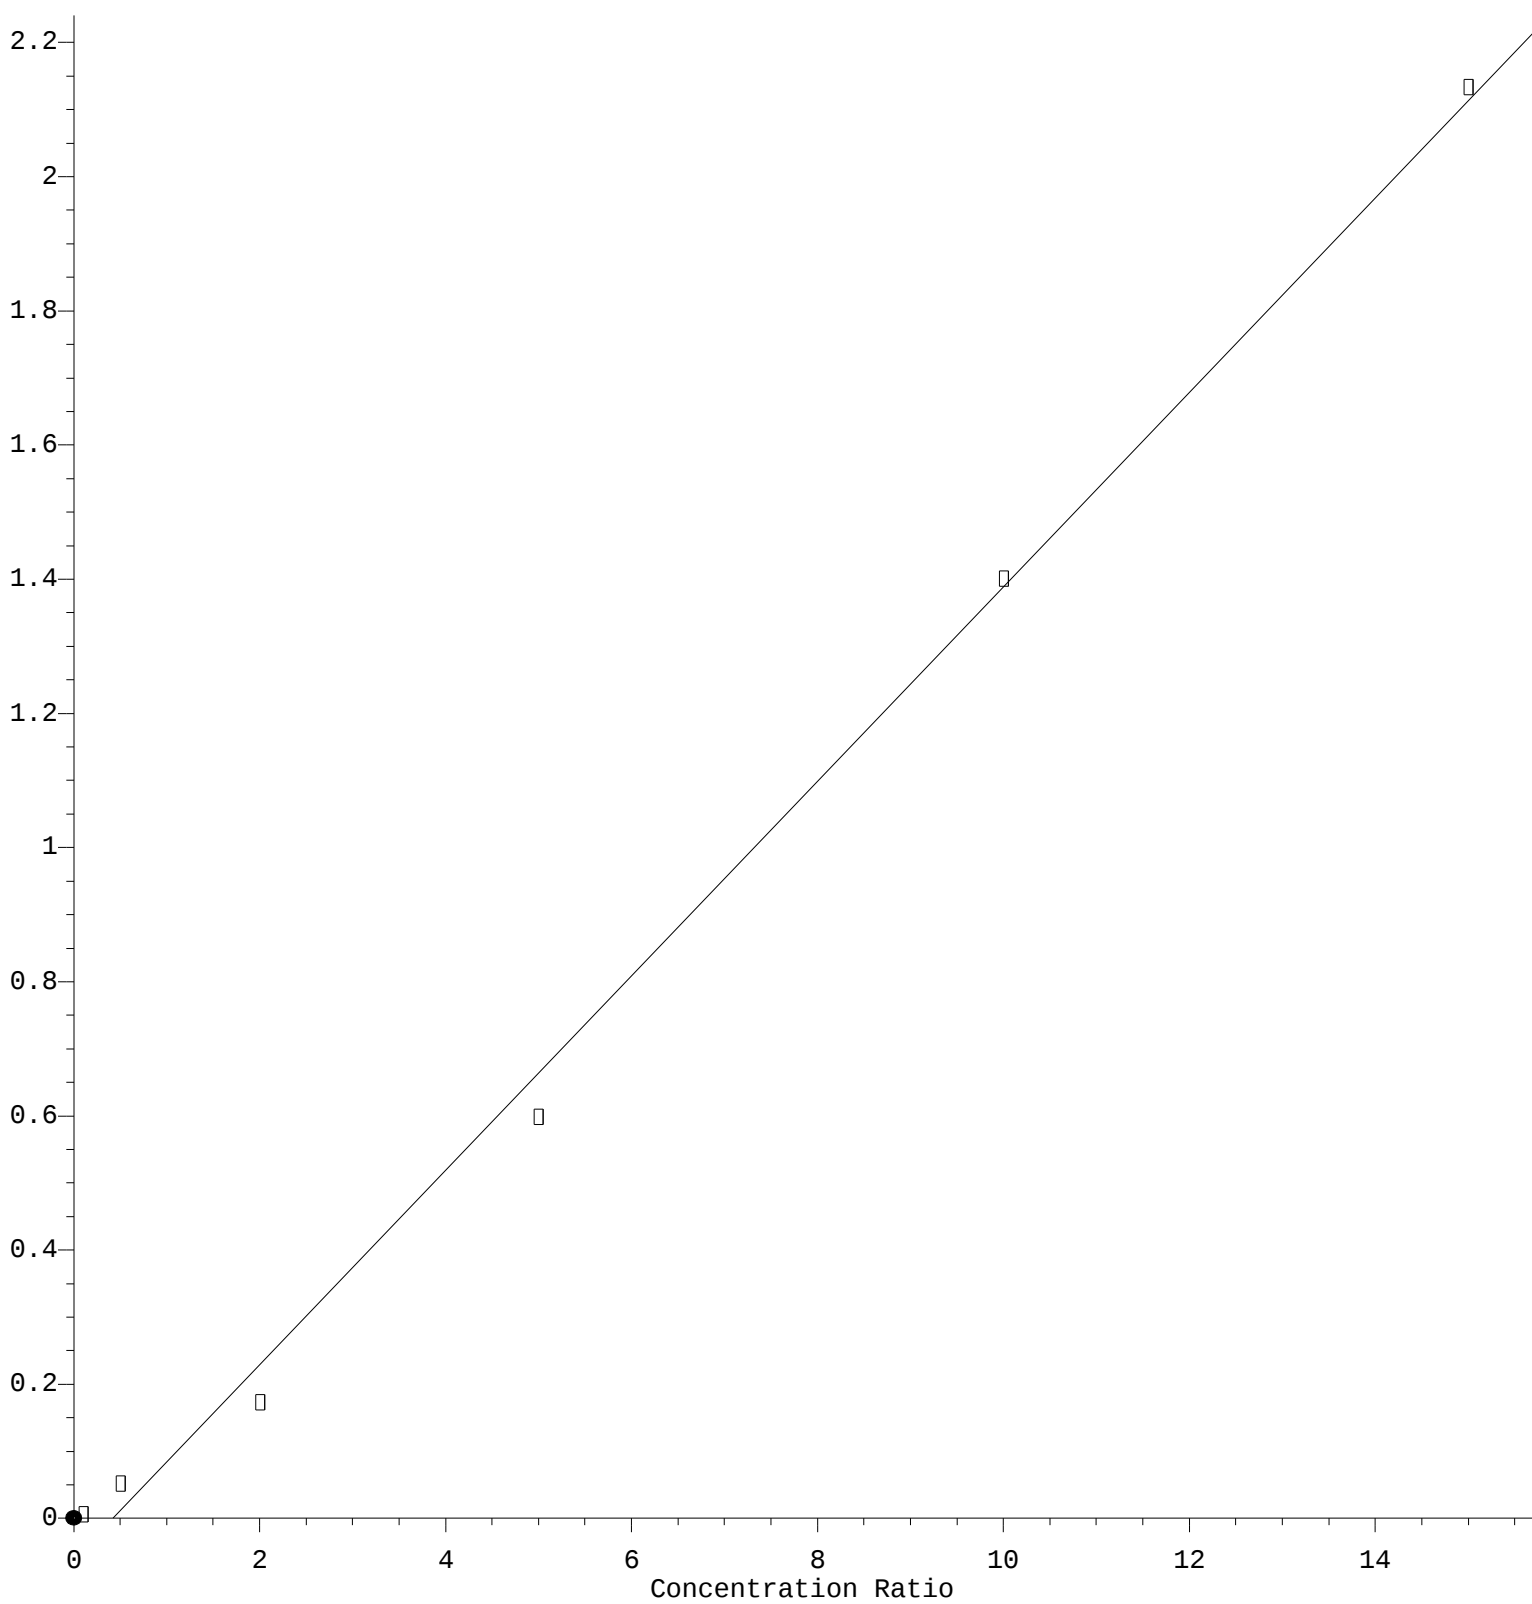

$$\text{Response} = 1.449\text{e-}001 * \text{Amt} - 6.030\text{e-}002$$


Coef of Det (r^2) = 0.996705 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070221W.M

Calibration Table Last Updated: Fri Jul 02 12:55:54 2021

Dibromochloromethane

Response Ratio

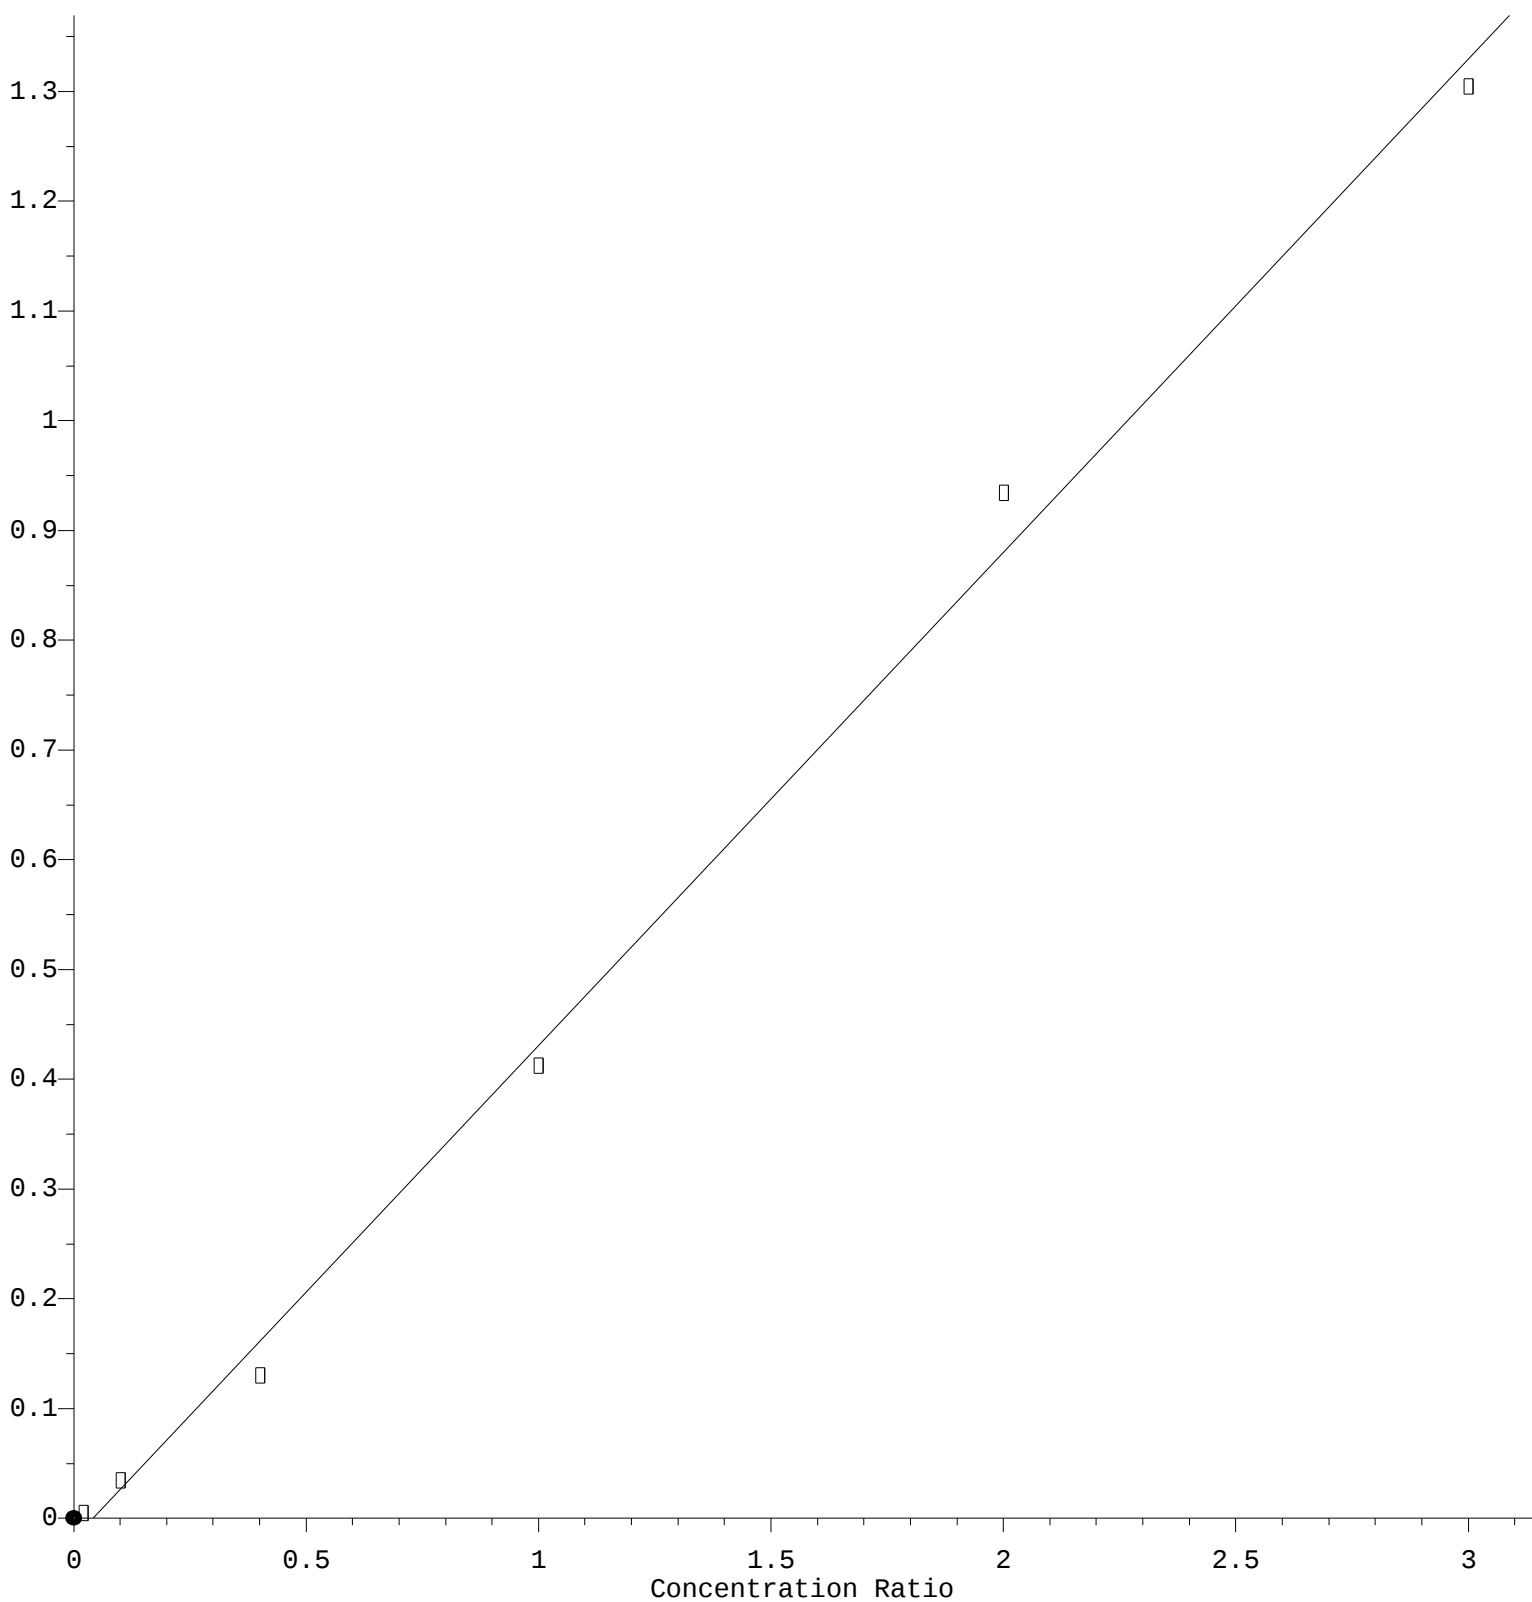

$$\text{Response} = 4.494\text{e-}001 * \text{Amt} - 1.840\text{e-}002$$


Coef of Det (r^2) = 0.996441 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070221W.M

Calibration Table Last Updated: Fri Jul 02 12:55:54 2021

Styrene

Response Ratio

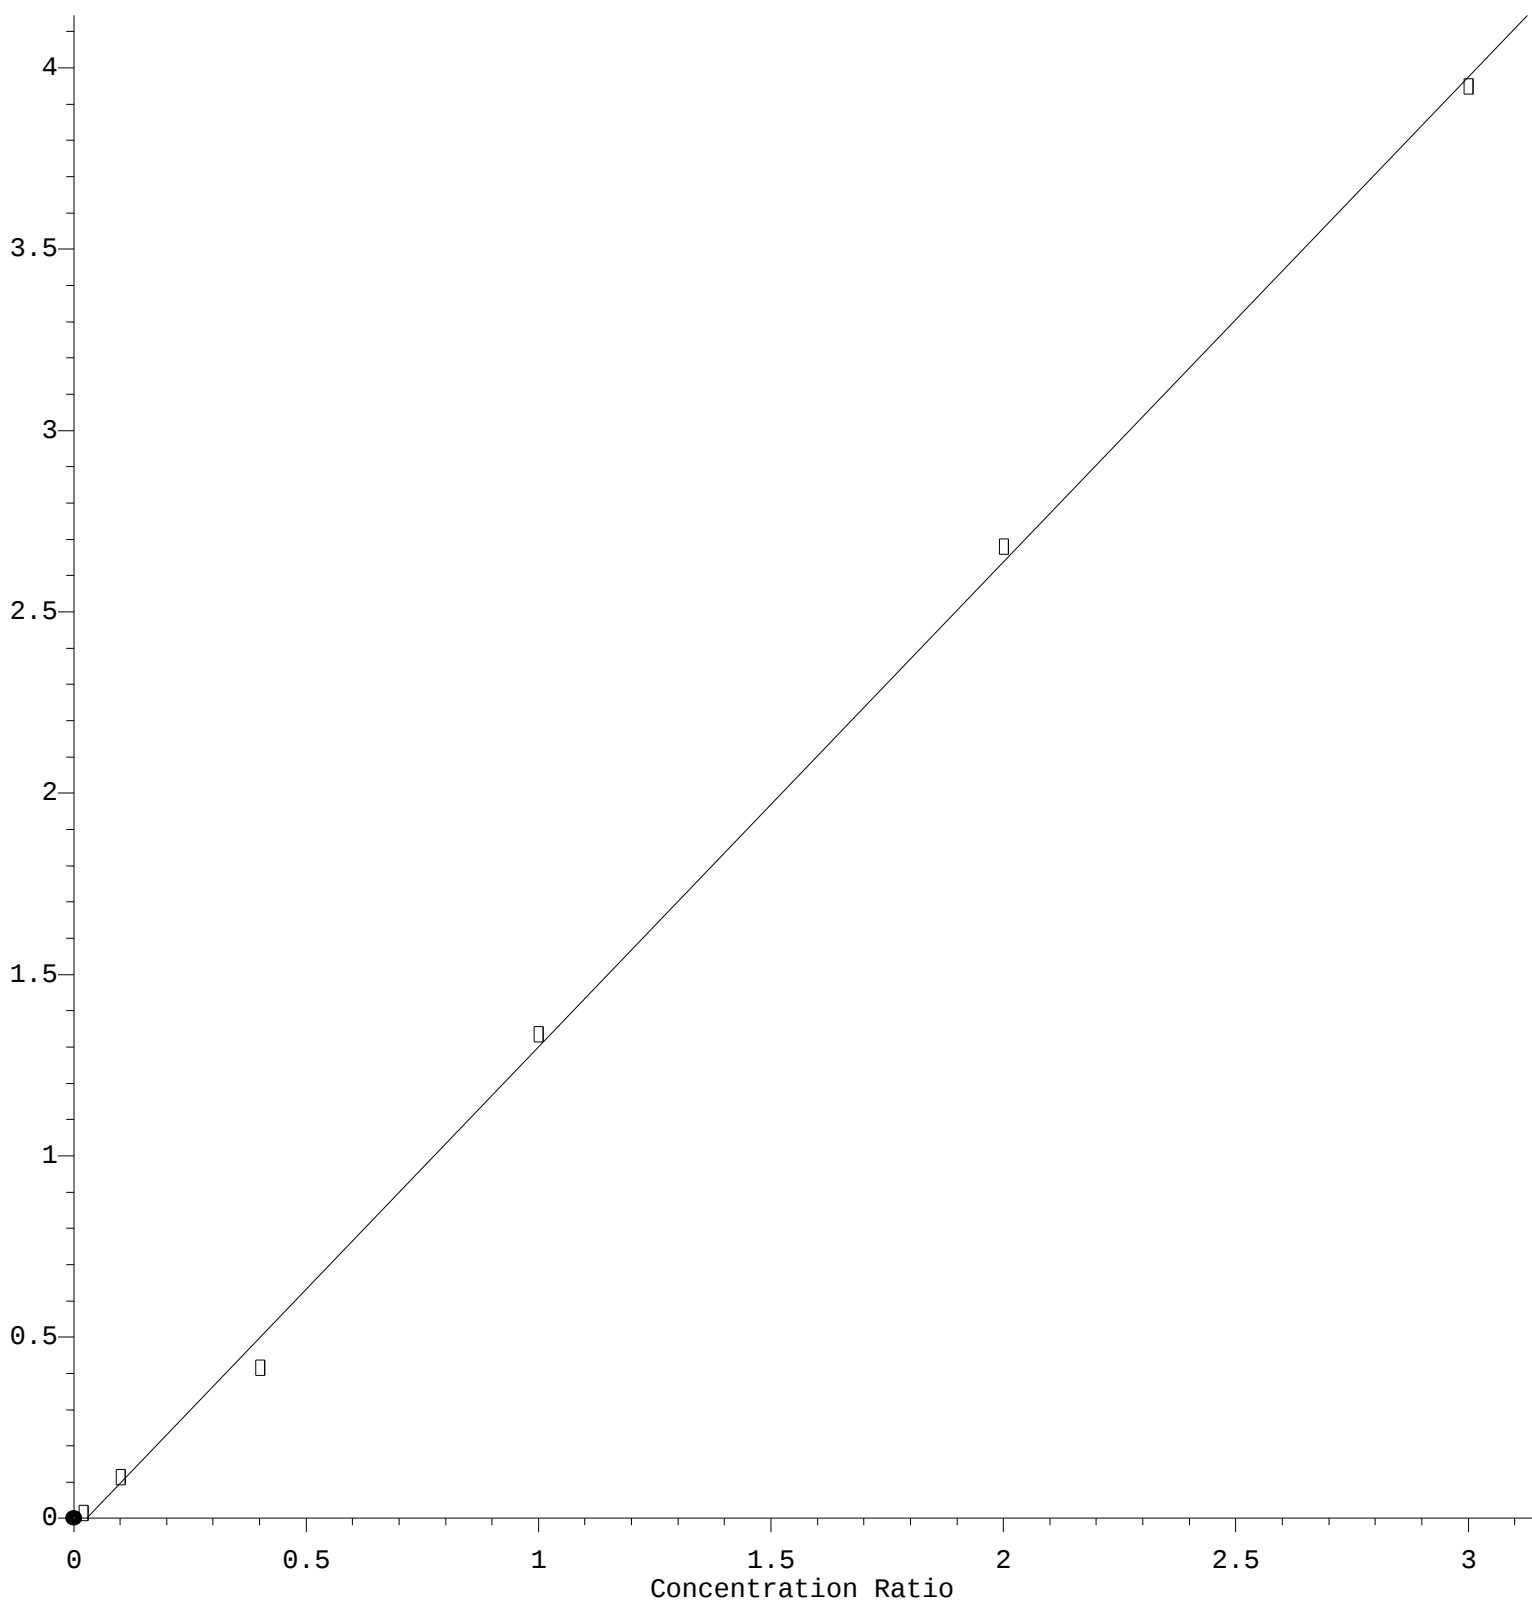

$$\text{Response} = 1.337\text{e}+000 * \text{Amt} - 3.599\text{e}-002$$


Coef of Det (r^2) = 0.999103 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070221W.M

Calibration Table Last Updated: Fri Jul 02 12:55:54 2021

Bromoform

Response Ratio

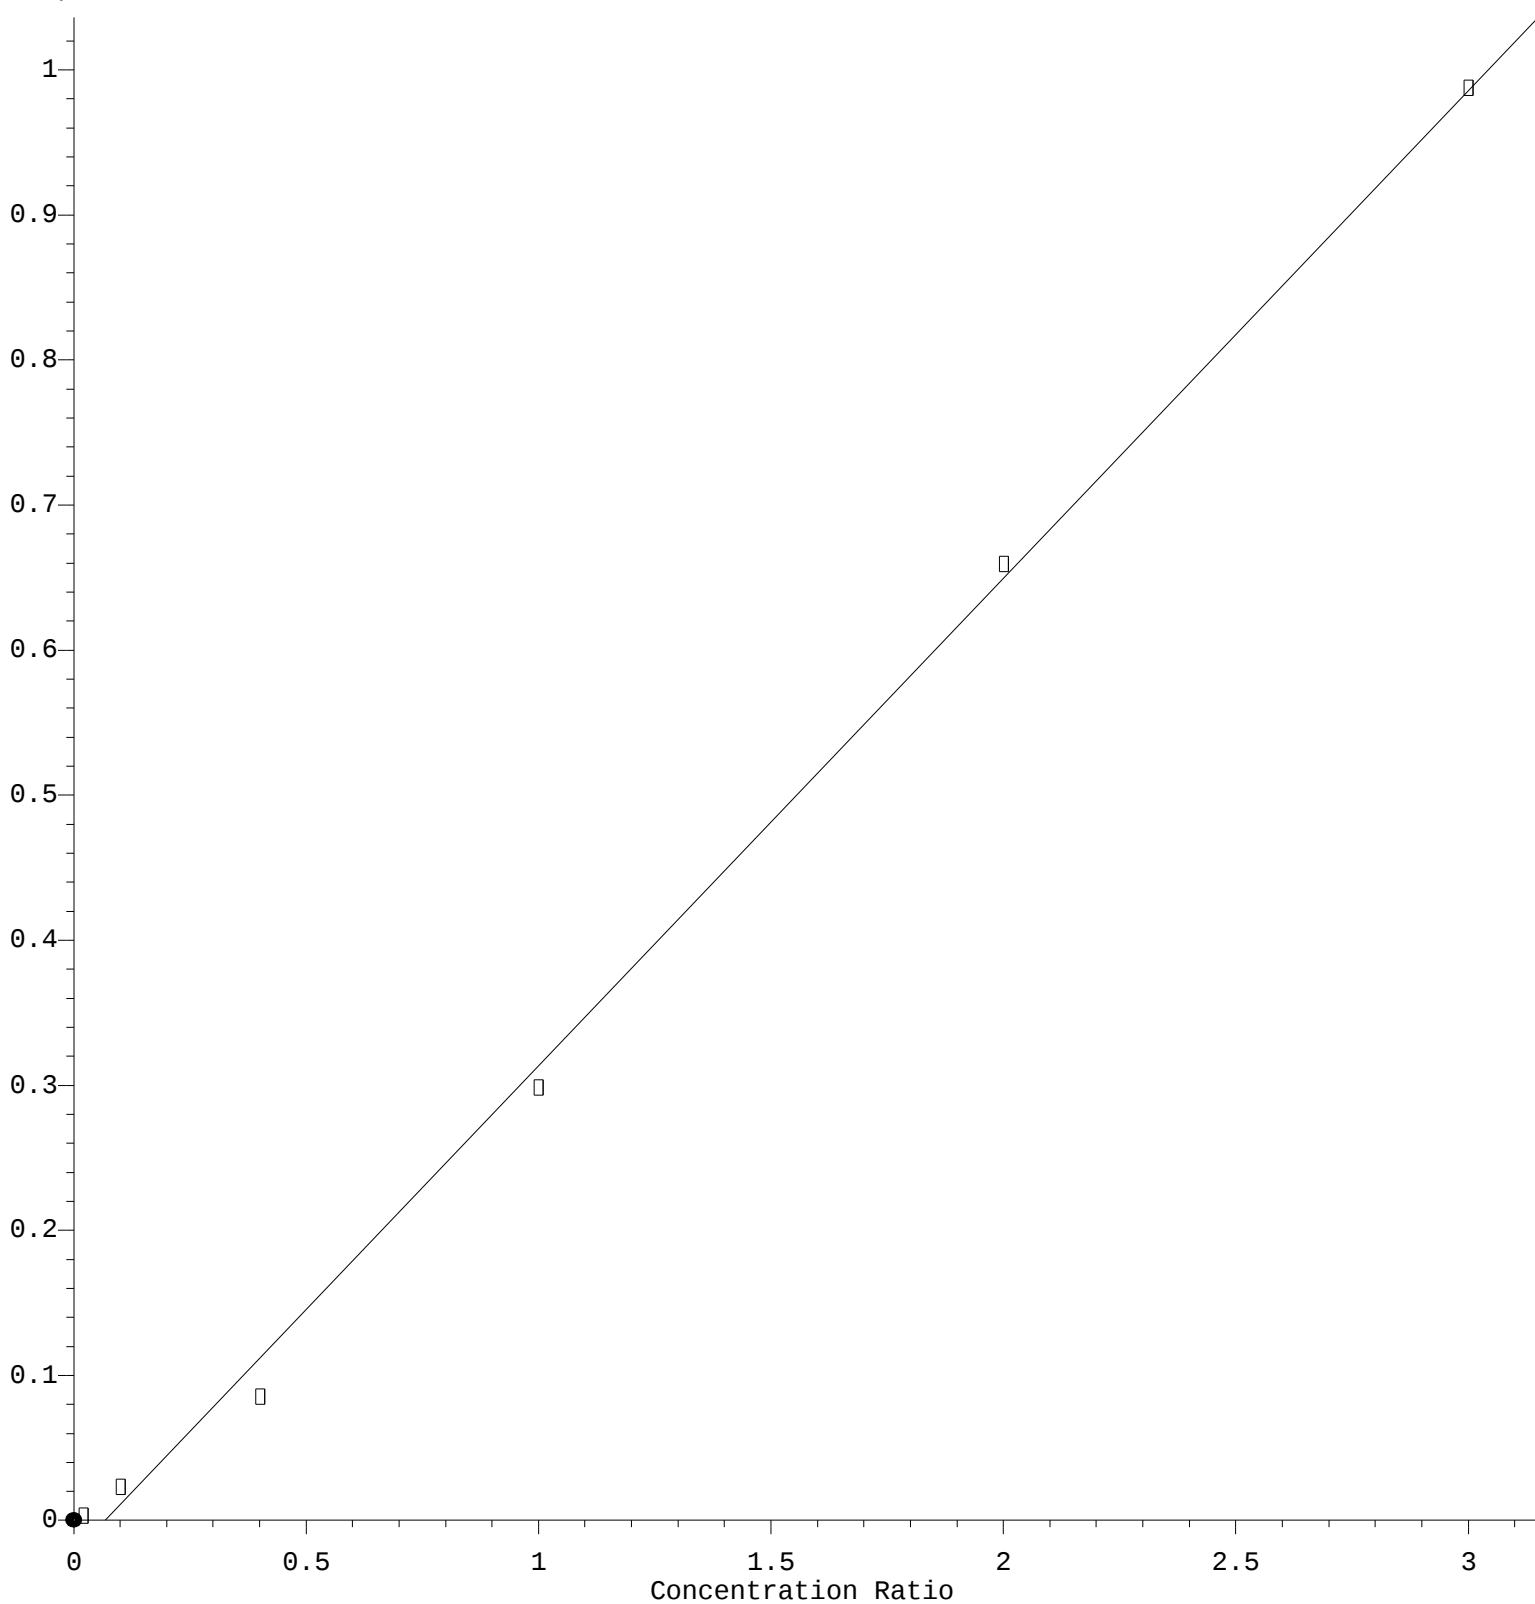

$$\text{Response} = 3.360\text{e-}001 * \text{Amt} - 2.253\text{e-}002$$


Coef of Det (r^2) = 0.998073 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070221W.M

Calibration Table Last Updated: Fri Jul 02 12:55:54 2021

Naphthalene

Response Ratio

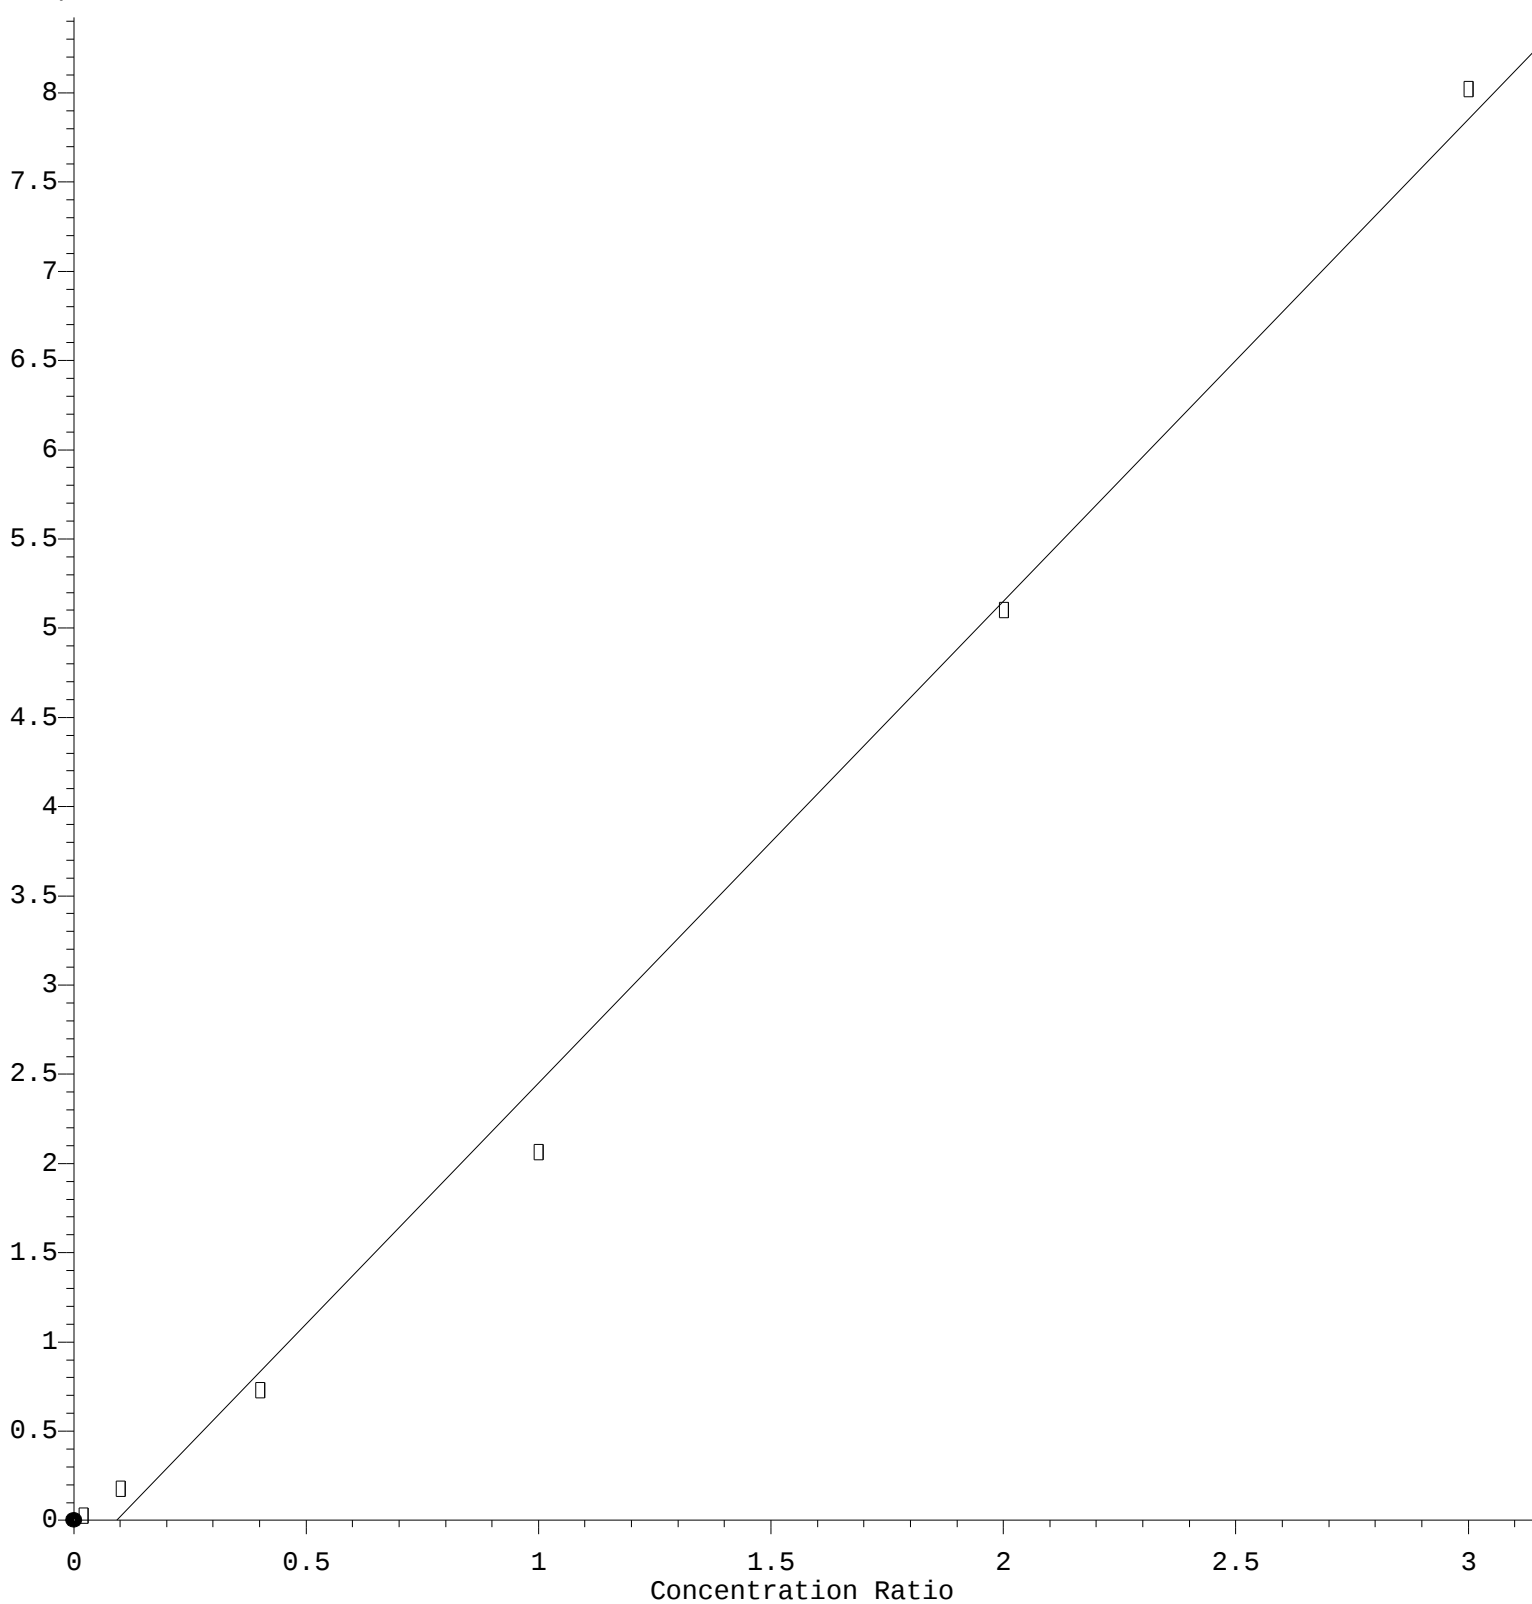

$$\text{Response} = 2.700\text{e}+000 * \text{Amt} - 2.482\text{e}-001$$

Coef of Det (r^2) = 0.994875 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070221W.M

Calibration Table Last Updated: Fri Jul 02 12:55:54 2021