
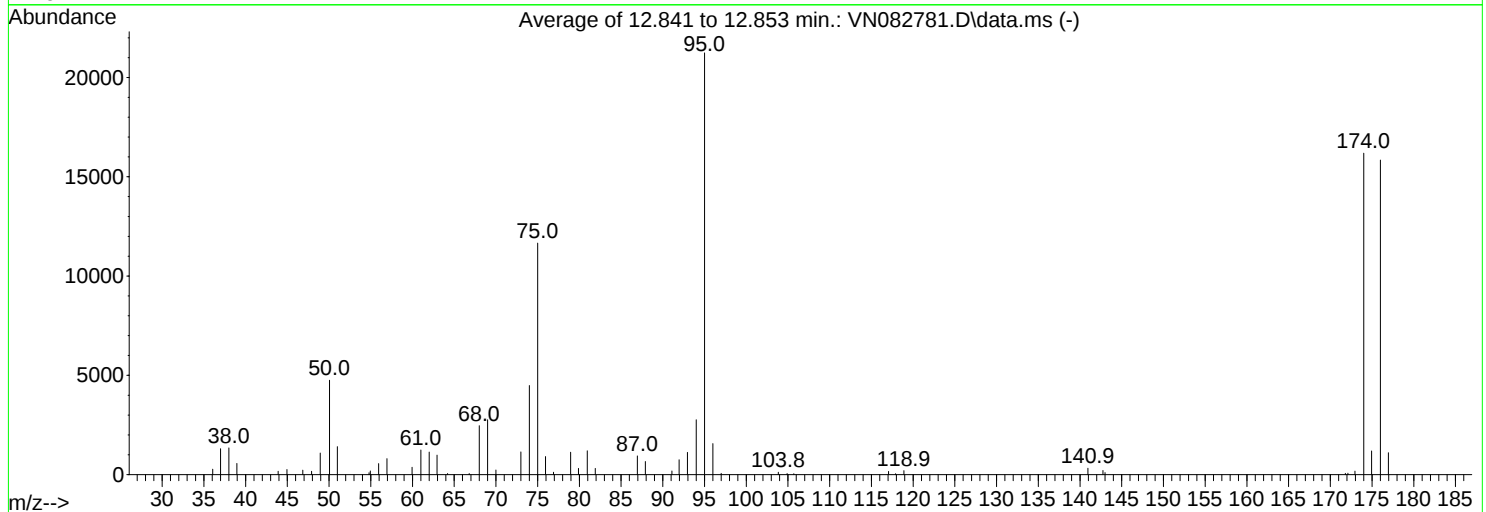


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070224\
Data File : VN082781.D
Acq On : 02 Jul 2024 09:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062724W.M
Title : SW846 8260
Last Update : Fri Jun 28 06:02:21 2024

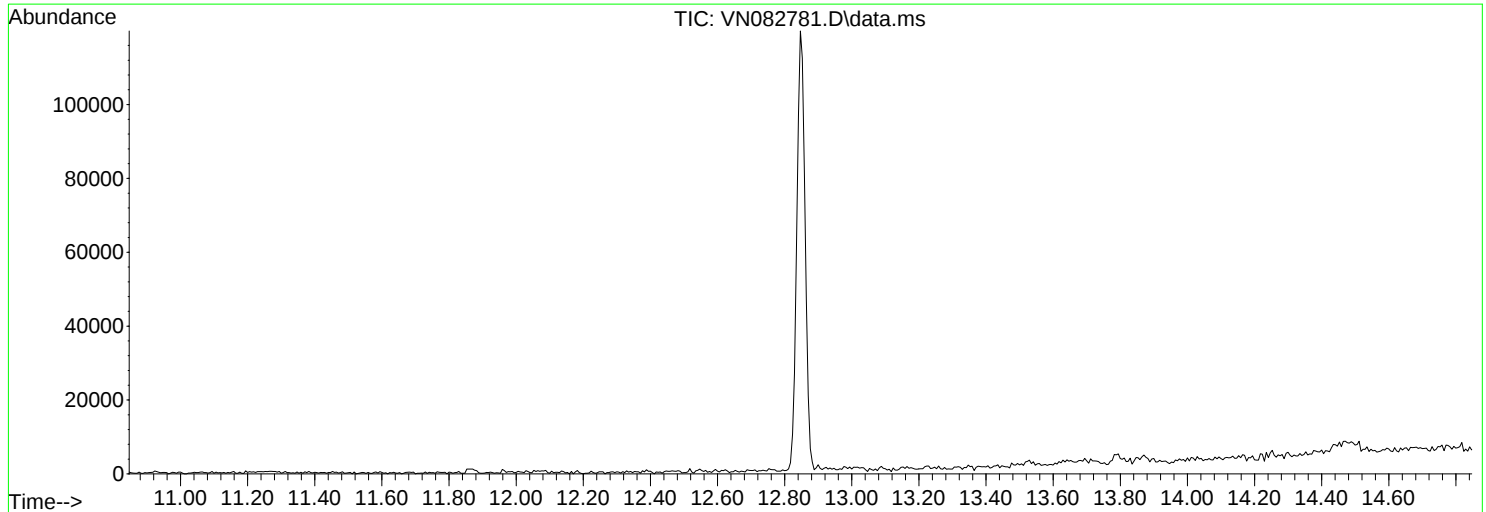

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.4	4753	PASS
75	95	30	60	54.9	11657	PASS
95	95	100	100	100.0	21240	PASS
96	95	5	9	7.4	1566	PASS
173	174	0.00	2	1.1	179	PASS
174	95	50	100	76.2	16187	PASS
175	174	5	9	7.4	1196	PASS
176	174	95	101	97.9	15839	PASS
177	176	5	9	7.0	1102	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	274	54.80	95	69.00	2766	86.95	94
37.00	1307	54.95	182	70.00	230	87.90	66
38.00	1343	55.95	556	73.00	1146	91.10	18
38.95	563	56.95	808	74.00	4490	91.95	74
43.90	168	59.95	367	75.00	11657	92.95	1120
44.95	260	61.00	1239	75.95	913	94.00	2767
46.85	227	62.00	1139	76.90	118	95.00	21240
47.90	166	62.95	987	78.95	1125	96.00	1566
48.95	1088	64.20	55	79.90	318	97.00	64
50.05	4753	66.80	59	80.95	1202	103.85	122
51.00	1410	68.00	2469	81.90	312	104.90	53

Average of 12.841 to 12.853 min.: VN082781.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.70	51	174.95	1196				
117.05	162	176.00	15839				
117.90	52	176.95	1102				
118.90	204						
140.95	319						
142.75	209						
143.00	109						
171.80	65						
172.10	72						
172.95	179						
174.00	16187						

Instrument :

MSVOA_N

ClientSampleId :

BFB