
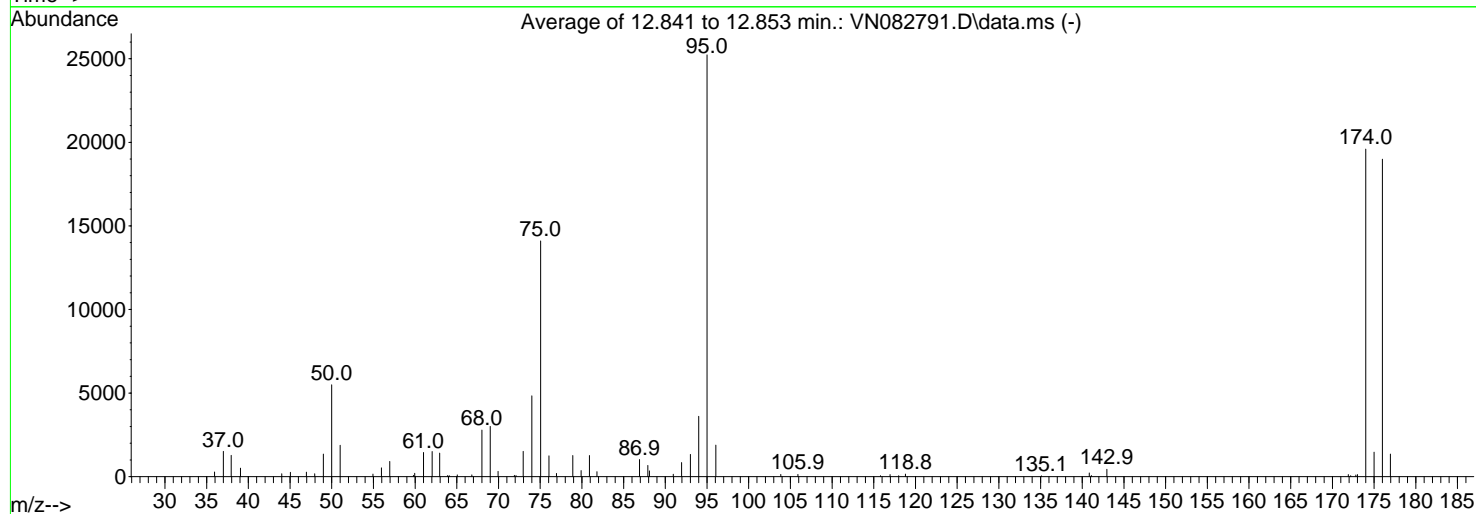


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070324\
 Data File : VN082791.D
 Acq On : 03 Jul 2024 09:13
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062724W.M
 Title : SW846 8260
 Last Update : Fri Jun 28 06:02:21 2024

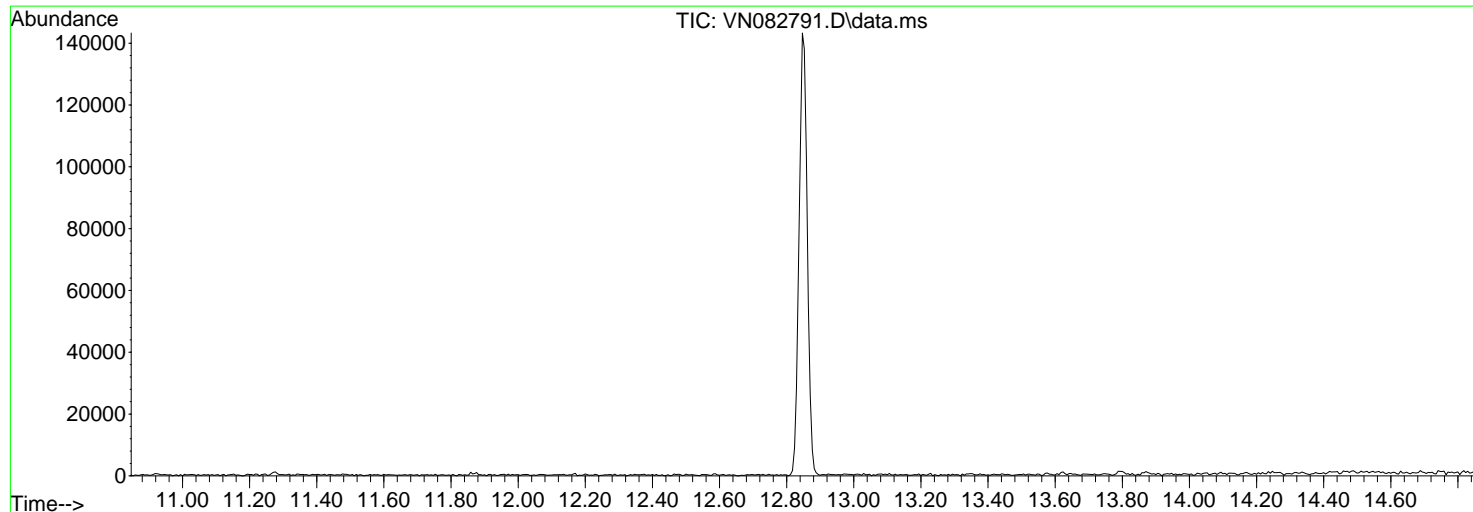

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	5491	PASS
75	95	30	60	55.9	14102	PASS
95	95	100	100	100.0	25232	PASS
96	95	5	9	7.5	1883	PASS
173	174	0.00	2	0.6	120	PASS
174	95	50	100	77.7	19598	PASS
175	174	5	9	7.5	1465	PASS
176	174	95	101	96.9	18987	PASS
177	176	5	9	7.1	1352	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	278	54.95	153	66.80	105	78.90	126
37.00	1510	55.95	523	68.00	2788	79.90	36
37.95	1272	56.95	905	69.00	3004	80.90	125
39.05	510	59.80	73	69.95	319	81.80	30
44.00	177	59.95	206	71.90	81	86.90	1026
45.05	261	61.00	1450	72.10	71	87.90	666
46.95	269	62.05	1503	72.95	1512	88.10	349
47.95	171	62.95	1411	74.00	4831	90.95	141
49.00	1352	63.90	65	75.05	14102	91.95	843
50.00	5491	64.10	57	76.05	1243	93.00	1333
51.00	1874	65.05	106	76.95	192	94.00	3607

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	25232	142.95	437				
96.05	1883	171.90	126				
103.85	133	172.20	62				
105.90	139	172.80	99				
115.80	54	173.00	120				
116.95	121	174.00	19598				
118.00	55	175.00	1465				
118.80	152	176.00	18987				
135.10	52	176.95	1352				
140.85	220						
141.10	72						