
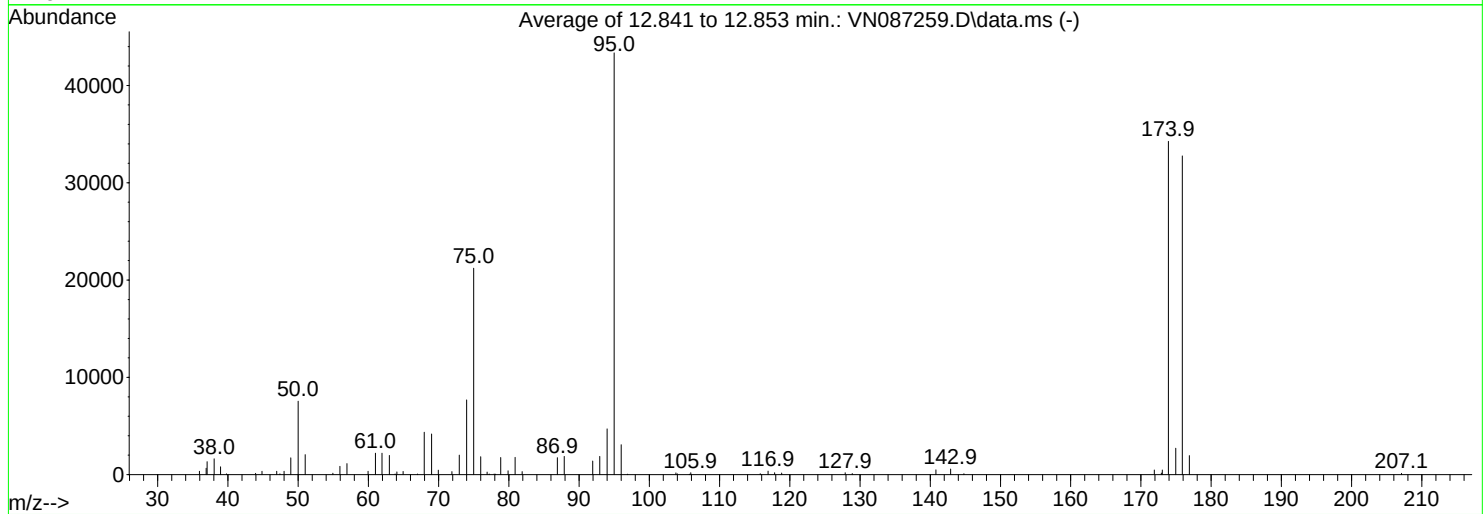


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070325\
Data File : VN087259.D
Acq On : 03 Jul 2025 10:17
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
Title : SW846 8260
Last Update : Tue Jul 01 03:15:00 2025

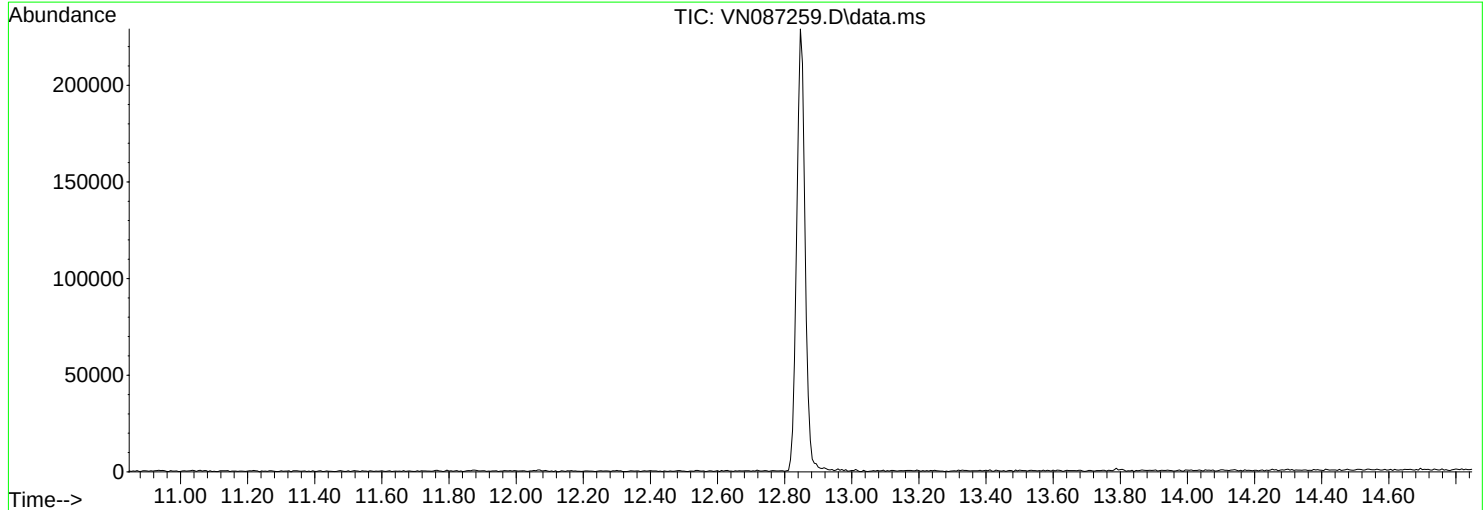

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	7554	PASS
75	95	30	60	48.9	21219	PASS
95	95	100	100	100.0	43355	PASS
96	95	5	9	7.1	3080	PASS
173	174	0.00	2	1.4	481	PASS
174	95	50	100	79.0	34261	PASS
175	174	5	9	7.9	2709	PASS
176	174	95	101	95.6	32760	PASS
177	176	5	9	6.0	1956	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	346	48.95	1726	64.05	281	76.90	261
36.90	666	50.00	7554	64.95	328	77.20	71
37.05	1337	51.00	2058	67.00	60	77.90	71
38.05	1626	54.95	147	67.95	4367	78.10	51
38.95	807	55.95	848	69.00	4172	78.85	1769
39.80	80	56.95	1132	69.95	462	79.90	396
43.95	140	59.95	344	71.90	311	80.90	1780
44.85	355	61.00	2213	72.95	2000	81.90	306
46.95	346	61.95	2199	74.00	7675	86.90	1740
47.40	82	63.00	1976	75.00	21219	87.90	1879
48.00	338	63.80	70	76.00	1848	91.95	1393

Average of 12.841 to 12.853 min.: VN087259.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	1881	117.85	196	174.95	2709		
94.00	4700	118.85	162	175.90	32760		
95.00	43355	127.90	193	176.90	1956		
96.00	3080	128.90	112	207.10	136		
96.90	50	140.80	486				
103.80	174	142.90	574				
104.00	80	144.80	98				
105.70	51	171.90	476				
105.90	190	172.90	167				
115.80	98	173.05	481				
116.90	364	173.90	34261				

Instrument :

MSVOA_N

ClientSampleId :

BFB