


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN070419\
Data File : VN056588.D
Acq On : 3 Jul 2019 16:12
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Title : SW846 8260
Last Update : Fri Jun 21 03:45:40 2019

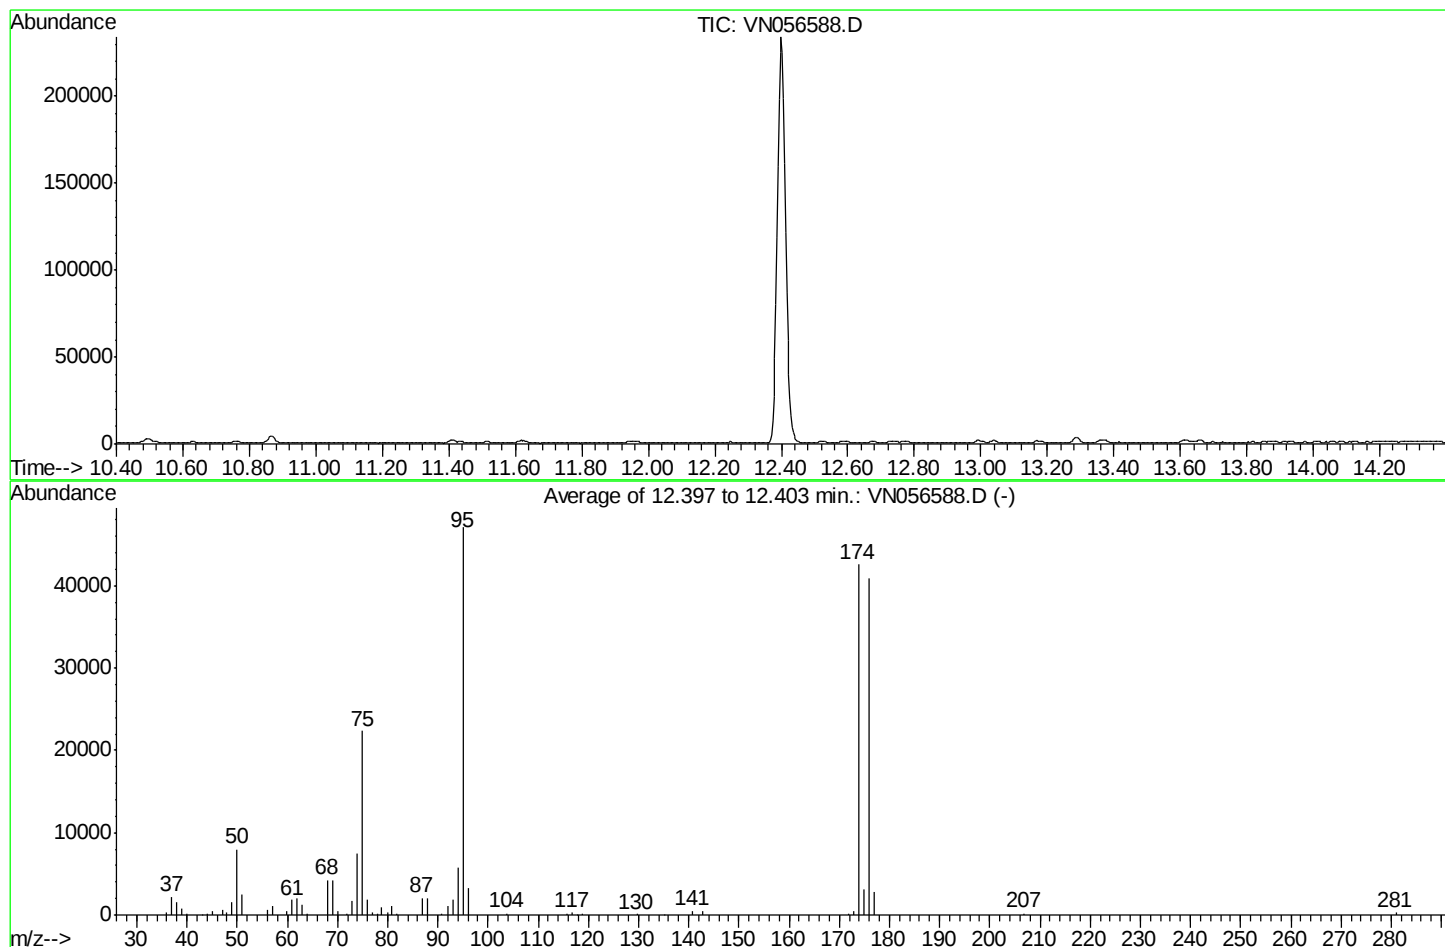

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8001	PASS
75	95	30	60	47.4	22322	PASS
95	95	100	100	100.0	47096	PASS
96	95	5	9	7.0	3319	PASS
173	174	0.00	2	1.1	469	PASS
174	95	50	100	90.3	42541	PASS
175	174	5	9	7.1	3039	PASS
176	174	95	101	96.0	40856	PASS
177	176	5	9	6.8	2779	PASS