

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070522\
 Data File : VN073318.D
 Acq On : 05 Jul 2022 16:23
 Operator : JC\MD
 Sample : N3564-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14B-11-1

Quant Time: Jul 06 01:15:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	276896	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	477043	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	449222	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	228985	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.375	65	181138	45.315	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	90.640%		
35) Dibromofluoromethane	7.951	113	151862	47.848	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.700%		
50) Toluene-d8	10.380	98	512268	45.444	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	90.880%		
62) 4-Bromofluorobenzene	12.668	95	229096	52.885	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	105.780%		
Target Compounds					Qvalue	
6) Chloroethane	2.975	64	836	0.426	ug/l #	42
11) Tert butyl alcohol	5.287	59	339	0.350	ug/l #	72
16) Acetone	4.228	43	59952	26.720	ug/l	91
18) Methyl Acetate	4.792	43	3244	0.516	ug/l #	72
20) Methylene Chloride	5.016	84	206357	52.332	ug/l	89
25) 2-Butanone	7.269	43	13627	3.815	ug/l	96
29) Tetrahydrofuran	7.628	42	1397	0.571	ug/l #	66
31) Cyclohexane	8.016	56	13925	2.127	ug/l #	67
36) 1,1-Dichloropropene	8.016	75	23588	4.830	ug/l #	48
37) Ethyl Acetate	7.345	43	44662	6.053	ug/l	98
38) Carbon Tetrachloride	8.016	117	29544	5.850	ug/l #	16
39) Methylcyclohexane	9.398	83	52532	8.640	ug/l	93
43) Isopropyl Acetate	8.492	43	201333	18.985	ug/l #	85
48) Methyl methacrylate	9.480	41	6510	1.326	ug/l #	37
49) 1,4-Dioxane	9.551	88	64	0.687	ug/l #	1
51) 4-Methyl-2-Pentanone	10.274	43	8178	1.216	ug/l	98
54) cis-1,3-Dichloropropene	10.180	75	59381	9.890	ug/l #	66
55) 1,1,2-Trichloroethane	10.816	97	4808	1.254	ug/l #	23
56) Ethyl methacrylate	10.722	69	2979	0.481	ug/l #	1
57) 1,3-Dichloropropane	11.027	76	4068	0.619	ug/l #	42
59) 2-Hexanone	10.998	43	161678	31.539	ug/l #	21
68) m/p-Xylenes	11.886	106	1470	0.211	ug/l #	34
73) Isopropylbenzene	12.521	105	7321	0.370	ug/l	94
74) N-amyl acetate	12.304	43	3539	0.357	ug/l #	46
76) 1,2,3-Trichloropropane	12.668	75	122226	20.414	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.668	75	122226	55.983	ug/l #	10
83) tert-Butylbenzene	13.257	119	3074	0.213	ug/l	91
85) sec-Butylbenzene	13.439	105	5206	0.268	ug/l	90
90) Hexachloroethane	14.151	117	2492	0.853	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	14.398	75	618	0.387	ug/l	65
95) Naphthalene	15.421	128	4487	0.254	ug/l #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070522\
Data File : VN073318.D
Acq On : 05 Jul 2022 16:23
Operator : JC\MD
Sample : N3564-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1

Quant Time: Jul 06 01:15:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




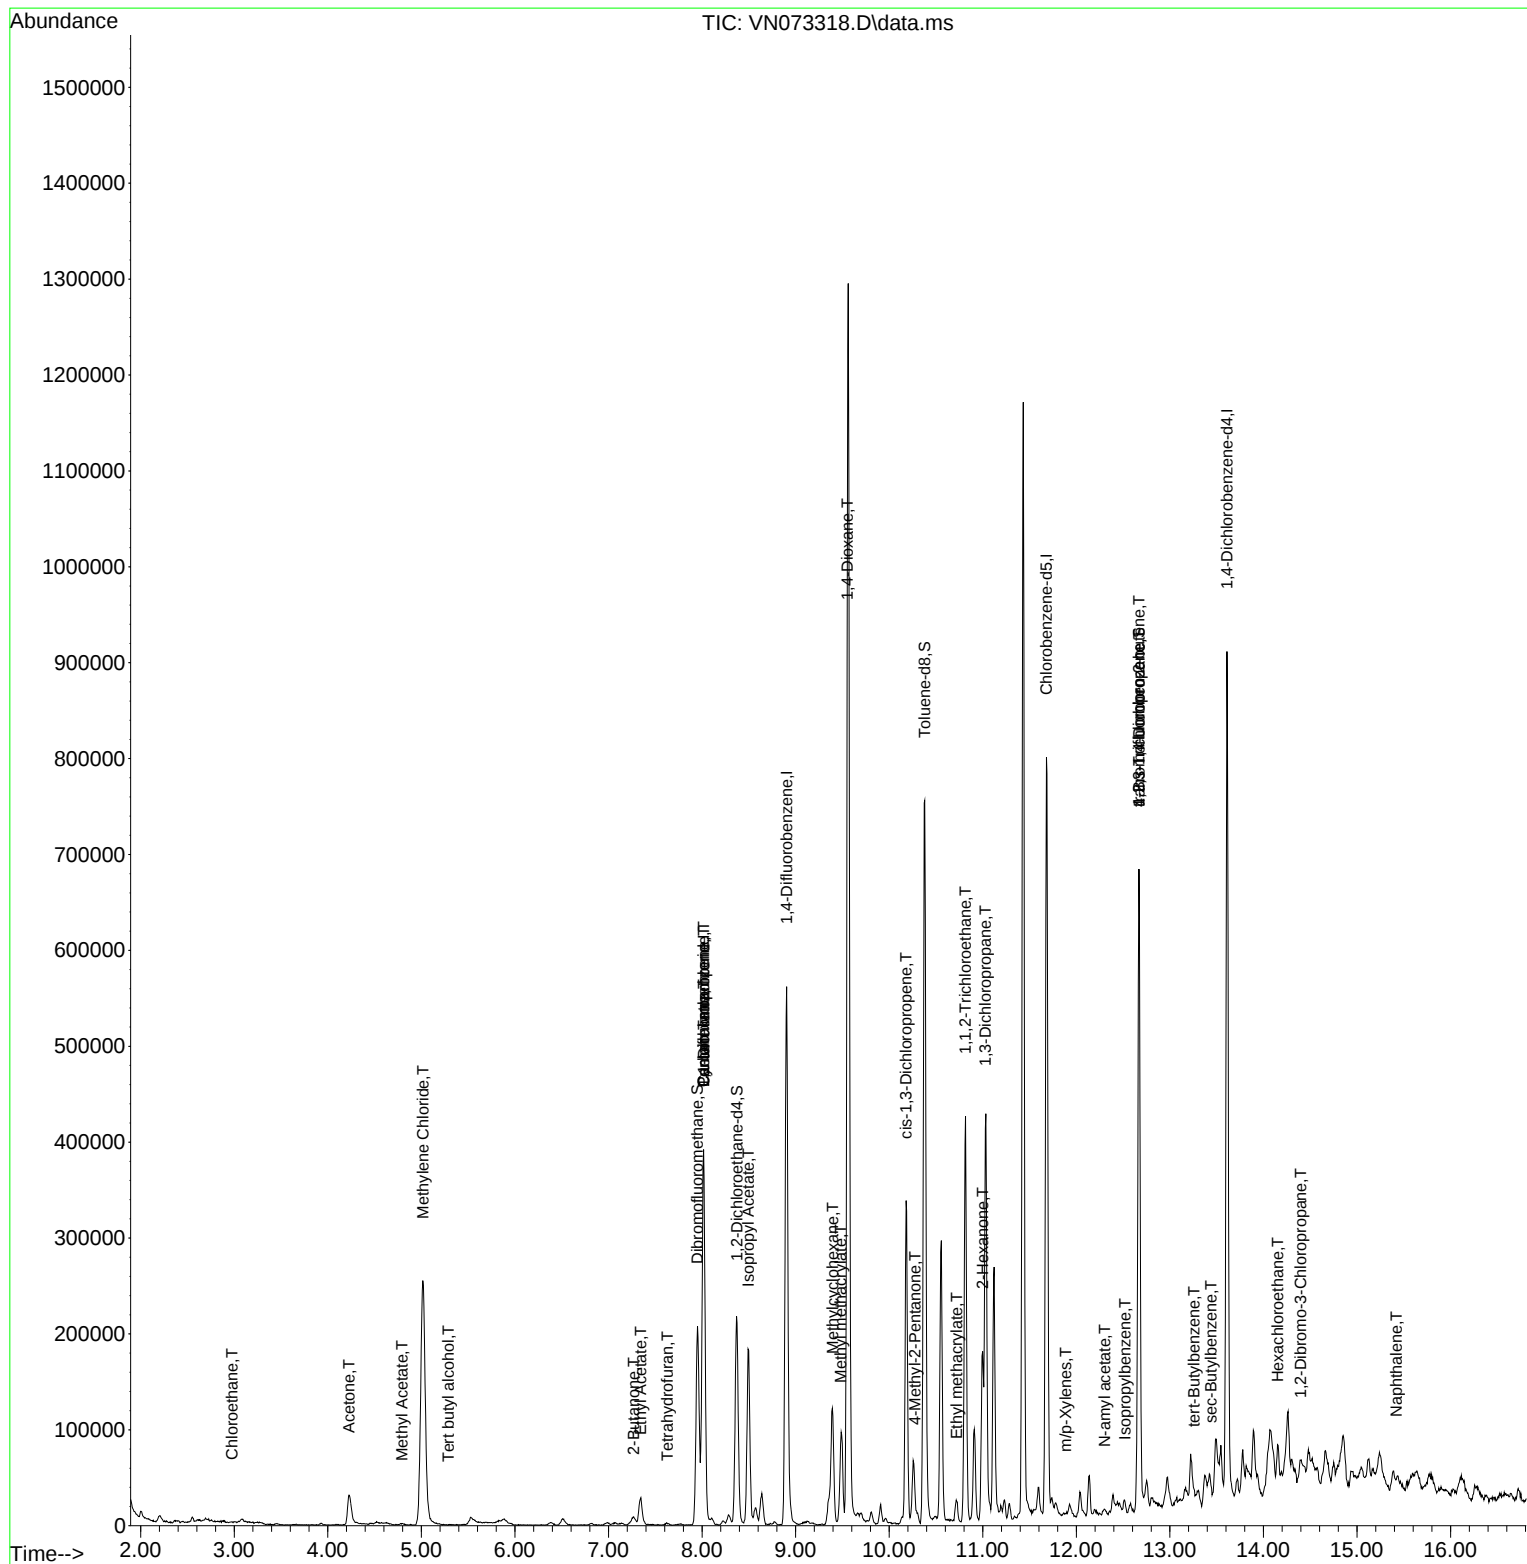


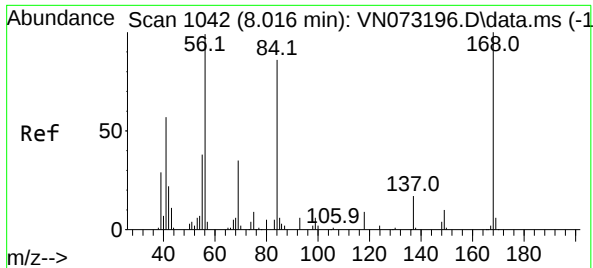

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion:168 Resp: 276896
Ion Ratio Lower Upper
168 100
99 61.4 42.3 63.5

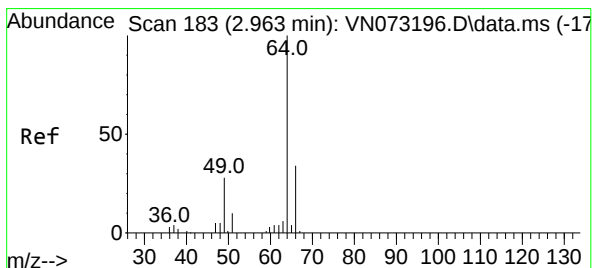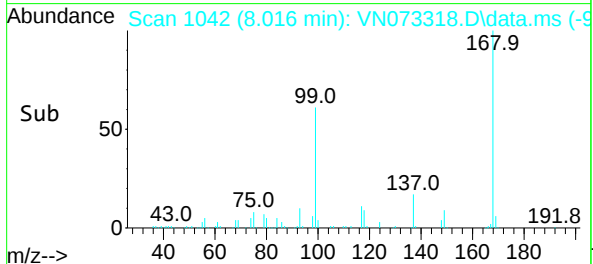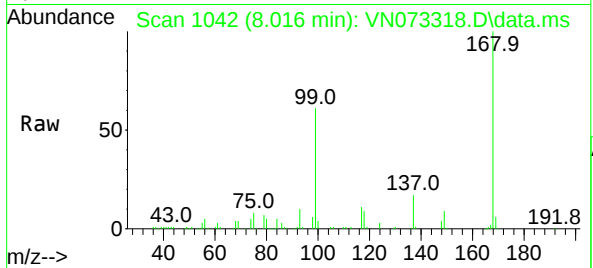

#6
Chloroethane
Concen: 0.426 ug/l
RT: 2.975 min Scan# 185
Delta R.T. 0.012 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 64 Resp: 836
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#


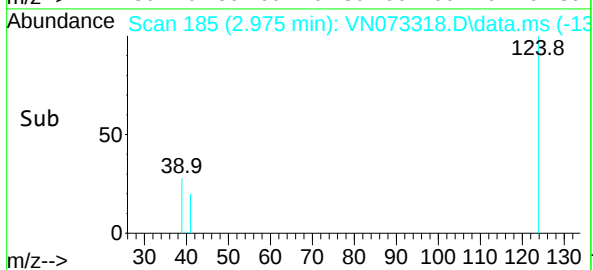

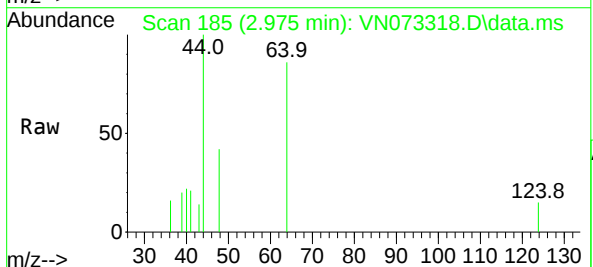


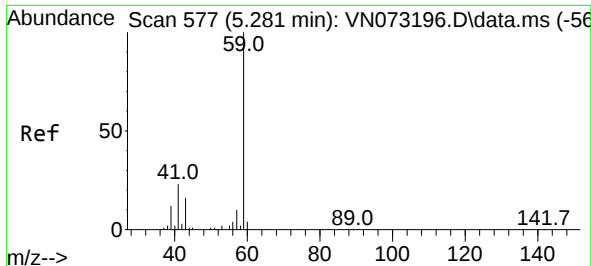

#11
Tert butyl alcohol
Concen: 0.350 ug/l
RT: 5.287 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion: 59 Resp: 339
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

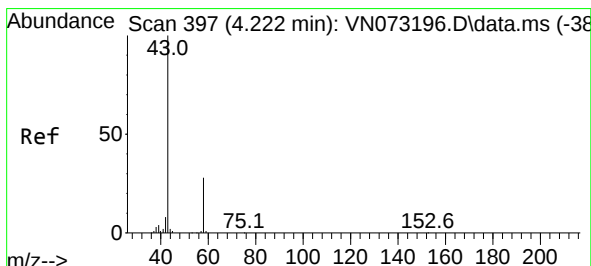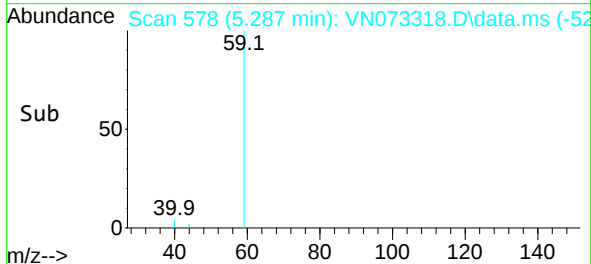

#16
Acetone
Concen: 26.720 ug/l
RT: 4.228 min Scan# 398
Delta R.T. 0.006 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 43 Resp: 59952
Ion Ratio Lower Upper
43 100
58 27.6 26.0 39.0



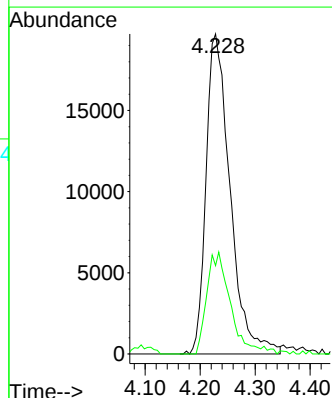
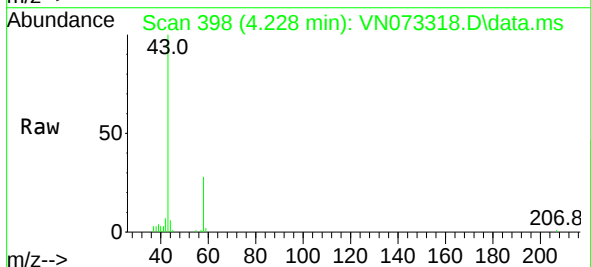




#18
Methyl Acetate
Concen: 0.516 ug/l
RT: 4.792 min Scan# 491
Delta R.T. 0.017 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion: 43 Resp: 3244
Ion Ratio Lower Upper
43 100
74 12.7 21.6 32.4#

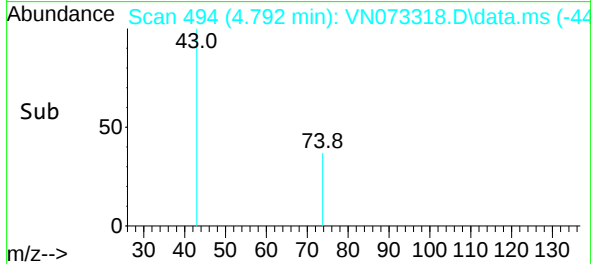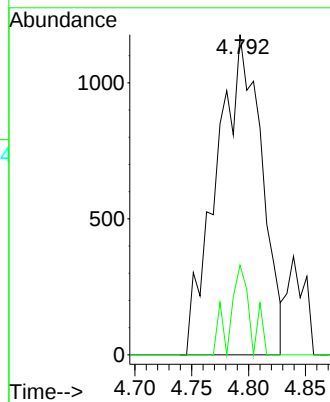

#20
Methylene Chloride
Concen: 52.332 ug/l
RT: 5.016 min Scan# 532
Delta R.T. 0.000 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 84 Resp: 206357
Ion Ratio Lower Upper
84 100
49 126.7 88.3 132.5
51 40.8 28.2 42.2
86 60.8 50.6 76.0


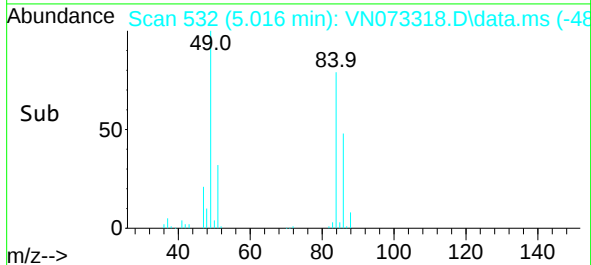
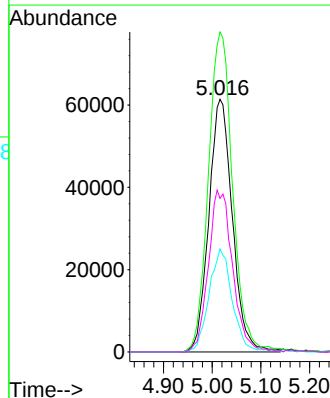
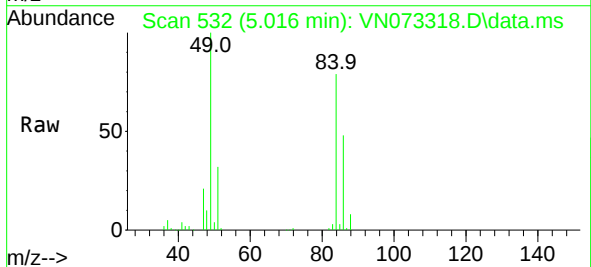




#25
2-Butanone
Concen: 3.815 ug/l
RT: 7.269 min Scan# 913
Delta R.T. 0.012 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion: 43 Resp: 13627
Ion Ratio Lower Upper
43 100
72 27.6 23.7 35.5

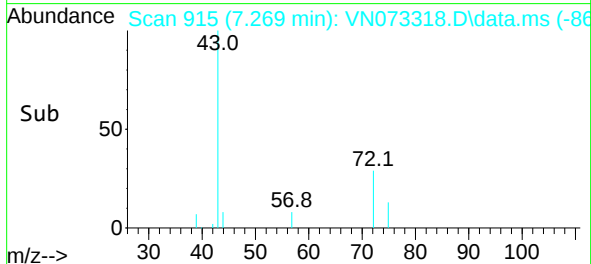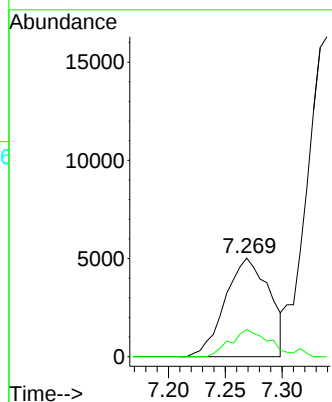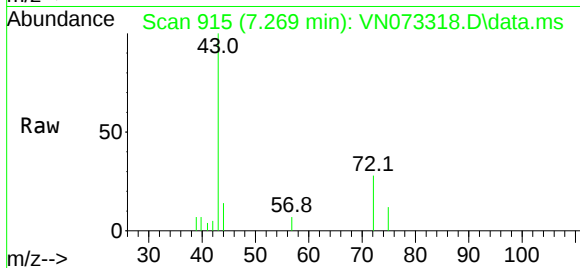

#29
Tetrahydrofuran
Concen: 0.571 ug/l
RT: 7.628 min Scan# 976
Delta R.T. 0.018 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 42 Resp: 1397
Ion Ratio Lower Upper
42 100
72 38.6 39.7 59.5#
71 11.0 36.6 55.0#


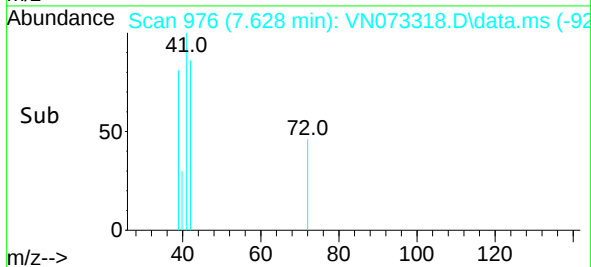
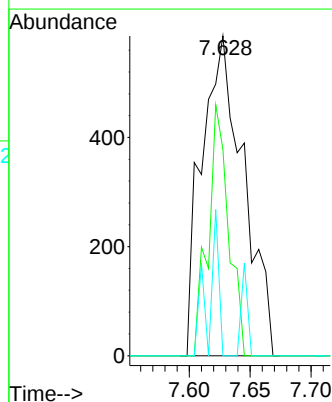
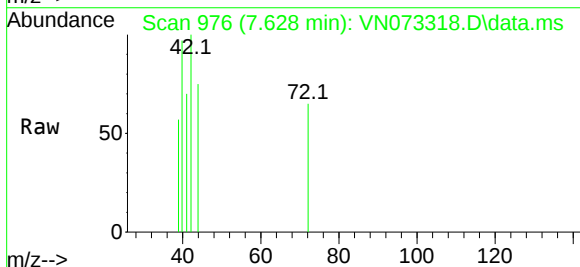




#31
Cyclohexane
Concen: 2.127 ug/l
RT: 8.016 min Scan# 1103
Delta R.T. -0.006 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion: 56 Resp: 13925
Ion Ratio Lower Upper
56 100
69 88.2 27.8 41.8#
84 106.9 76.9 115.3

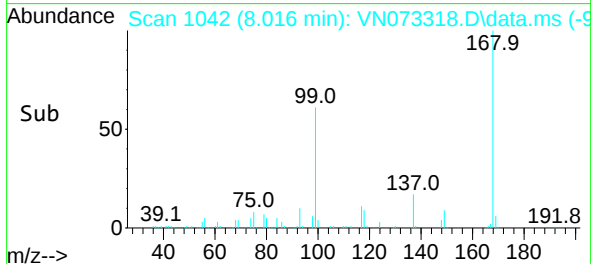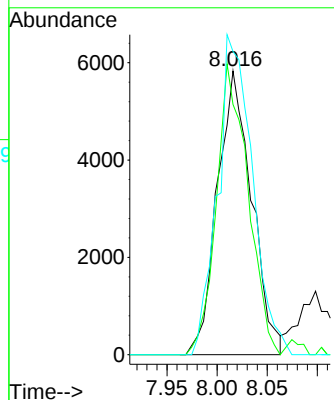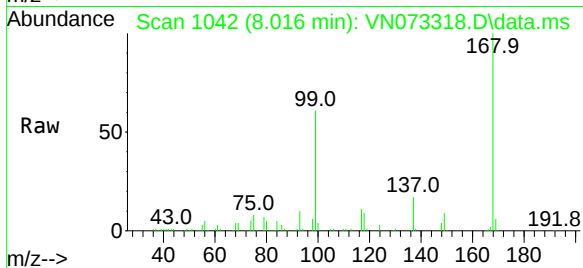

#33
1,2-Dichloroethane-d4
Concen: 45.315 ug/l
RT: 8.375 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 65 Resp: 181138
Ion Ratio Lower Upper
65 100
67 51.4 0.0 104.8

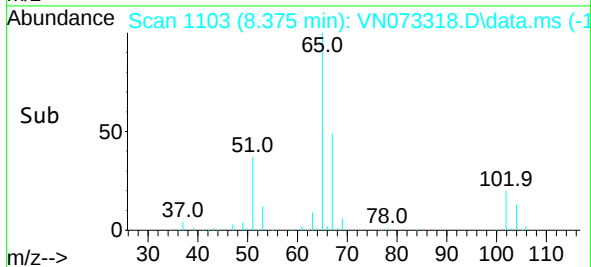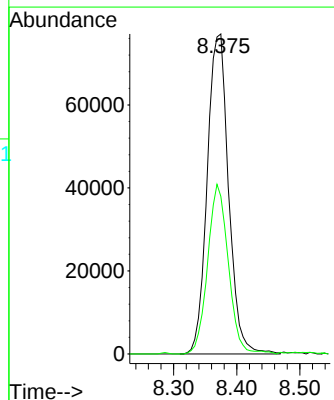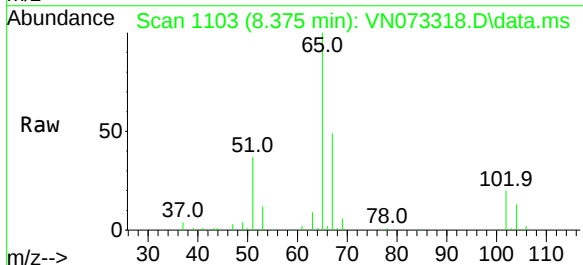

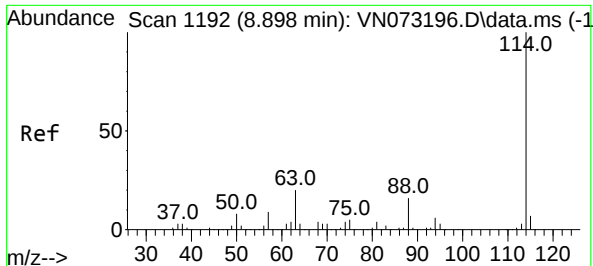

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23

Instrument :

MSVOA_N

ClientSampleId :

WC-14B-11-1





Tgt Ion:114 Resp: 477043

Ion Ratio Lower Upper

114 100

63 21.7 0.0 40.0

88 15.4 0.0 32.6

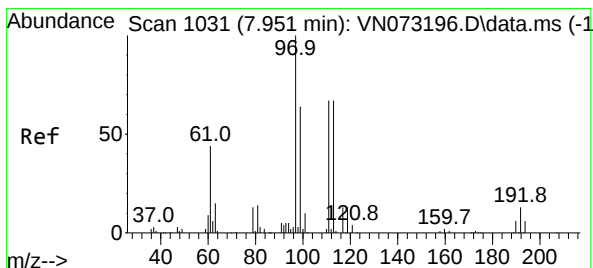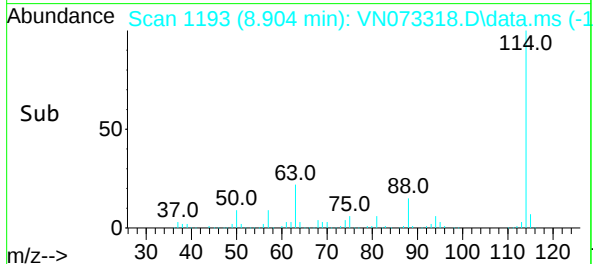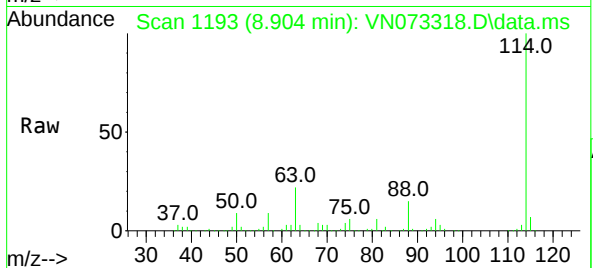

#35

Dibromofluoromethane

Concen: 47.848 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23




Tgt Ion:113 Resp: 151862


Ion Ratio Lower Upper

113 100

111 104.3 81.4 122.0

192 18.8 17.0 25.6

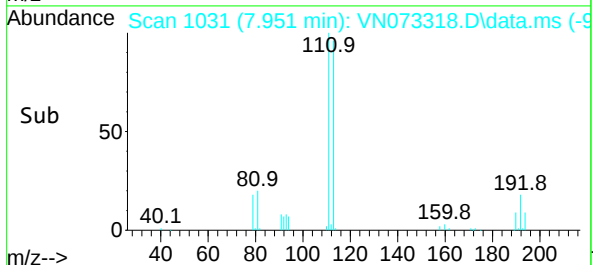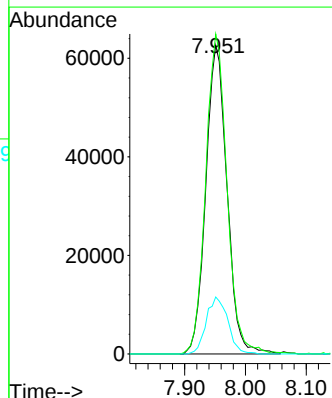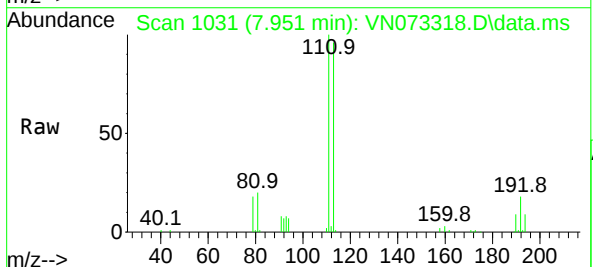

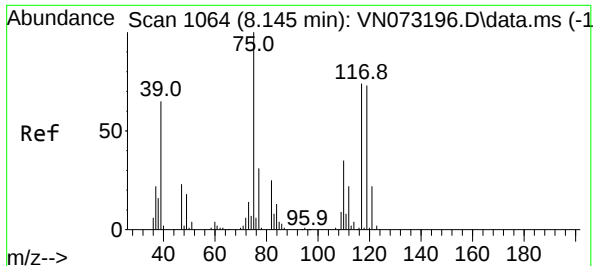

#36

1,1-Dichloropropene

Concen: 4.830 ug/l

RT: 8.016 min Scan# 1

Delta R.T. -0.129 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23

Instrument :

MSVOA_N

ClientSampleId :

WC-14B-11-1





Tgt Ion: 75 Resp: 23588

Ion Ratio Lower Upper

75 100

110 8.1 18.3 54.8#

77 0.0 25.1 37.7#

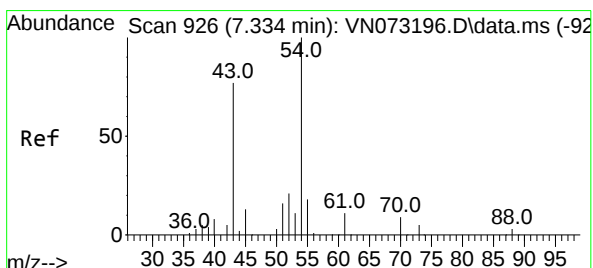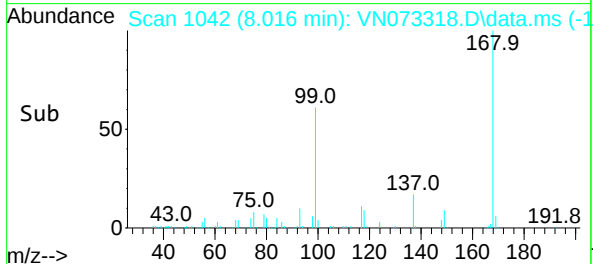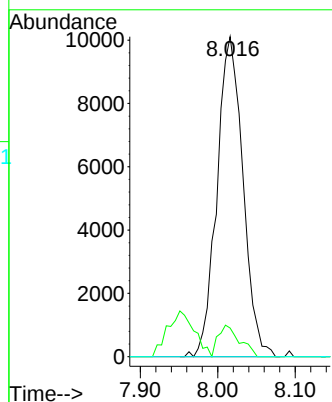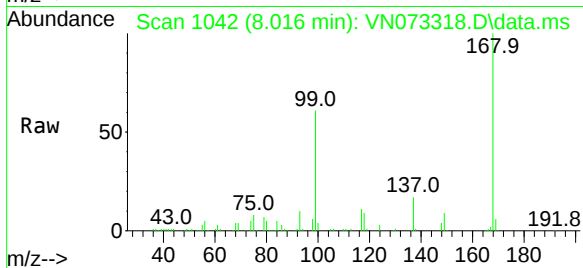

#37

Ethyl Acetate

Concen: 6.053 ug/l

RT: 7.345 min Scan# 928

Delta R.T. 0.011 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23




Tgt Ion: 43 Resp: 44662


Ion Ratio Lower Upper

43 100

61 13.7 11.8 17.6

70 10.6 9.3 13.9


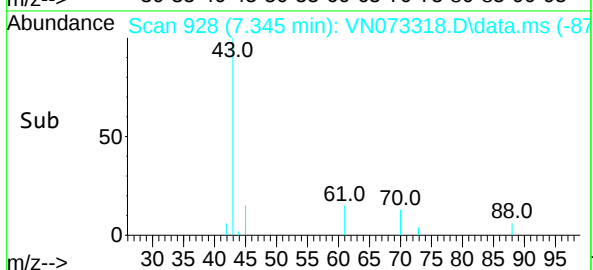

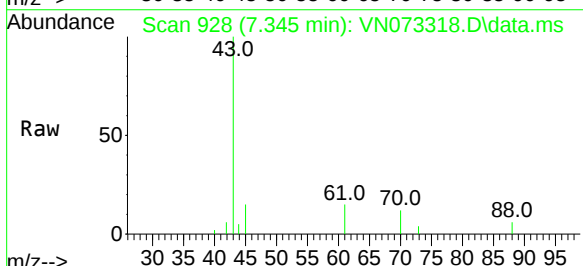


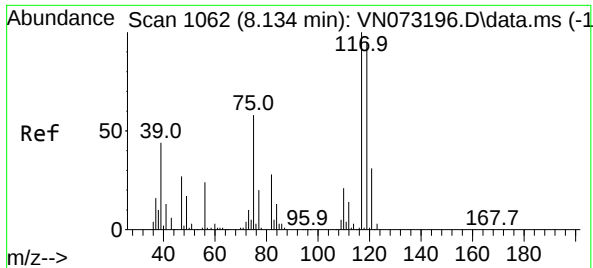

#38
Carbon Tetrachloride
Concen: 5.850 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.118 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion:117 Resp: 29544
Ion Ratio Lower Upper
117 100
119 4.5 75.8 113.8#
121 0.0 24.6 37.0#

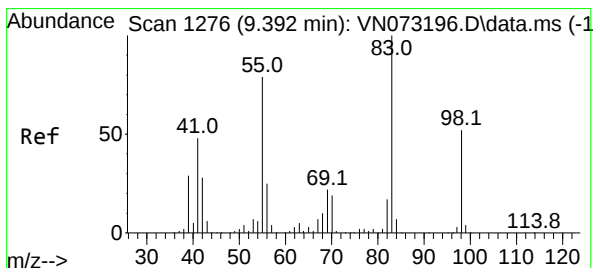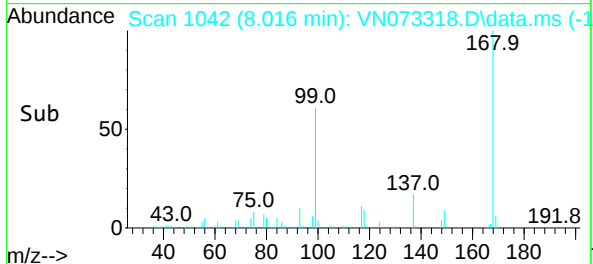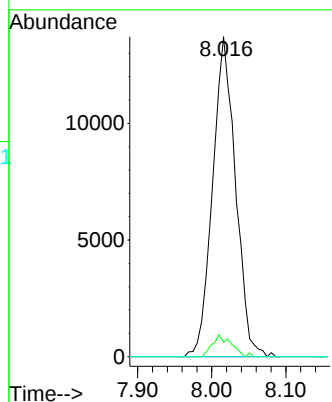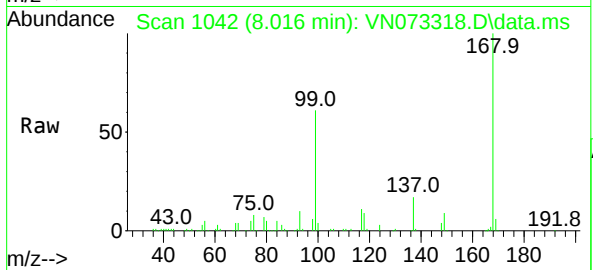

#39
Methylcyclohexane
Concen: 8.640 ug/l
RT: 9.398 min Scan# 1277
Delta R.T. 0.006 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 83 Resp: 52532
Ion Ratio Lower Upper
83 100
55 74.7 57.8 86.8
98 40.7 39.4 59.2


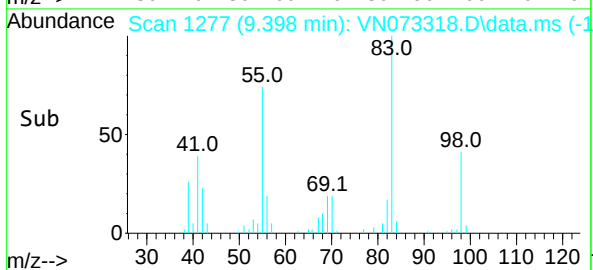
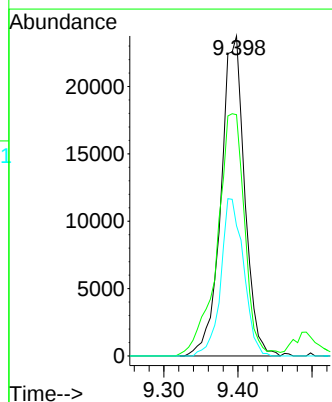
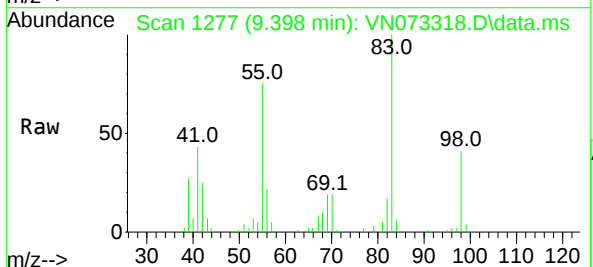


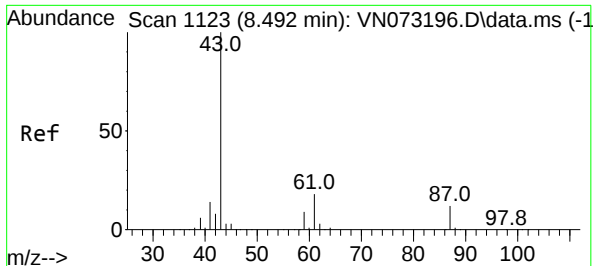

#43
Isopropyl Acetate
Concen: 18.985 ug/l
RT: 8.492 min Scan# 1123
Delta R.T. 0.000 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion: 43 Resp: 201333
Ion Ratio Lower Upper
43 100
61 17.9 21.9 32.9#
87 11.3 12.0 18.0#

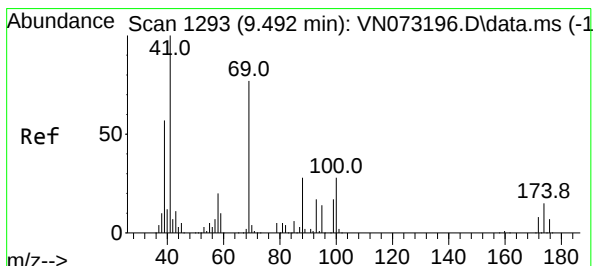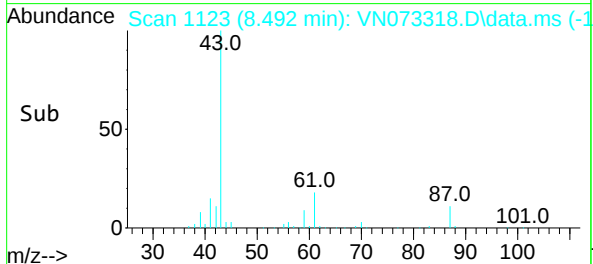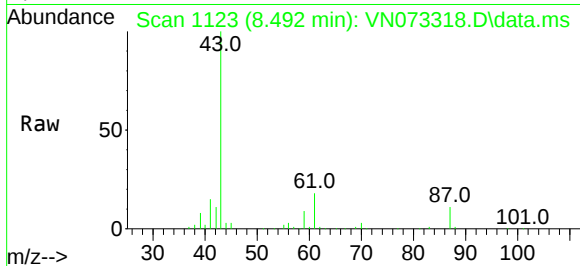

#48
Methyl methacrylate
Concen: 1.326 ug/l
RT: 9.480 min Scan# 1291
Delta R.T. -0.012 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 41 Resp: 6510
Ion Ratio Lower Upper
41 100
69 0.0 74.7 112.1#
39 50.9 45.6 68.4

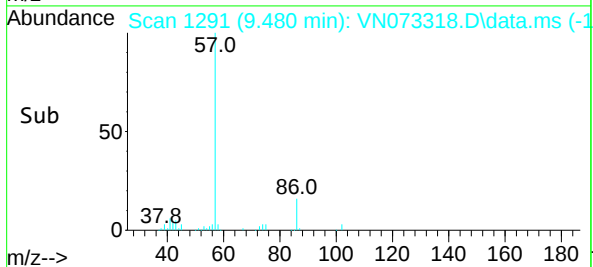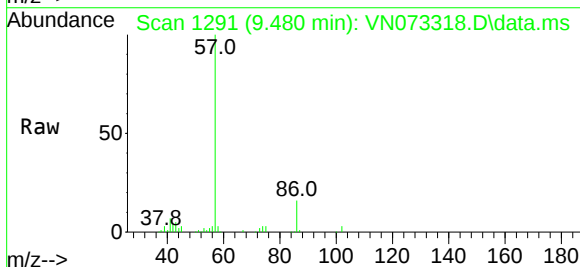

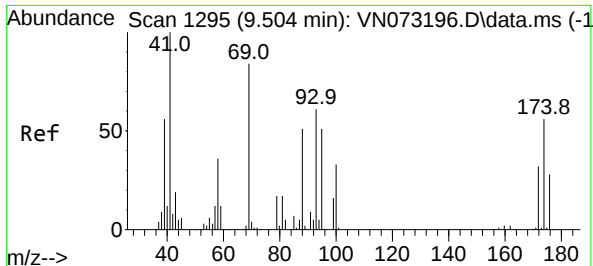

#49

1,4-Dioxane

Concen: 0.687 ug/l

RT: 9.551 min Scan# 11

Delta R.T. 0.047 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23

Instrument :

MSVOA_N

ClientSampleId :

WC-14B-11-1





Tgt Ion: 88 Resp: 64

Ion Ratio Lower Upper

88 100

43 2061385.9 20.2 30.4#

58 8781.3 54.2 81.4#

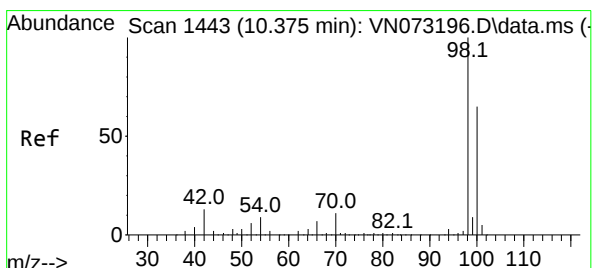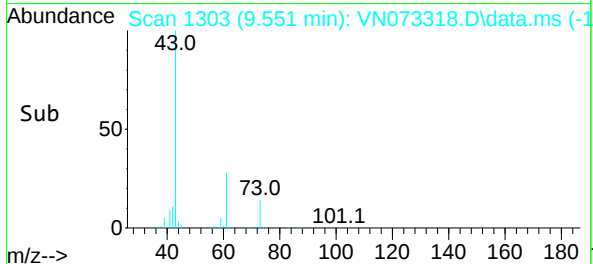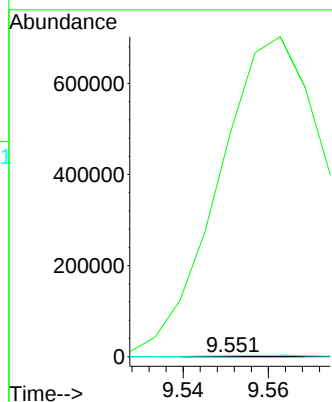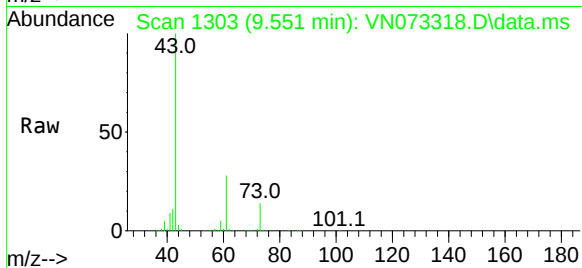

#50

Toluene-d8

Concen: 45.444 ug/l

RT: 10.380 min Scan# 1444

Delta R.T. 0.005 min

Lab File: VN073318.D




Acq: 05 Jul 2022 16:23


Tgt Ion: 98 Resp: 512268

Ion Ratio Lower Upper

98 100

100 65.7 52.6 78.8


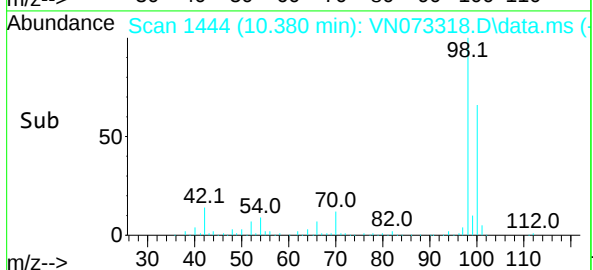

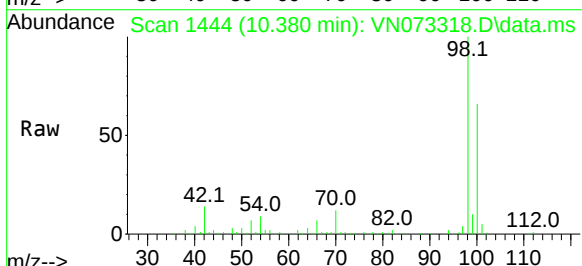


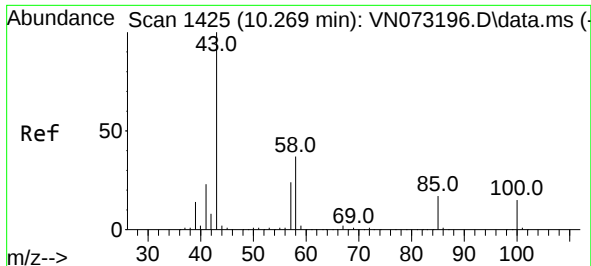

#51
4-Methyl-2-Pentanone
Concen: 1.216 ug/l
RT: 10.274 min Scan# 1425
Delta R.T. 0.005 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion: 43 Resp: 8178
Ion Ratio Lower Upper
43 100
58 43.6 34.1 51.1

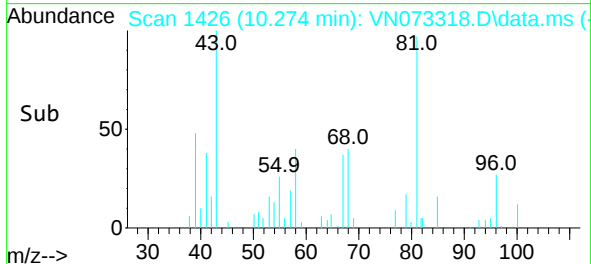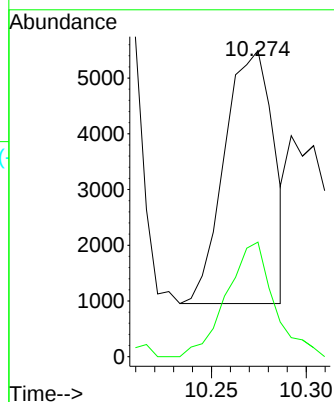

#54
cis-1,3-Dichloropropene
Concen: 9.890 ug/l
RT: 10.180 min Scan# 1410
Delta R.T. 0.052 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 75 Resp: 59381
Ion Ratio Lower Upper
75 100
77 1.2 25.2 37.8#
39 32.3 35.7 53.5#


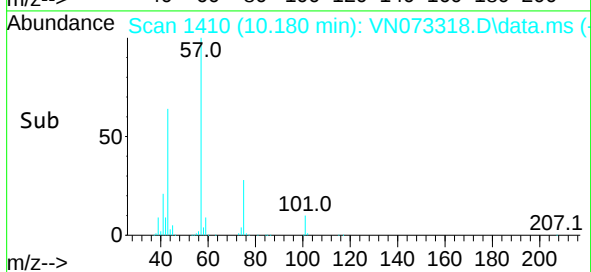
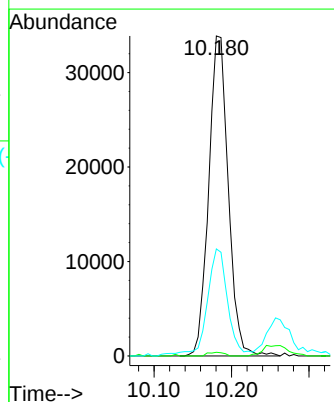
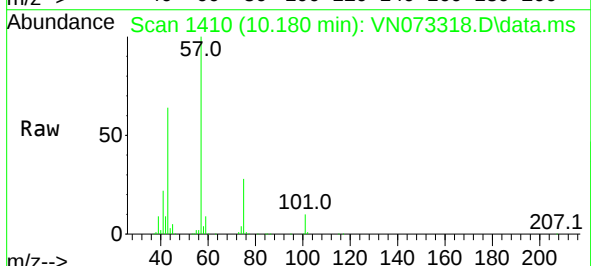


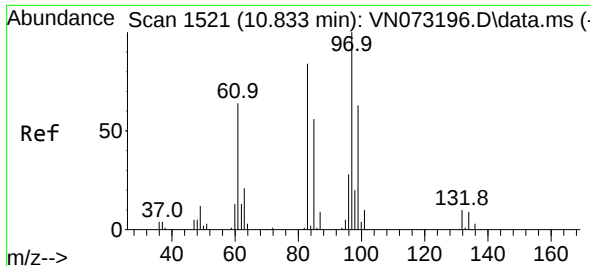

#55
1,1,2-Trichloroethane
Concen: 1.254 ug/l
RT: 10.816 min Scan# 1502
Delta R.T. -0.017 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion: 97	Resp: 4808
Ion Ratio	Lower Upper
97 100	
83 16.0	66.2 99.4#
85 0.0	43.9 65.9#
99 0.0	50.6 76.0#

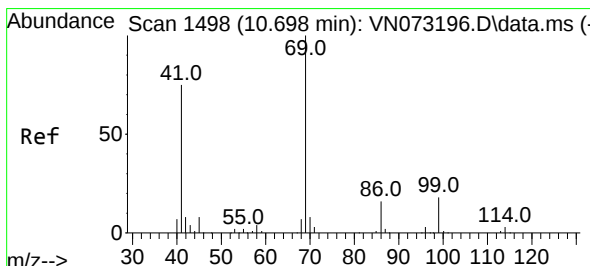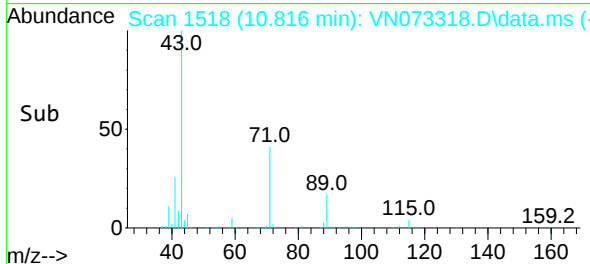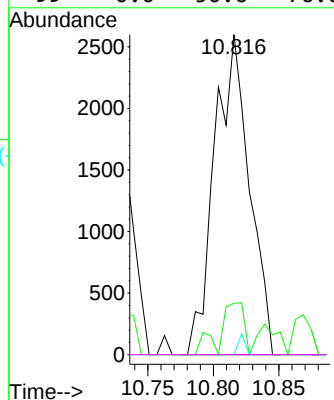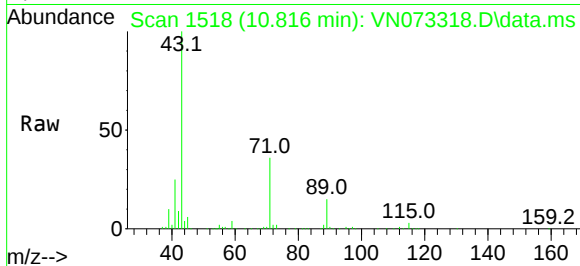

#56
Ethyl methacrylate
Concen: 0.481 ug/l
RT: 10.722 min Scan# 1502
Delta R.T. 0.024 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 69	Resp: 2979
Ion Ratio	Lower Upper
69 100	
41 149.5	47.8 71.6#
39 84.0	27.3 40.9#

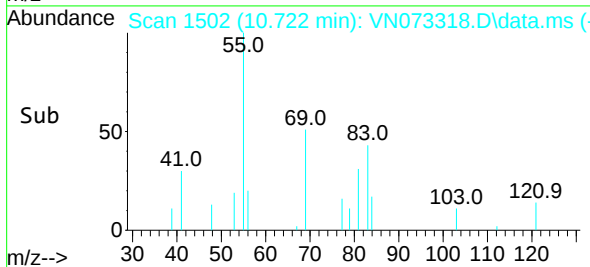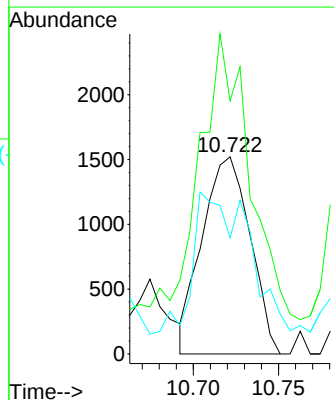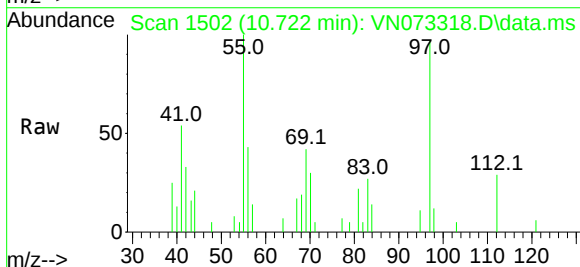

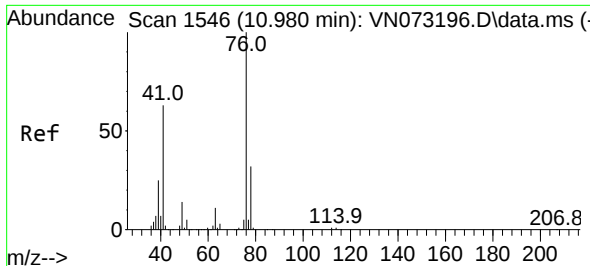

#57

1,3-Dichloropropane

Concen: 0.619 ug/l

RT: 11.027 min Scan# 11

Delta R.T. 0.047 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23

Instrument :

MSVOA_N

ClientSampleId :





WC-14B-11-1

Tgt Ion: 76 Resp: 4068

Ion Ratio Lower Upper

76 100

78 0.0 26.2 39.2#

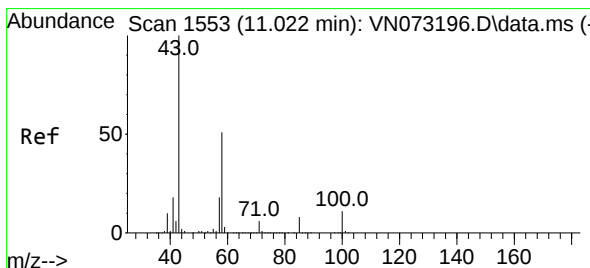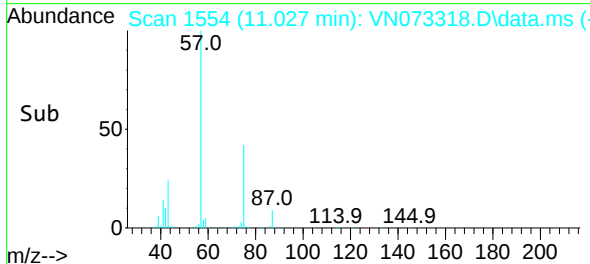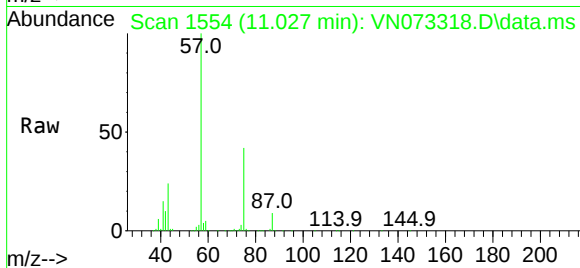

#59

2-Hexanone

Concen: 31.539 ug/l

RT: 10.998 min Scan# 1549

Delta R.T. -0.024 min

Lab File: VN073318.D




Acq: 05 Jul 2022 16:23


Tgt Ion: 43 Resp: 161678

Ion Ratio Lower Upper

43 100

58 0.0 29.7 89.1#


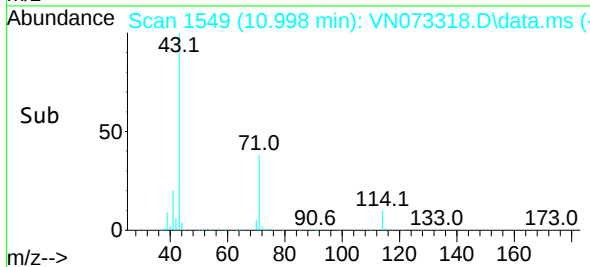

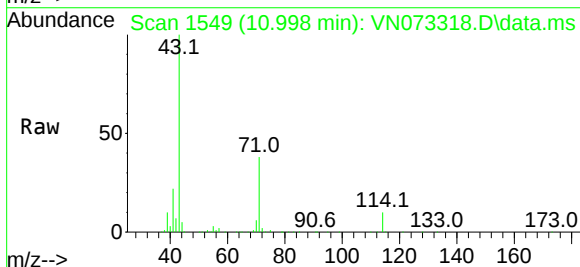


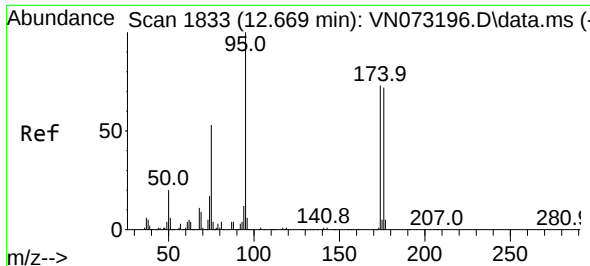

#62
4-Bromofluorobenzene
Concen: 52.885 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.001 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion: 95 Resp: 229096
Ion Ratio Lower Upper
95 100
174 75.8 0.0 167.6
176 71.5 0.0 163.4

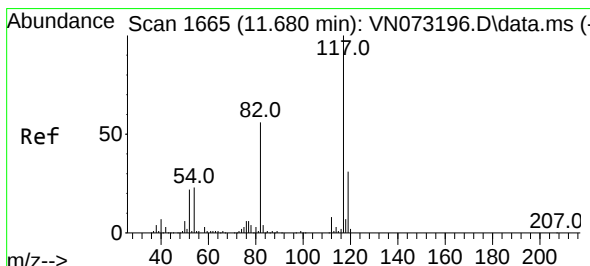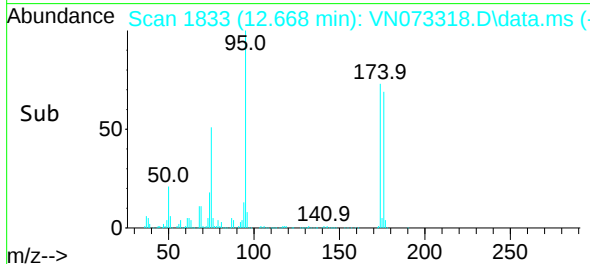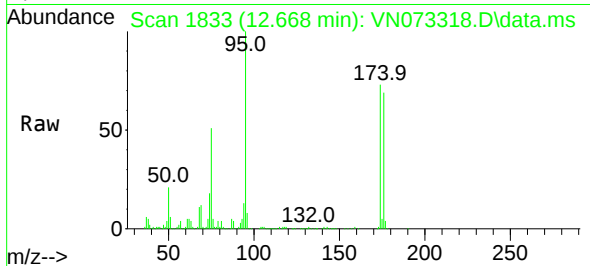

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1665
Delta R.T. 0.000 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 117 Resp: 449222
Ion Ratio Lower Upper
117 100
82 58.2 44.2 66.2
119 32.3 25.4 38.0


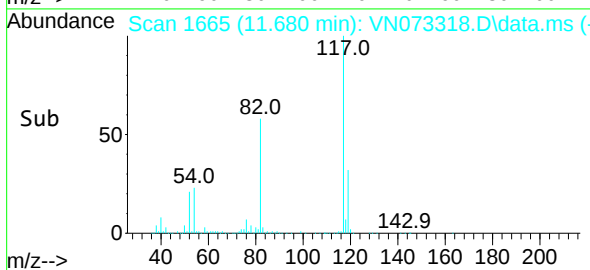

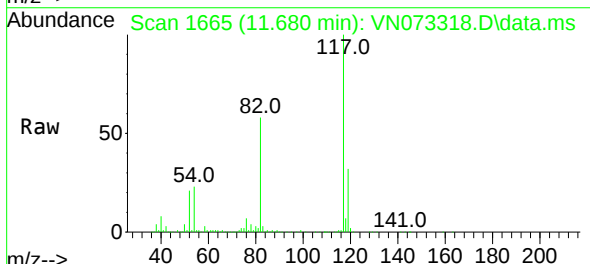




#68
m/p-Xylenes
Concen: 0.211 ug/l
RT: 11.886 min Scan# 1701
Delta R.T. -0.006 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion:106 Resp: 1470
Ion Ratio Lower Upper
106 100
91 297.4 158.9 238.3#

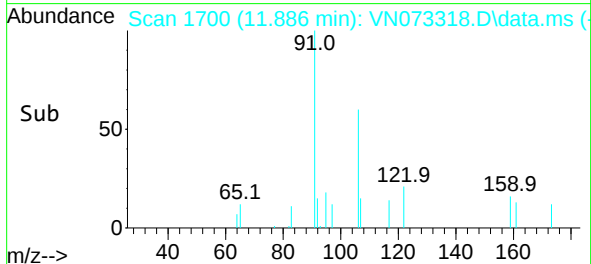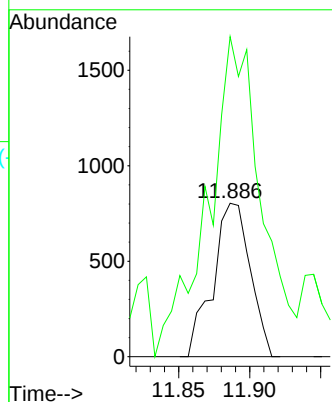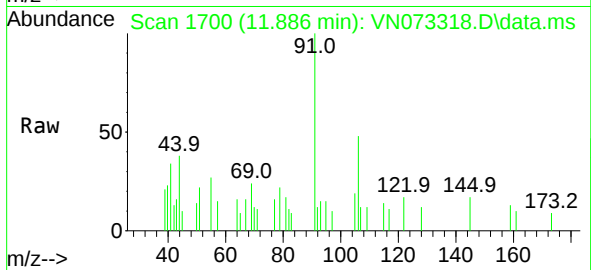

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion:152 Resp: 228985
Ion Ratio Lower Upper
152 100
115 63.8 28.9 86.7
150 155.2 0.0 356.2




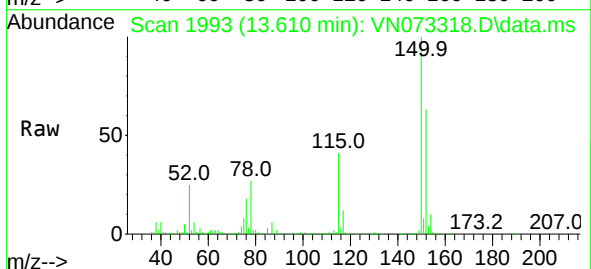


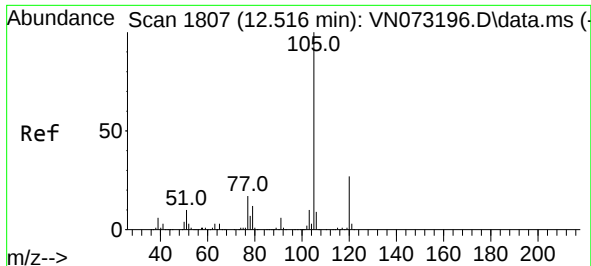

#73
Isopropylbenzene
Concen: 0.370 ug/l
RT: 12.521 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion:105 Resp: 7321
Ion Ratio Lower Upper
105 100
120 23.7 13.5 40.4

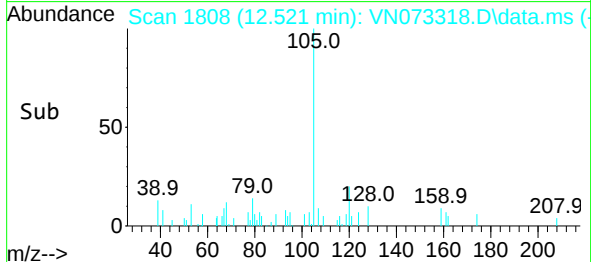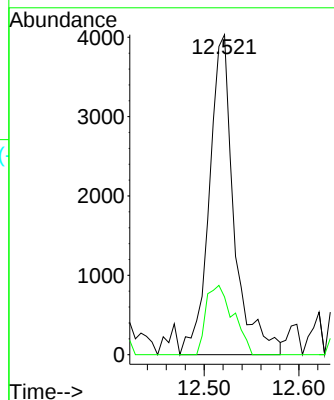

#74
N-ethyl acetate
Concen: 0.357 ug/l
RT: 12.304 min Scan# 1771
Delta R.T. -0.023 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion: 43 Resp: 3539
Ion Ratio Lower Upper
43 100
70 32.1 39.0 58.4#
55 84.5 21.1 31.7#
61 1.5 21.1 31.7#

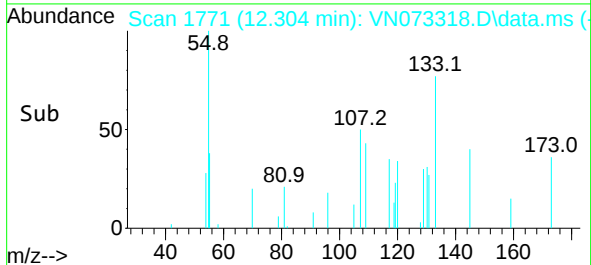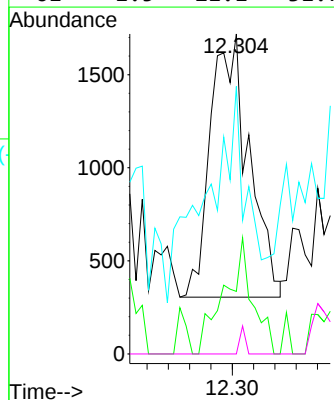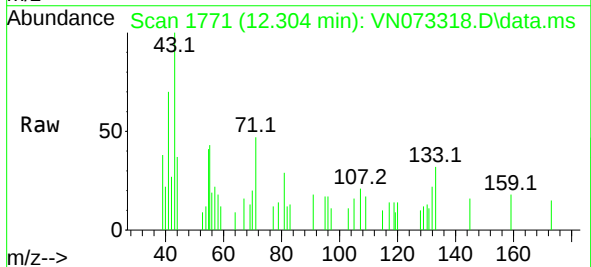



#76

1,2,3-Trichloropropane

Concen: 20.414 ug/l

RT: 12.668 min Scan# 1833

Delta R.T. -0.148 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23

Instrument :

MSVOA_N

ClientSampleId :





WC-14B-11-1

Tgt Ion: 75 Resp: 122226

Ion Ratio Lower Upper

75 100

77 2.5 98.5 295.5#

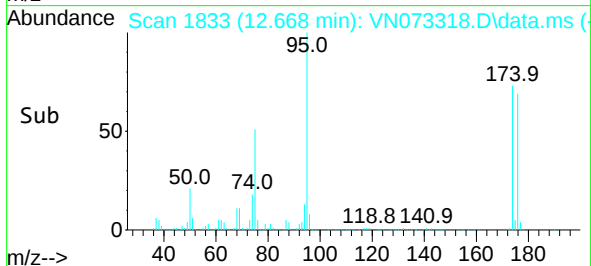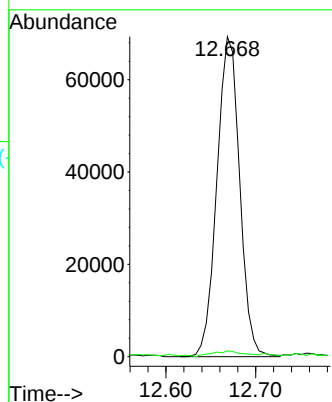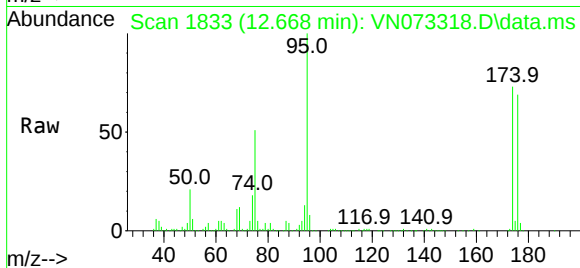

#81

trans-1,4-Dichloro-2-butene

Concen: 55.983 ug/l

RT: 12.668 min Scan# 1833

Delta R.T. 0.105 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23




Tgt Ion: 75 Resp: 122226


Ion Ratio Lower Upper

75 100

53 0.0 78.0 117.0#

89 0.0 37.2 55.8#


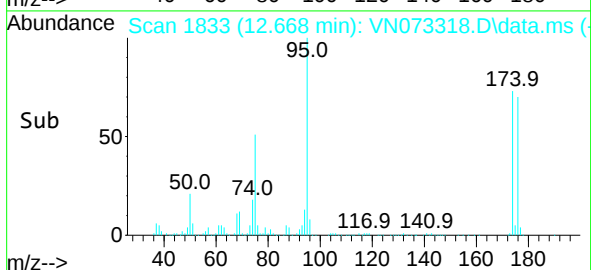

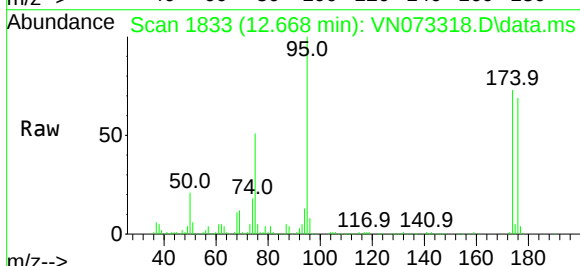


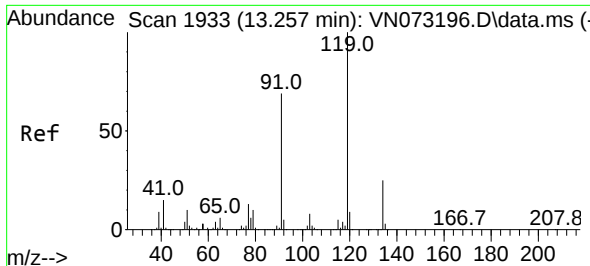

#83
tert-Butylbenzene
Concen: 0.213 ug/l
RT: 13.257 min Scan# 1933
Delta R.T. -0.000 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23




Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1


Tgt Ion:119 Resp: 3074
Ion Ratio Lower Upper
119 100
91 56.2 31.6 94.8
134 22.8 13.7 41.1

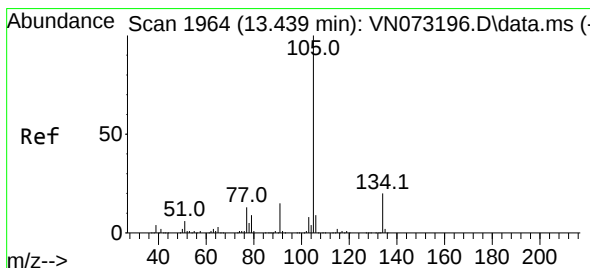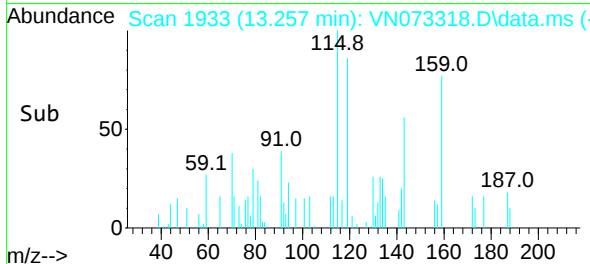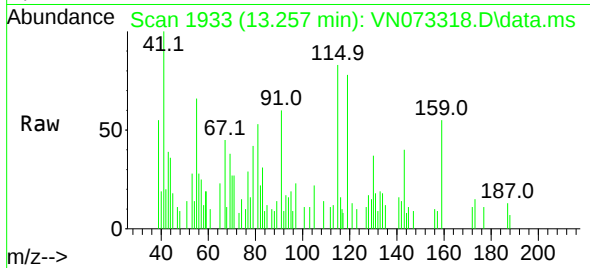

#85
sec-Butylbenzene
Concen: 0.268 ug/l
RT: 13.439 min Scan# 1964
Delta R.T. -0.000 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Tgt Ion:105 Resp: 5206
Ion Ratio Lower Upper
105 100
134 25.2 10.4 31.1

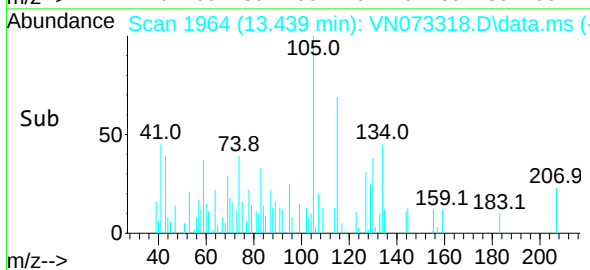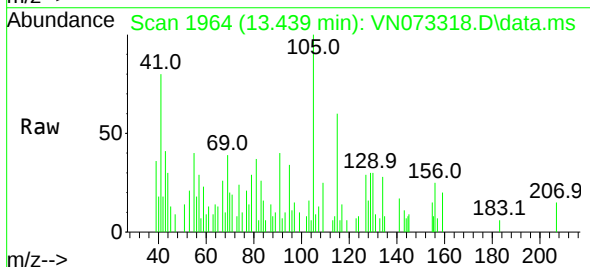

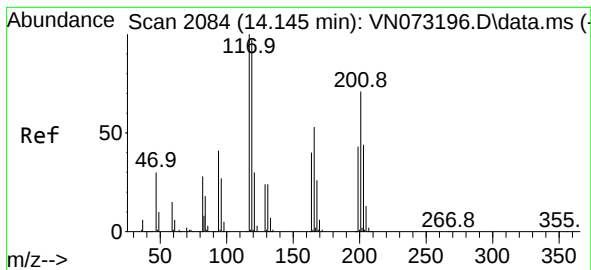

#90

Hexachloroethane

Concen: 0.853 ug/l

RT: 14.151 min Scan# 2107

Delta R.T. 0.006 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23

Instrument :

MSVOA_N

ClientSampleId :





WC-14B-11-1

Tgt Ion:117 Resp: 2492

Ion Ratio Lower Upper

117 100

201 0.0 40.6 122.0#

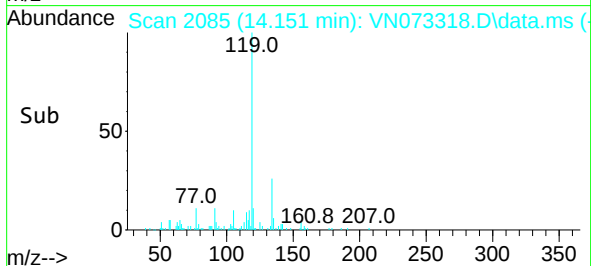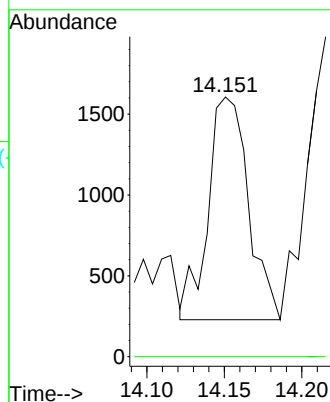

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.387 ug/l

RT: 14.398 min Scan# 2127

Delta R.T. -0.141 min

Lab File: VN073318.D

Acq: 05 Jul 2022 16:23




Tgt Ion: 75 Resp: 618


Ion Ratio Lower Upper

75 100

155 50.3 44.9 134.5


157 84.6 59.0 176.8

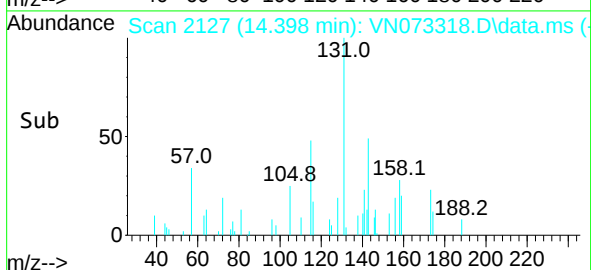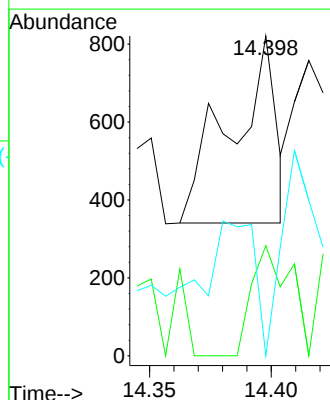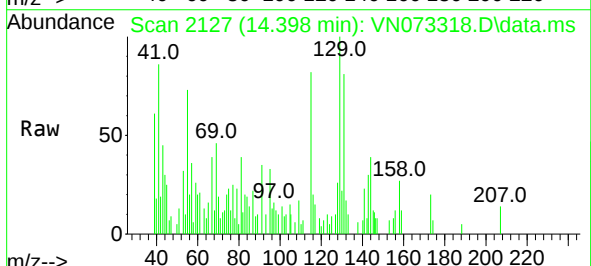



#95
Naphthalene
Concen: 0.254 ug/l
RT: 15.421 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN073318.D
Acq: 05 Jul 2022 16:23

Instrument :
MSVOA_N
ClientSampleId :
WC-14B-11-1

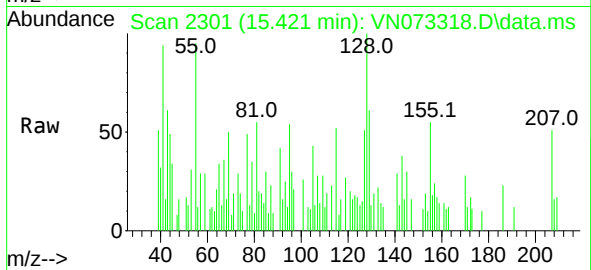

Tgt Ion:128 Resp: 4487
Ion Ratio Lower Upper
128 100
127 7.1 10.3 15.5#
129 10.4 8.6 13.0

