

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070620\
 Data File : VN062386.D
 Acq On : 7 Jul 2020 00:46
 Operator : JC/MD
 Sample : PB129462ZHE#02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB129462ZHE#02

Quant Time: Jul 07 05:23:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070620W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 07 05:08:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	928262	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	1686244	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	1666696	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	615710	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	841098	50.09	ug/l	0.00
Spiked Amount			Recovery	=	100.18%	
35) Dibromofluoromethane	7.55	113	572245	49.75	ug/l	0.00
Spiked Amount			Recovery	=	99.50%	
50) Toluene-d8	10.06	98	2228473	51.82	ug/l	0.00
Spiked Amount			Recovery	=	103.64%	
62) 4-Bromofluorobenzene	12.38	95	788316	47.87	ug/l	0.00
Spiked Amount			Recovery	=	95.74%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
8) Diethyl Ether	3.37	74	3410	0.480	ug/l	85
11) Tert butyl alcohol	4.74	59	976	0.420	ug/l #	72
13) Acrolein	3.58	56	672	1.017	ug/l	83
16) Acetone	3.78	43	60347	7.796	ug/l	99
18) Methyl Acetate	4.29	43	25429	1.122	ug/l #	76
20) Methylene Chloride	4.50	84	150705	12.189	ug/l	96
23) Vinyl Acetate	5.84	43	380	Below Cal	#	56
25) 2-Butanone	6.79	43	5441	0.558	ug/l #	61
31) Cyclohexane	7.62	56	29550	1.388	ug/l #	26
36) 1,1-Dichloropropene	7.63	75	86353	4.874	ug/l #	53
38) Carbon Tetrachloride	7.63	117	100984	5.668	ug/l #	17
43) Isopropyl Acetate	8.13	43	382216	10.879	ug/l	99
48) Methyl methacrylate	9.15	41	20748	1.157	ug/l #	19
49) 1,4-Dioxane	9.17	88	682	2.800	ug/l #	18
51) 4-Methyl-2-Pentanone	9.95	43	40284	1.575	ug/l #	85
54) cis-1,3-Dichloropropene	9.88	75	128531	5.751	ug/l #	64
57) 1,3-Dichloropropane	10.74	76	25402	1.134	ug/l #	45
59) 2-Hexanone	10.74	43	431679	30.315	ug/l #	53
74) N-amyl acetate	12.01	43	16029	0.655	ug/l #	55
76) 1,2,3-Trichloropropane	12.38	75	449873	30.250	ug/l #	100
78) n-propylbenzene	12.57	91	686	0.294	ug/l #	72
80) 1,3,5-Trimethylbenzene	12.71	105	14179	0.370	ug/l	95
81) trans-1,4-Dichloro-2-buten	12.38	75	449873	86.506	ug/l #	4
93) 1,2,4-Trichlorobenzene	14.99	180	93	2.739	ug/l #	76
94) Hexachlorobutadiene	14.93	225	32	Below Cal	#	1
95) Naphthalene	15.12	128	1417	2.118	ug/l #	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN070620\
Data File : VN062386.D
Acq On : 7 Jul 2020 00:46
Operator : JC/MD
Sample : PB129462ZHE#02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB129462ZHE#02

Quant Time: Jul 07 05:23:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N070620W.M
Quant Title : SW846 8260
QLast Update : Tue Jul 07 05:08:51 2020
Response via : Initial Calibration

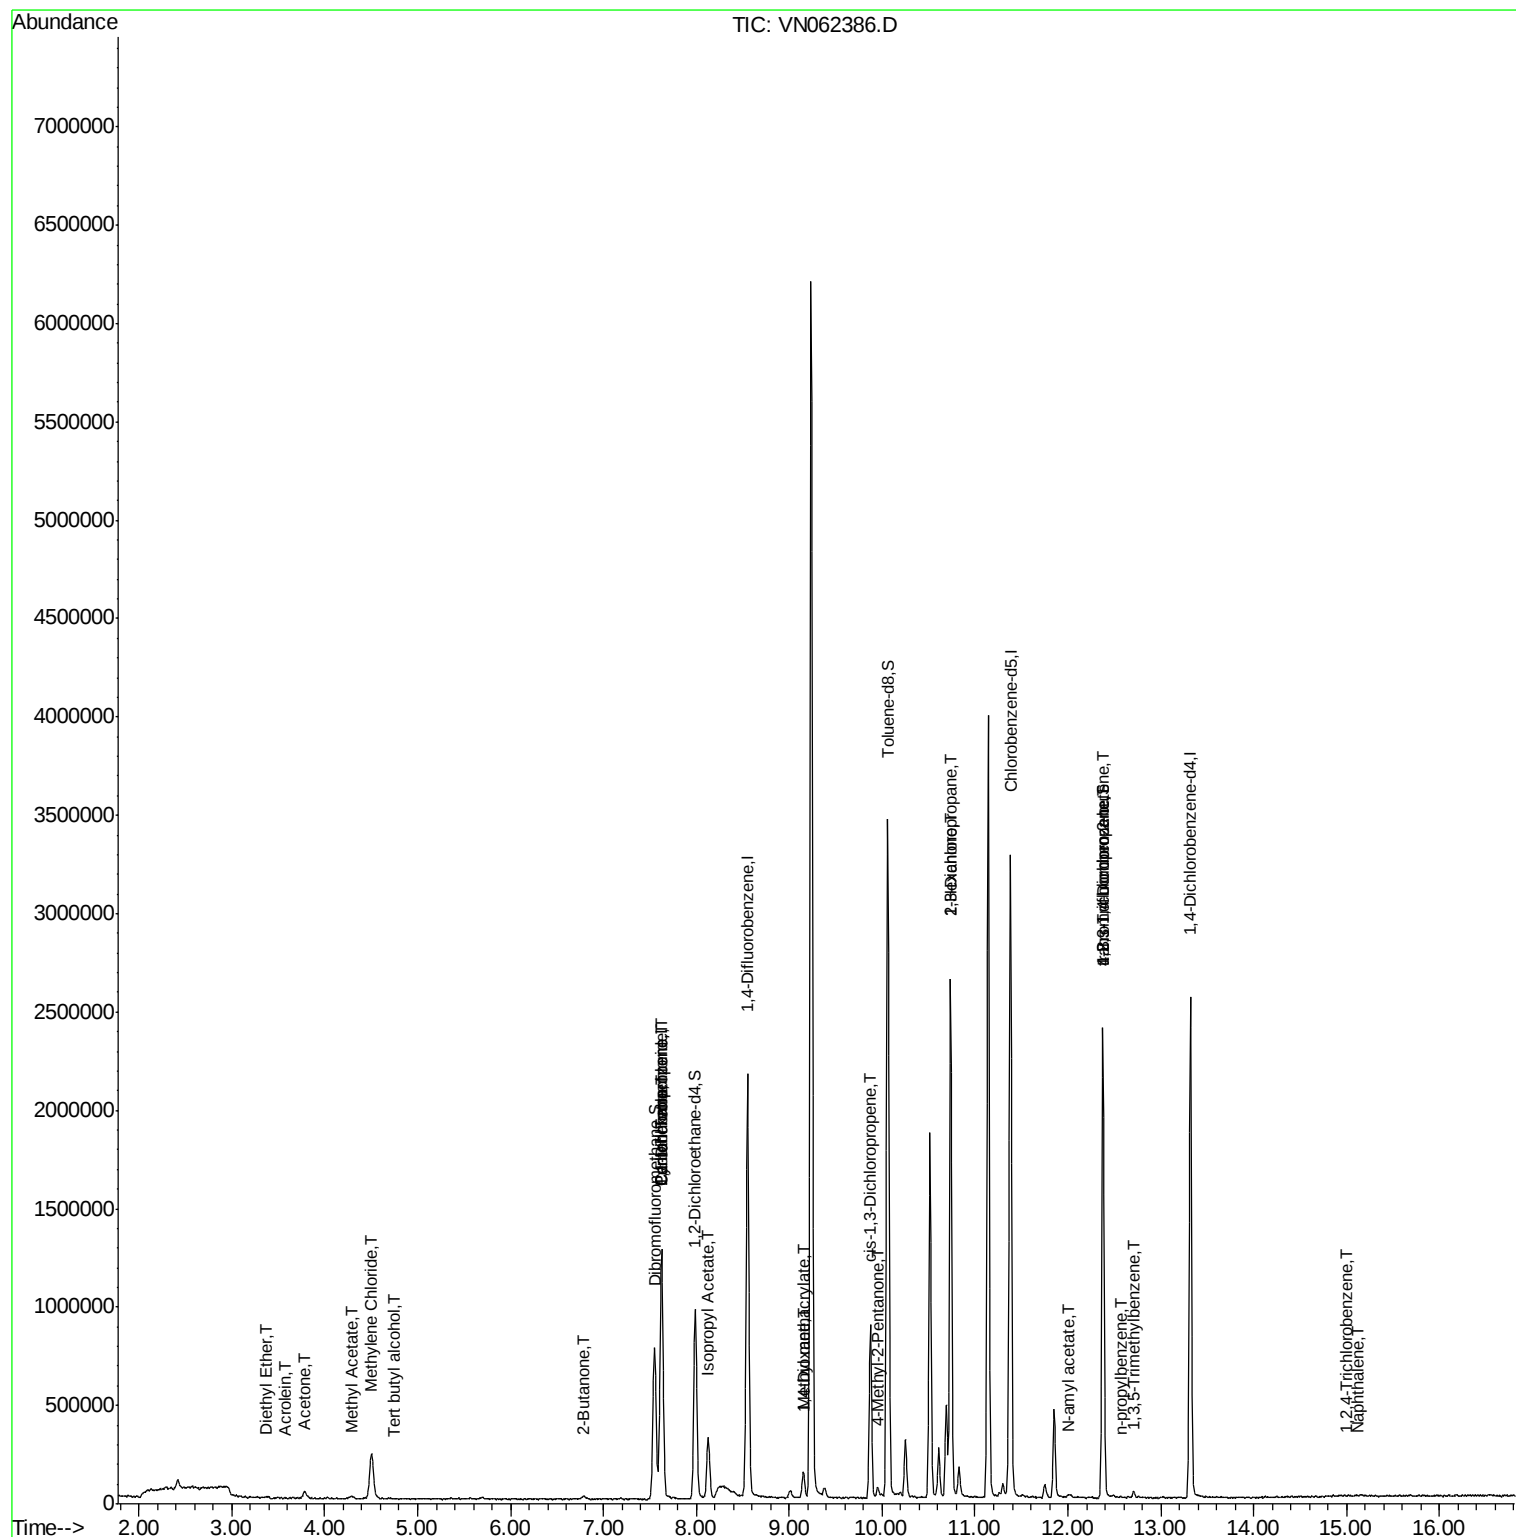



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :


PB129462ZHE#02

Tot Ion:168 Resp: 928262

Ion Ratio Lower Upper

168 100

99 65.2 52.9 79.3

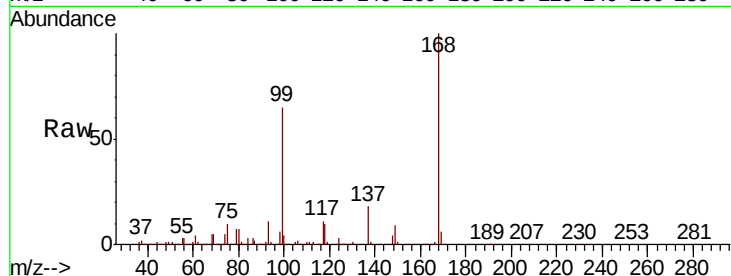

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63

400000



300000

200000

100000

0

Time-->

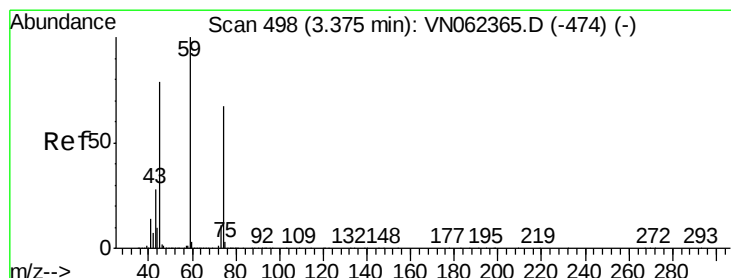

#8

Diethyl Ether

Concen: 0.480 ug/l

RT: 3.37 min Scan# 497

Delta R.T. -0.00 min

Lab File: VN062386.D


Acq: 7 Jul 2020 00:46

Tgt Ion: 74 Resp: 3410

Ion Ratio Lower Upper

74 100

45 103.6 59.9 179.7

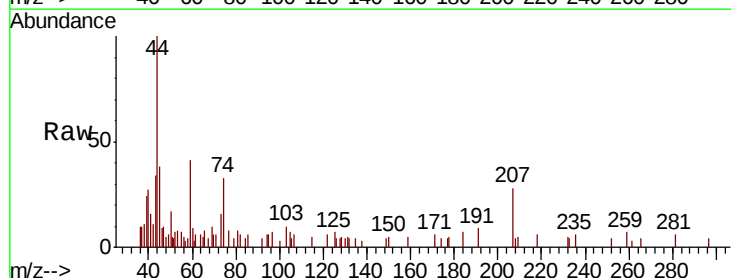

Abundance Ion 74.00 (73.70 to 74.70): VNO

Ion 45.00 (44.70 to 45.70): VNO

3.37

2000


1500


1000

500

0

Time-->









#11
Tert butyl alcohol
Concen: 0.420 ug/l
RT: 4.74 min Scan# 923
Delta R.T. 0.01 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46




Instrument :
MSVOA_N
ClientSampleId :
PB129462ZHE#02


Tot Ion: 59 Resp: 976
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#

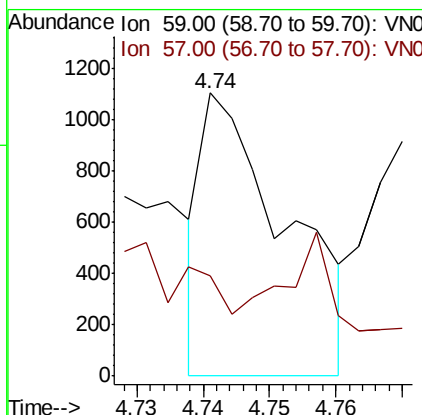

#13
Acrolein
Concen: 1.017 ug/l
RT: 3.58 min Scan# 561
Delta R.T. 0.01 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46

Tgt Ion: 56 Resp: 672
Ion Ratio Lower Upper
56 100
55 59.8 59.6 89.4

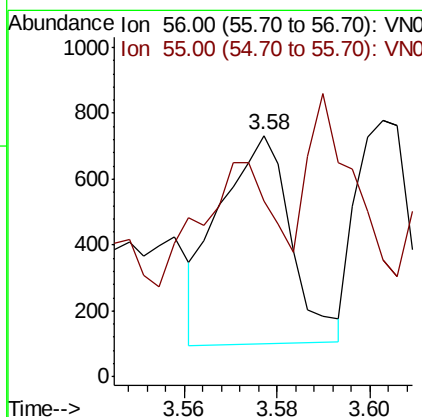



#16

Acetone

Concen: 7.796 ug/l

RT: 3.78 min Scan# 624

Delta R.T. 0.01 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :





PB129462ZHE#02

Tot Ion: 43 Resp: 60347

Ion Ratio Lower Upper

43 100

58 24.4 19.8 29.8

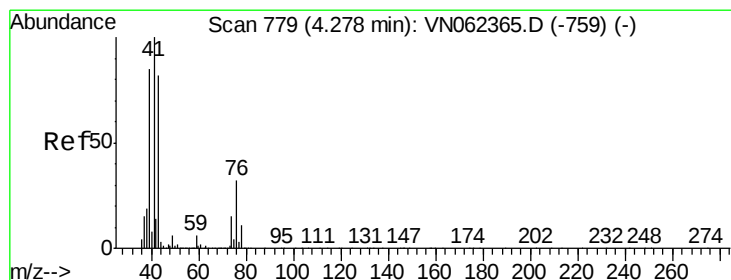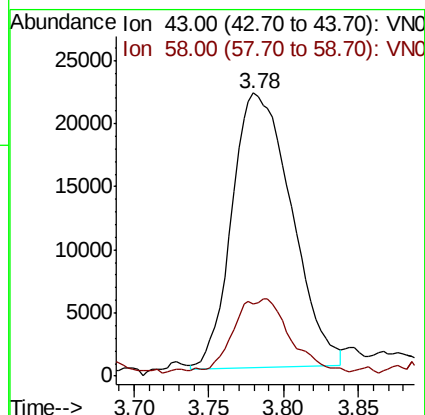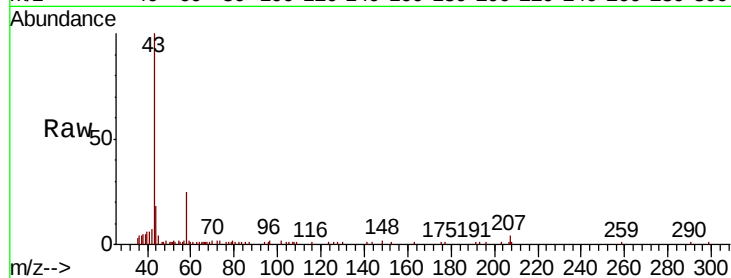

#18

Methyl Acetate

Concen: 1.122 ug/l

RT: 4.29 min Scan# 782

Delta R.T. 0.01 min

Lab File: VN062386.D




Acq: 7 Jul 2020 00:46


Tgt Ion: 43 Resp: 25429

Ion Ratio Lower Upper

43 100

74 7.0 14.2 21.4#



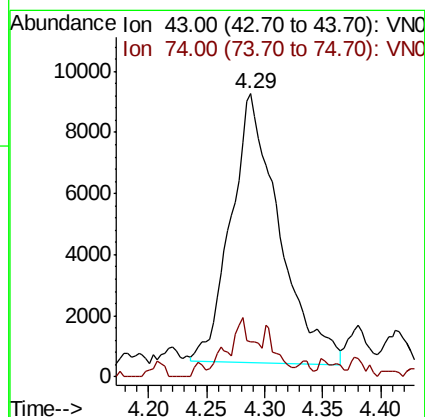
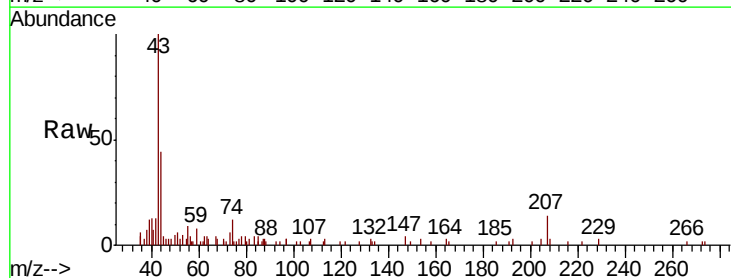


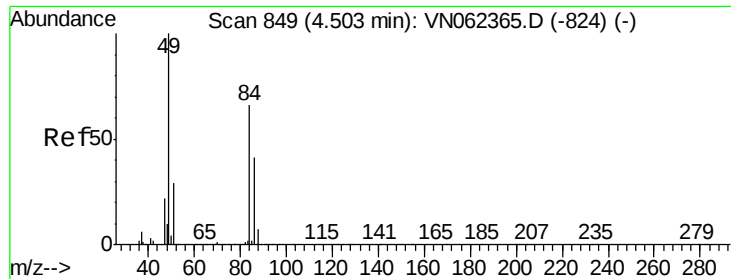

#20
Methvlene Chloride
Concen: 12.189 ug/l
RT: 4.50 min Scan# 849
Delta R.T. 0.00 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46




Instrument :
MSVOA_N
ClientSampleId :
PB129462ZHE#02


Tot Ion: 84 Resp: 150705
Ion Ratio Lower Upper
84 100
49 157.1 121.8 182.6
51 47.2 35.0 52.4
86 61.4 50.3 75.5

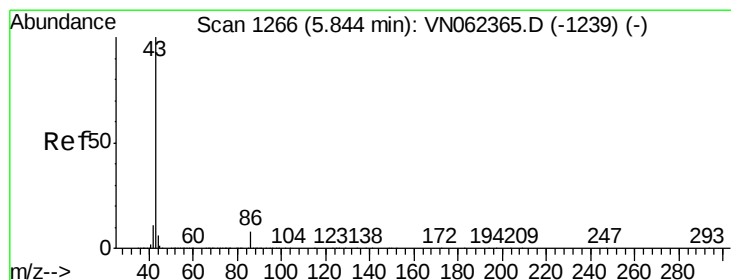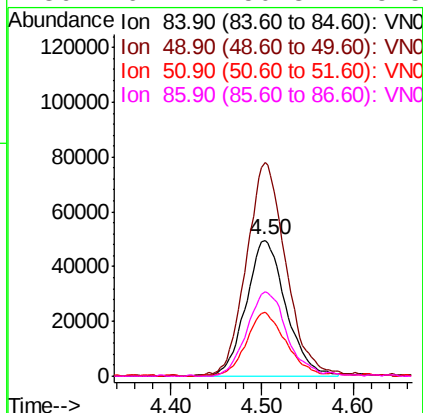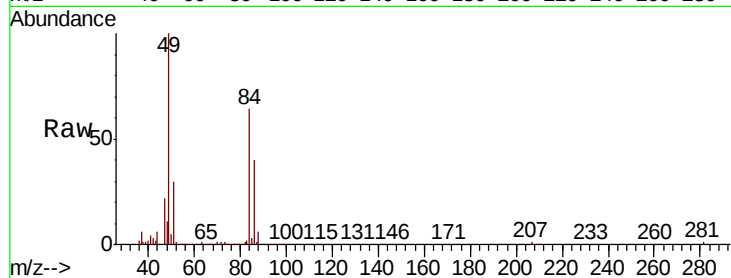

#23
Vinyl Acetate
Concen: Below Cal
RT: 5.84 min Scan# 1264
Delta R.T. -0.01 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46

Tgt Ion: 43 Resp: 380
Ion Ratio Lower Upper
43 100
86 23.8 6.6 9.8#


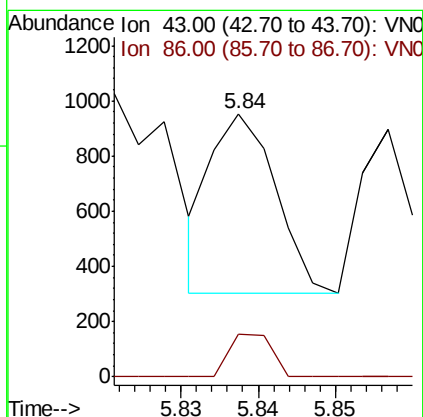
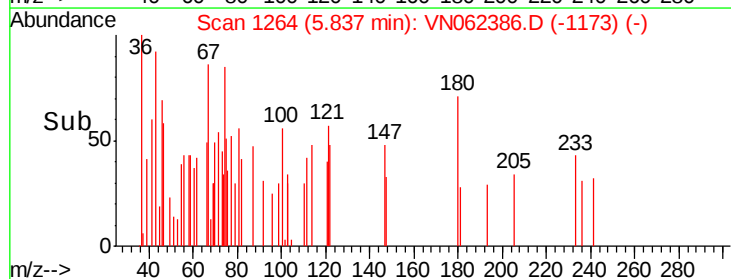
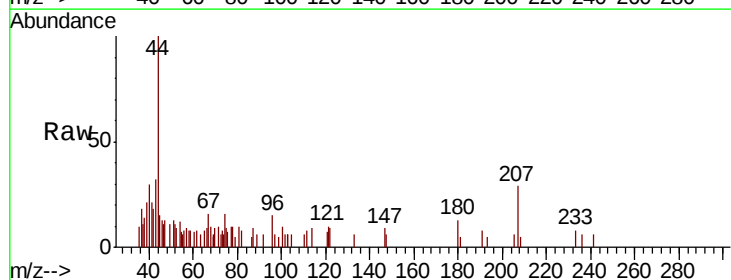


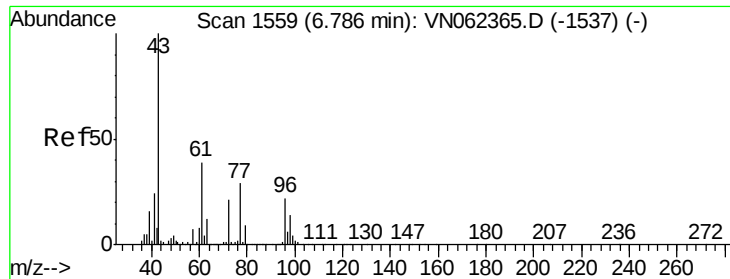

#25
2-Butanone
Concen: 0.558 ug/l
RT: 6.79 min Scan# 1560
Delta R.T. 0.00 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46




Instrument :
MSVOA_N
ClientSampleId :
PB129462ZHE#02


Tot Ion: 43 Resp: 5441
Ion Ratio Lower Upper
43 100
72 2.3 16.4 24.6#

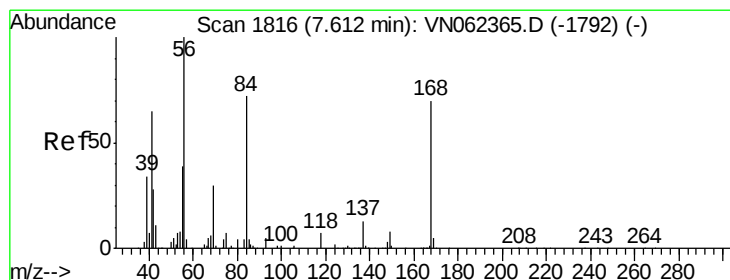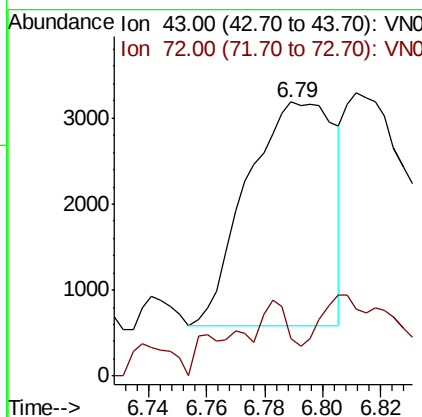

#31
Cyclohexane
Concen: 1.388 ug/l
RT: 7.62 min Scan# 1818
Delta R.T. 0.01 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46

Tgt Ion: 56 Resp: 29550
Ion Ratio Lower Upper
56 100
69 145.8 23.7 35.5#
84 84.4 57.2 85.8

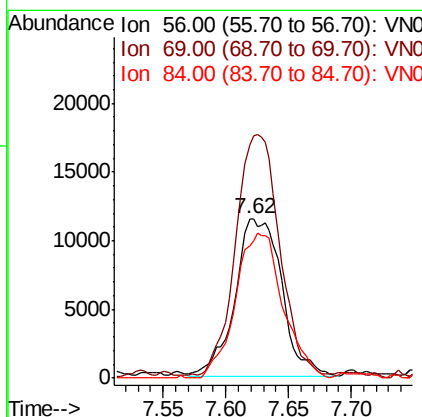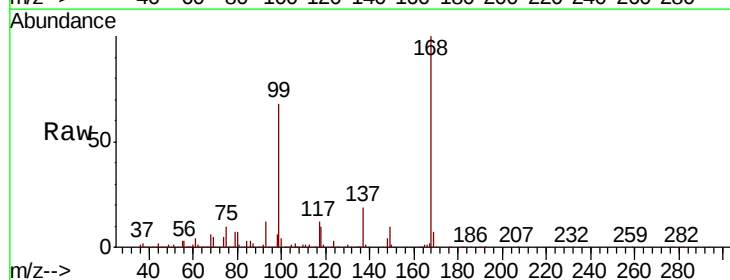



#33

1,2-Dichloroethane-d4

Concen: 50.091 ug/l

RT: 7.99 min Scan# 1933

Delta R.T. 0.00 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :


PB129462ZHE#02

Tot Ion: 65 Resp: 841098

Ion Ratio Lower Upper




65 100

67 51.1 0.0 101.0

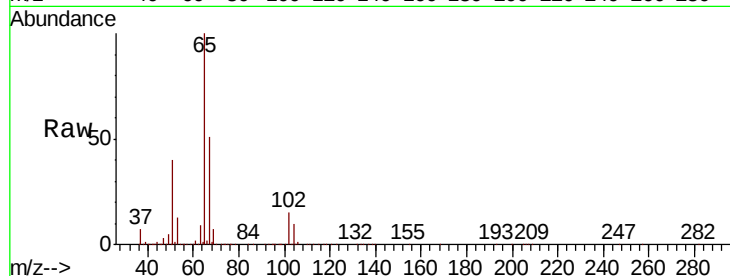

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

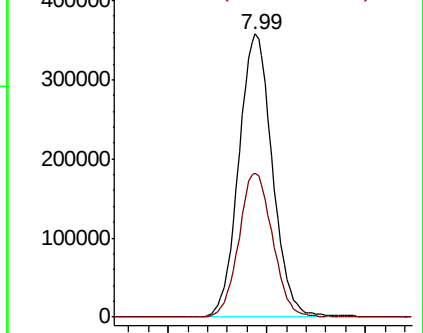

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2108

Delta R.T. -0.00 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46


Tgt Ion: 114 Resp: 1686244

Ion Ratio Lower Upper

114 100

63 24.9 0.0 49.0



88 17.7 0.0 34.0




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0




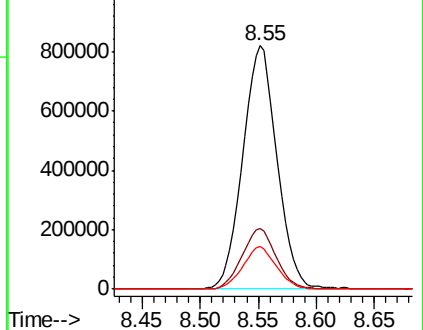




#35
 Dibromofluoromethane
 Concen: 49.745 ug/l
 RT: 7.55 min Scan# 1797
 Delta R.T. 0.00 min
 Lab File: VN062386.D
 Acq: 7 Jul 2020 00:46




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129462ZHE#02


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.4	83.2	124.8
192	17.4	14.2	21.2

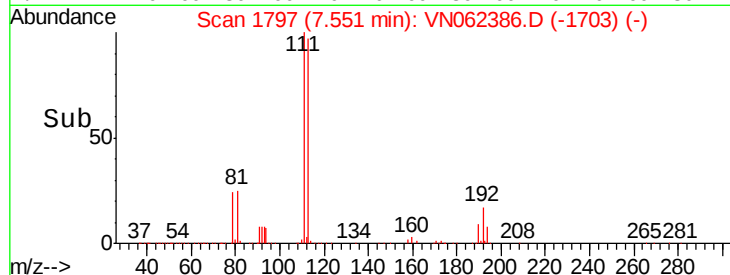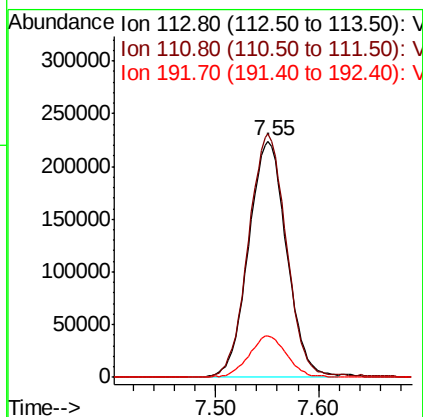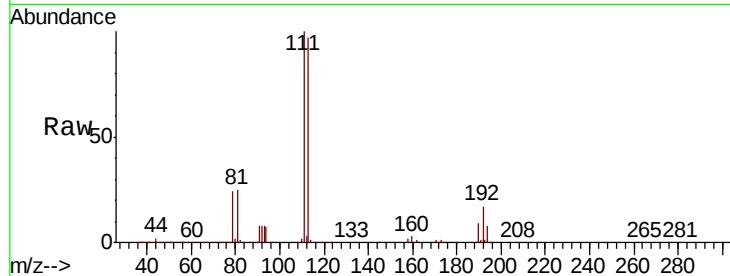

#36
 1,1-Dichloropropene
 Concen: 4.874 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.13 min
 Lab File: VN062386.D
 Acq: 7 Jul 2020 00:46

Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.9	15.7	47.1#
77	0.7	24.3	36.5#

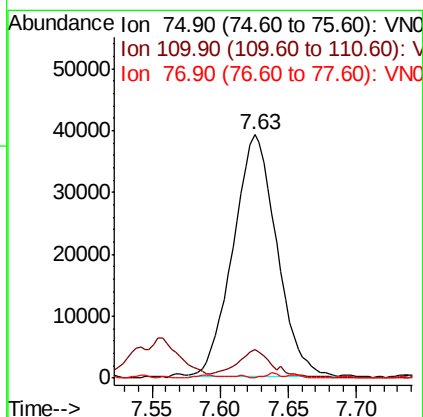



#38

Carbon Tetrachloride

Concen: 5.668 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.11 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :

PB129462ZHE#02


Tot Ion:117 Resp: 100984

Ion Ratio Lower Upper




117 100

119 6.3 75.9 113.9#

121 0.0 24.6 36.8#

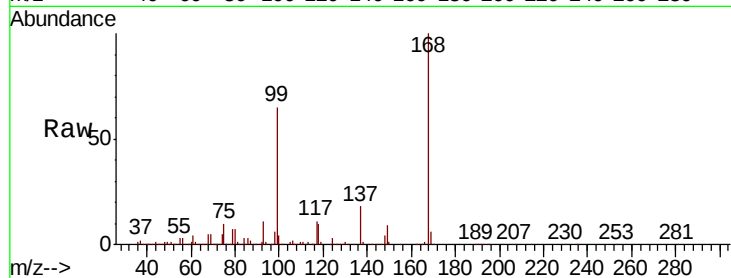

Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

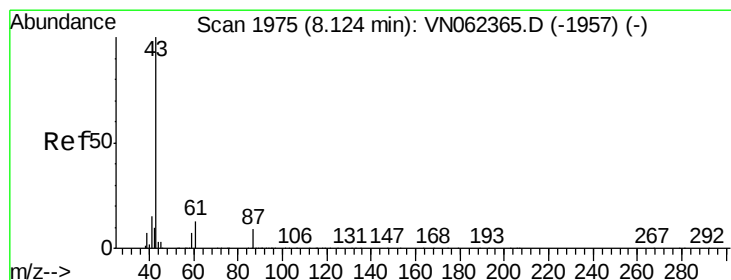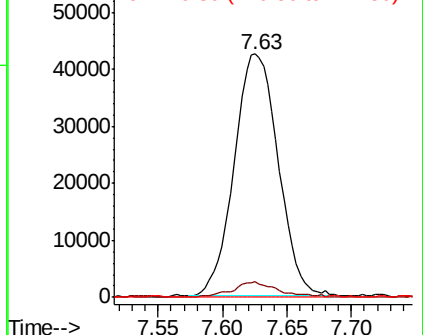

#43

Isopropyl Acetate

Concen: 10.879 ug/l

RT: 8.13 min Scan# 1976

Delta R.T. 0.00 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46


Tgt Ion: 43 Resp: 382216

Ion Ratio Lower Upper



43 100


61 15.5 13.1 19.7

87 9.5 7.5 11.3

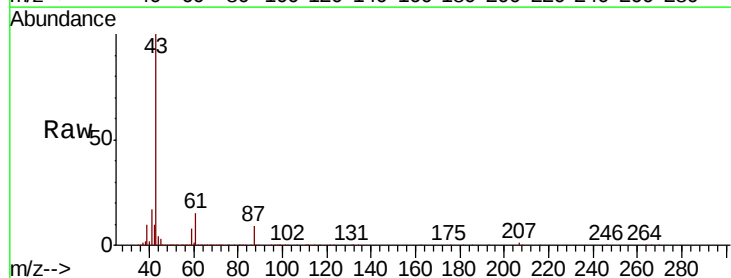

Abundance Ion 43.00 (42.70 to 43.70): V
Ion 61.00 (60.70 to 61.70): V
Ion 87.00 (86.70 to 87.70): V




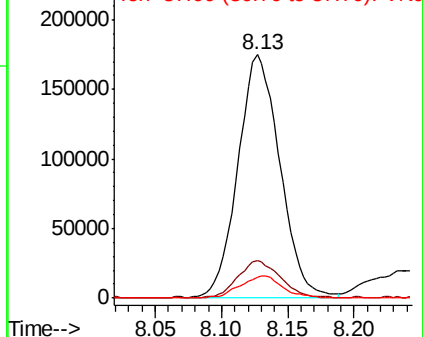




#48
Methyl methacrylate
Concen: 1.157 ug/l
RT: 9.15 min Scan# 2295
Delta R.T. -0.01 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46




Instrument :
MSVOA_N
ClientSampleId :
PB129462ZHE#02


Tot Ion: 41 Resp: 20748
Ion Ratio Lower Upper
41 100
69 1.0 51.5 77.3#
39 0.0 51.2 76.8#

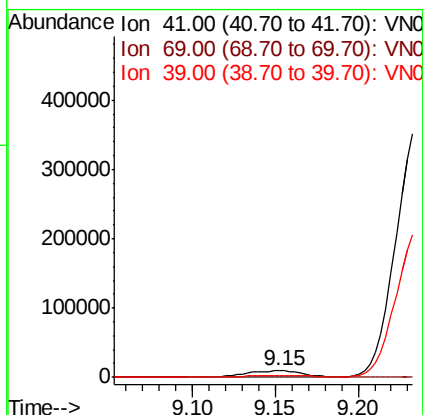

#49
1,4-Dioxane
Concen: 2.800 ug/l
RT: 9.17 min Scan# 2299
Delta R.T. -0.00 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46

Tgt Ion: 88 Resp: 682
Ion Ratio Lower Upper
88 100
43 0.0 34.0 51.0#
58 0.0 63.0 94.4#

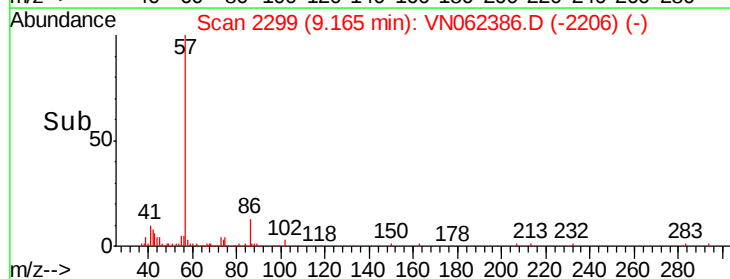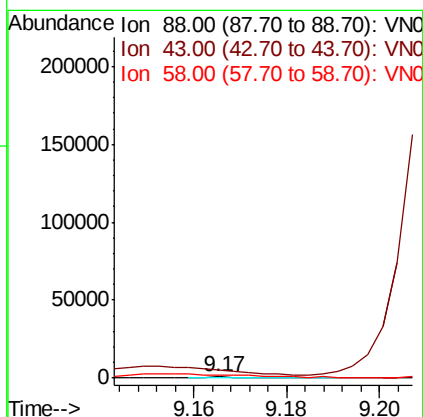



#50

Toluene-d8

Concen: 51.822 ug/l

RT: 10.06 min Scan# 2577

Delta R.T. -0.00 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :





PB129462ZHE#02

Tot Ion: 98 Resp: 2228473

Ion Ratio Lower Upper

98 100

100 62.9 50.2 75.2

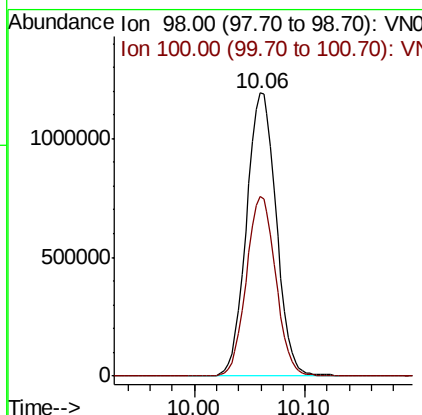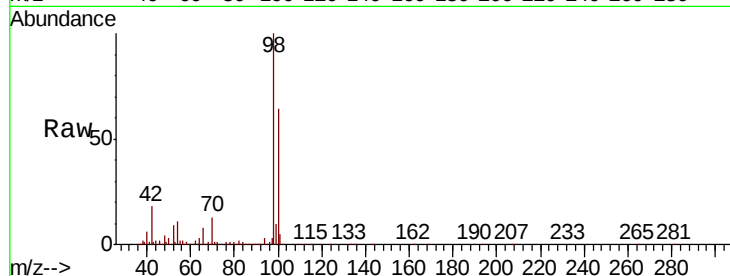

#51

4-Methyl-2-Pentanone

Concen: 1.575 ug/l

RT: 9.95 min Scan# 2543

Delta R.T. -0.00 min

Lab File: VN062386.D




Acq: 7 Jul 2020 00:46


Tgt Ion: 43 Resp: 40284

Ion Ratio Lower Upper

43 100

58 25.9 27.6 41.4#

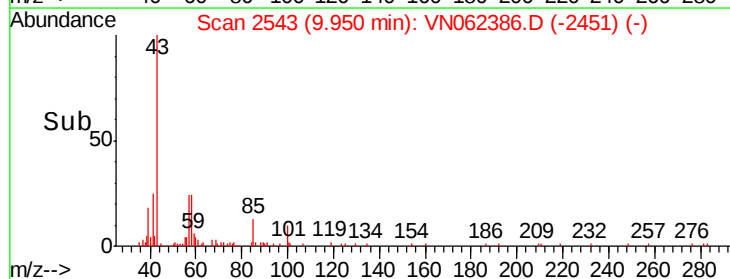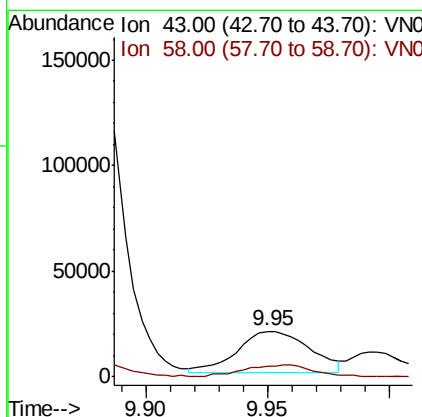



#54

cis-1,3-Dichloropropene

Concen: 5.751 ug/l

RT: 9.88 min Scan# 2520

Delta R.T. 0.07 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :

PB129462ZHE#02


Tot Ion: 75 Resp: 128531

Ion Ratio Lower Upper

75 100

77 0.5 26.0 39.0#




39 47.7 55.3 82.9#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 76.90 (76.60 to 77.60): VN0

Ion 39.00 (38.70 to 39.70): VN0

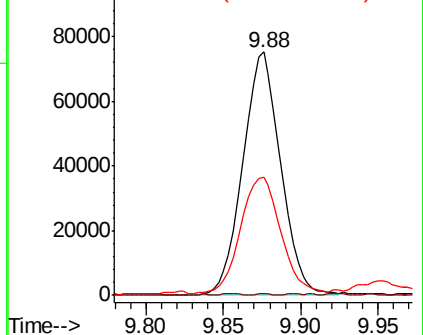

#57

1,3-Dichloropropane

Concen: 1.134 ug/l

RT: 10.74 min Scan# 2788

Delta R.T. 0.06 min

Lab File: VN062386.D


Acq: 7 Jul 2020 00:46

Tgt Ion: 76 Resp: 25402

Ion Ratio Lower Upper



76 100


78 0.7 25.0 37.4#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

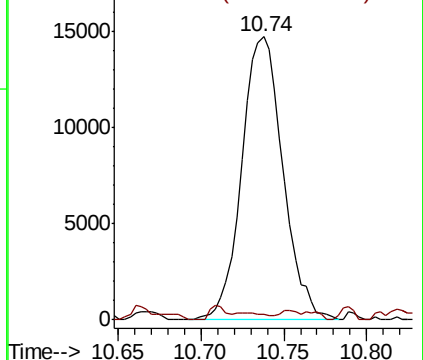



#59

2-Hexanone

Concen: 30.315 ug/l

RT: 10.74 min Scan# 2788

Delta R.T. 0.02 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :





PB129462ZHE#02

Tot Ion: 43 Resp: 431679

Ion Ratio Lower Upper

43 100

58 16.0 23.5 70.6#

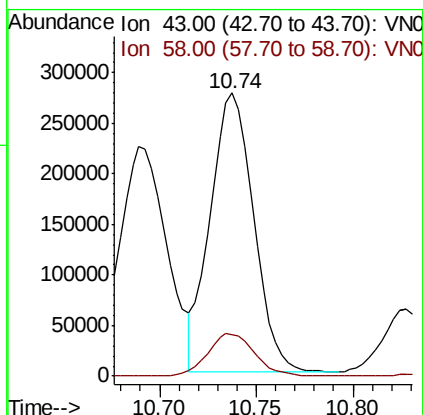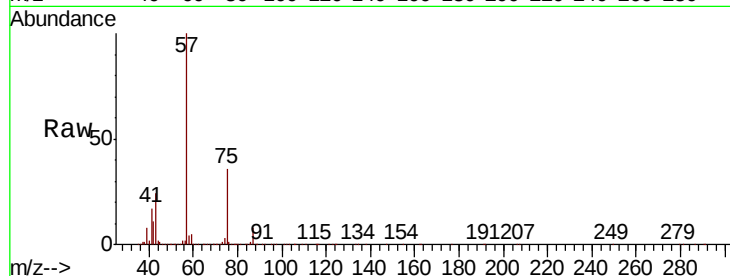

#62

4-Bromofluorobenzene

Concen: 47.866 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.00 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46




Tgt Ion: 95 Resp: 788316


Ion Ratio Lower Upper

95 100

174 71.5 0.0 145.8

176 69.4 0.0 140.2


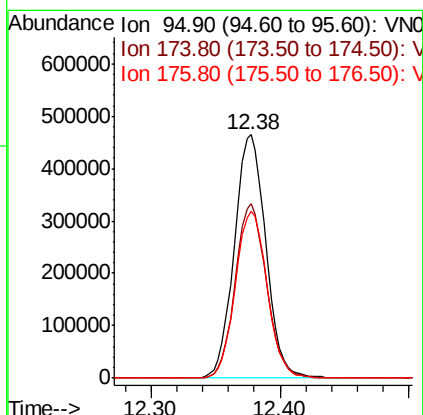






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. -0.00 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46




Instrument :
MSVOA_N
ClientSampleId :
PB129462ZHE#02


Tot Ion:117 Resp: 1666696
Ion Ratio Lower Upper
117 100
82 61.6 49.4 74.2
119 31.8 25.6 38.4

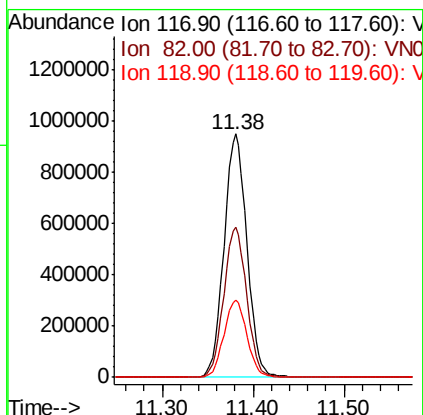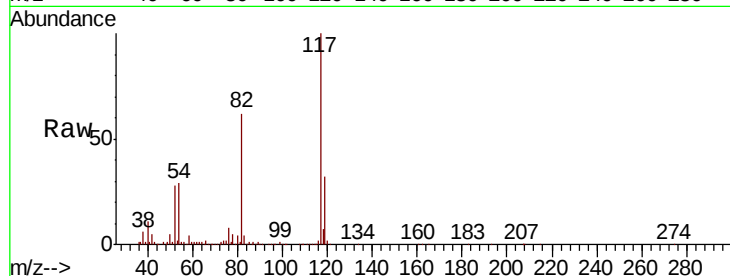

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3591
Delta R.T. -0.00 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46

Tgt Ion:152 Resp: 615710
Ion Ratio Lower Upper
152 100
115 63.4 30.5 91.5
150 157.2 0.0 346.8

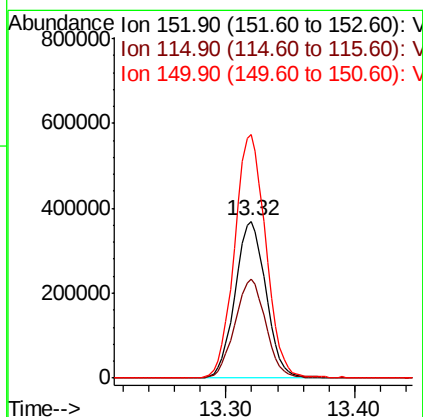



#74

N-amvl acetate

Concen: 0.655 ug/l

RT: 12.01 min Scan# 3183

Delta R.T. -0.04 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :

PB129462ZHE#02

Tot Ion: 43 Resp: 16029


Ion Ratio Lower Upper

43 100

70 1.2 25.9 38.9#

55 7.1 17.4 26.0#

61 0.0 15.6 23.4#



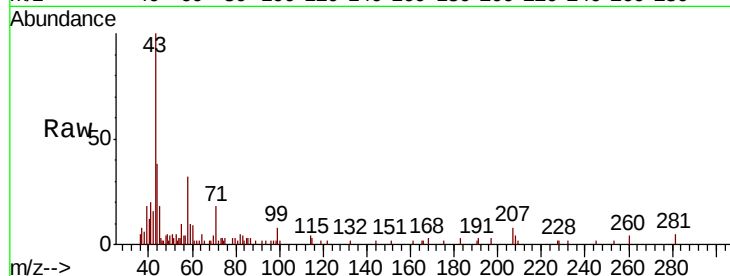


Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

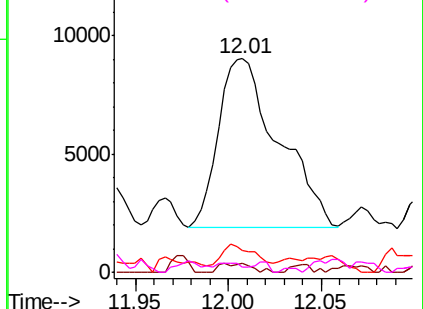

#76

1,2,3-Trichloropropane

Concen: 30.250 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.15 min

Lab File: VN062386.D


Acq: 7 Jul 2020 00:46

Tgt Ion: 75 Resp: 449873

Ion Ratio Lower Upper



75 100


77 1.4 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

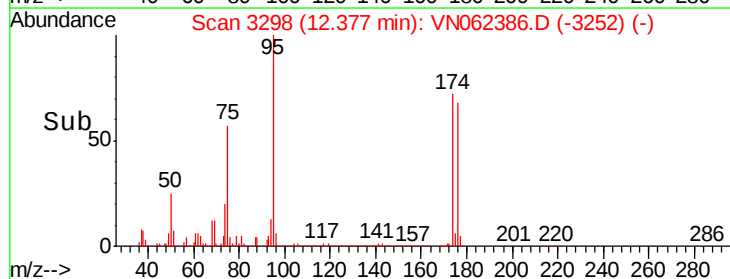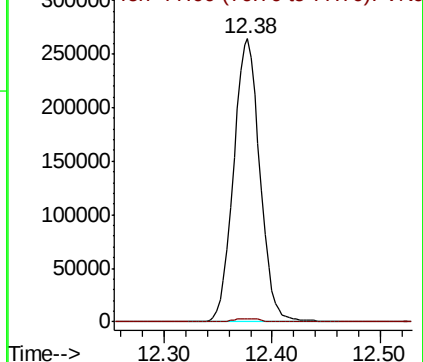

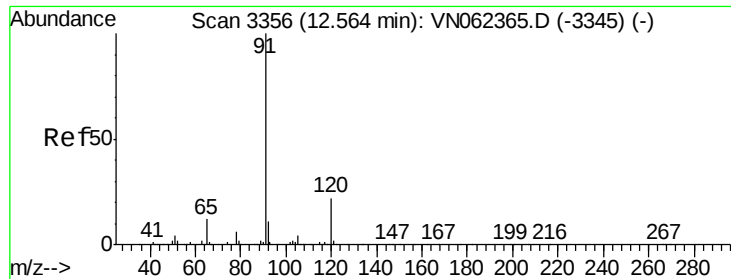

#78

n-propylbenzene

Concen: 0.294 ug/l

RT: 12.57 min Scan# 3357

Delta R.T. 0.00 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :


PB129462ZHE#02

Tot Ion: 91 Resp: 686




Ion Ratio Lower Upper

91 100

120 35.0 10.9 32.6#

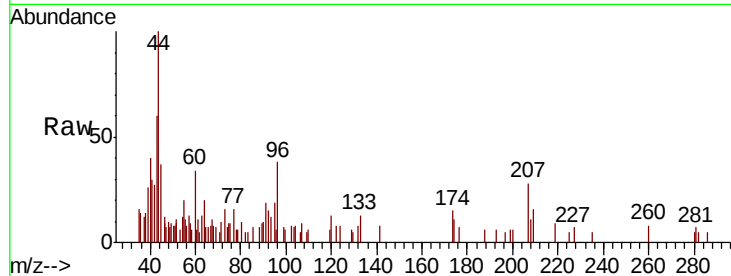

Abundance Ion 91.00 (90.70 to 91.70): VN062365.D (-3345) (-)

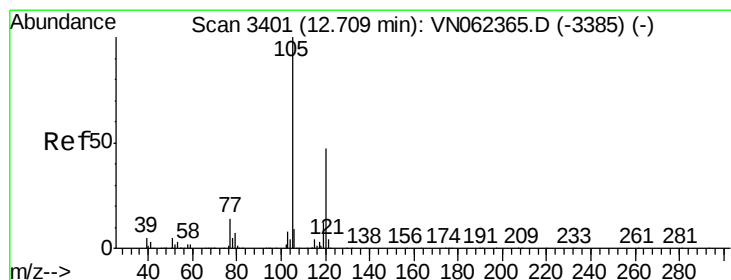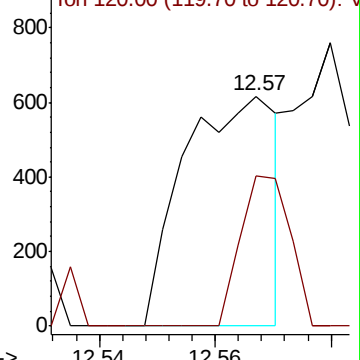

#80

1,3,5-Trimethylbenzene

Concen: 0.370 ug/l

RT: 12.71 min Scan# 3401

Delta R.T. -0.00 min

Lab File: VN062386.D


Acq: 7 Jul 2020 00:46

Tgt Ion:105 Resp: 14179



Ion Ratio Lower Upper


105 100

120 43.0 23.2 69.6

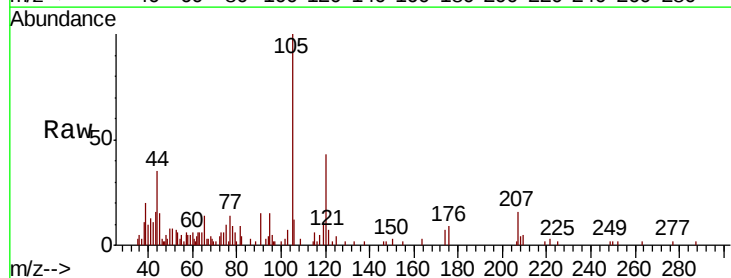

Abundance Ion 105.00 (104.70 to 105.70): VN062365.D (-3385) (-)




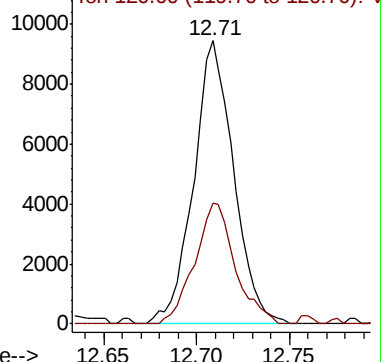


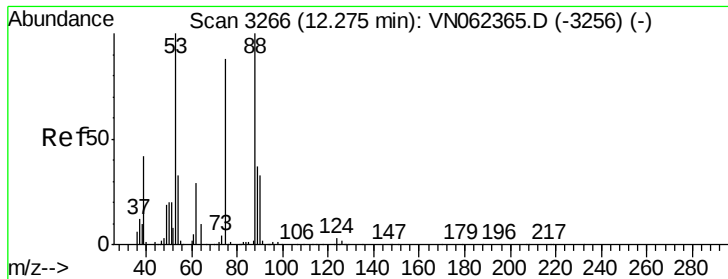

#81
trans-1,4-Dichloro-2-butene
Concen: 86.506 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.10 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46




Instrument :
MSVOA_N
ClientSampleId :
PB129462ZHE#02


Tot Ion: 75 Resp: 449873
Ion Ratio Lower Upper
75 100
53 0.2 92.3 138.5#
89 0.0 37.0 55.4#

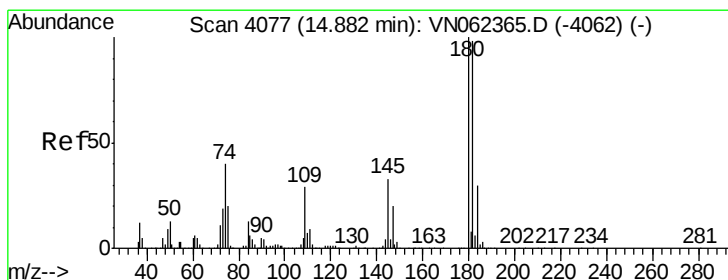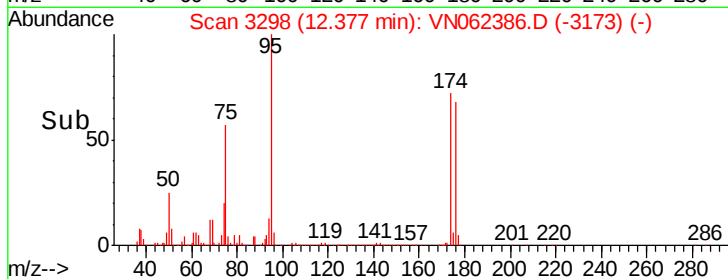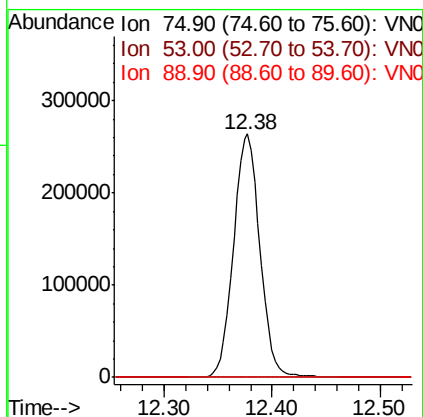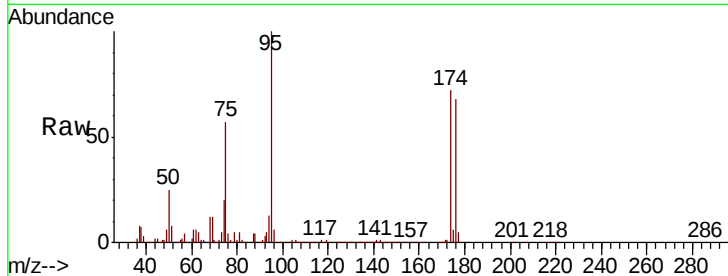

#93
1,2,4-Trichlorobenzene
Concen: 2.739 ug/l
RT: 14.99 min Scan# 4112
Delta R.T. 0.11 min
Lab File: VN062386.D
Acq: 7 Jul 2020 00:46

Tgt Ion: 180 Resp: 93
Ion Ratio Lower Upper
180 100
182 107.5 47.6 142.8
145 0.0 15.9 47.7#

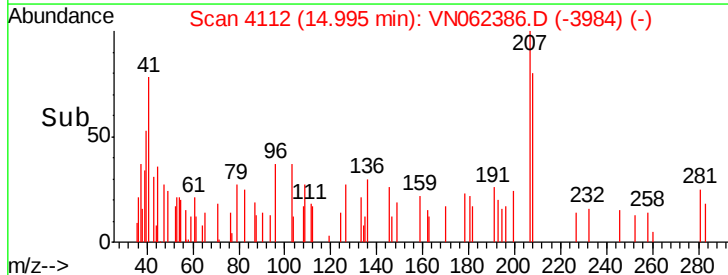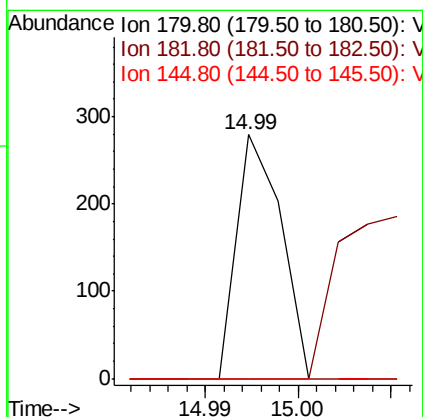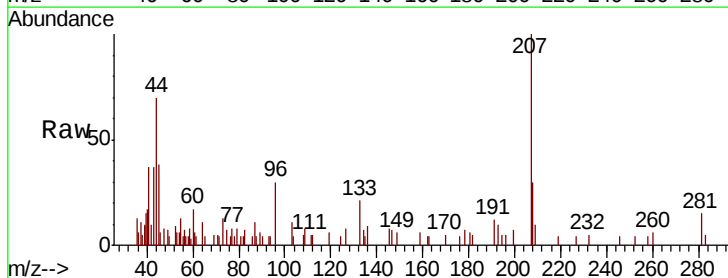

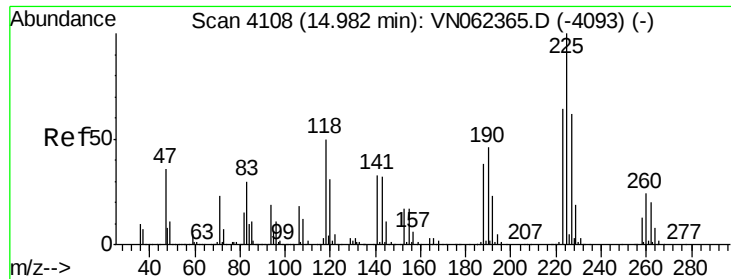

#94

Hexachlorobutadiene

Concen: Below Cal

RT: 14.93 min Scan# 4092

Delta R.T. -0.05 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46

Instrument :

MSVOA_N

ClientSampleId :

PB129462ZHE#02


Tot Ion:225 Resp: 32

Ion Ratio Lower Upper

225 100

223 481.3 31.7 95.1#




227 0.0 30.3 90.8#

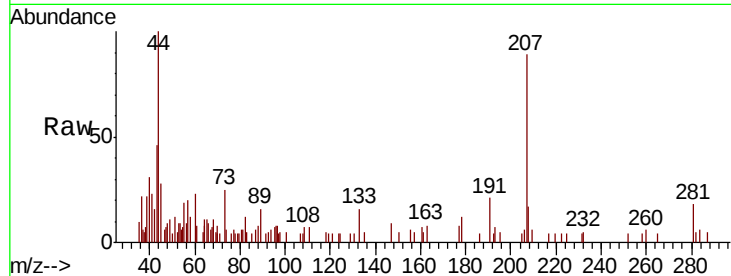

Abundance Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

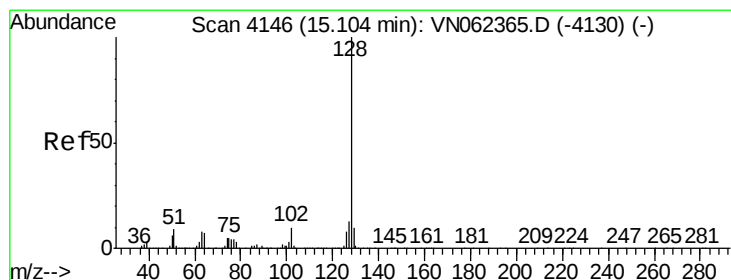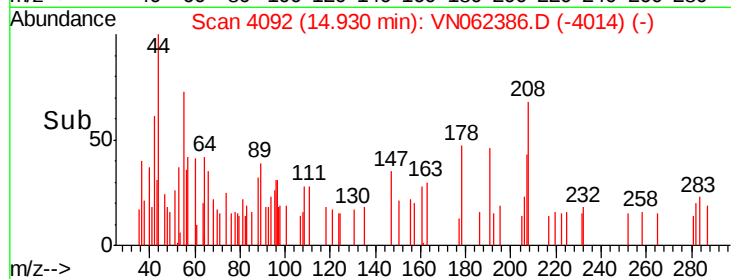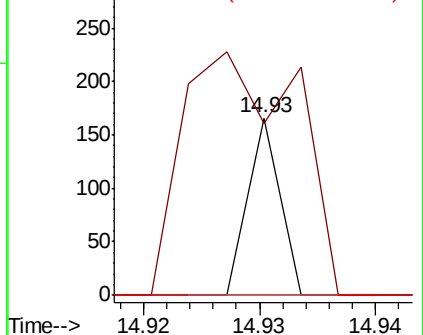

#95

Naphthalene

Concen: 2.118 ug/l

RT: 15.12 min Scan# 4151

Delta R.T. 0.02 min

Lab File: VN062386.D

Acq: 7 Jul 2020 00:46


Tgt Ion:128 Resp: 1417

Ion Ratio Lower Upper

128 100

127 9.4 10.8 16.2#

129 0.0 8.6 12.8#

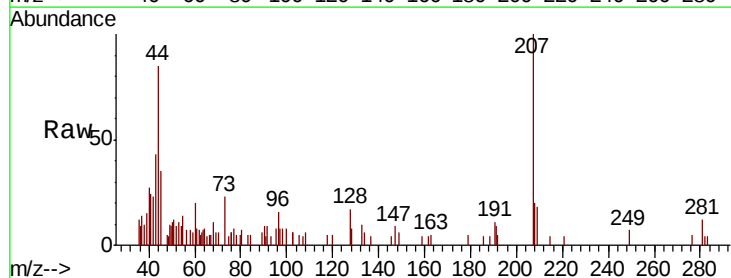

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

